
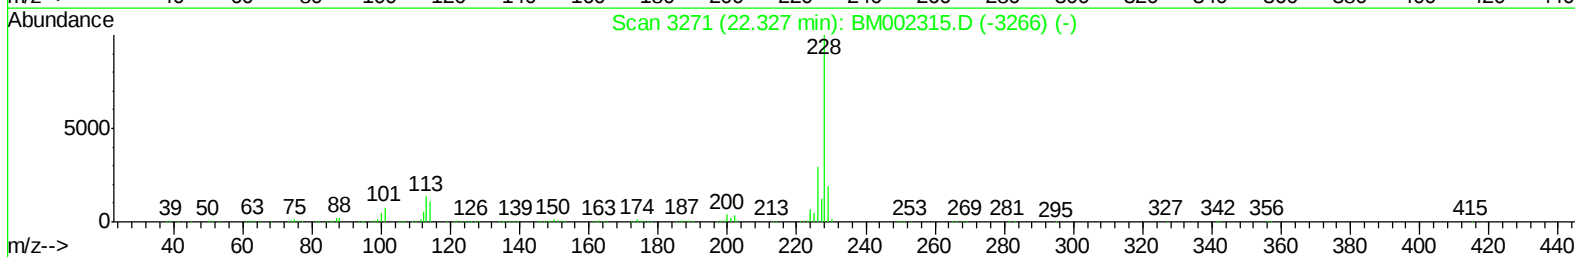
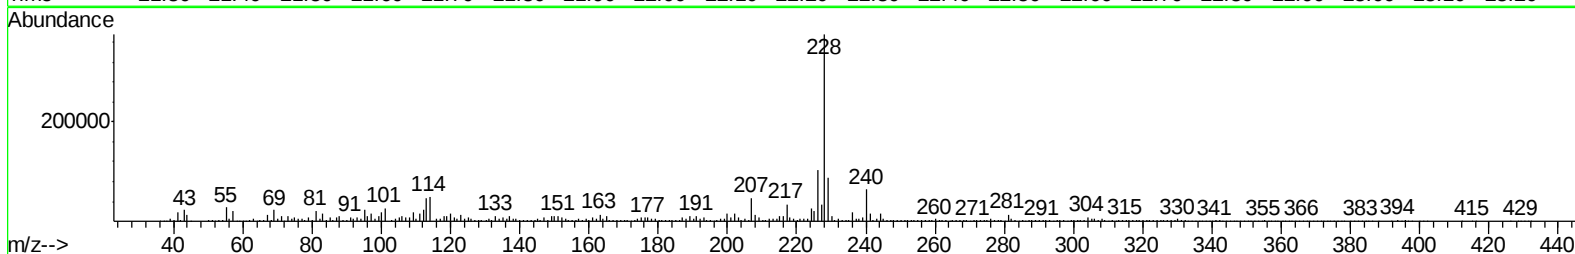


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081015\
Data File : BM002316.D
Acq On : 10 Aug 2015 17:14
Operator : UM/IZ
Sample : G3065-21DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 11 01:35:46 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM080715.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 11 01:34:33 2015
Response via : Initial Calibration

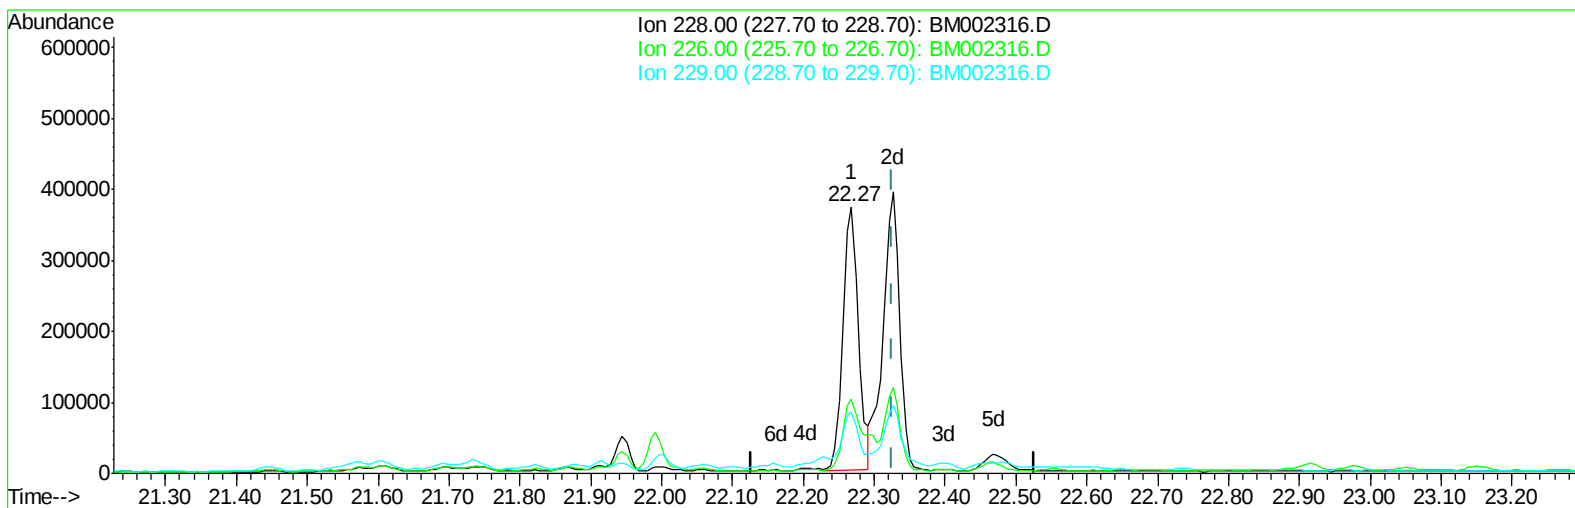

TIC: BM002316.D

(85) Chrysene




22.268min (-0.059) 25.65ng/ul

response 568199

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	27.80
229.00	19.40	23.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081015\
Data File : BM002316.D
Acq On : 10 Aug 2015 17:14
Operator : UM/IZ
Sample : G3065-21DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 11 01:35:46 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM080715.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 11 01:34:33 2015
Response via : Initial Calibration

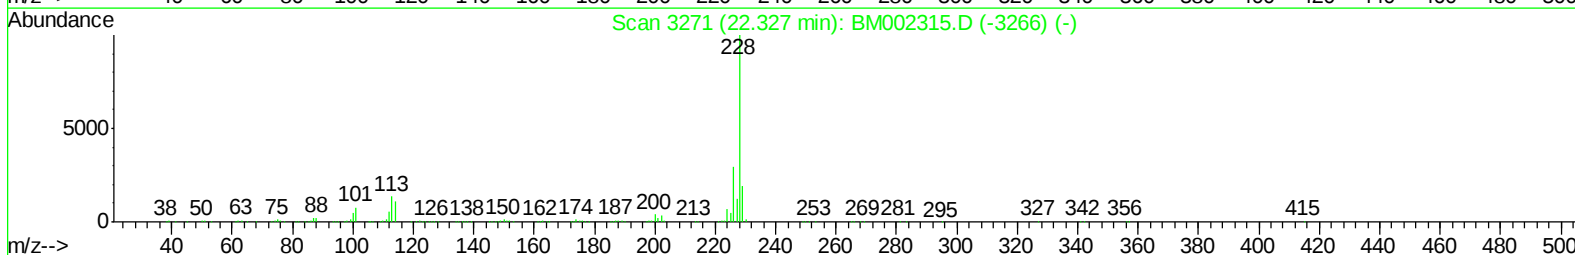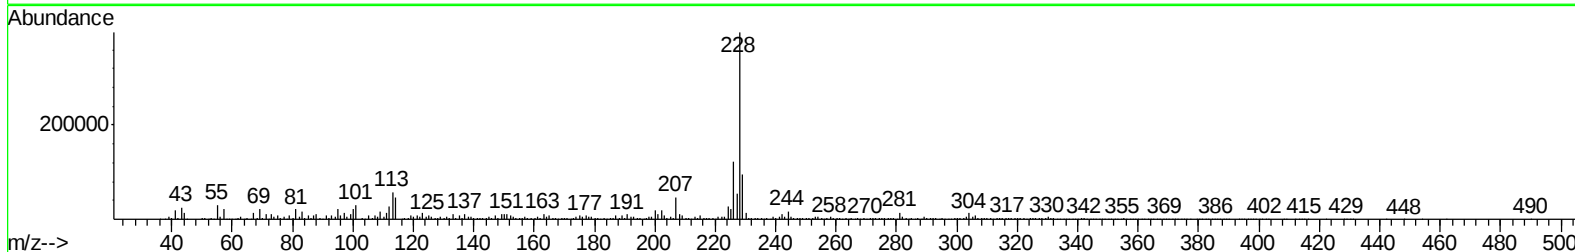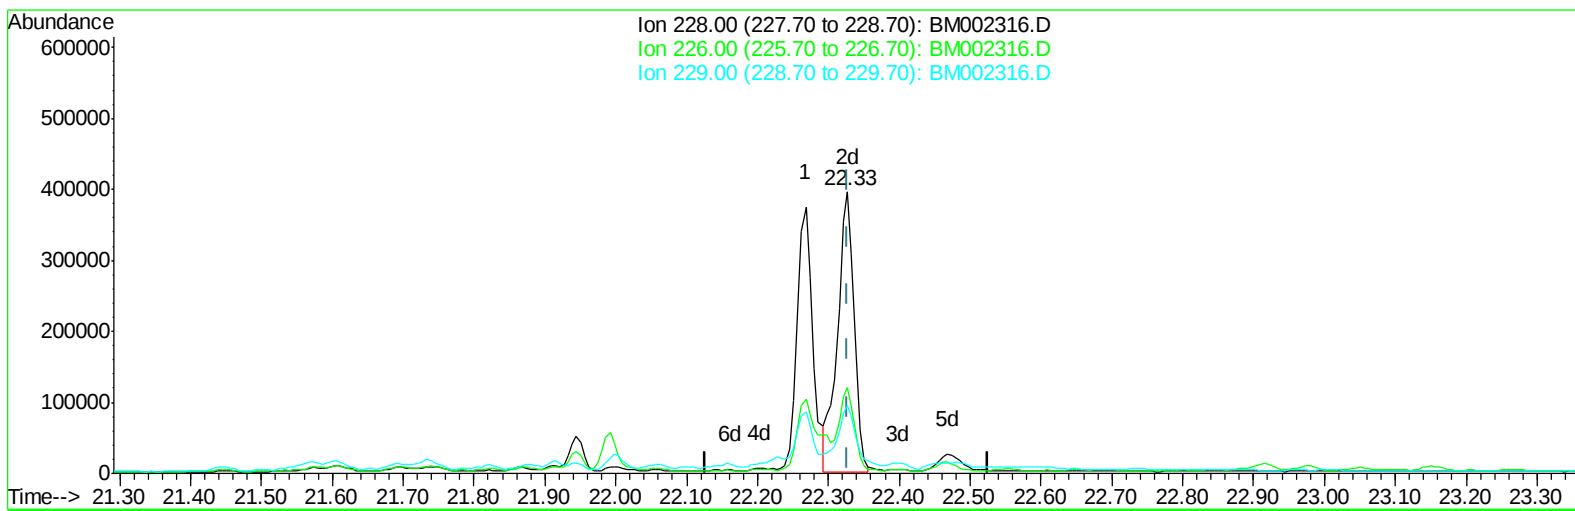

TIC: BM002316.D

(85) Chrysene




22.327min (-0.000) 29.41ng/ul m

response 651382

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	30.68
229.00	19.40	24.25#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081015\
Data File : BM002316.D
Acq On : 10 Aug 2015 17:14
Operator : UM/IZ
Sample : G3065-21DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 11 01:35:46 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM080715.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 11 01:34:33 2015
Response via : Initial Calibration

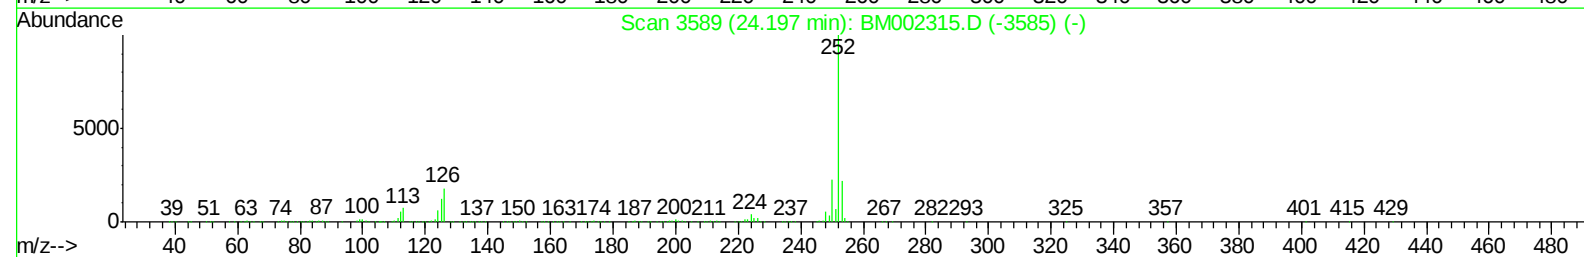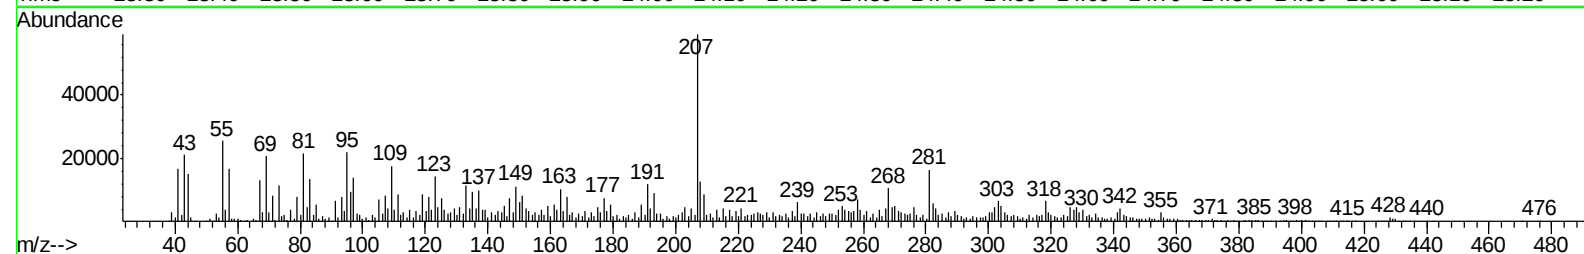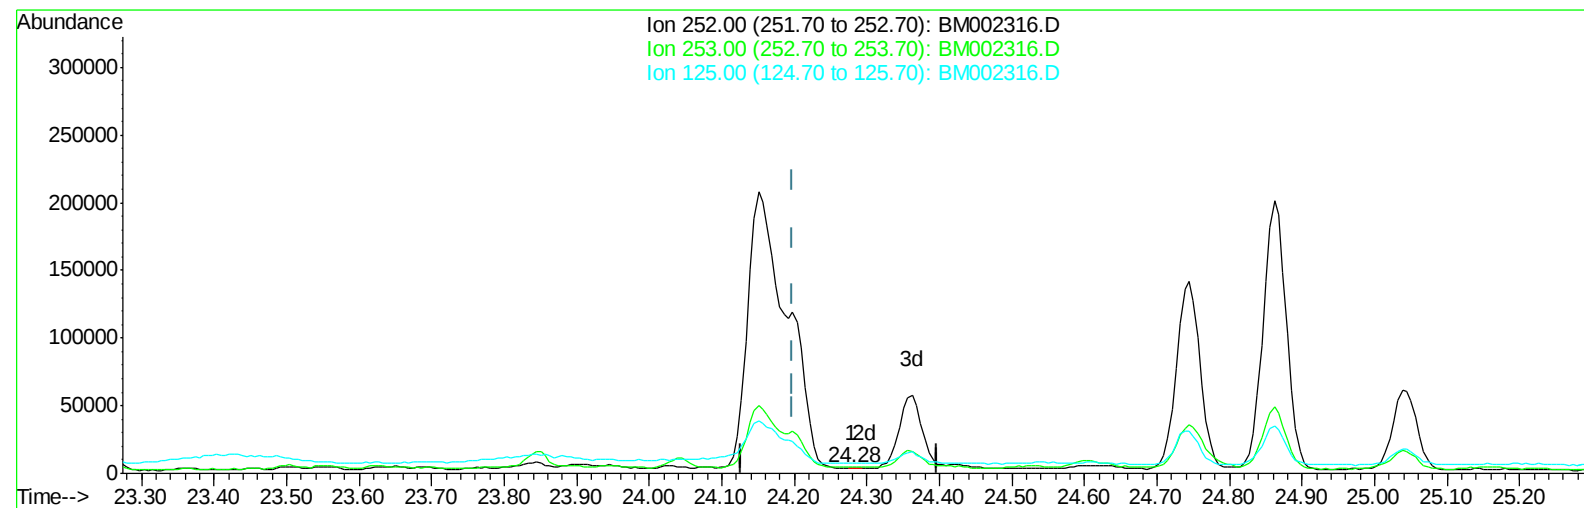

TIC: BM002316.D

(89) Benzo(k)fluoranthene




24.280min (+0.082) 0.02ng/ul

response 347

Ion	Exp%	Act%
252.00	100	100
253.00	21.60	120.31#
125.00	12.80	181.50#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081015\
Data File : BM002316.D
Acq On : 10 Aug 2015 17:14
Operator : UM/IZ
Sample : G3065-21DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Aug 11 01:35:46 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM080715.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 11 01:34:33 2015
Response via : Initial Calibration

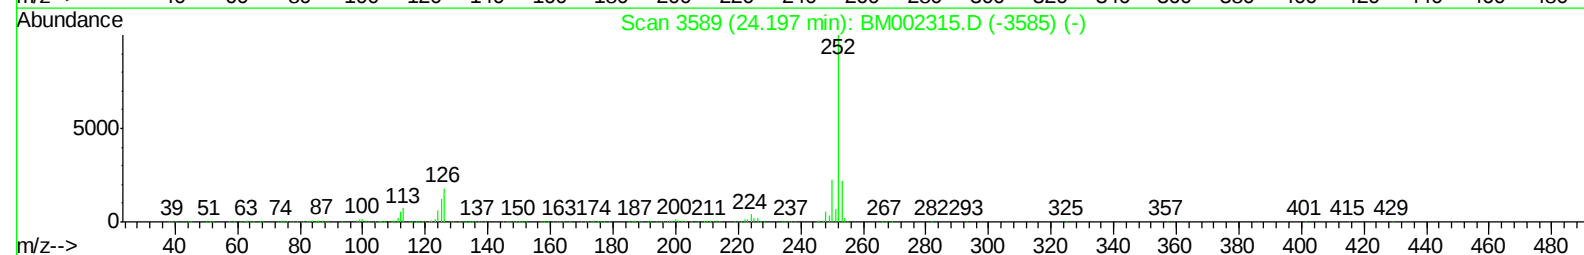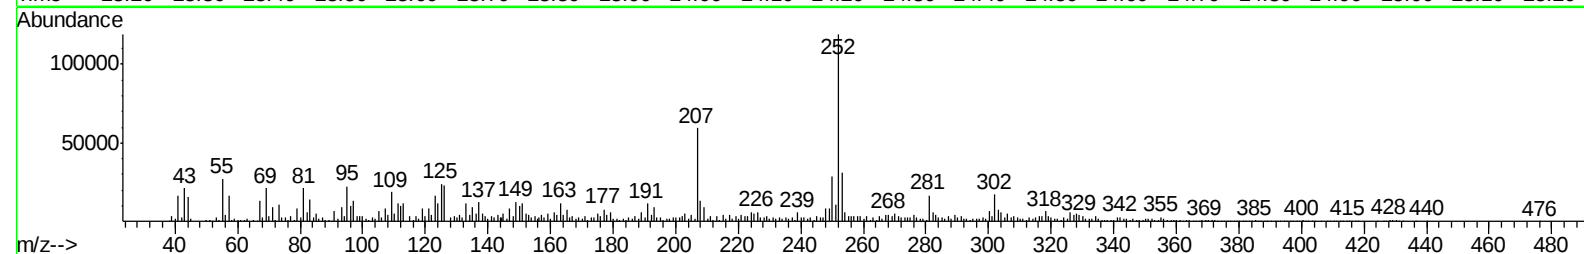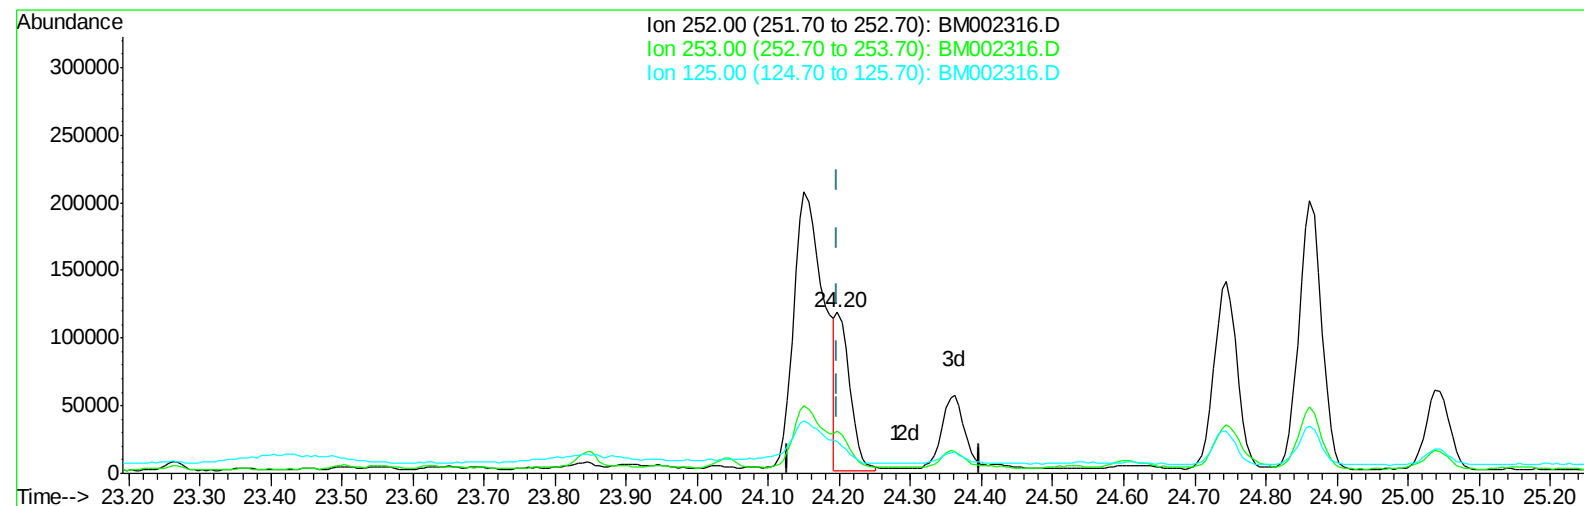

TIC: BM002316.D

(89) Benzo(k)fluoranthene

24.197min (-0.000) 7.18ng/ul m

response 159719

Ion	Exp%	Act%
252.00	100	100
253.00	21.60	26.04#
125.00	12.80	20.20#
0.00	0.00	0.00