

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081016\
 Data File : BM007023.D
 Acq On : 11 Aug 2016 05:00
 Operator : UM/SJ
 Sample : H4302-06DL 4X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA0H0DL

Quant Time: Aug 11 06:51:20 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080916.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 10 01:30:54 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	388616	20.00	ng/ul	0.00
7) Naphthalene-d8	10.60	136	1712708	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.45	164	1062791	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.19	188	2532370	20.00	ng/ul	0.00
29) Chrysene-d12	21.37	240	2497964	20.00	ng/ul	0.00
34) Perylene-d12	23.65	264	2114333	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.33	96	2474	0.29	ng/uL	0.00
3) Phenol-d5	6.97	99	116993	3.38	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	7.15	67	72362	3.74	ng/ul	0.00
5) 2-Chlorophenol-d4	7.35	132	96309	3.67	ng/ul	0.00
6) 4-Methylphenol-d8	8.51	113	84168	2.87	ng/ul	0.00
8) Nitrobenzene-d5	8.97	128	45344	3.47	ng/ul	0.00
9) 2-Nitrophenol-d4	9.69	143	47793	3.19	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.22	165	108740	3.72	ng/ul	0.00
12) 4-Chloroaniline-d4	10.74	131	82219	2.40	ng/ul	0.00
16) Dimethylphthalate-d6	13.86	166	372623	4.10	ng/ul	-0.01
17) Acenaphthylene-d8	14.14	160	452886	4.26	ng/ul	0.00
20) 4-Nitrophenol-d4	14.63	143	36275	2.22	ng/ul	-0.01
21) Fluorene-d10	15.44	176	339825	4.40	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.55	200	30620	2.23	ng/ul	0.00
26) Anthracene-d10	17.29	188	536059	4.54	ng/ul	0.00
30) Pyrene-d10	19.58	212	619867	5.46	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.51	264	446196	4.59	ng/ul	0.00

Target Compounds


					Qvalue
11) Naphthalene	10.65	128	169964	1.98 ng/ul	97
19) Acenaphthene	14.51	153	221472	3.12 ng/ul	96
22) Fluorene	15.49	166	132560	1.57 ng/ul	99
25) Phenanthrene	17.23	178	3209477	23.66 ng/ul	99
27) Anthracene	17.32	178	613004	4.37 ng/ul	100
28) Fluoranthene	19.25	202	5948700	34.81 ng/ul	98
31) Pyrene	19.62	202	4926970	34.00 ng/ul	98
32) Benzo(a)anthracene	21.36	228	2749193	18.69 ng/ul	99
33) Chrysene	21.41	228	2531116	18.96 ng/ul	98
35) Benzo(b)fluoranthene	22.97	252	3559095	27.10 ng/ul	98
36) Benzo(k)fluoranthene	22.97	252	3559095	28.68 ng/ul	98
38) Benzo(a)pyrene	23.55	252	2309378	19.11 ng/ul	97
39) Indeno(1,2,3-cd)pyrene	25.96	276	1947389	16.25 ng/ul	97
40) Dibenzo(a,h)anthracene	26.22	278	320072	3.23 ng/ul	97
41) Benzo(g,h,i)perylene	26.66	276	1907899	19.37 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081016\
Data File : BM007023.D
Acq On : 11 Aug 2016 05:00
Operator : UM/SJ
Sample : H4302-06DL 4X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA0H0DL

Quant Time: Aug 11 06:51:20 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080916.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 10 01:30:54 2016
Response via : Initial Calibration

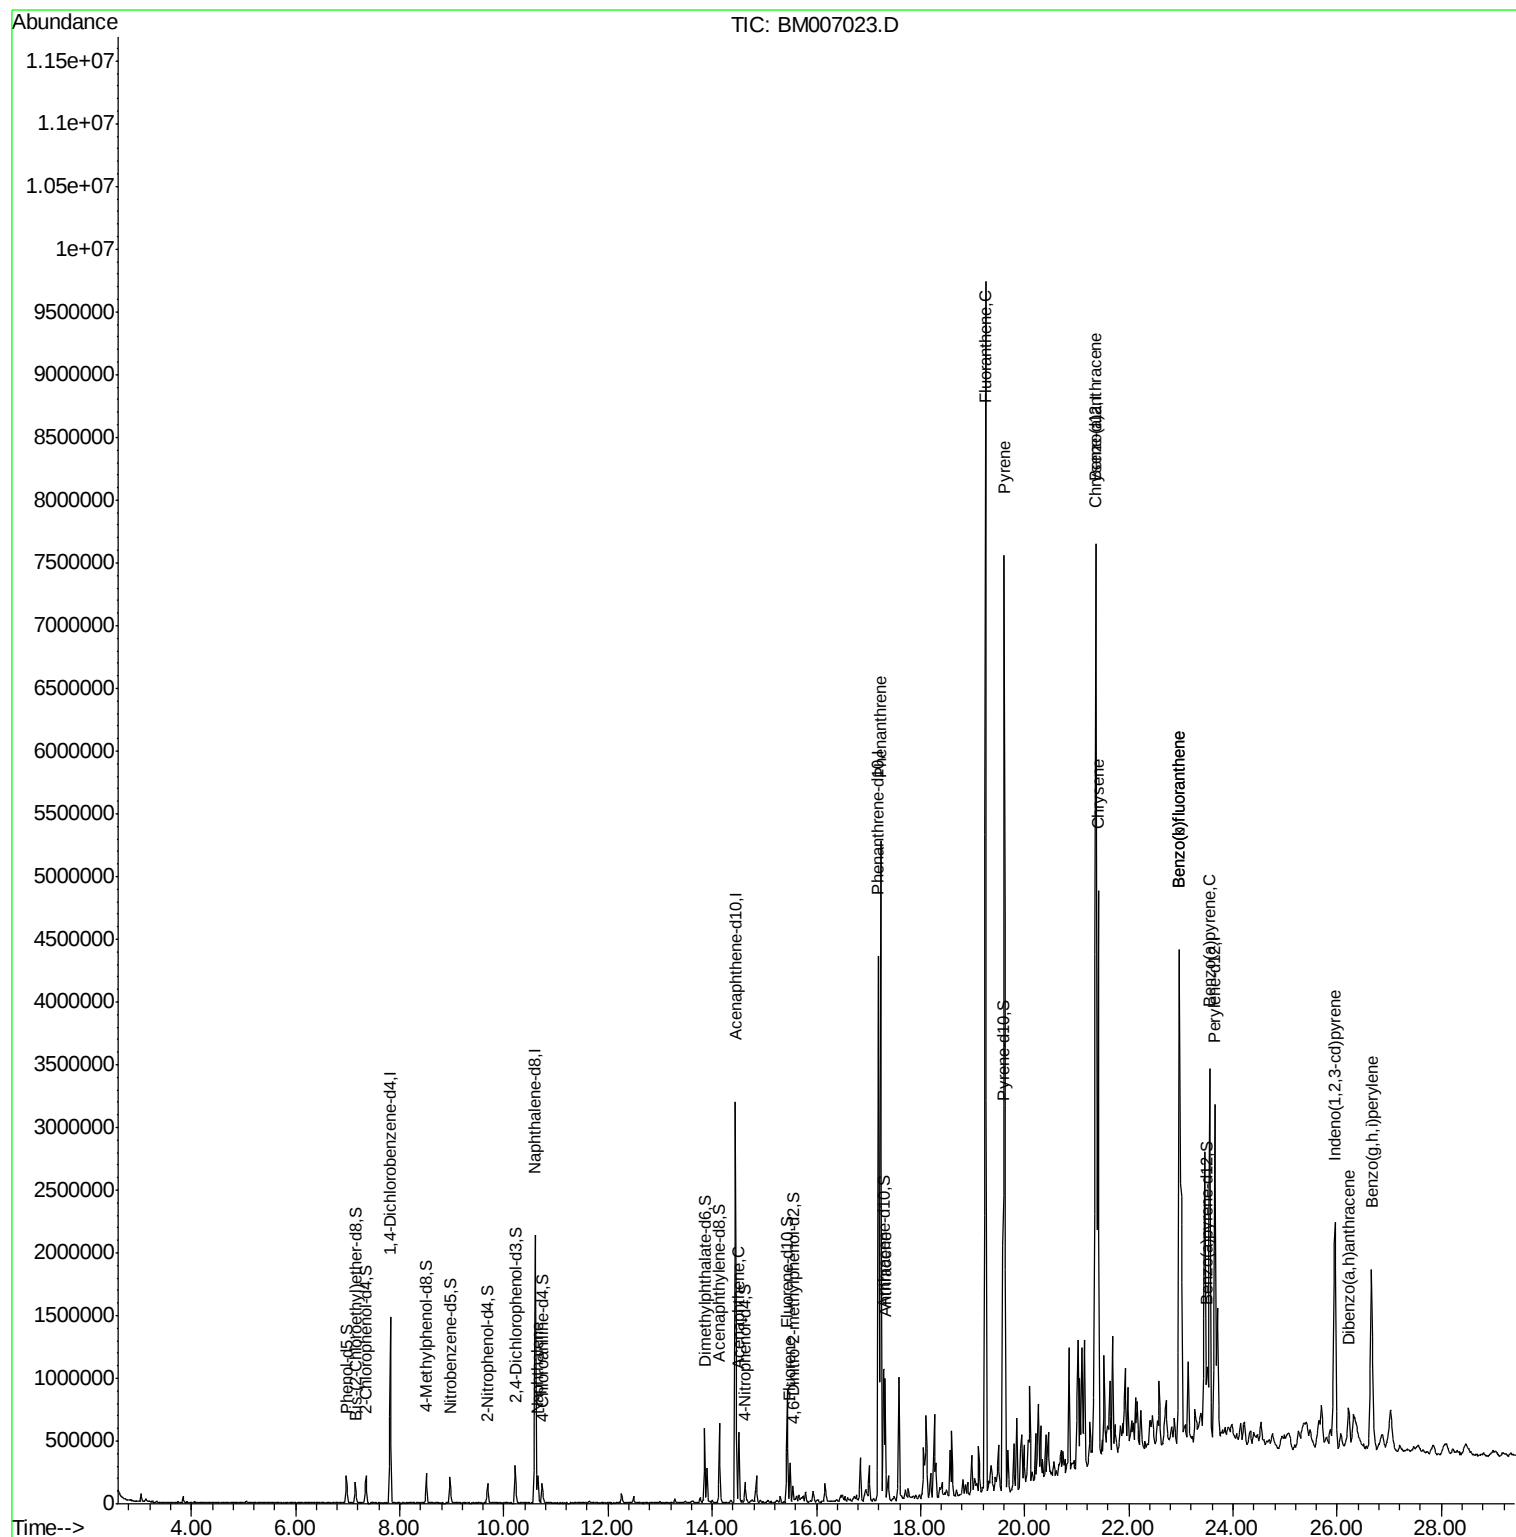

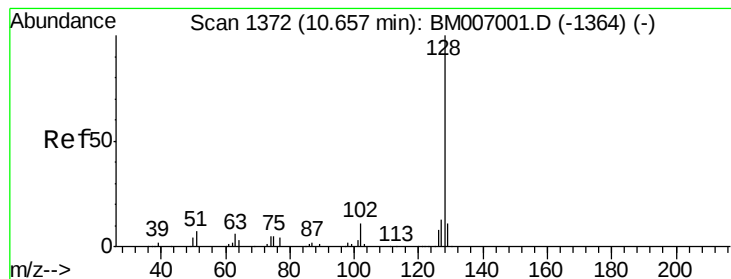

#11

Naphthalene

Concen: 1.98 ng/ul

RT: 10.65 min Scan# 1371

Delta R.T. -0.01 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00

Instrument :

BNA_M

ClientSampleId :

DA0H0DL


Tgt Ion:128 Resp: 169964

Ion Ratio Lower Upper

128 100

129 12.0 8.9 13.3




127 14.1 10.4 15.6



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

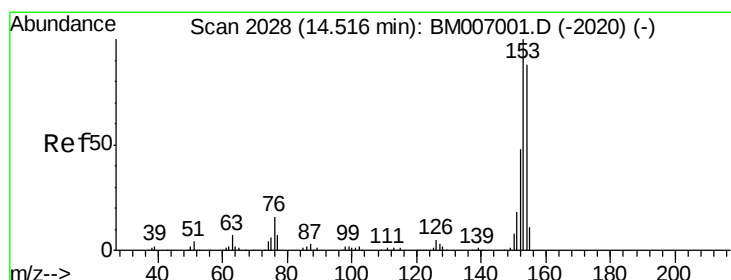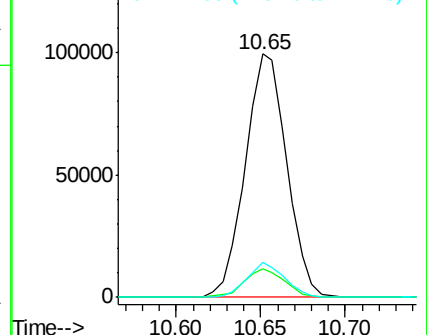

#19

Acenaphthene

Concen: 3.12 ng/ul

RT: 14.51 min Scan# 2027

Delta R.T. -0.01 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00


Tgt Ion:153 Resp: 221472

Ion Ratio Lower Upper

153 100

152 48.1 37.0 55.6



154 92.4 70.9 106.3




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

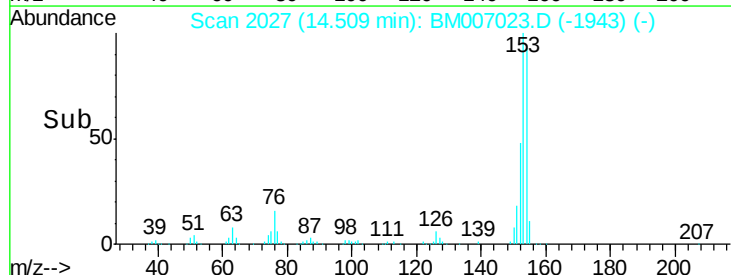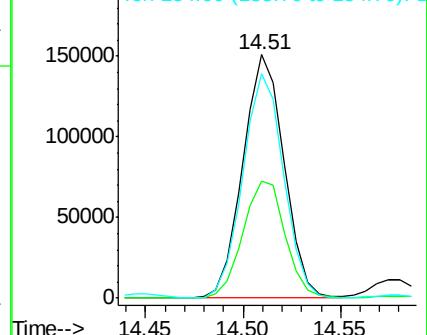

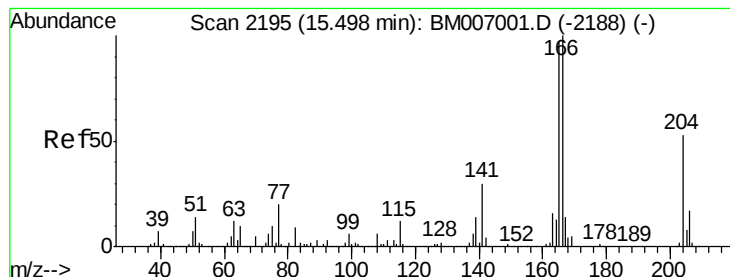

#22

Fluorene

Concen: 1.57 ng/ul

RT: 15.49 min Scan# 2194

Delta R.T. -0.01 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00

Instrument :

BNA_M

ClientSampleId :

DA0H0DL


Tgt Ion:166 Resp: 132560

Ion Ratio Lower Upper

166 100

165 96.2 76.6 115.0




167 14.4 10.7 16.1

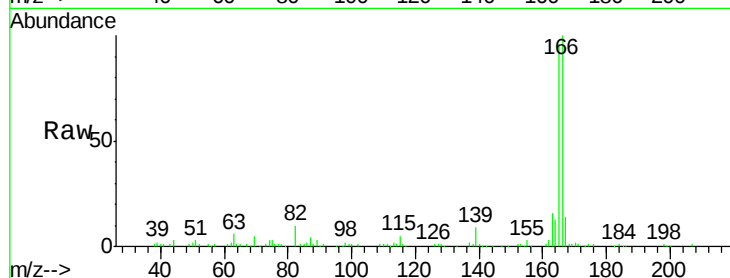

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

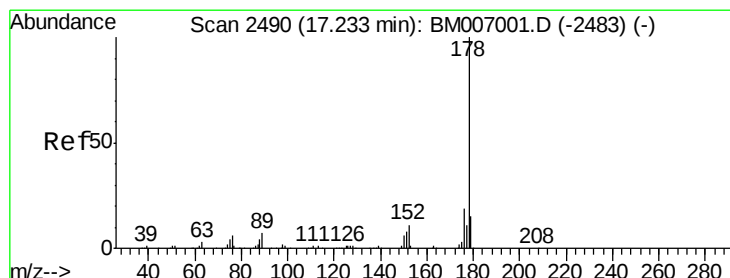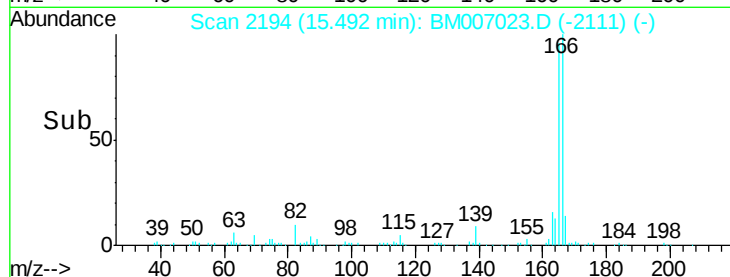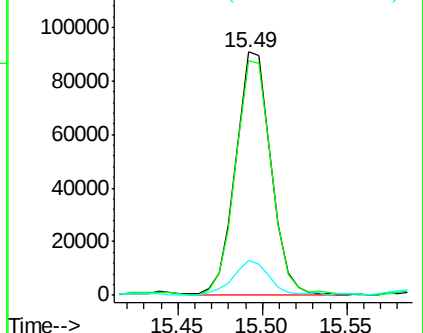

#25

Phenanthrene

Concen: 23.66 ng/ul

RT: 17.23 min Scan# 2490

Delta R.T. -0.01 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00


Tgt Ion:178 Resp: 3209477

Ion Ratio Lower Upper

178 100

179 15.5 12.2 18.2



176 19.3 15.2 22.8

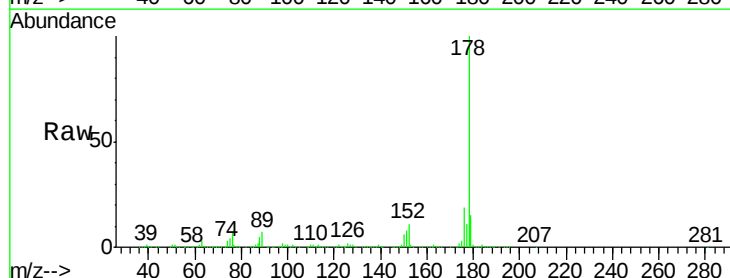


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

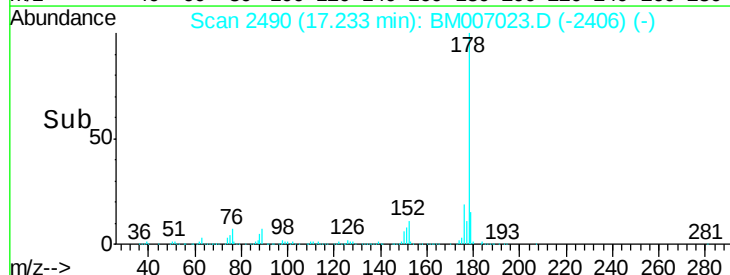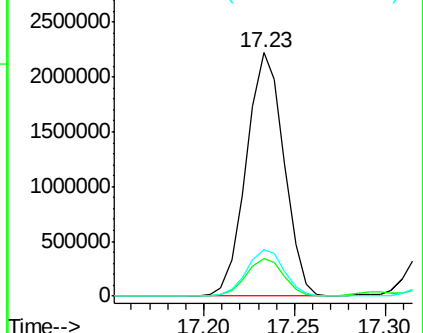

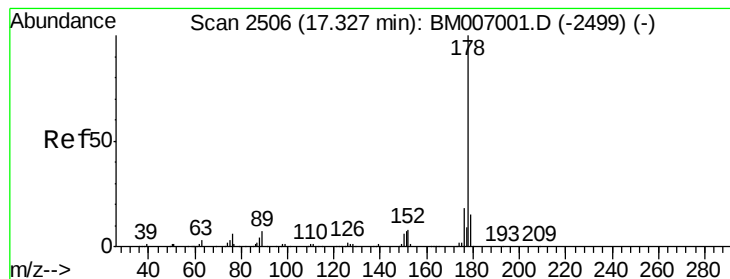

#27

Anthracene

Concen: 4.37 ng/ul

RT: 17.32 min Scan# 2505

Delta R.T. -0.01 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00

Instrument :

BNA_M

ClientSampleId :

DA0H0DL


Tgt Ion:178 Resp: 613004

Ion Ratio Lower Upper

178 100

179 15.6 12.5 18.7




176 18.5 15.0 22.4

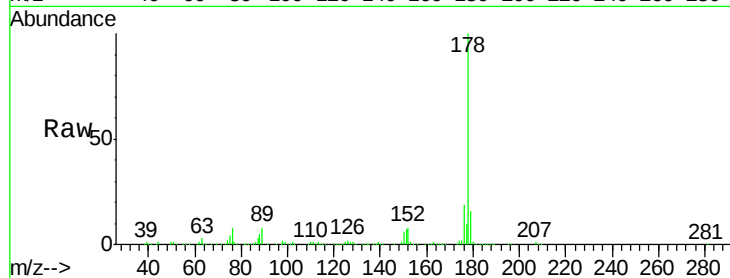

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

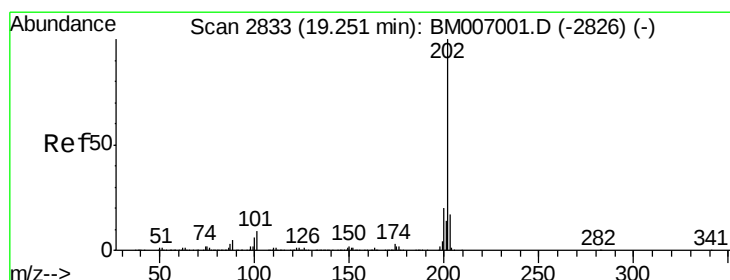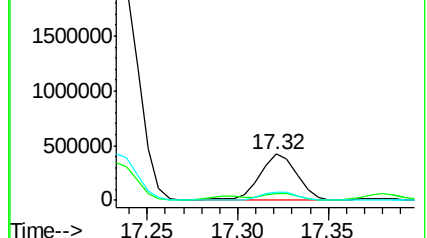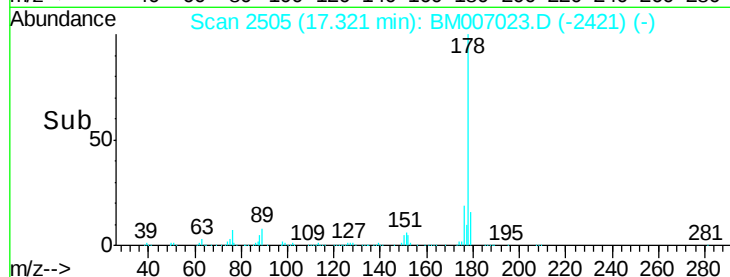

#28

Fluoranthene

Concen: 34.81 ng/ul

RT: 19.25 min Scan# 2833

Delta R.T. -0.00 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00


Tgt Ion:202 Resp: 5948700

Ion Ratio Lower Upper

202 100

101 8.5 7.4 11.2



100 6.4 5.8 8.6

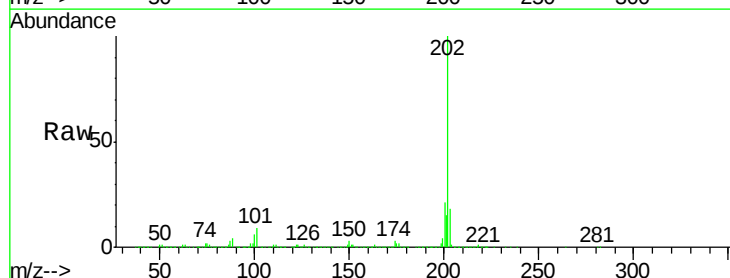


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

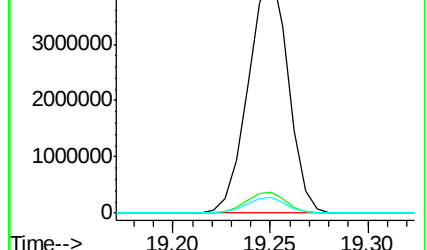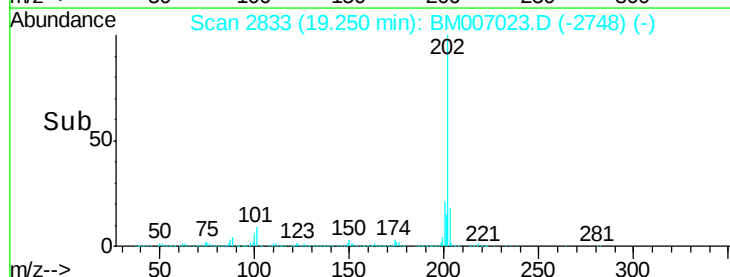

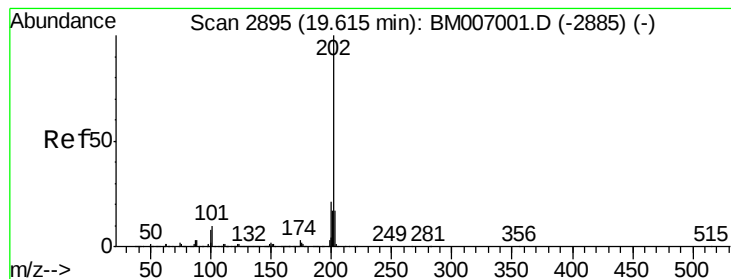

#31

Pyrene

Concen: 34.00 ng/ul

RT: 19.62 min Scan# 2895

Delta R.T. -0.00 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00

Instrument :

BNA_M

ClientSampleId :

DA0H0DL


Tgt Ion:202 Resp: 4926970

Ion Ratio Lower Upper

202 100

101 9.9 8.5 12.7




100 8.2 7.1 10.7



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

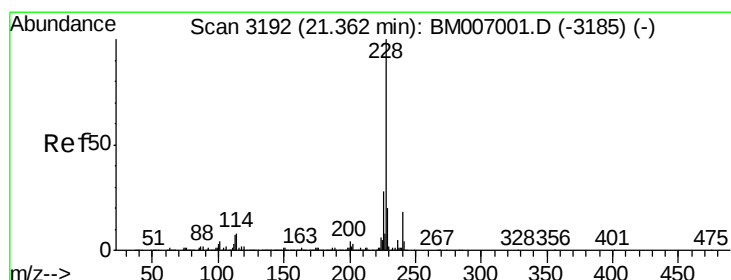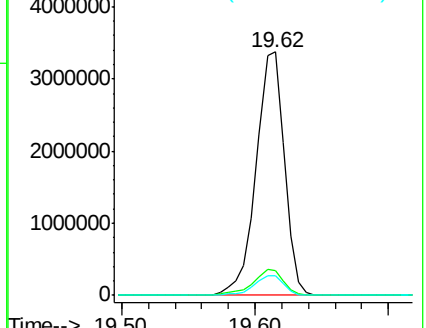

#32

Benzo(a)anthracene

Concen: 18.69 ng/ul

RT: 21.36 min Scan# 3191

Delta R.T. -0.01 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00


Tgt Ion:228 Resp: 2749193

Ion Ratio Lower Upper

228 100

229 20.3 15.8 23.6



226 27.4 21.9 32.9




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

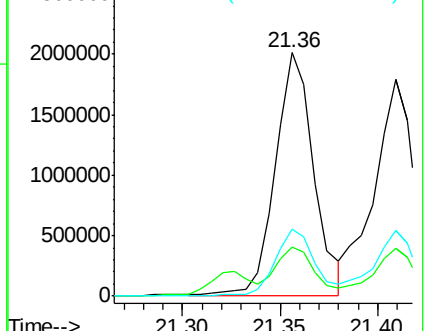



#33

Chrysene

Concen: 18.96 ng/ul

RT: 21.41 min Scan# 3200

Delta R.T. -0.01 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00

Instrument :

BNA_M

ClientSampleId :

DA0H0DL





Tgt Ion:228 Resp: 2531116

Ion Ratio Lower Upper

228 100

226 30.2 24.2 36.4

229 22.3 15.9 23.9

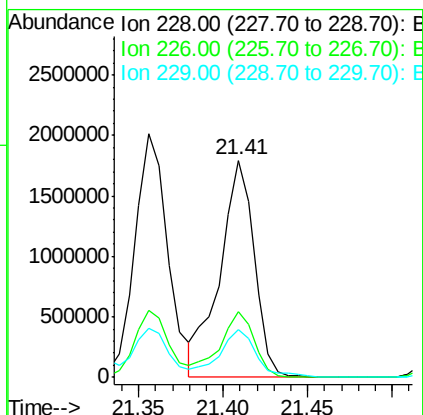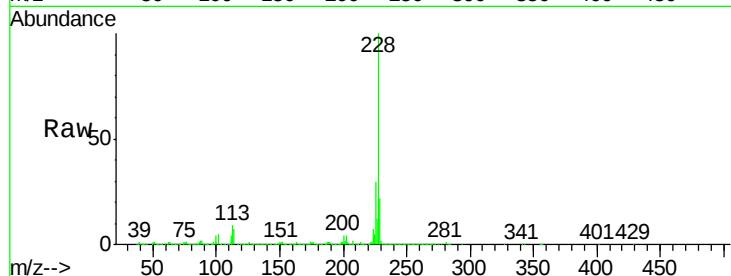

#35

Benzo(b)fluoranthene

Concen: 27.10 ng/ul

RT: 22.97 min Scan# 3465

Delta R.T. -0.00 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00




Tgt Ion:252 Resp: 3559095


Ion Ratio Lower Upper

252 100

253 23.2 17.4 26.2

125 7.8 6.0 9.0

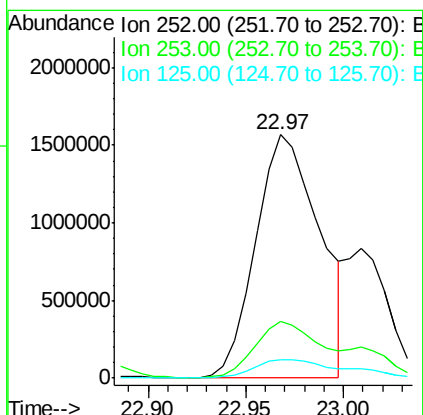



#36

Benzo(k)fluoranthene

Concen: 28.68 ng/ul

RT: 22.97 min Scan# 3465

Delta R.T. -0.05 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00

Instrument :

BNA_M

ClientSampleId :

DA0H0DL


Tgt Ion:252 Resp: 3559095

Ion Ratio Lower Upper

252 100

253 23.2 17.8 26.6




125 7.8 6.2 9.4



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

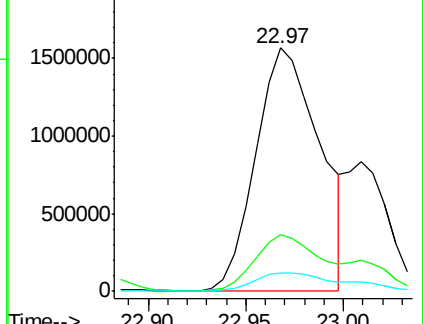

#38

Benzo(a)pyrene

Concen: 19.11 ng/ul

RT: 23.55 min Scan# 3564

Delta R.T. -0.01 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00


Tgt Ion:252 Resp: 2309378

Ion Ratio Lower Upper

252 100

253 23.8 17.7 26.5



125 8.4 6.8 10.2




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

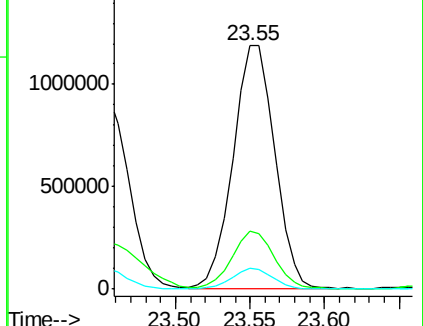







#39

Indeno(1,2,3-cd)pyrene
Concen: 16.25 ng/ul
RT: 25.96 min Scan# 3973
Delta R.T. -0.01 min
Lab File: BM007023.D
Acq: 11 Aug 2016 05:00

Instrument :
BNA_M
ClientSampleId :
DA0H0DL




Tgt Ion:276 Resp: 1947389
Ion Ratio Lower Upper
276 100
138 15.5 14.9 22.3
277 24.6 19.8 29.6

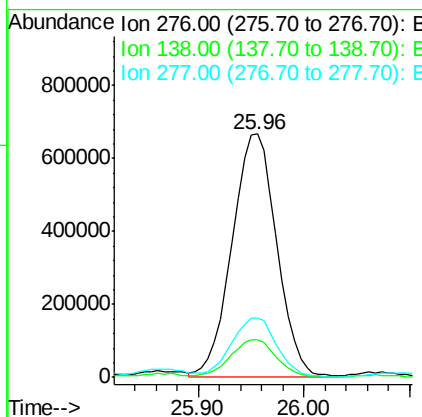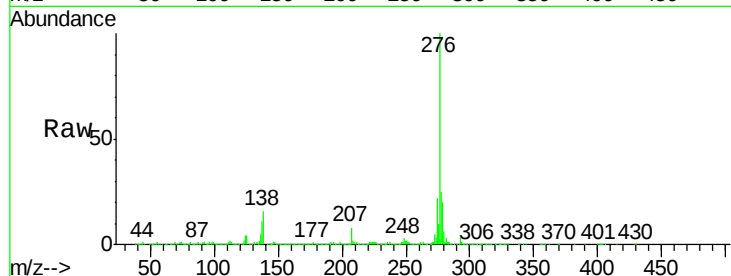


#40

Dibenzo(a,h)anthracene
Concen: 3.23 ng/ul
RT: 26.22 min Scan# 4018
Delta R.T. 0.24 min
Lab File: BM007023.D
Acq: 11 Aug 2016 05:00

Tgt Ion:278 Resp: 320072
Ion Ratio Lower Upper
278 100
139 13.7 10.3 15.5
279 25.1 18.8 28.2

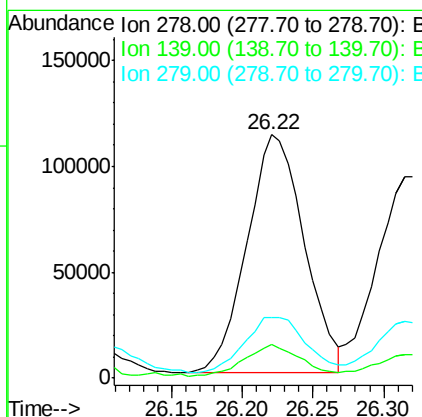



#41

Benzo(g,h,i)perylene

Concen: 19.37 ng/ul

RT: 26.66 min Scan# 4092

Delta R.T. -0.01 min

Lab File: BM007023.D

Acq: 11 Aug 2016 05:00

Instrument :

BNA_M

ClientSampleId :

DA0H0DL


Tgt Ion:276 Resp: 1907899

Ion Ratio Lower Upper

276 100

138 15.8 14.0 21.0

277 24.4 19.6 29.4



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

