
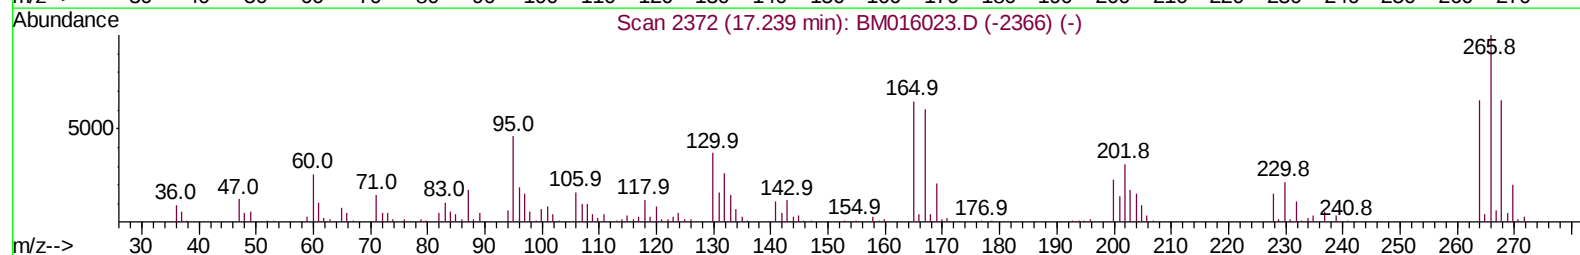
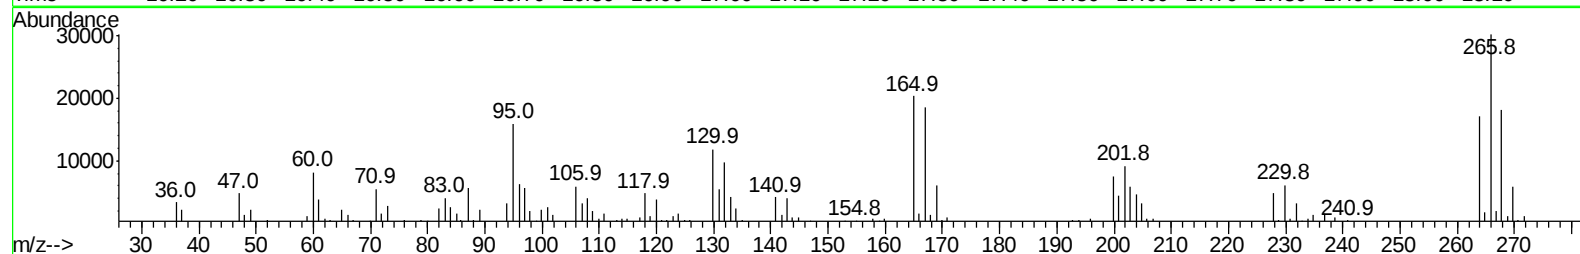


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM081018\  
Data File : BM016297.D  
Acq On : 10 Aug 2018 15:44  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 01:01:28 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 10 18:44:22 2018  
Response via : Initial Calibration

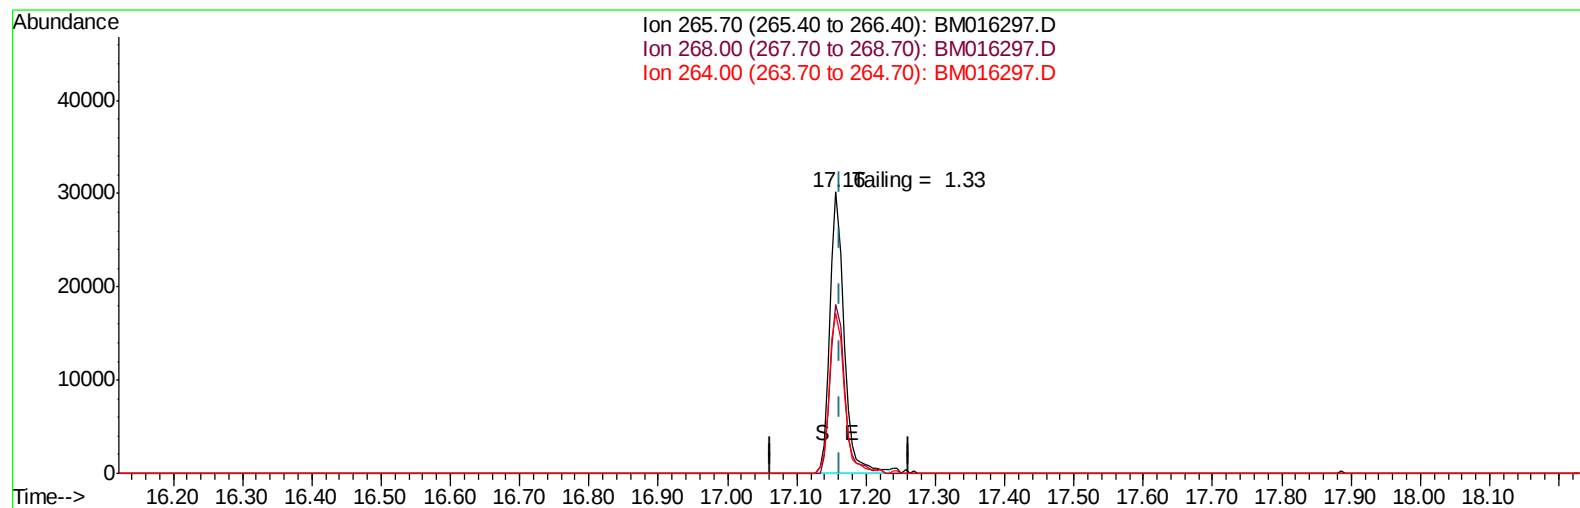

TIC: BM016297.D

(69) Pentachlorophenol (C)




17.157min (-0.006) 0.00ng

response 42855

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.00 | 59.87 |
| 264.00 | 61.20 | 56.69 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM081018\  
 Data File : BM016297.D  
 Acq On : 10 Aug 2018 15:44  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 01:01:28 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Aug 10 18:44:22 2018  
 Response via : Initial Calibration

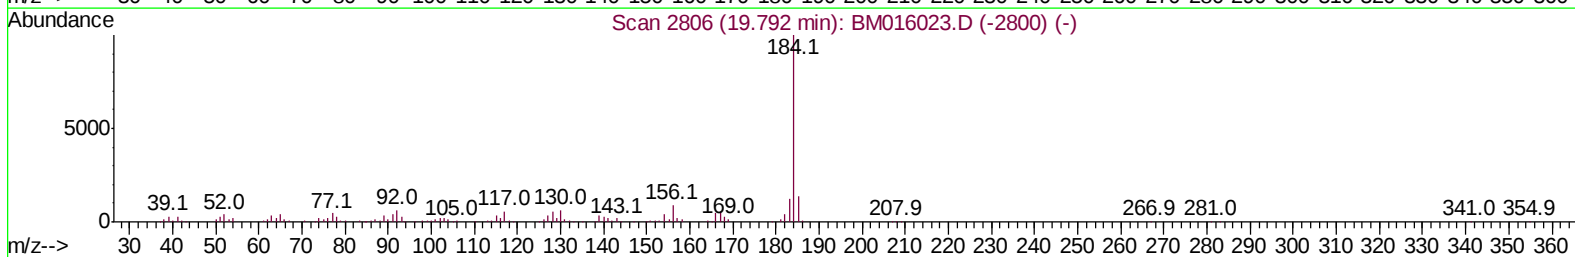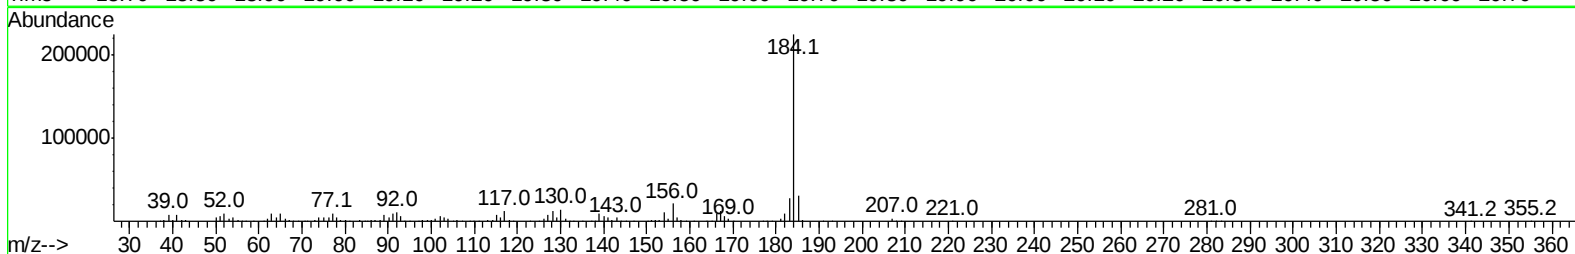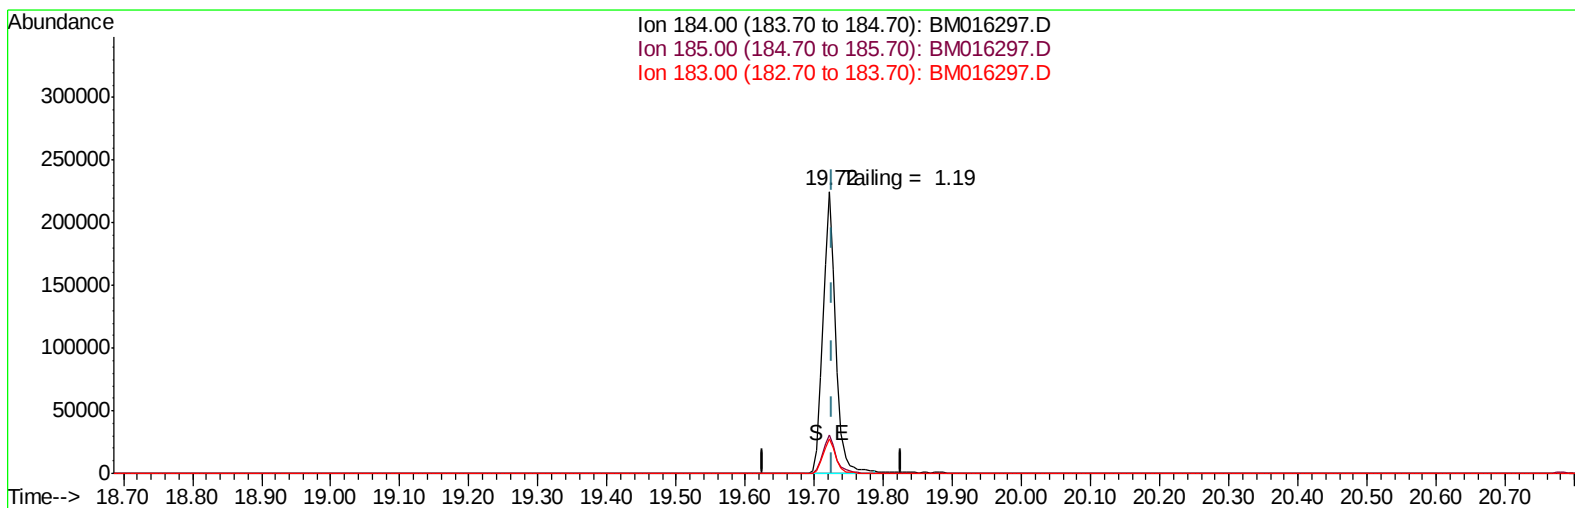

TIC: BM016297.D

(76) Benzidine

19.721min (-0.006) 42931.81ng

response 284329

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.10 | 13.51 |
| 183.00 | 11.10 | 12.44 |
| 0.00   | 0.00  | 0.00  |