

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM081018\  
 Data File : BM016315.D  
 Acq On : 11 Aug 2018 02:43  
 Operator : SJ/JU  
 Sample : J4272-18  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 JC-03-080918-I

Quant Time: Aug 11 06:28:08 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM072318.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Aug 10 18:44:22 2018  
 Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|-----------------------------|-------|------|----------|--------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 8.13  | 152  | 26393    | 20.00  | ng    | 0.00     |
| 21) Naphthalene-d8          | 10.94 | 136  | 90570    | 20.00  | ng    | -0.01    |
| 38) Acenaphthene-d10        | 14.76 | 164  | 40624    | 20.00  | ng    | -0.01    |
| 63) Phenanthrene-d10        | 17.50 | 188  | 77327    | 20.00  | ng    | -0.01    |
| 75) Chrysene-d12            | 21.63 | 240  | 91786    | 20.00  | ng    | -0.01    |
| 86) Perylene-d12            | 23.96 | 264  | 106614   | 20.00  | ng    | -0.02    |
| System Monitoring Compounds |       |      |          |        |       |          |
| 5) 2-Fluorophenol           | 5.66  | 112  | 248385   | 156.33 | ng    | 0.00     |
| 7) Phenol-d6                | 7.30  | 99   | 248306   | 119.67 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 9.31  | 82   | 243540   | 125.07 | ng    | -0.01    |
| 41) 2,4,6-Tribromophenol    | 16.25 | 330  | 74242    | 144.09 | ng    | -0.01    |
| 44) 2-Fluorobiphenyl        | 13.38 | 172  | 416248   | 124.67 | ng    | -0.01    |
| 78) Terphenyl-d14           | 20.07 | 244  | 575620   | 131.28 | ng    | -0.01    |


| Target Compounds | Qvalue |
|------------------|--------|
|------------------|--------|

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM081018\  
Data File : BM016315.D  
Acq On : 11 Aug 2018 02:43  
Operator : SJ/JU  
Sample : J4272-18  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
JC-03-080918-I

Quant Time: Aug 11 06:28:08 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM072318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 10 18:44:22 2018  
Response via : Initial Calibration

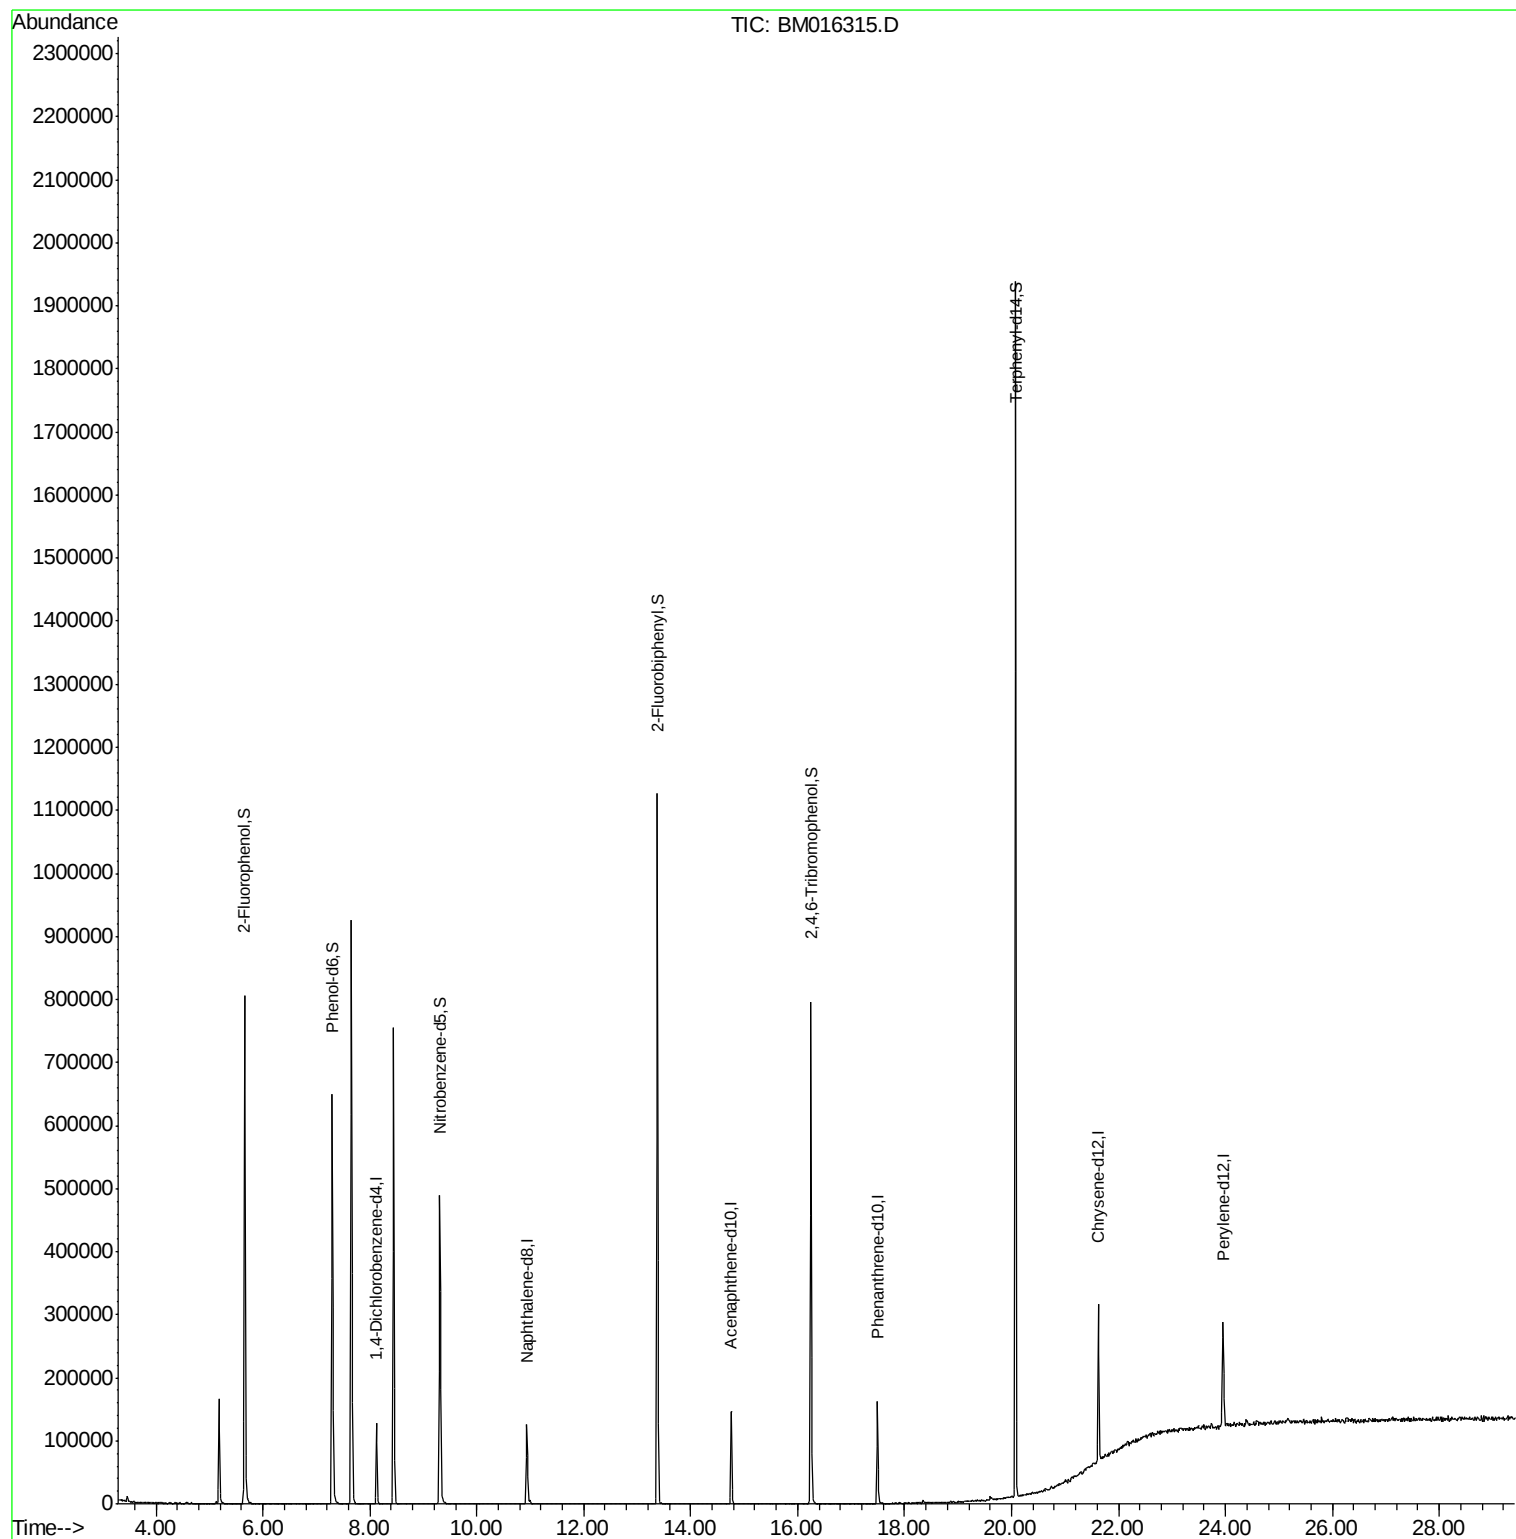







#1  
 1,4-Dichlorobenzene-d4  
 Concen: 20.000 ng  
 RT: 8.13 min Scan# 823  
 Delta R.T. -0.01 min  
 Lab File: BM016315.D  
 Acq: 11 Aug 2018 02:43

Instrument :  
 BNA\_M  
 ClientSampleId :  
 JC-03-080918-I

Tgt Ion:152 Resp: 26393  
 Ion Ratio Lower Upper  
 152 100  
 150 147.7 119.5 179.3  
 115 69.2 43.0 64.4#

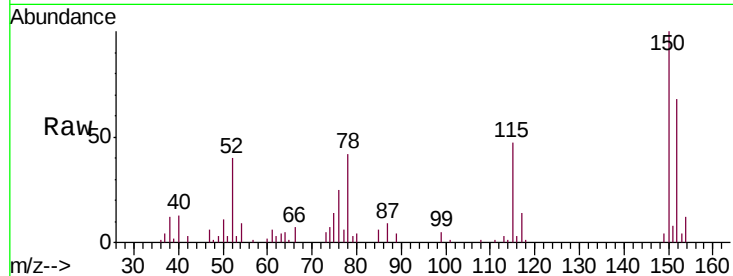


Abundance Ion 152.00 (151.70 to 152.70): E  
 Ion 150.00 (149.70 to 150.70): E  
 Ion 115.00 (114.70 to 115.70): E

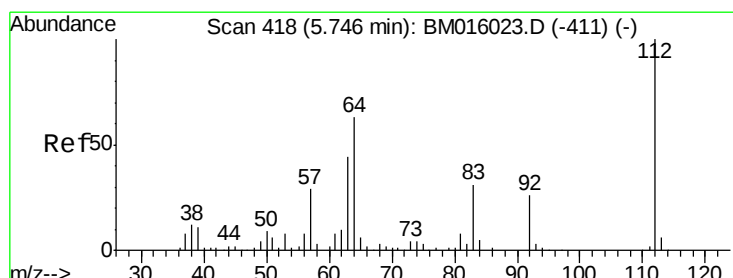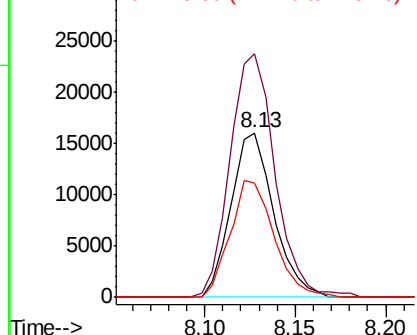
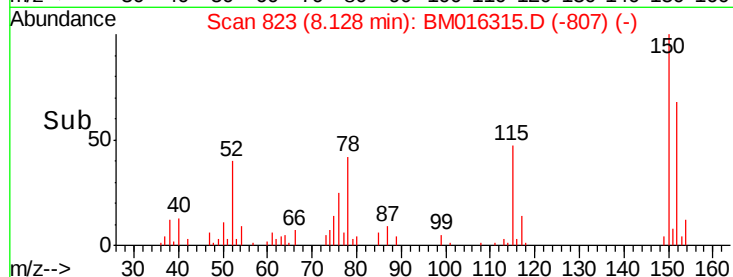



#5  
 2-Fluorophenol  
 Concen: Below ng  
 RT: 5.66 min Scan# 403  
 Delta R.T. -0.01 min  
 Lab File: BM016315.D  
 Acq: 11 Aug 2018 02:43

Tgt Ion:112 Resp: 248385  
 Ion Ratio Lower Upper  
 112 100  
 64 62.0 38.6 57.8#  
 63 47.7 19.3 28.9#

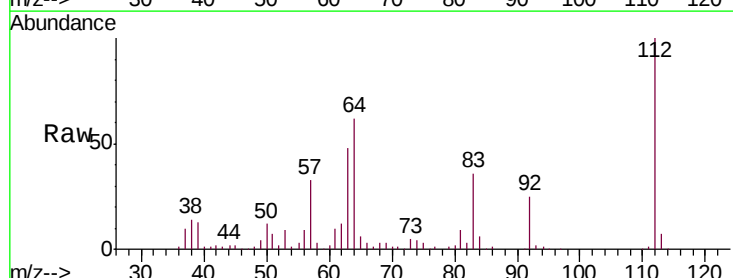

Abundance Ion 112.00 (111.70 to 112.70): E  
 Ion 64.00 (63.70 to 64.70): BM0  
 Ion 63.00 (62.70 to 63.70): BM0

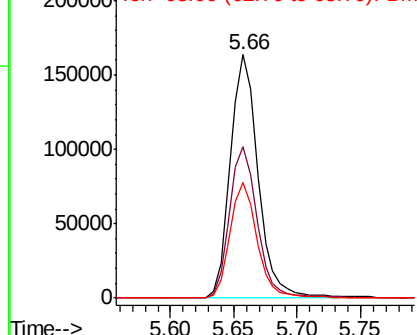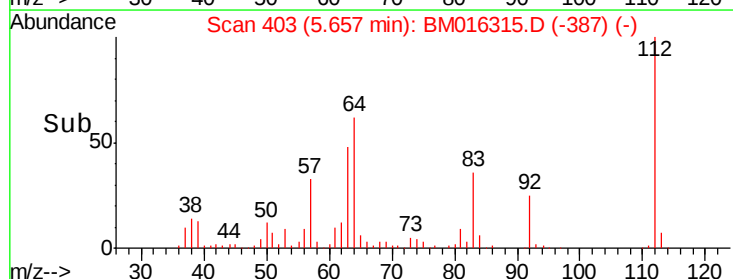

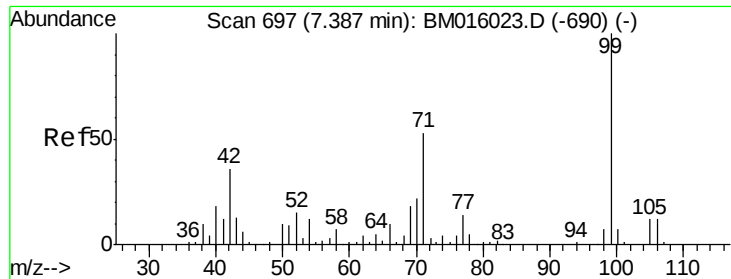

#7

Phenol-d6

Concen: N.D. ng

RT: 7.30 min Scan# 682

Delta R.T. -0.01 min

Lab File: BM016315.D

Acq: 11 Aug 2018 02:43

Instrument :

BNA\_M

ClientSampleId :

JC-03-080918-I


Tgt Ion: 99 Resp: 248306

Ion Ratio Lower Upper

99 100

42 40.6 11.0 16.4#




71 57.0 23.4 35.2#

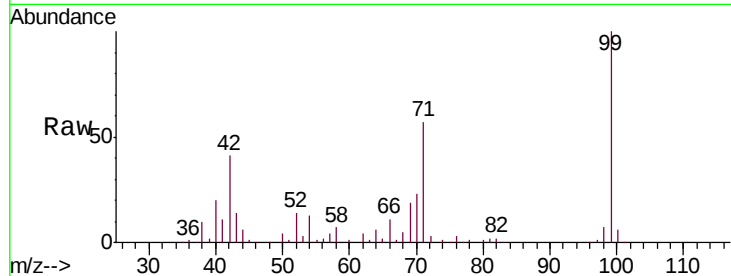

Abundance Ion 99.00 (98.70 to 99.70): BM016315.D (-666) (-)

Ion 42.00 (41.70 to 42.70): BM016315.D (-666) (-)

Ion 71.00 (70.70 to 71.70): BM016315.D (-666) (-)

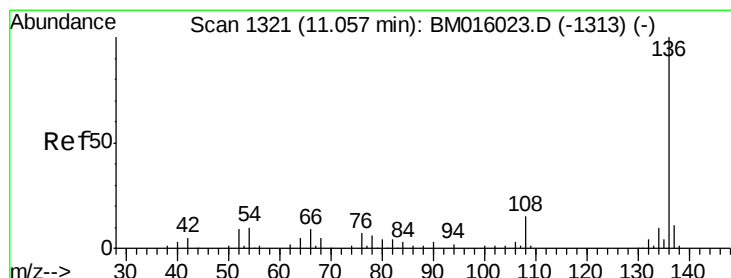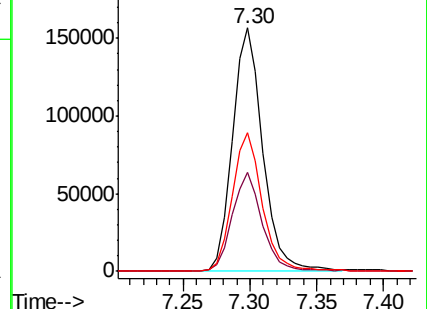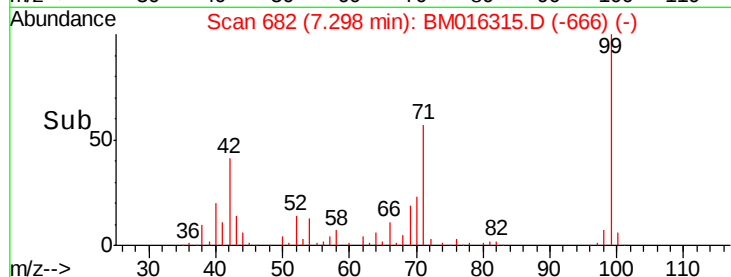

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.94 min Scan# 1301

Delta R.T. -0.01 min

Lab File: BM016315.D

Acq: 11 Aug 2018 02:43

Tgt Ion: 136 Resp: 90570


Ion Ratio Lower Upper

136 100

137 12.6 8.7 13.1

54 10.5 4.6 6.8#

68 2.8 3.7 5.5#


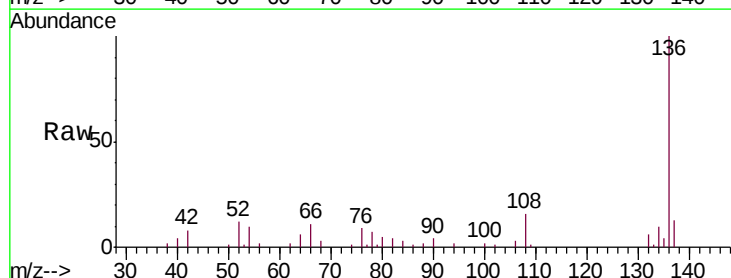



Abundance Ion 136.00 (135.70 to 136.70): BM016315.D (-1286) (-)

Ion 137.00 (136.70 to 137.70): BM016315.D (-1286) (-)

Ion 54.00 (53.70 to 54.70): BM016315.D (-1286) (-)

Ion 68.00 (67.70 to 68.70): BM016315.D (-1286) (-)

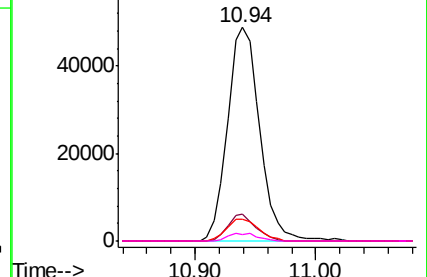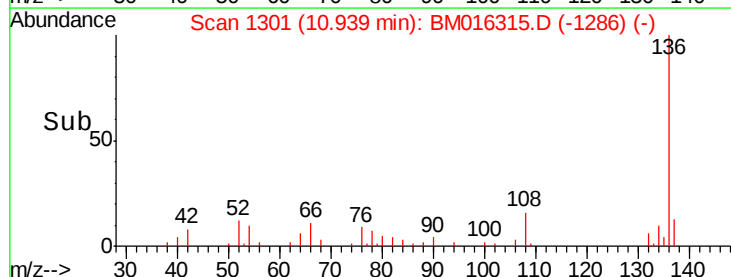


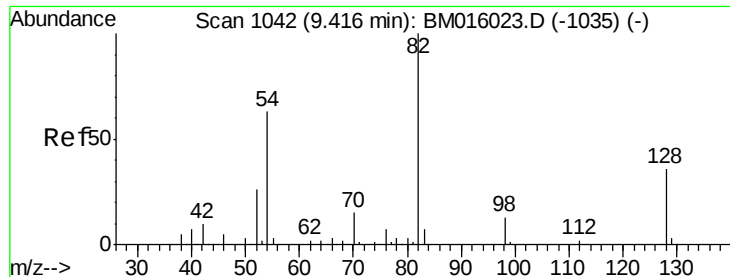




#23  
Nitrobenzene-d5  
Concen: N.D. ng  
RT: 9.31 min Scan# 1024  
Delta R.T. -0.01 min  
Lab File: BM016315.D  
Acq: 11 Aug 2018 02:43

Instrument :  
BNA\_M  
ClientSampleId :  
JC-03-080918-I

Tgt Ion: 82 Resp: 243540  
Ion Ratio Lower Upper  
82 100  
128 35.3 32.8 49.2  
54 63.0 40.6 60.8#

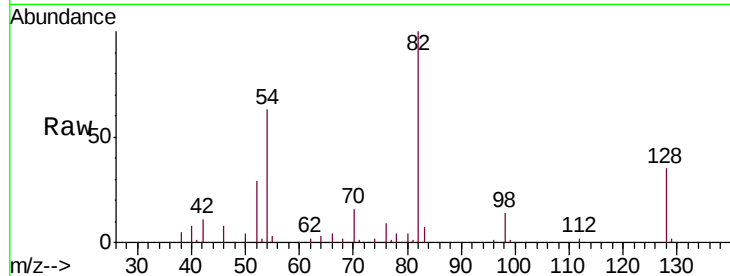


Abundance Ion 82.00 (81.70 to 82.70): BM016315.D (-1009) (-)  
Ion 128.00 (127.70 to 128.70): BM016315.D (-1009) (-)  
Ion 54.00 (53.70 to 54.70): BM016315.D (-1009) (-)

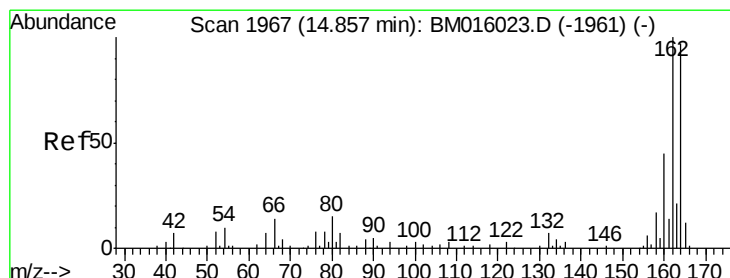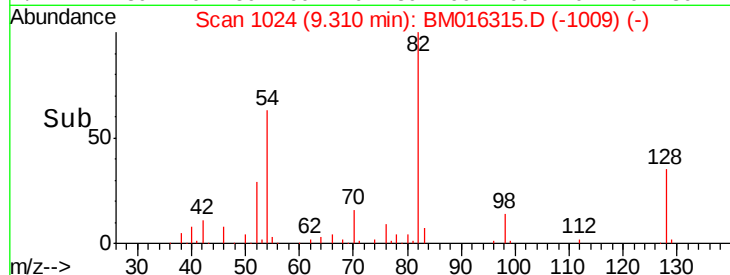
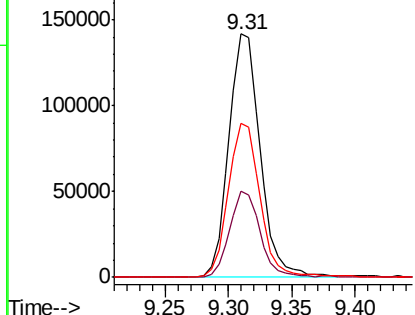



#38  
Acenaphthene-d10  
Concen: 20.000 ng  
RT: 14.76 min Scan# 1950  
Delta R.T. -0.01 min  
Lab File: BM016315.D  
Acq: 11 Aug 2018 02:43

Tgt Ion: 164 Resp: 40624  
Ion Ratio Lower Upper  
164 100  
162 109.6 82.4 123.6  
160 49.8 35.8 53.6

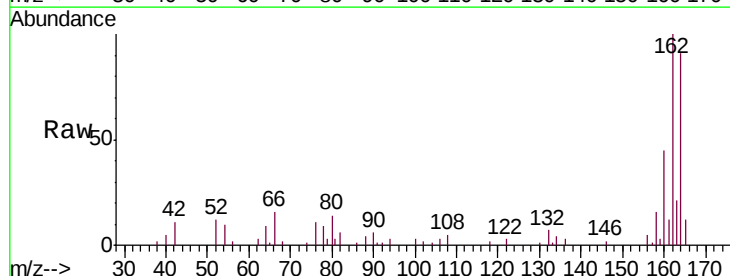

Abundance Ion 164.00 (163.70 to 164.70): BM016315.D (-1935) (-)  
Ion 162.00 (161.70 to 162.70): BM016315.D (-1935) (-)  
Ion 160.00 (159.70 to 160.70): BM016315.D (-1935) (-)

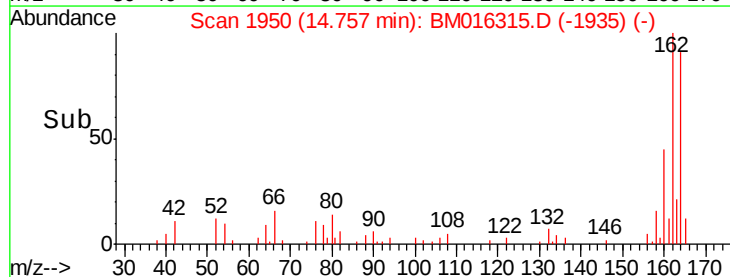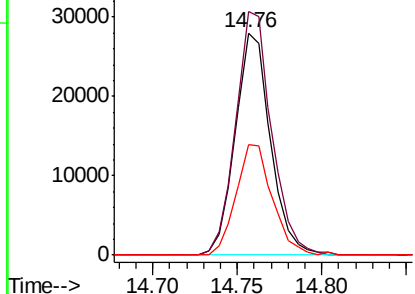


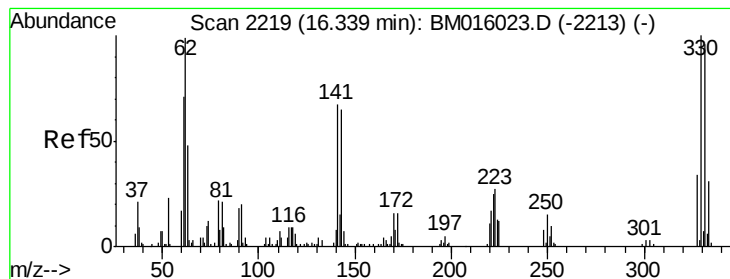




#41  
 2,4,6-Tribromophenol  
 Concen: N.D. ng  
 RT: 16.25 min Scan# 2204  
 Delta R.T. -0.01 min  
 Lab File: BM016315.D  
 Acq: 11 Aug 2018 02:43

Instrument :  
 BNA\_M  
 ClientSampleId :  
 JC-03-080918-I

Tgt Ion: 330 Resp: 74242  
 Ion Ratio Lower Upper  
 330 100  
 332 98.4 0.0 0.0#  
 141 86.7 0.0 0.0#

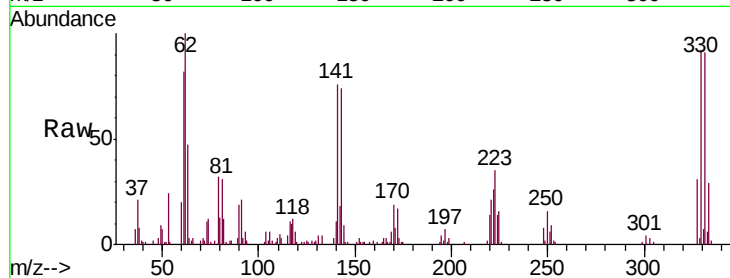


Abundance Ion 329.80 (329.50 to 330.50): E  
 Ion 331.80 (331.50 to 332.50): E  
 Ion 141.00 (140.70 to 141.70): E

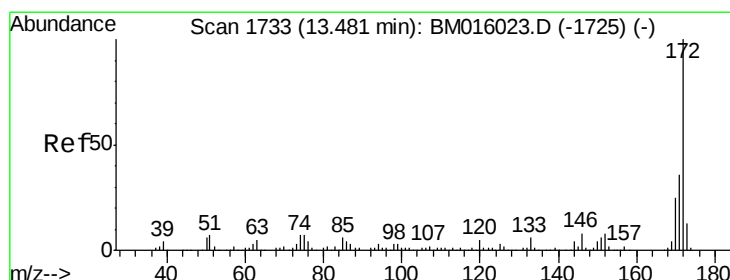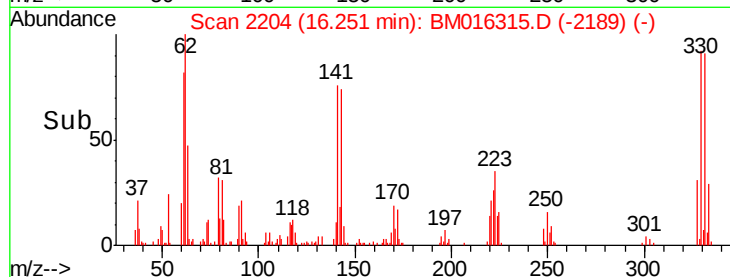
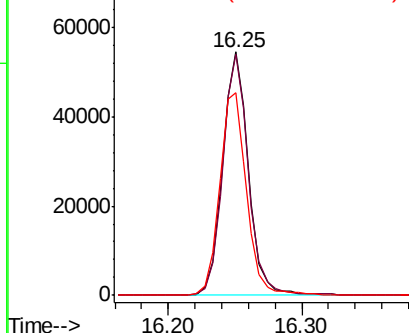



#44  
 2-Fluorobiphenyl  
 Concen: N.D. ng  
 RT: 13.38 min Scan# 1716  
 Delta R.T. -0.01 min  
 Lab File: BM016315.D  
 Acq: 11 Aug 2018 02:43

Tgt Ion: 172 Resp: 416248  
 Ion Ratio Lower Upper  
 172 100  
 171 37.0 28.5 42.7  
 170 24.8 18.8 28.2

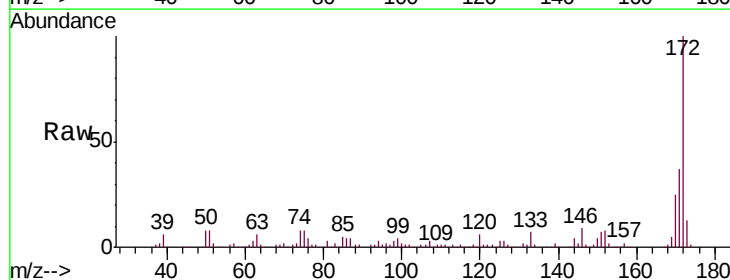

Abundance Ion 172.00 (171.70 to 172.70): E  
 Ion 171.00 (170.70 to 171.70): E  
 Ion 170.00 (169.70 to 170.70): E



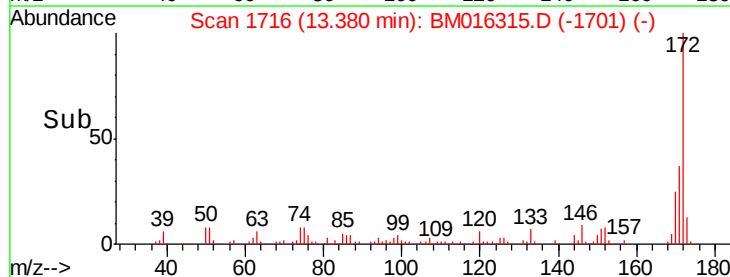
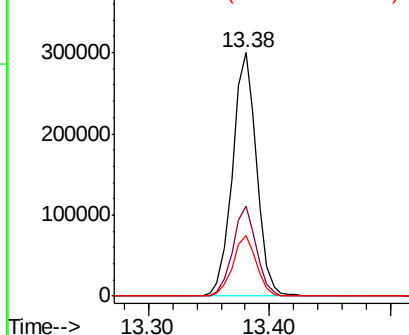


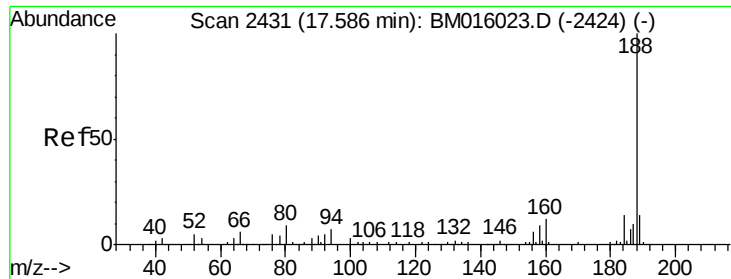

#63  
Phenanthrene-d10  
Concen: 20.000 ng  
RT: 17.50 min Scan# 2416  
Delta R.T. -0.01 min  
Lab File: BM016315.D  
Acq: 11 Aug 2018 02:43




Instrument :  
BNA\_M  
ClientSampleId :  
JC-03-080918-I


Tgt Ion:188 Resp: 77327  
Ion Ratio Lower Upper  
188 100  
94 8.1 8.7 13.1#  
80 7.8 9.3 13.9#

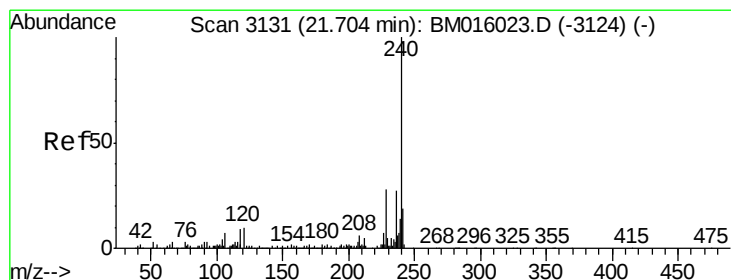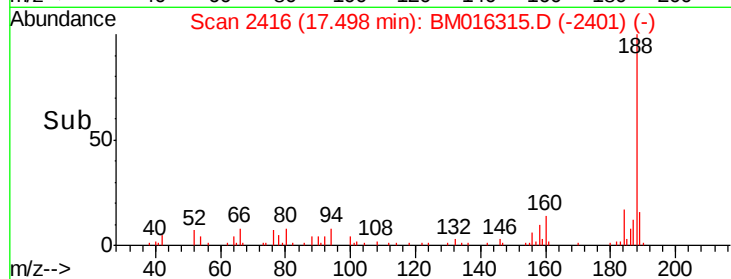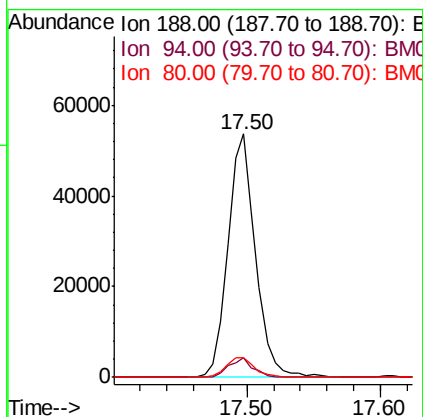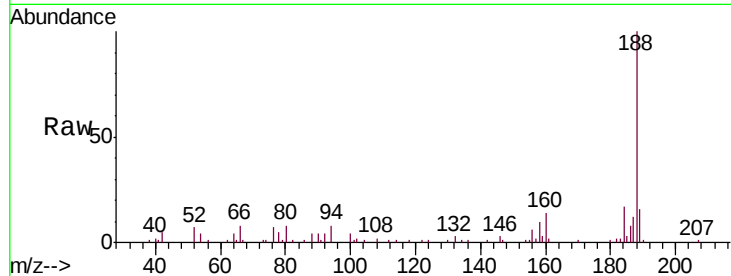

#75  
Chrysene-d12  
Concen: 20.000 ng  
RT: 21.63 min Scan# 3118  
Delta R.T. -0.01 min  
Lab File: BM016315.D  
Acq: 11 Aug 2018 02:43

Tgt Ion:240 Resp: 91786  
Ion Ratio Lower Upper  
240 100  
120 7.0 8.2 12.2#  
236 28.1 20.0 30.0

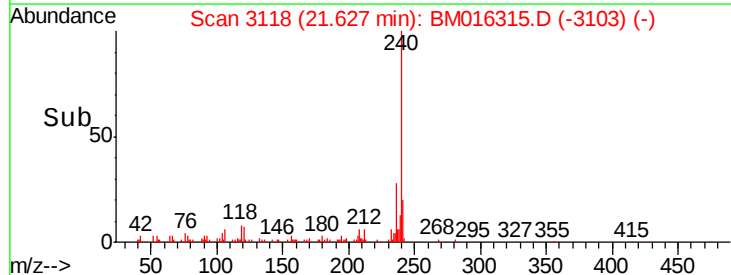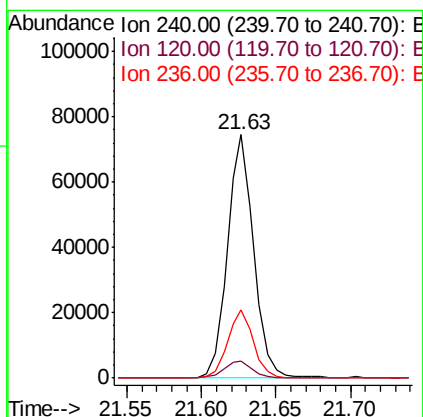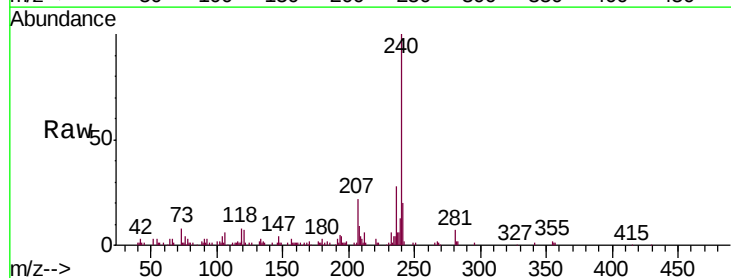

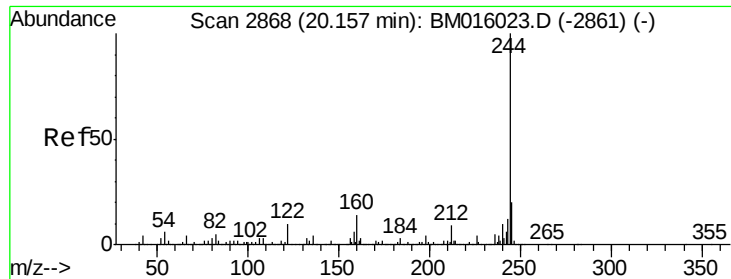

#78

Terphenyl-d14

Concen: N.D. ng

RT: 20.07 min Scan# 2854

Delta R.T. -0.01 min

Lab File: BM016315.D

Acq: 11 Aug 2018 02:43

Instrument :

BNA\_M

ClientSampleId :

JC-03-080918-I


Tgt Ion:244 Resp: 575620

Ion Ratio Lower Upper

244 100

212 10.3 4.9 7.3#




122 9.3 6.2 9.4

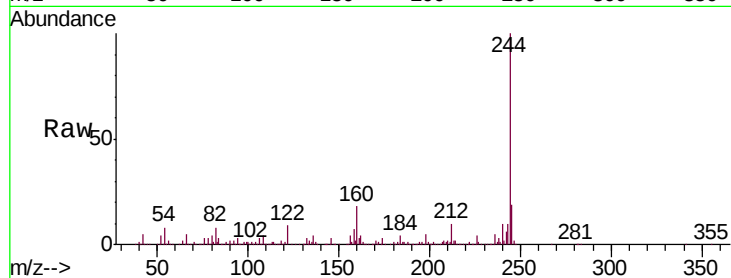

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

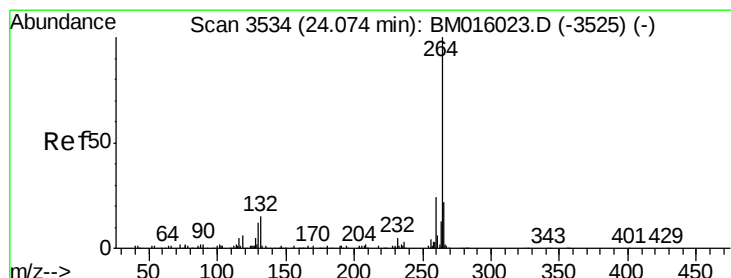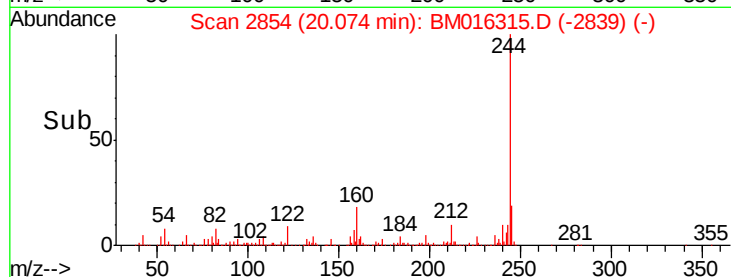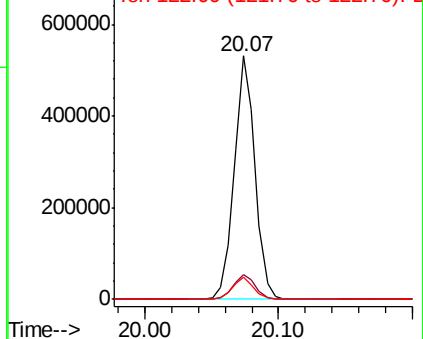

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.96 min Scan# 3514

Delta R.T. -0.02 min

Lab File: BM016315.D

Acq: 11 Aug 2018 02:43


Tgt Ion:264 Resp: 106614

Ion Ratio Lower Upper

264 100

260 26.3 18.6 27.8

265 23.2 17.3 25.9

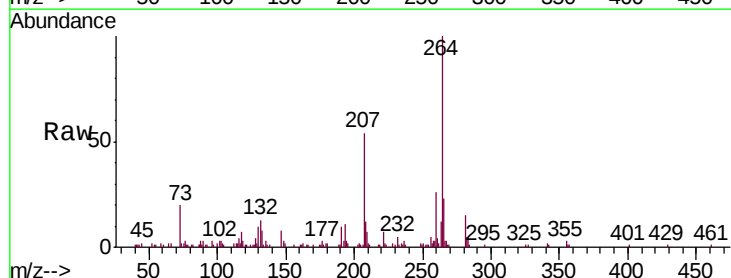

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

