


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081018\
 Data File : BM016297.D
 Acq On : 10 Aug 2018 15:44
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 10 18:44:22 2018

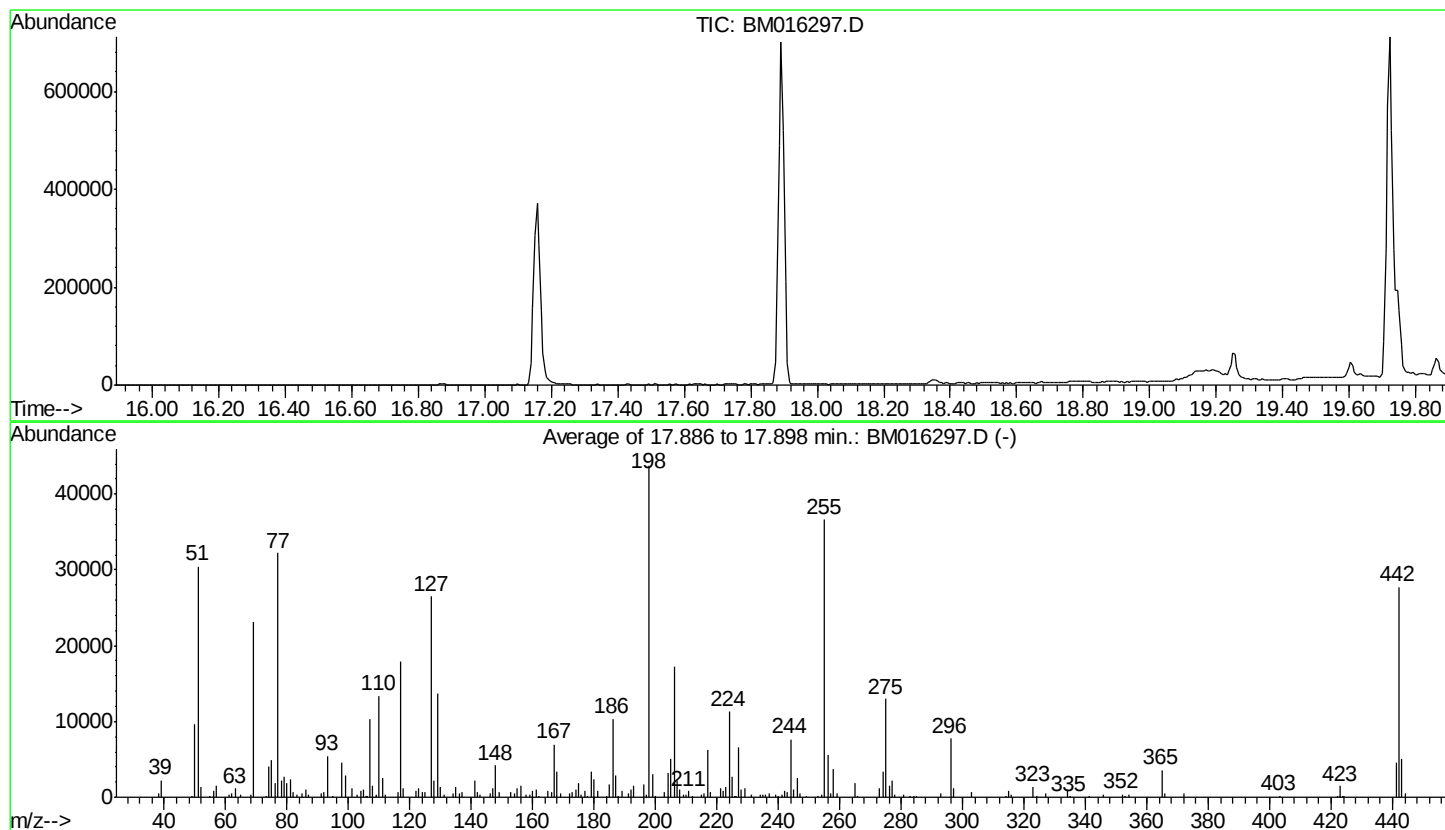

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.5	30434	PASS
68	69	0.00	2	1.4	326	PASS
69	198	0.00	100	52.8	23101	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	60.5	26456	PASS
197	198	0.00	2	0.7	289	PASS
198	198	100	100	100.0	43760	PASS
199	198	5	9	7.0	3071	PASS
275	198	10	60	29.7	12996	PASS
365	198	1	100	8.2	3570	PASS
441	198	0.01	100	10.4	4543	PASS
442	198	50	100	63.4	27749	PASS
443	442	15	24	18.3	5089	PASS