
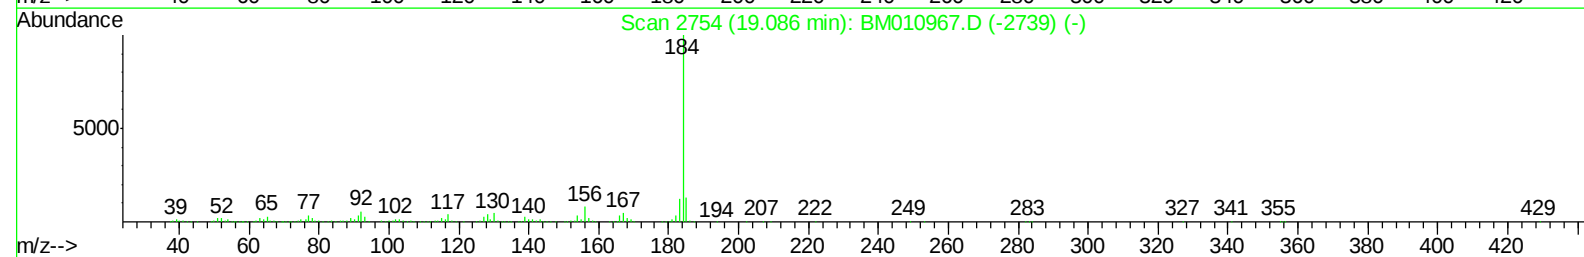
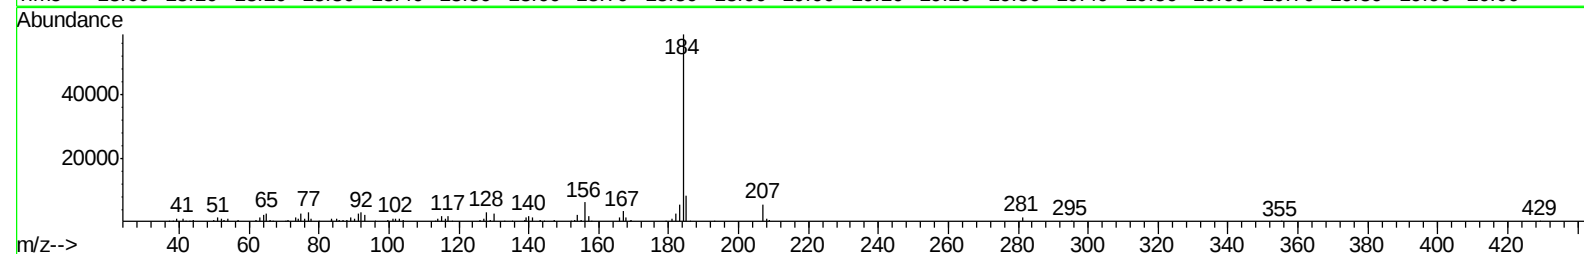


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081117\
Data File : BM011198.D
Acq On : 11 Aug 2017 11:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 00:22:36 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

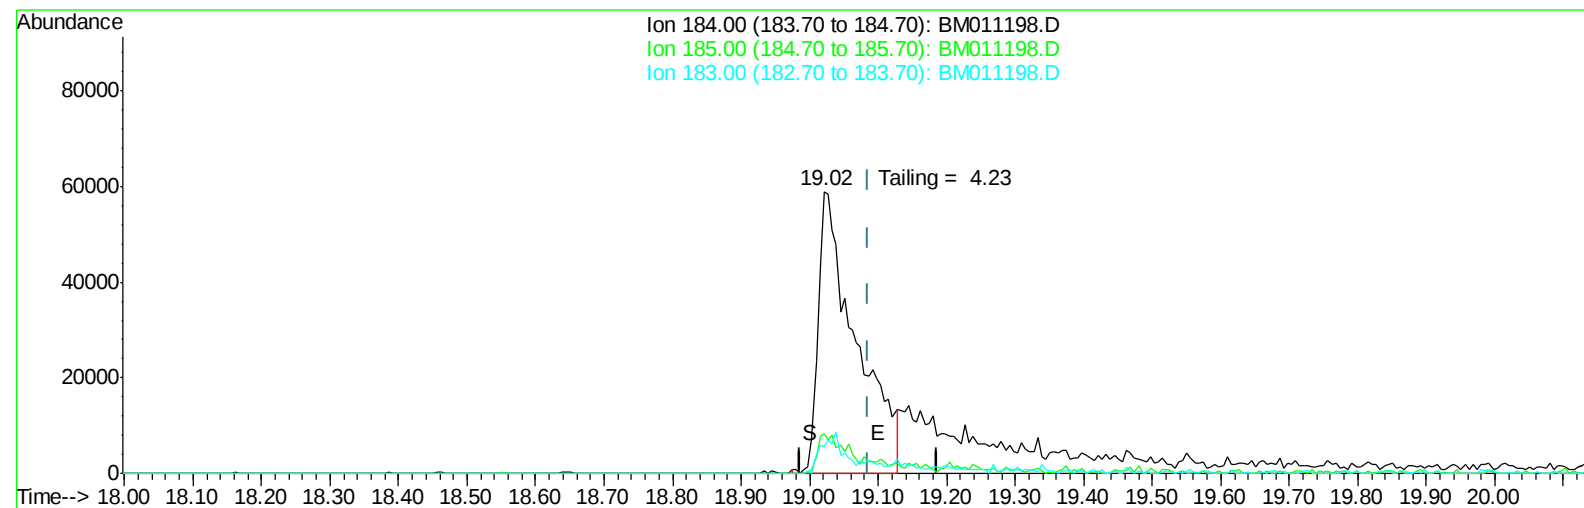

TIC: BM011198.D

(76) Benzidine




19.021min (-0.065) 0.00ng

response 217149

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.93
183.00	11.10	9.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081117\
Data File : BM011198.D
Acq On : 11 Aug 2017 11:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 00:22:36 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

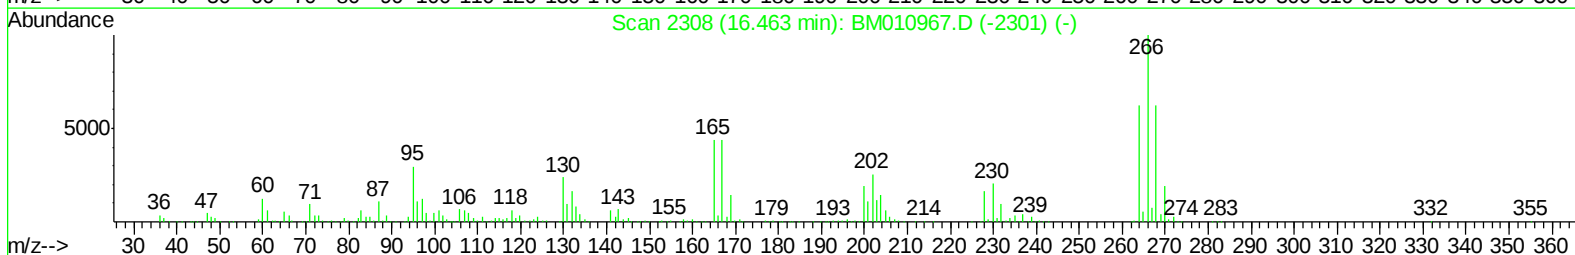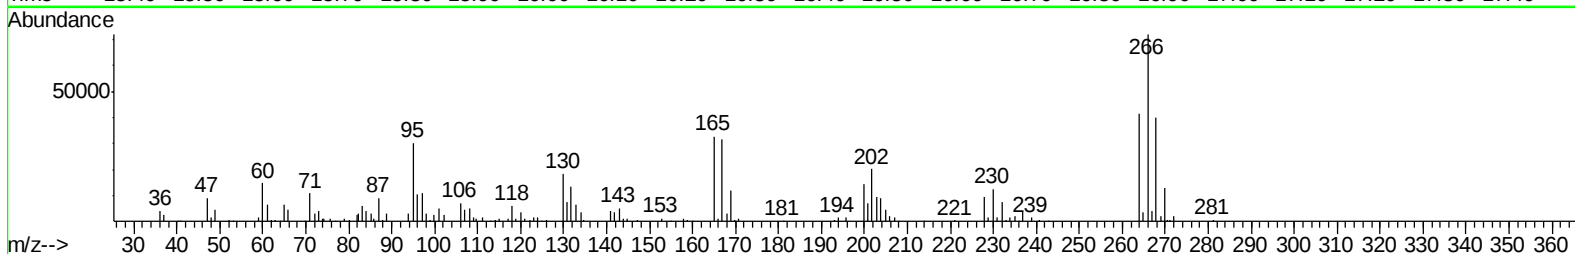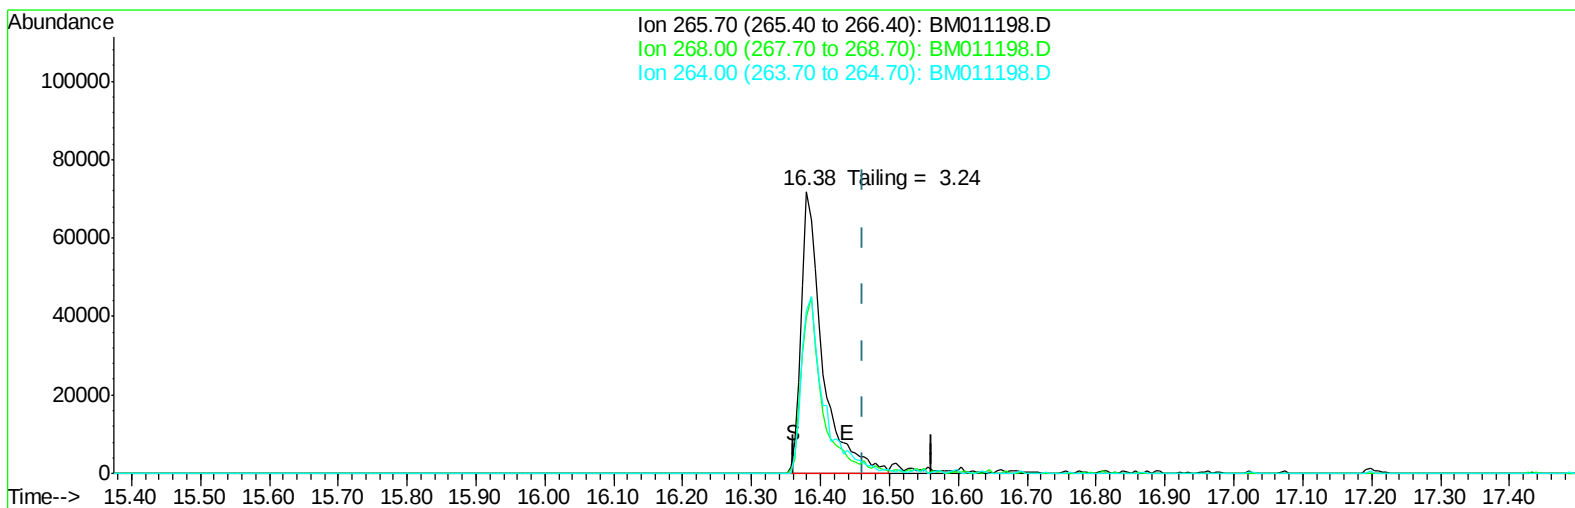

TIC: BM011198.D

(69) Pentachlorophenol (C)

16.380min (-0.082) 0.00ng

response 119485

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	55.53
264.00	61.20	63.22
0.00	0.00	0.00