


Data Path : Z:\HPCHEM1\BNA M\Data\BM081117\
 Data File : BM011198.D
 Acq On : 11 Aug 2017 11:44
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

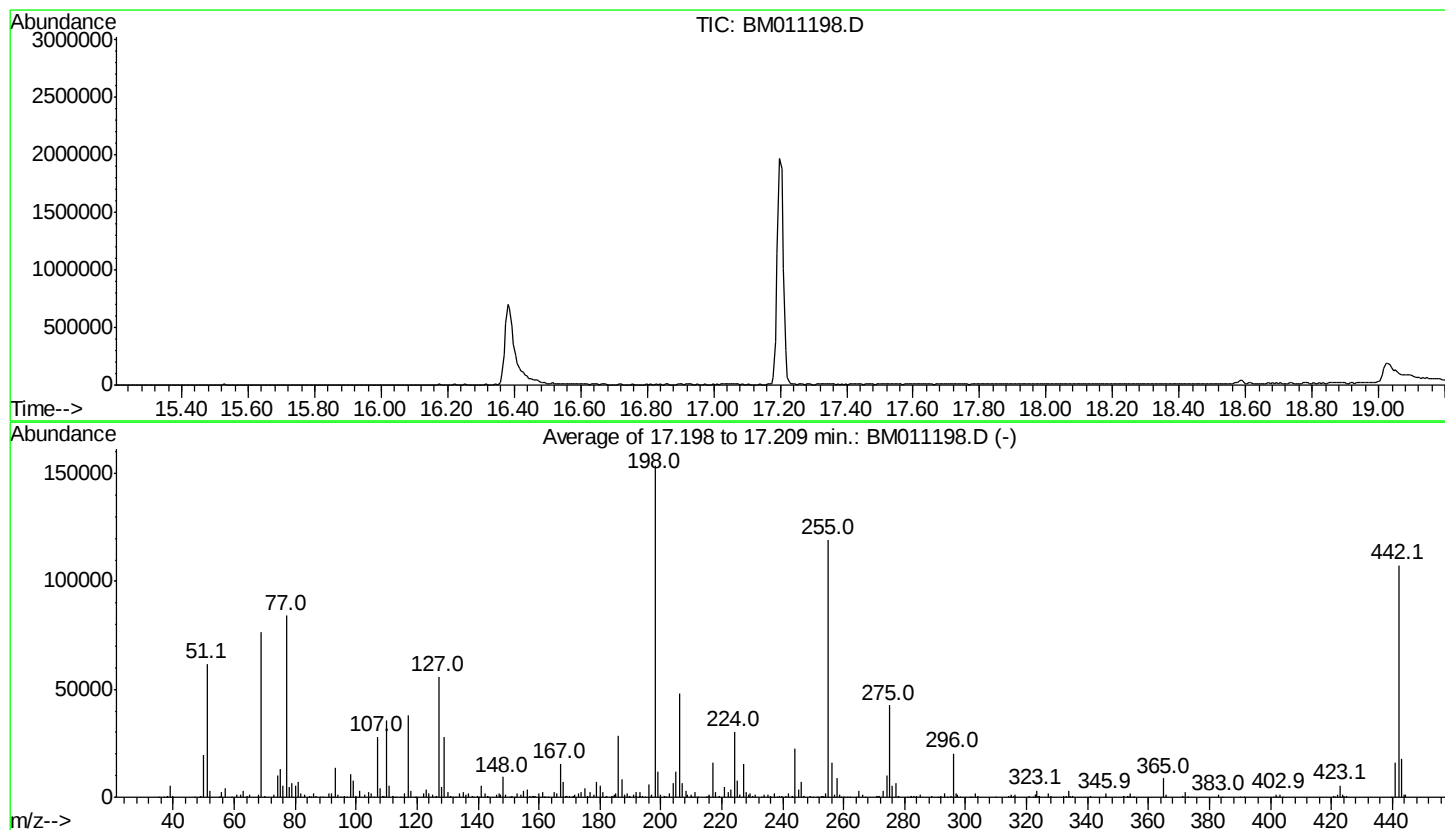

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	61704	PASS
68	69	0.00	2	1.4	1040	PASS
69	198	0.00	100	49.7	76362	PASS
70	69	0.00	2	0.5	385	PASS
127	198	10	80	36.4	55928	PASS
197	198	0.00	2	0.6	986	PASS
198	198	100	100	100.0	153674	PASS
199	198	5	9	7.7	11768	PASS
275	198	10	60	27.8	42648	PASS
365	198	1	100	5.7	8707	PASS
441	442	0.01	24	15.1	16256	PASS
442	198	50	100	70.0	107570	PASS
443	442	15	24	16.3	17579	PASS