

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081120\
 Data File : BM027034.D
 Acq On : 11 Aug 2020 17:26
 Operator : JU/CG
 Sample : L3636-12
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFMN9

Quant Time: Aug 11 18:01:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 11 17:05:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	69871	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	244253	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	154587	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	351049	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	384420	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	409430	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	9045	5.88	ng/uL	0.00
5) Phenol-d5	6.82	99	31054	5.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	92039	24.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	86186	20.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	53801	12.70	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	48762	25.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	50609	25.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	105059	24.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	9434	1.92	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	369984	30.01	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	416604	28.36	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	8970	4.31	ng/ul	0.00
58) Fluorene-d10	15.27	176	330404	30.75	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	50158	26.16	ng/ul	0.00
71) Anthracene-d10	17.12	188	566123	32.73	ng/ul	0.00
79) Pyrene-d10	19.42	212	650364	33.92	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	730273	31.95	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.74	163	57195	4.427	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081120\
Data File : BM027034.D
Acq On : 11 Aug 2020 17:26
Operator : JU/CG
Sample : L3636-12
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFMN9

Quant Time: Aug 11 18:01:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 11 17:05:07 2020
Response via : Initial Calibration

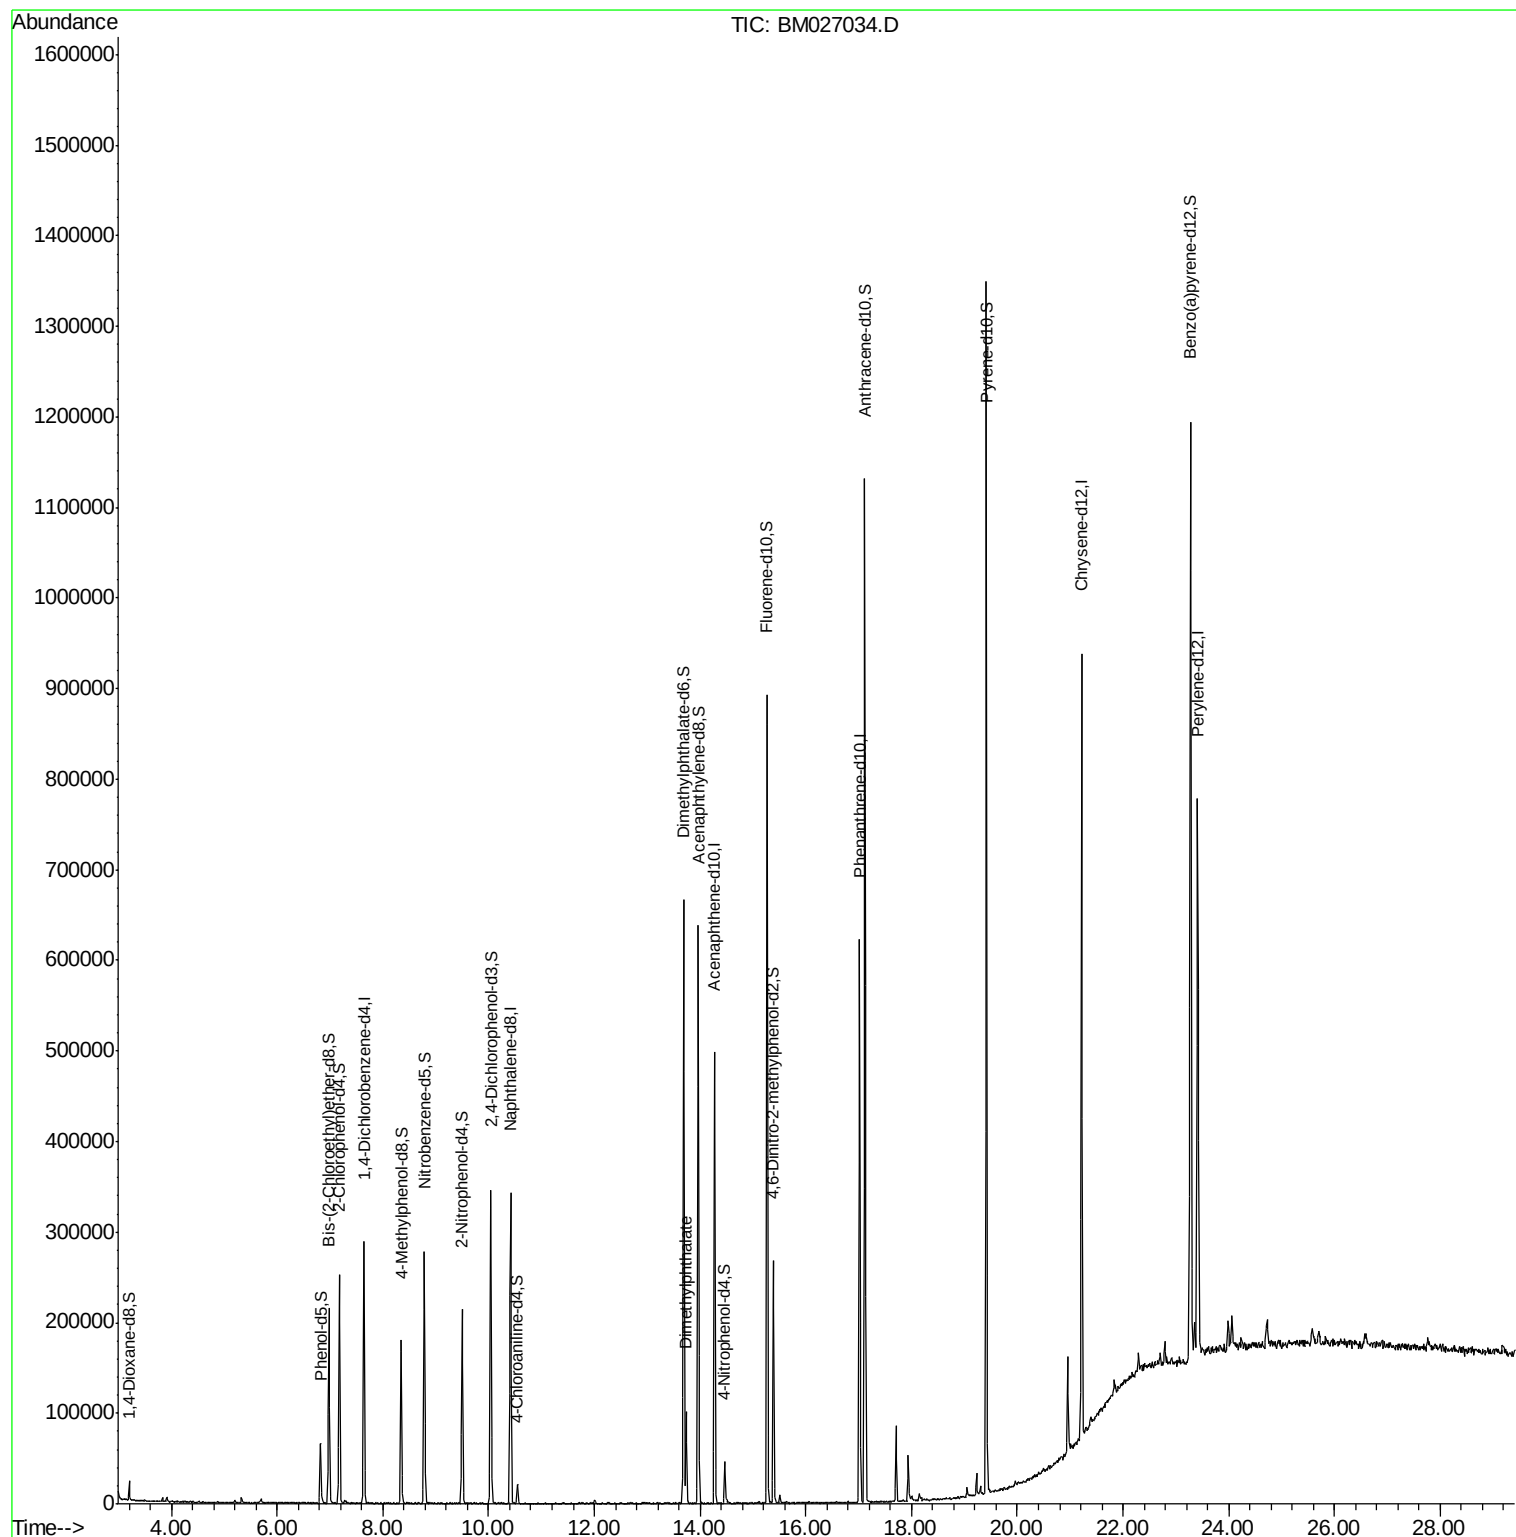

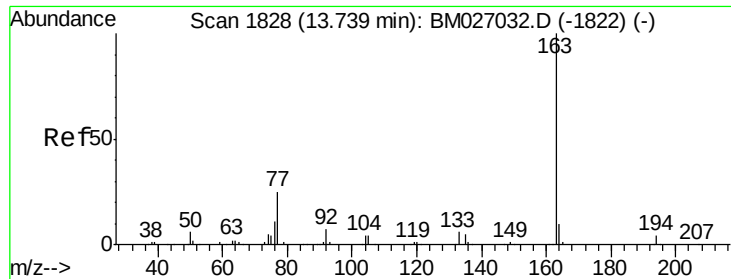

#45

Dimethylphthalate

Concen: 4.427 ng/ul

RT: 13.74 min Scan# 1828

Delta R.T. -0.00 min

Lab File: BM027034.D

Acq: 11 Aug 2020 17:26

Instrument :

BNA_M

ClientSampleId :

BFMN9


Tot Ion:163 Resp: 57195

Ion Ratio Lower Upper

163 100

194 3.7 3.2 4.8

164 9.7 8.2 12.2

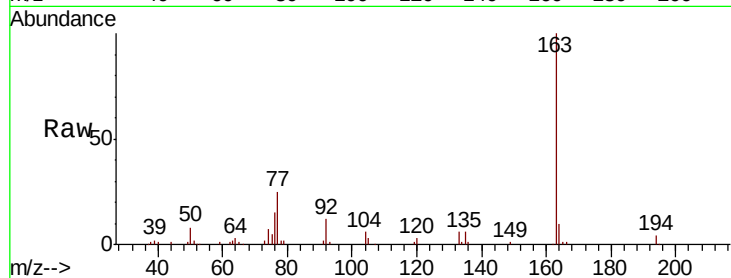

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

