

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081120\
 Data File : BM027035.D
 Acq On : 11 Aug 2020 18:03
 Operator : JU/CG
 Sample : L3636-13
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFMP0

Quant Time: Aug 11 18:35:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 11 17:05:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	65615	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	235135	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	150852	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	325426	20.00	ng/ul	0.00
78) Chrysene-d12	21.21	240	346608	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	378892	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	8904	6.17	ng/uL	0.00
5) Phenol-d5	6.82	99	34057	6.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	97373	27.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	94452	23.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	58858	14.80	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	52235	28.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	54237	28.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	112399	27.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	8184	1.73	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	369765	30.74	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	450520	31.43	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	9937	4.89	ng/ul	0.00
58) Fluorene-d10	15.27	176	337748	32.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	48680	27.39	ng/ul	0.00
71) Anthracene-d10	17.12	188	559678	34.91	ng/ul	0.00
79) Pyrene-d10	19.42	212	633998	36.67	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.28	264	714318	33.77	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.74	163	62867	4.987	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081120\
Data File : BM027035.D
Acq On : 11 Aug 2020 18:03
Operator : JU/CG
Sample : L3636-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFMP0

Quant Time: Aug 11 18:35:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 11 17:05:07 2020
Response via : Initial Calibration

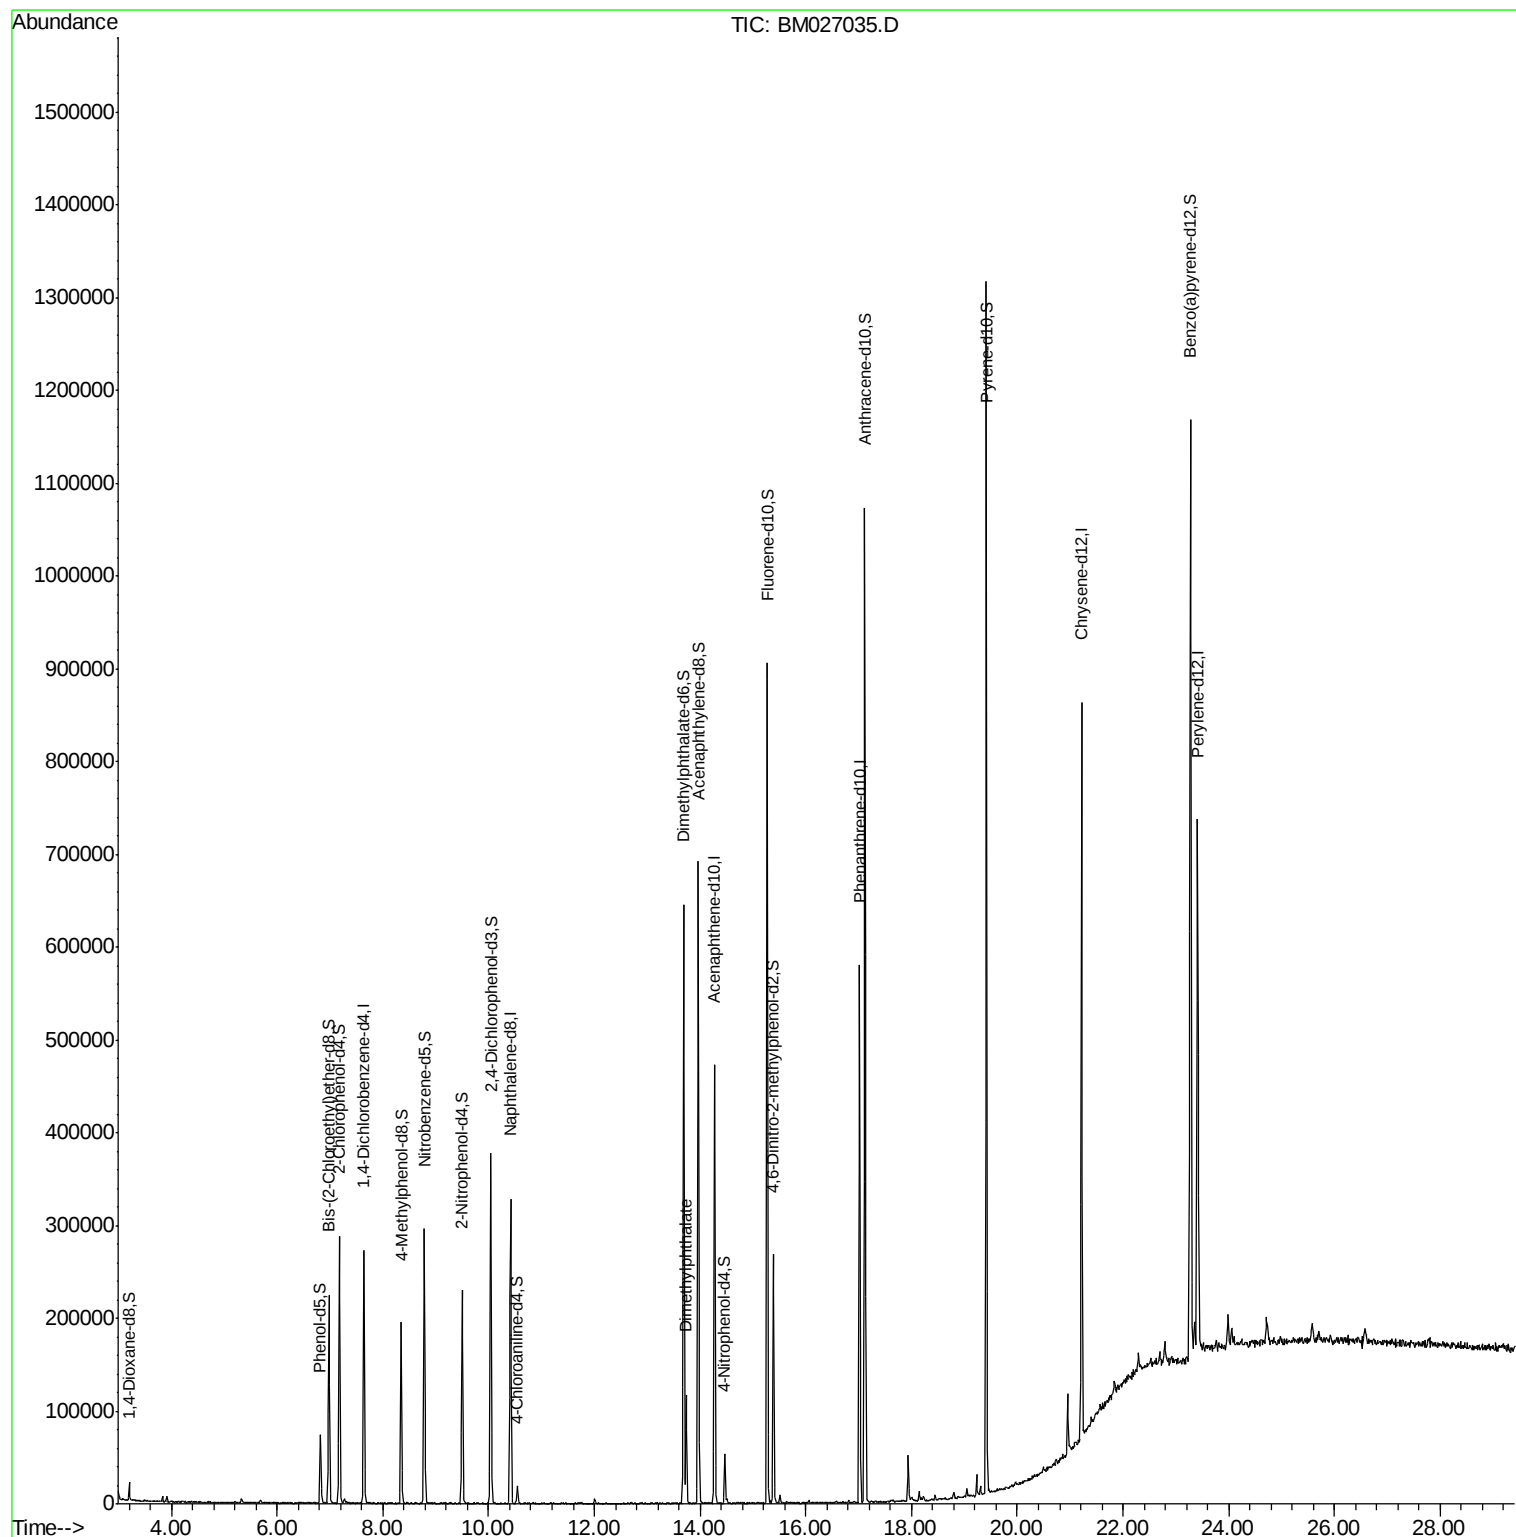

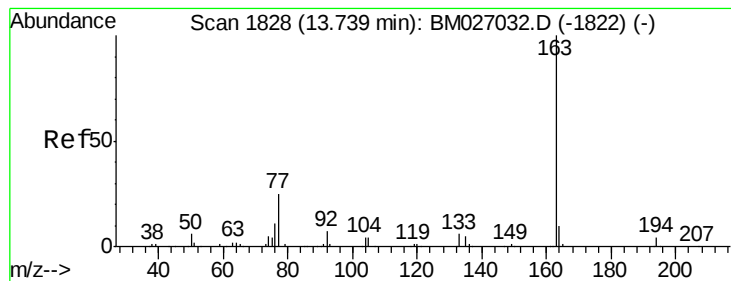

#45

Dimethylphthalate

Concen: 4.987 ng/ul

RT: 13.74 min Scan# 1828

Delta R.T. -0.00 min

Lab File: BM027035.D

Acq: 11 Aug 2020 18:03

Instrument :

BNA_M

ClientSampleId :

BFMP0


Tot Ion:163 Resp: 62867

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 9.1 8.2 12.2

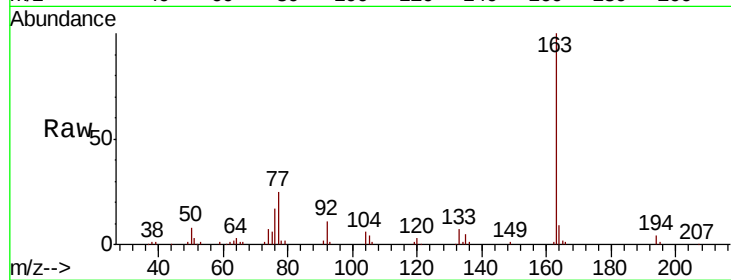

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

