

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081121\
 Data File : BM031663.D
 Acq On : 11 Aug 2021 16:53
 Operator : CG/JU
 Sample : M3246-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA7

Quant Time: Aug 11 17:30:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 11 16:24:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.573	152	1242	0.400	ng/ul	0.00
4) Naphthalene-d8	10.334	136	4738	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.209	164	2811	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.957	188	5151	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.159	240	3984	0.400	ng/ul	# 0.00
23) Perylene-d12	23.319	264	3984	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.182	96	5027	3.644	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.930	152	1740	0.218	ng/ul	0.00
18) Fluoranthene-d10	18.993	212	3145	0.237	ng/ul	0.00
Target Compounds						
						Qvalue
10) Acenaphthylene	13.927	152	362	0.030	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081121\
Data File : BM031663.D
Acq On : 11 Aug 2021 16:53
Operator : CG/JU
Sample : M3246-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA7


Quant Time: Aug 11 17:30:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 11 16:24:11 2021
Response via : Initial Calibration

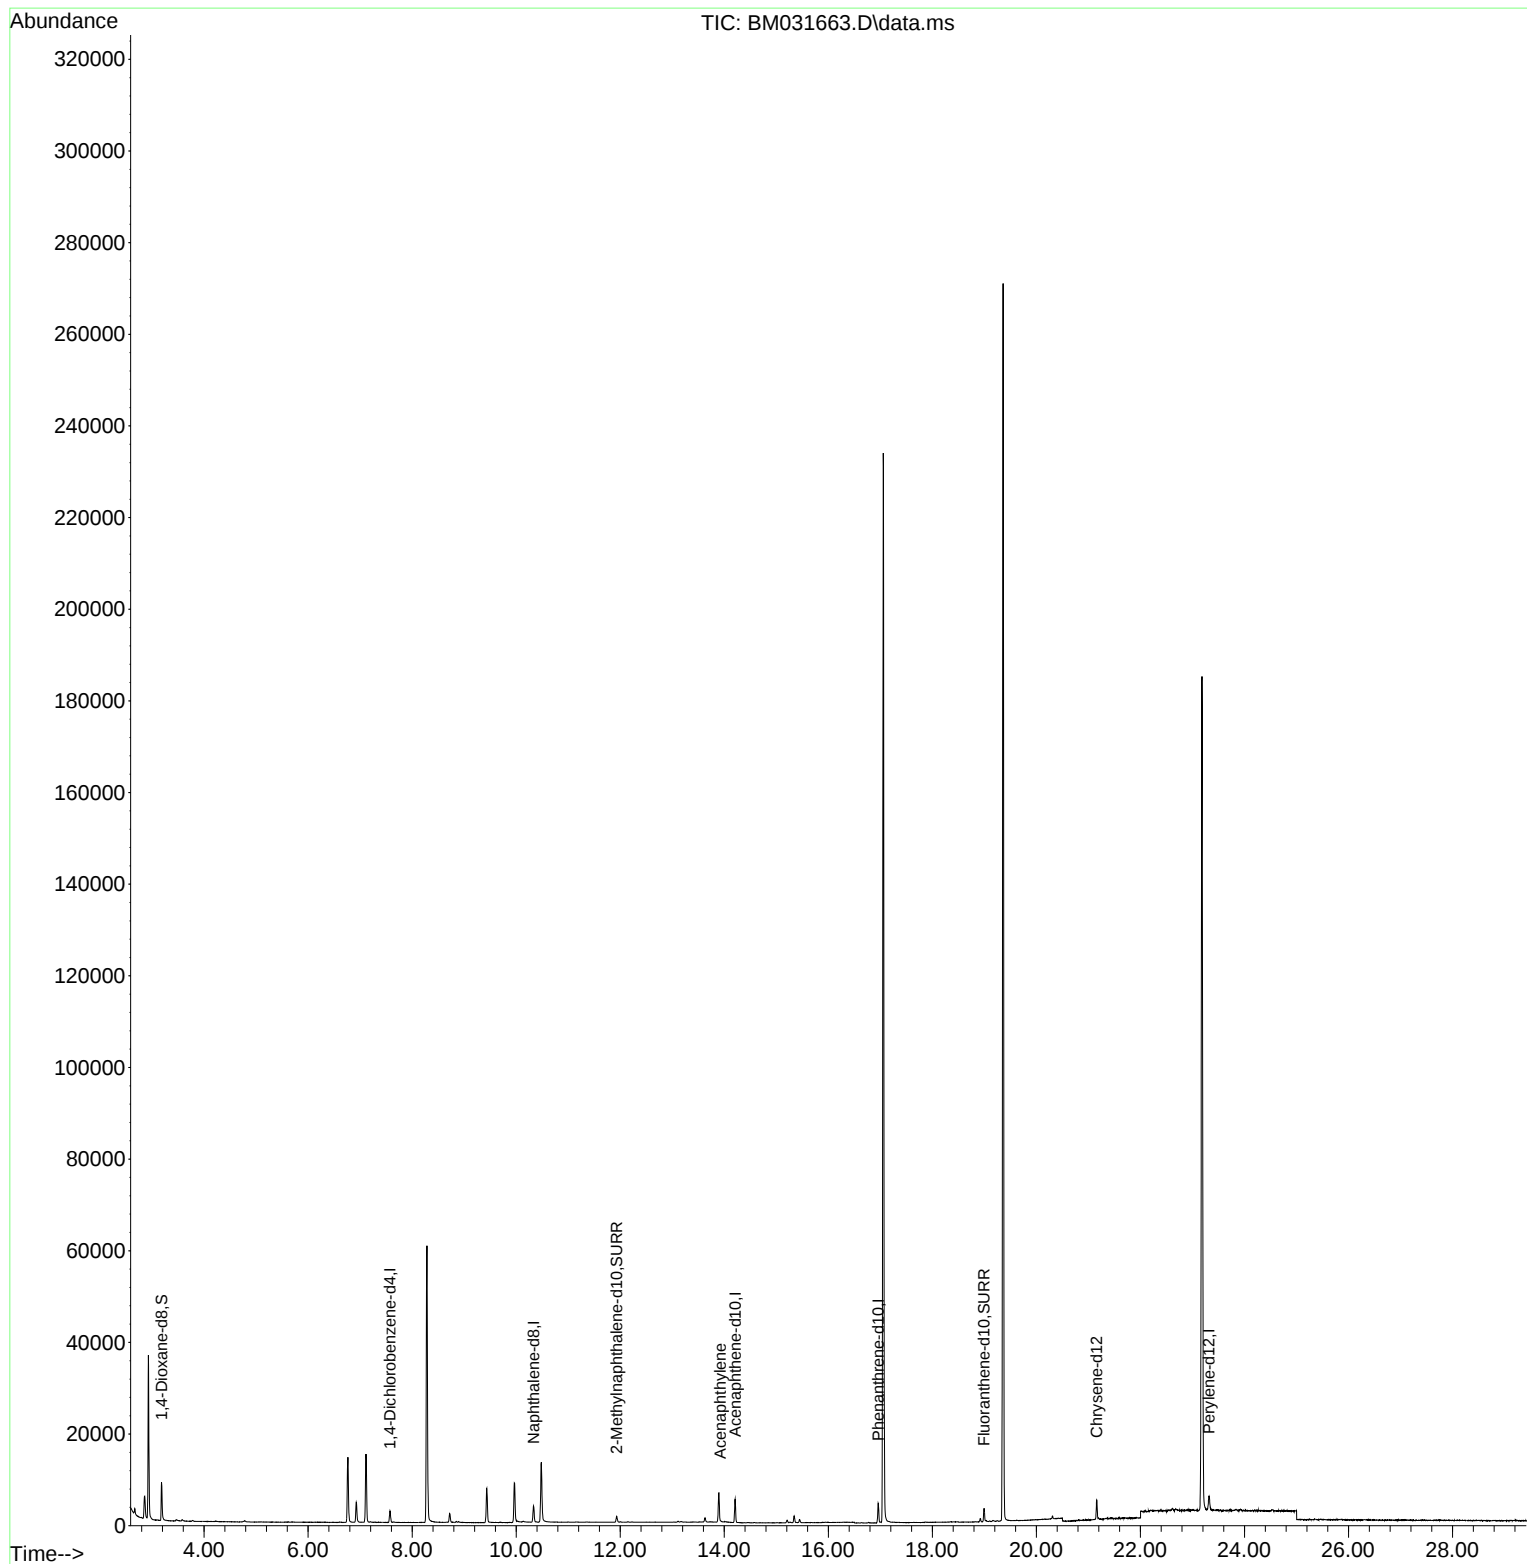

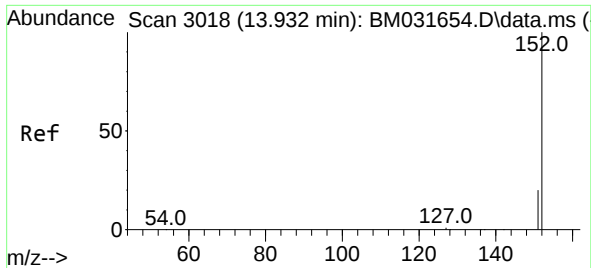

#10
Acenaphthylene
Concen: 0.030 ng/ul
RT: 13.927 min Scan# 3017
Delta R.T. -0.004 min
Lab File: BM031663.D
Acq: 11 Aug 2021 16:53

Instrument :
BNA_M
ClientSampleId :
C0AA7

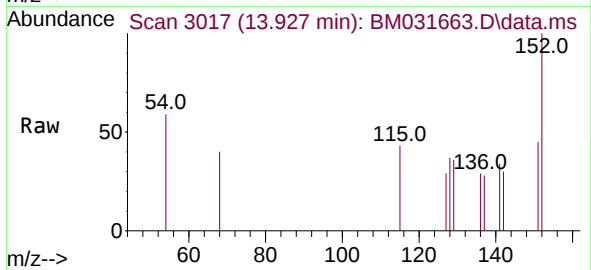

Tgt Ion:	152	Resp:	362
Ion	Ratio	Lower	Upper
152	100		
151	44.9	16.9	25.3#
153	0.0	0.0	0.0

