
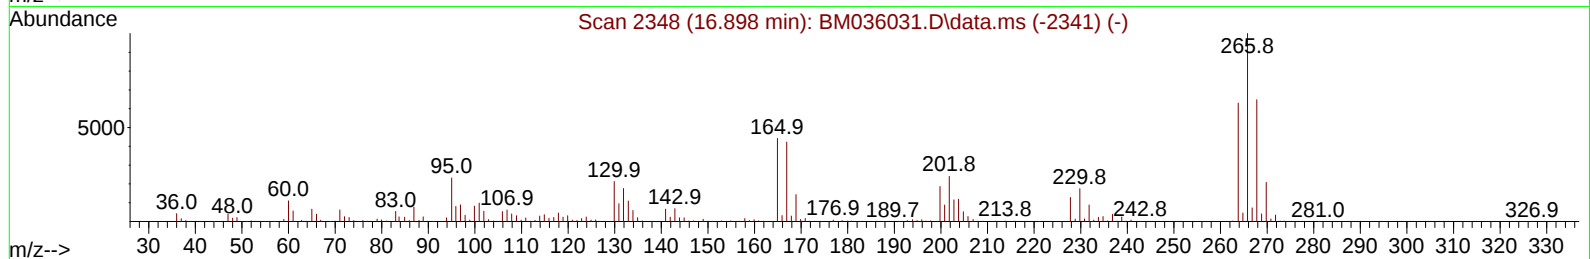
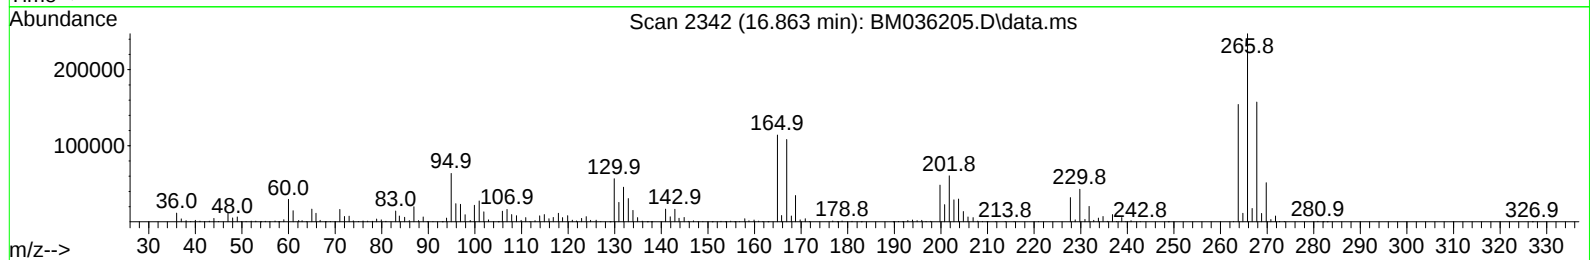


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081122\
Data File : BM036205.D
Acq On : 11 Aug 2022 11:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 08:52:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 10 22:19:26 2022
Response via : Initial Calibration

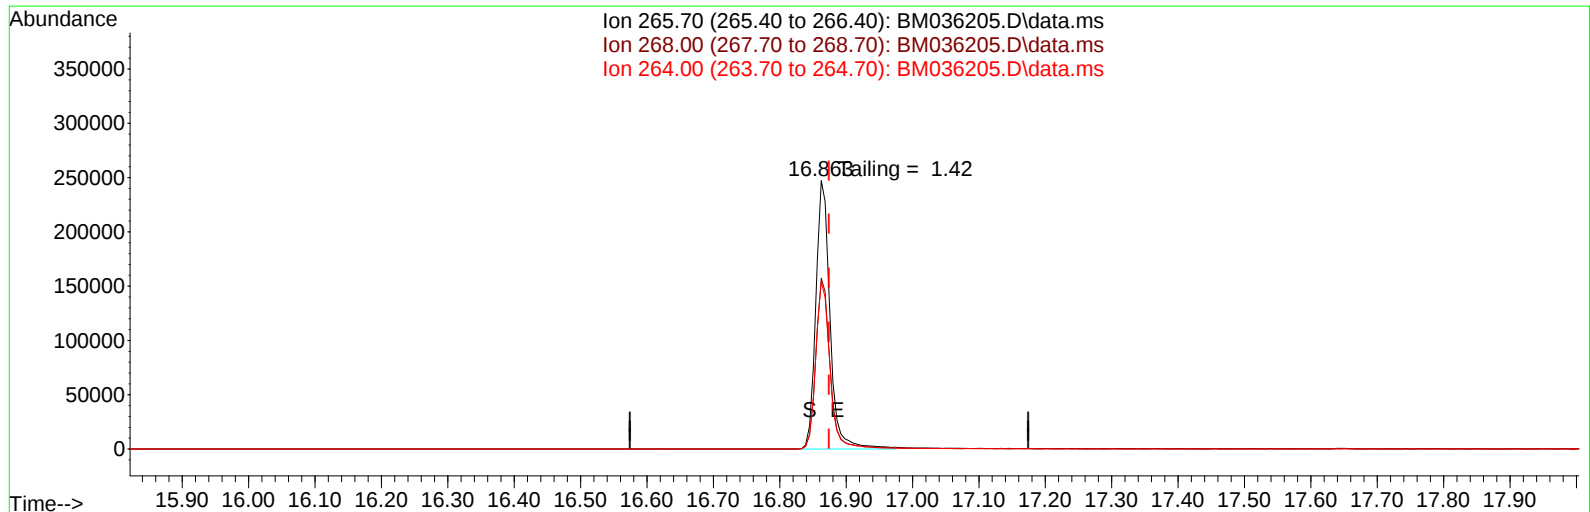

TIC: BM036205.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.012) 69158.25 ng

response 371418

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.70
264.00	63.30	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081122\
Data File : BM036205.D
Acq On : 11 Aug 2022 11:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 12 08:52:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 10 22:19:26 2022
Response via : Initial Calibration

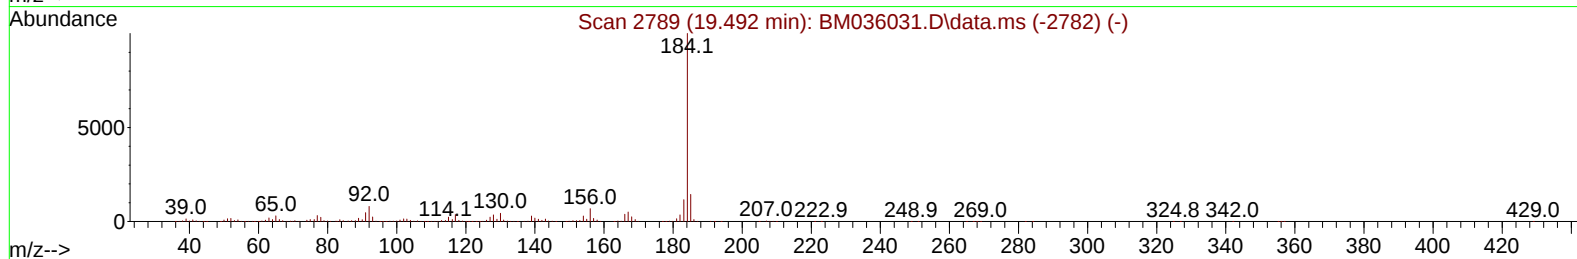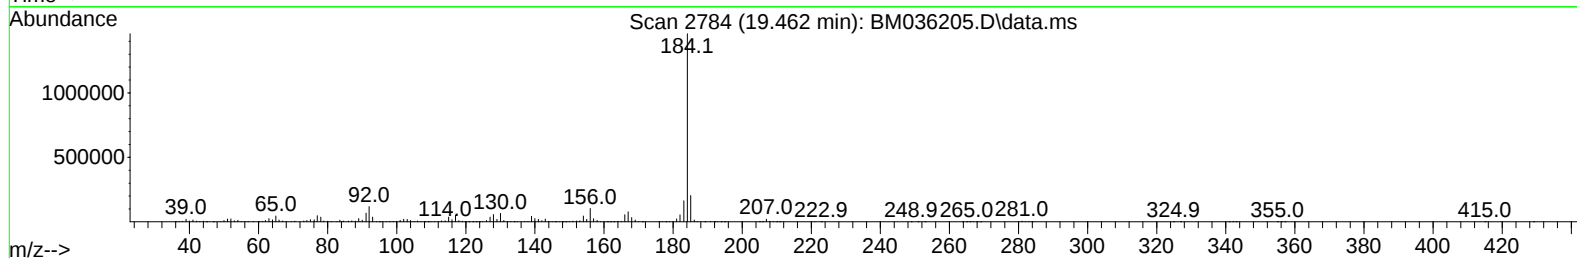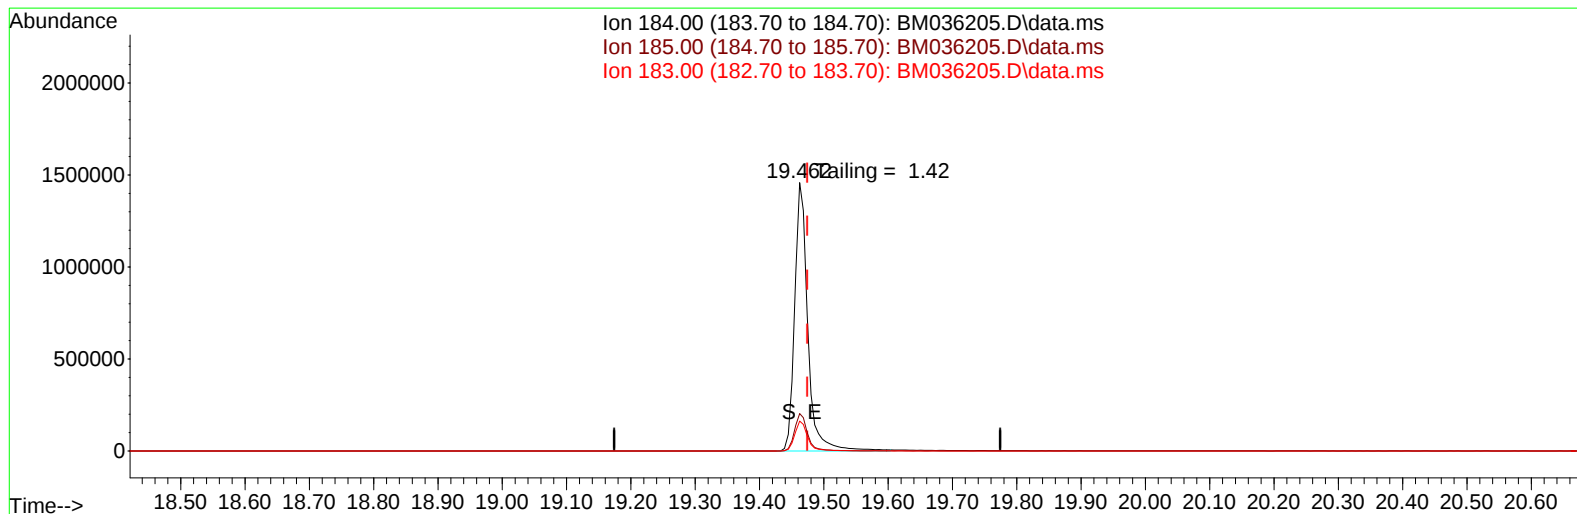

TIC: BM036205.D\data.ms

(77) Benzidine**19.462min (-0.012) 45344.90 ng****response 2089082**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.95
183.00	11.90	11.15
0.00	0.00	0.00