

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081122\
 Data File : BM036221.D
 Acq On : 11 Aug 2022 22:26
 Operator : CG/JU
 Sample : N4143-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 RB-21204

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.410	388	395	409	rVB	5045220	7378284	58.02%	8.227%
2	7.028	662	670	683	rBV	4932466	7848126	61.71%	8.751%
3	7.822	793	805	813	rBV	1141922	1846638	14.52%	2.059%
4	8.998	997	1005	1017	rBV	3283043	5333795	41.94%	5.947%
5	10.628	1275	1282	1295	rBV	1711474	2809757	22.09%	3.133%
6	12.316	1563	1569	1573	rBV	290949	609538	4.79%	0.680%
7	12.769	1643	1646	1651	rBV5	147472	341661	2.69%	0.381%
8	12.904	1665	1669	1674	rBV4	176963	351212	2.76%	0.392%
9	13.098	1695	1702	1709	rBV	8542252	12717072	100.00%	14.180%
10	13.245	1723	1727	1733	rBV2	560779	974677	7.66%	1.087%
11	13.880	1831	1835	1840	rBV	1807488	2669150	20.99%	2.976%
12	14.004	1852	1856	1864	rVB3	1212363	2111750	16.61%	2.355%
13	14.122	1872	1876	1880	rBV3	1192742	1837130	14.45%	2.048%
14	14.210	1885	1891	1895	rBV4	2398418	5057832	39.77%	5.640%
15	14.292	1901	1905	1911	rVB	3980025	5918764	46.54%	6.600%
16	14.427	1924	1928	1932	rBV3	2657868	4867931	38.28%	5.428%
17	14.469	1932	1935	1943	rVB2	3371596	5616414	44.16%	6.262%
18	14.557	1945	1950	1955	rBV2	2224637	5149220	40.49%	5.741%
19	15.263	2066	2070	2076	rBV2	5803488	8485628	66.73%	9.462%
20	23.756	3510	3514	3519	rVB2	1422716	2424853	19.07%	2.704%
21	27.068	4070	4077	4094	rVB3	1632226	5335078	41.95%	5.949%




Sum of corrected areas: 89684510

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081122\
Data File : BM036221.D
Acq On : 11 Aug 2022 22:26
Operator : CG/JU
Sample : N4143-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RB-21204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

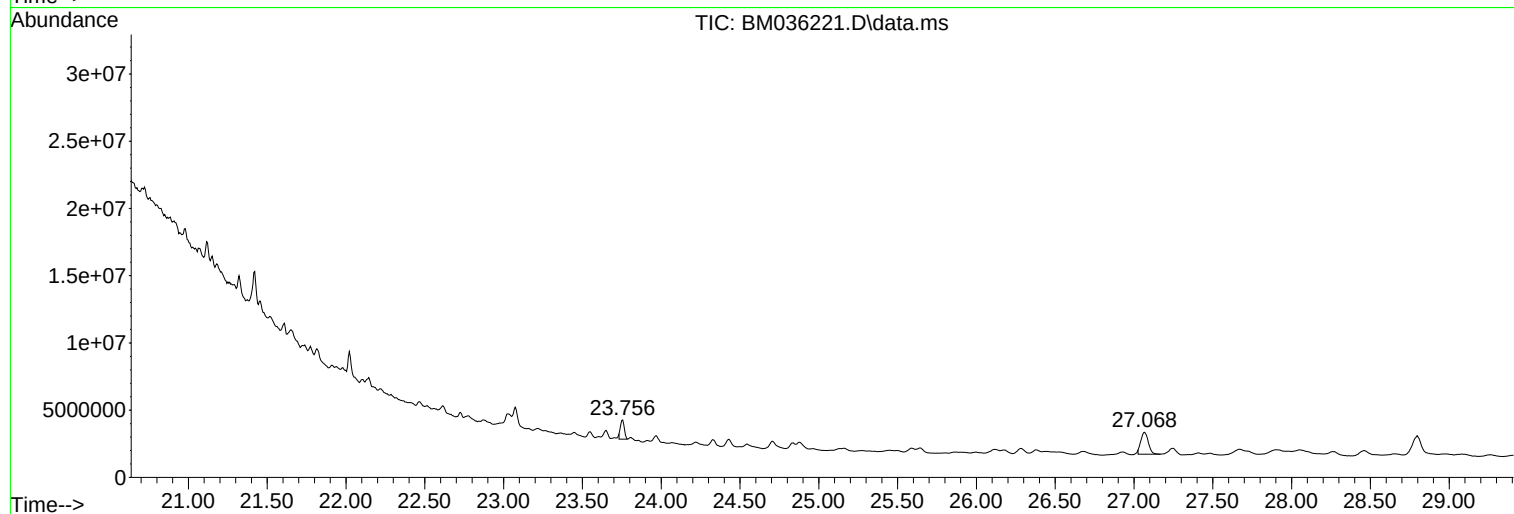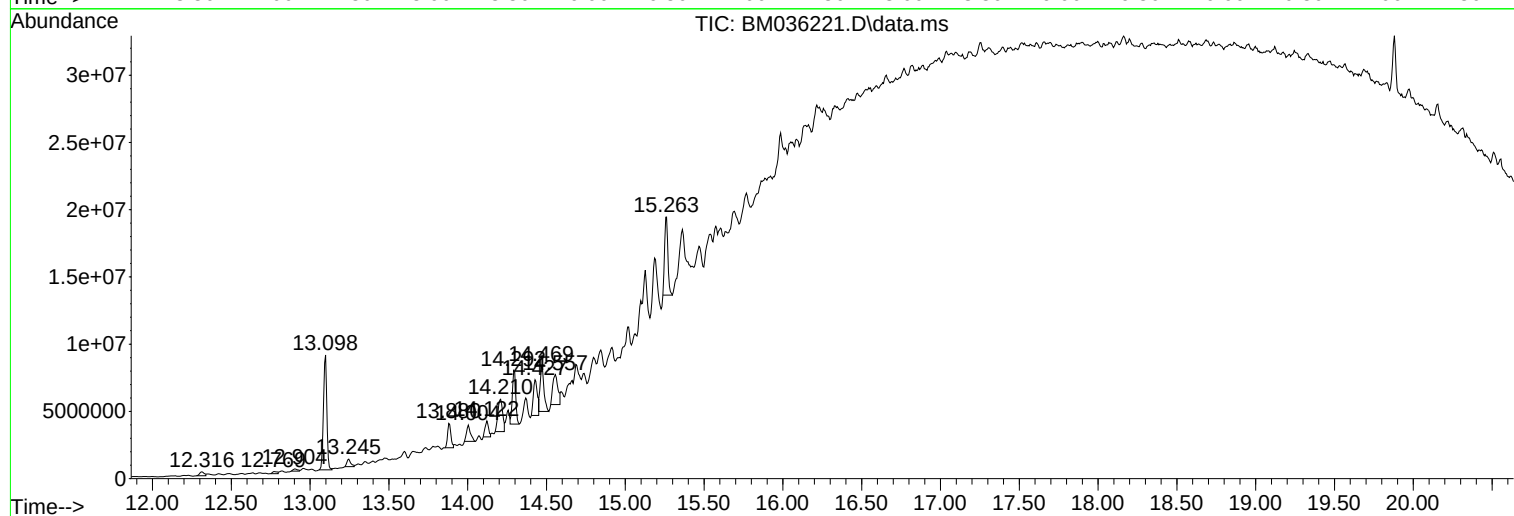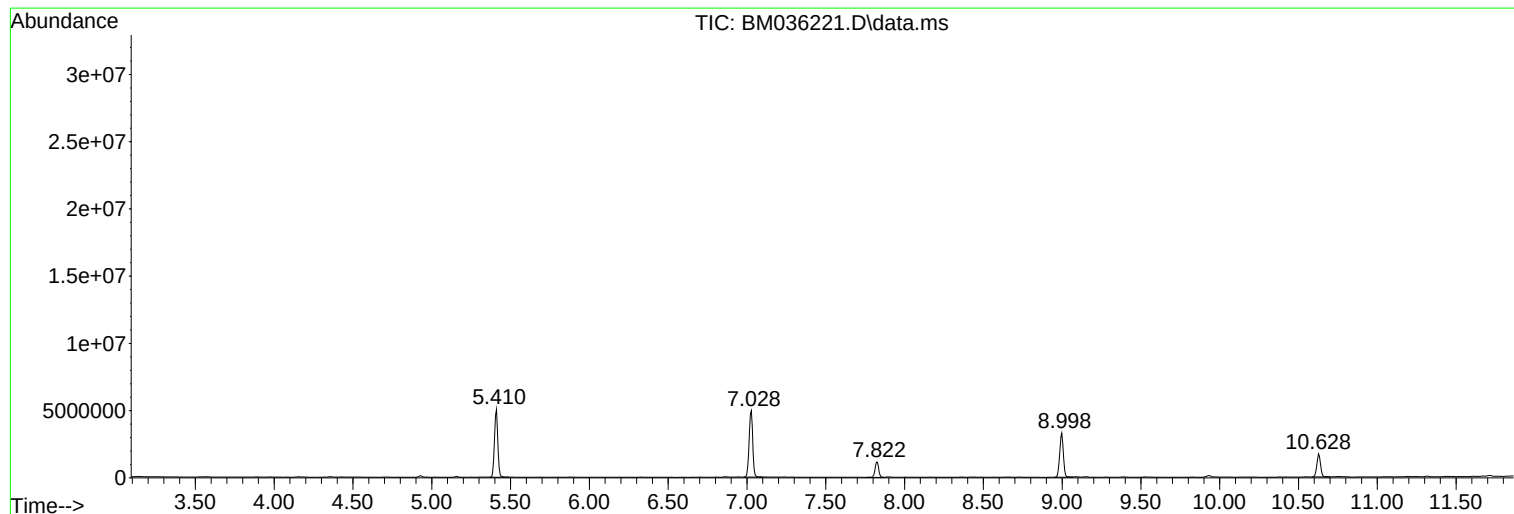

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081122\
Data File : BM036221.D
Acq On : 11 Aug 2022 22:26
Operator : CG/JU
Sample : N4143-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RB-21204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081122\
Data File : BM036221.D
Acq On : 11 Aug 2022 22:26
Operator : CG/JU
Sample : N4143-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RB-21204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------