
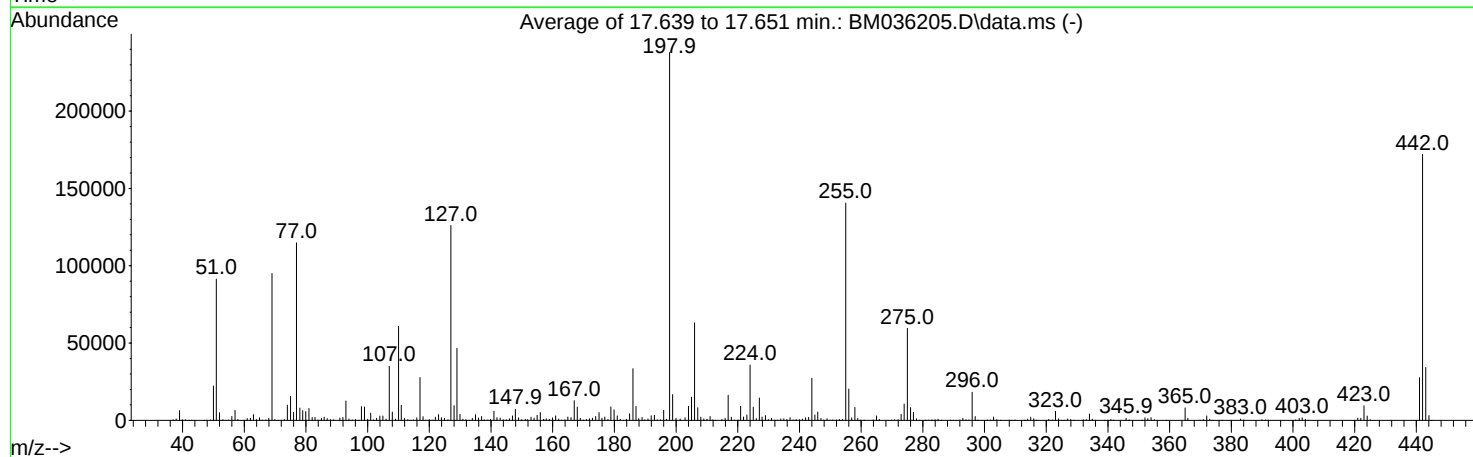


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081122\
 Data File : BM036205.D
 Acq On : 11 Aug 2022 11:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 10 22:19:26 2022

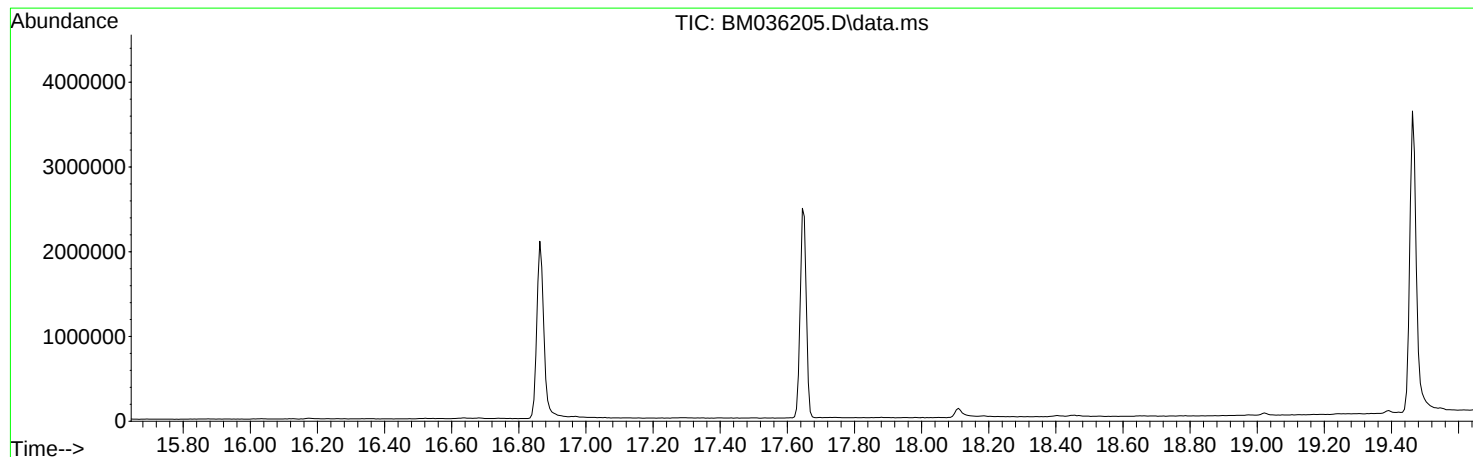




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	91378	PASS
68	69	0.00	2	1.4	1374	PASS
69	198	0.00	100	39.9	95047	PASS
70	69	0.00	2	0.6	543	PASS
127	198	10	80	53.0	126013	PASS
197	198	0.00	2	0.3	724	PASS
198	198	100	100	100.0	237931	PASS
199	198	5	9	7.0	16620	PASS
275	198	10	60	25.0	59496	PASS
365	198	1	100	3.4	8027	PASS
441	198	0.01	100	11.6	27589	PASS
442	442	50	100	100.0	171976	PASS
443	442	15	24	19.9	34253	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081122\
 Data File : BM036205.D
 Acq On : 11 Aug 2022 11:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 12 08:52:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 10 22:19:26 2022
 Response via : Initial Calibration

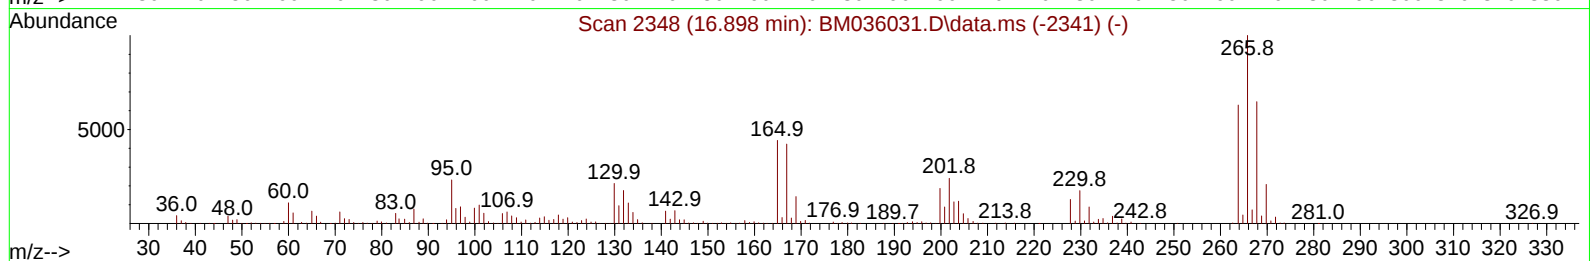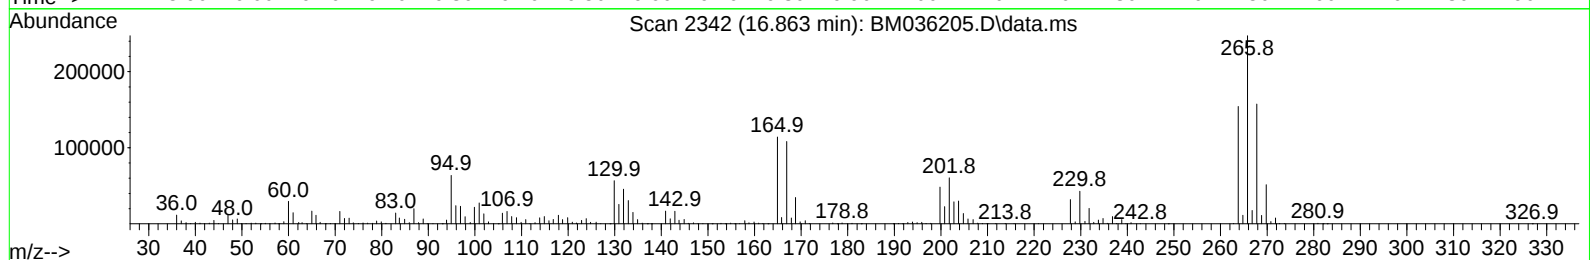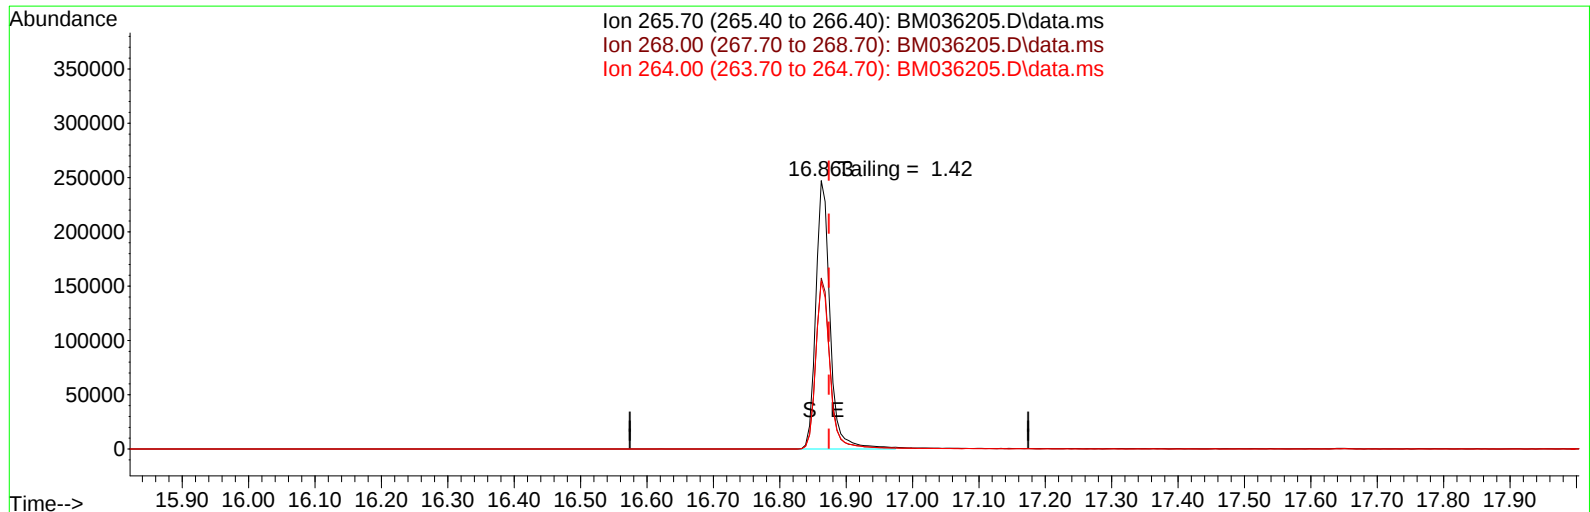

TIC: BM036205.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.012) 69158.25 ng




response 371418

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.70
264.00	63.30	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081122\
Data File : BM036205.D
Acq On : 11 Aug 2022 11:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 12 08:52:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 10 22:19:26 2022
Response via : Initial Calibration

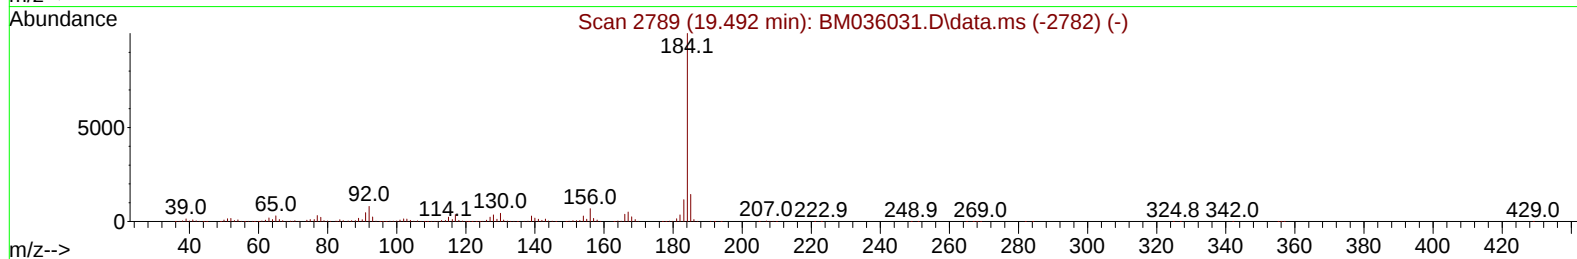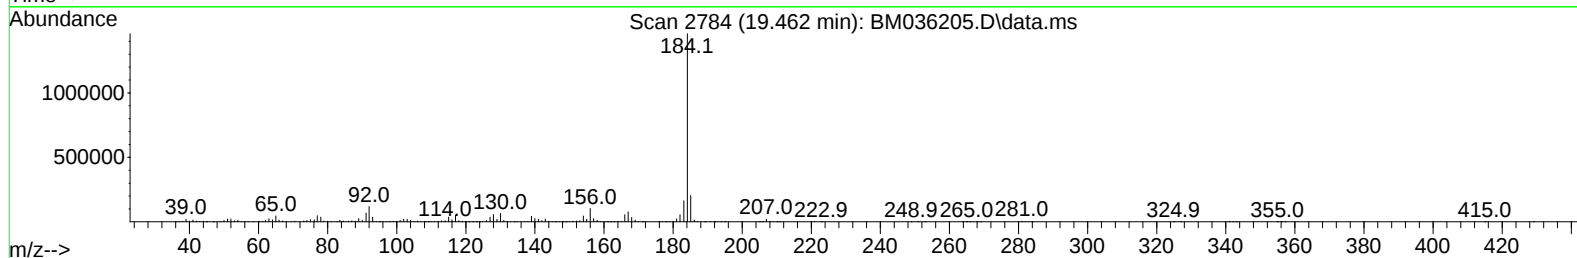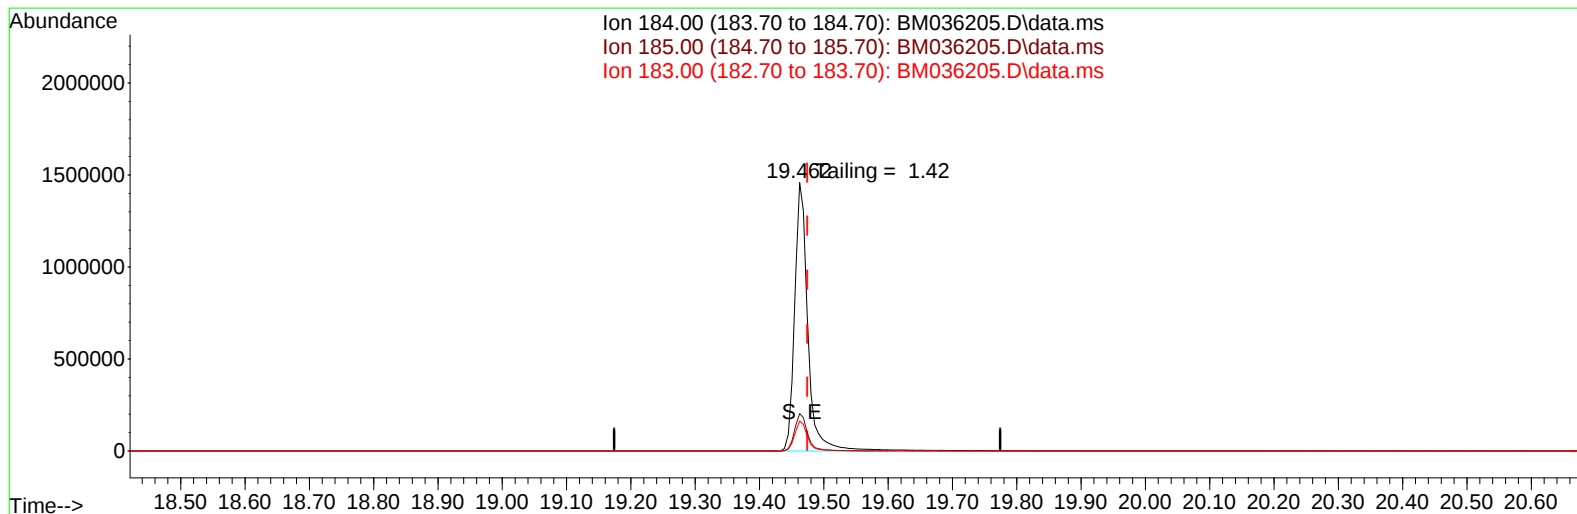

TIC: BM036205.D\data.ms

(77) Benzidine

19.462min (-0.012) 45344.90 ng

response 2089082

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.95
183.00	11.90	11.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/11/2022	BNA_M	<u>BM036205.D</u>
Compound Name	Response	Retention Time
DDT	931097	20.692
DDD	10171	20.251
DDE	1726	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11897	942994	1.26

Instrument :
BNA_M
ClientSampleId :
DFTPP