

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081215\
 Data File : BM002335.D
 Acq On : 11 Aug 2015 22:54
 Operator : UM/IZ
 Sample : G3162-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9C78

Quant Time: Aug 12 04:45:54 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080715MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 12 04:37:00 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.90	152	177888	20.00	ng/ul	0.00
2) Naphthalene-d8	11.77	136	858431	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.48	164	503727	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.19	188	1059694	20.00	ng/ul	0.00
17) Chrysene-d12	22.27	240	1024310	20.00	ng/ul	-0.01
22) Perylene-d12	24.97	264	818224	20.00	ng/ul	-0.01
System Monitoring Compounds						
7) Acenaphthylene-d8	15.19	160	1507835	28.89	ng/ul	0.00
10) Fluorene-d10	16.45	176	996632	27.46	ng/ul	0.00
14) Anthracene-d10	18.29	188	1415547	27.53	ng/ul	0.00
18) Pyrene-d10	20.50	212	1460102	29.39	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.79	264	1155354	26.59	ng/ul	-0.01
Target Compounds						
23) Benzo(b)fluoranthene	24.13	252	64927	1.28	ng/ul#	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081215\
Data File : BM002335.D
Acq On : 11 Aug 2015 22:54
Operator : UM/IZ
Sample : G3162-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9C78

Quant Time: Aug 12 04:45:54 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080715MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 12 04:37:00 2015
Response via : Initial Calibration

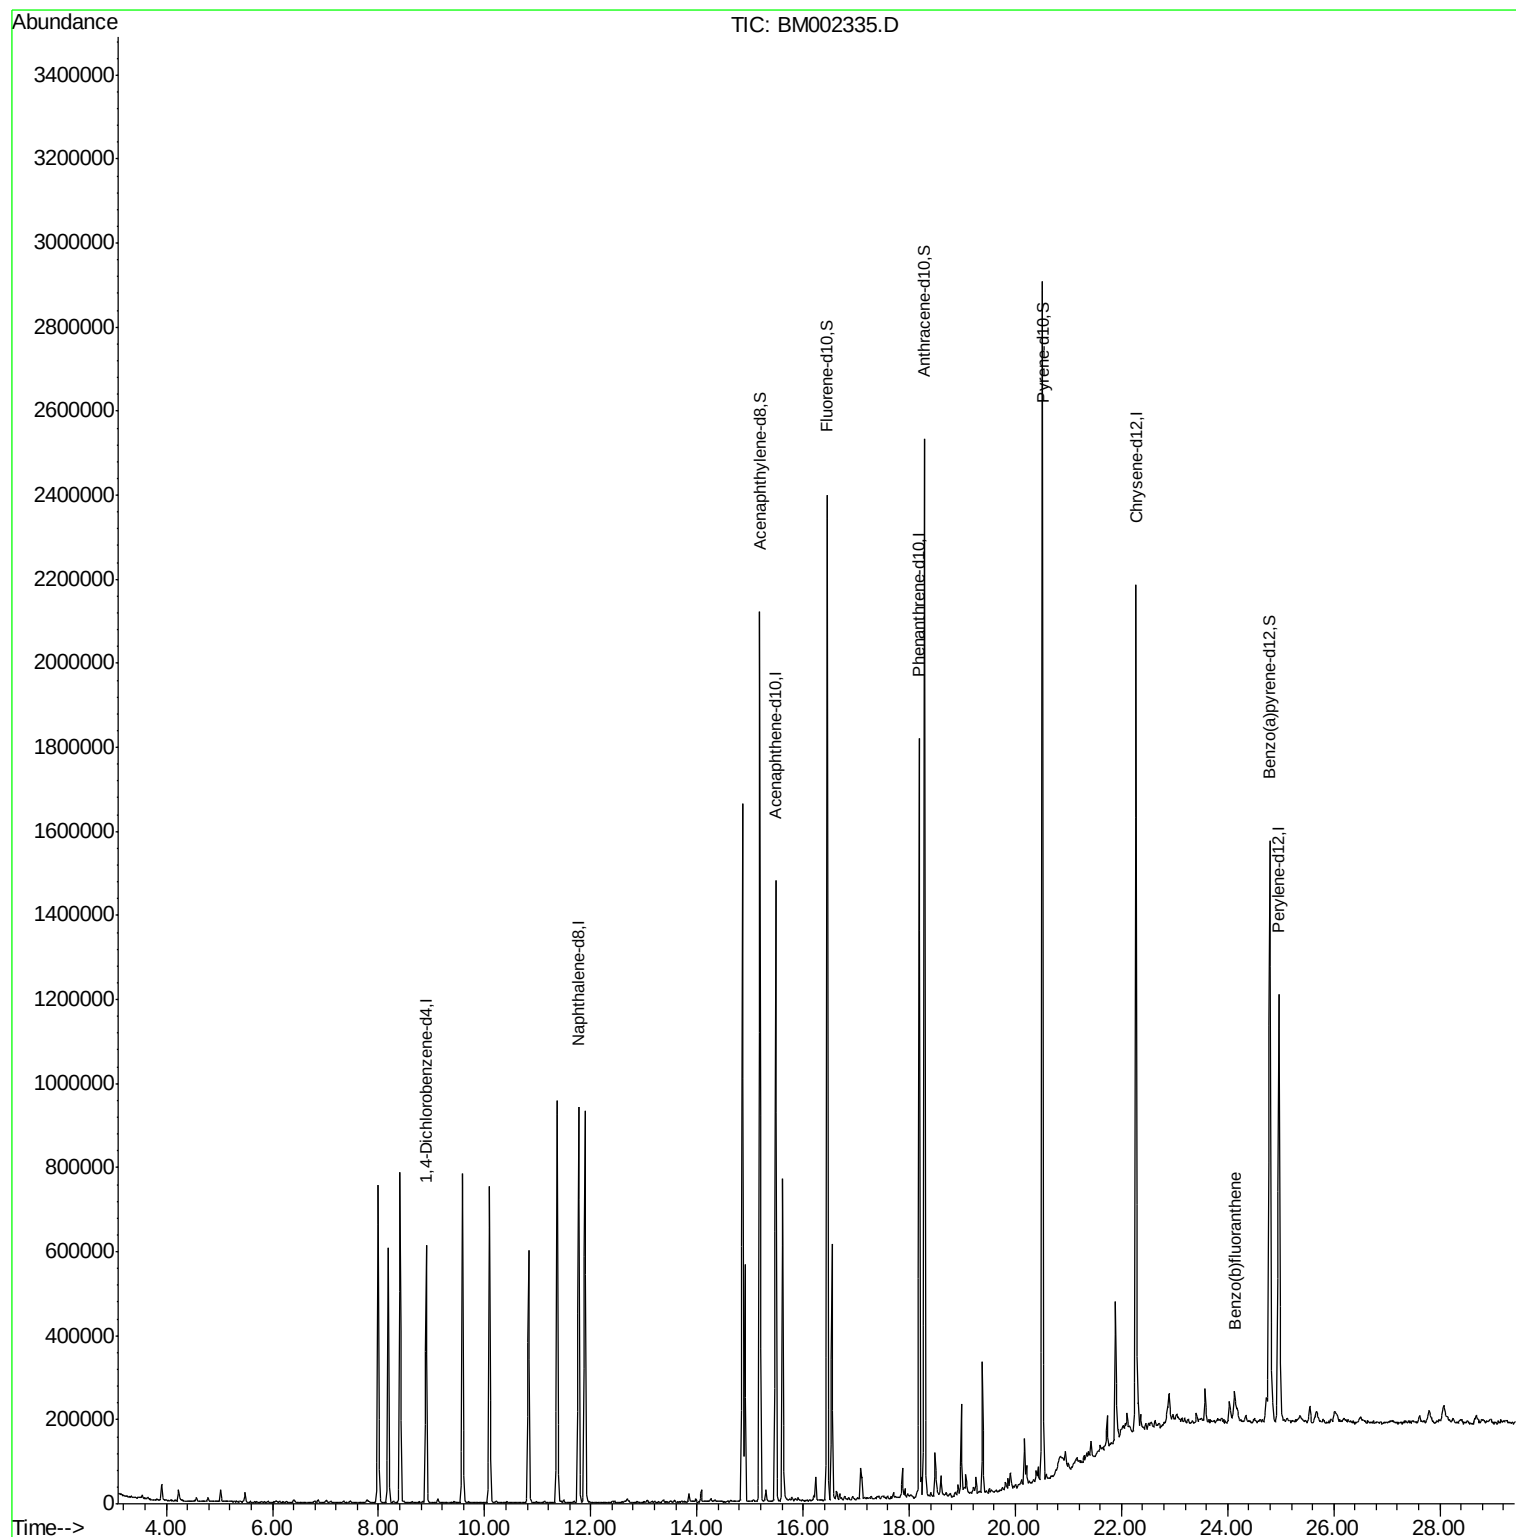

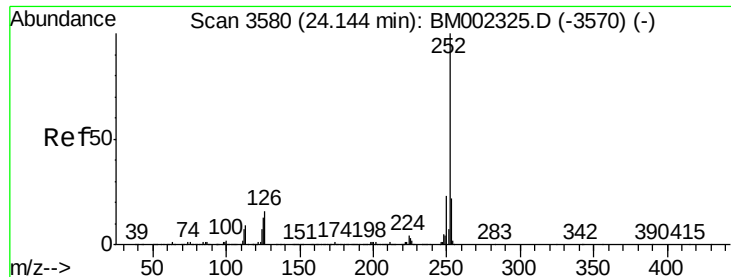

#23

Benzo(b)fluoranthene

Concen: 1.28 ng/ul

RT: 24.13 min Scan# 3578

Delta R.T. -0.01 min

Lab File: BM002335.D

Acq: 11 Aug 2015 22:54

Instrument :

BNA_M

ClientSampleId :

D9C78

Tgt Ion: 252 Resp: 64927

Ion Ratio Lower Upper

252 100

253 22.6 17.9 26.9

125 16.2 10.3 15.5#

