

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081215\
 Data File : BM002367.D
 Acq On : 12 Aug 2015 18:56
 Operator : UM/IZ
 Sample : G3163-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9C97MSD

Quant Time: Aug 13 00:46:07 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080715MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 13 00:45:03 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.90	152	199641	20.00	ng/ul	0.00
2) Naphthalene-d8	11.78	136	934831	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.49	164	504512	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.20	188	910681	20.00	ng/ul	0.00
17) Chrysene-d12	22.29	240	637964	20.00	ng/ul	0.00
22) Perylene-d12	24.99	264	633094	20.00	ng/ul	0.00

System Monitoring Compounds						
7) Acenaphthylene-d8	15.19	160	1317680	25.21	ng/ul	0.00
10) Fluorene-d10	16.46	176	856364	23.56	ng/ul	0.00
14) Anthracene-d10	18.30	188	1101642	24.93	ng/ul	0.00
18) Pyrene-d10	20.52	212	902085	29.16	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.81	264	818724	24.36	ng/ul	0.00


Target Compounds				Qvalue		
3) Naphthalene	11.83	128	64856	1.32	ng/ul	98
4) 2-Methylnaphthalene	13.37	142	38083	1.08	ng/ul	93
8) Acenaphthylene	15.22	152	139232	2.57	ng/ul	99
9) Acenaphthene	15.55	153	813662	22.29	ng/ul	99
13) Phenanthrene	18.24	178	457282	8.72	ng/ul	100
15) Anthracene	18.33	178	219096	4.05	ng/ul	99
16) Fluoranthene	20.19	202	810341	13.96	ng/ul	99
19) Pyrene	20.54	202	1808575	43.85	ng/ul	98
20) Benzo(a)anthracene	22.27	228	508361	13.05	ng/ul	98
21) Chrysene	22.33	228	507394	13.75	ng/ul	96
23) Benzo(b)fluoranthene	24.16	252	906177	23.03	ng/ul	97
24) Benzo(k)fluoranthene	24.16	252	234422	6.20	ng/ul	96
26) Benzo(a)pyrene	24.87	252	530977	14.10	ng/ul	95
27) Indeno(1,2,3-cd)pyrene	27.84	276	368828	8.55	ng/ul	94
28) Dibenzo(a,h)anthracene	27.84	278	106909	2.92	ng/ul#	81
29) Benzo(g,h,i)perylene	28.74	276	314056	8.63	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081215\
Data File : BM002367.D
Acq On : 12 Aug 2015 18:56
Operator : UM/IZ
Sample : G3163-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9C97MSD

Quant Time: Aug 13 00:46:07 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080715MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 13 00:45:03 2015
Response via : Initial Calibration

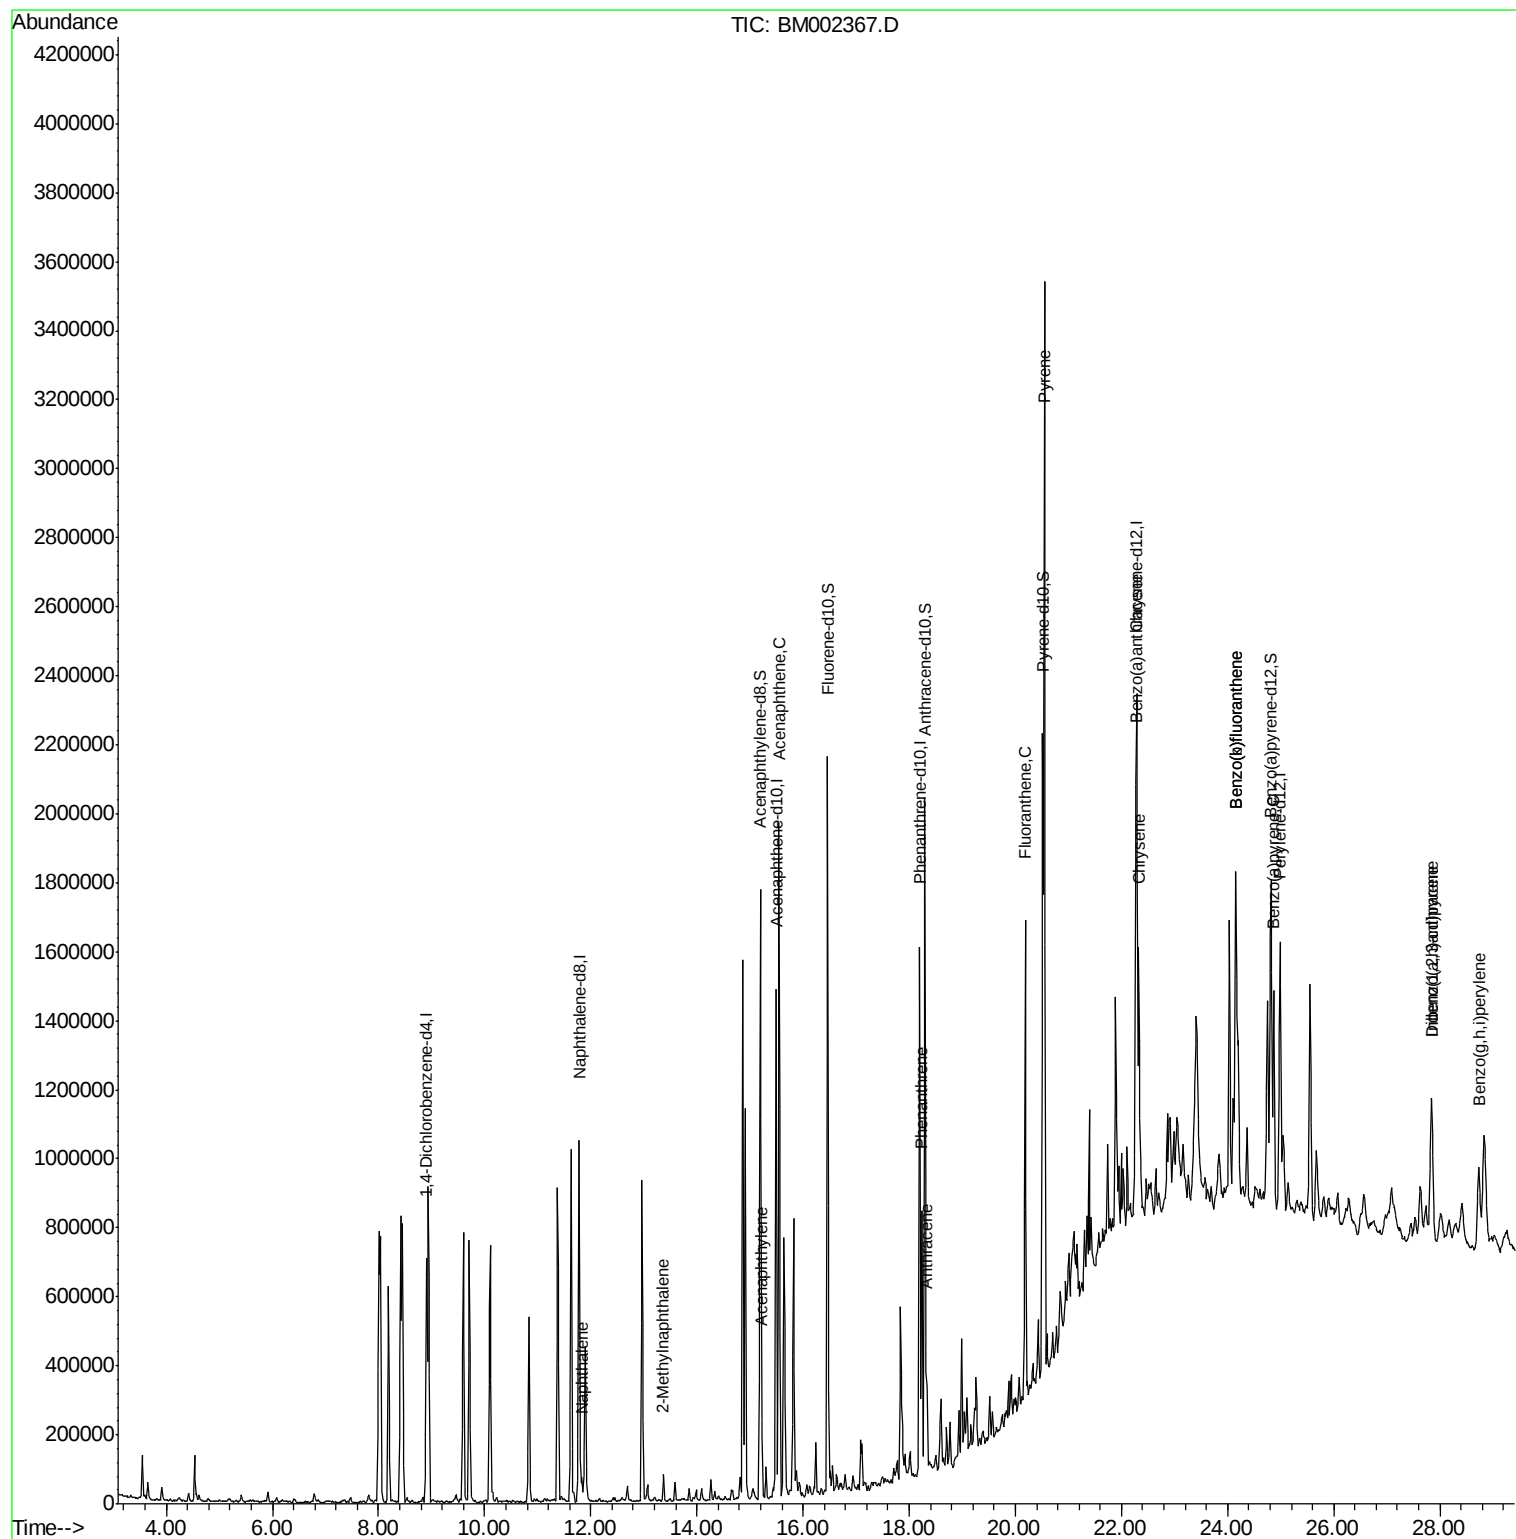

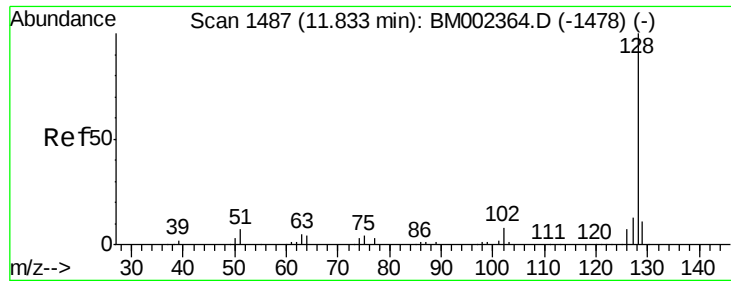

#3

Naphthalene

Concen: 1.32 ng/ul

RT: 11.83 min Scan# 1486

Delta R.T. -0.01 min

Lab File: BM002367.D

Acq: 12 Aug 2015 18:56

Instrument :

BNA_M

ClientSampleId :

D9C97MSD


Tgt Ion:128 Resp: 64856

Ion Ratio Lower Upper

128 100

129 12.3 8.6 12.8




127 13.0 10.4 15.6

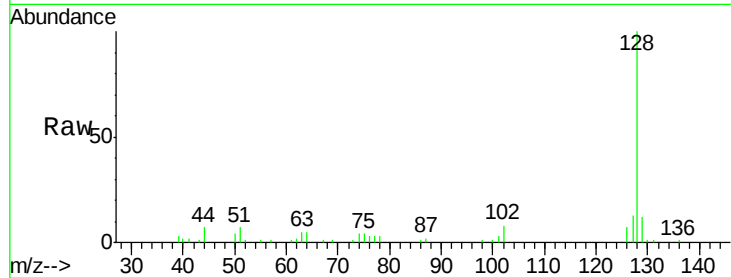

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

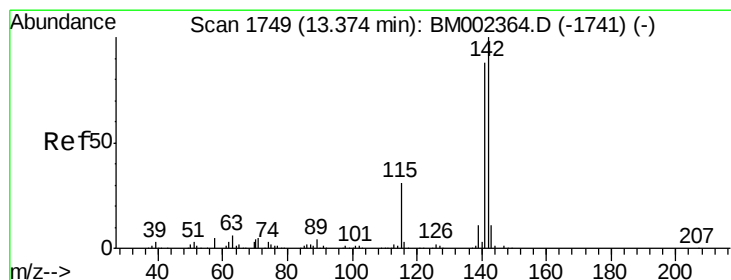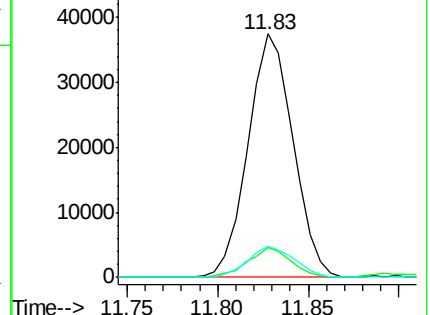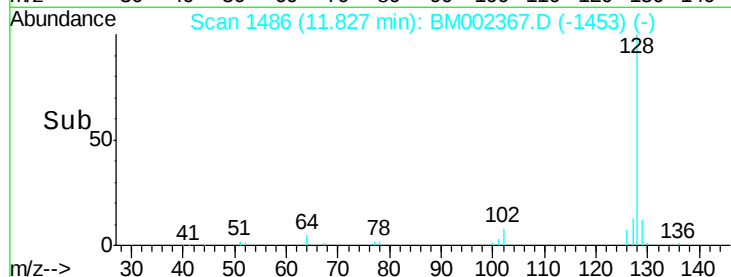

#4

2-Methylnaphthalene

Concen: 1.08 ng/ul

RT: 13.37 min Scan# 1748

Delta R.T. -0.01 min

Lab File: BM002367.D


Acq: 12 Aug 2015 18:56

Tgt Ion:142 Resp: 38083

Ion Ratio Lower Upper



142 100


141 83.7 72.5 108.7

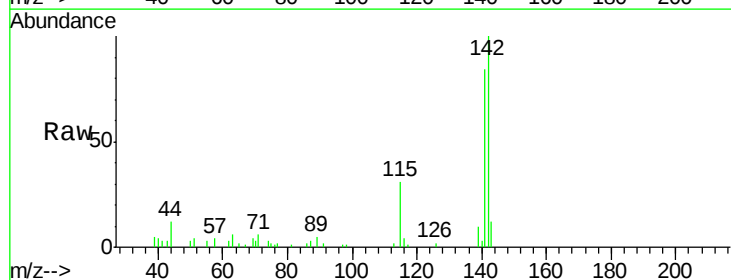

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E



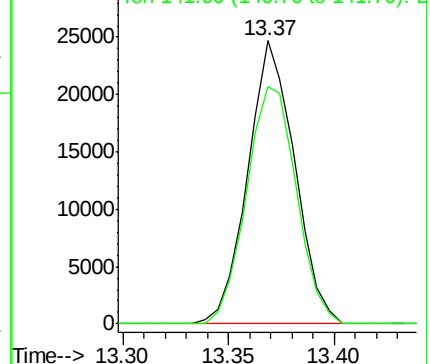
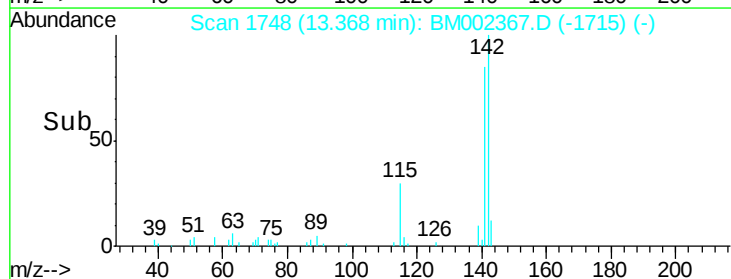


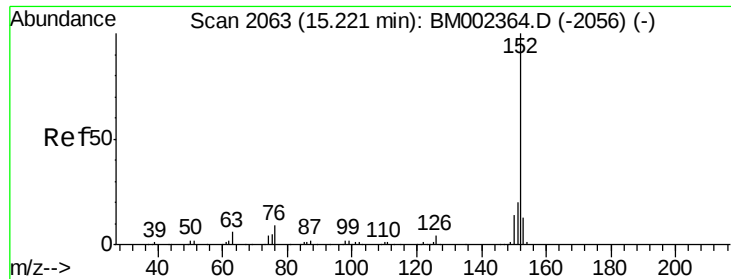

#8
Acenaphthylene
Concen: 2.57 ng/ul
RT: 15.22 min Scan# 2063
Delta R.T. -0.00 min
Lab File: BM002367.D
Acq: 12 Aug 2015 18:56




Instrument :
BNA_M
ClientSampleId :
D9C97MSD


Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.3	15.9	23.9
153	13.4	10.6	15.8

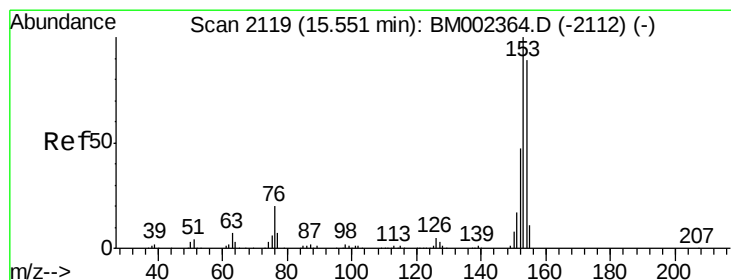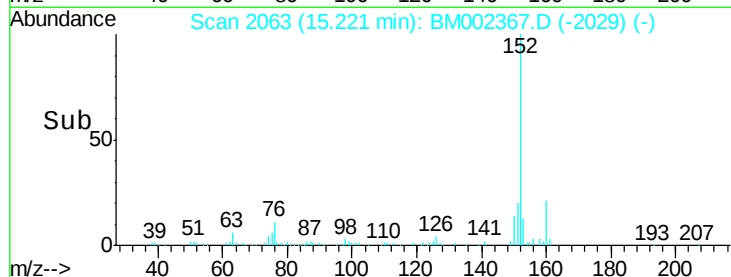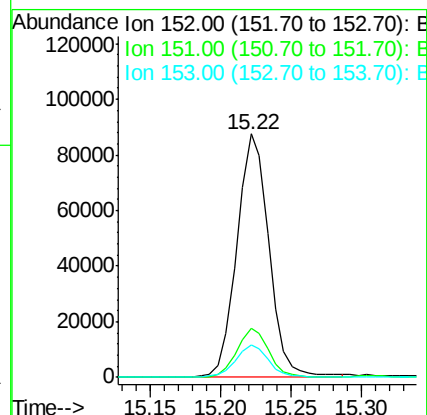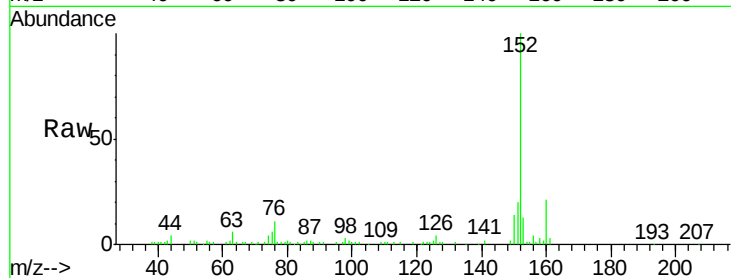

#9
Acenaphthene
Concen: 22.29 ng/ul
RT: 15.55 min Scan# 2119
Delta R.T. -0.00 min
Lab File: BM002367.D
Acq: 12 Aug 2015 18:56

Tgt Ion	Ratio	Lower	Upper
153	100		
152	46.6	36.6	55.0
154	88.3	71.5	107.3

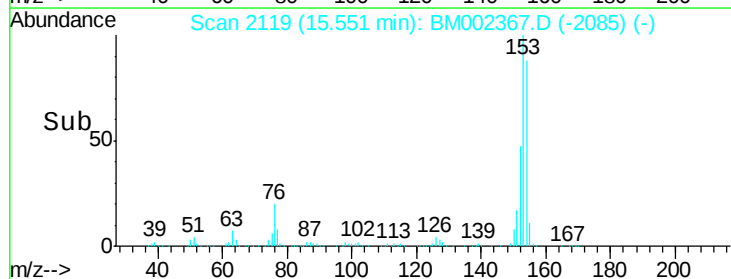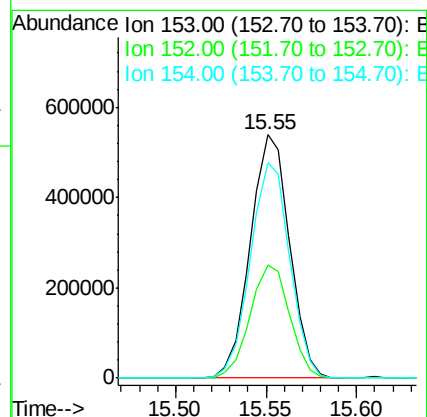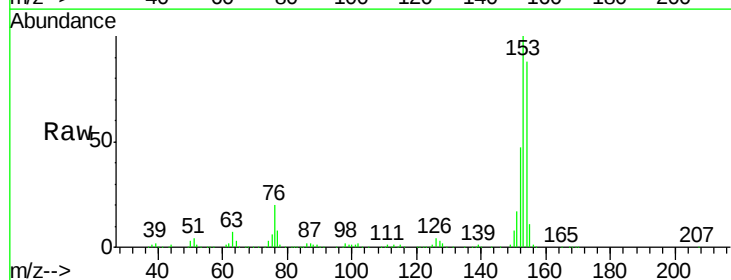

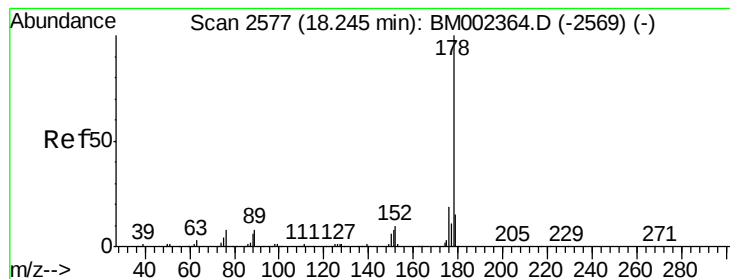

#13

Phenanthrene

Concen: 8.72 ng/ul

RT: 18.24 min Scan# 2576

Delta R.T. -0.01 min

Lab File: BM002367.D

Acq: 12 Aug 2015 18:56

Instrument :

BNA_M

ClientSampleId :

D9C97MSD


Tgt Ion:178 Resp: 457282

Ion Ratio Lower Upper

178 100

179 15.4 12.3 18.5




176 18.8 15.3 22.9

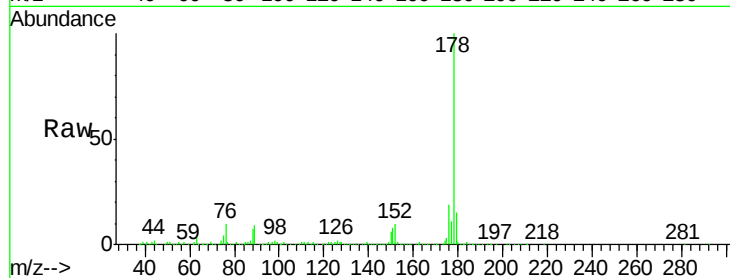

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

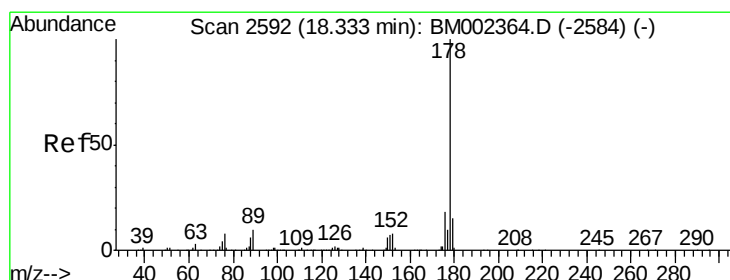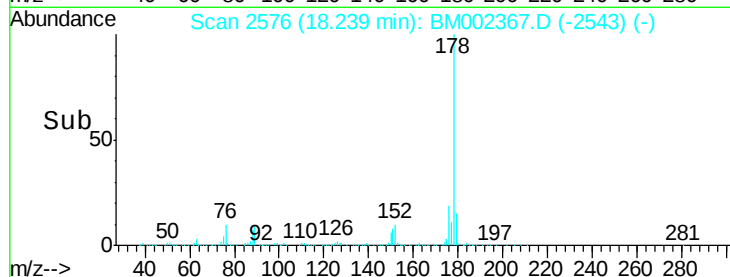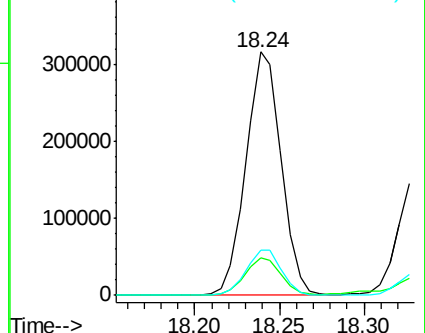

#15

Anthracene

Concen: 4.05 ng/ul

RT: 18.33 min Scan# 2592

Delta R.T. -0.00 min

Lab File: BM002367.D

Acq: 12 Aug 2015 18:56


Tgt Ion:178 Resp: 219096

Ion Ratio Lower Upper

178 100

179 16.0 12.3 18.5



176 18.2 14.5 21.7

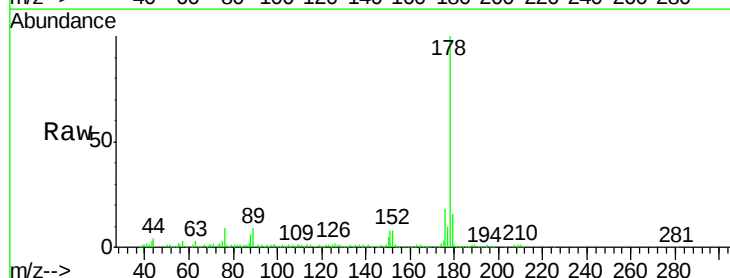


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

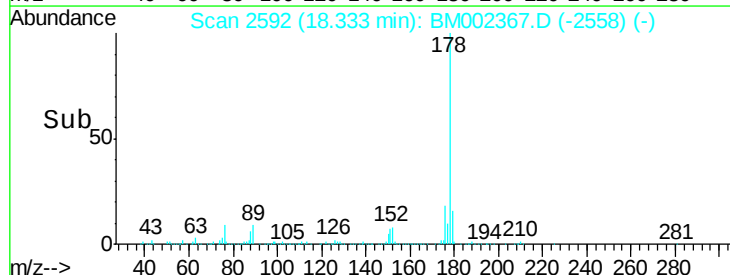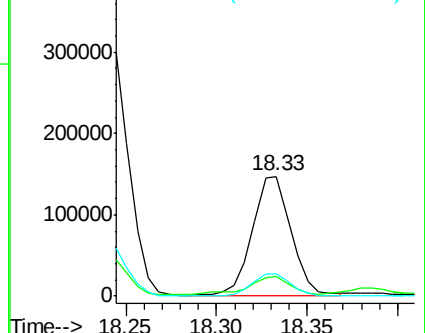

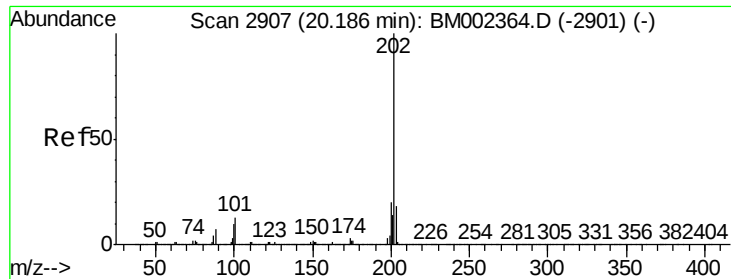

#16

Fluoranthene

Concen: 13.96 ng/ul

RT: 20.19 min Scan# 2907

Delta R.T. -0.00 min

Lab File: BM002367.D

Acq: 12 Aug 2015 18:56

Instrument :

BNA_M

ClientSampleId :

D9C97MSD


Tgt Ion:202 Resp: 810341

Ion Ratio Lower Upper

202 100

101 13.0 10.6 15.8




100 10.0 8.2 12.4

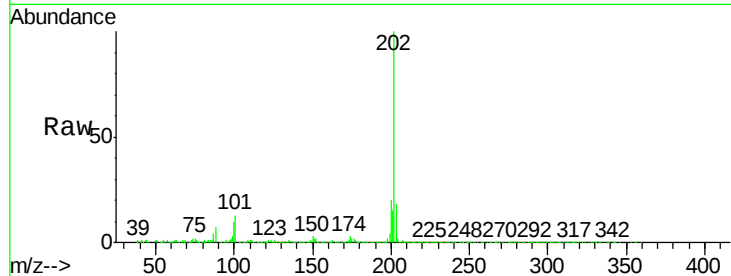

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

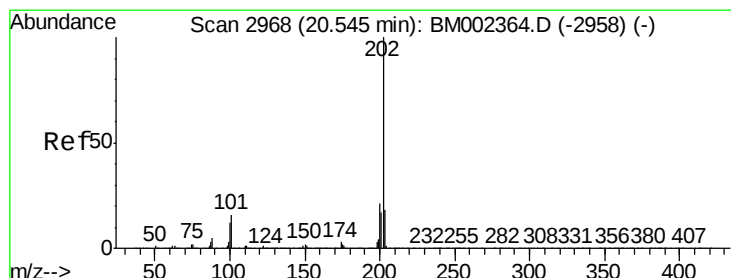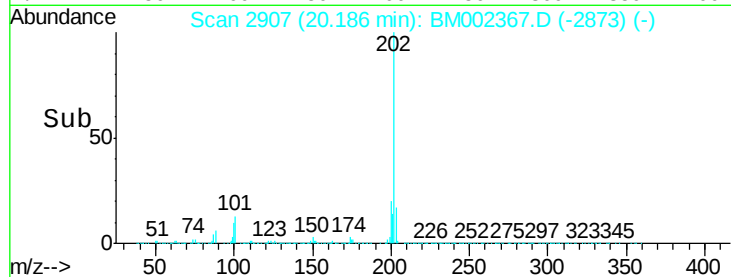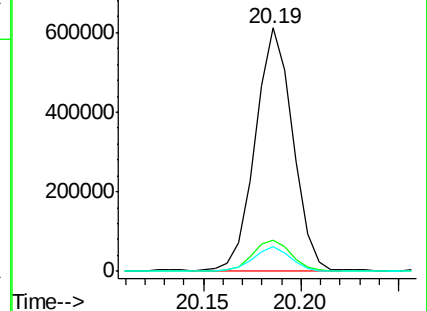

#19

Pyrene

Concen: 43.85 ng/ul

RT: 20.54 min Scan# 2968

Delta R.T. -0.00 min

Lab File: BM002367.D

Acq: 12 Aug 2015 18:56


Tgt Ion:202 Resp: 1808575

Ion Ratio Lower Upper

202 100

101 15.8 13.0 19.6



100 12.7 11.0 16.4

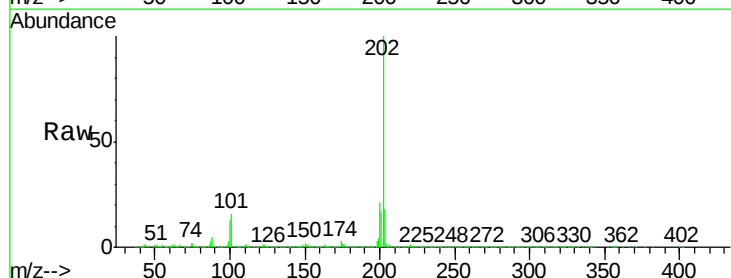


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

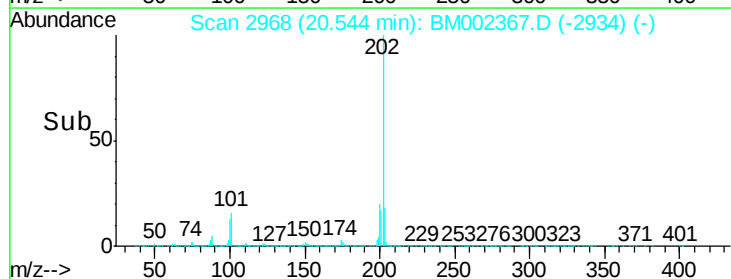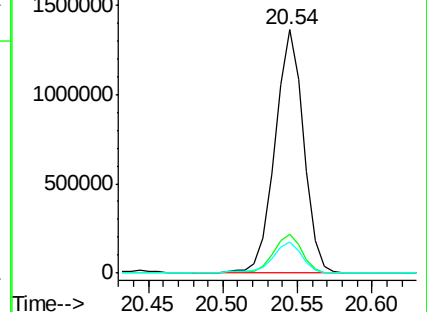

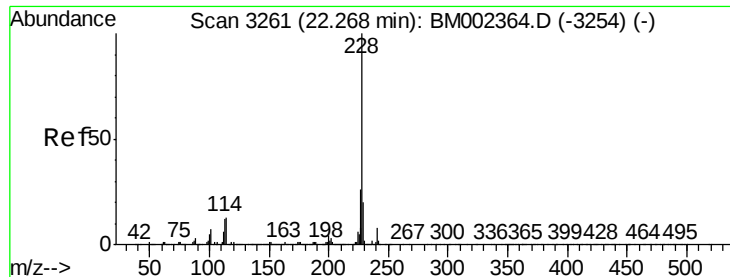

#20

Benzo(a)anthracene

Concen: 13.05 ng/ul

RT: 22.27 min Scan# 3261

Delta R.T. -0.00 min

Lab File: BM002367.D

Acq: 12 Aug 2015 18:56

Instrument :

BNA_M

ClientSampleId :

D9C97MSD


Tgt Ion:228 Resp: 508361

Ion Ratio Lower Upper

228 100

229 21.2 15.7 23.5




226 27.4 21.4 32.0

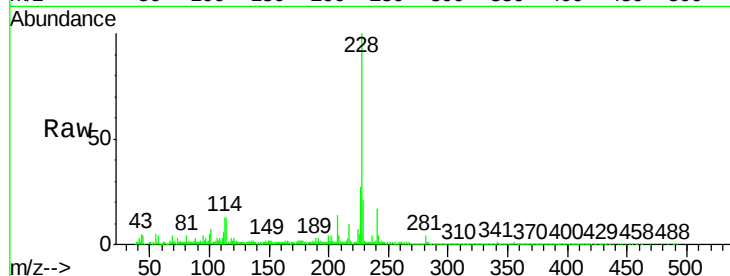

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

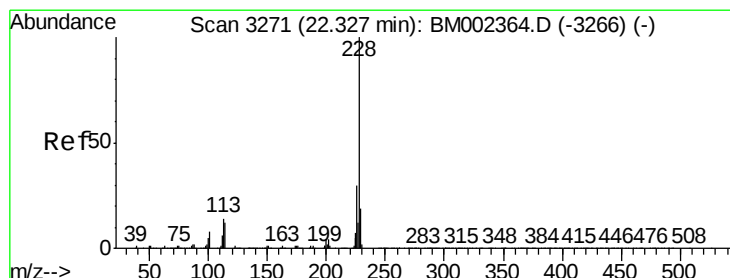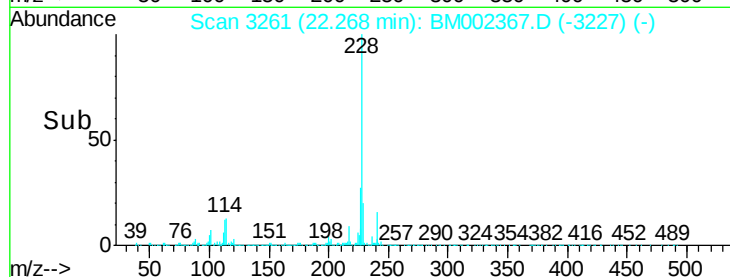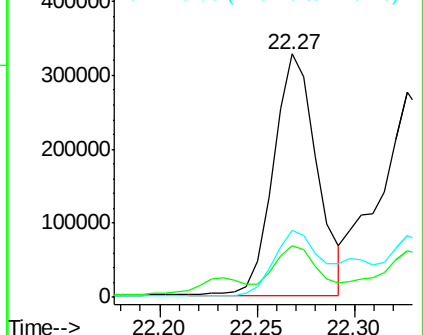

#21

Chrysene

Concen: 13.75 ng/ul

RT: 22.33 min Scan# 3271

Delta R.T. -0.00 min

Lab File: BM002367.D

Acq: 12 Aug 2015 18:56


Tgt Ion:228 Resp: 507394

Ion Ratio Lower Upper

228 100

226 30.3 23.4 35.0



229 22.7 15.5 23.3

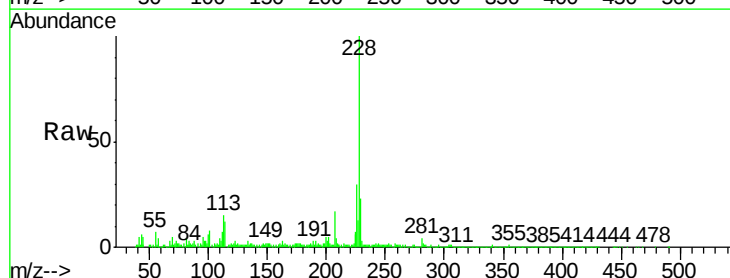


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

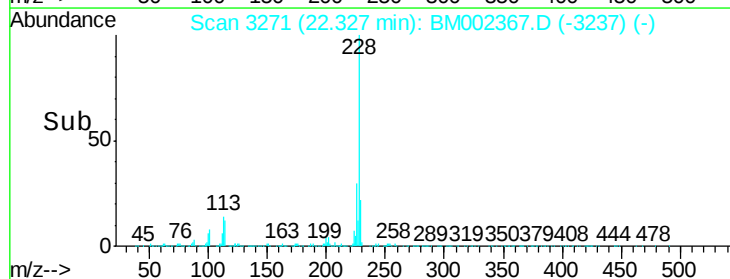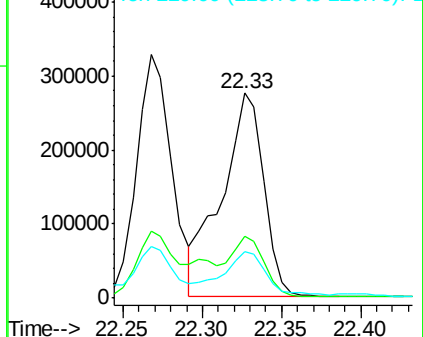

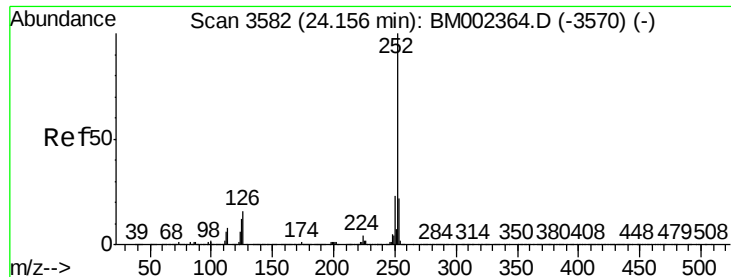

#23

Benzo(b)fluoranthene

Concen: 23.03 ng/ul

RT: 24.16 min Scan# 3582

Delta R.T. -0.00 min

Lab File: BM002367.D

Acq: 12 Aug 2015 18:56

Instrument :

BNA_M

ClientSampleId :

D9C97MSD


Tgt Ion:252 Resp: 906177

Ion Ratio Lower Upper

252 100

253 23.4 17.9 26.9




125 14.5 10.3 15.5

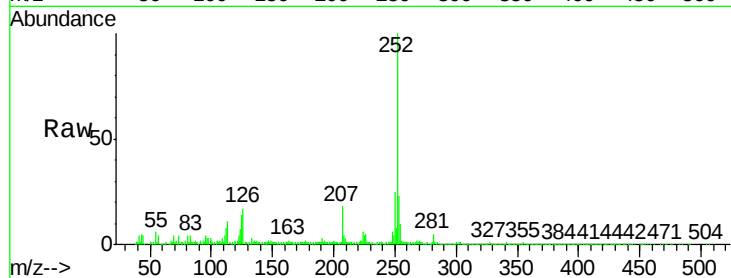

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

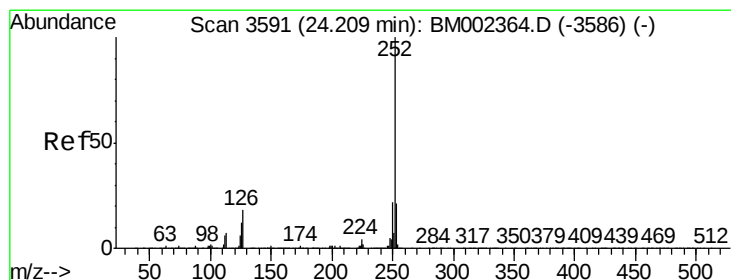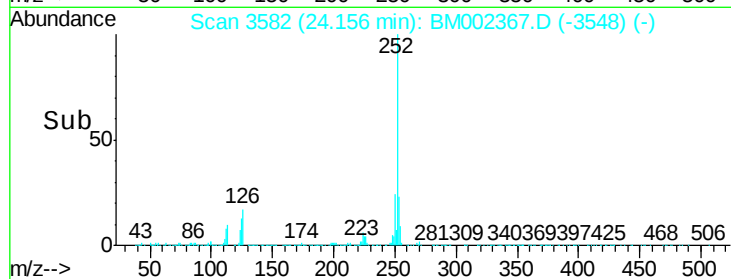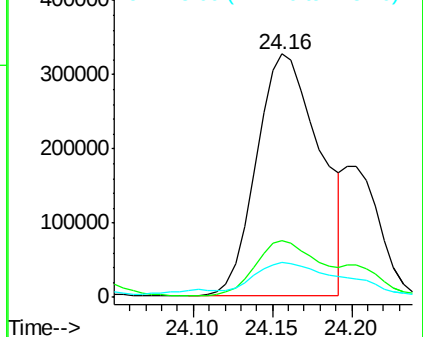

#24

Benzo(k)fluoranthene

Concen: 6.20 ng/ul

RT: 24.16 min Scan# 3582

Delta R.T. -0.05 min

Lab File: BM002367.D

Acq: 12 Aug 2015 18:56


Tgt Ion:252 Resp: 234422

Ion Ratio Lower Upper

252 100

253 23.4 17.3 25.9



125 14.5 10.2 15.4

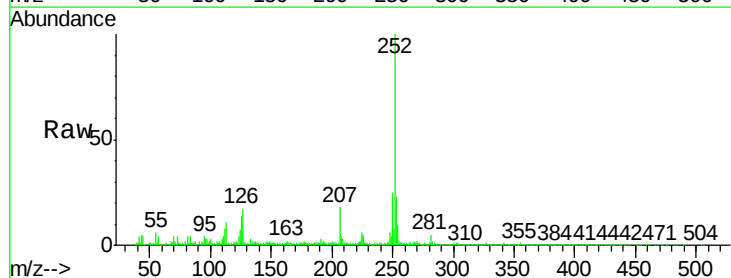


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

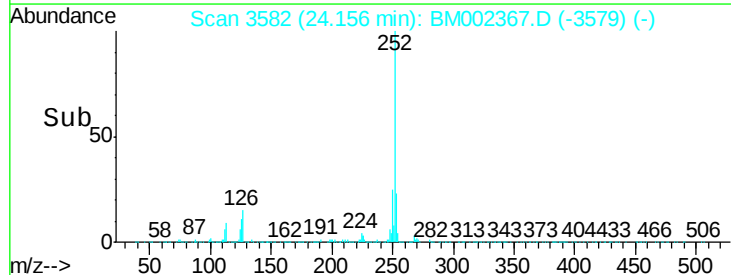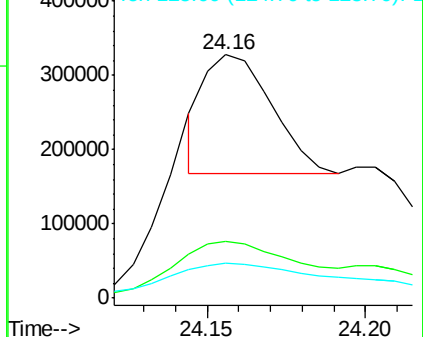

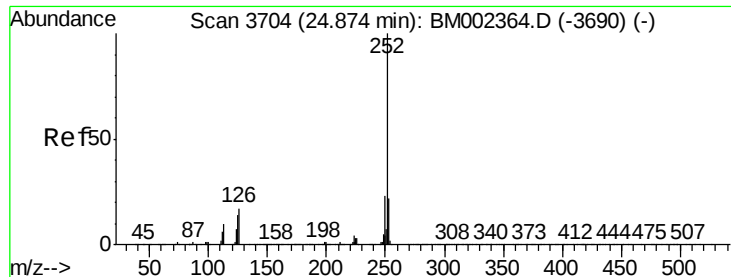

#26

Benzo(a)pyrene

Concen: 14.10 ng/ul

RT: 24.87 min Scan# 3703

Delta R.T. -0.01 min

Lab File: BM002367.D

Acq: 12 Aug 2015 18:56





Instrument :

BNA_M

ClientSampleId :

D9C97MSD

Tgt Ion:	252	Resp:	530977
Ion	Ratio	Lower	Upper
252	100		
253	23.5	17.3	25.9
125	16.1	11.0	16.6

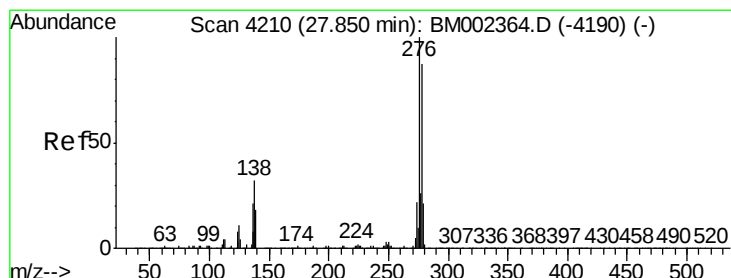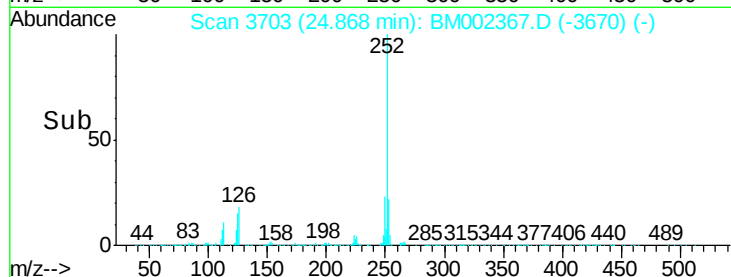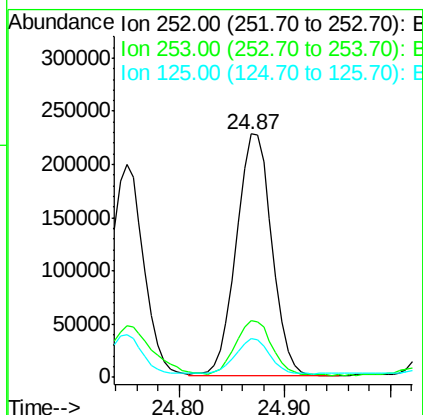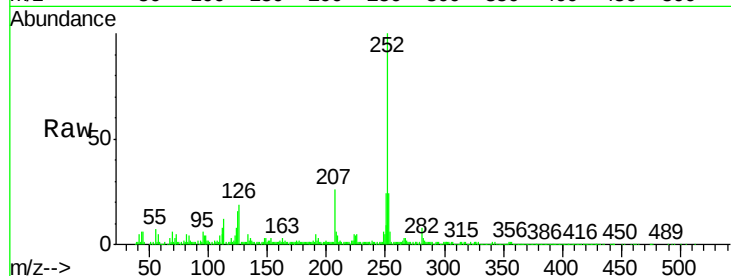

#27

Indeno(1,2,3-cd)pyrene

Concen: 8.55 ng/ul




RT: 27.84 min Scan# 4209


Delta R.T. -0.01 min

Lab File: BM002367.D

Acq: 12 Aug 2015 18:56

Tgt Ion:	276	Resp:	368828
Ion	Ratio	Lower	Upper
276	100		
138	26.7	25.6	38.4
277	25.7	21.0	31.4


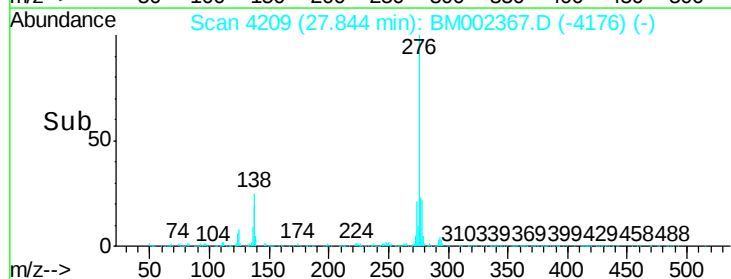
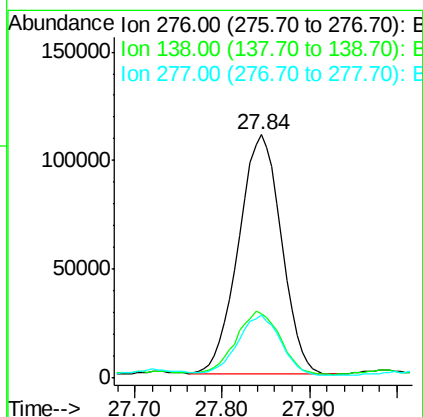
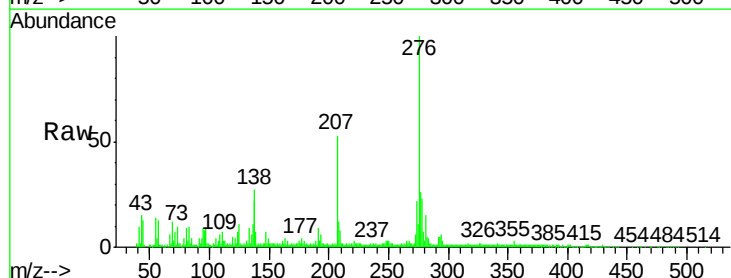


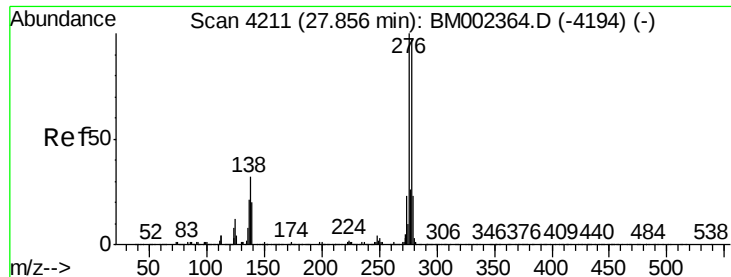

#28
Dibenzo(a,h)anthracene
Concen: 2.92 ng/ul
RT: 27.84 min Scan# 4208
Delta R.T. -0.02 min
Lab File: BM002367.D
Acq: 12 Aug 2015 18:56

Instrument :
BNA_M
ClientSampleId :
D9C97MSD

Tgt Ion	Ratio	Lower	Upper
278	100		
139	31.5	16.4	24.6#
279	31.2	18.8	28.2#

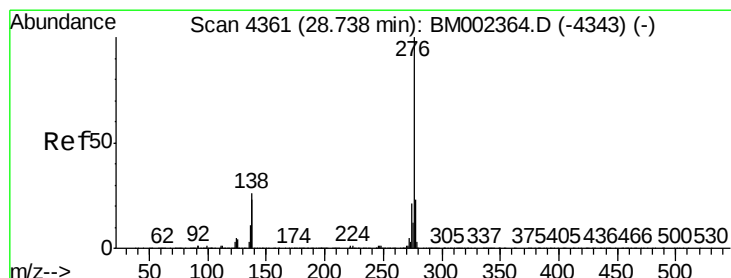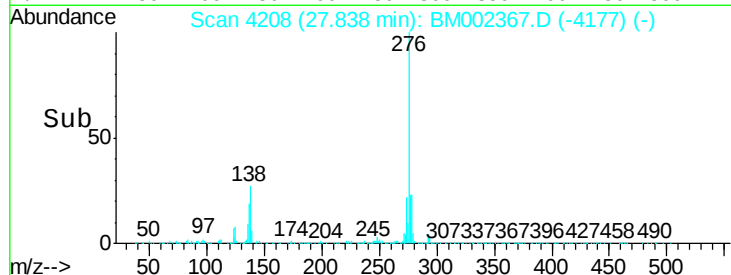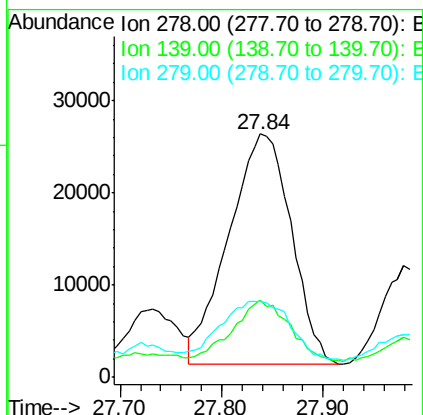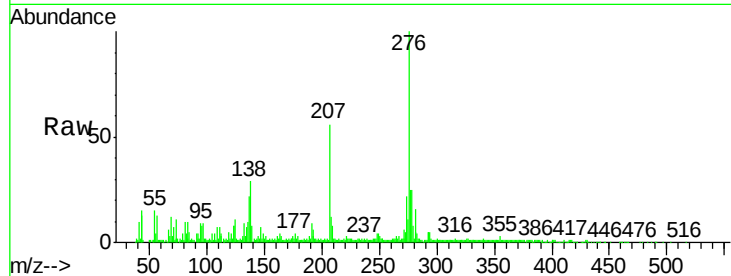

#29
Benzo(g,h,i)perylene
Concen: 8.63 ng/ul
RT: 28.74 min Scan# 4361
Delta R.T. -0.00 min
Lab File: BM002367.D
Acq: 12 Aug 2015 18:56

Tgt Ion	Ratio	Lower	Upper
276	100		
138	27.8	20.5	30.7
277	23.9	19.0	28.6

