


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081215\
 Data File : BM002324.D
 Acq On : 11 Aug 2015 13:40
 Operator : UM/IZ
 Sample : DFTPP95
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP95

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080715MA.M
 Title : SVOA CALIBRATION
 Last Update : Wed Aug 12 02:22:13 2015

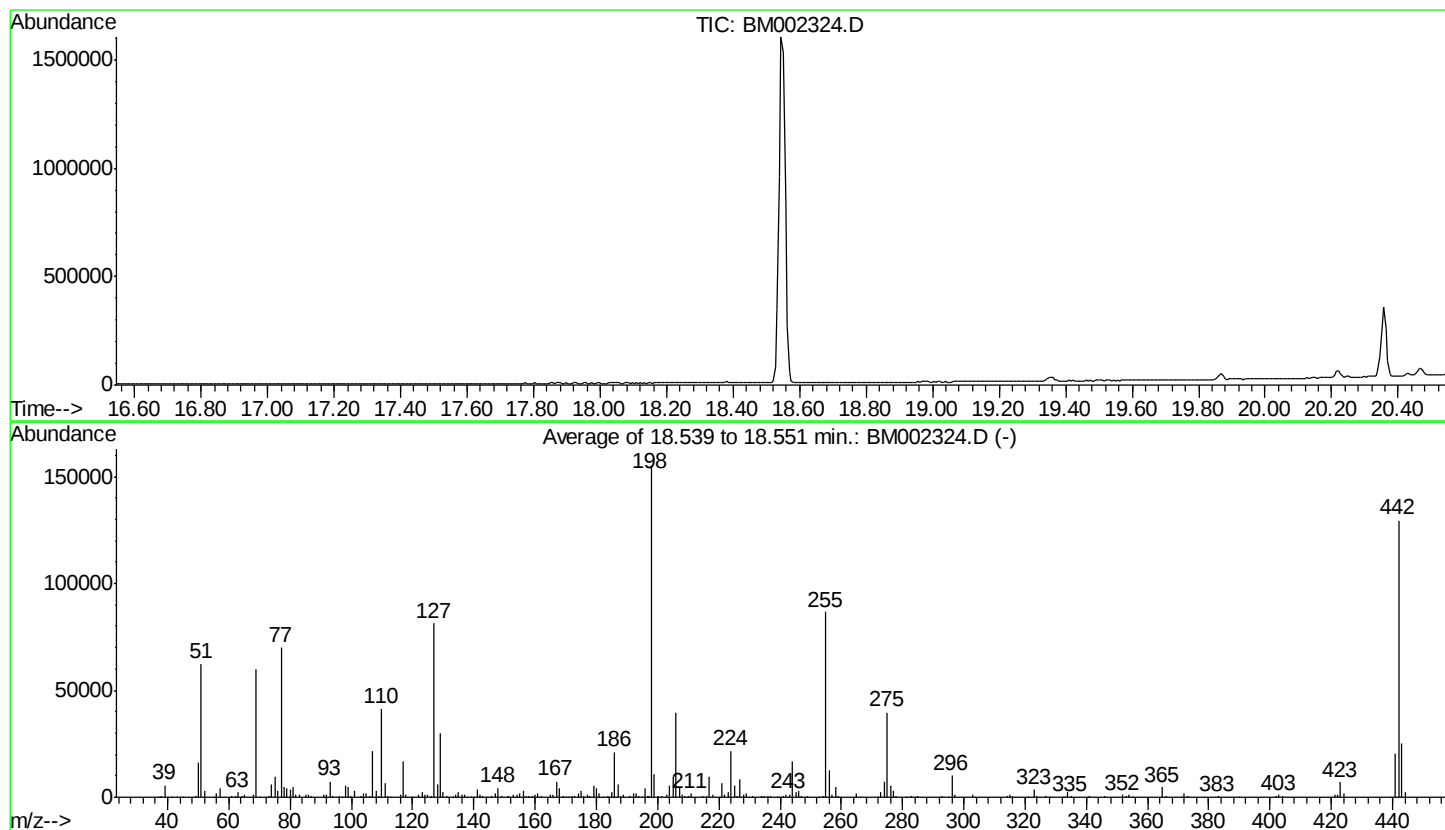

AutoFind: Scans 2627, 2628, 2629; Background Corrected with Scan 2622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	62533	PASS
68	69	0.00	2	1.8	1092	PASS
69	198	0.00	100	38.4	59658	PASS
70	69	0.00	2	0.5	272	PASS
127	198	10	80	52.4	81280	PASS
197	198	0.00	2	0.4	598	PASS
198	198	100	100	100.0	155184	PASS
199	198	5	9	7.0	10809	PASS
275	198	10	60	25.7	39824	PASS
365	198	1	100	3.0	4636	PASS
441	443	0.01	100	81.1	20184	PASS
442	198	50	100	83.6	129674	PASS
443	442	15	24	19.2	24888	PASS

m/z	Abundance
38.10	639.0
39.00	4511.0
40.00	1048.0
41.00	452.0
43.00	373.0
44.00	6758.0
49.00	460.0
50.00	14087.0
51.00	51608.0
52.00	2686.0
54.90	651.0
56.00	1595.0
57.00	3588.0
61.00	564.0
62.00	750.0
63.00	1888.0
64.10	383.0
65.00	1063.0
68.00	894.0
69.00	47816.0
73.00	939.0
74.00	4988.0
75.00	7710.0
76.00	2720.0
77.10	56168.0
78.00	4049.0
79.00	3652.0
80.00	2756.0
81.00	4087.0
82.00	1092.0
83.00	862.0
85.00	814.0
86.00	1071.0
86.90	564.0
91.00	1047.0
92.00	879.0
93.00	6032.0
93.90	389.0
95.90	425.0
96.90	316.0
98.00	4388.0
99.00	3847.0
100.00	380.0
101.00	2285.0
103.00	733.0
104.00	1219.0
104.90	1405.0
106.00	354.0
107.00	17192.0
108.00	2505.0
109.10	502.0
110.00	32120.0
111.00	5037.0
112.00	692.0
115.90	910.0
117.00	13421.0
117.90	1095.0
122.00	1057.0
123.00	1526.0
124.00	745.0
125.00	725.0
127.00	62440.0
128.00	4857.0
129.00	22512.0
130.00	1994.0
131.00	362.0
133.90	761.0
134.90	2128.0
136.00	741.0
137.00	1030.0
140.90	2678.0
142.00	1187.0
143.00	708.0
146.00	466.0
146.90	1546.0
148.00	3094.0
149.00	601.0
150.90	341.0
153.00	880.0
154.00	781.0
155.00	1744.0
156.00	2411.0
157.00	430.0
157.90	419.0
158.90	395.0
159.90	942.0
161.00	1405.0
161.90	352.0
164.90	1242.0
166.00	870.0
167.00	5332.0

Instrument :
BNA_M
ClientSampleId :
DFTPP95

168.00	3419.0
168.90	422.0
171.90	480.0
173.00	790.0
174.00	1123.0
175.00	2230.0
176.00	662.0
177.00	910.0
178.00	364.0
179.00	3831.0
180.00	2670.0
181.00	1328.0
184.00	309.0
184.90	1762.0
186.00	15002.0
187.00	4331.0
188.00	530.0
189.00	1106.0
190.90	626.0
191.90	1351.0
193.00	1602.0
193.90	314.0
195.90	2888.0
197.00	666.0
197.90	108816.0
198.90	7786.0
200.00	521.0
201.60	503.0
203.00	901.0
204.00	3499.0
205.00	6658.0
206.00	27400.0
207.00	5521.0
208.00	1236.0
208.90	547.0
209.80	413.0
210.30	406.0
211.00	945.0
216.10	478.0
217.00	6710.0
218.00	853.0
221.00	4250.0
221.80	1170.0
223.00	1704.0
224.00	14304.0
225.00	3930.0
226.10	321.0
227.00	5350.0
228.00	783.0
228.90	1120.0
231.00	590.0
233.90	466.0
235.00	468.0
236.90	534.0
240.90	307.0
242.00	735.0
243.00	761.0
244.00	11142.0
245.10	1438.0
246.00	2124.0
246.90	514.0
248.90	523.0
254.10	538.0
255.00	56624.0
256.00	8920.0
256.90	758.0
258.00	3313.0
258.90	453.0
265.00	1238.0
273.00	1808.0
274.00	4459.0
275.00	25040.0
276.00	3535.0
277.00	2315.0
278.00	387.0
281.00	471.0
283.00	335.0
285.00	450.0
293.00	341.0
296.00	6544.0
297.00	949.0
302.90	764.0
314.00	354.0
314.90	727.0
316.10	312.0
323.00	2209.0
324.00	382.0
326.80	469.0
334.00	1379.0
335.00	404.0
345.90	459.0
352.00	508.0
353.00	621.0
354.00	573.0
365.00	2696.0

Instrument :
BNA_M
ClientSampleId :
DFTPP95

366.10	303.0
372.00	1054.0
383.00	300.0
401.90	424.0
403.00	581.0
421.00	575.0
422.00	601.0
423.00	3571.0
423.90	973.0
441.00	10082.0
442.00	66912.0
443.00	13361.0
444.00	1217.0

Instrument :
BNA_M
ClientSampleId :
DFTPP95

m/z	Abundance
36.90	308.0
38.10	992.0
39.10	6506.0
40.00	1188.0
41.10	534.0
43.00	470.0
44.00	6278.0
44.90	349.0
49.00	522.0
50.00	19184.0
51.00	73752.0
52.00	3858.0
55.00	758.0
56.00	2298.0
57.00	5096.0
61.00	757.0
62.00	1066.0
63.00	3017.0
64.00	585.0
65.00	1492.0
68.10	1253.0
69.00	71192.0
70.00	402.0
73.00	1316.0
74.00	7422.0
75.00	11002.0
76.10	3723.0
77.10	83968.0
78.00	5630.0
79.00	4953.0
80.00	4044.0
81.00	6022.0
82.00	1671.0
83.00	1514.0
85.00	1231.0
86.00	1566.0
86.90	765.0
91.00	1472.0
92.00	1563.0
93.00	8362.0
93.90	669.0
96.00	528.0
97.00	341.0
98.00	6726.0
99.00	5825.0
99.90	550.0
101.00	3134.0
103.00	964.0
104.00	2254.0
105.00	2001.0
105.90	691.0
107.00	25304.0
108.00	4002.0
109.10	777.0
110.00	49976.0
111.00	7459.0
112.00	894.0
112.90	359.0
115.90	1374.0
117.00	19072.0
118.00	1529.0
120.00	428.0
122.00	1636.0
123.00	2534.0
124.00	1158.0
124.90	1171.0
126.20	614.0
127.00	97248.0
128.00	7617.0
129.00	35520.0
130.00	2838.0
131.00	782.0
133.00	363.0
133.90	904.0
135.00	2826.0
136.00	1136.0
137.00	1678.0
139.00	310.0
140.00	504.0
141.00	4818.0
141.90	1554.0
142.90	990.0
144.00	300.0
145.90	775.0
147.00	2444.0
148.00	5186.0
149.00	1075.0
151.10	619.0
151.80	405.0
153.00	1411.0
154.00	1171.0

Instrument :
BNA_M
ClientSampleId :
DFTPP95

155.00	2484.0
156.00	3798.0
157.00	790.0
158.00	845.0
159.00	666.0
160.00	1423.0
160.90	2085.0
162.00	683.0
165.00	1635.0
166.00	1312.0
167.00	8482.0
168.00	4428.0
169.00	850.0
171.00	361.0
172.00	731.0
173.00	945.0
174.00	1723.0
175.00	3487.0
176.00	1087.0
177.00	1541.0
178.00	694.0
179.00	6543.0
180.00	4767.0
181.00	2046.0
182.00	471.0
183.90	554.0
185.00	3210.0
186.00	24728.0
187.00	7028.0
187.90	986.0
189.00	1279.0
190.90	814.0
192.00	2152.0
193.00	2153.0
194.00	577.0
196.00	5333.0
197.10	1128.0
197.90	184576.0
198.90	12643.0
200.00	903.0
201.40	957.0
202.90	1294.0
204.00	6385.0
205.00	10825.0
206.00	46632.0
207.00	7362.0
208.00	2036.0
208.90	791.0
210.10	824.0
210.90	1846.0
214.80	550.0
216.00	1168.0
216.90	11756.0
218.00	1473.0
220.10	311.0
221.00	7848.0
223.00	2665.0
224.00	25408.0
225.00	6576.0
226.00	642.0
227.00	9897.0
227.90	1412.0
228.90	2399.0
229.90	312.0
231.00	886.0
233.90	619.0
234.90	479.0
235.90	508.0
237.00	781.0
238.90	385.0
239.90	313.0
240.90	589.0
242.00	1402.0
243.00	1439.0
244.00	19592.0
245.00	2443.0
245.90	3672.0
247.00	790.0
248.90	701.0
254.10	793.0
255.00	101480.0
256.00	14446.0
257.00	1308.0
258.00	5330.0
258.90	997.0
265.00	2045.0
266.00	358.0
271.90	354.0
272.90	3029.0
274.00	8128.0
275.00	47440.0
276.00	6540.0
277.00	3325.0
278.00	679.0
281.10	402.0

Instrument :
BNA_M
ClientSampleId :
DFTPP95

282.90	461.0
284.00	389.0
285.00	625.0
292.90	887.0
295.10	301.0
296.00	11976.0
296.90	1650.0
303.00	1461.0
303.90	396.0
314.00	683.0
314.90	1241.0
316.00	812.0
321.00	364.0
323.00	3729.0
323.90	811.0
326.90	981.0
328.00	436.0
332.00	371.0
332.90	395.0
334.00	2542.0
335.00	762.0
341.00	586.0
345.90	947.0
352.00	1069.0
353.00	723.0
354.00	1421.0
354.90	304.0
365.00	5323.0
366.00	855.0
371.00	408.0
372.10	2469.0
373.00	653.0
383.00	627.0
402.00	729.0
402.90	1437.0
404.00	618.0
421.00	1094.0
422.00	1197.0
423.00	7646.0
424.00	2031.0
441.00	22752.0
442.00	144640.0
443.00	27056.0
444.00	2699.0

Instrument :
BNA_M
ClientSampleId :
DFTPP95

m/z	Abundance
38.00	686.0
39.10	5435.0
40.00	1249.0
41.10	499.0
43.10	433.0
44.00	6192.0
49.00	577.0
50.00	15504.0
51.00	62240.0
52.00	3107.0
55.10	547.0
56.00	1857.0
57.00	4519.0
61.00	746.0
62.00	886.0
63.00	2207.0
64.00	406.0
65.00	1391.0
68.10	1130.0
69.00	59968.0
70.00	414.0
72.90	958.0
74.00	5934.0
75.00	9569.0
76.00	3138.0
77.10	69760.0
78.00	4324.0
79.00	4426.0
80.00	3277.0
81.00	4877.0
81.90	1296.0
83.00	1197.0
85.00	956.0
85.90	1290.0
87.00	628.0
91.00	1145.0
92.00	1215.0
93.00	7373.0
93.90	518.0
96.00	575.0
98.00	5571.0
99.00	4643.0
100.00	410.0
101.00	2899.0
102.90	1020.0
103.90	1546.0
105.00	1588.0
106.00	616.0
107.00	22376.0
108.00	3452.0
109.00	745.0
110.00	42280.0
111.00	6632.0
112.00	706.0
116.00	1304.0
117.00	17408.0
118.00	1238.0
120.00	313.0
122.00	1259.0
123.00	2673.0
123.90	997.0
125.00	1116.0
126.10	607.0
127.00	84152.0
128.00	6404.0
129.00	31632.0
130.00	2822.0
131.00	589.0
133.00	479.0
134.00	1113.0
134.90	2487.0
135.90	960.0
137.00	1485.0
137.80	390.0
139.90	423.0
141.00	4192.0
142.00	1319.0
143.00	901.0
144.00	373.0
145.90	769.0
147.00	2294.0
148.00	4429.0
149.00	1034.0
151.10	488.0
151.80	320.0
153.00	1257.0
153.90	998.0
155.00	2040.0
156.00	3617.0
157.00	798.0
157.90	865.0

Instrument :
BNA_M
ClientSampleId :
DFTPP95

158.90	587.0
159.90	1345.0
161.00	1781.0
161.90	504.0
165.00	1496.0
166.00	1163.0
167.00	8271.0
168.00	4061.0
169.00	737.0
169.90	349.0
171.00	381.0
171.90	745.0
173.00	1000.0
174.00	1742.0
175.00	3519.0
175.90	836.0
176.90	1541.0
178.00	388.0
179.00	5741.0
180.00	4629.0
181.00	2074.0
182.00	367.0
183.90	492.0
185.00	3101.0
186.00	23352.0
187.00	6736.0
188.00	937.0
188.90	1513.0
190.90	890.0
192.00	1906.0
193.00	2575.0
194.00	574.0
195.10	311.0
196.00	5041.0
196.80	1064.0
197.90	172160.0
198.90	11998.0
200.00	834.0
201.30	936.0
203.00	1150.0
204.00	6339.0
205.00	10722.0
206.00	44496.0
207.00	6901.0
207.90	1716.0
209.00	741.0
210.00	679.0
211.00	1854.0
214.80	424.0
216.00	792.0
217.00	10999.0
218.00	1644.0
221.00	7836.0
221.80	1733.0
223.00	2721.0
224.00	25272.0
225.00	6233.0
226.00	605.0
227.00	9438.0
228.00	1406.0
228.90	2263.0
231.00	784.0
234.00	643.0
234.90	689.0
236.00	479.0
237.00	809.0
239.00	373.0
241.00	651.0
242.00	1406.0
243.00	1404.0
244.00	19392.0
245.00	2647.0
246.00	3651.0
246.90	790.0
249.00	686.0
252.90	368.0
254.00	687.0
255.00	102320.0
256.00	15134.0
257.00	1274.0
258.00	5521.0
259.00	927.0
265.00	2359.0
266.00	346.0
273.00	3040.0
274.00	8606.0
275.00	46992.0
276.00	6228.0
277.00	4053.0
277.90	560.0
281.00	474.0
283.00	493.0
284.90	635.0
292.90	965.0
296.00	11862.0

Instrument :
BNA_M
ClientSampleId :
DFTPP95

297.00	1698.0
302.90	1516.0
303.90	322.0
314.10	570.0
315.00	1462.0
316.00	825.0
321.00	352.0
323.00	4465.0
324.00	800.0
326.90	957.0
327.90	408.0
331.90	314.0
333.00	325.0
334.00	2578.0
335.00	603.0
341.00	440.0
346.00	900.0
352.00	1422.0
353.00	868.0
354.00	1592.0
355.00	367.0
364.90	5890.0
365.90	1000.0
370.90	360.0
372.00	2301.0
373.00	650.0
383.00	571.0
390.00	335.0
402.00	1109.0
403.00	1446.0
404.00	633.0
421.00	1252.0
421.90	1092.0
423.00	9522.0
424.00	1842.0
441.00	27720.0
442.00	177472.0
443.00	34248.0
444.00	3098.0

Instrument :
BNA_M
ClientSampleId :
DFTPP95

Scan 2622 (18.509 min): BM002324.D
DFTPP95

m/z	Abundance
40.00	961.0
41.10	413.0
43.00	338.0
44.00	6357.0
55.00	415.0
73.00	547.0
207.00	1572.0
208.00	360.0
281.10	405.0

Instrument :
BNA_M
ClientSampleId :
DFTPP95