

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081216\
 Data File : BM007055.D
 Acq On : 12 Aug 2016 23:06
 Operator : UM/SJ
 Sample : H4389-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PR002-SS005-0612-01

Quant Time: Aug 13 00:44:46 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 12 23:03:04 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	223276	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	876672	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	516578	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1232642	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1576291	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	1674666	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	23063	4.51	ng/uL	0.01
5) Phenol-d5	6.97	99	438651	24.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	261827	25.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	362498	25.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	346050	23.25	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	170704	26.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	187356	27.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	359153	25.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	409786	24.17	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	1166046	27.32	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1411832	27.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	174356	22.79	ng/ul	0.00
57) Fluorene-d10	15.43	176	1018018	27.28	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	149692	21.98	ng/ul	0.00
70) Anthracene-d10	17.28	188	1643559	28.78	ng/ul	0.00
76) Pyrene-d10	19.57	212	1947350	29.27	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	2219833	28.98	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.90	163	612881	14.37 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081216\
Data File : BM007055.D
Acq On : 12 Aug 2016 23:06
Operator : UM/SJ
Sample : H4389-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PR002-SS005-0612-01

Quant Time: Aug 13 00:44:46 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 12 23:03:04 2016
Response via : Initial Calibration

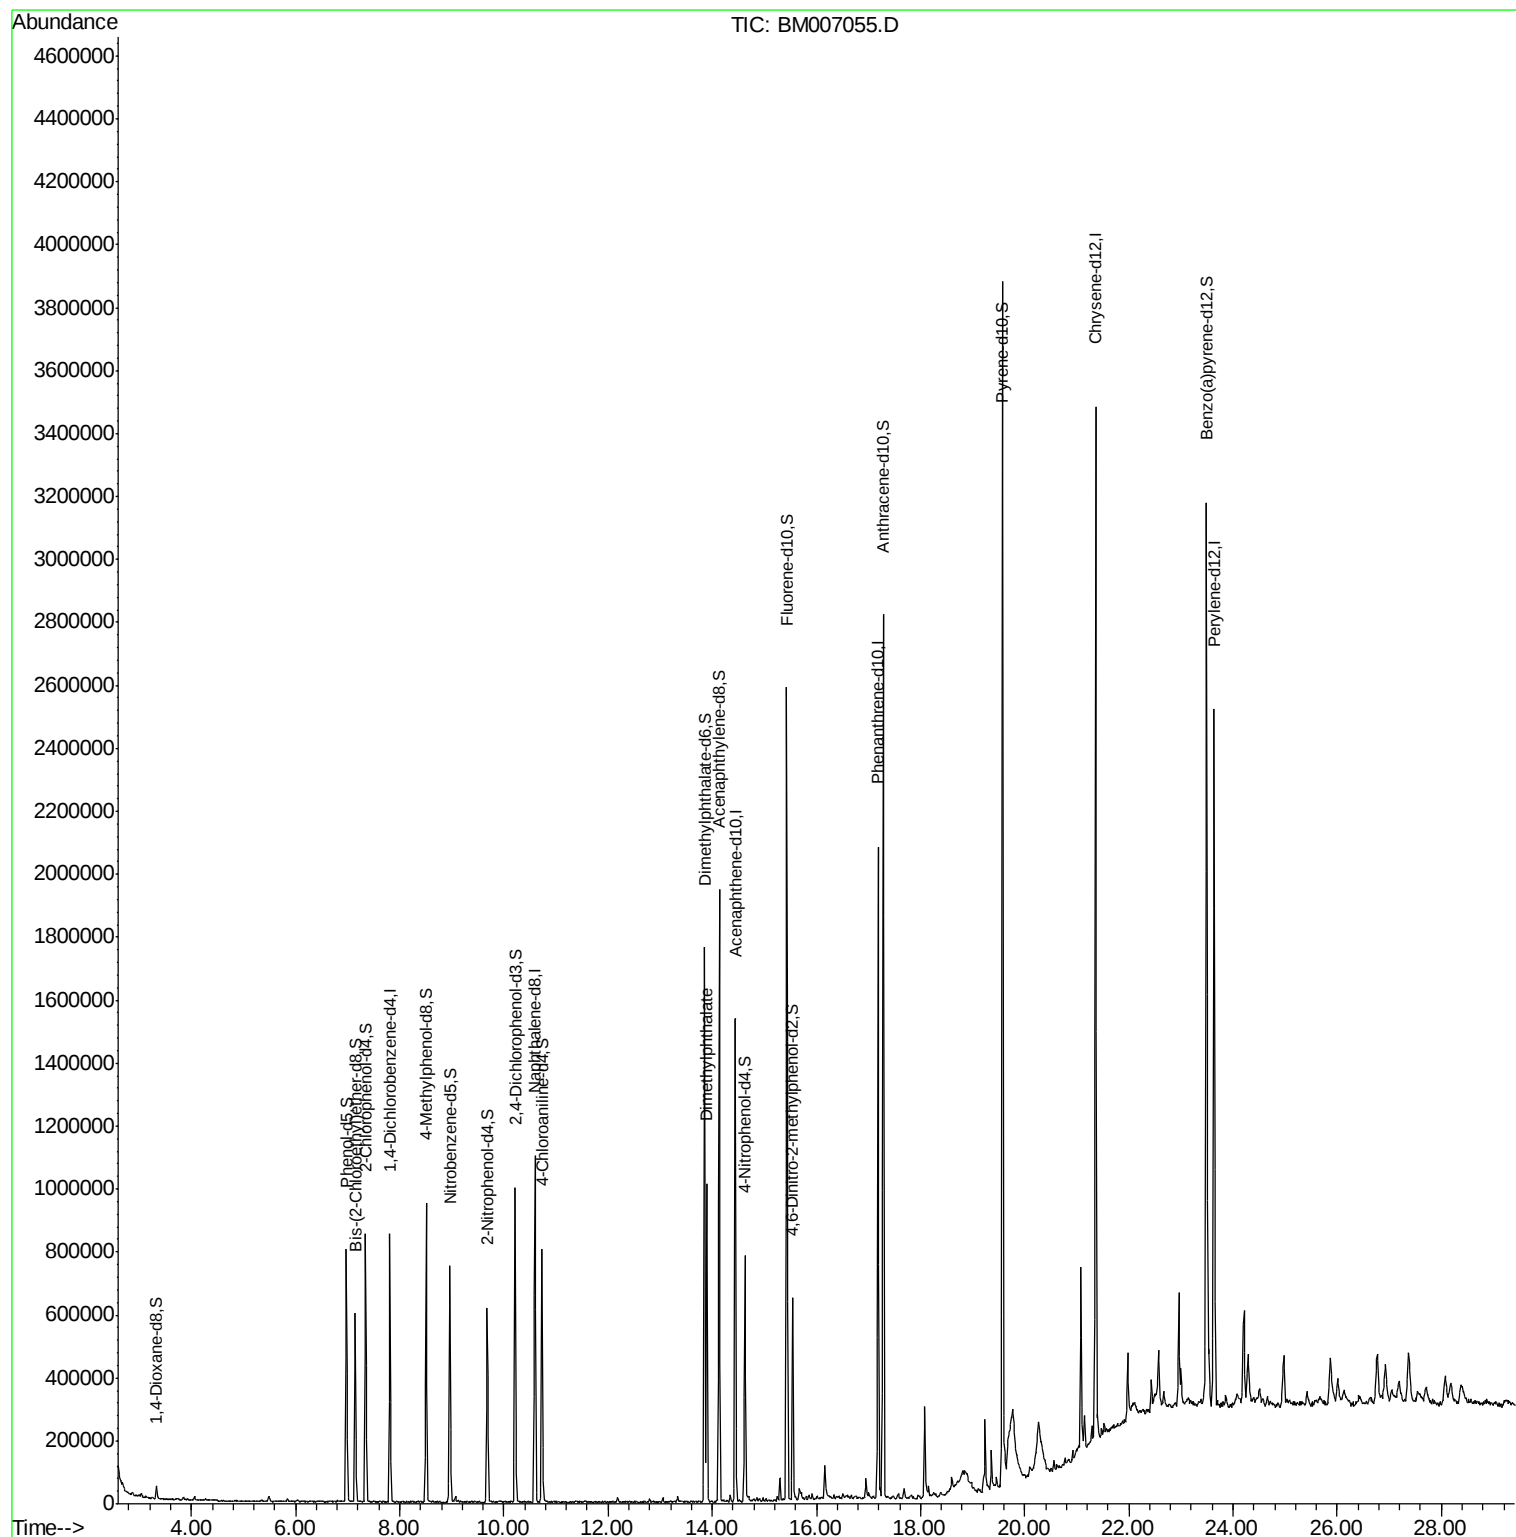

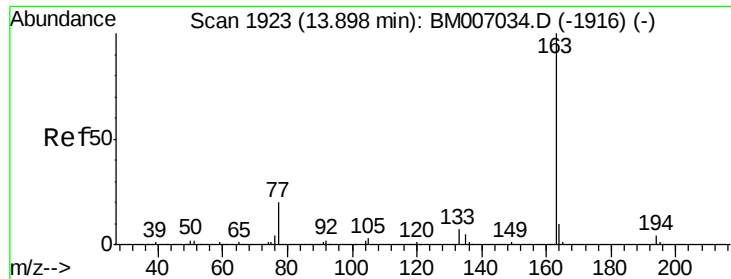

#44

Dimethylphthalate

Concen: 14.37 ng/ul

RT: 13.90 min Scan# 1923

Delta R.T. -0.00 min

Lab File: BM007055.D


Acq: 12 Aug 2016 23:06

Instrument :

BNA_M

ClientSampleId :

PR002-SS005-0612-01

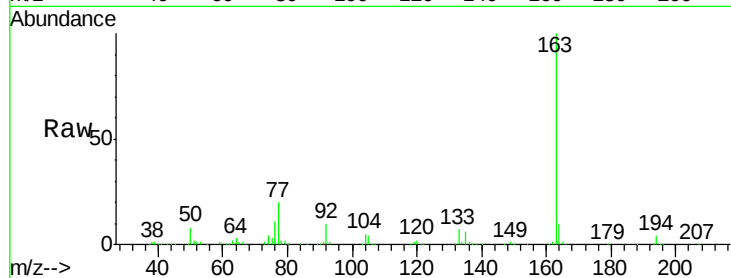

Tgt Ion:	163	Resp:	612881
Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.2
164	10.2	7.8	11.8

