

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081216\
 Data File : BM007058.D
 Acq On : 13 Aug 2016 00:55
 Operator : UM/SJ
 Sample : H4389-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PR002-SS005-3642-01

Quant Time: Aug 13 03:42:08 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 00:47:53 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	225687	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	876730	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	509878	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1219977	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1614104	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	1695623	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	34148	6.61	ng/uL	0.00
5) Phenol-d5	6.97	99	634217	34.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	379346	36.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	524357	36.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	510285	33.92	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	244765	38.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	272108	40.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	505896	35.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	660919	38.98	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	1590430	37.75	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1954031	38.61	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	252179	33.40	ng/ul	0.00
57) Fluorene-d10	15.43	176	1376295	37.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	221667	32.88	ng/ul	0.00
70) Anthracene-d10	17.28	188	2195386	38.84	ng/ul	0.00
76) Pyrene-d10	19.57	212	2625924	38.54	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	3045179	39.26	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.90	163	813273	19.31	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081216\
Data File : BM007058.D
Acq On : 13 Aug 2016 00:55
Operator : UM/SJ
Sample : H4389-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PR002-SS005-3642-01

Quant Time: Aug 13 03:42:08 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 00:47:53 2016
Response via : Initial Calibration

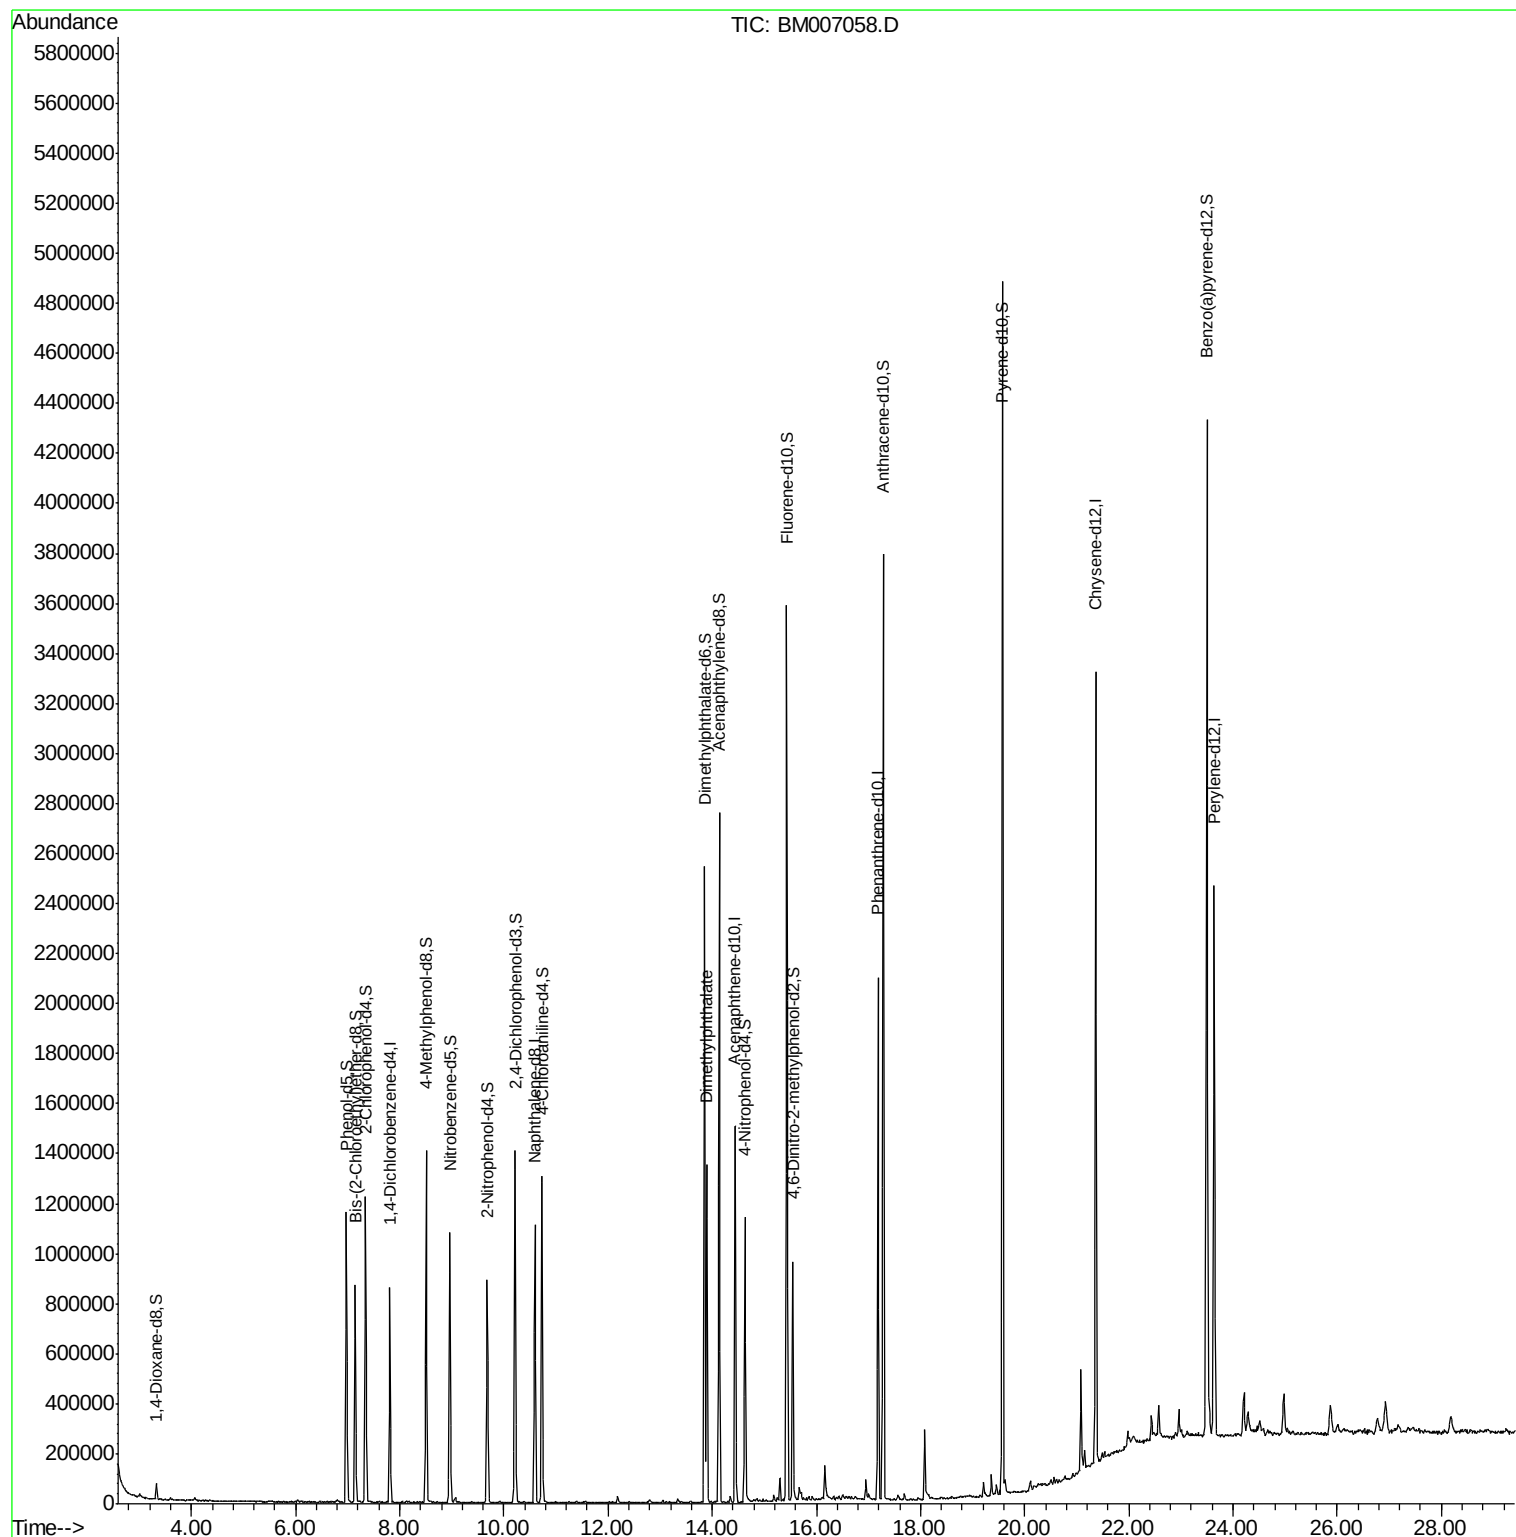

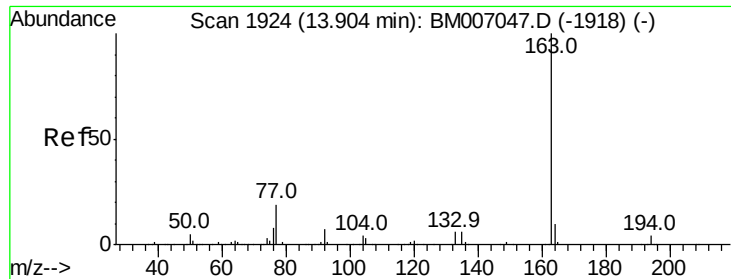

#44

Dimethylphthalate

Concen: 19.31 ng/ul

RT: 13.90 min Scan# 1923

Delta R.T. -0.01 min

Lab File: BM007058.D

Acq: 13 Aug 2016 00:55

Instrument :

BNA_M

ClientSampleId :

PR002-SS005-3642-01


Tot Ion:163 Resp: 813273

Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.2

164 10.3 7.8 11.8

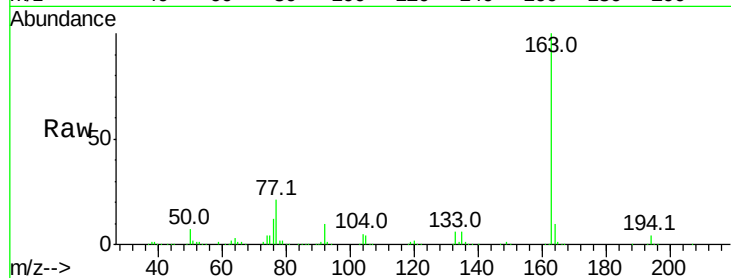

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

