
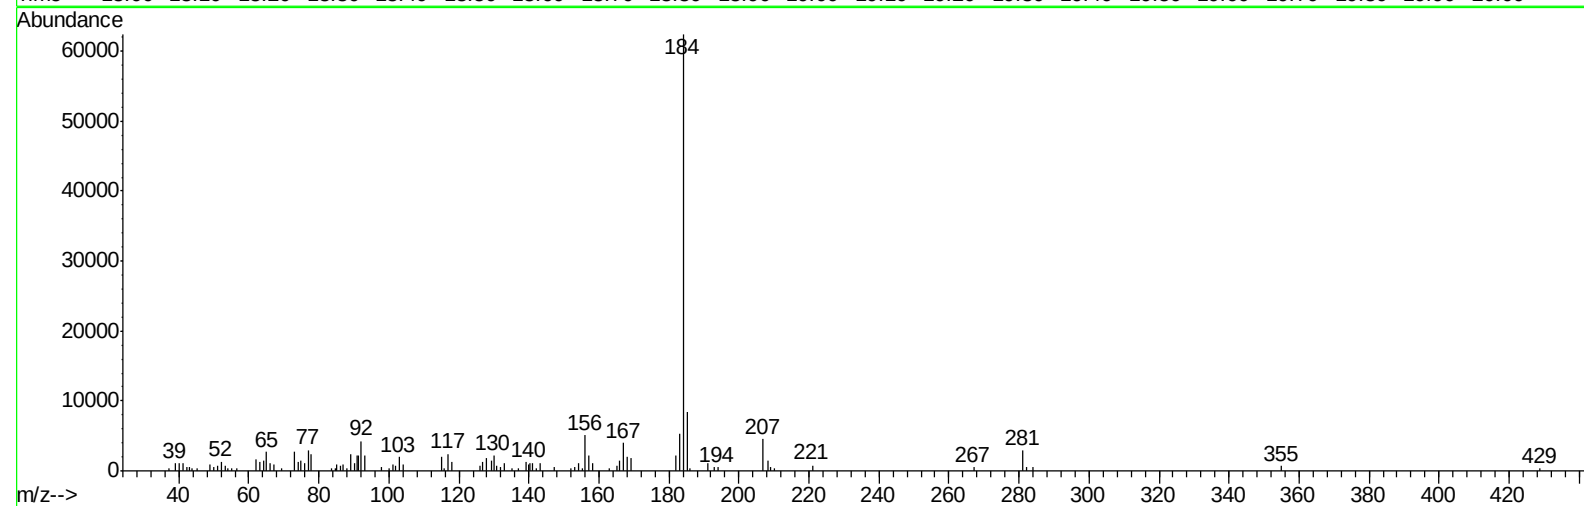


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081217\
Data File : BM011213.D
Acq On : 12 Aug 2017 11:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 04:40:11 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

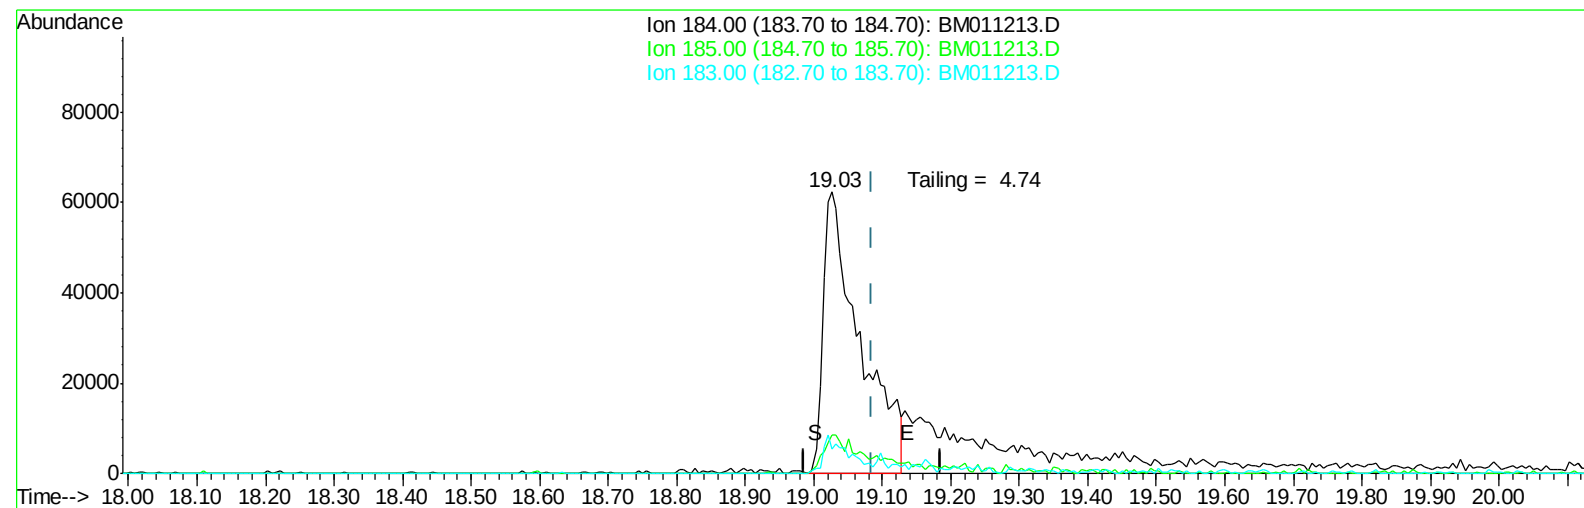

TIC: BM011213.D

(76) Benzidine



19.027min (-0.059) 90116.37ng

response 232830

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.46
183.00	11.10	8.50#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081217\
Data File : BM011213.D
Acq On : 12 Aug 2017 11:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 04:40:11 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM072617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 26 17:29:06 2017
Response via : Initial Calibration

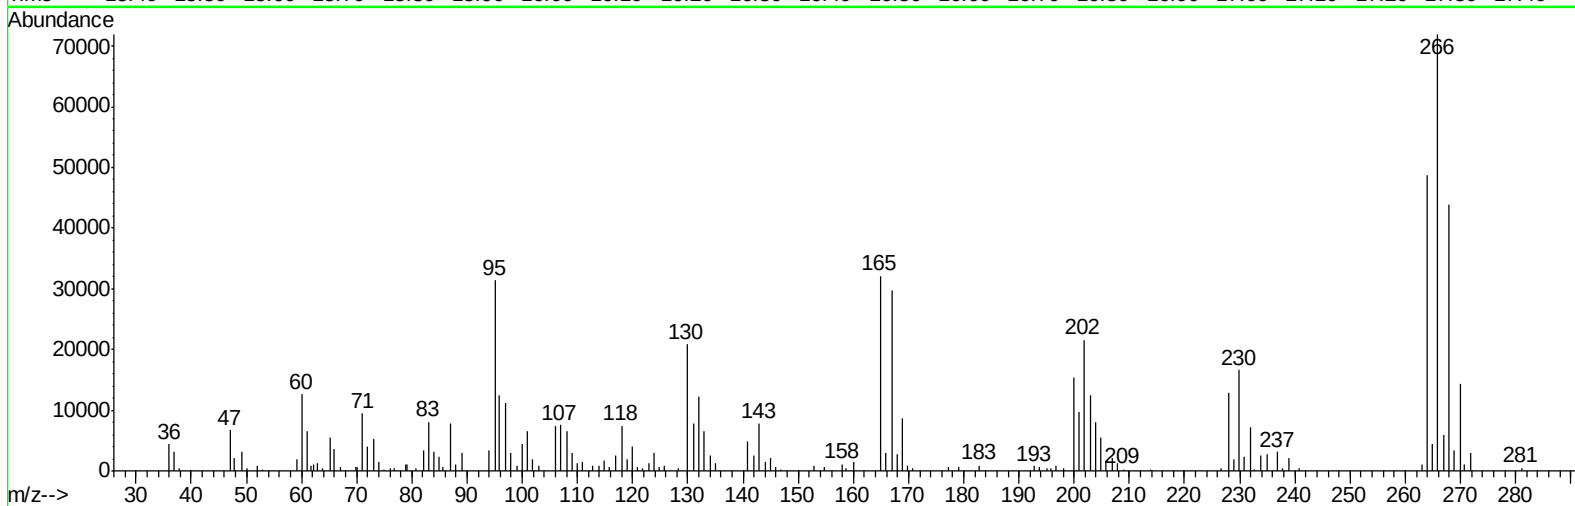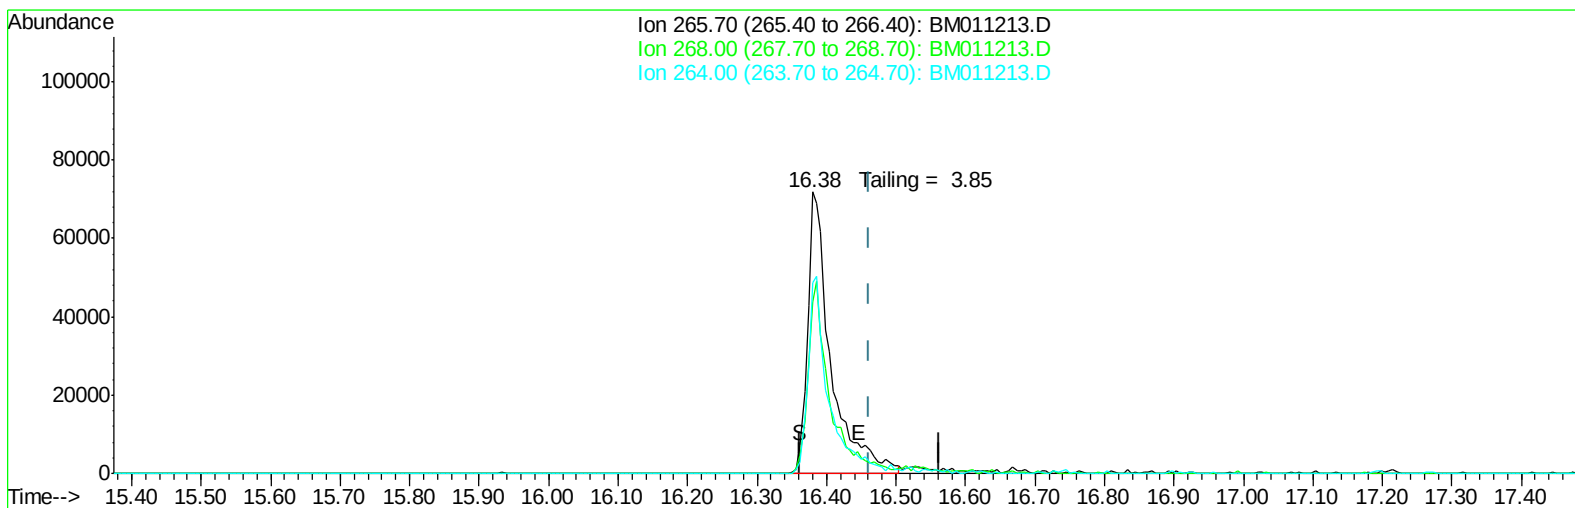

TIC: BM011213.D

(69) Pentachlorophenol (C)

16.380min (-0.083) 0.00ng

response 121781

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.06
264.00	61.20	67.67
0.00	0.00	0.00