


Data Path : Z:\HPCHEM1\BNA M\Data\BM081217\
 Data File : BM011213.D
 Acq On : 12 Aug 2017 11:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 14 16:03:18 2017

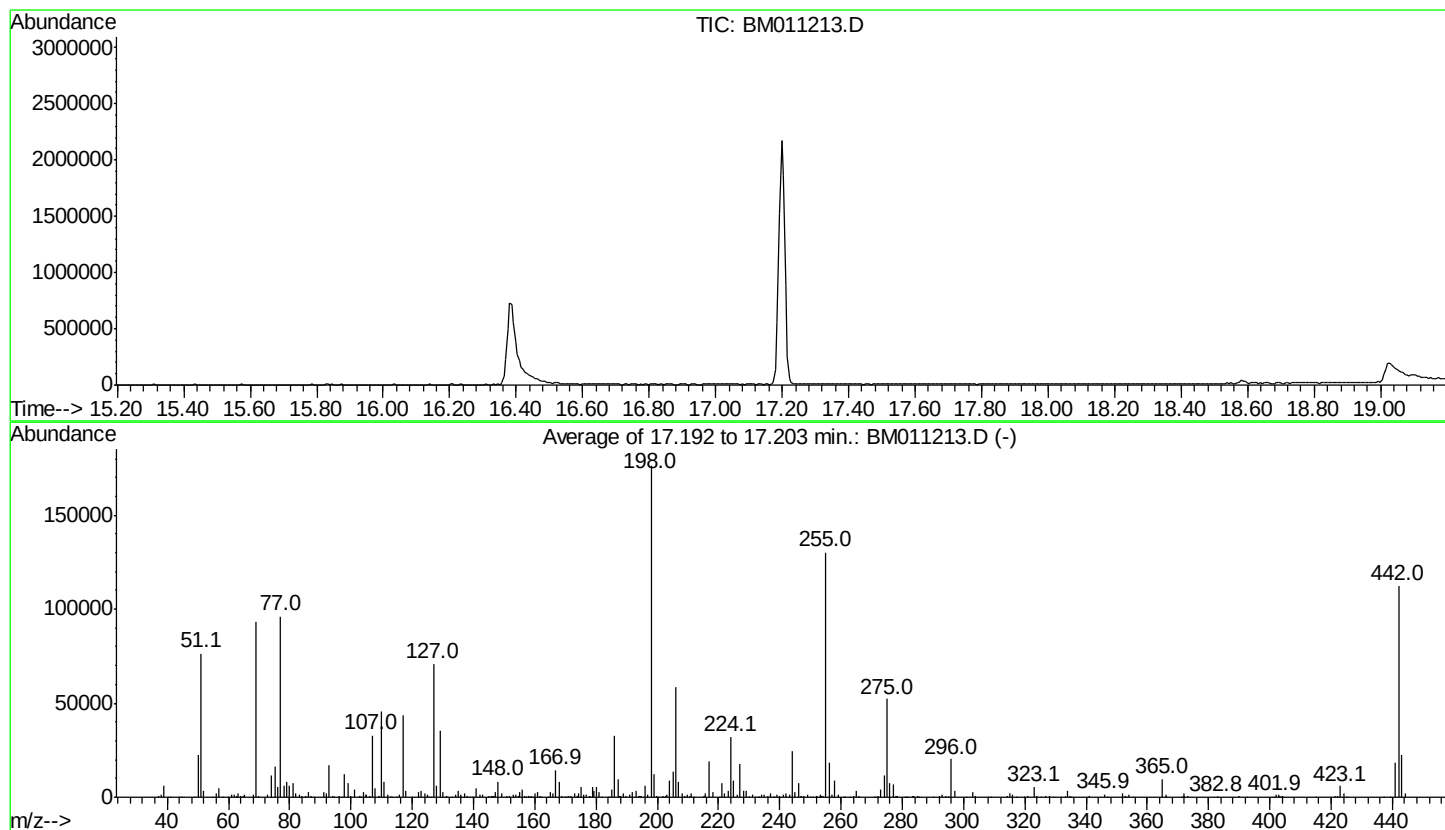

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	76560	PASS
68	69	0.00	2	1.8	1655	PASS
69	198	0.00	100	53.1	93557	PASS
70	69	0.00	2	0.9	847	PASS
127	198	10	80	40.2	70834	PASS
197	198	0.00	2	0.6	1087	PASS
198	198	100	100	100.0	176320	PASS
199	198	5	9	6.8	12024	PASS
275	198	10	60	29.6	52141	PASS
365	198	1	100	5.5	9636	PASS
441	443	0.01	100	79.6	18106	PASS
442	198	50	100	63.9	112589	PASS
443	442	15	24	20.2	22760	PASS