

Data File : BM022094.D
Acq On : 14 Aug 2019 06:25
Operator : HP/JU
Sample : K4183-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH6

Quant Time: Aug 14 08:20:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 08:16:48 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	957	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.38	136	3994	0.40	ng/ul	-0.04
6) Acenaphthene-d10	14.26	164	2057	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.11	188	182338	0.40	ng/ul	0.07
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.43	264	4860	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	1097	0.17	ng/ul	-0.03
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.28	252	978	0.059	ng/ul#	Qvalue 10




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM022094.D
Acq On : 14 Aug 2019 06:25
Operator : HP/JU
Sample : K4183-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH6

Quant Time: Aug 14 08:20:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 08:16:48 2019
Response via : Initial Calibration

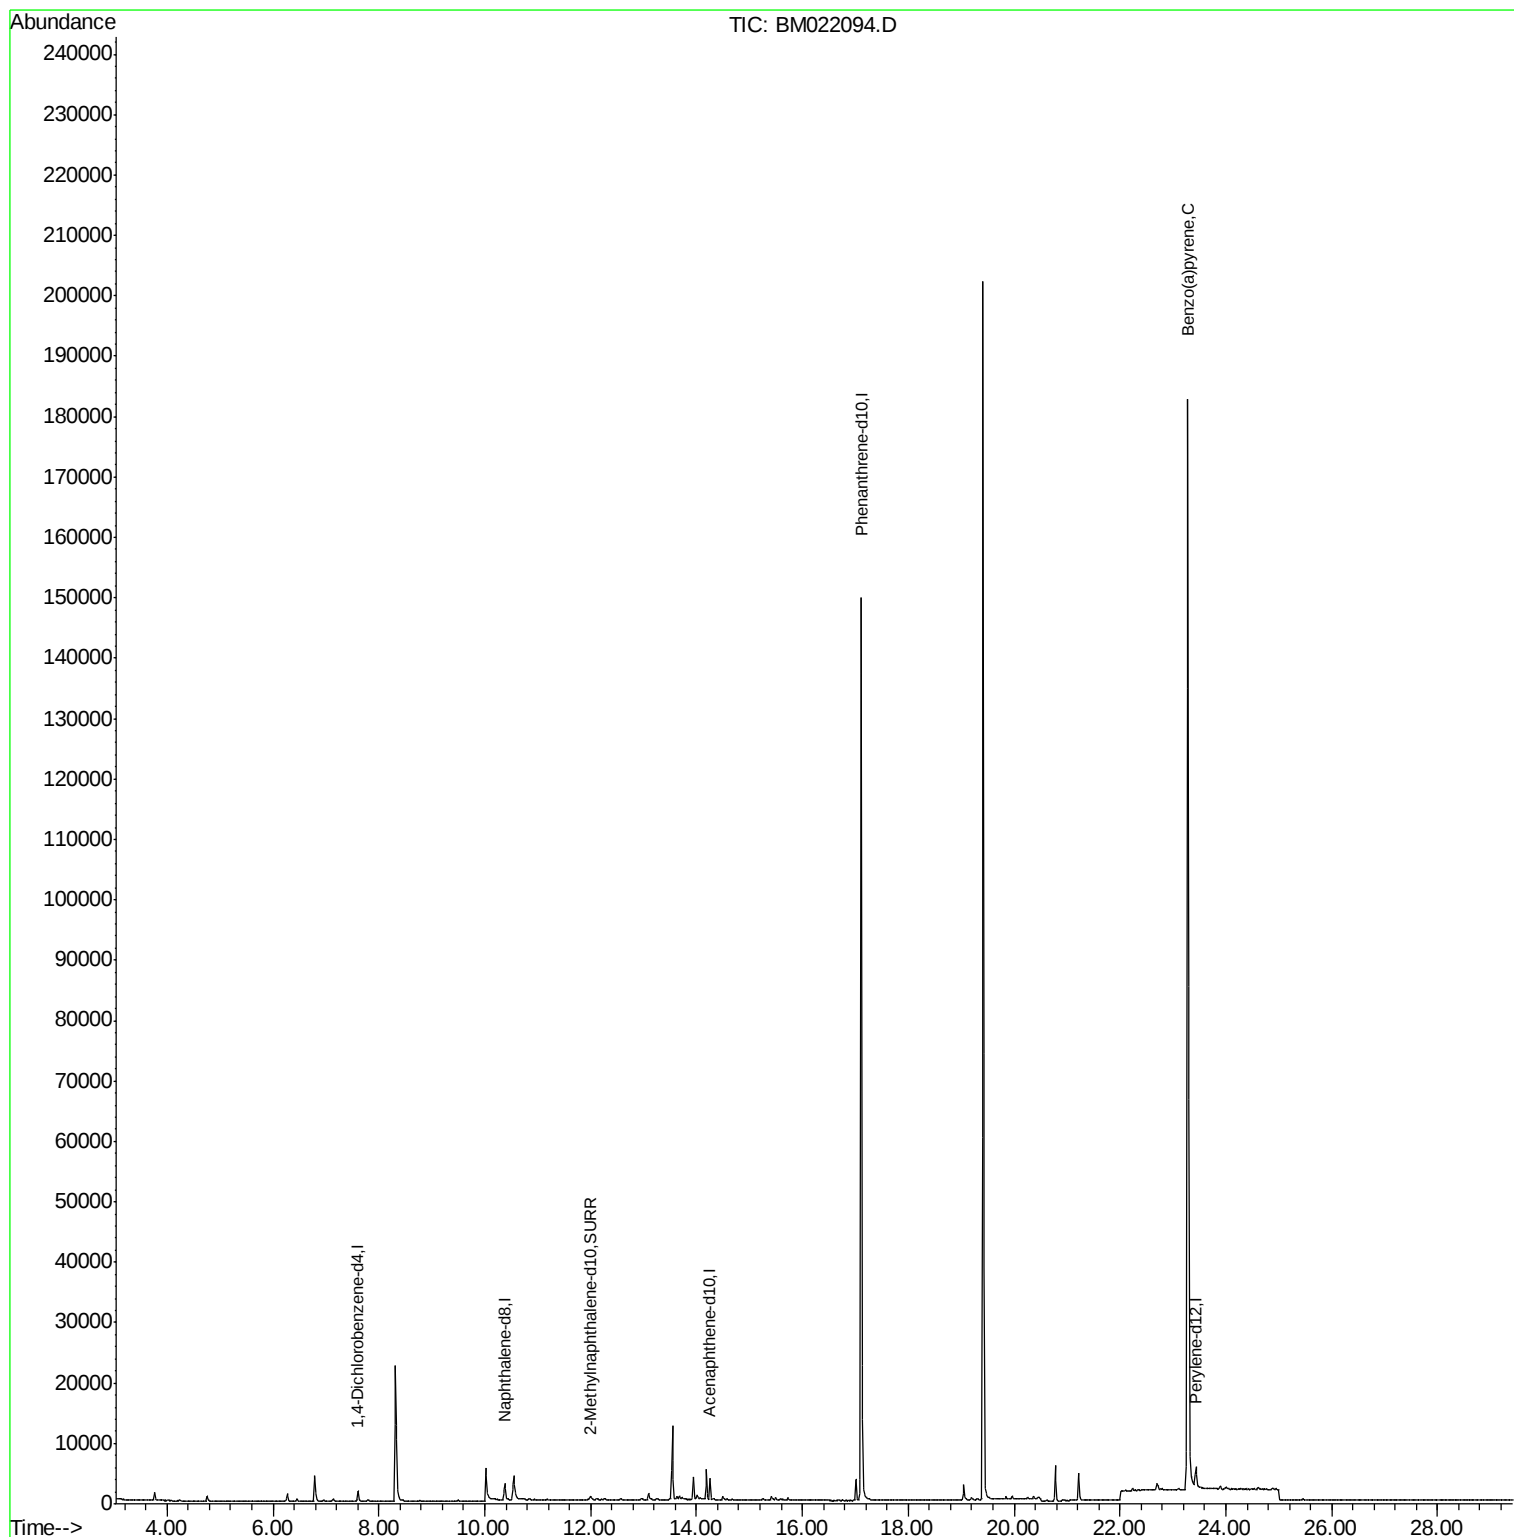

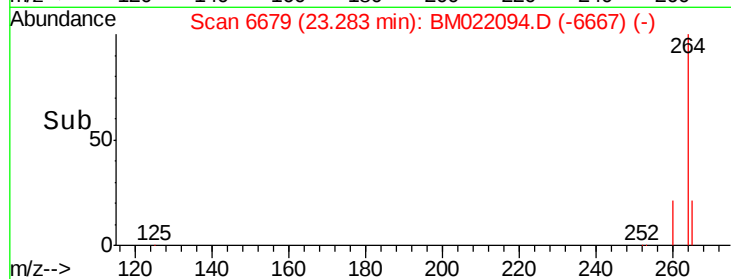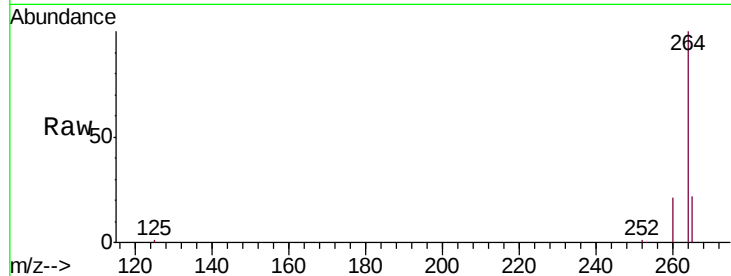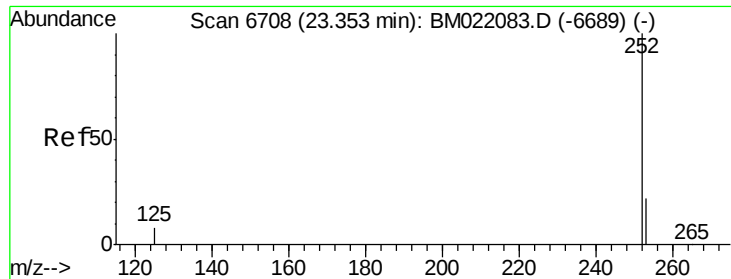

#23

Benzo(a)pyrene

Concen: 0.059 ng/ul

RT: 23.28 min Scan# 6679

Delta R.T. -0.07 min

Lab File: BM022094.D

Acq: 14 Aug 2019 06:25

Instrument :

BNA_M

ClientSampleId :

C0AH6

Tgt Ion: 252 Resp: 978

Ion Ratio Lower Upper

252 100

253 77.2 31.7 47.5#

125 85.5 14.6 21.8#

