


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
Data File : BM022031.D
Acq On : 12 Aug 2019 14:39
Operator : HP/JU
Sample : K3962-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP07

Manual Integrations
APPROVED

mohammad
8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:47:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 14:07:26 2019
Response via : Initial Calibration

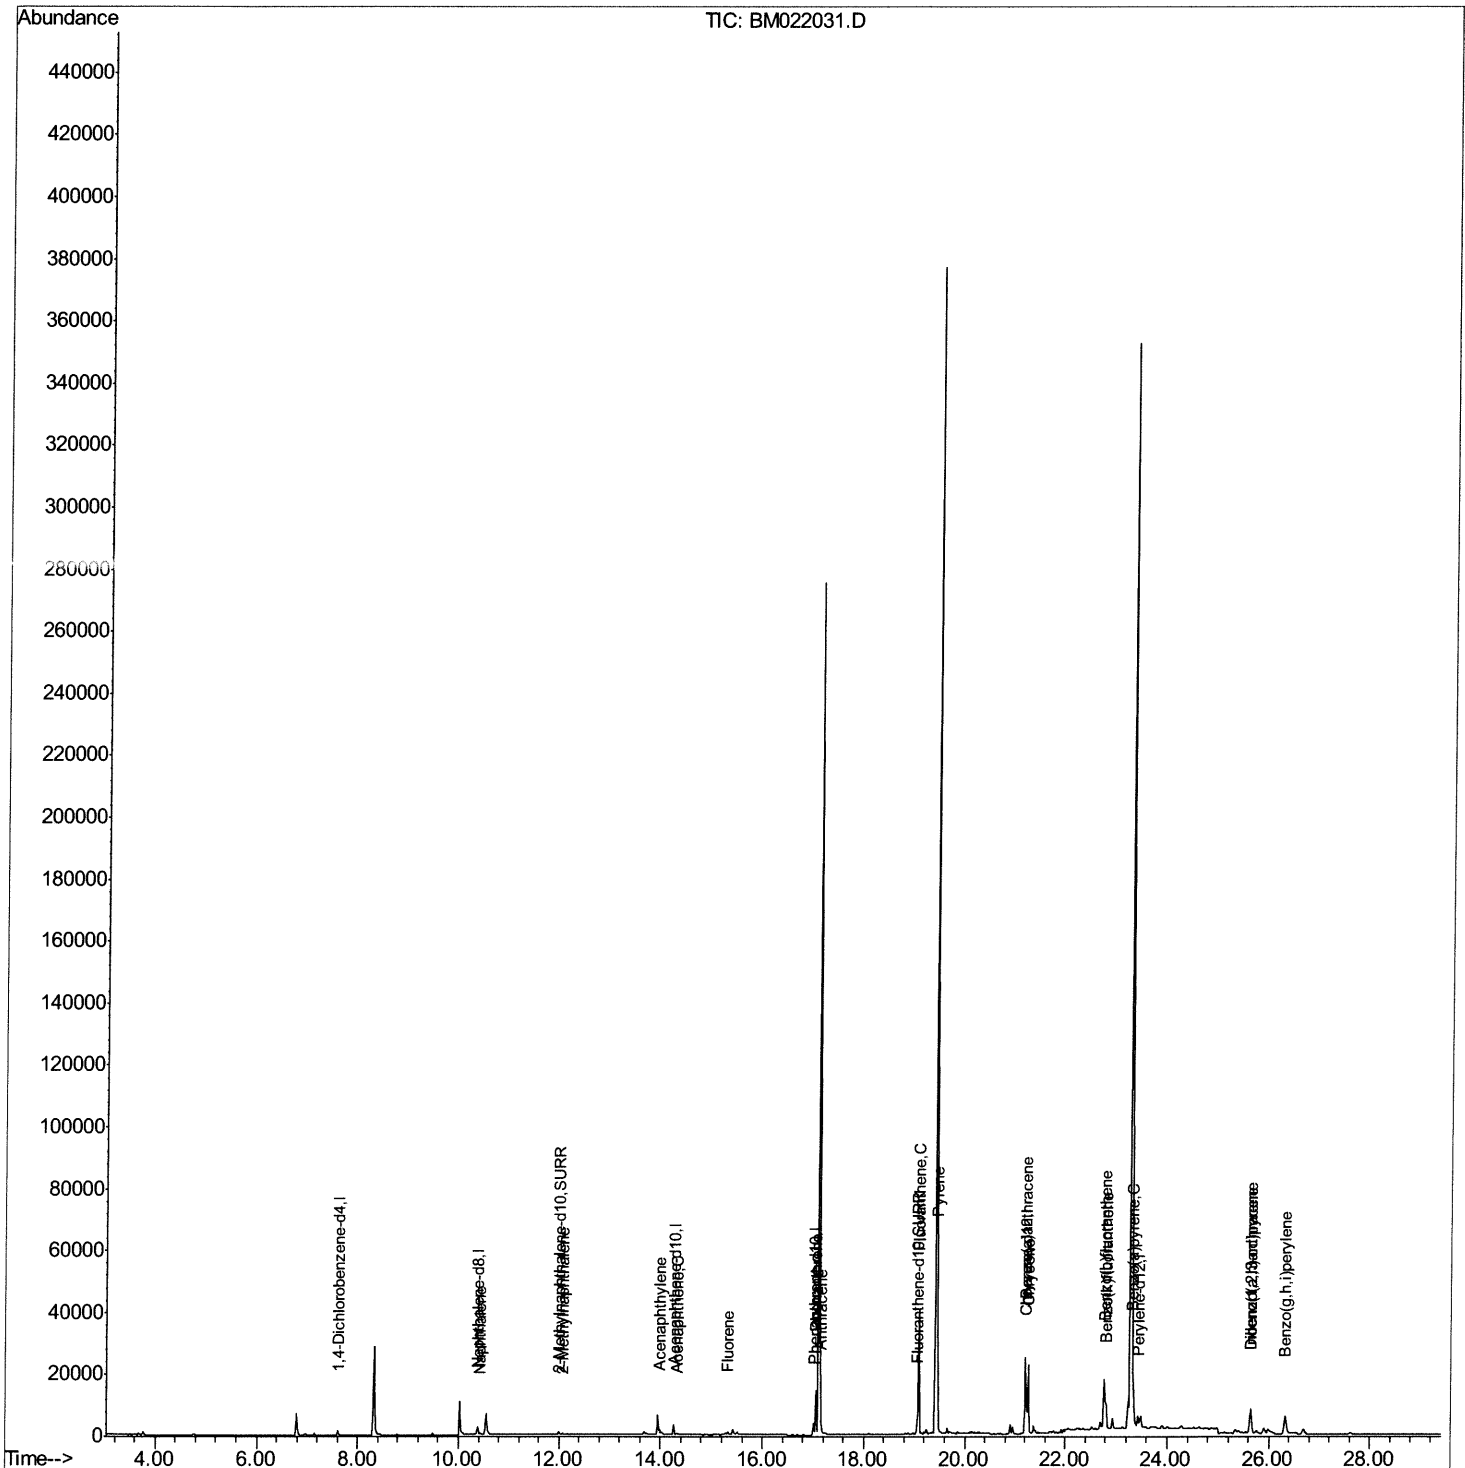

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP07

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:36:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

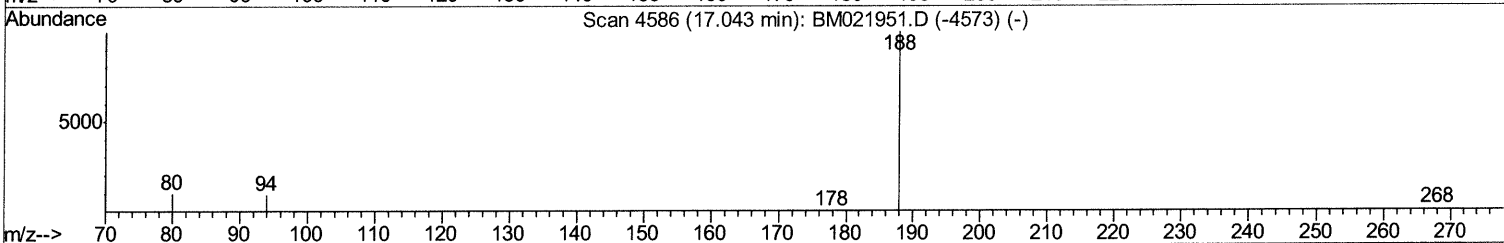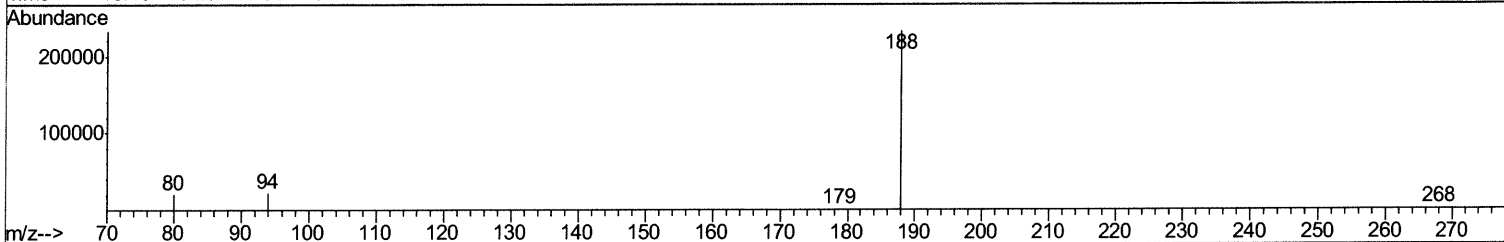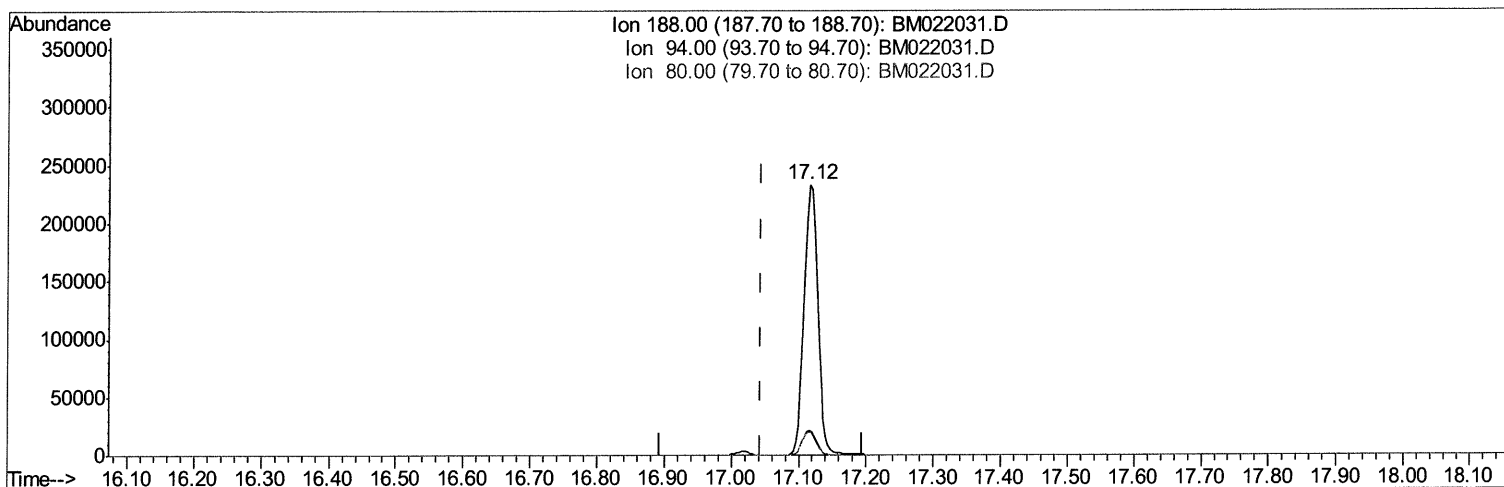

TIC: BM022031.D

(10) Phenanthrene-d10 (I)
 17.116min (+0.071) 0.40ng/ul
 response 326150

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	9.33
80.00	11.40	8.86#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BEP07

Manual Integrations
APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:36:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

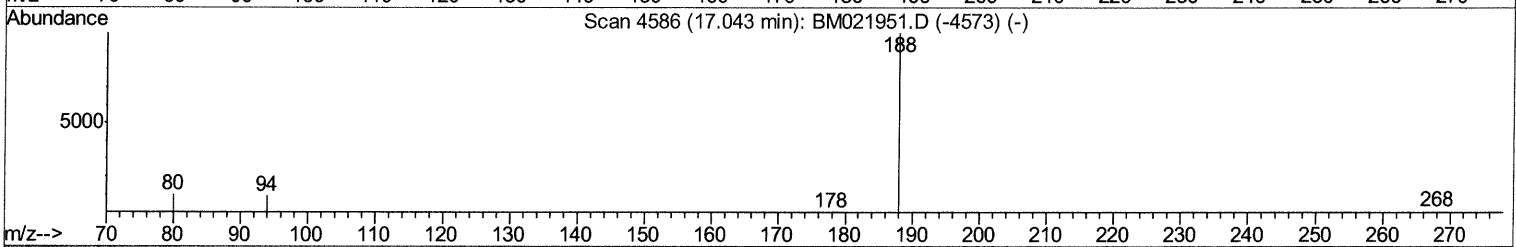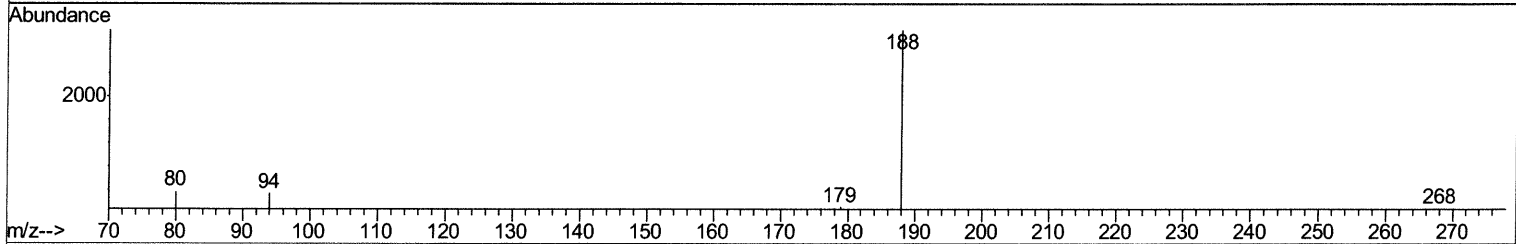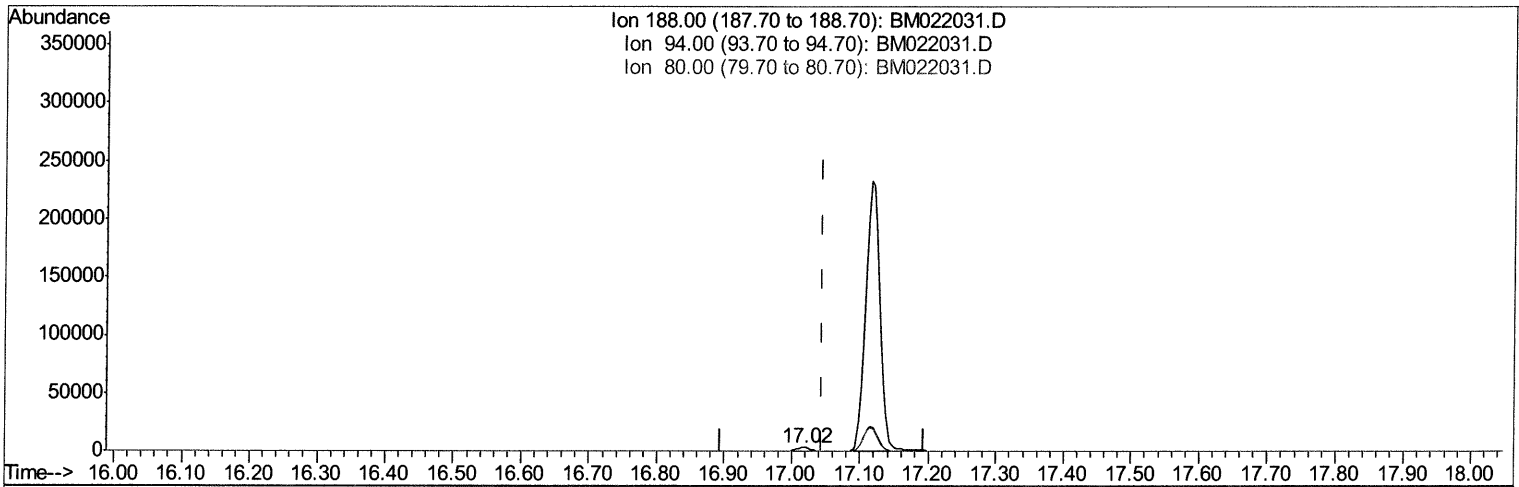

TIC: BM022031.D

(10) Phenanthrene-d10 (I)

17.018min (-0.026) 0.40ng/ul m *JU 08/13/19*

response 4447

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.33
80.00	11.40	11.13
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
Data File : BM022031.D
Acq On : 12 Aug 2019 14:39
Operator : HP/JU
Sample : K3962-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP07

Manual Integrations
APPROVED

mohammad
8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:37:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 14:07:26 2019
Response via : Initial Calibration

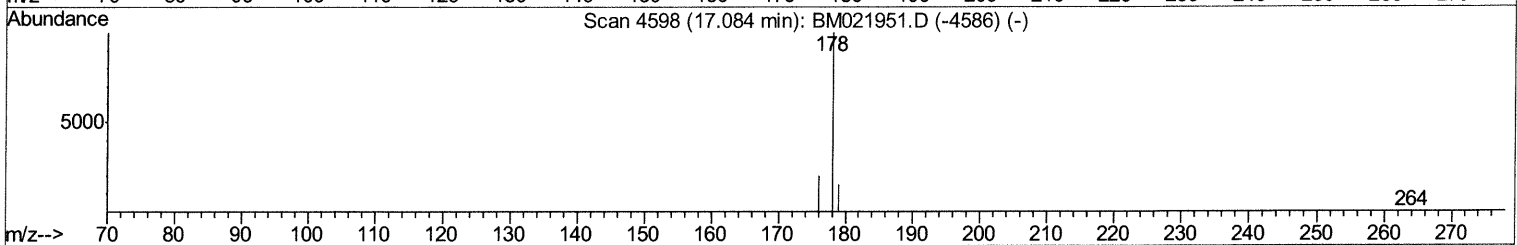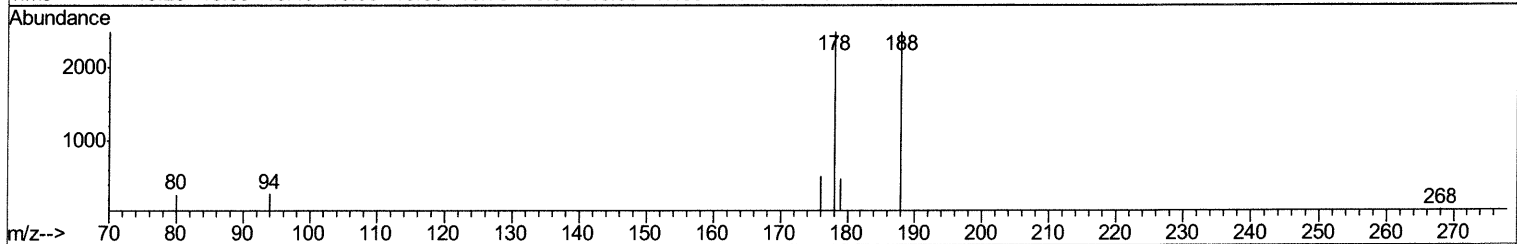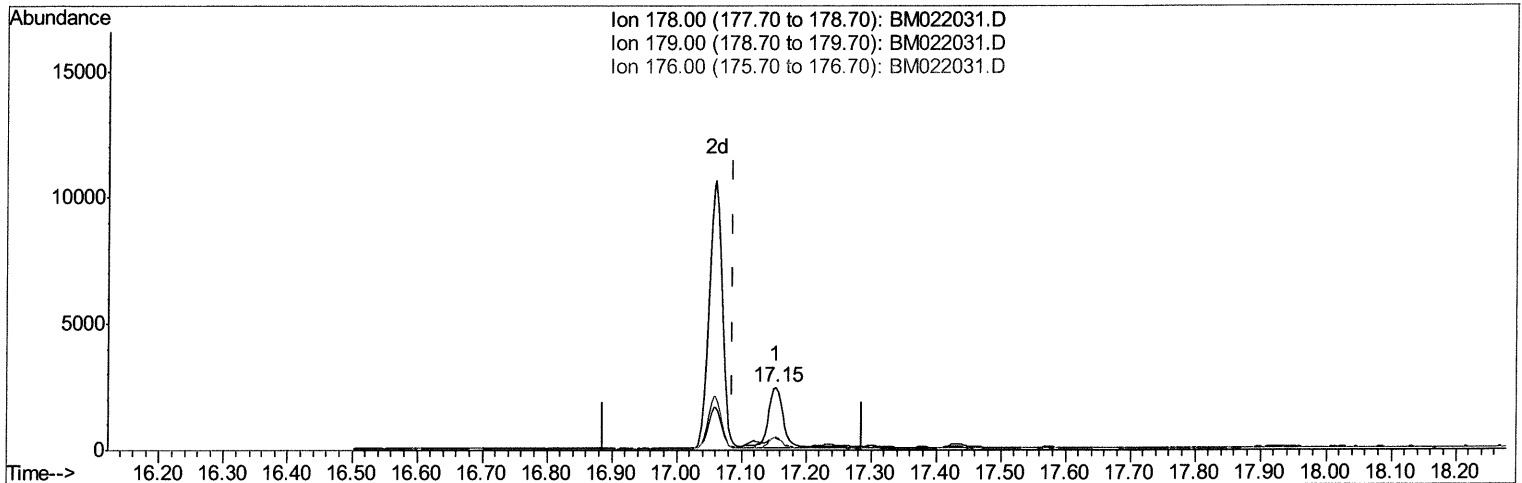

TIC: BM022031.D

(12) Phenanthrene

17.154min (+0.068) 0.29ng/ul

response 3790

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	19.66
176.00	21.00	21.19
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP07

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:37:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

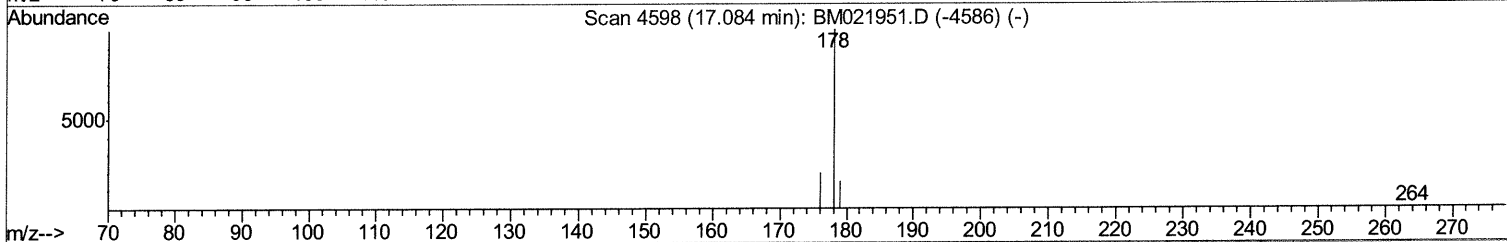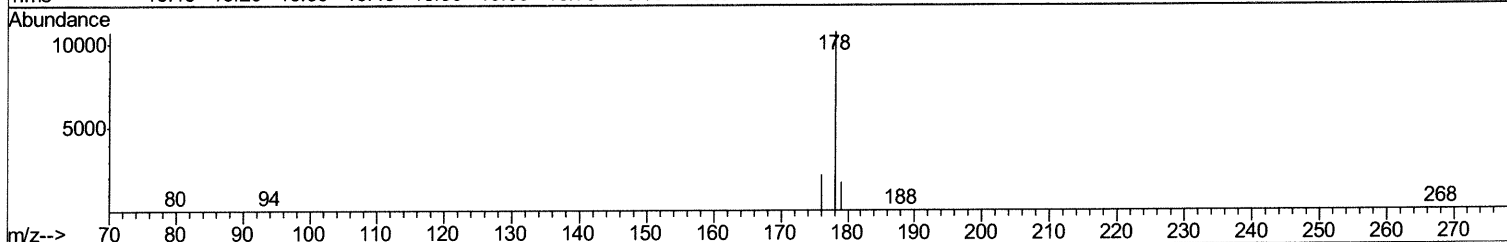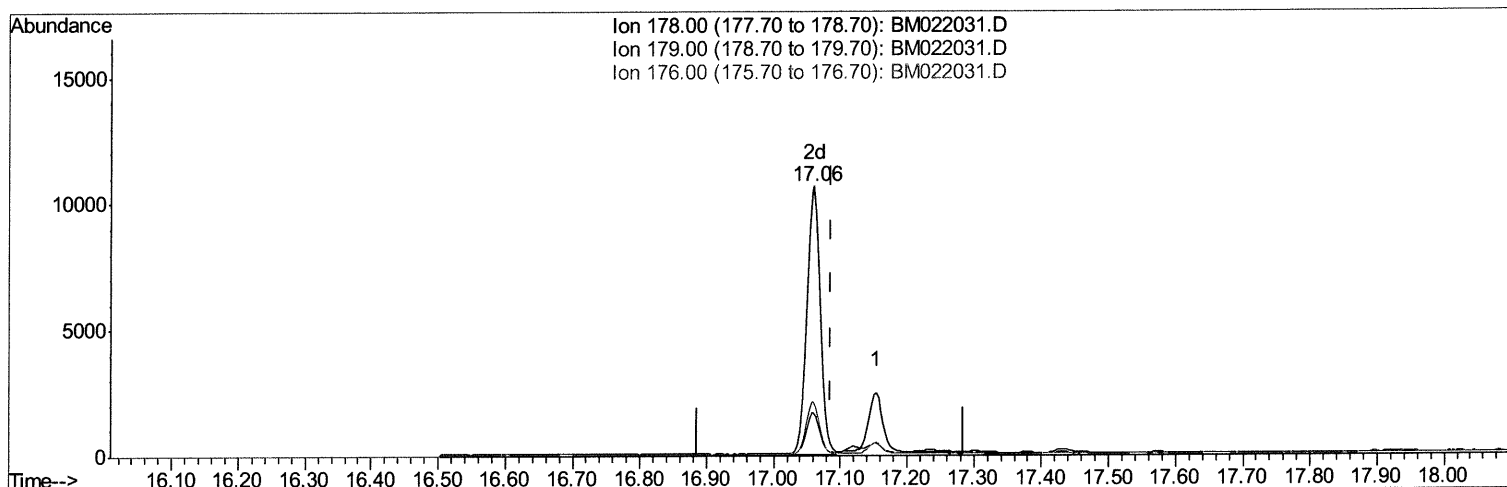

(12) Phenanthrene

17.060min (-0.026) 1.17ng/ul m *JU 08/13/19*

response 15140

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	15.95
176.00	21.00	20.15
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP07

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:37:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

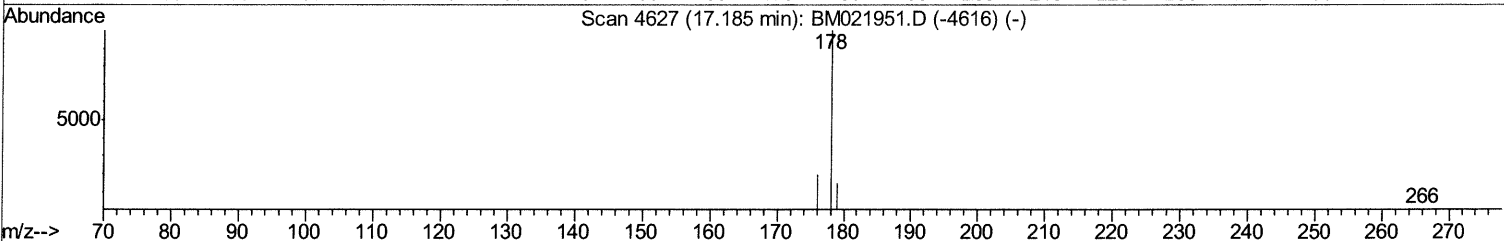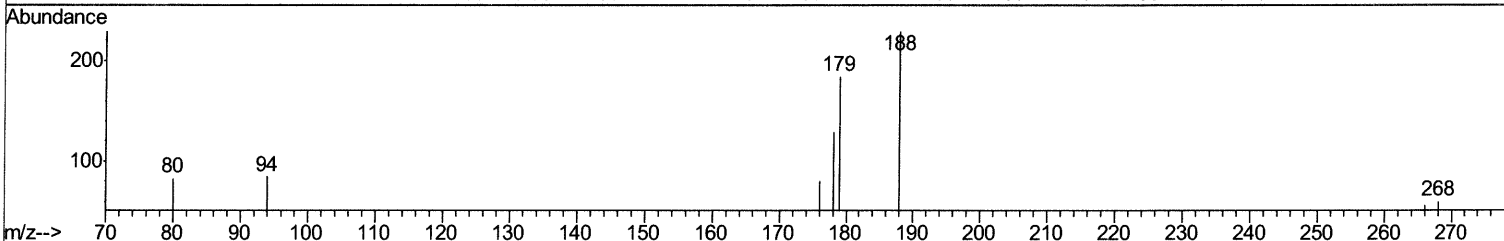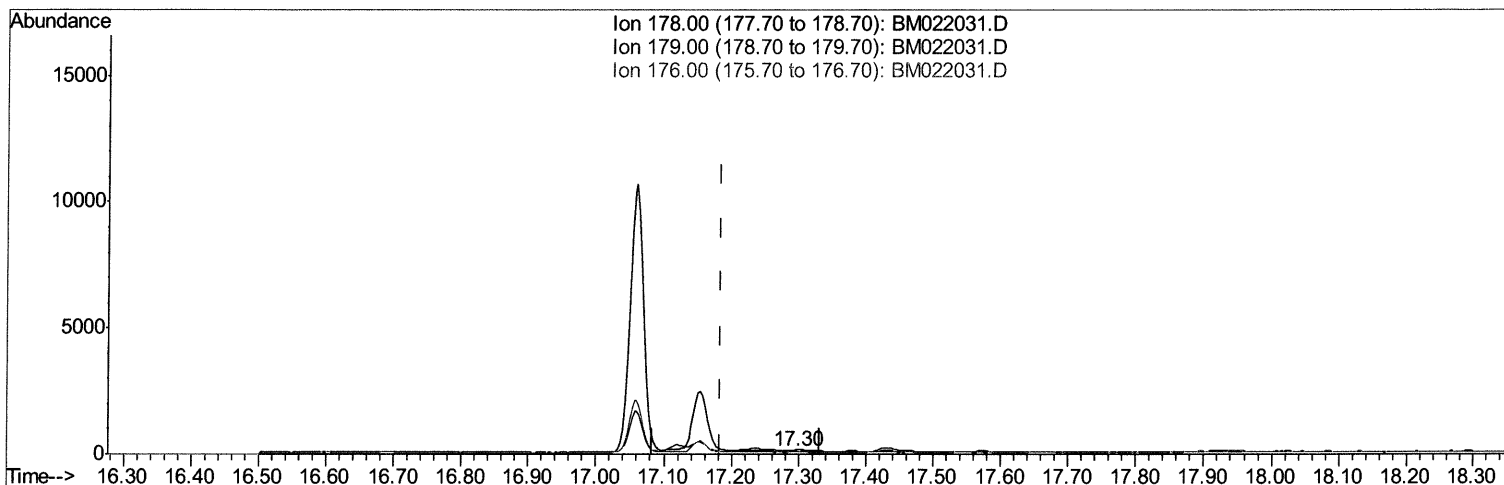

TIC: BM022031.D

(13) Anthracene

17.296min (+0.113) 0.01ng/ul

response 94

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	142.64#
176.00	20.80	62.02#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BEP07

Manual Integrations
APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:37:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

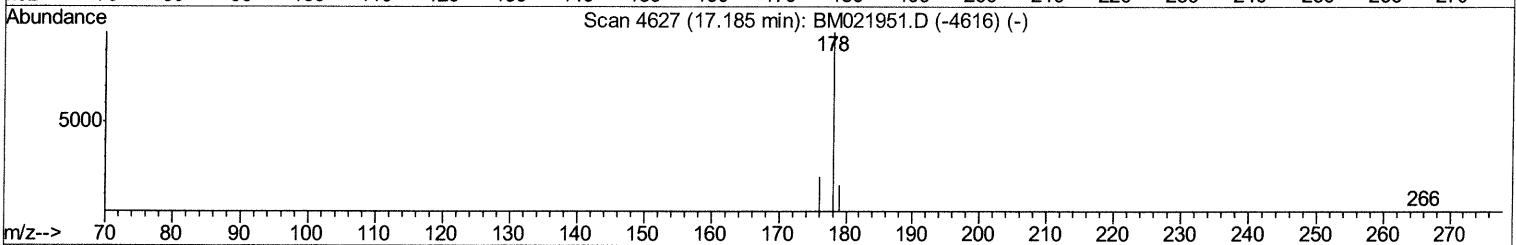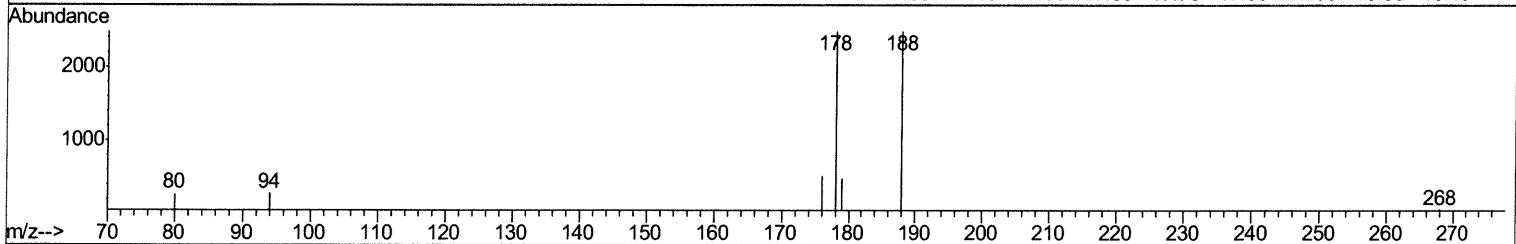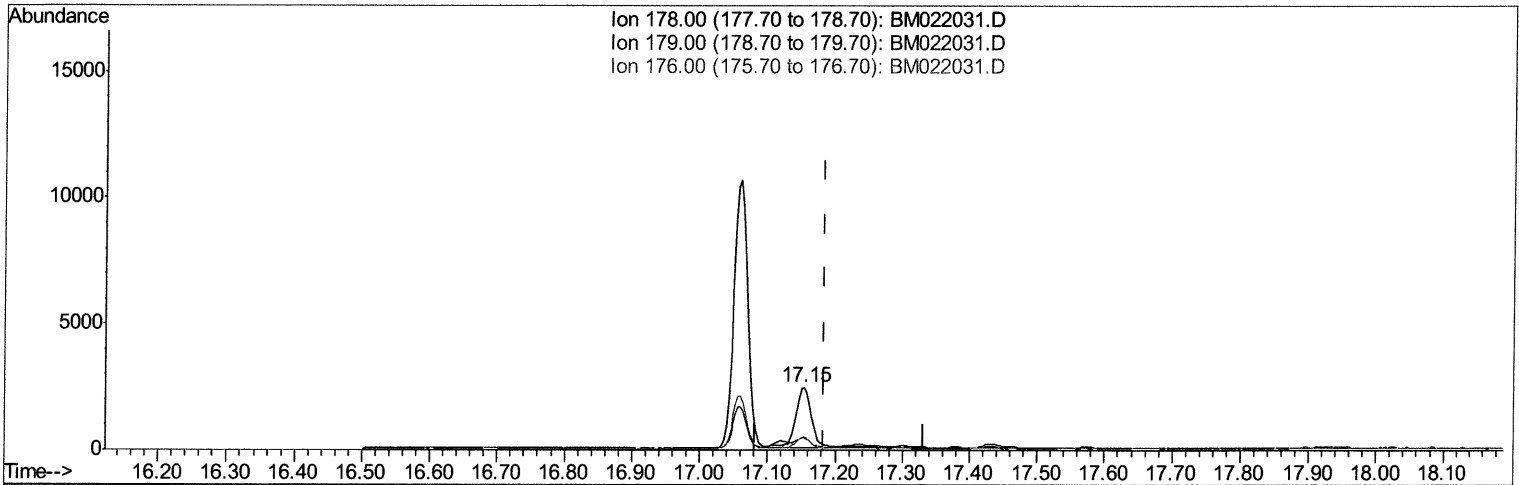

TIC: BM022031.D

(13) Anthracene

17.154min (-0.029) 0.32ng/ul m

JU
 08/13/19

response 3559

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	19.66
176.00	20.80	21.19
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP07

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:37:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

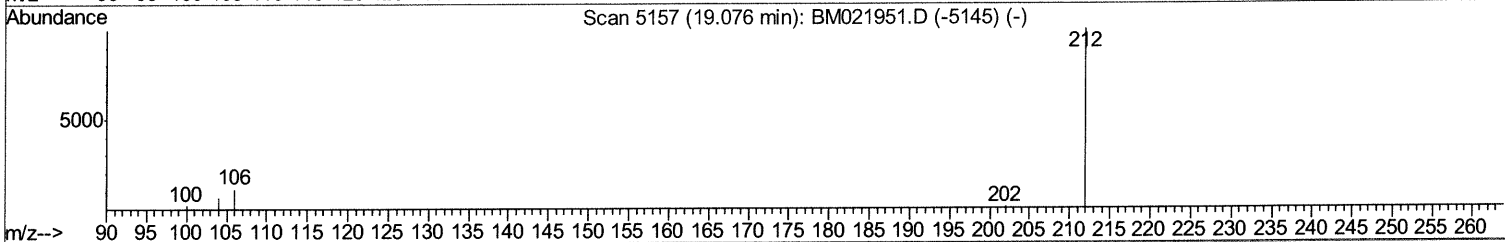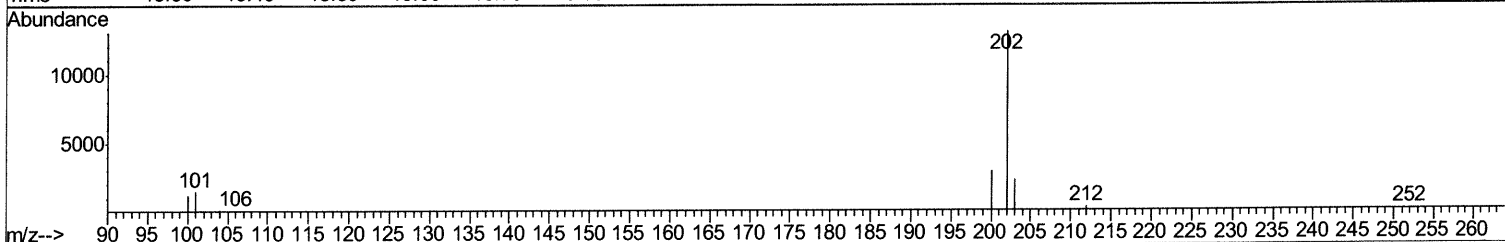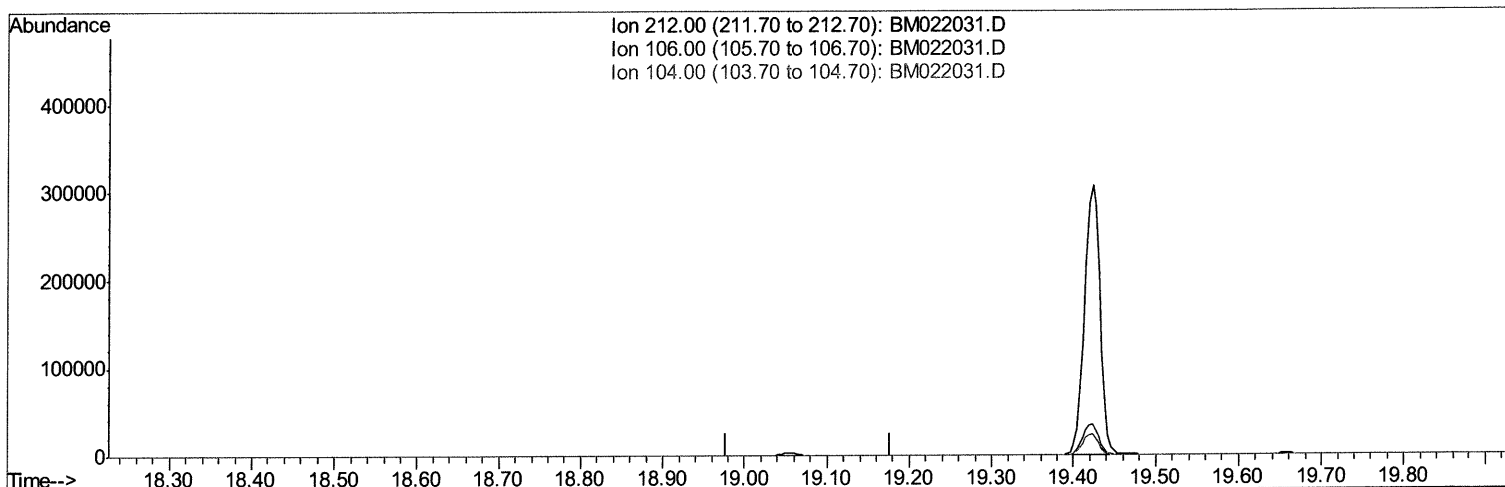

(14) Fluoranthene-d10 (SURR)

19.077min (-19.077) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BEP07

Manual Integrations
APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:37:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

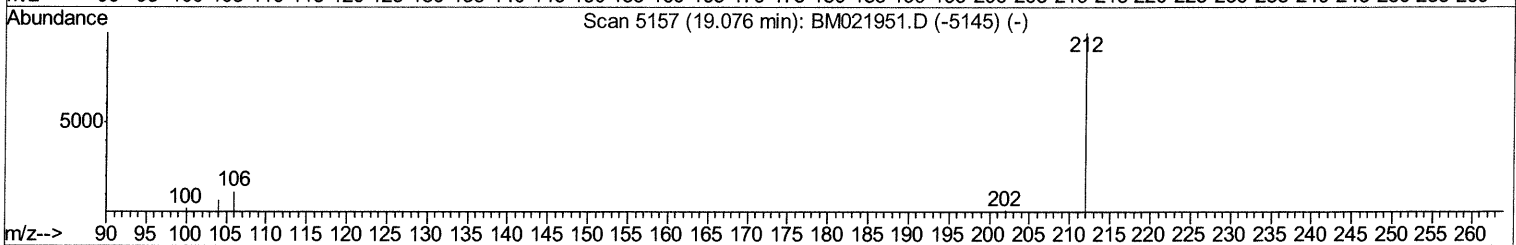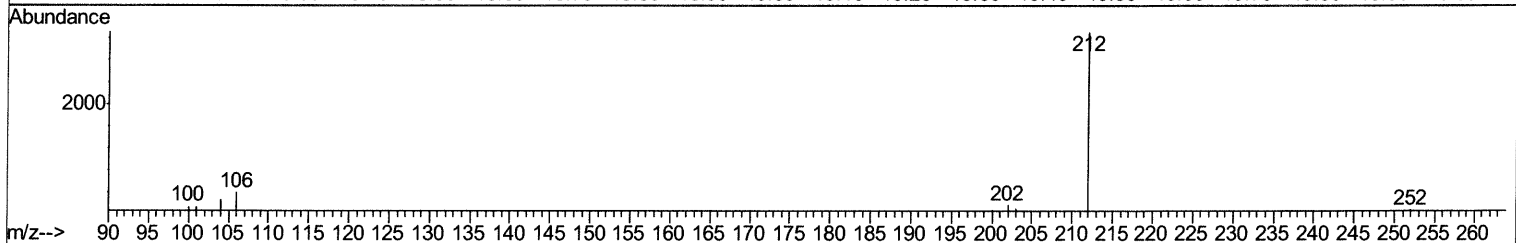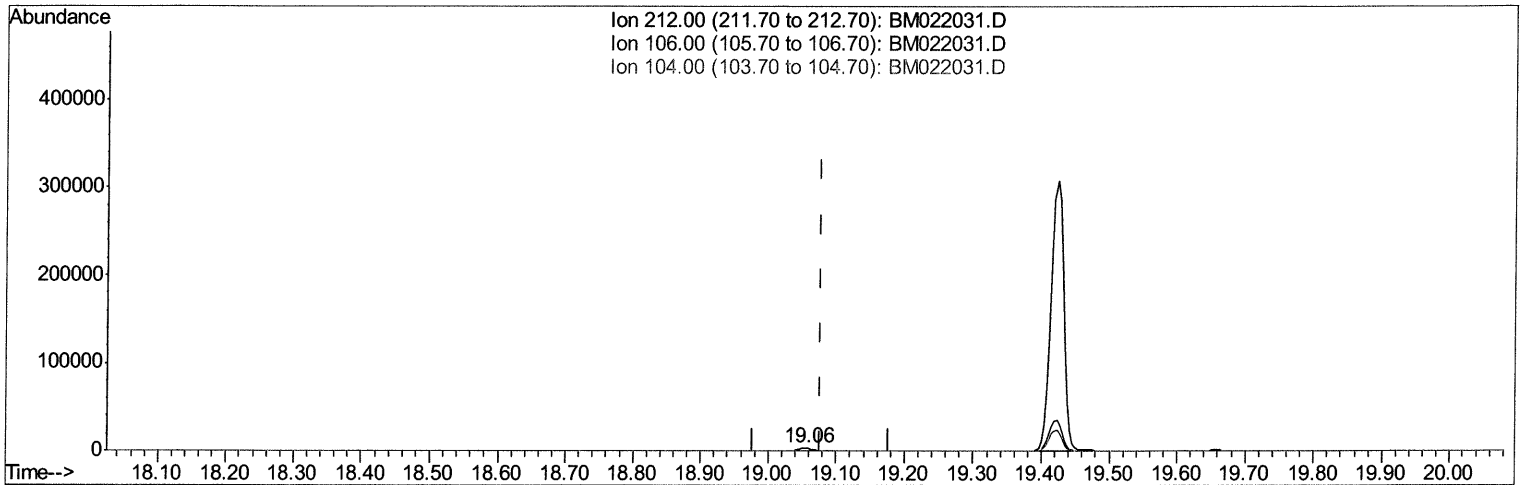

TIC: BM022031.D

(14) Fluoranthene-d10 (SURR)

19.057min (-0.021) 0.31ng/ul m

JU
08/13/19

response 4581

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
Data File : BM022031.D
Acq On : 12 Aug 2019 14:39
Operator : HP/JU
Sample : K3962-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP07

Manual Integrations
APPROVED

mohammad
8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:37:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 14:07:26 2019
Response via : Initial Calibration

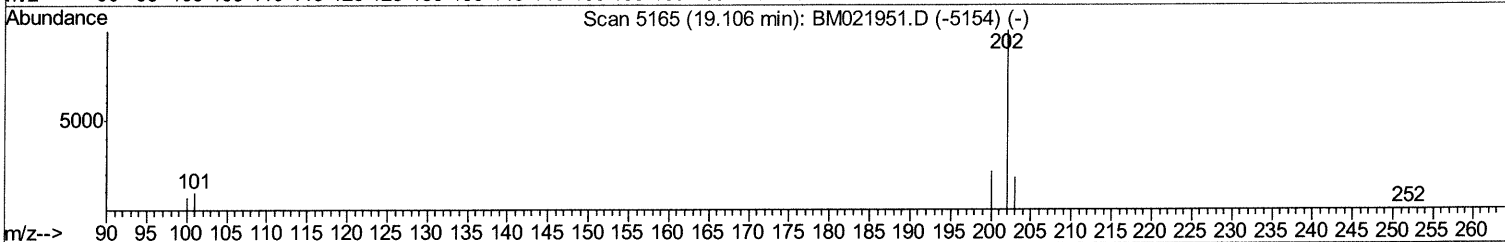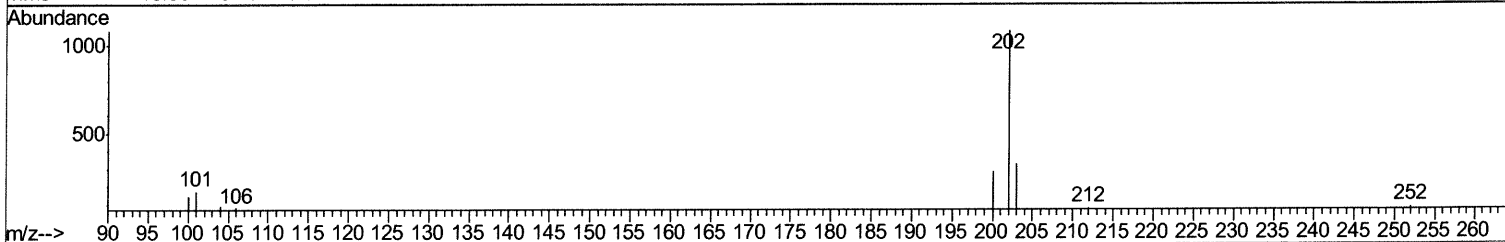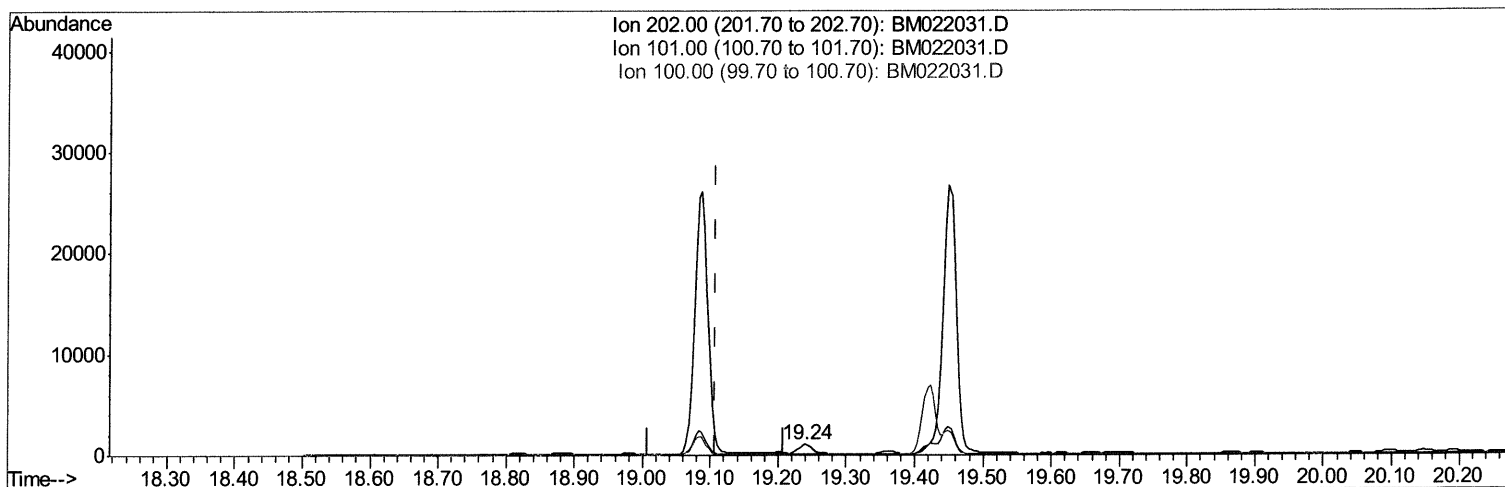

(15) Fluoranthene (C)

19.240min (+0.132) 0.07ng/ul

response 1203

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	16.39
100.00	8.10	13.52
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP07

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:37:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

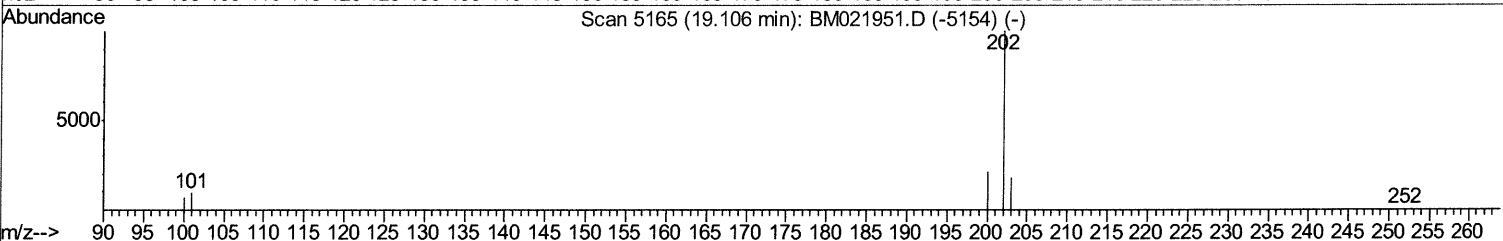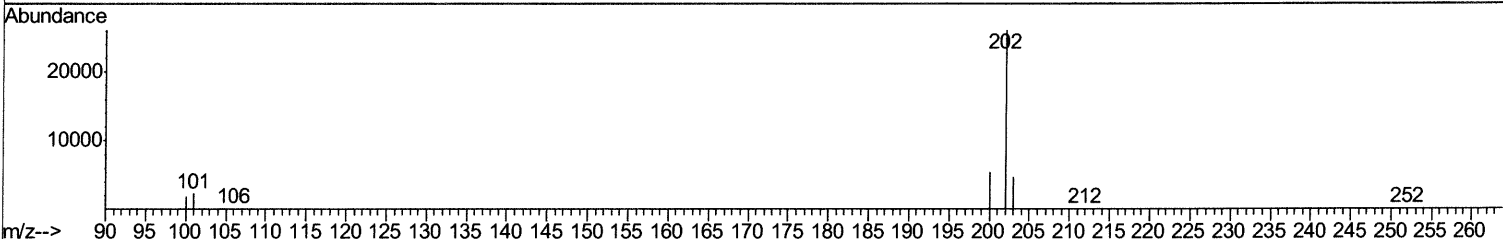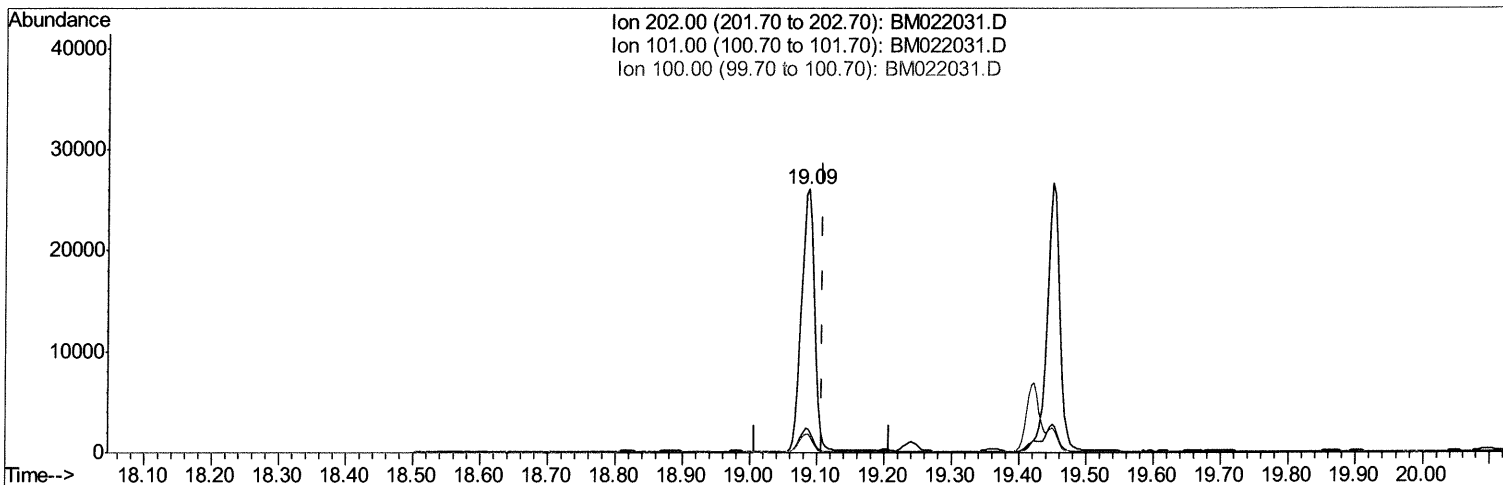

TIC: BM022031.D

(15) Fluoranthene (C)

19.087min (-0.021) 2.05ng/ul m

JU
 08/13/19

response 35493

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	8.98
100.00	8.10	6.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP07

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:37:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

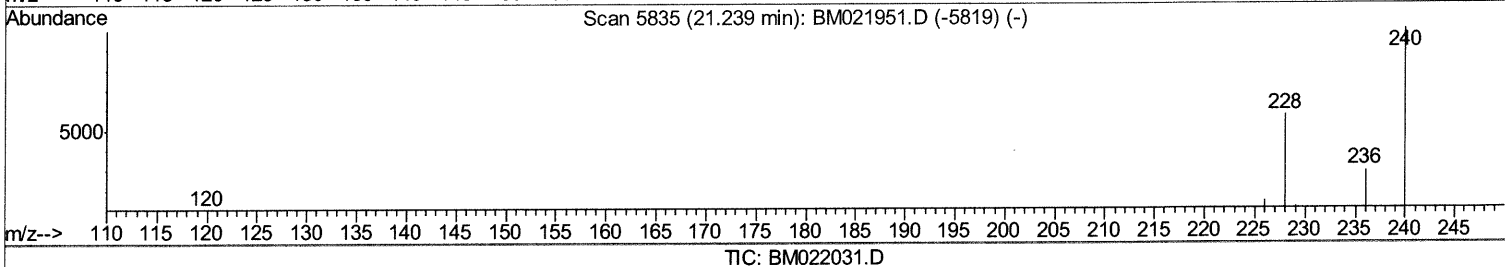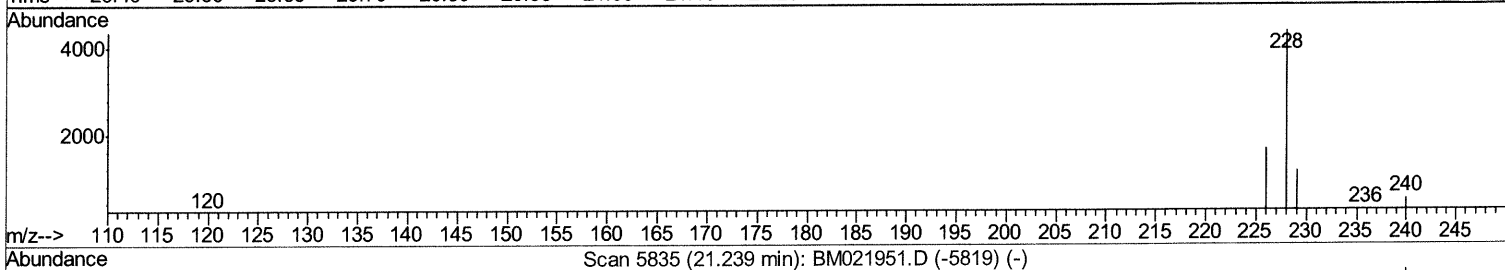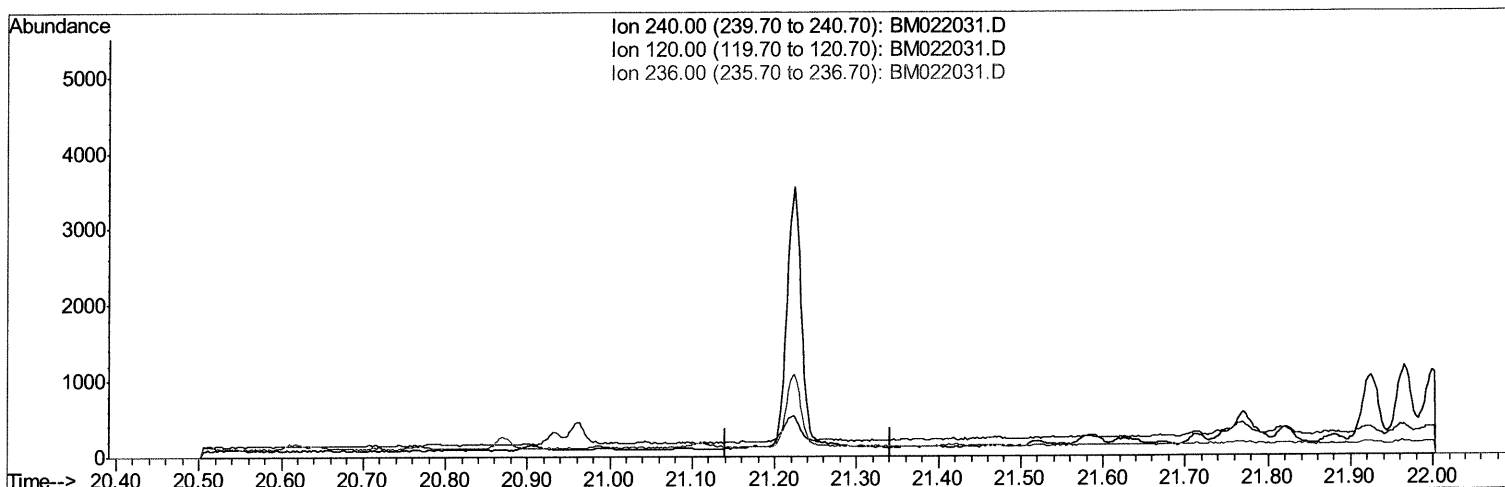

(16) Chrysene-d12 (I)

21.241min (-21.241) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.20	0.00#
236.00	32.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
Data File : BM022031.D
Acq On : 12 Aug 2019 14:39
Operator : HP/JU
Sample : K3962-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP07

Manual Integrations
APPROVED

mohammad
8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:37:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 14:07:26 2019
Response via : Initial Calibration

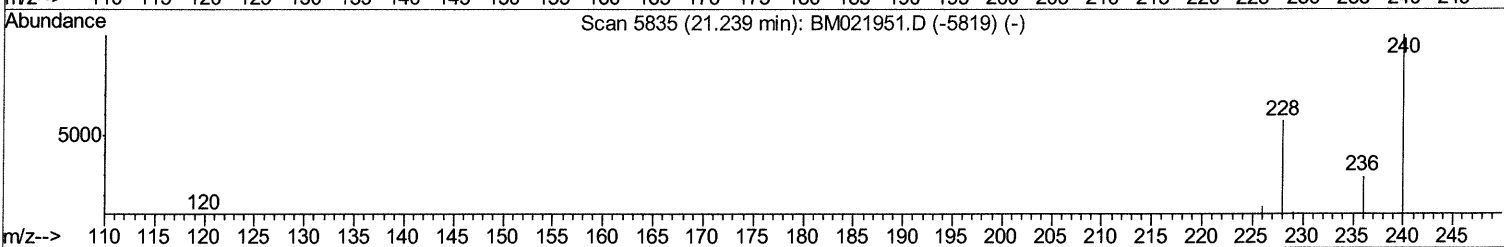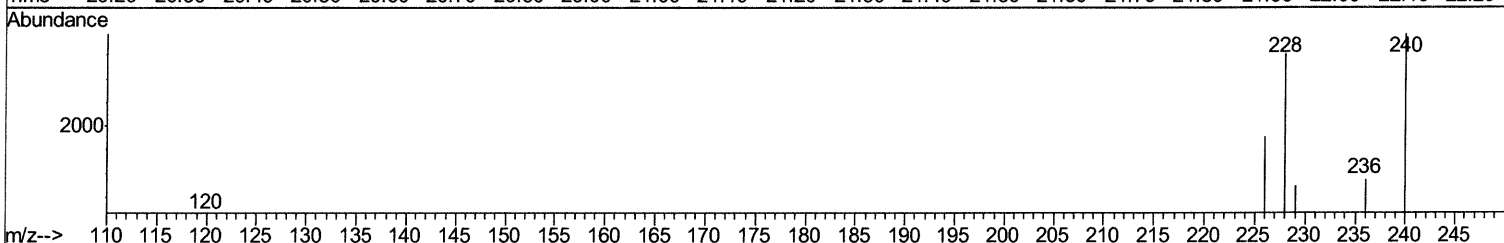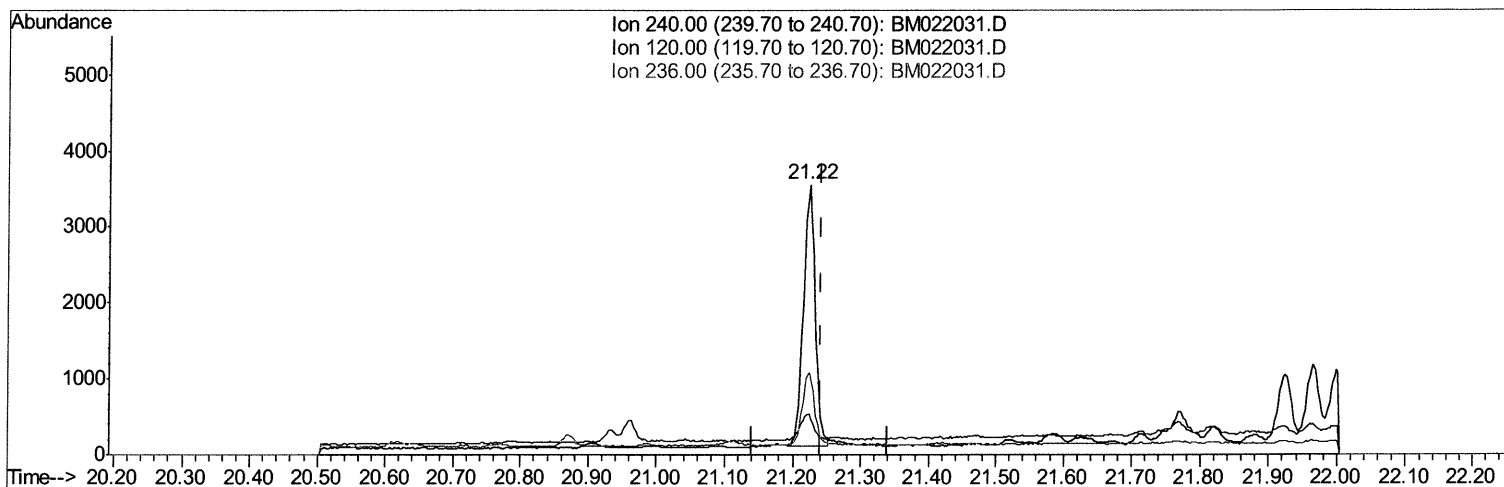

TIC: BM022031.D

(16) Chrysene-d12 (I)

21.224min (-0.017) 0.40ng/ul m

50
08/13/15

response 4197

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	14.84
236.00	32.30	30.62
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
Data File : BM022031.D
Acq On : 12 Aug 2019 14:39
Operator : HP/JU
Sample : K3962-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEP07

Manual Integrations
APPROVED

mohammad
8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:45:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 12 14:07:26 2019
Response via : Initial Calibration

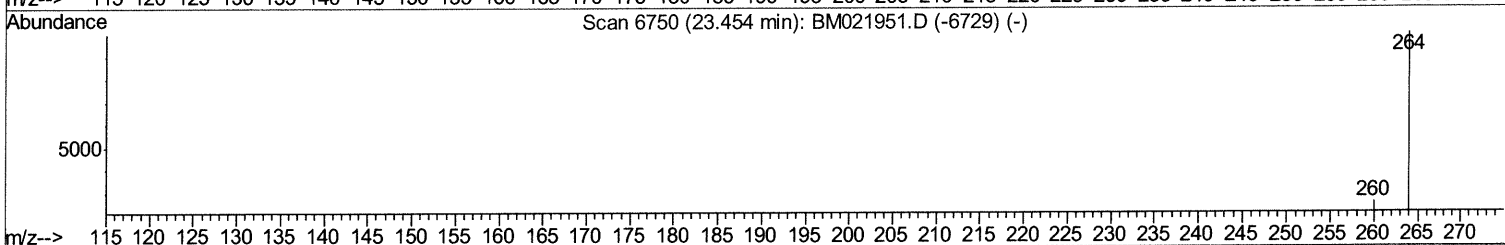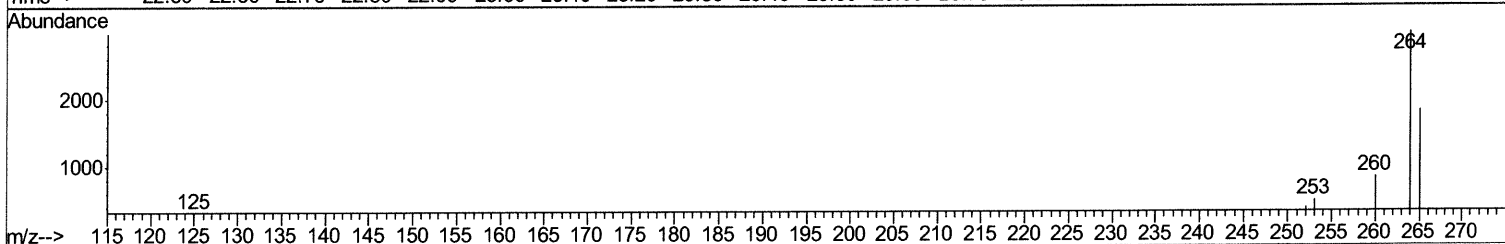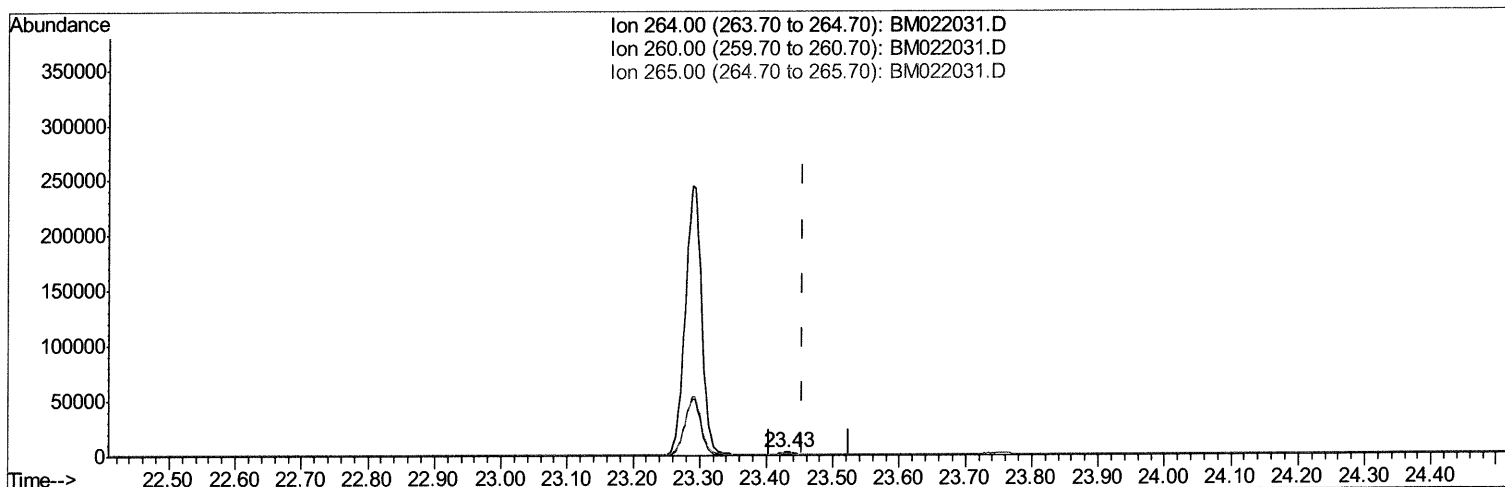

TIC: BM022031.D

(20) Perylene-d12 (I)

23.430min (-0.024) 0.40ng/ul

response 5085

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	28.03
265.00	117.00	61.28#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 BEP07

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:45:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

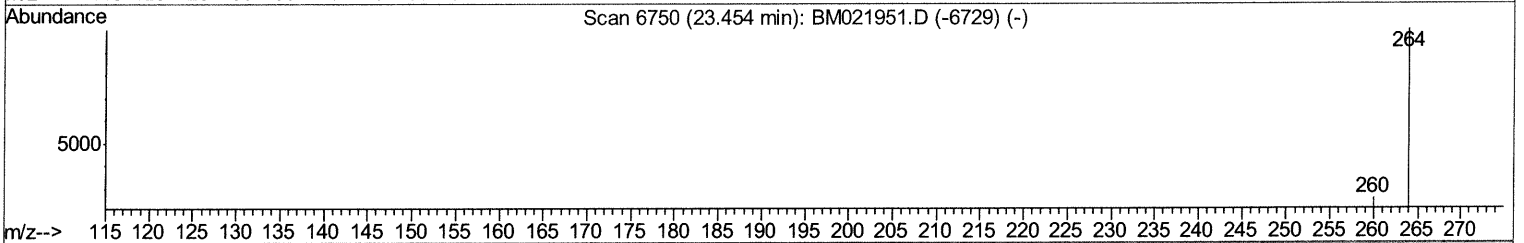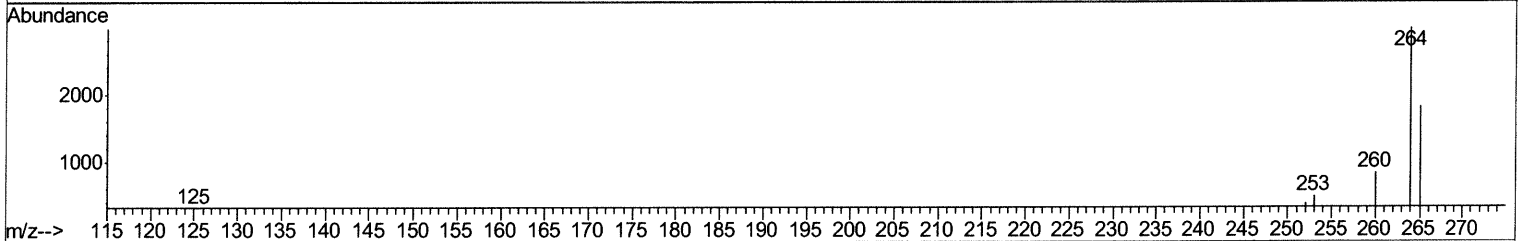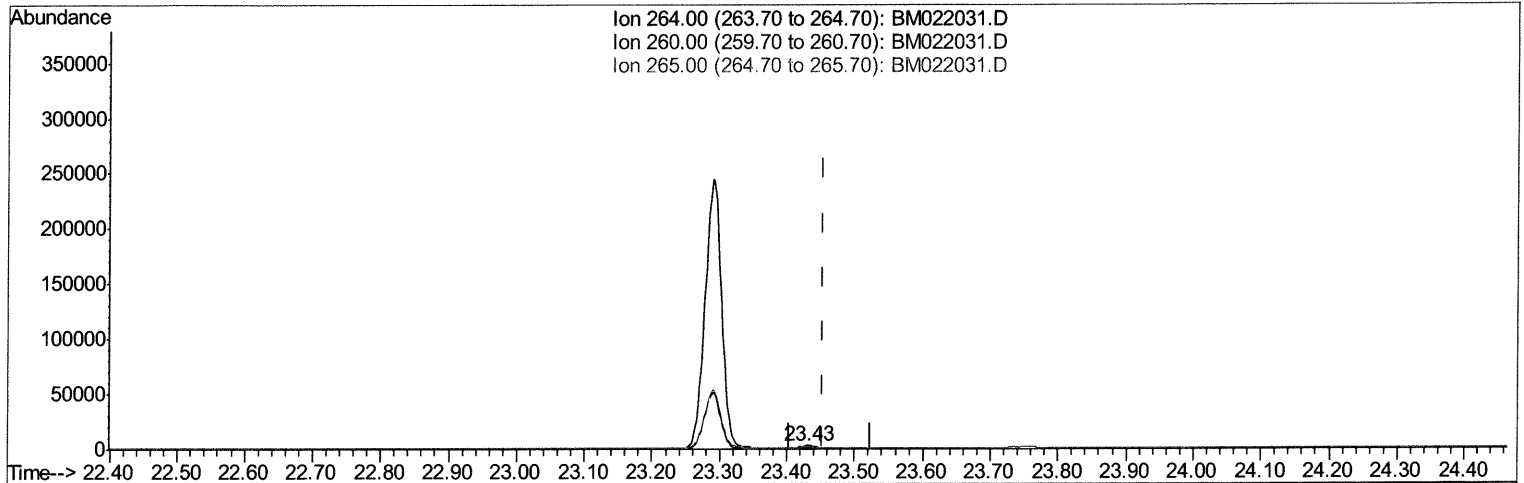

TIC: BM022031.D

(20) Perylene-d12 (I)

23.430min (-0.024) 0.40ng/ul m

JU
 08/13/15

response 3909

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	28.03
265.00	117.00	61.28#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP07

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:46:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

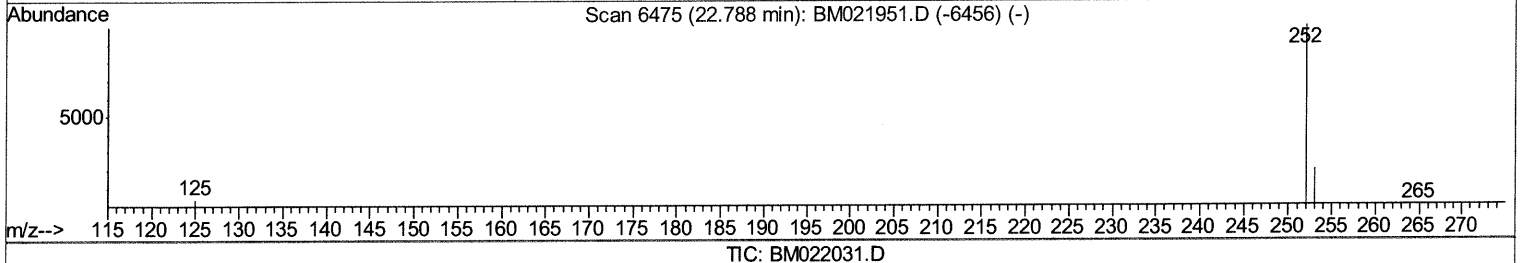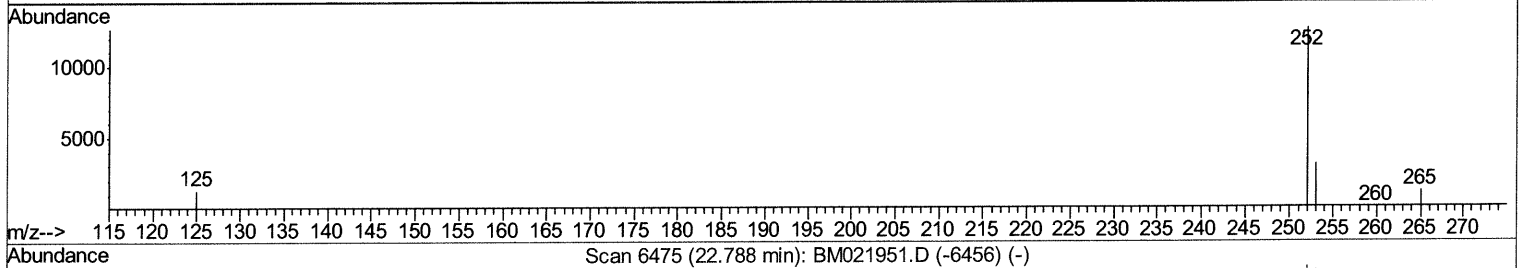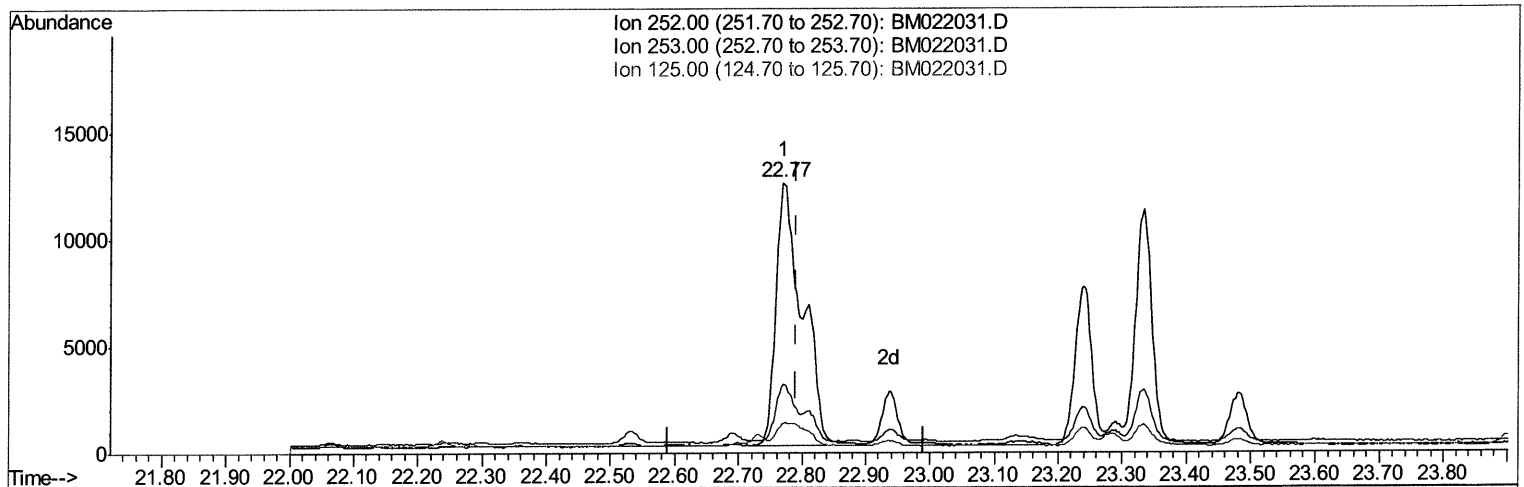

(21) Benzo(b)fluoranthene
 22.769min (-0.022) 2.71ng/ul
 response 35691

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	24.92
125.00	15.50	10.73
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP07

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:46:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

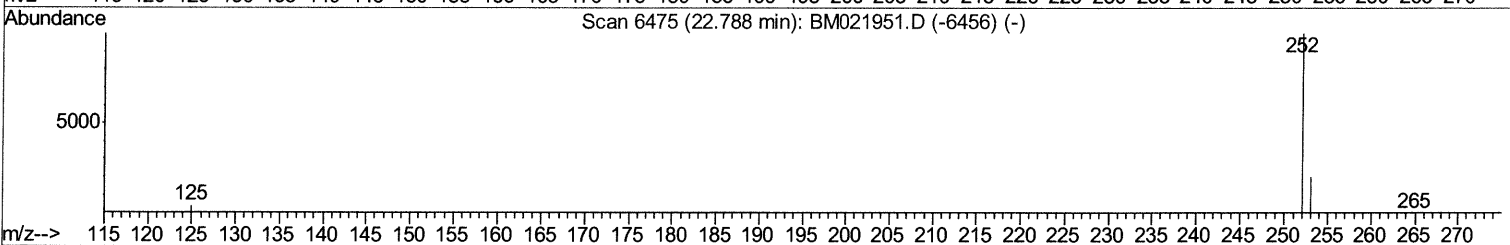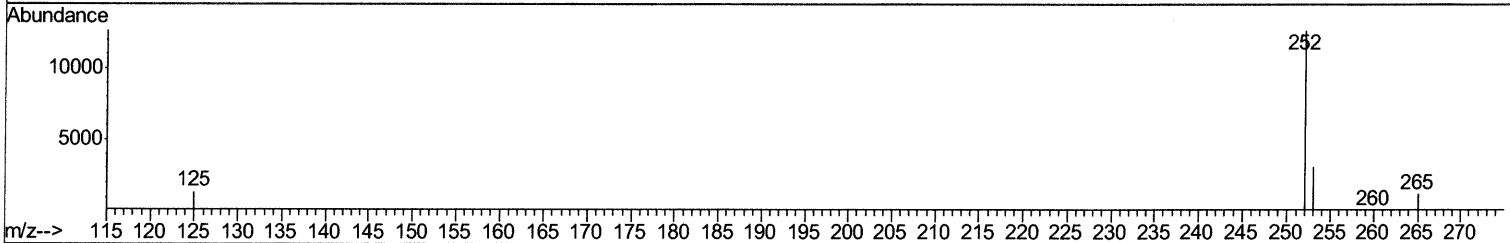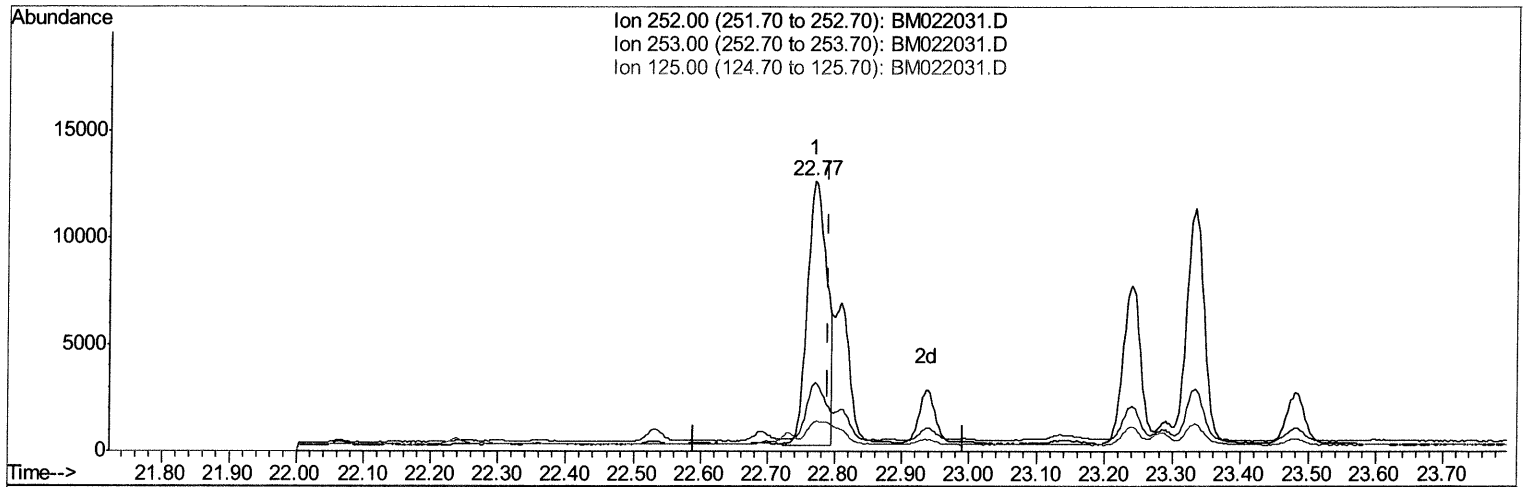

TIC: BM022031.D

(21) Benzo(b)fluoranthene

22.769min (-0.022) 1.91ng/ul m *JU 08/13/15*

response 25157

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	24.92
125.00	15.50	10.73
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP07

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:46:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

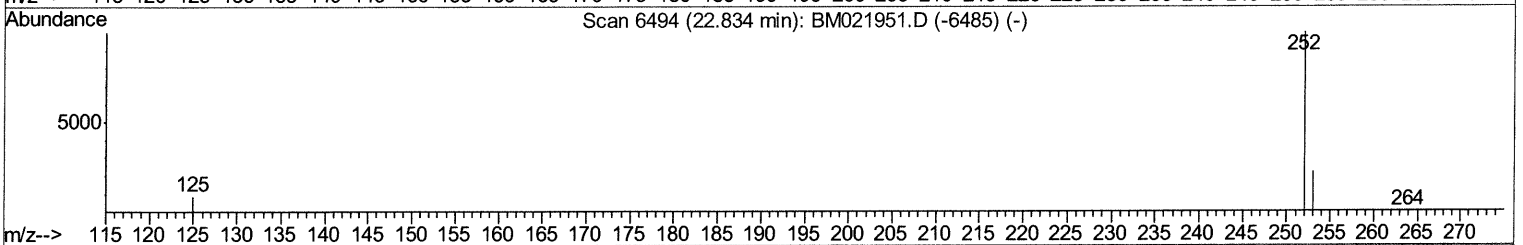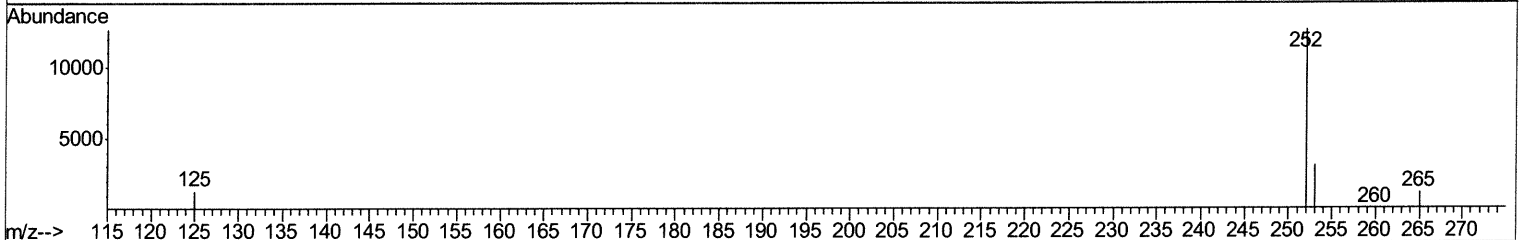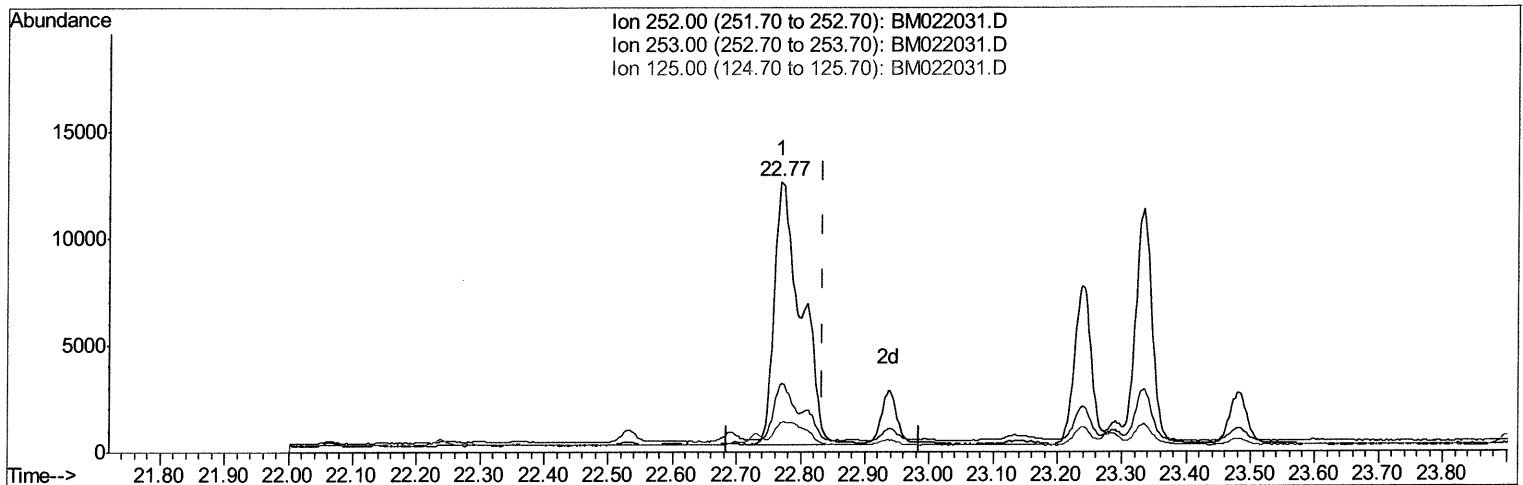

TIC: BM022031.D

(22) Benzo(k)fluoranthene
 22.769min (-0.066) 2.39ng/ui
 response 35691

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	24.92#
125.00	15.20	10.73#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BEP07

Manual Integrations
APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:46:01 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 12 14:07:26 2019
 Response via : Initial Calibration

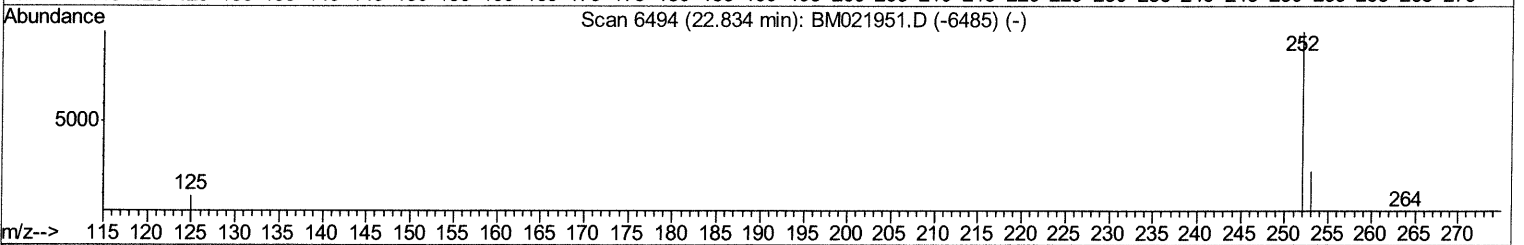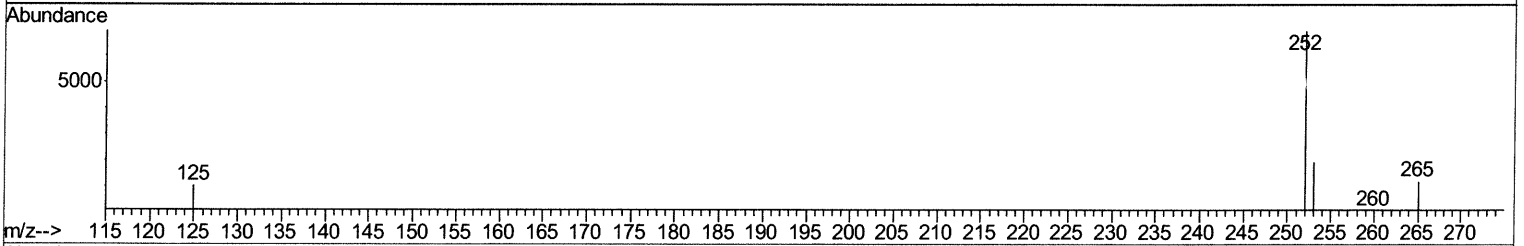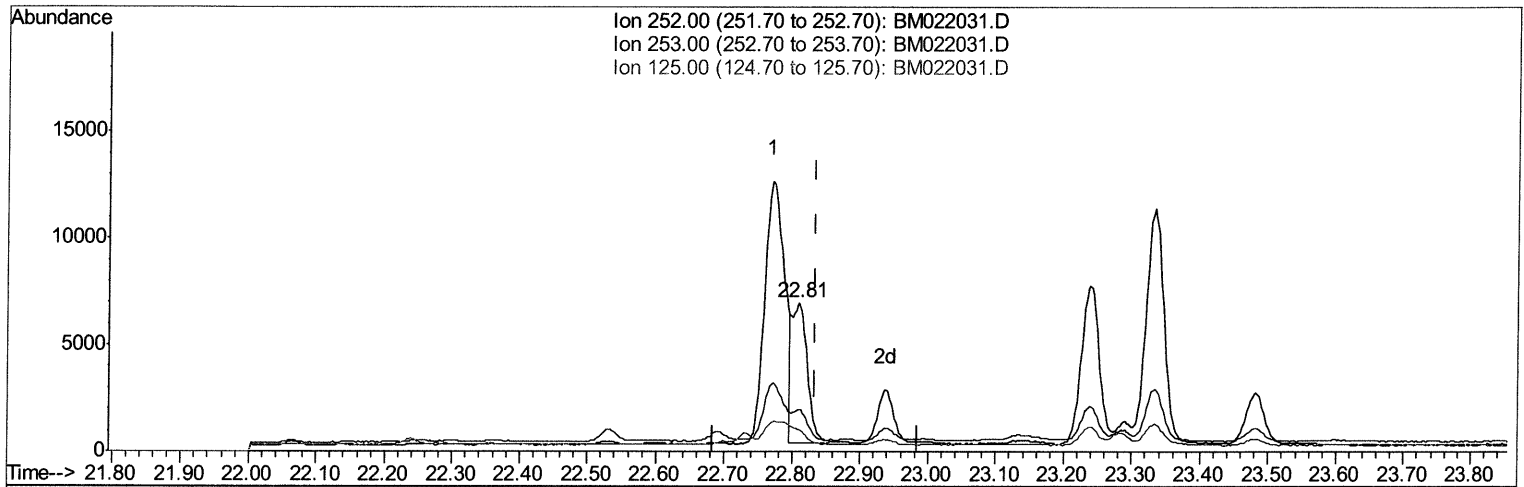

(22) Benzo(k)fluoranthene

22.810min (-0.024) 0.71ng/ul m

Handwritten: 08/12/15

response 10539

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	28.09
125.00	15.20	14.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022031.D
 Acq On : 12 Aug 2019 14:39
 Operator : HP/JU
 Sample : K3962-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEP07

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:47:28 AM

Quant Time: Aug 12 15:47:03 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Aug 12 14:07:26 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	769	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	3356	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.26	164	1869	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.02	188	4447m→	0.40	ng/ul	-0.03
16) Chrysene-d12	21.22	240	4197m→	0.40	ng/ul	-0.02
20) Perylene-d12	23.43	264	3909m→	0.40	ng/ul	-0.02

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.00	152	1510	0.27	ng/ul	-0.02
14) Fluoranthene-d10	19.06	212	4581m→	0.31	ng/ul	-0.02

Target Compounds

					Qvalue	
3) Naphthalene	10.43	128	554	0.058	ng/ul#	79
5) 2-Methylnaphthalene	12.08	142	285	0.045	ng/ul	98
7) Acenaphthylene	13.99	152	2188	0.251	ng/ul#	84
8) Acenaphthene	14.32	153	474	0.066	ng/ul	94
9) Fluorene	15.32	166	731	0.092	ng/ul#	95
12) Phenanthrene	17.06	178	15140m→	1.170	ng/ul	79
13) Anthracene	17.15	178	3559m→	0.322	ng/ul	98
15) Fluoranthene	19.09	202	35493m→	2.048	ng/ul	100
17) Pyrene	19.45	202	35721	2.071	ng/ul	99
18) Benzo(a)anthracene	21.21	228	20442	1.362	ng/ul	98
19) Chrysene	21.26	228	22224	1.151	ng/ul	80
21) Benzo(b)fluoranthene	22.77	252	25157m→	1.908	ng/ul	96
22) Benzo(k)fluoranthene	22.81	252	10539m→	0.706	ng/ul	83
23) Benzo(a)pyrene	23.33	252	19747	1.473	ng/ul#	99
24) Indeno(1,2,3-cd)pyrene	25.64	276	12785	0.799	ng/ul#	83
25) Dibenzo(a,h)anthracene	25.64	278	3441	0.266	ng/ul#	99
26) Benzo(g,h,i)perylene	26.32	276	12598	0.874	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed