

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (QT Reviewed)


Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:51:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

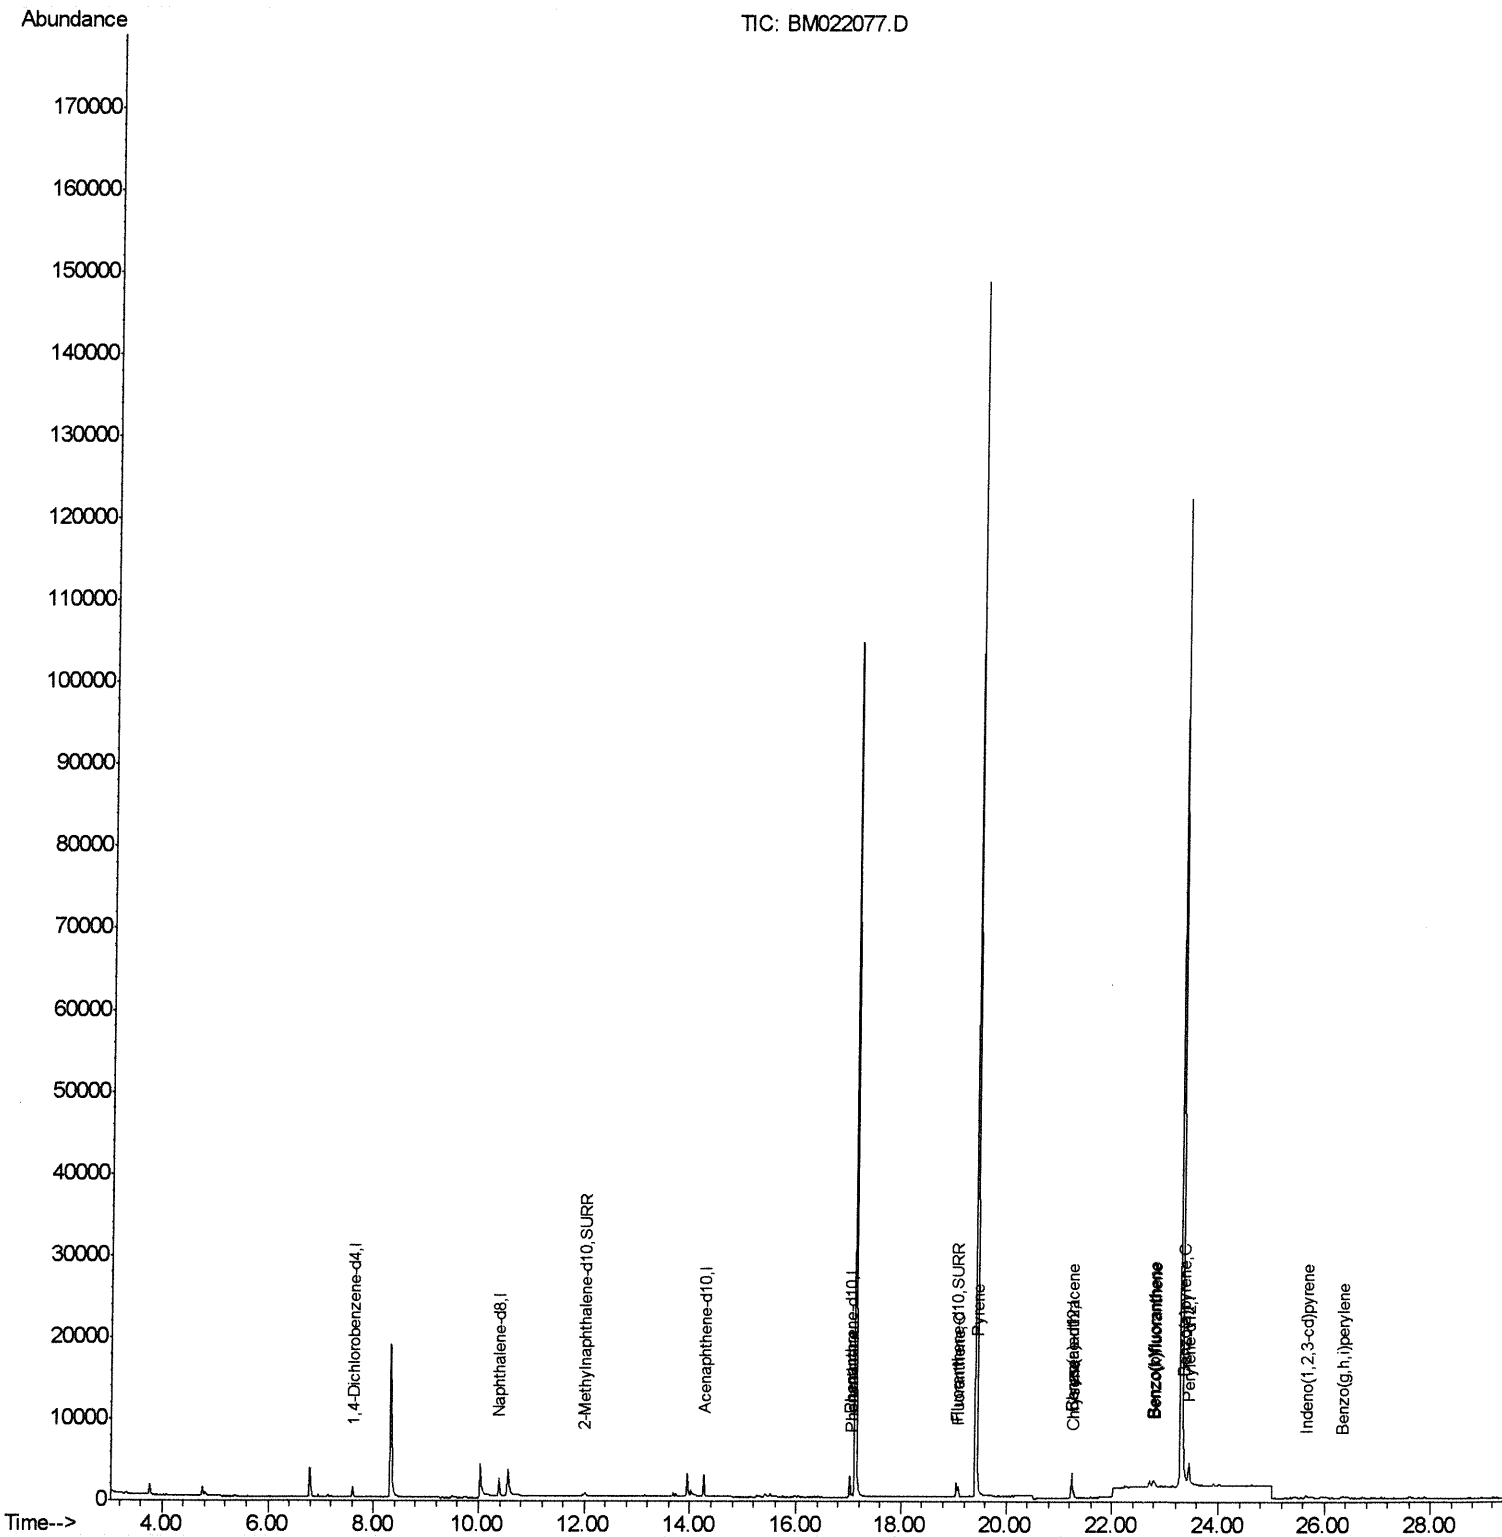

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)



Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:22:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

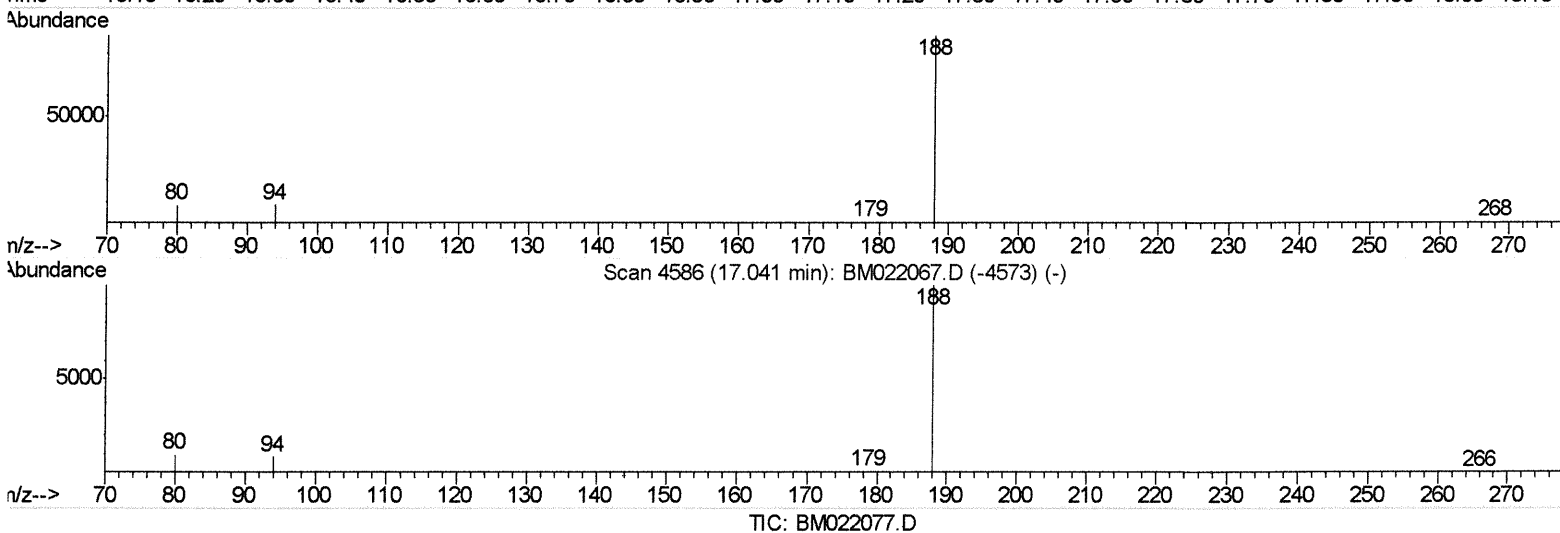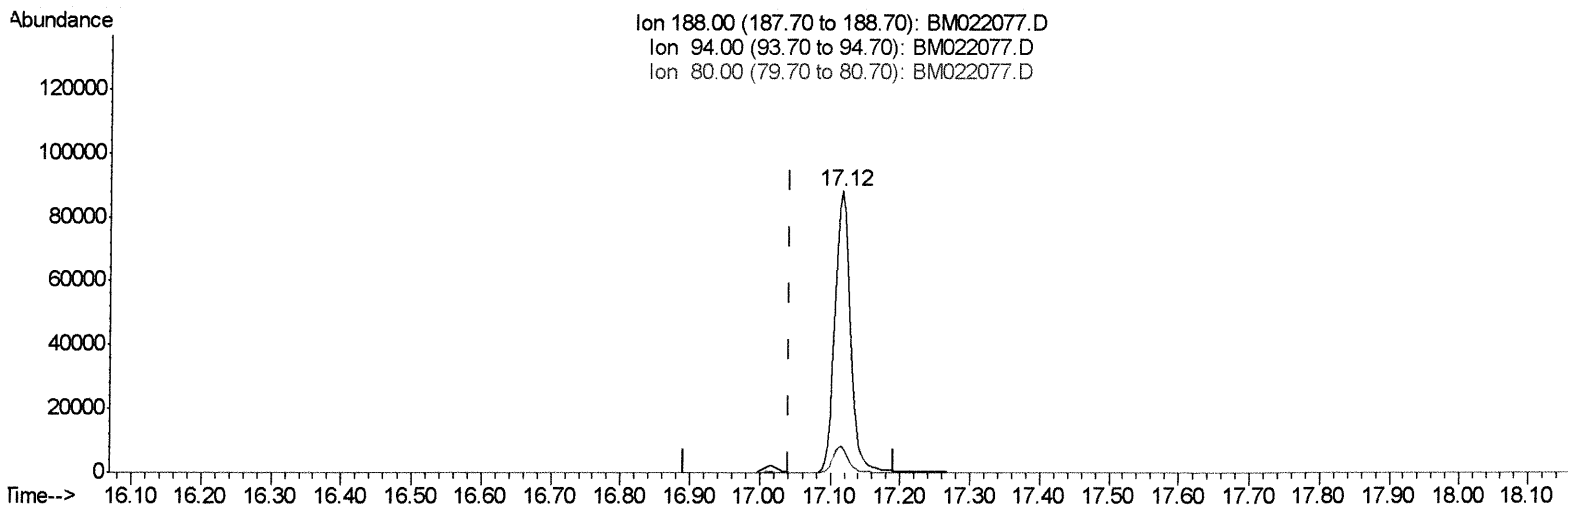

(10) Phenanthrene-d10 (I)

17.116min (+0.075) 0.40ng/ul

response 132049

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	9.47
80.00	11.40	8.96#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)




Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:22:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

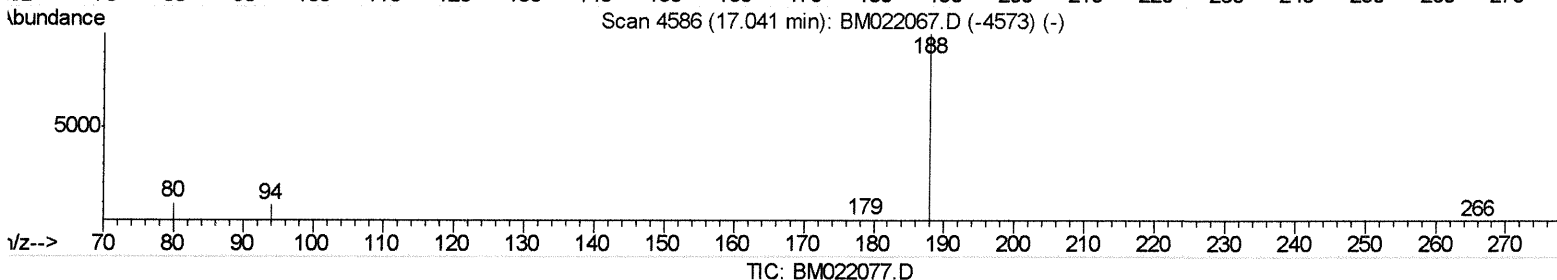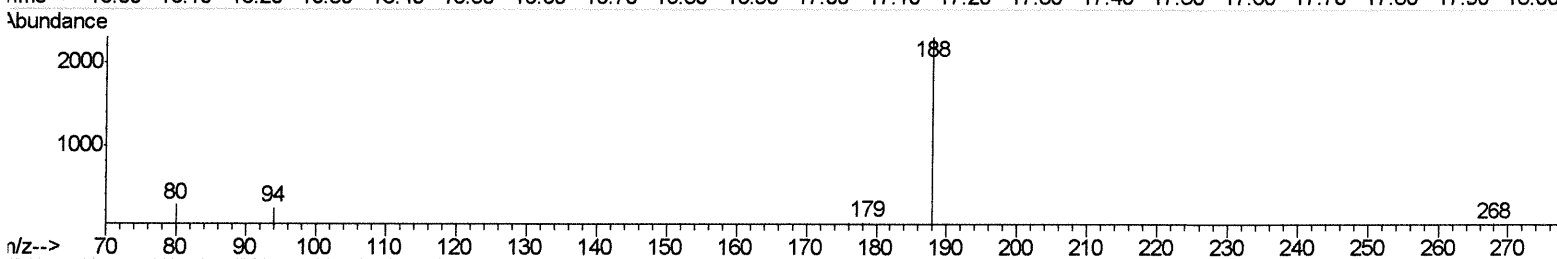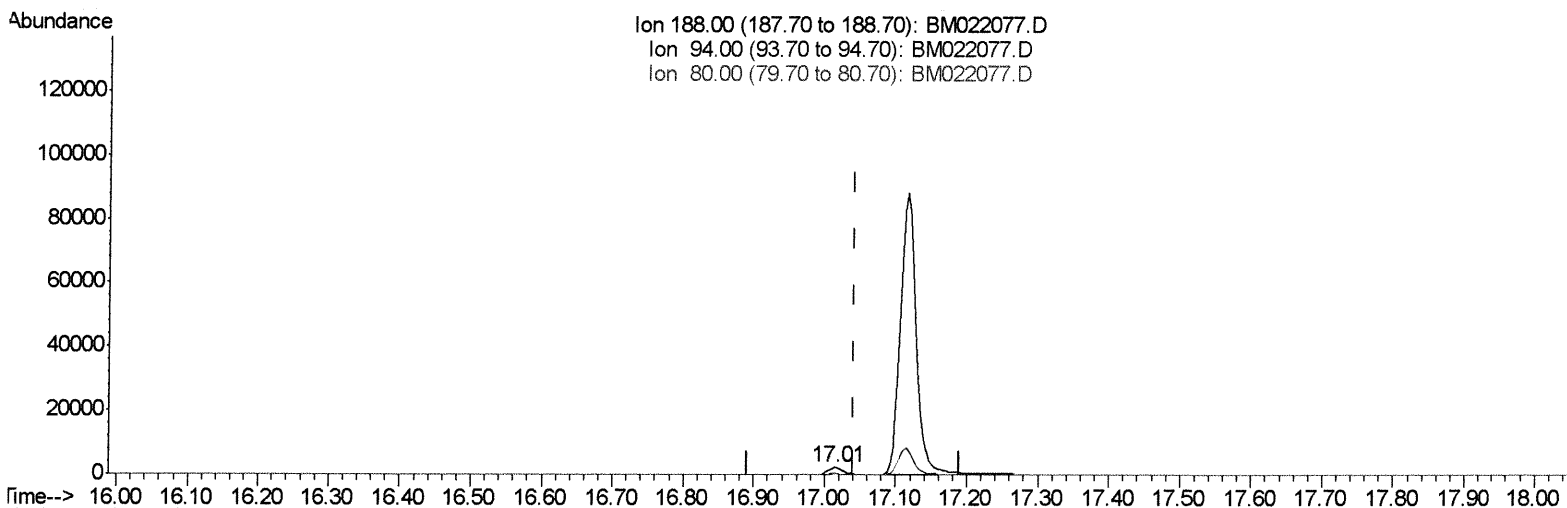

(10) Phenanthrene-d10 (I)

17.015min (-0.026) 0.40ng/ul m

JU
08/14/19

response 3398

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.18
80.00	11.40	11.87
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)



Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:48:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

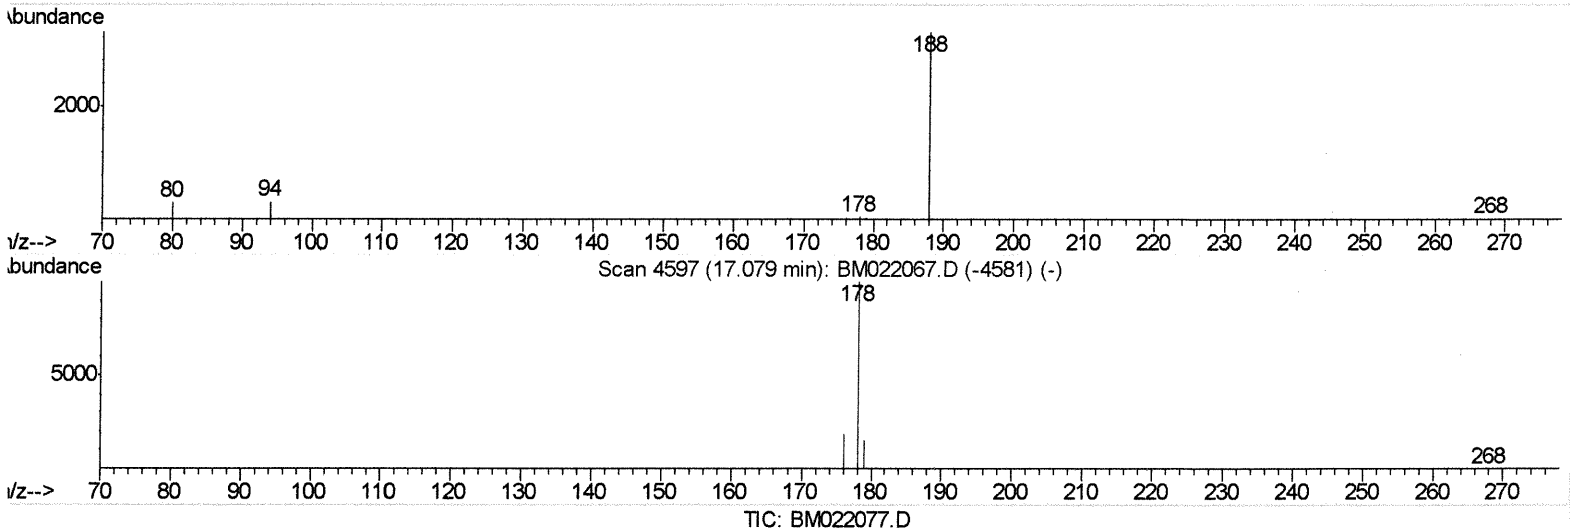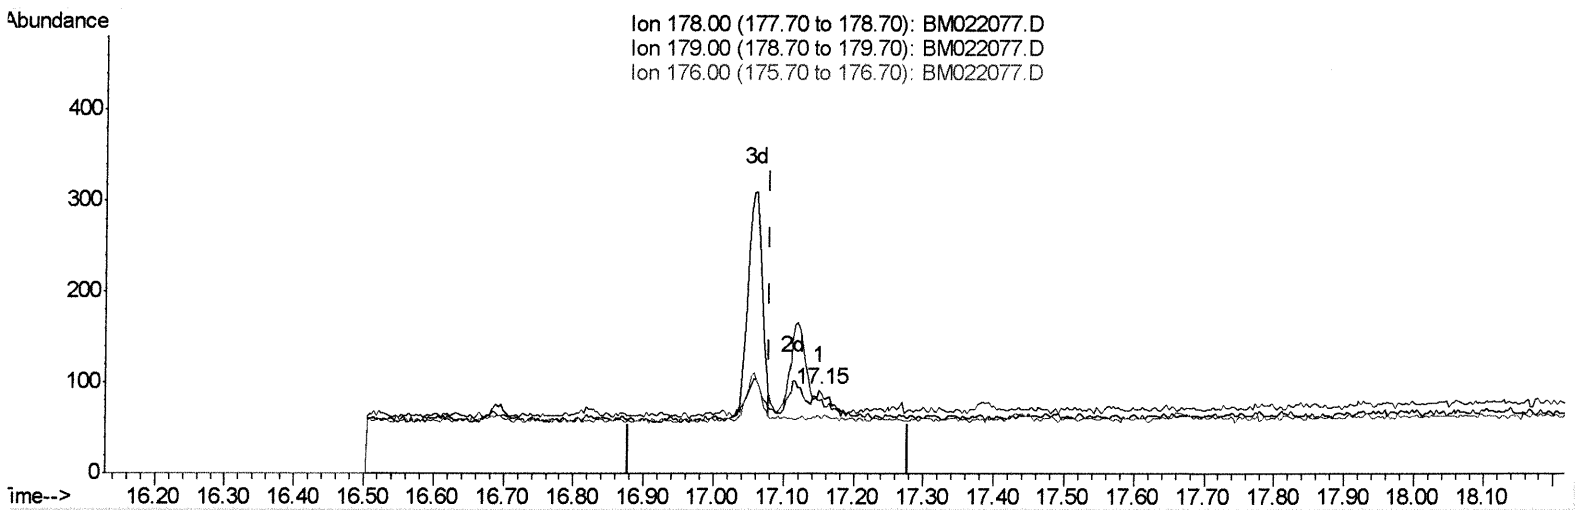

(12) Phenanthrene

17.150min (+0.071) 0.01ng/ul

response 59

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	86.96#
176.00	21.00	69.57#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)


Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:48:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

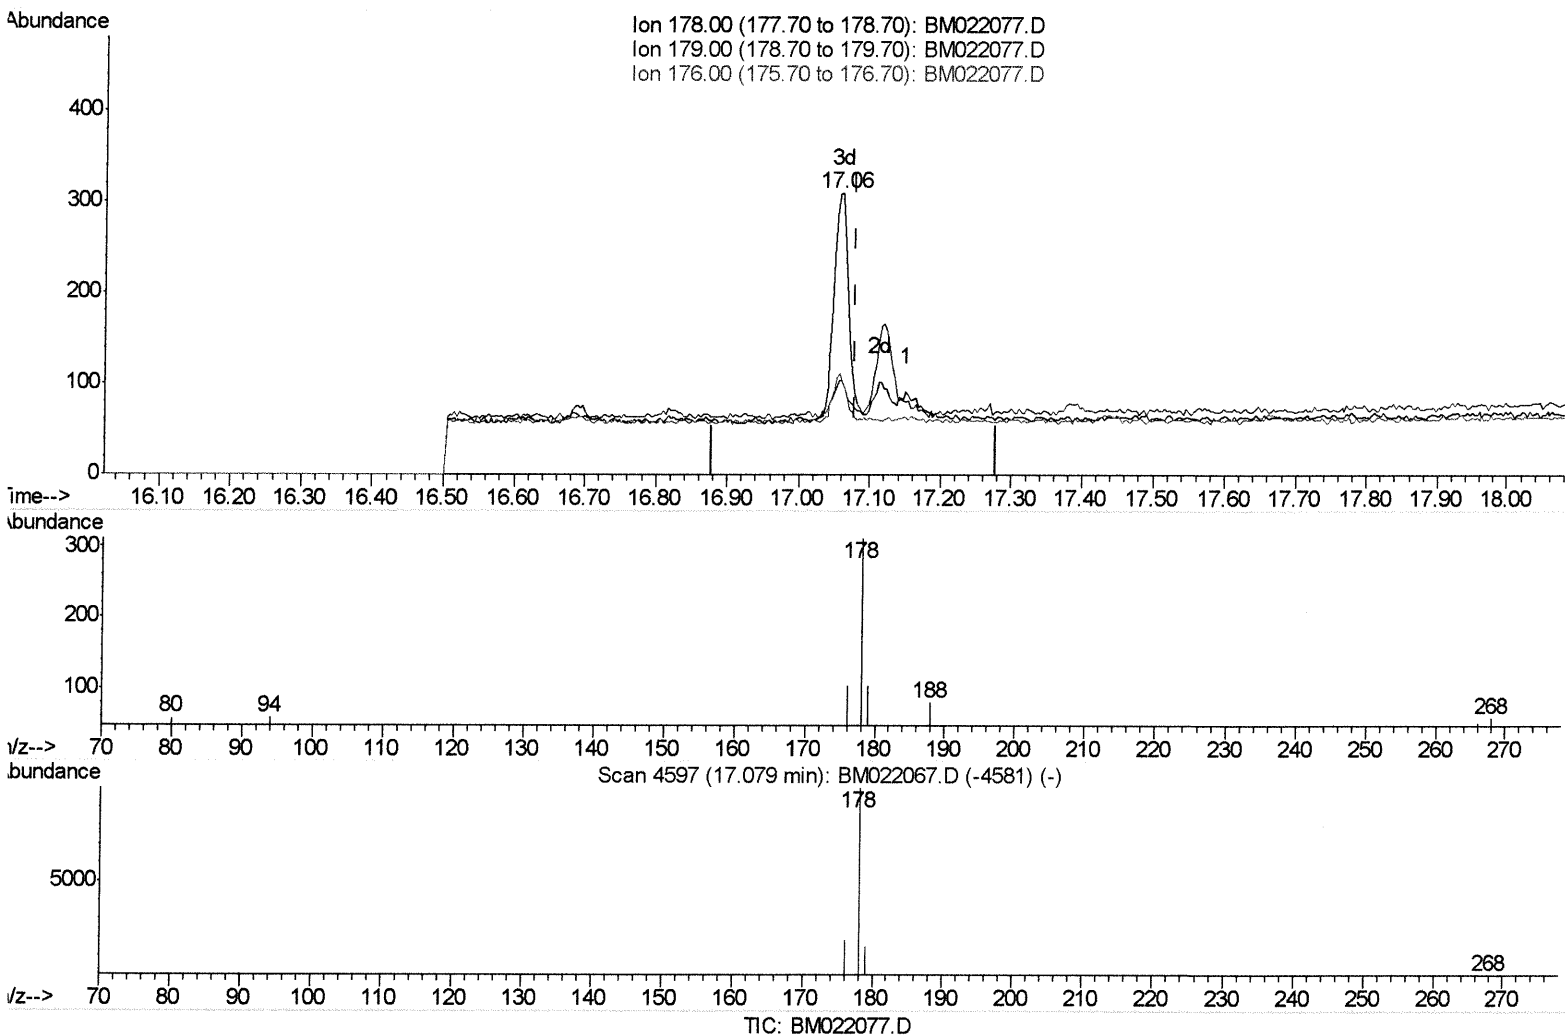

(12) Phenanthrene

17.060min (-0.019) 0.04ng/ul m

JU
08/14/19

response 355

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	33.23#
176.00	21.00	33.23#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)



Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:48:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

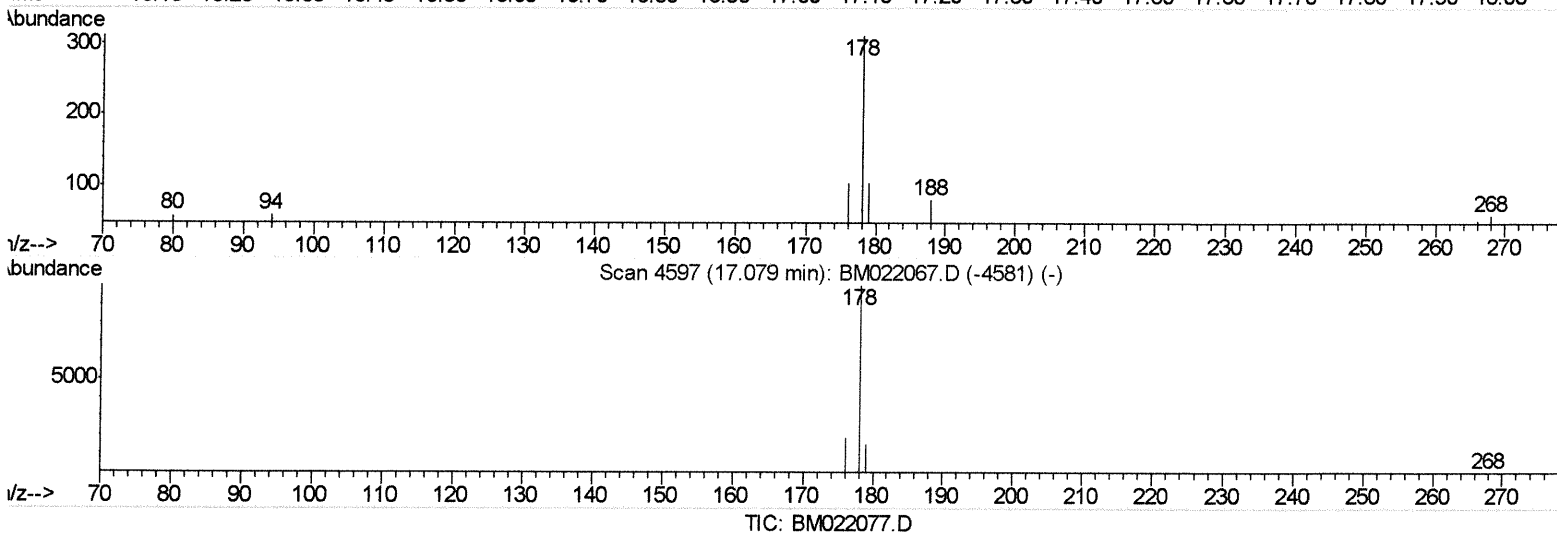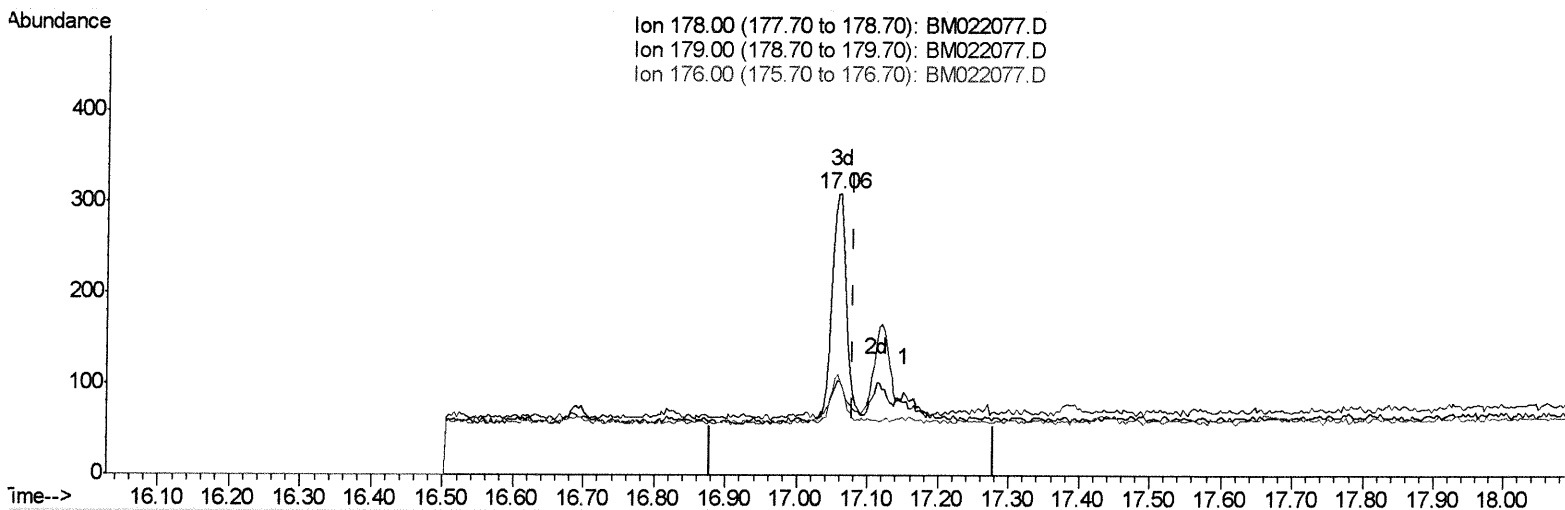

(12) Phenanthrene

17.060min (-0.019) 0.04ng/ul m *JU 08/14/19*



response 356

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	33.23#
176.00	21.00	33.23#
0.00	0.00	0.00

Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:48:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

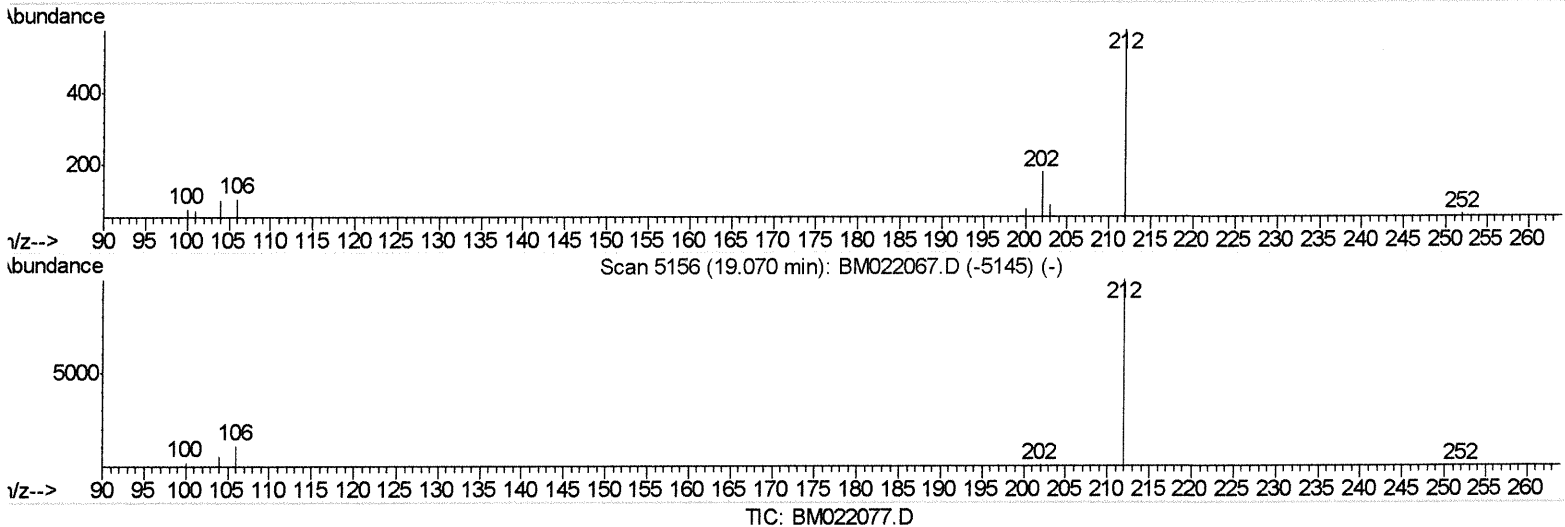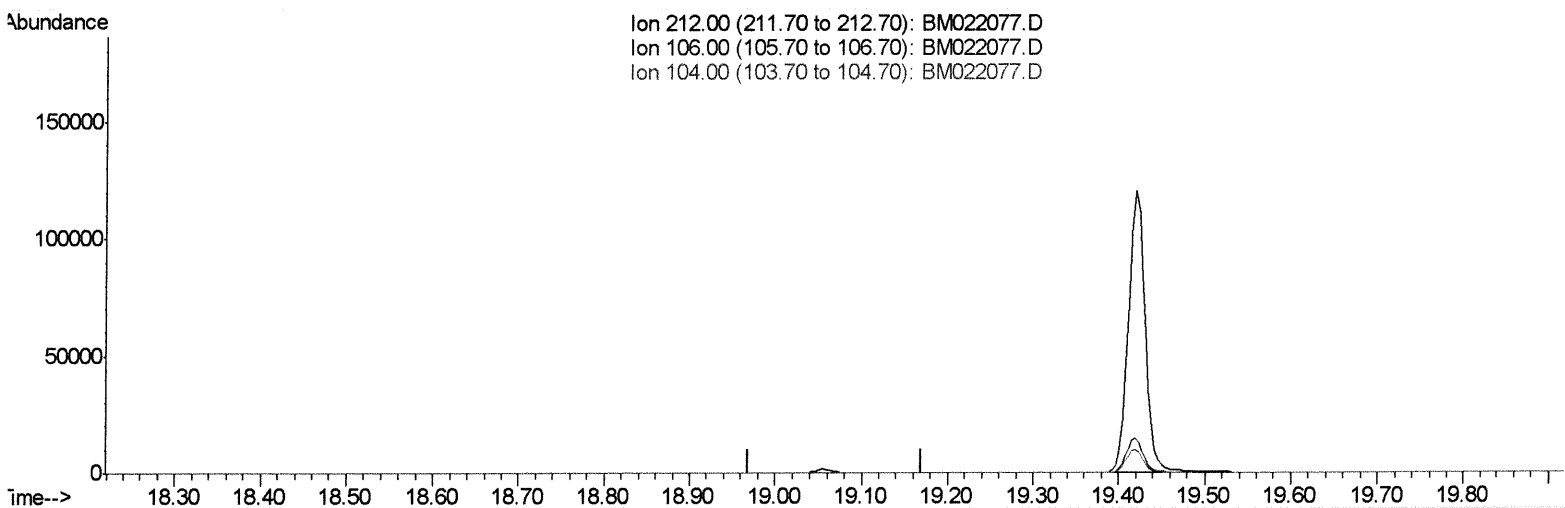

Ion	Exp%	Act%
212.00	100	0.00
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)



Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:48:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

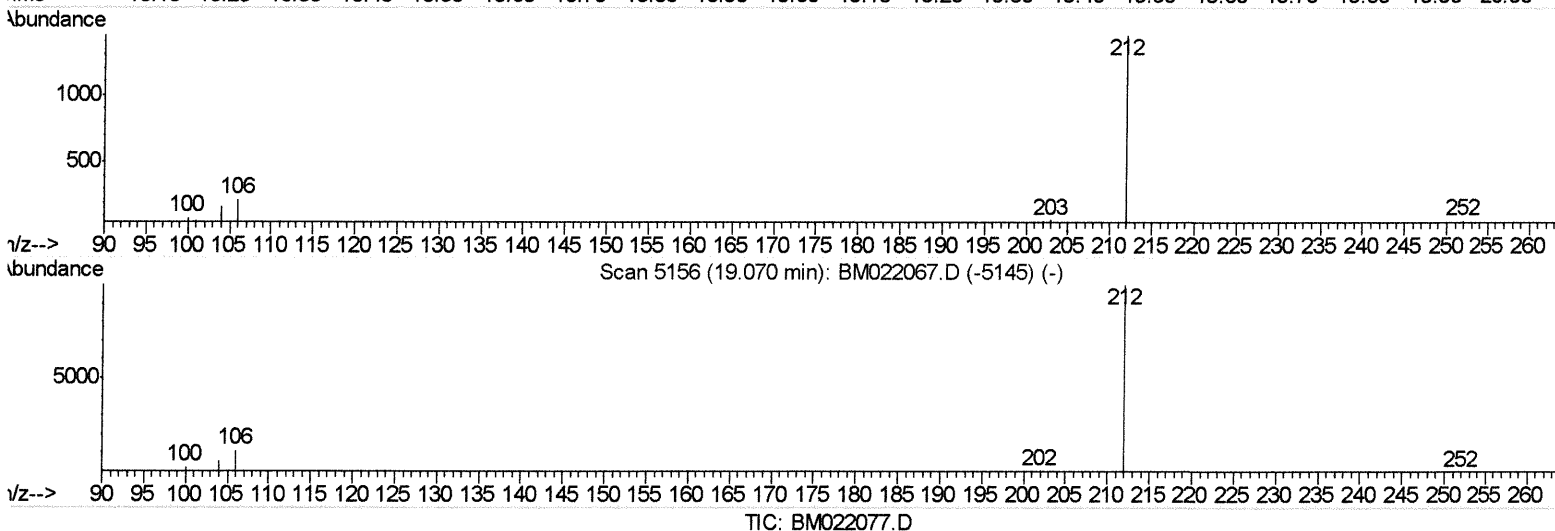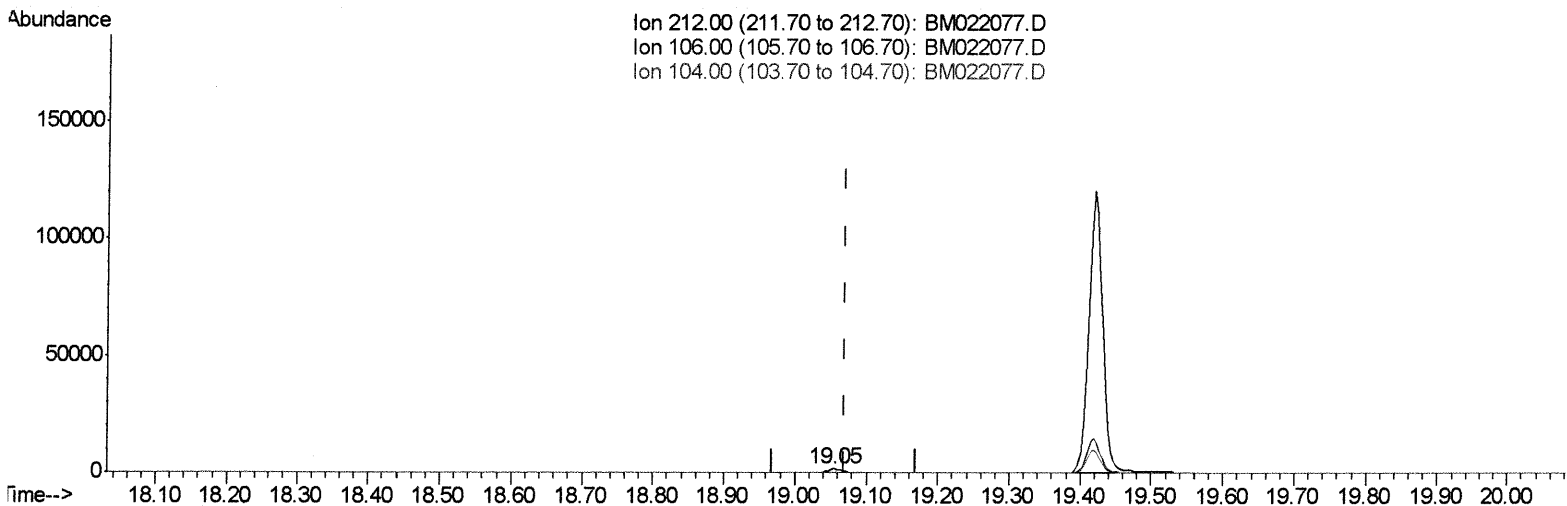

(14) Fluoranthene-d10 (SURR)

19.053min (-0.017) 0.18ng/ul m

JU
08/14/19

response 2118

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)




Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:48:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

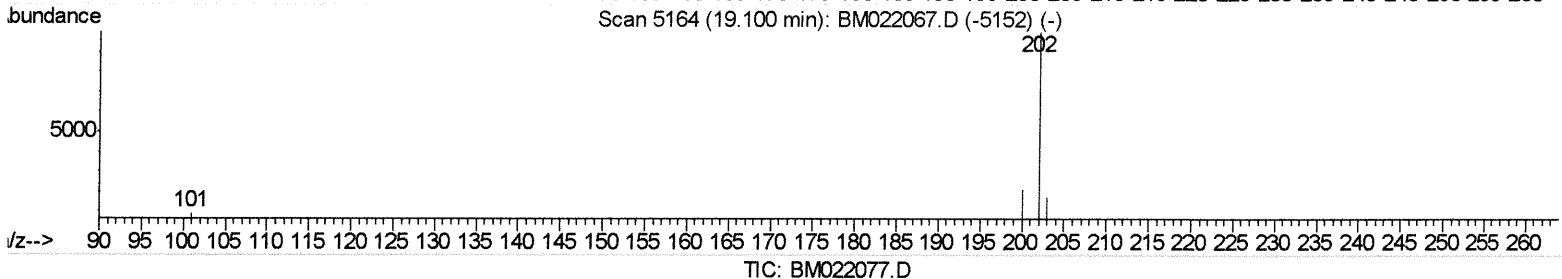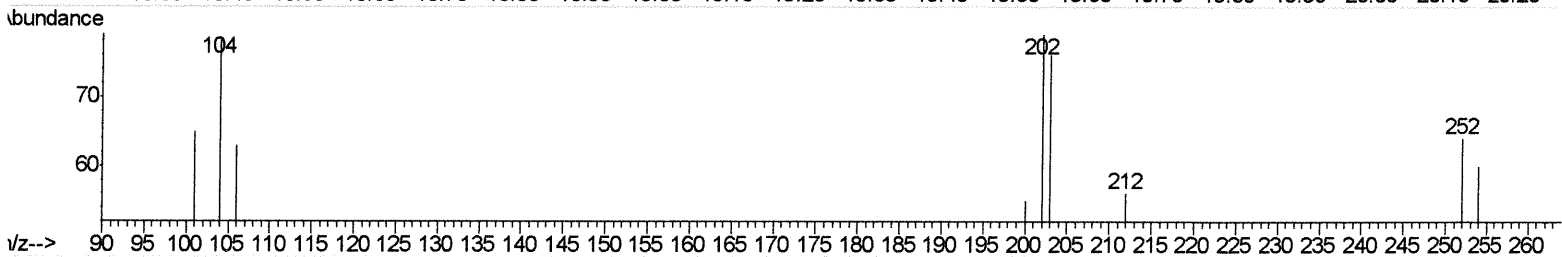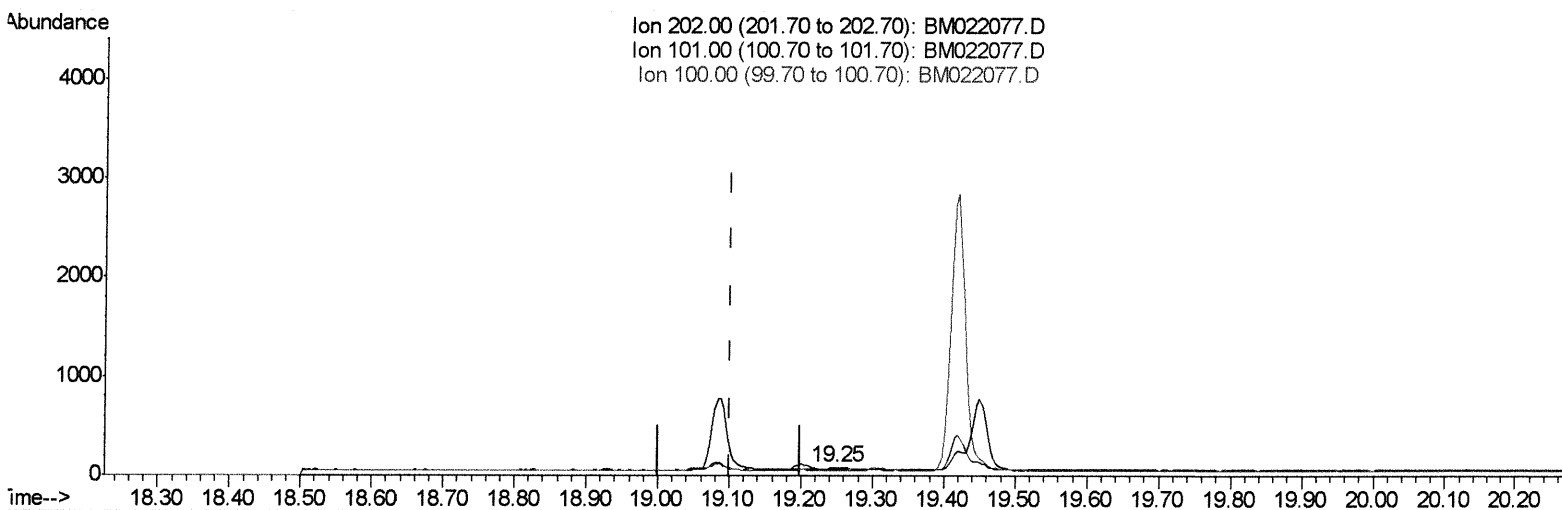

(15) Fluoranthene (C)

19.247min (+0.147) 0.00ng/ul

response 32

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	82.28#
100.00	8.10	65.82#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)



Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:48:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

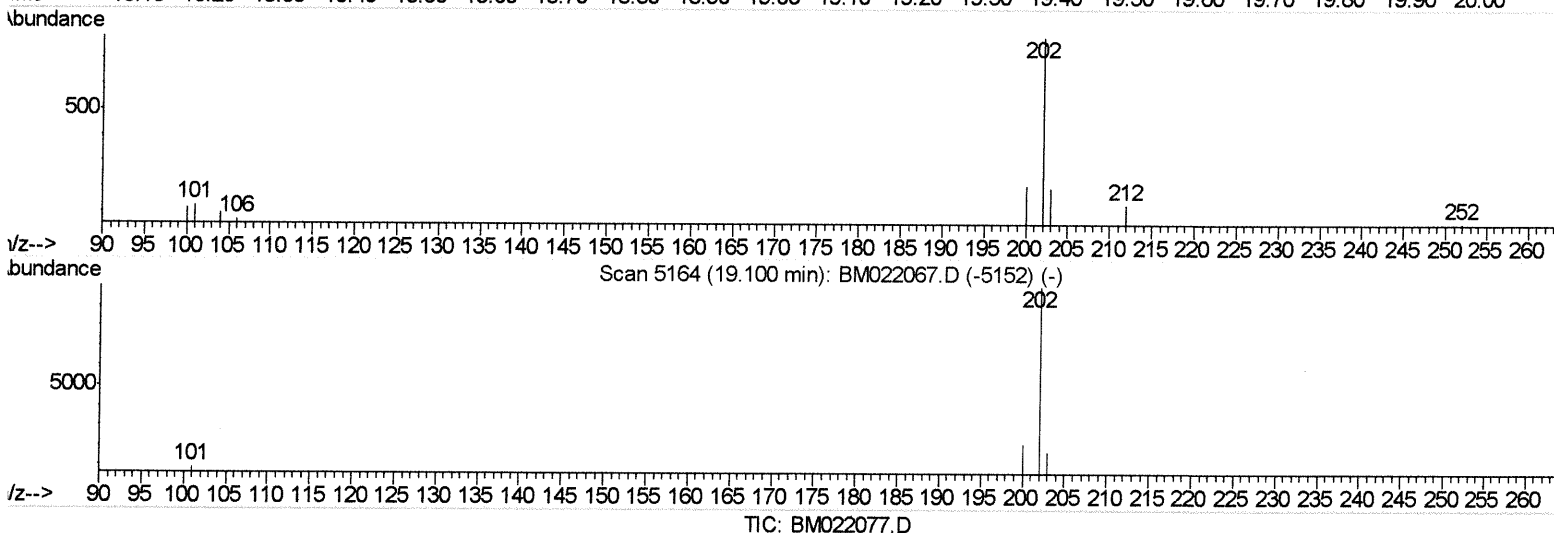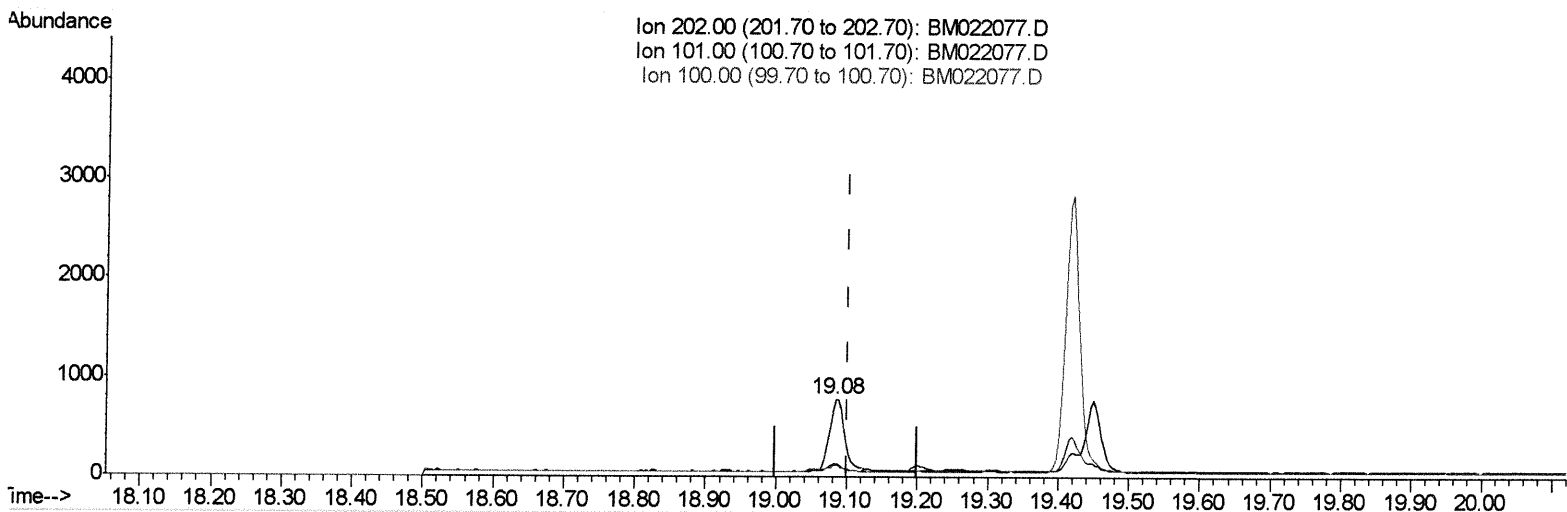

(15) Fluoranthene (C)

19.083min (-0.017) 0.08ng/ul m

JU
08/14/19

response 1083

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	16.35
100.00	8.10	14.94
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)


Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:48:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

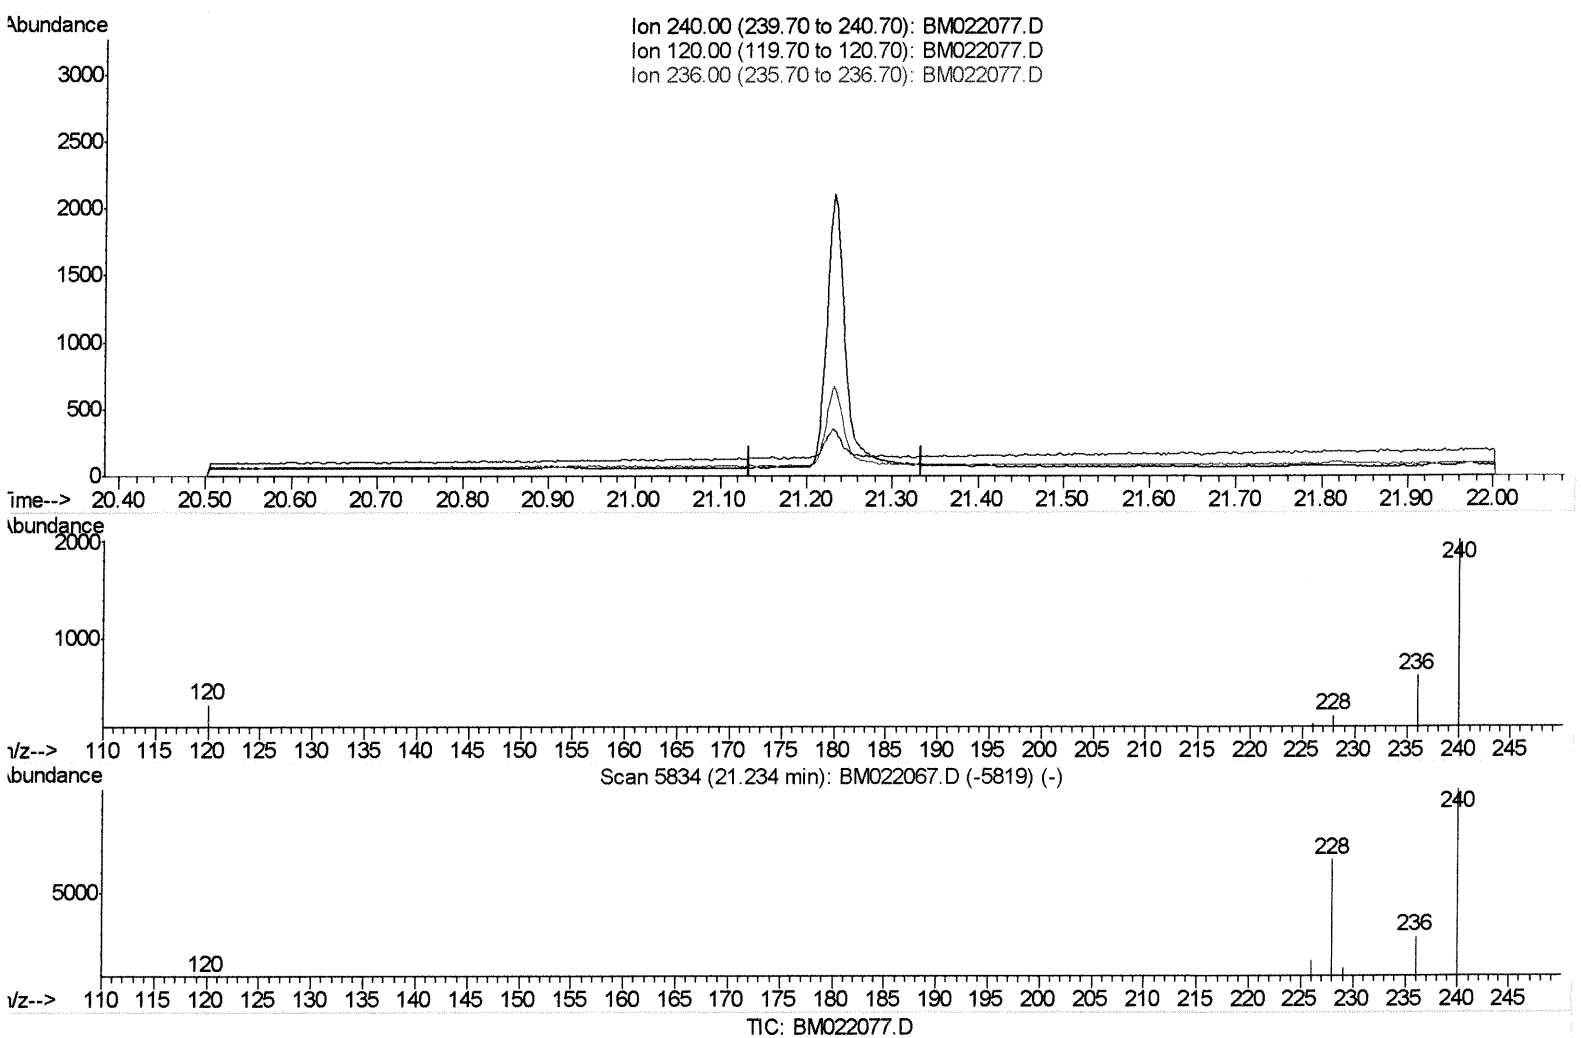

(16) Chrysene-d12 (I)

21.234min (-21.234) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.20	0.00#
236.00	32.30	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)




Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:48:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

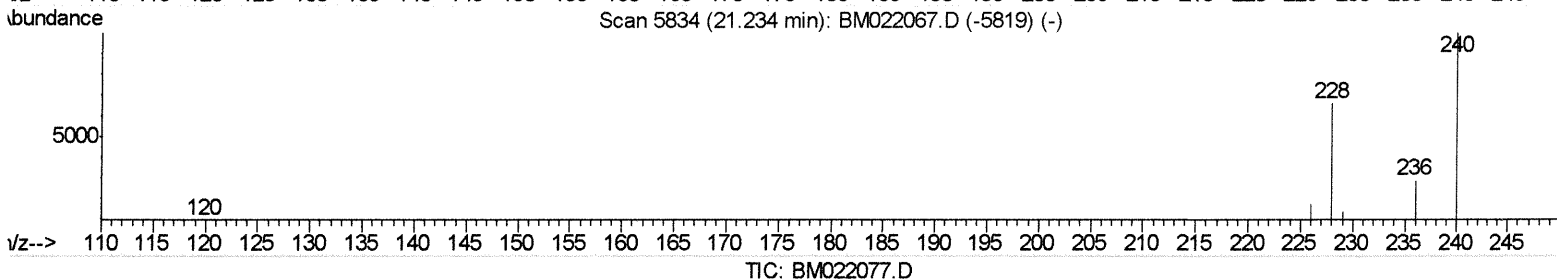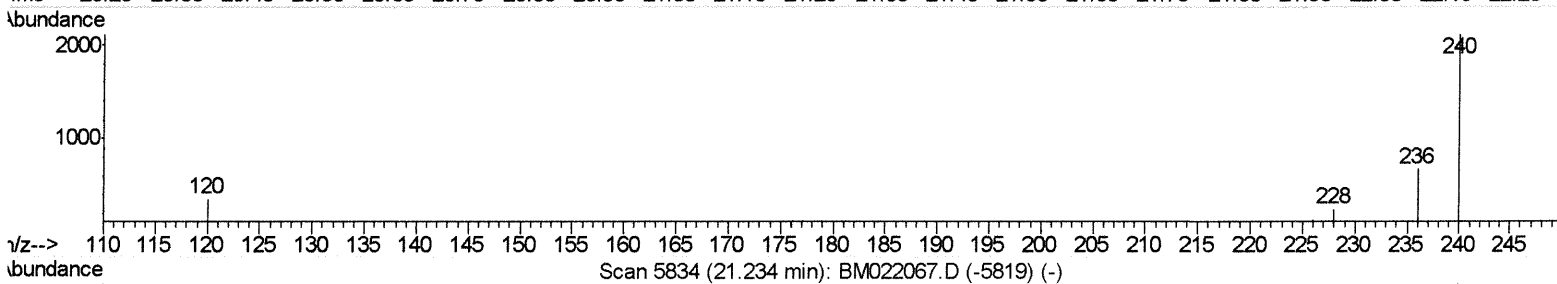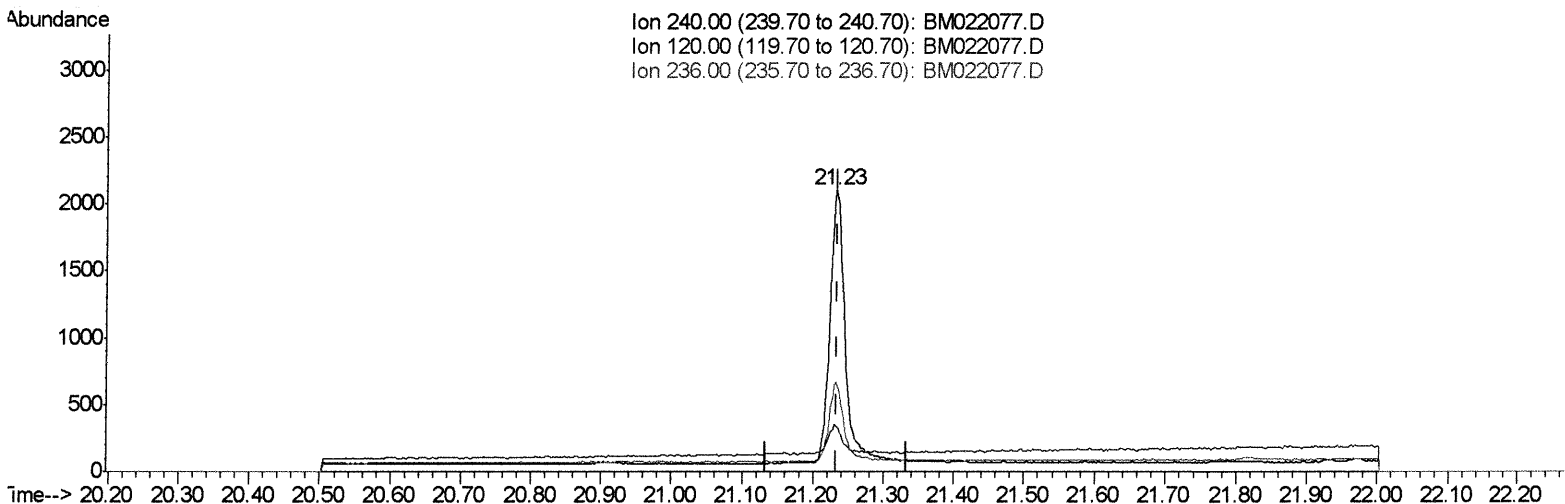

(16) Chrysene-d12 (I)

21.231min (-0.003) 0.40ng/ul m *JU* 08/14/19

response 2938

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	16.56
236.00	32.30	31.80
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)




Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:50:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

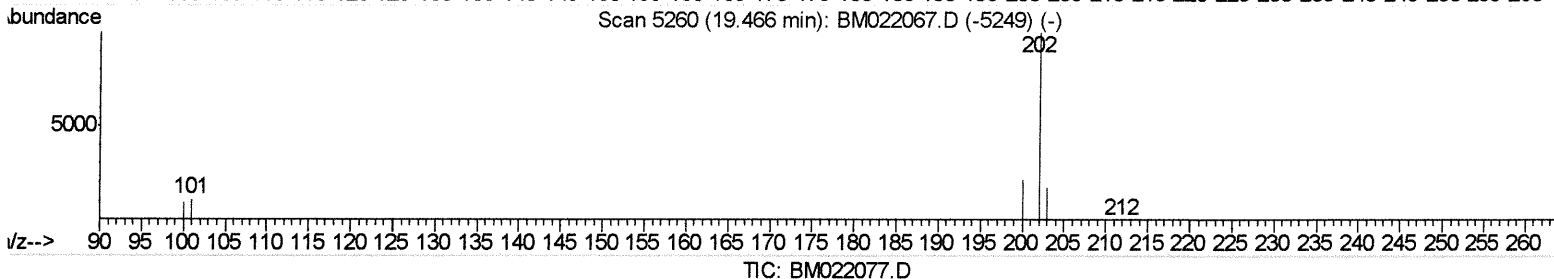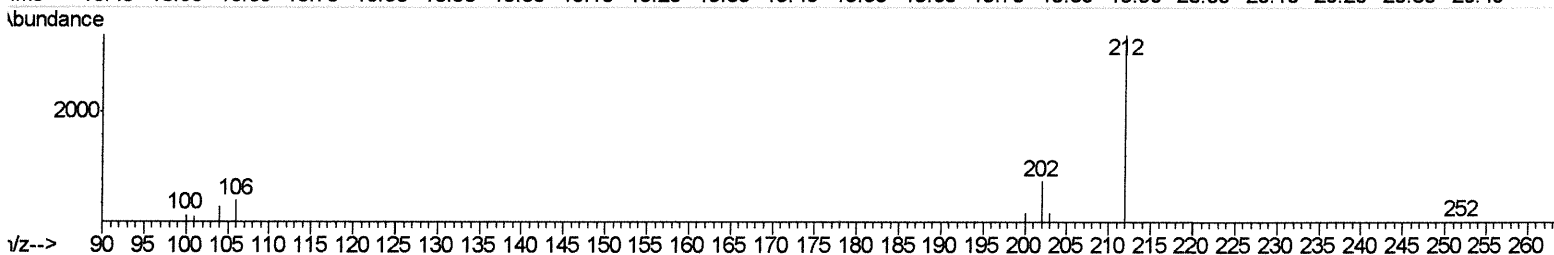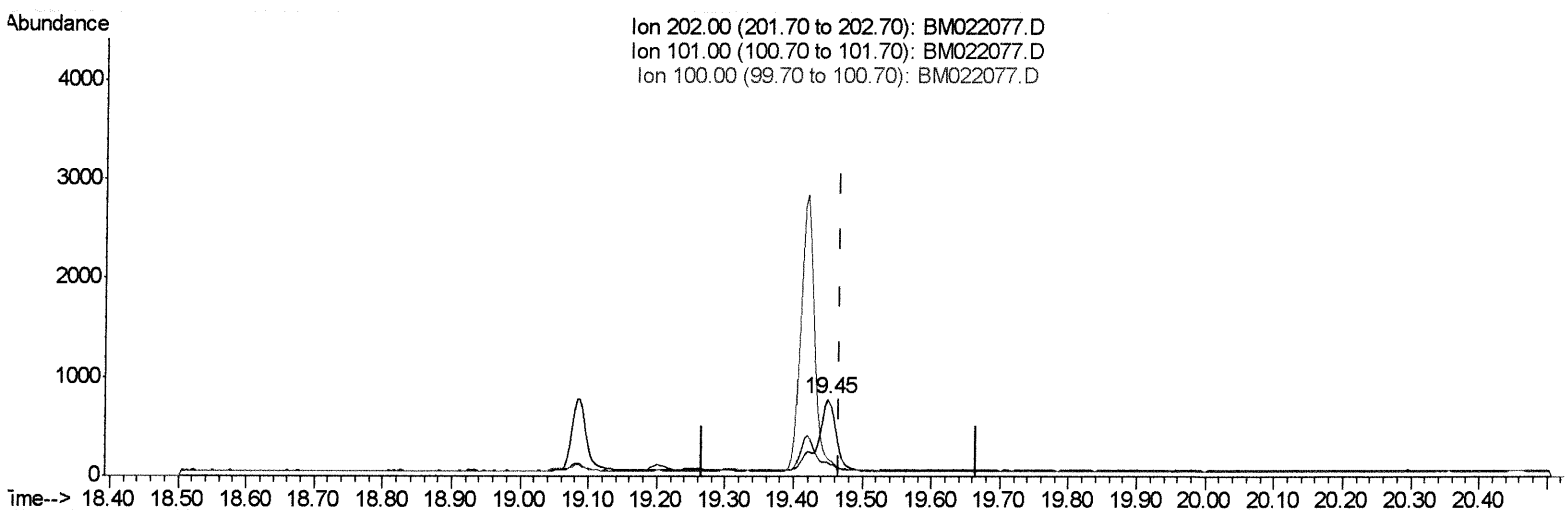

(17) Pyrene

19.449min (-0.017) 0.11ng/ul

response 1275

Ion	Exp%	Act%
202.00	100	100
101.00	10.40	17.99#
100.00	9.00	22.62#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)




Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:50:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

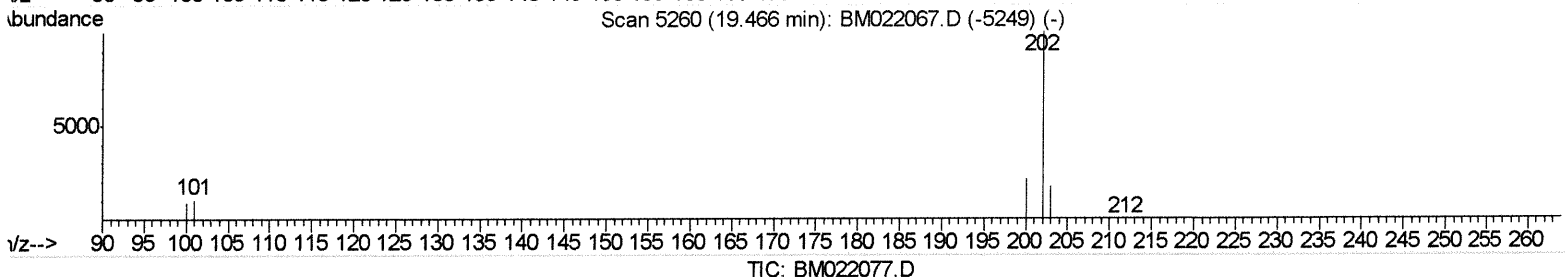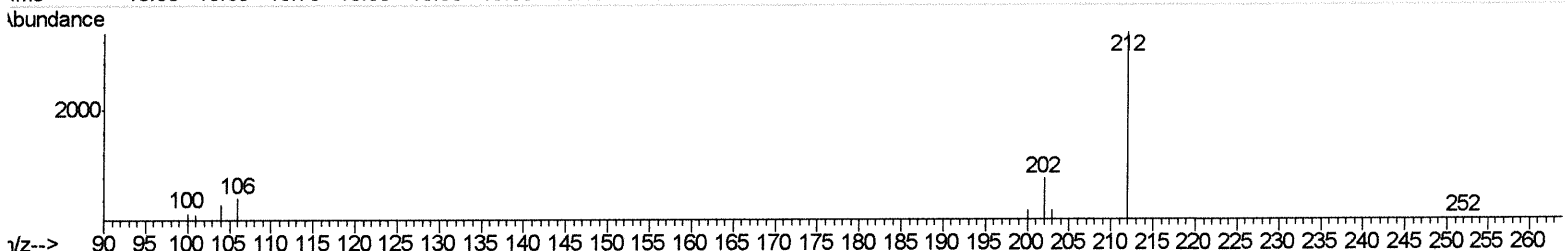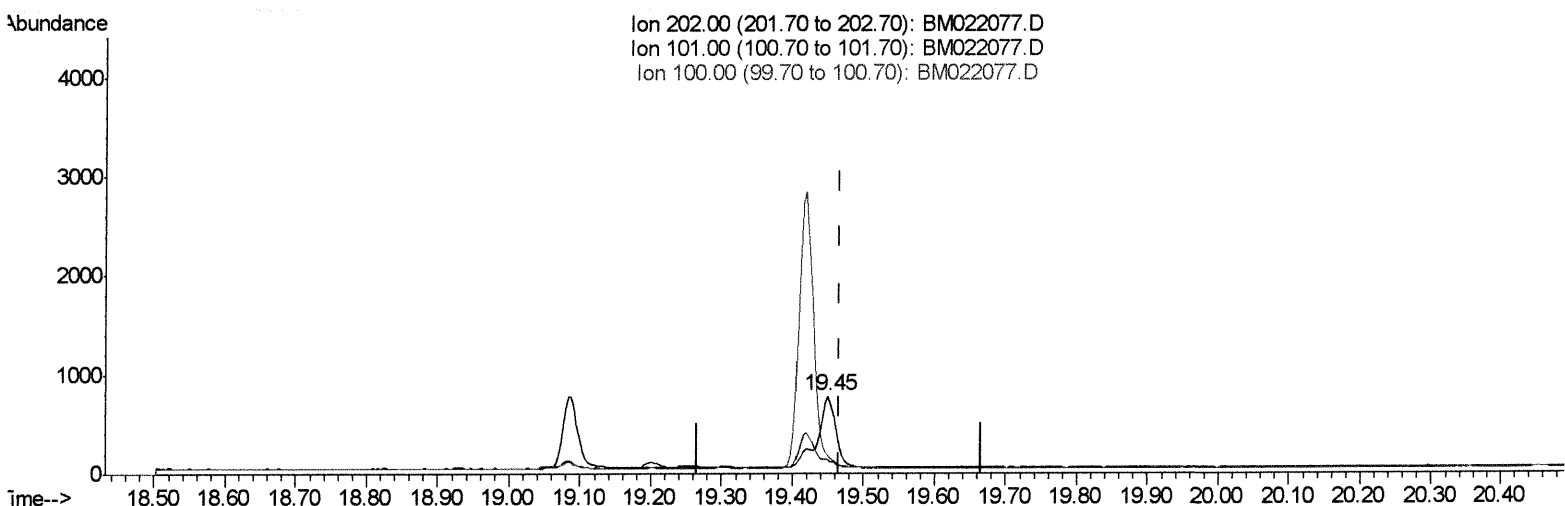

(17) Pyrene

19.449min (-0.017) 0.09ng/ul m *JU* 08/14/19

response 1030

Ion	Exp%	Act%
202.00	100	100
101.00	10.40	17.99#
100.00	9.00	22.62#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)




Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:50:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

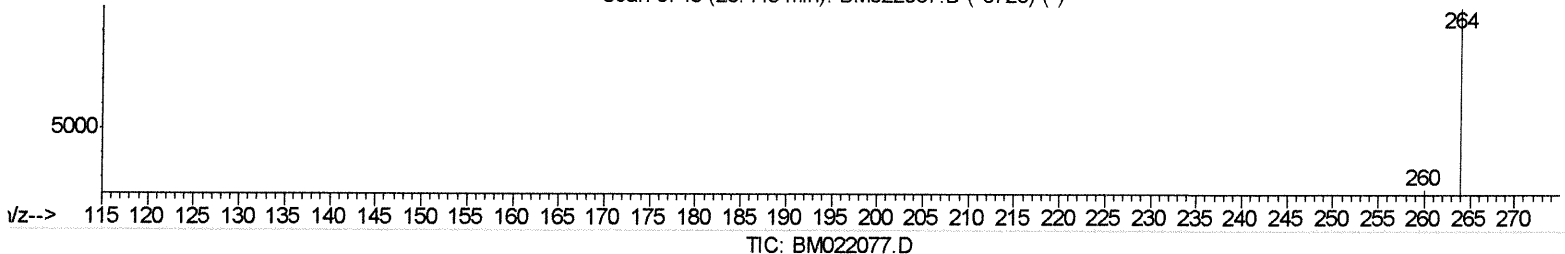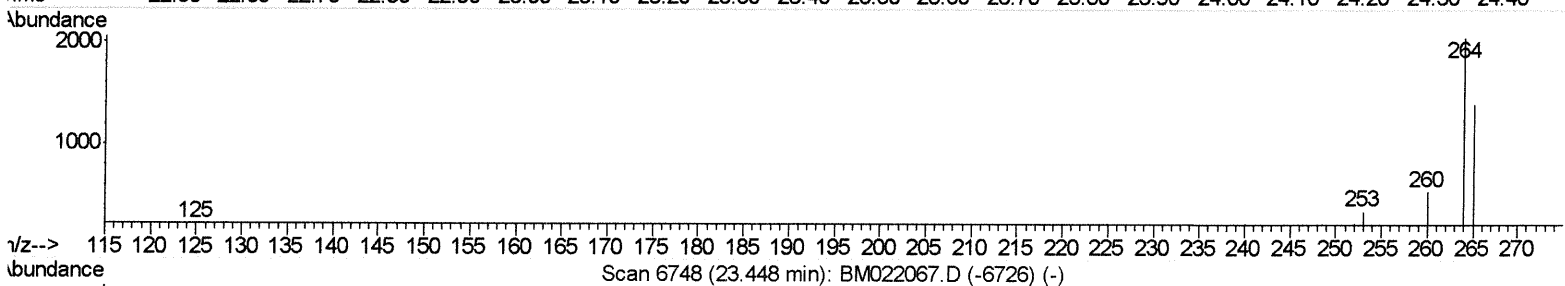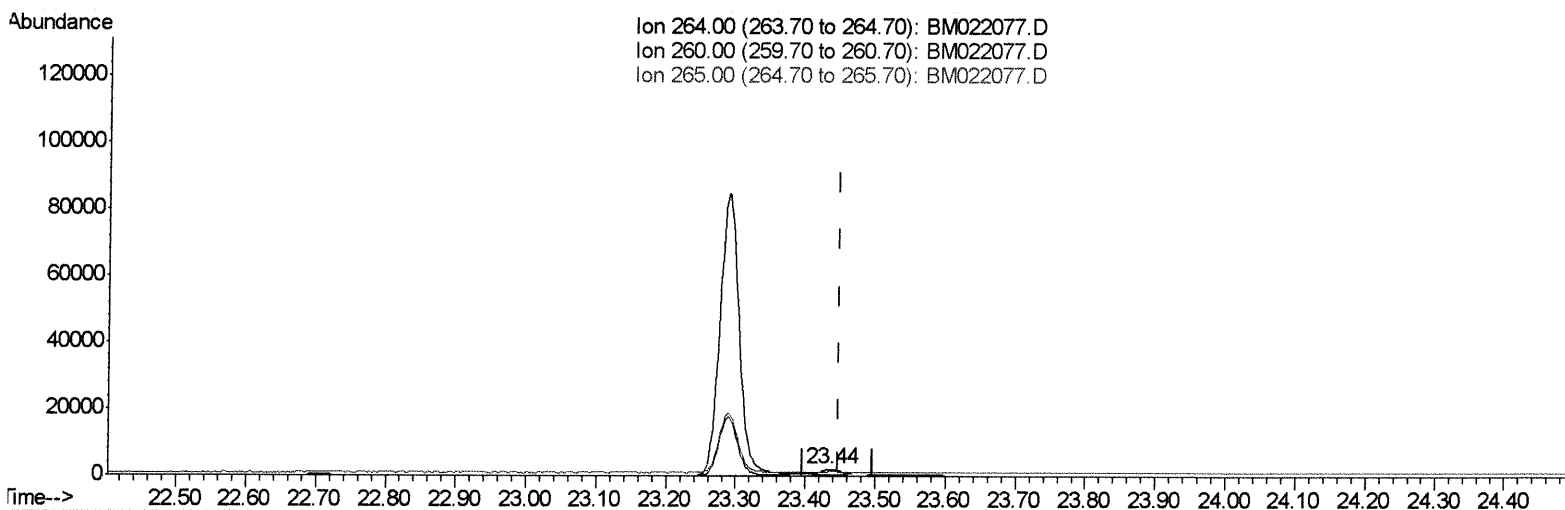

(20) Perylene-d12 (I)

23.435min (-0.012) 0.40ng/ul

response 3624

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	26.91
265.00	117.00	68.60#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)




Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:50:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

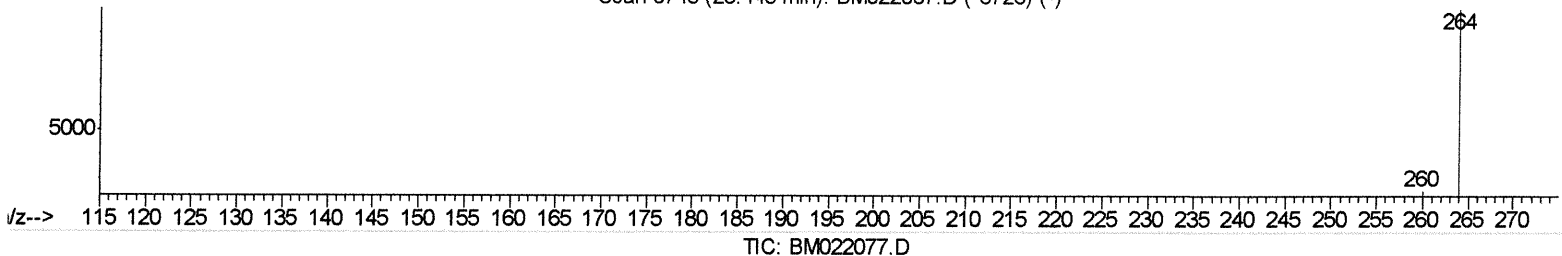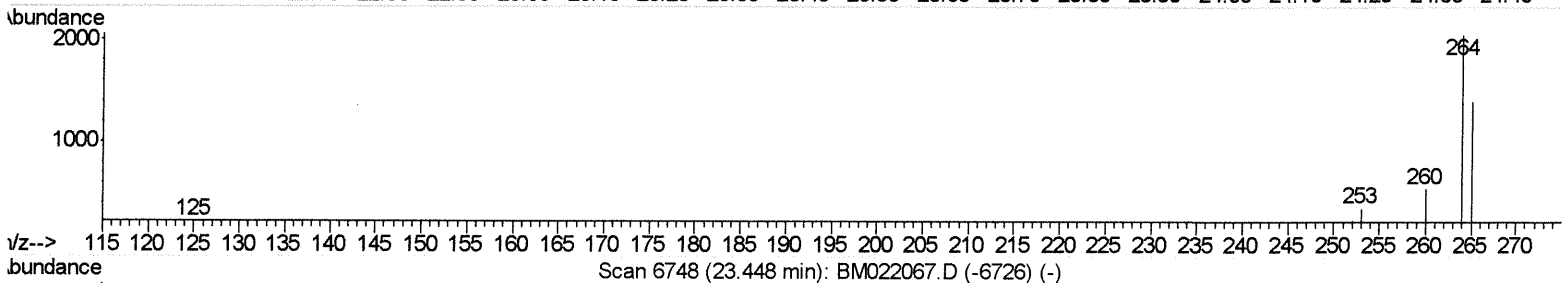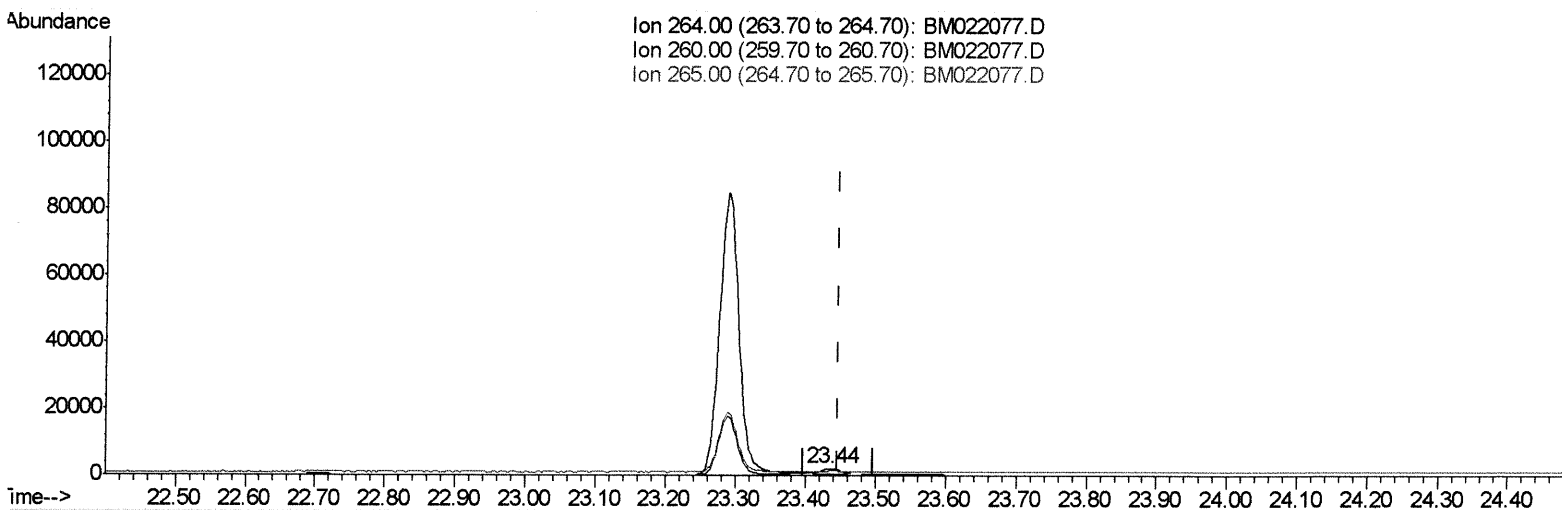

(20) Perylene-d12 (I)

23.435min (-0.012) 0.40ng/ul m

JU
08/14/19

response 2993

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	26.91
265.00	117.00	68.60#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)




Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:50:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

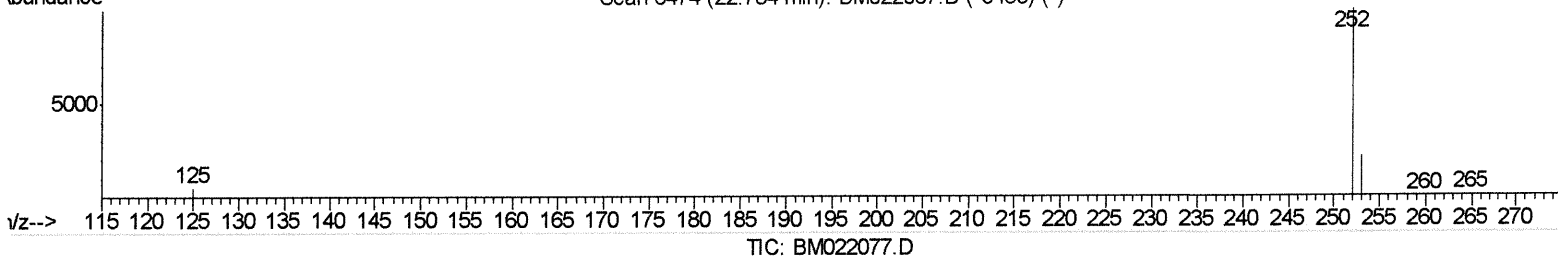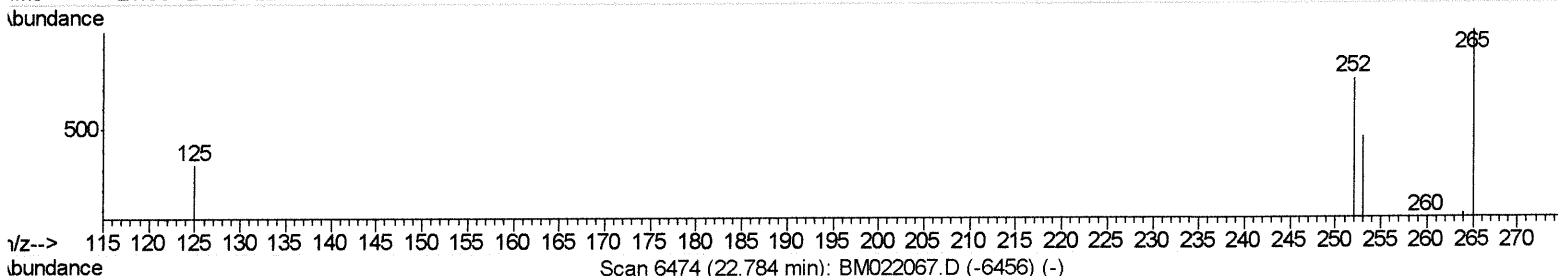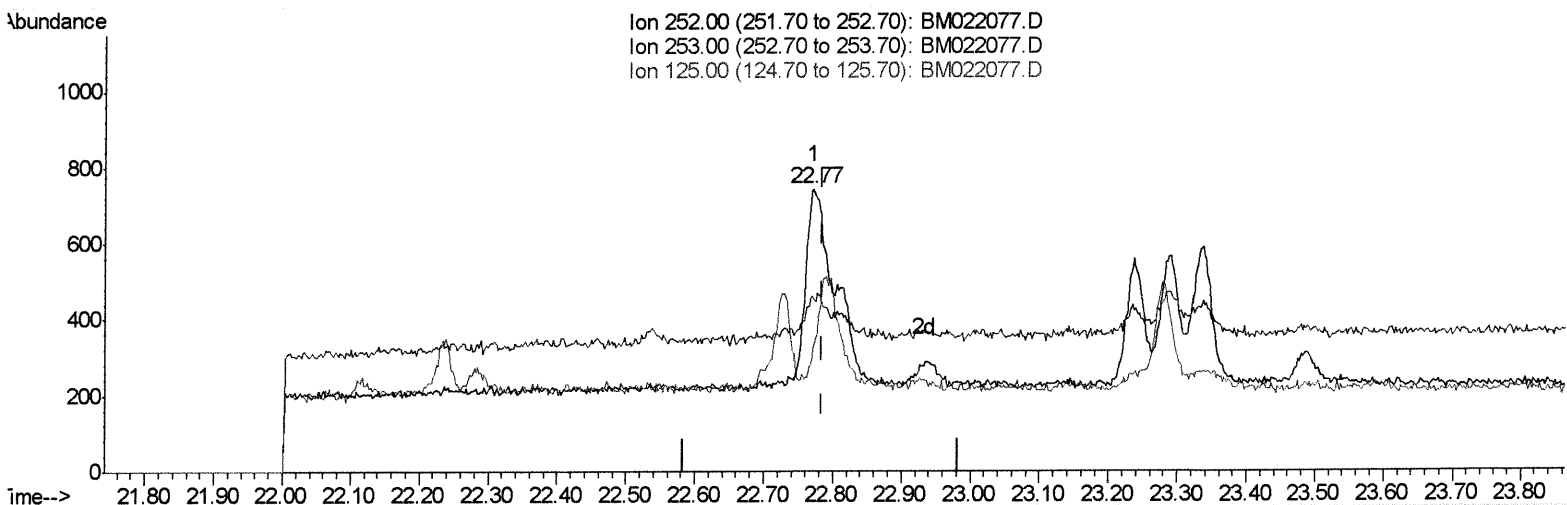

(21) Benzo(b)fluoranthene

22.771min (-0.012) 0.15ng/ul

response 1515

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	61.46
125.00	15.50	43.94#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)




Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:50:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

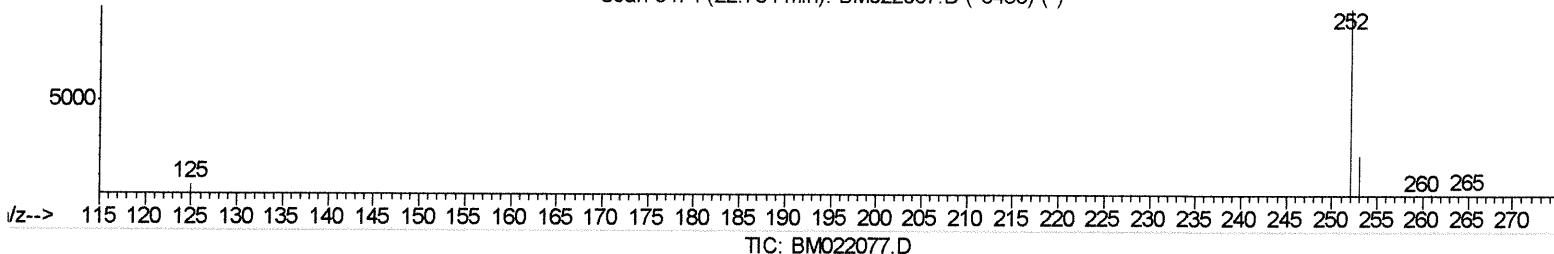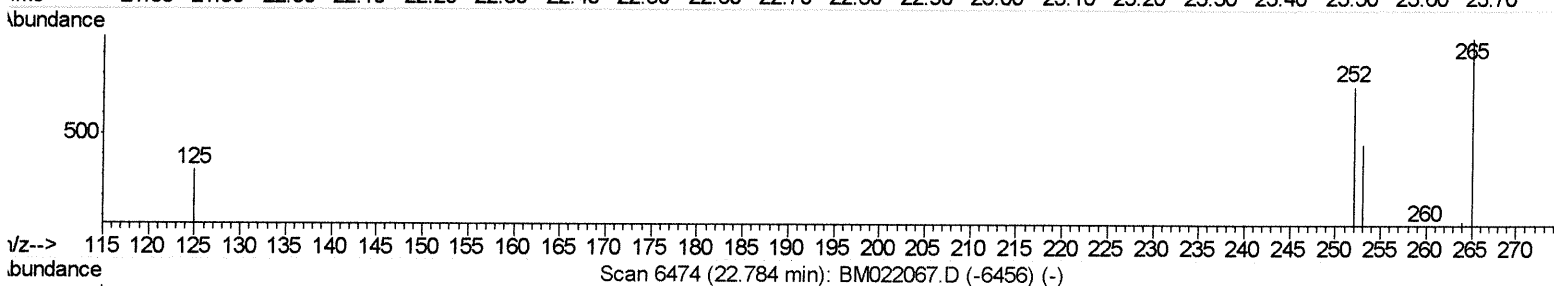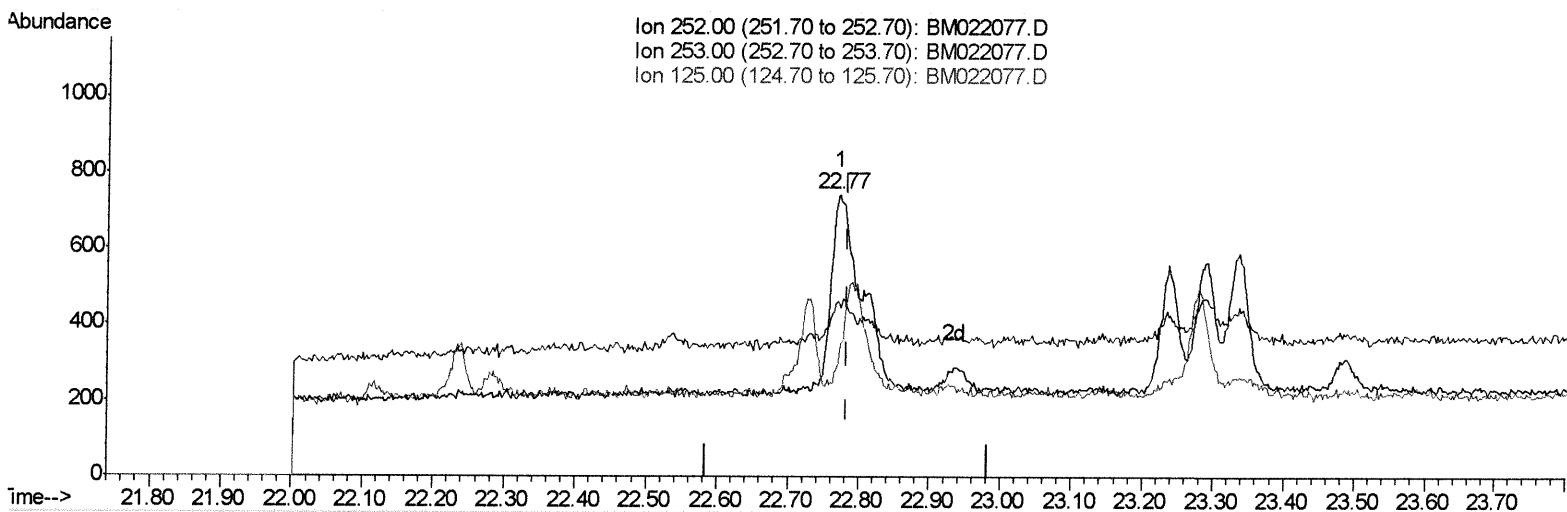

(21) Benzo(b)fluoranthene

22.771min (-0.012) 0.11ng/ul m

JU
08/14/19

response 1107

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	61.46
125.00	15.50	43.94#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)

Data File : BM022077.D

Acq On : 13 Aug 2019 19:25

Operator : HP/JU

Sample : K4183-01

Misc :

ALS Vial : 57 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM



Quant Time: Aug 14 07:50:57 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Aug 14 07:18:38 2019

Response via : Initial Calibration

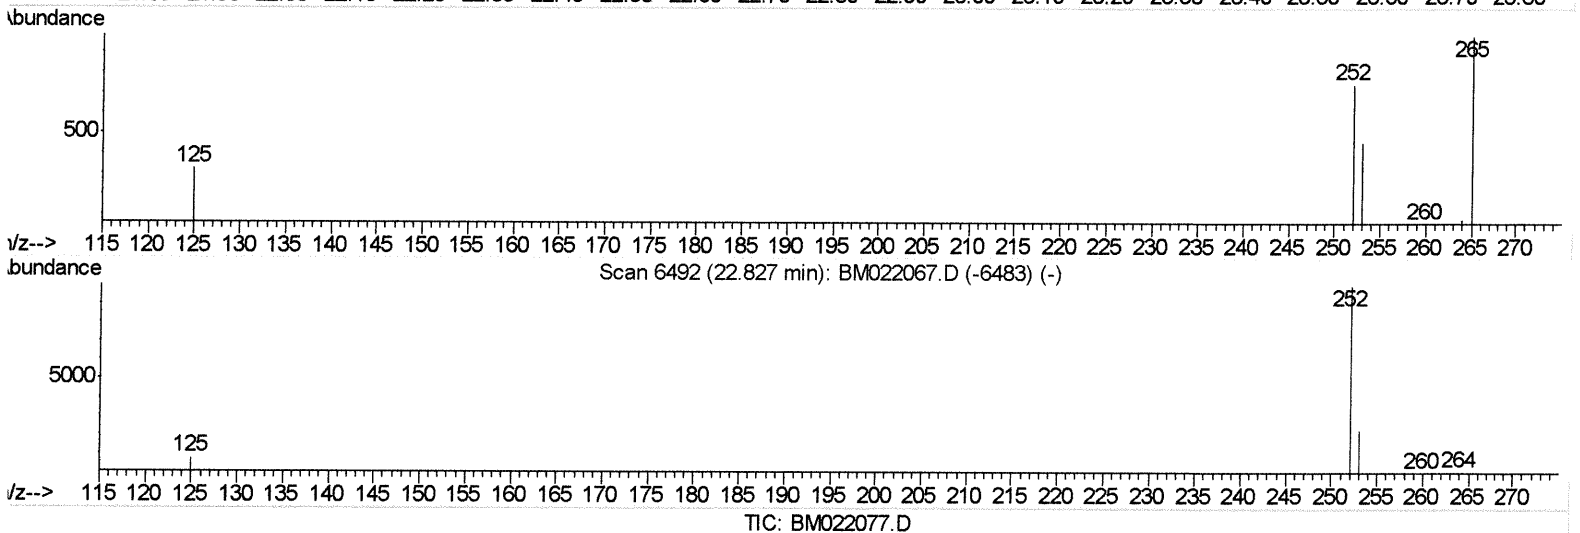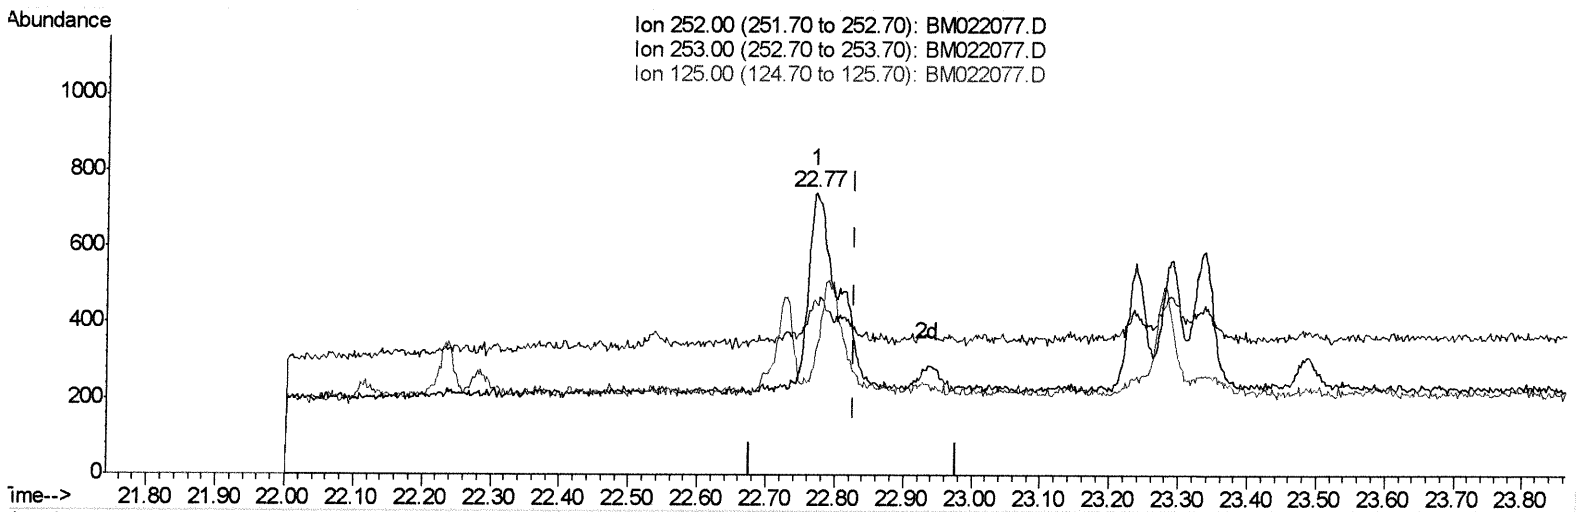

(22) Benzo(k)fluoranthene

22.771min (-0.056) 0.13ng/ul

response 1515

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	61.46#
125.00	15.20	43.94#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (Qedit)




Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:50:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

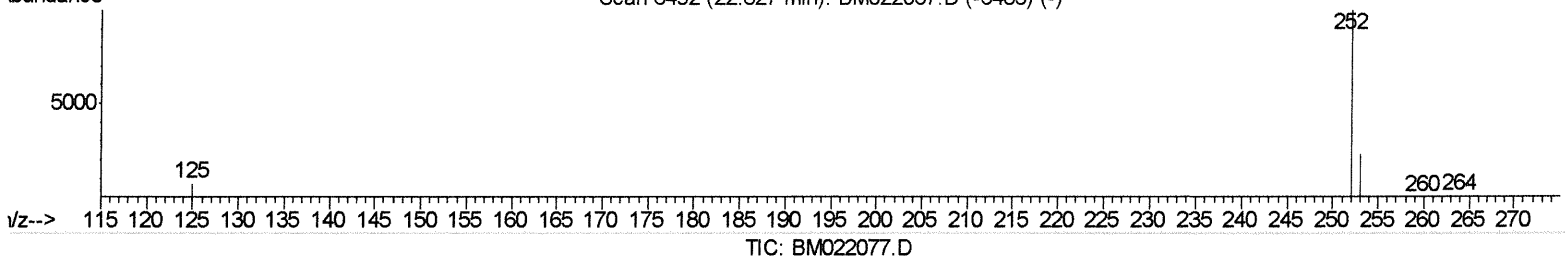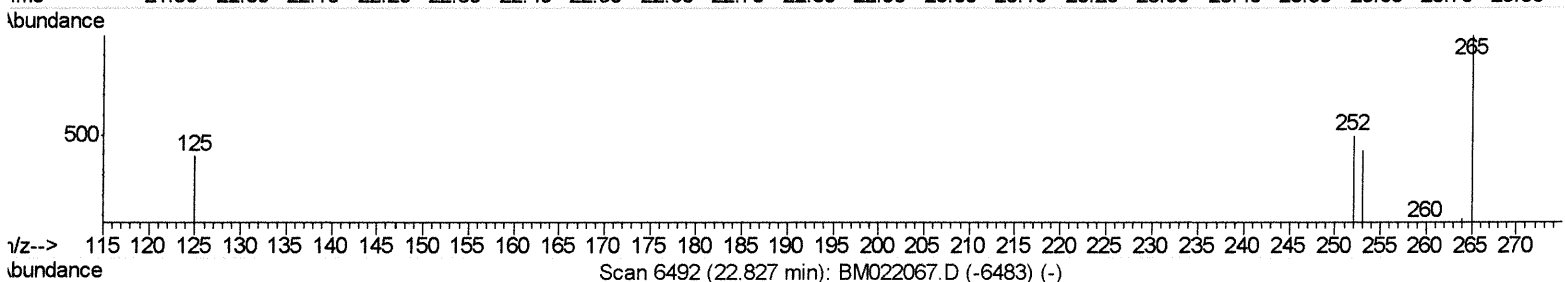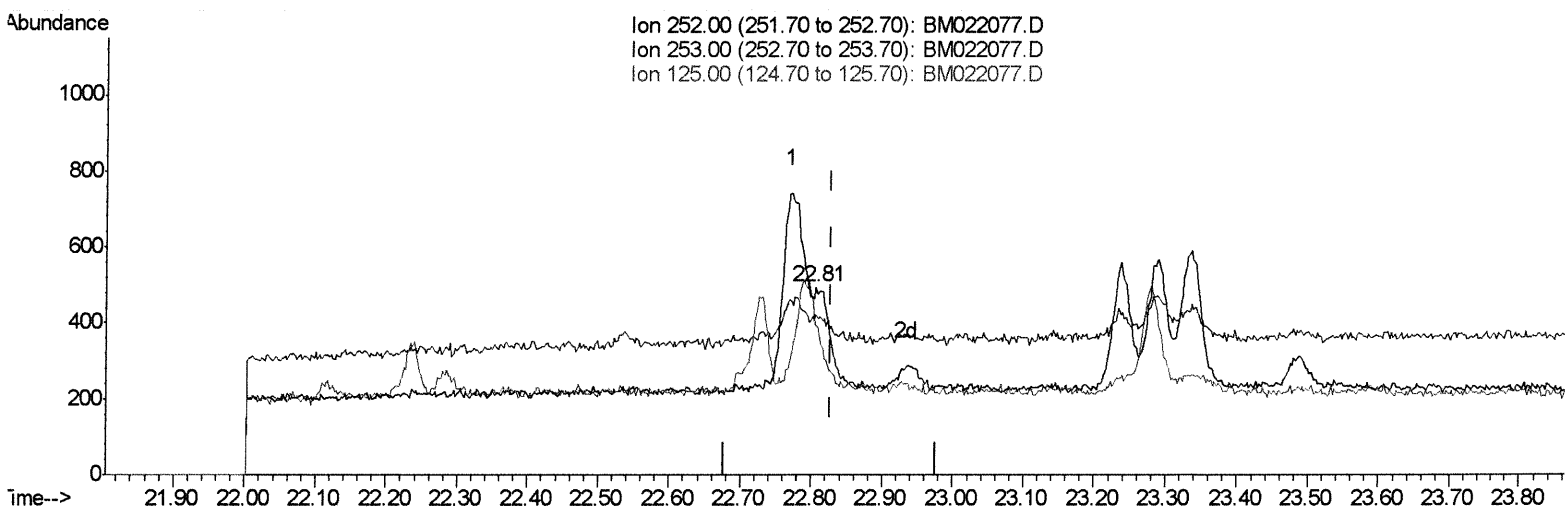

(22) Benzo(k)fluoranthene

22.805min (-0.022) 0.03ng/ul m

JU
08/14/19

response 379

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	85.40#
125.00	15.20	79.92#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
Quantitation Report (QT Reviewed)

Data File : BM022077.D
Acq On : 13 Aug 2019 19:25
Operator : HP/JU
Sample : K4183-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

mohammad
8/15/2019 5:07:40 PM

Quant Time: Aug 14 07:51:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 14 07:18:38 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	718	0.40	ng/ul	0.00
2) Naphthalene-d8	10.38	136	2945	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	1534	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.01	188	3398m→	0.40	ng/ul	-0.03
16) Chrysene-d12	21.23	240	2938m→	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	2993m→	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	883	0.18	ng/ul	-0.02
14) Fluoranthene-d10	19.05	212	2118m	0.18	ng/ul	-0.02
Target Compounds						
					Qvalue	
12) Phenanthrene	17.06	178	356m→	0.036	ng/ul	> 74
15) Fluoranthene	19.08	202	1083m→	0.082	ng/ul	> 81
17) Pyrene	19.45	202	1030m→	0.085	ng/ul	> 41
18) Benzo(a)anthracene	21.22	228	624	0.059	ng/ul#	100
19) Chrysene	21.27	228	693	0.051	ng/ul#	48
21) Benzo(b)fluoranthene	22.77	252	1107m→	0.110	ng/ul	> 74
22) Benzo(k)fluoranthene	22.81	252	379m→	0.033	ng/ul	> 81
23) Benzo(a)pyrene	23.34	252	671	0.065	ng/ul#	41
24) Indeno(1,2,3-cd)pyrene	25.66	276	564	0.046	ng/ul#	100
26) Benzo(g,h,i)perylene	26.34	276	569	0.052	ng/ul#	48

(#) = qualifier out of range (m) = manual integration (+) = signals summed