


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022114.D
 Acq On : 14 Aug 2019 18:49
 Operator : HP/JU
 Sample : K4183-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH0

Manual Integrations
 APPROVED

mohammad
 8/15/2019 5:09:23 PM

Quant Time: Aug 15 11:07:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

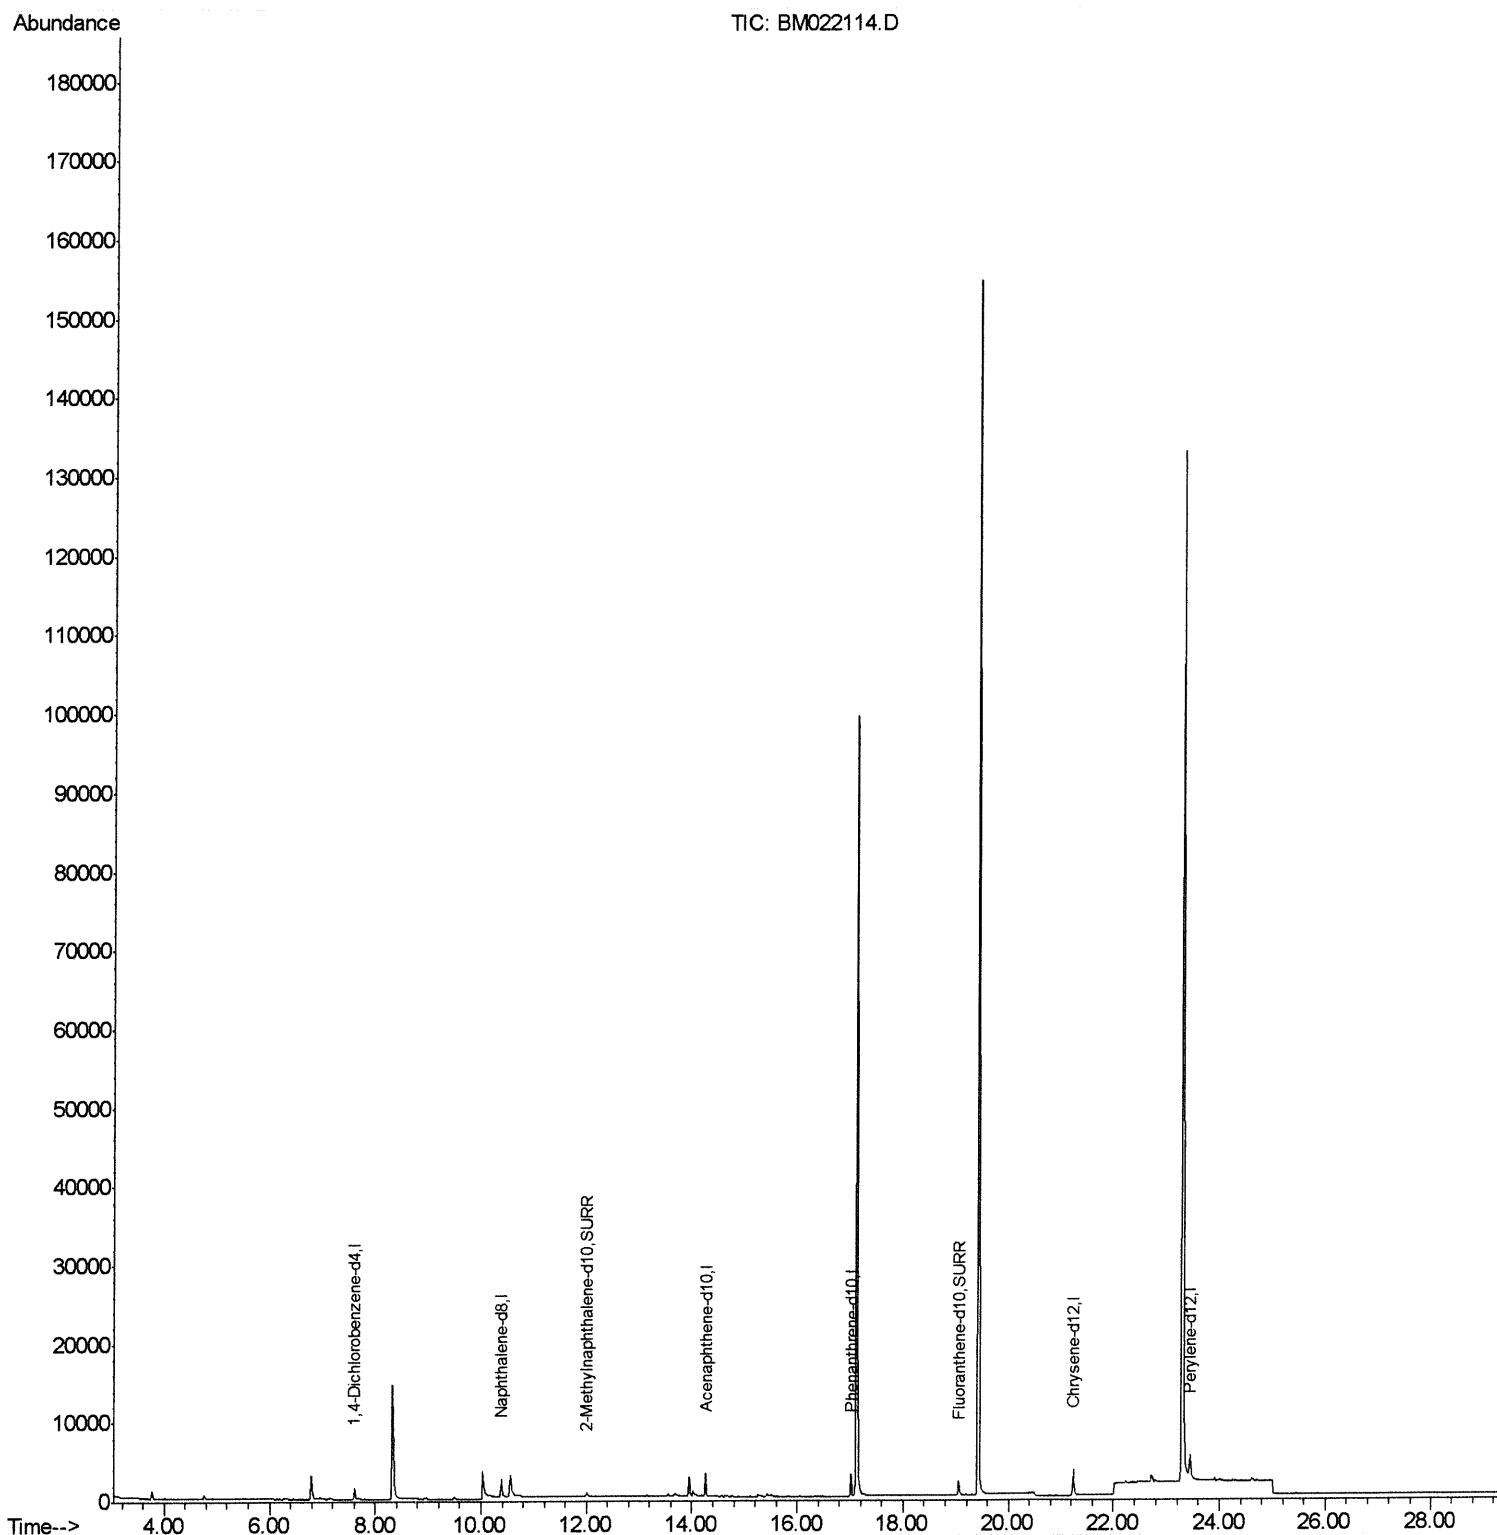




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022114.D
 Acq On : 14 Aug 2019 18:49
 Operator : HP/JU
 Sample : K4183-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH0

Manual Integrations
 APPROVED

mohammad
 8/15/2019 5:09:23 PM

Quant Time: Aug 15 11:05:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

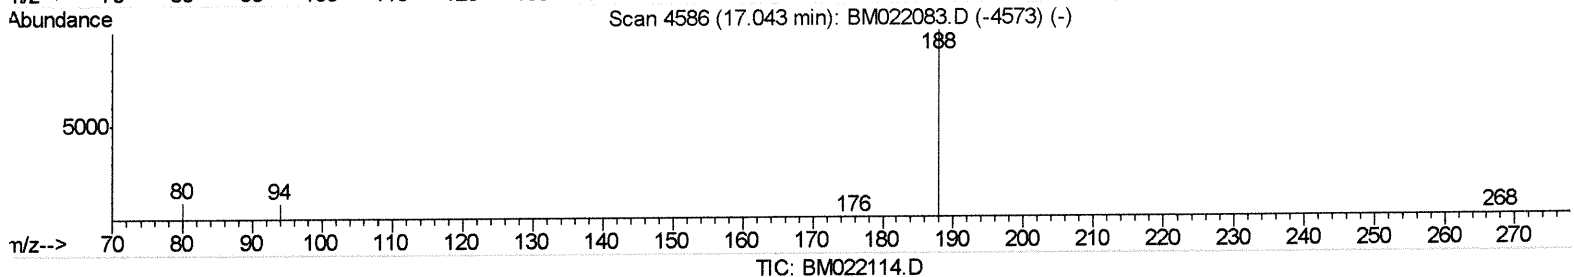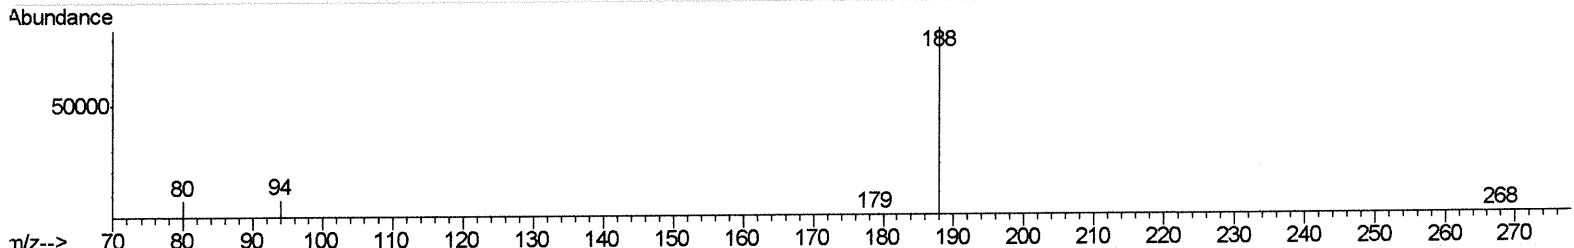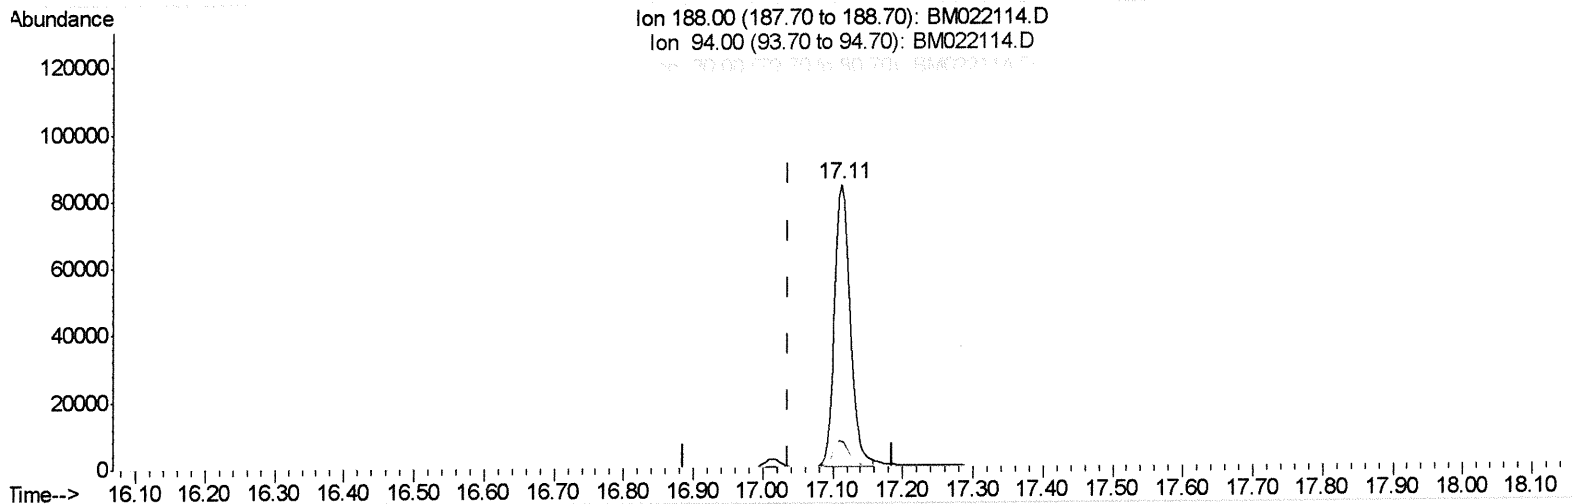

(10) Phenanthrene-d10 (I)
 17.112min (+0.076) 0.40ng/ul
 response 130543

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	9.19
80.00	11.40	8.68#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022114.D
 Acq On : 14 Aug 2019 18:49
 Operator : HP/JU
 Sample : K4183-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH0

Manual Integrations
 APPROVED

mohammad
 8/15/2019 5:09:23 PM

Quant Time: Aug 15 11:05:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

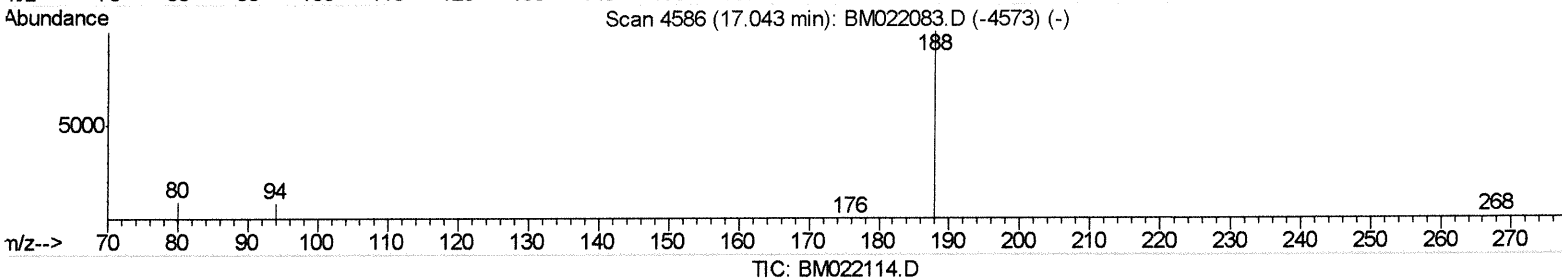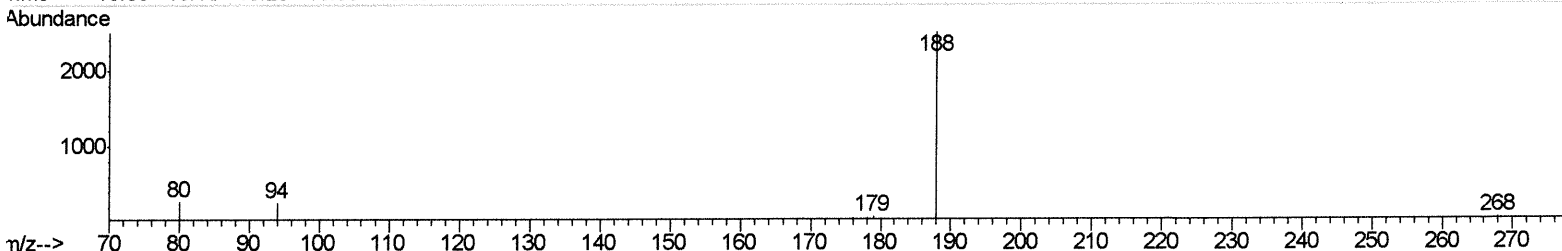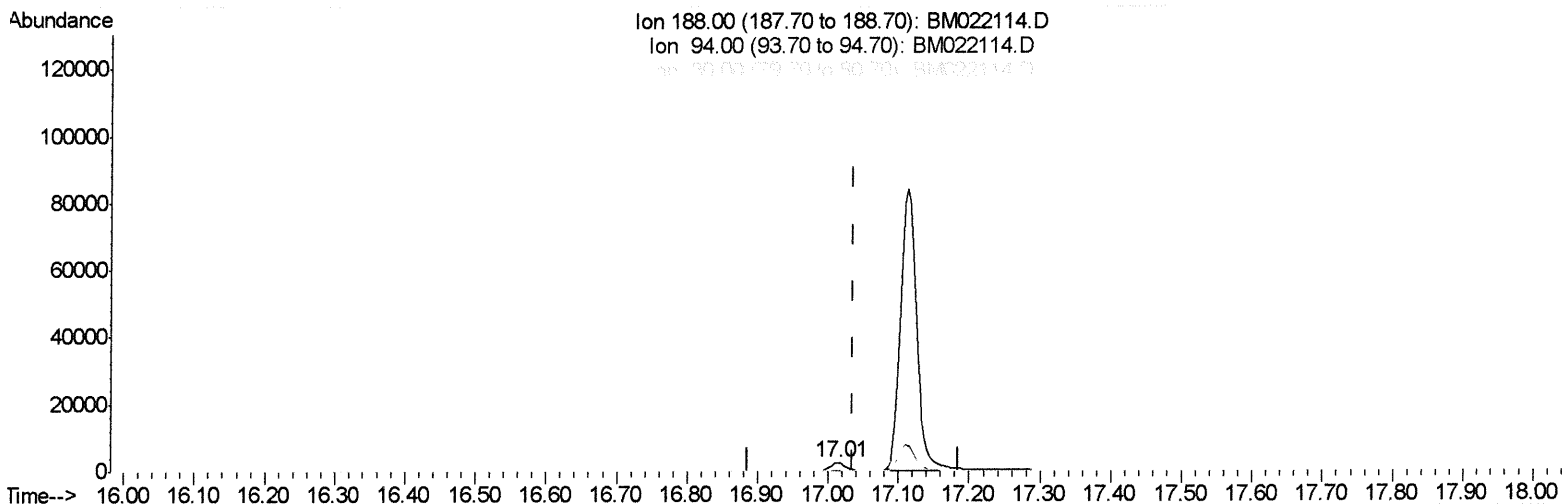

(10) Phenanthrene-d10 (I)

17.015min (-0.021) 0.40ng/ul m

JU
 08/15/19

response 3864

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.58
80.00	11.40	11.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022114.D
 Acq On : 14 Aug 2019 18:49
 Operator : HP/JU
 Sample : K4183-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH0

Manual Integrations
 APPROVED

mohammad
 8/15/2019 5:09:23 PM

Quant Time: Aug 15 11:05:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

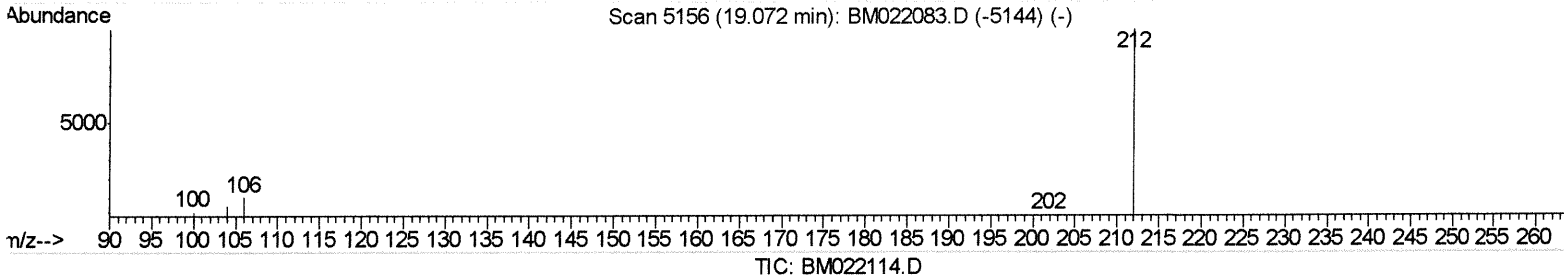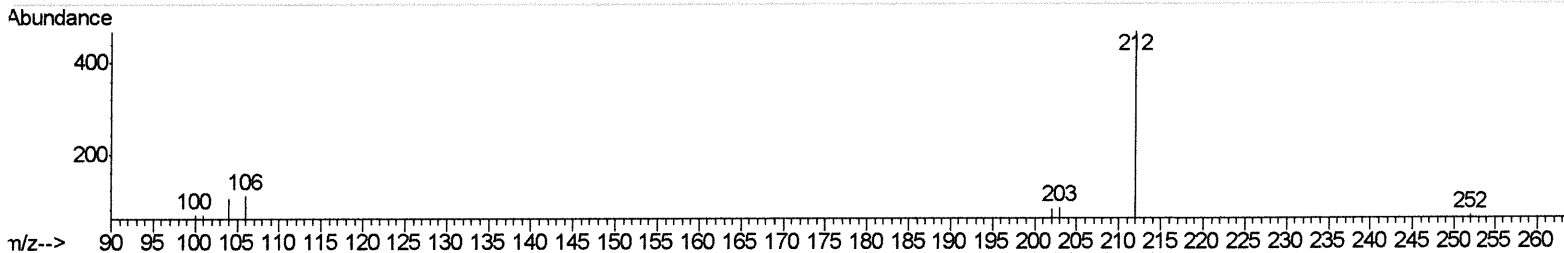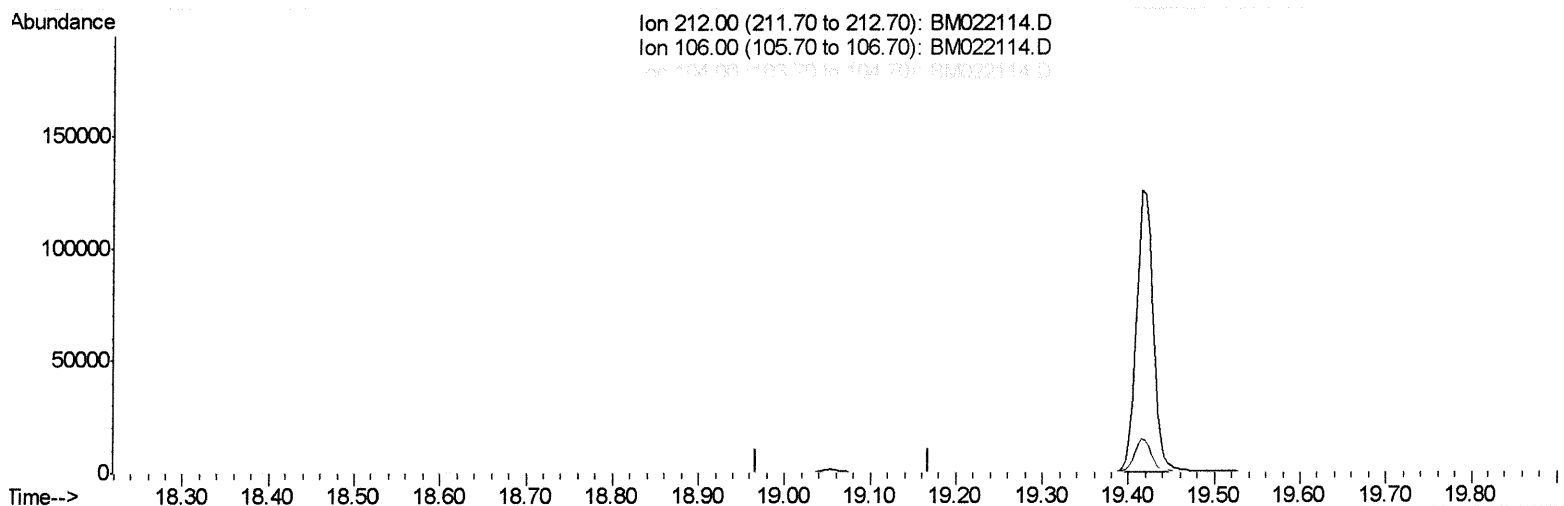

(14) Fluoranthene-d10 (SURR)

19.068min (-19.068) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022114.D
 Acq On : 14 Aug 2019 18:49
 Operator : HP/JU
 Sample : K4183-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH0

Manual Integrations
 APPROVED

mohammad
 8/15/2019 5:09:23 PM

Quant Time: Aug 15 11:05:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

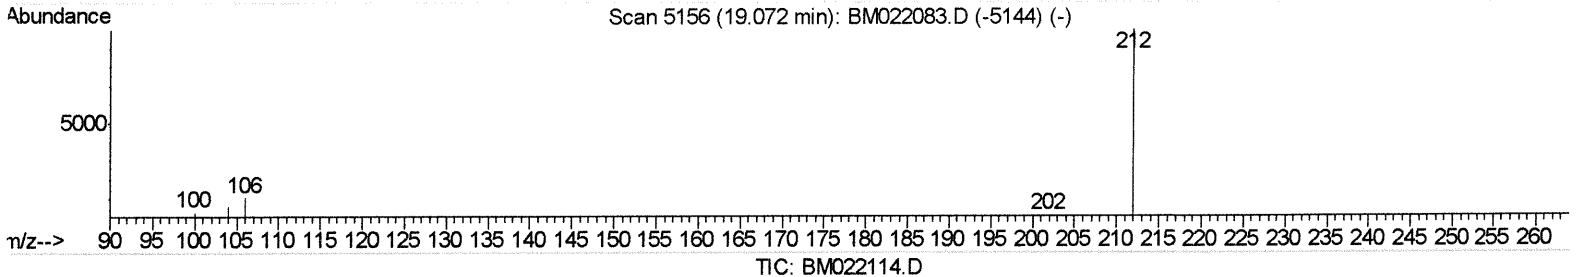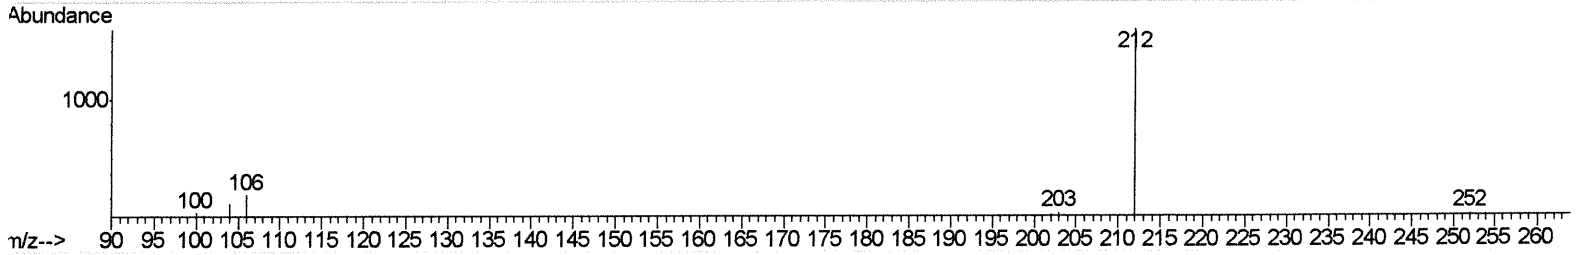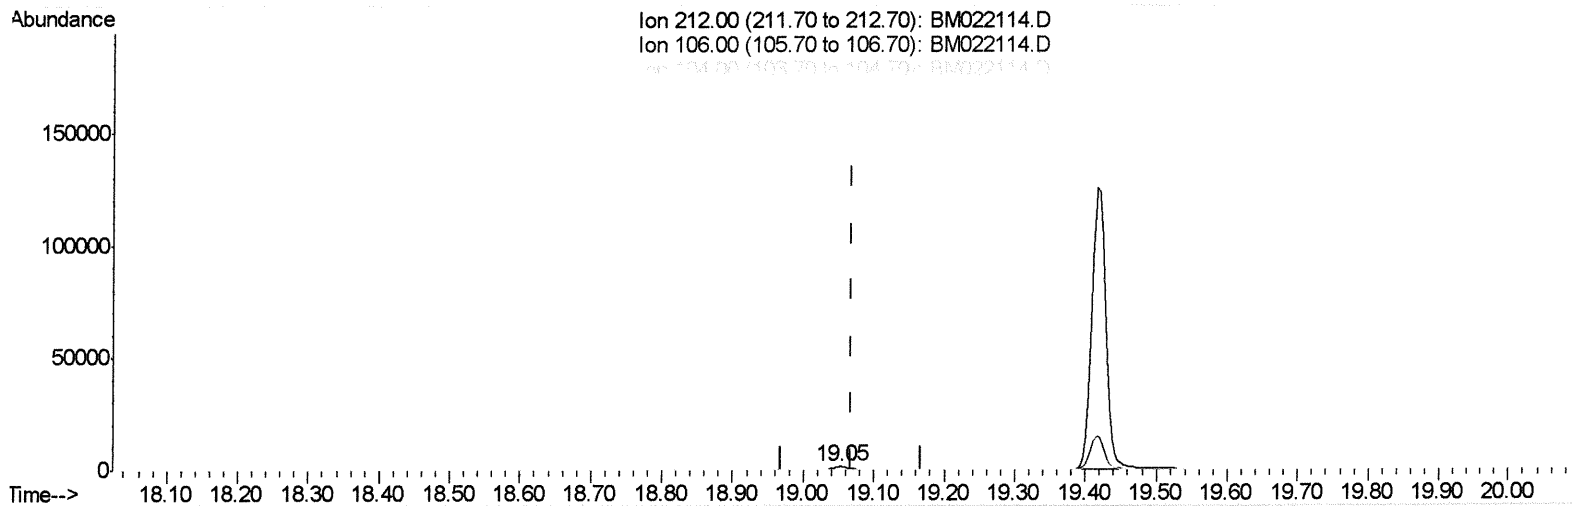

(14) Fluoranthene-d10 (SURR)

19.053min (-0.015) 0.18ng/ul m *JU 8/15/19*

response 2332

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022114.D
 Acq On : 14 Aug 2019 18:49
 Operator : HP/JU
 Sample : K4183-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH0

Manual Integrations
 APPROVED

mohammad
 8/15/2019 5:09:23 PM

Quant Time: Aug 15 11:05:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

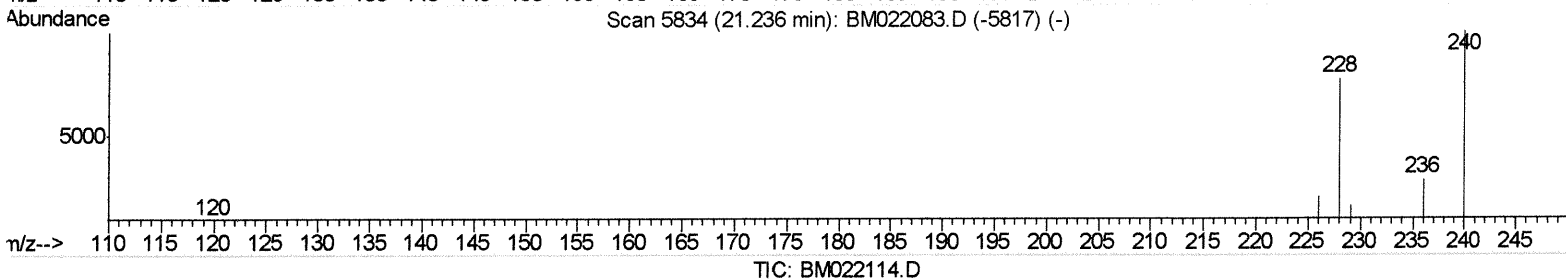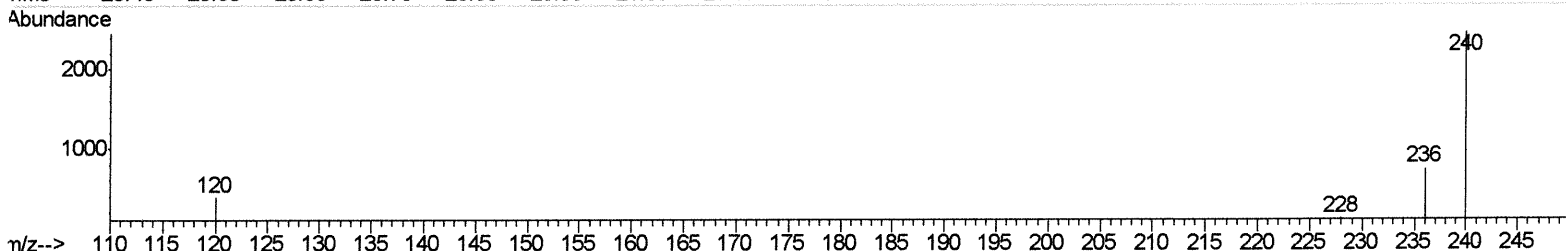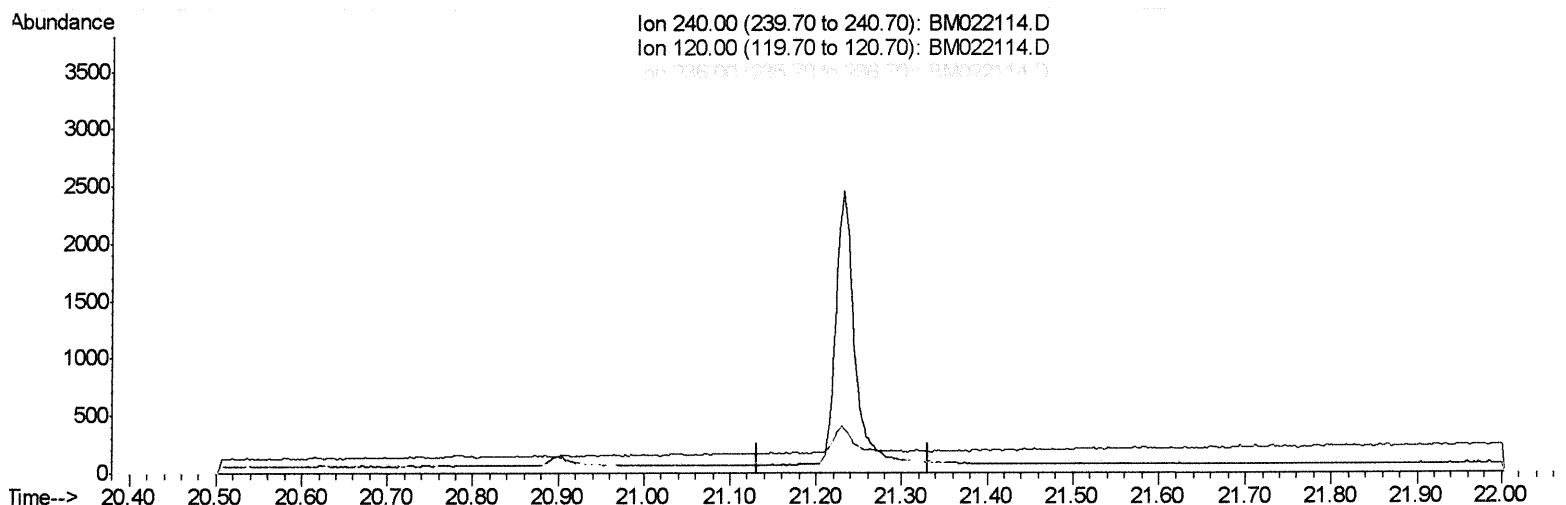

(16) Chrysene-d12 (I)
 21.231min (-21.231) 0.00ng/ul
 response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.20	0.00#
236.00	32.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022114.D
 Acq On : 14 Aug 2019 18:49
 Operator : HP/JU
 Sample : K4183-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH0

Manual Integrations
 APPROVED

mohammad
 8/15/2019 5:09:23 PM

Quant Time: Aug 15 11:05:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

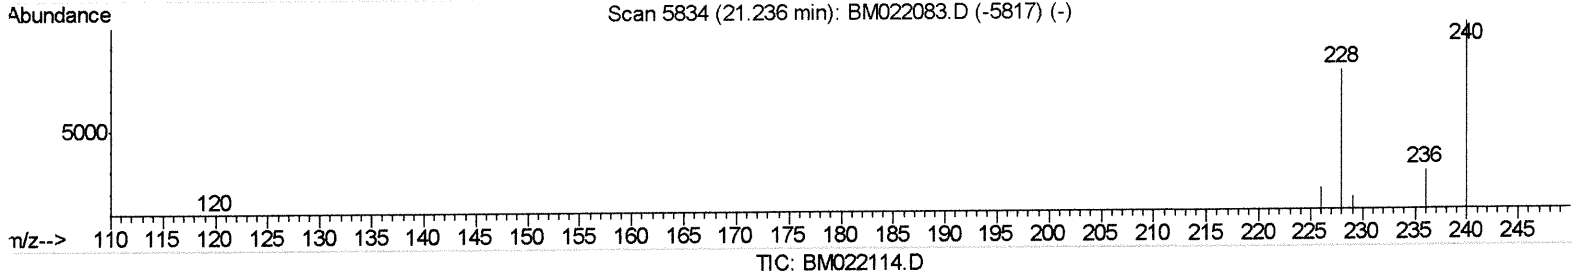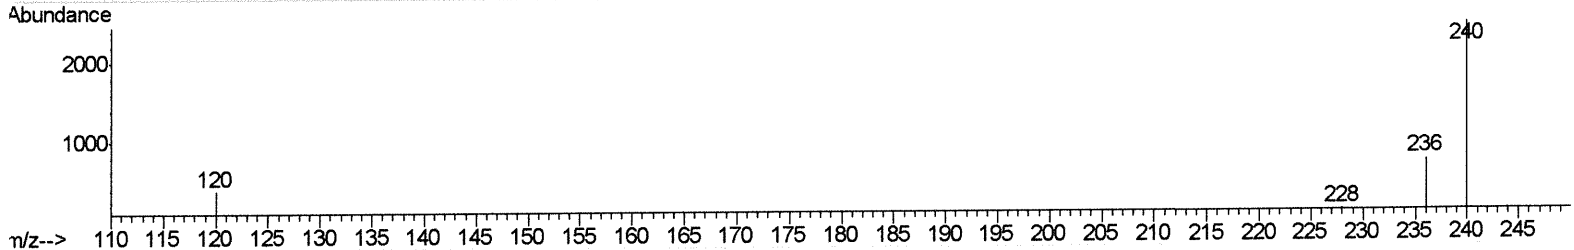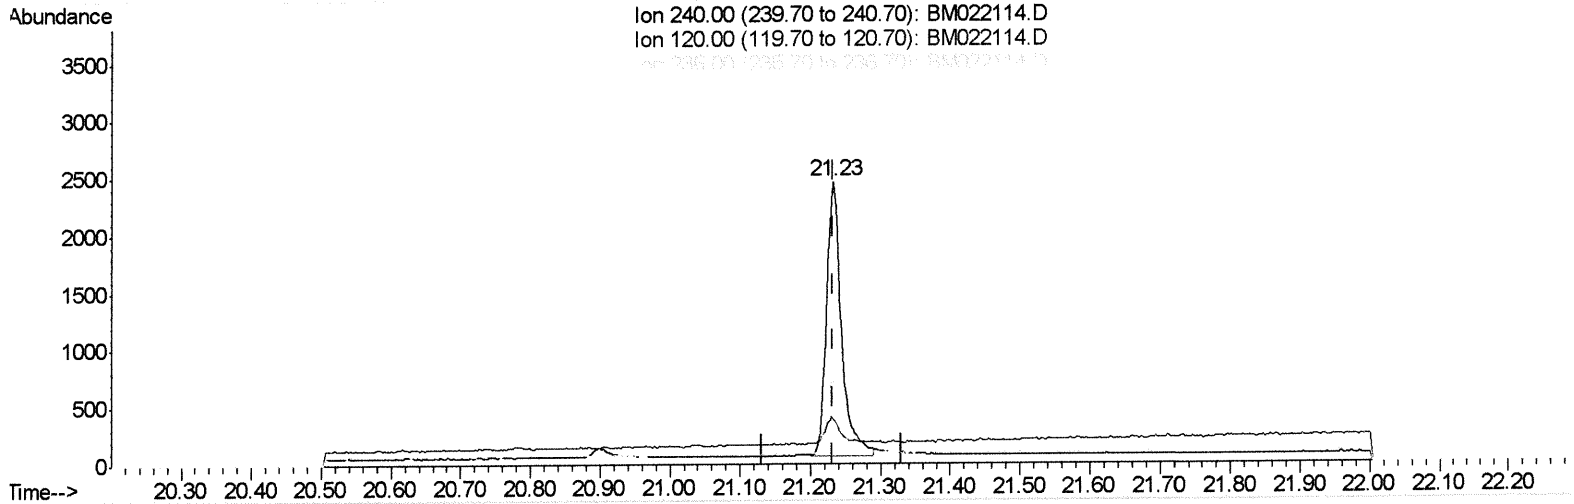

(16) Chrysene-d12 (I)

21.231min (+0.000) 0.40ng/ul m *JU 08/15/19*

response 3617

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	15.75
236.00	32.30	29.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081219\
 Data File : BM022114.D
 Acq On : 14 Aug 2019 18:49
 Operator : HP/JU
 Sample : K4183-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAH0

Manual Integrations
 APPROVED

mohammad
 8/15/2019 5:09:23 PM

Quant Time: Aug 15 11:07:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 14 13:53:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	817	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.38	136	3247	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.26	164	1699	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.01	188	3864m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.23	240	3617m	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	4017	0.40	ng/ul	0.00

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	812	0.15	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	2332m	0.18	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed