


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM081219\
 Data File : BM022020.D
 Acq On : 12 Aug 2019 07:59
 Operator : HP/JU
 Sample : DFTPP03
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP03

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 13 05:22:05 2019

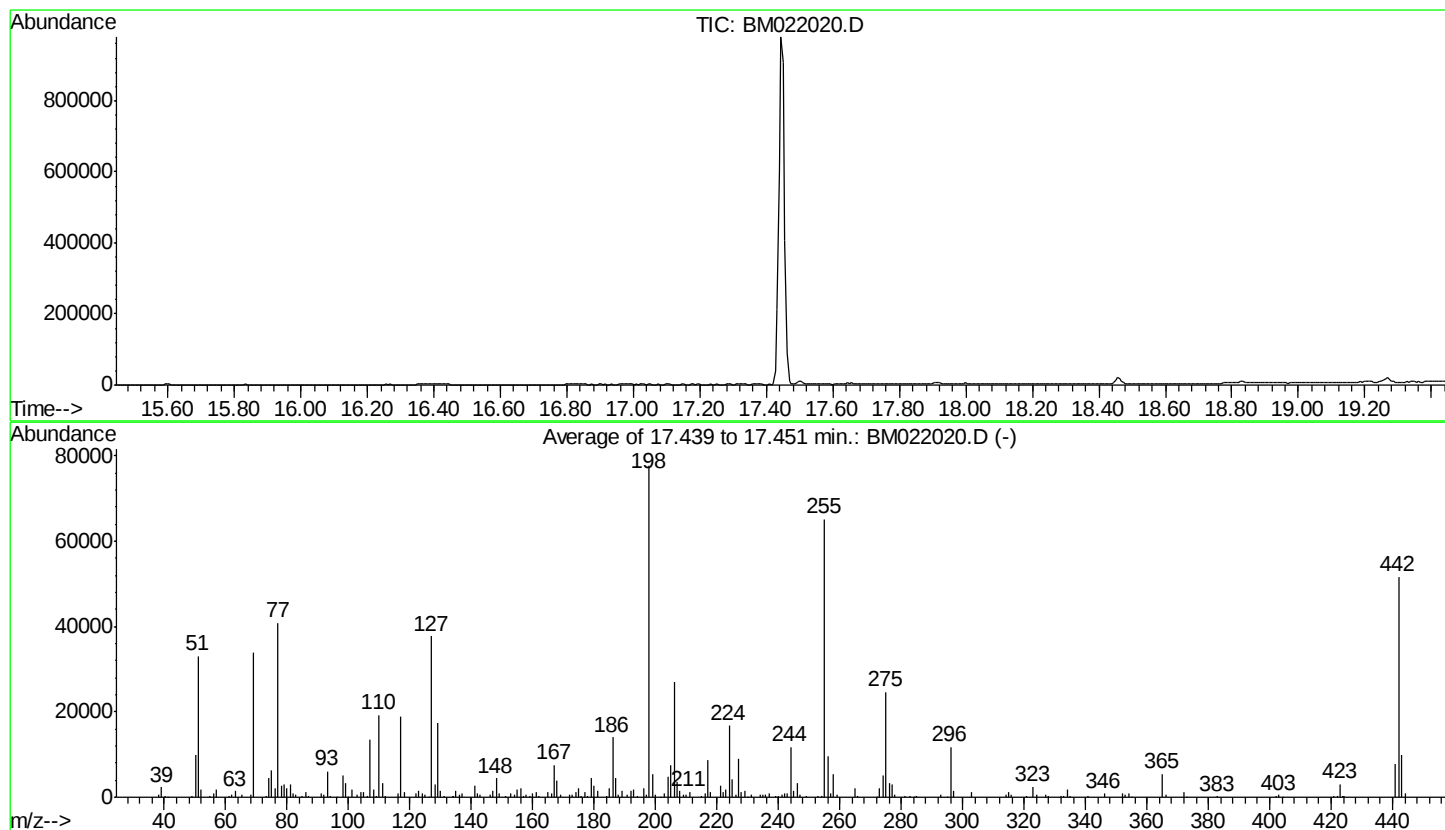

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	33093	PASS
68	69	0.00	2	1.9	632	PASS
69	198	0.00	100	43.6	33906	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	37738	PASS
197	198	0.00	2	0.8	630	PASS
198	198	100	100	100.0	77709	PASS
199	198	5	9	7.0	5471	PASS
275	198	10	60	31.8	24734	PASS
365	198	1	100	7.1	5488	PASS
441	198	0.01	100	10.2	7899	PASS
442	198	50	100	66.5	51677	PASS
443	442	15	24	19.0	9843	PASS

m/z	Abundance
44.00	779.0
73.00	453.0
206.90	662.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

m/z	Abundance
37.90	473.0
39.00	1950.0
40.10	340.0
44.00	746.0
49.10	300.0
50.10	8500.0
51.00	28560.0
52.00	1550.0
55.90	878.0
57.00	1543.0
61.00	418.0
62.00	555.0
63.00	1168.0
65.10	535.0
67.90	565.0
69.00	28632.0
72.90	636.0
74.00	3715.0
75.00	5458.0
76.10	1639.0
77.10	34624.0
78.00	2347.0
79.00	2676.0
80.00	1853.0
81.00	2513.0
82.00	660.0
83.00	504.0
84.90	421.0
86.00	955.0
86.90	325.0
91.00	648.0
91.90	577.0
93.00	4804.0
94.10	384.0
98.00	4147.0
99.00	2762.0
101.00	1512.0
102.90	355.0
104.00	953.0
105.00	1004.0
107.00	11306.0
108.00	1412.0
109.00	425.0
110.00	15438.0
111.00	2971.0
115.90	639.0
117.00	15427.0
118.00	1113.0
122.00	733.0
122.90	1334.0
123.90	599.0
125.00	443.0
127.00	30368.0
128.00	2380.0
129.00	14194.0
129.90	1156.0
130.90	402.0
133.90	409.0
135.00	1261.0
136.00	622.0
137.00	791.0
141.00	2370.0
142.00	737.0
142.80	384.0
146.00	393.0
147.00	1049.0
148.00	3126.0
149.00	633.0
152.90	750.0
154.00	523.0
155.00	1290.0
156.00	1791.0
157.90	464.0
158.90	314.0
159.90	840.0
161.00	1058.0
162.00	334.0
165.00	916.0
165.90	549.0
167.00	5700.0
168.00	3135.0
169.00	398.0
171.90	312.0
173.00	464.0
173.90	831.0
175.00	1583.0
175.90	365.0
176.90	948.0
178.00	330.0
178.90	3419.0
180.00	2144.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

181.00	949.0
185.00	1727.0
186.00	9946.0
187.00	3151.0
187.90	335.0
188.90	1223.0
190.90	535.0
192.00	1056.0
193.00	1373.0
194.00	365.0
195.90	1545.0
197.00	474.0
197.90	55968.0
198.90	4208.0
200.00	371.0
202.90	630.0
204.00	3227.0
205.00	5395.0
206.00	18560.0
207.00	3156.0
207.90	1092.0
209.00	571.0
210.00	405.0
210.90	870.0
214.90	322.0
215.90	538.0
216.90	6542.0
217.90	714.0
221.00	2113.0
221.90	797.0
222.90	1246.0
224.00	11900.0
225.00	2542.0
226.00	334.0
227.00	6273.0
228.00	858.0
229.00	1172.0
230.90	376.0
233.90	338.0
235.00	382.0
235.90	306.0
236.90	620.0
241.10	311.0
242.00	693.0
243.00	665.0
244.00	8049.0
245.00	1064.0
246.00	2316.0
246.90	520.0
248.90	347.0
252.90	372.0
255.00	43344.0
256.00	6589.0
257.00	627.0
258.00	3592.0
258.90	436.0
265.00	1210.0
272.90	1269.0
274.00	3489.0
275.00	15978.0
276.00	2308.0
276.90	2163.0
277.90	486.0
281.00	335.0
284.90	318.0
293.00	402.0
296.00	8207.0
296.90	959.0
303.00	735.0
313.90	367.0
314.90	825.0
315.90	462.0
323.00	1670.0
323.90	394.0
326.90	464.0
334.00	1197.0
335.00	353.0
346.00	483.0
351.90	556.0
353.00	332.0
354.10	424.0
365.00	3074.0
366.00	309.0
372.00	745.0
402.90	325.0
423.00	1546.0
423.90	458.0
441.00	3960.0
442.00	27056.0
443.00	5198.0
444.00	522.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

m/z	Abundance
38.00	475.0
39.00	2748.0
40.00	329.0
41.00	334.0
44.00	770.0
49.10	394.0
50.10	12235.0
51.00	39784.0
52.00	2191.0
55.00	352.0
56.00	1257.0
57.00	2401.0
61.00	624.0
62.00	671.0
63.00	1657.0
65.00	607.0
68.00	749.0
69.00	40576.0
73.00	912.0
74.00	5594.0
75.00	7417.0
76.10	2814.0
77.10	48072.0
78.10	3194.0
79.00	3706.0
80.00	2655.0
81.00	3564.0
82.00	999.0
82.90	814.0
84.90	505.0
85.90	1231.0
86.90	493.0
91.00	937.0
92.00	936.0
93.00	7473.0
94.00	435.0
96.00	305.0
98.00	5972.0
99.00	3950.0
99.90	307.0
100.90	2075.0
102.90	558.0
103.90	1493.0
105.00	1414.0
106.00	319.0
107.00	15985.0
108.00	2488.0
109.10	507.0
110.00	23352.0
111.00	3858.0
111.90	551.0
116.00	1229.0
117.00	21832.0
118.00	1374.0
121.90	1316.0
123.00	1656.0
123.90	899.0
124.90	731.0
126.10	314.0
127.00	43864.0
128.00	3264.0
129.00	20720.0
130.00	1681.0
131.00	454.0
134.10	672.0
135.00	1775.0
136.00	864.0
137.00	1201.0
141.00	3251.0
142.00	946.0
142.90	801.0
145.90	628.0
146.90	1780.0
148.00	5240.0
149.00	900.0
151.10	349.0
152.90	952.0
154.00	699.0
155.00	1931.0
156.00	2138.0
157.00	411.0
157.90	813.0
159.00	488.0
159.90	1104.0
161.00	1543.0
161.90	468.0
165.00	1475.0
166.00	931.0
167.00	8721.0
168.00	4757.0
169.00	619.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

171.90	521.0
173.00	719.0
174.00	1254.0
175.00	2721.0
176.00	654.0
177.00	1555.0
177.90	463.0
178.90	5358.0
180.00	3179.0
181.00	1923.0
183.90	459.0
185.00	2365.0
186.00	16832.0
187.00	5343.0
187.90	617.0
188.90	1367.0
190.90	700.0
192.00	1776.0
193.00	2005.0
194.00	381.0
196.00	2664.0
197.00	675.0
197.90	92712.0
198.90	6043.0
199.90	591.0
201.50	394.0
202.90	1308.0
204.00	5656.0
205.00	8774.0
206.00	32272.0
207.00	4767.0
207.90	1629.0
209.00	576.0
210.00	610.0
210.90	1335.0
214.90	546.0
216.00	1023.0
216.90	9913.0
217.90	1235.0
221.00	3254.0
221.90	1296.0
222.90	2125.0
224.00	18976.0
225.00	5223.0
226.00	729.0
227.00	10183.0
228.00	1441.0
228.90	1717.0
229.90	319.0
231.00	707.0
233.90	573.0
235.00	819.0
235.90	571.0
236.90	949.0
239.00	371.0
239.90	558.0
241.10	544.0
242.00	1197.0
242.90	1228.0
244.00	14303.0
245.00	1882.0
246.00	3734.0
247.00	857.0
248.90	460.0
254.00	532.0
255.00	76840.0
256.00	11414.0
257.00	787.0
258.00	6391.0
258.90	891.0
265.00	2597.0
265.90	430.0
272.10	325.0
273.00	2124.0
274.00	5954.0
275.00	29848.0
276.00	3813.0
277.00	3610.0
278.00	793.0
282.90	386.0
283.90	345.0
285.10	616.0
292.90	741.0
294.90	348.0
296.00	13533.0
297.00	1859.0
303.00	1211.0
314.00	562.0
315.00	1481.0
316.00	636.0
320.90	303.0
323.00	2814.0
323.90	570.0
326.90	894.0
327.90	358.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

m/z	Abundance
38.00	553.0
39.00	2464.0
44.00	805.0
49.20	315.0
50.10	8591.0
51.00	30936.0
52.00	1458.0
54.90	307.0
55.90	1023.0
56.90	1853.0
61.00	315.0
61.90	626.0
63.00	1358.0
65.00	694.0
68.00	584.0
69.00	32512.0
73.00	969.0
74.00	4161.0
75.00	5858.0
76.00	2129.0
77.00	39976.0
78.00	2455.0
79.00	3030.0
80.00	1992.0
81.00	3037.0
82.00	883.0
83.00	659.0
84.90	425.0
86.00	1121.0
87.00	459.0
91.00	770.0
91.90	760.0
93.00	6016.0
93.90	345.0
98.00	4912.0
99.00	3549.0
101.00	1695.0
102.90	679.0
103.90	1063.0
105.00	1177.0
105.90	381.0
107.00	13630.0
108.00	1760.0
108.90	350.0
110.00	19240.0
111.00	3336.0
111.90	517.0
115.90	749.0
117.00	19304.0
118.00	1325.0
122.00	1017.0
123.00	1559.0
124.00	902.0
125.00	569.0
127.00	38984.0
128.00	3038.0
129.00	17568.0
129.90	1775.0
131.10	311.0
133.80	482.0
135.00	1412.0
136.00	663.0
137.00	946.0
141.00	2740.0
142.00	956.0
142.90	537.0
145.90	500.0
147.00	1553.0
148.00	5071.0
149.00	758.0
150.90	355.0
152.90	849.0
153.90	920.0
155.00	1786.0
156.00	2098.0
156.90	387.0
158.00	706.0
158.90	516.0
160.00	810.0
160.90	1243.0
161.90	327.0
165.00	1033.0
166.00	896.0
167.00	8202.0
167.90	3589.0
168.90	536.0
172.00	626.0
172.90	657.0
174.00	1163.0
175.00	2466.0
175.80	346.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

177.00	1120.0
178.00	515.0
178.90	5104.0
179.90	2971.0
181.00	1647.0
184.00	440.0
185.00	2346.0
186.00	15473.0
187.00	4899.0
187.90	497.0
188.90	1559.0
190.90	546.0
192.00	1692.0
193.00	1968.0
193.90	390.0
195.90	2321.0
197.00	742.0
197.90	84448.0
198.90	6164.0
199.90	553.0
202.90	1005.0
204.00	5107.0
205.00	8755.0
206.00	29944.0
207.00	4677.0
208.00	1384.0
208.90	592.0
210.00	574.0
211.00	1421.0
214.90	495.0
216.00	923.0
216.90	9753.0
218.00	1262.0
220.90	3049.0
221.90	1152.0
223.00	2061.0
224.00	19232.0
225.00	4449.0
226.00	389.0
227.00	10243.0
228.00	1426.0
228.90	1937.0
231.00	661.0
234.00	620.0
234.90	665.0
235.90	523.0
237.00	841.0
238.90	421.0
239.90	335.0
240.90	526.0
241.90	1058.0
243.00	1228.0
244.00	13115.0
245.00	1885.0
246.00	3720.0
246.90	700.0
248.90	465.0
252.90	356.0
253.90	477.0
255.00	75384.0
256.00	10435.0
257.00	1052.0
258.00	6247.0
258.90	950.0
265.00	2971.0
265.90	351.0
273.00	2625.0
274.00	5773.0
275.00	28376.0
276.00	3617.0
277.00	3682.0
277.90	642.0
281.00	386.0
283.00	471.0
284.90	644.0
292.90	918.0
296.00	13402.0
297.00	1823.0
303.00	1304.0
313.90	631.0
314.90	1754.0
315.90	644.0
321.00	347.0
323.00	3007.0
324.00	515.0
326.90	796.0
328.00	383.0
332.00	345.0
333.00	325.0
334.00	2128.0
334.90	477.0
340.90	393.0
346.00	1042.0
352.00	946.0
353.10	577.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

354.00	1080.0
355.00	362.0
365.00	7113.0
366.00	847.0
372.00	1615.0
373.00	456.0
383.00	456.0
402.00	624.0
403.00	765.0
404.00	348.0
420.90	545.0
422.00	565.0
423.00	4373.0
424.10	885.0
441.00	11119.0
442.00	69664.0
443.00	13494.0
444.00	1029.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03

331.90	368.0
333.00	350.0
334.00	2336.0
335.00	515.0
341.00	463.0
346.00	887.0
351.90	864.0
353.00	587.0
354.00	806.0
365.00	6278.0
366.00	658.0
372.00	1460.0
382.90	407.0
401.90	593.0
403.00	539.0
421.00	716.0
422.10	525.0
423.00	3504.0
423.90	864.0
441.00	8618.0
442.00	58312.0
443.00	10838.0
444.00	1175.0

Instrument :
BNA_M
ClientSampleId :
DFTPP03