

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081220\
 Data File : BM027042.D
 Acq On : 12 Aug 2020 11:12
 Operator : JU/CG
 Sample : L3612-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBFM9

Quant Time: Aug 12 12:09:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 12 11:04:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	61017	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	214056	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	145307	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	310306	20.00	ng/ul	0.00
78) Chrysene-d12	21.21	240	366345	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	419043	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	7189	5.35	ng/uL	0.00
5) Phenol-d5	6.82	99	140252	29.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	98169	30.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	114462	30.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	112077	30.30	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	52526	30.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	53054	30.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	121600	32.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	144480	33.63	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	384136	33.15	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	469239	33.98	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	46816	23.93	ng/ul	0.00
58) Fluorene-d10	15.27	176	343789	34.04	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	44492	26.25	ng/ul	0.00
71) Anthracene-d10	17.12	188	546913	35.78	ng/ul	0.00
79) Pyrene-d10	19.42	212	640746	35.07	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	813693	34.79	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.73	163	85193	7.016	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081220\
Data File : BM027042.D
Acq On : 12 Aug 2020 11:12
Operator : JU/CG
Sample : L3612-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBFM9

Quant Time: Aug 12 12:09:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 12 11:04:55 2020
Response via : Initial Calibration

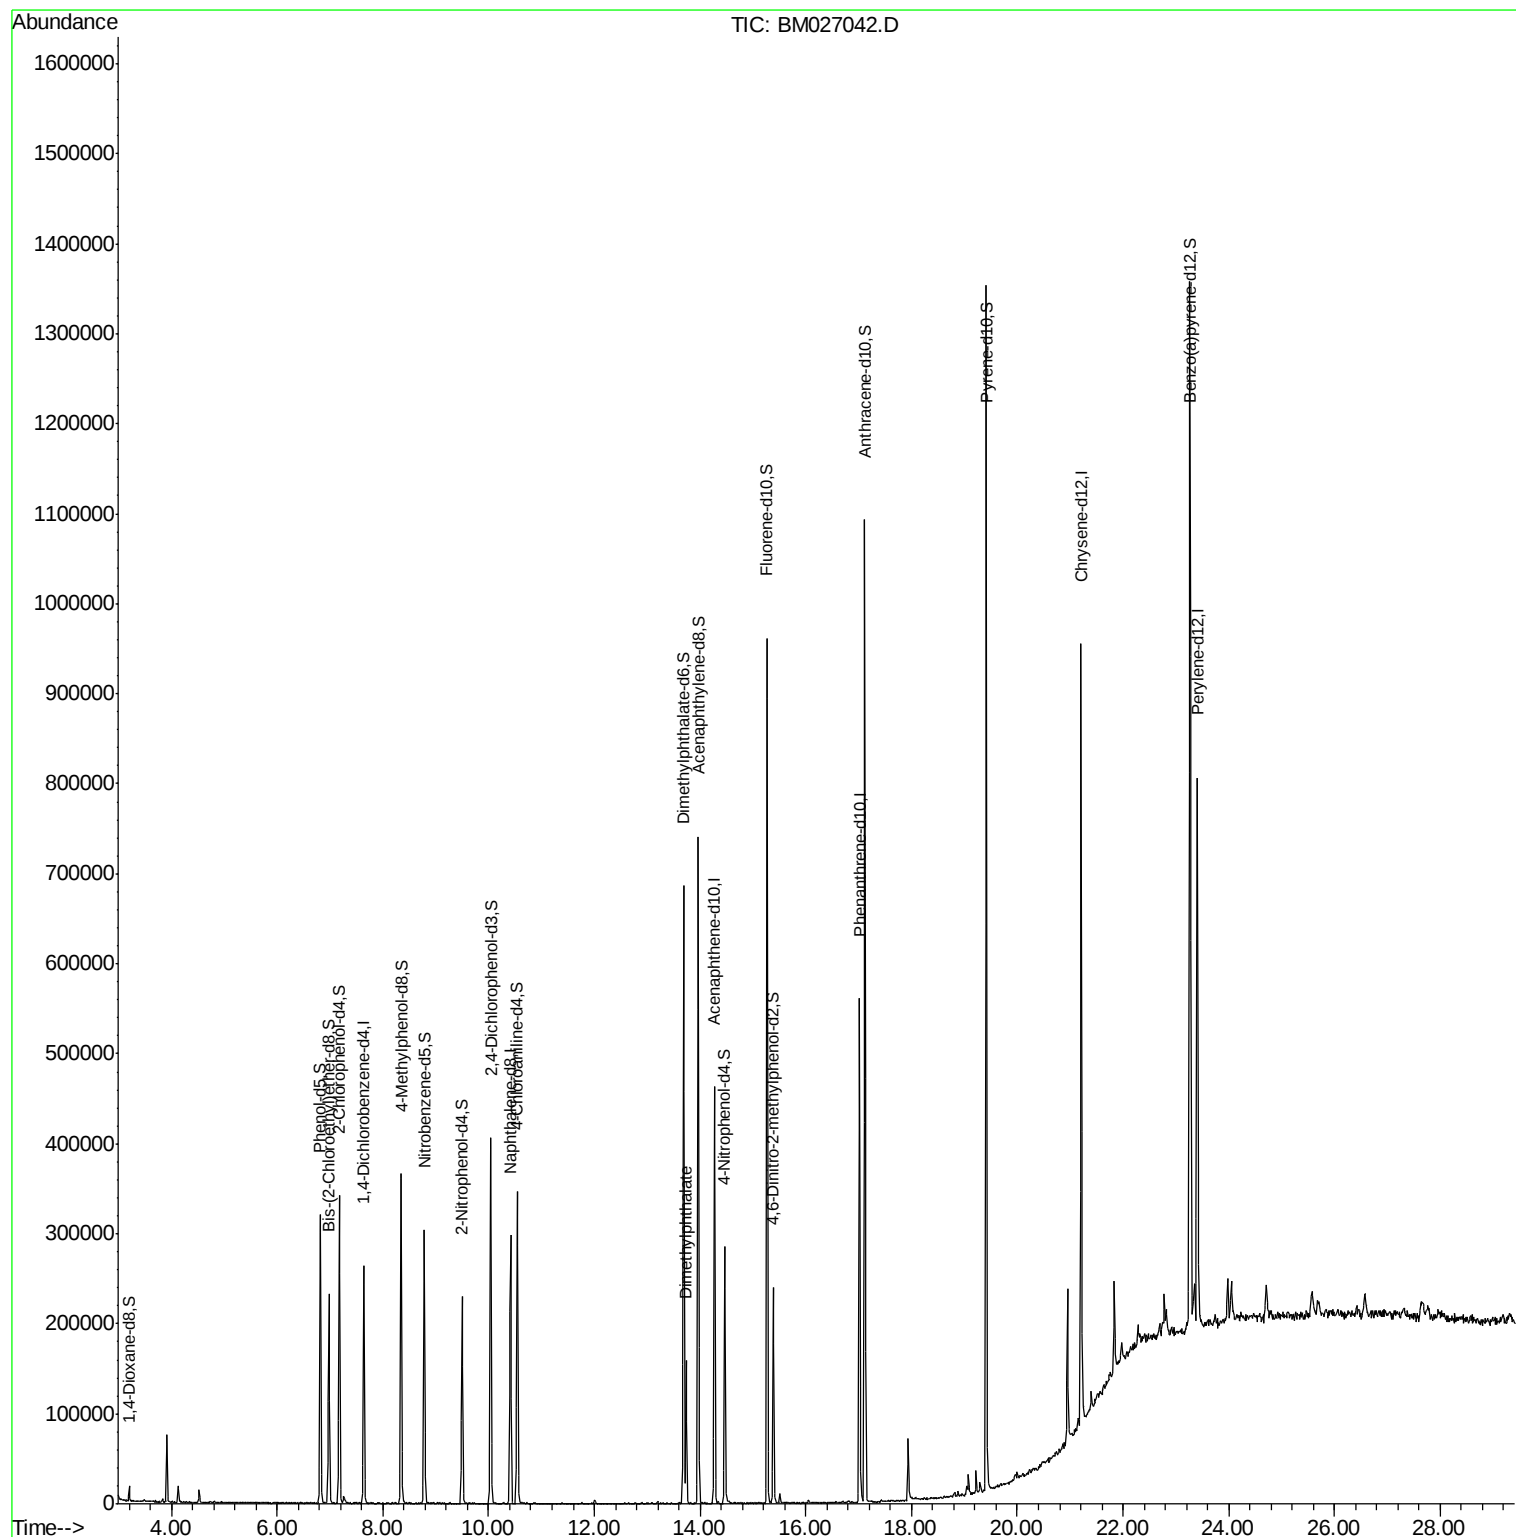

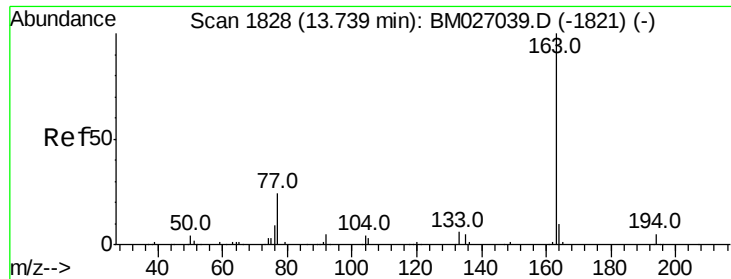

#45

Dimethylphthalate

Concen: 7.016 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. -0.01 min

Lab File: BM027042.D

Acq: 12 Aug 2020 11:12

Instrument :

BNA_M

ClientSampleId :

DBFM9


Tot Ion:163 Resp: 85193

Ion Ratio Lower Upper

163 100

194 4.4 3.2 4.8

164 9.6 8.2 12.2

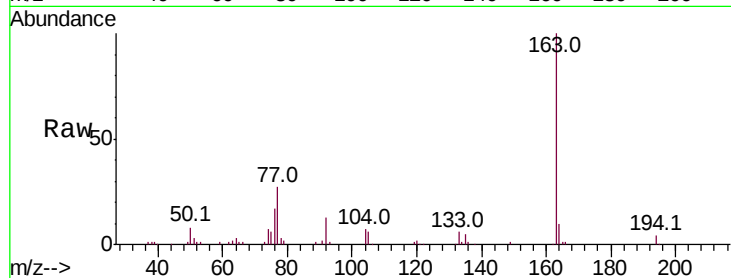

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

