

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081220\
 Data File : BM027046.D
 Acq On : 12 Aug 2020 13:39
 Operator : JU/CG
 Sample : L3612-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBFN0

Quant Time: Aug 12 14:10:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 12 11:04:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	99999	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	355804	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	221342	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	469262	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	492496	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	526706	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	4913	2.23	ng/uL	0.00
5) Phenol-d5	6.82	99	93022	11.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	74245	13.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	79069	12.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	74520	12.29	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	36591	12.98	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	33892	11.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	77748	12.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	90254	12.64	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	252096	14.28	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	274763	13.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	22258	7.47	ng/ul	0.00
58) Fluorene-d10	15.27	176	206067	13.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	22965	8.96	ng/ul	0.00
71) Anthracene-d10	17.12	188	308335	13.34	ng/ul	0.00
79) Pyrene-d10	19.42	212	334865	13.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	384544	13.08	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	55231	2.986	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081220\
Data File : BM027046.D
Acq On : 12 Aug 2020 13:39
Operator : JU/CG
Sample : L3612-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBFN0

Quant Time: Aug 12 14:10:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 12 11:04:55 2020
Response via : Initial Calibration

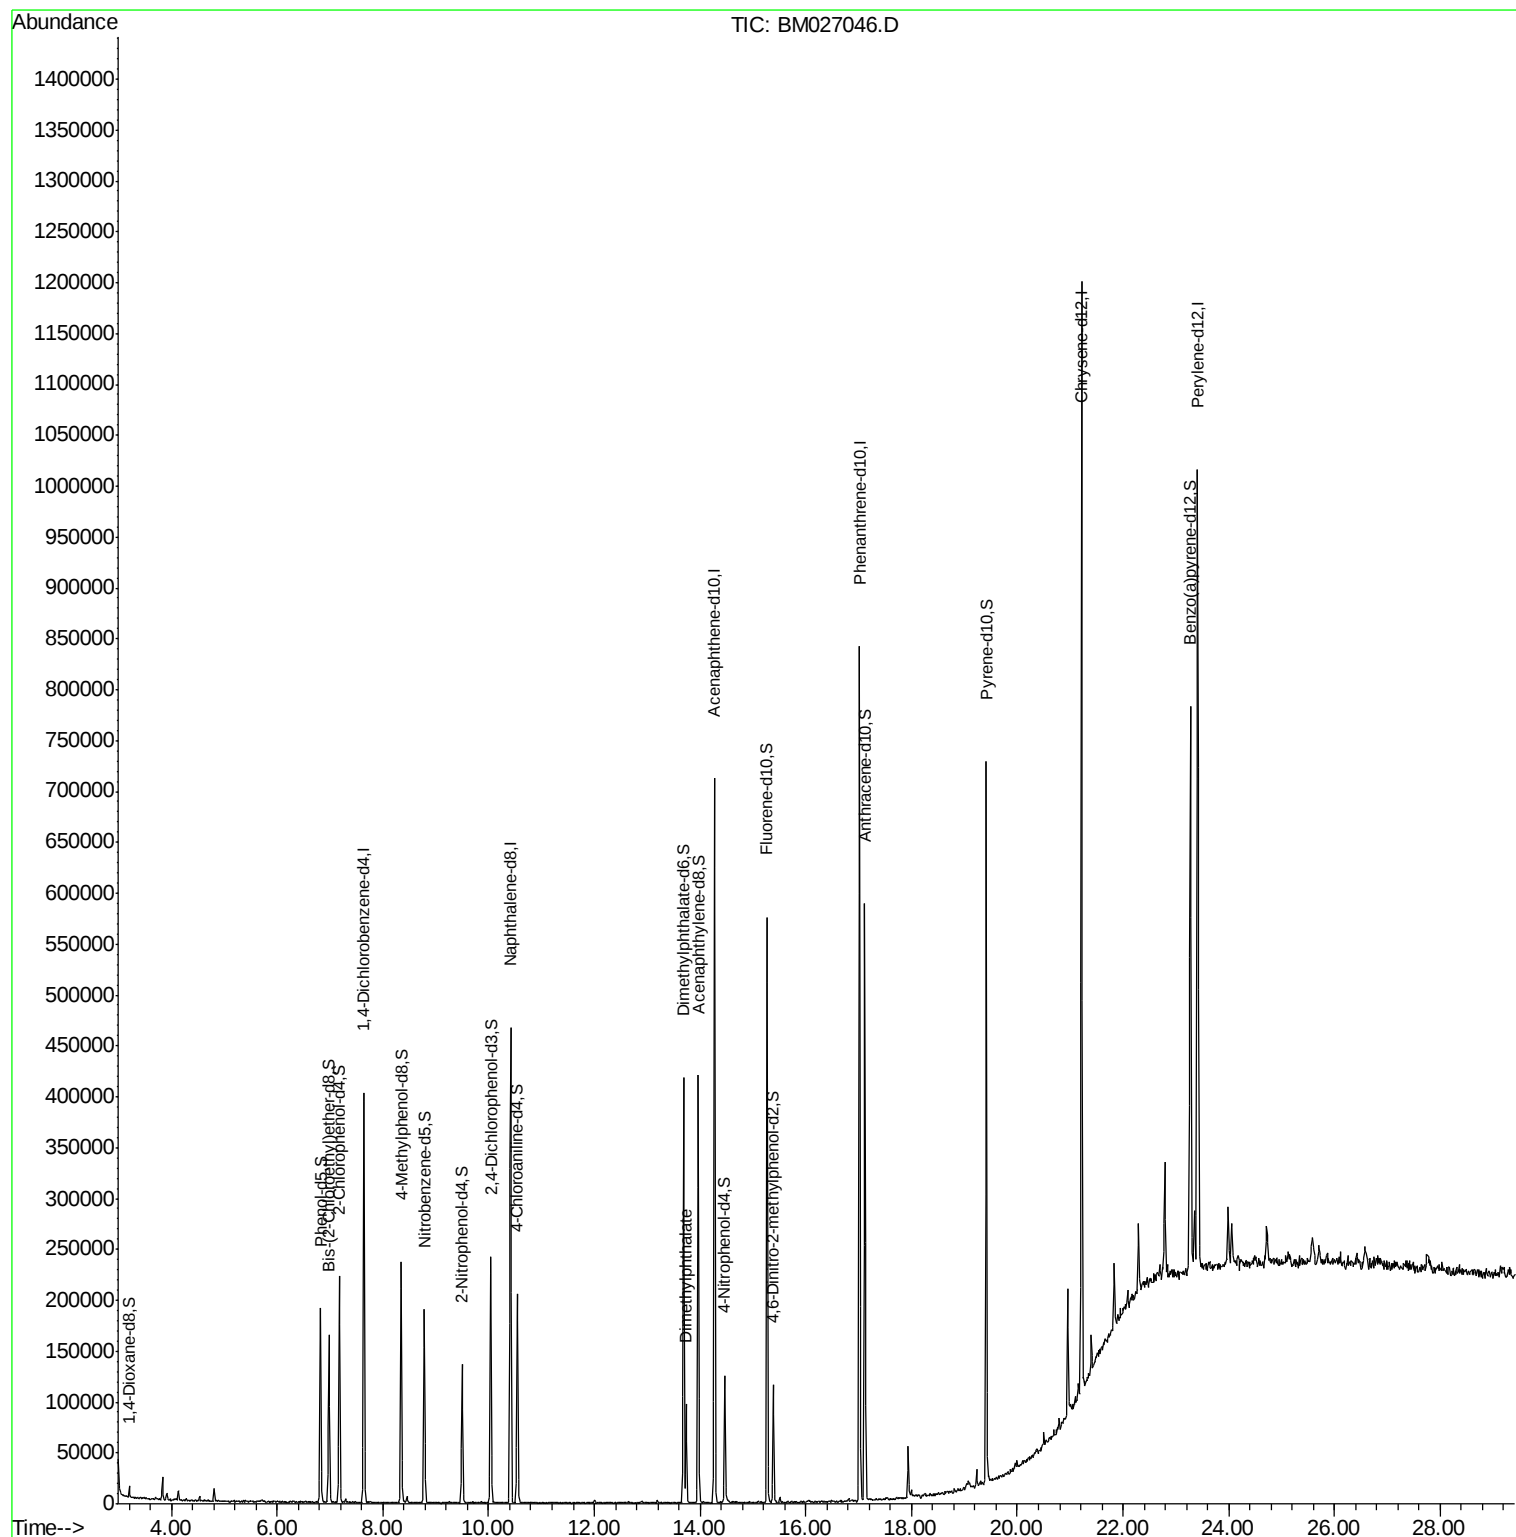

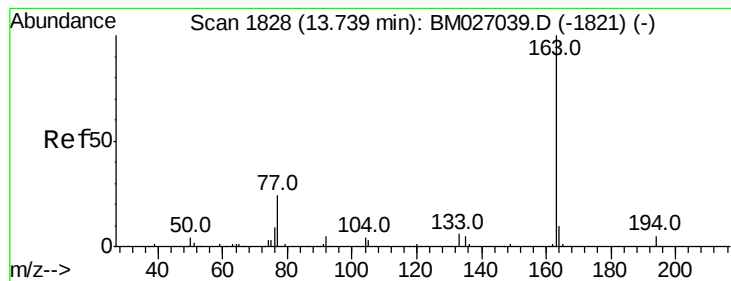

#45

Dimethylphthalate

Concen: 2.986 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. -0.01 min

Lab File: BM027046.D

Acq: 12 Aug 2020 13:39

Instrument :

BNA_M

ClientSampleId :

DBFN0


Tot Ion:163 Resp: 55231

Ion Ratio Lower Upper

163 100

194 4.6 3.2 4.8

164 10.5 8.2 12.2

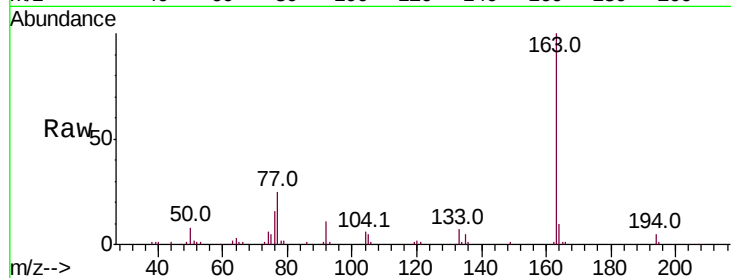

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

