

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081220\
 Data File : BM027048.D
 Acq On : 12 Aug 2020 14:53
 Operator : JU/CG
 Sample : L3612-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBFN4

Quant Time: Aug 12 15:52:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 12 11:04:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	102229	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	370014	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	225667	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	467866	20.00	ng/ul	0.00
78) Chrysene-d12	21.22	240	487685	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	518052	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	4865	2.16	ng/uL	0.00
5) Phenol-d5	6.82	99	87751	11.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	71922	13.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	72551	11.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	69136	11.16	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	33702	11.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	33071	10.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	70992	11.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	82337	11.09	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	242768	13.49	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	248071	11.57	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	23317	7.68	ng/ul	0.00
58) Fluorene-d10	15.27	176	187110	11.93	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	22786	8.92	ng/ul	0.00
71) Anthracene-d10	17.12	188	266629	11.57	ng/ul	0.00
79) Pyrene-d10	19.42	212	301671	12.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	333065	11.52	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.74	163	70270	3.726	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081220\
Data File : BM027048.D
Acq On : 12 Aug 2020 14:53
Operator : JU/CG
Sample : L3612-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBFN4

Quant Time: Aug 12 15:52:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 12 11:04:55 2020
Response via : Initial Calibration

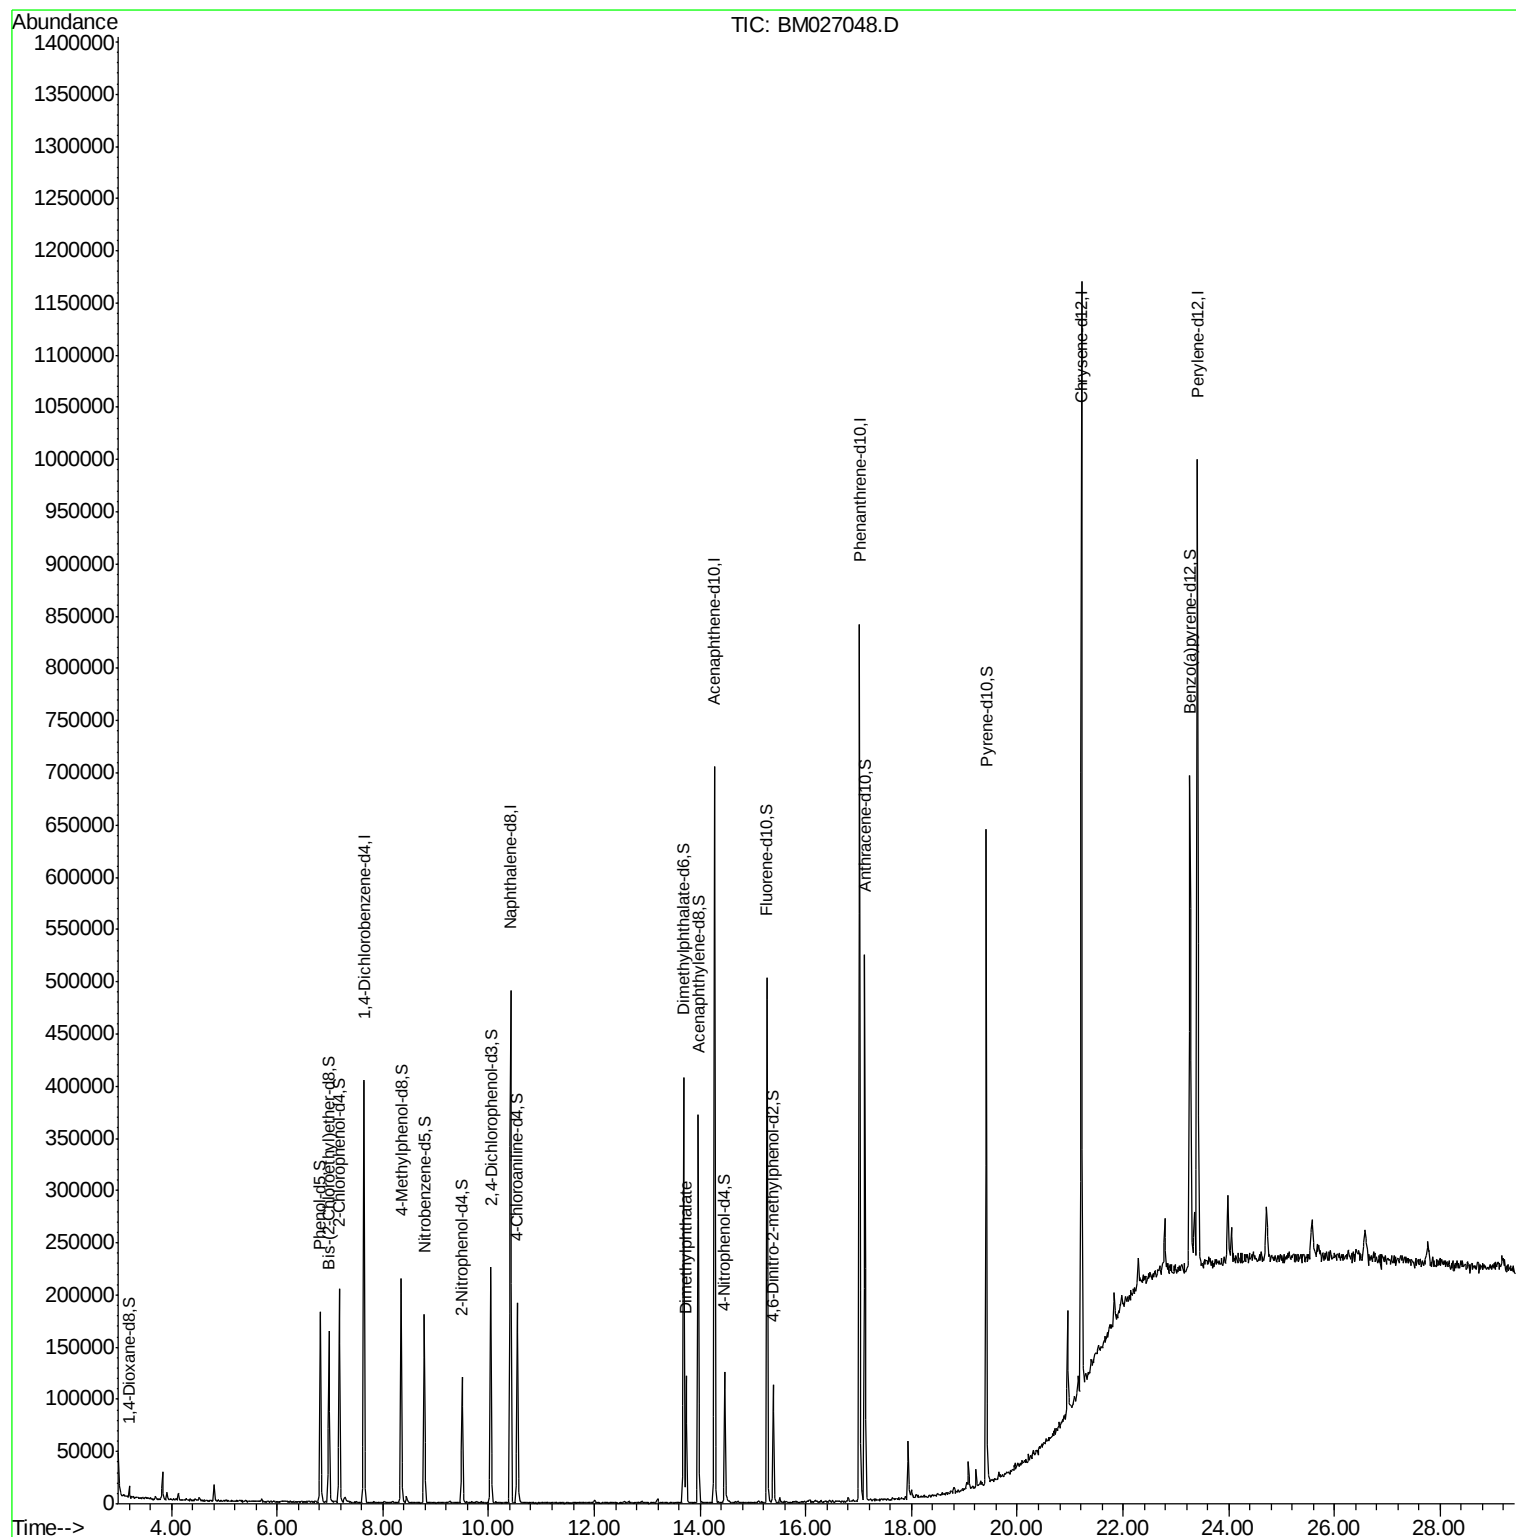

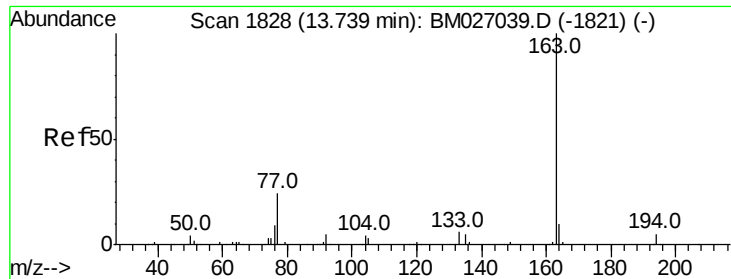

#45

Dimethylphthalate

Concen: 3.726 ng/ul

RT: 13.74 min Scan# 1828

Delta R.T. -0.00 min

Lab File: BM027048.D

Acq: 12 Aug 2020 14:53

Instrument :

BNA_M

ClientSampleId :

DBFN4


Tot Ion:163 Resp: 70270

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 9.3 8.2 12.2

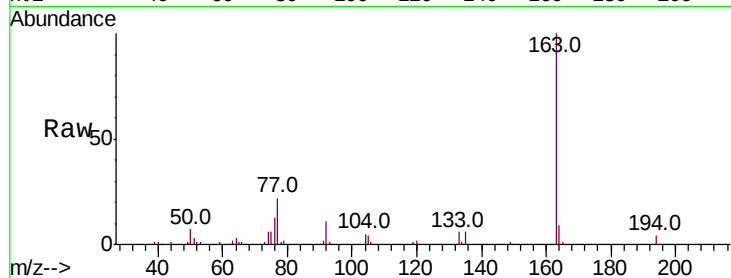

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

