


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081224\
Data File : BM047150.D
Acq On : 12 Aug 2024 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Aug 11 23:47:58 2024

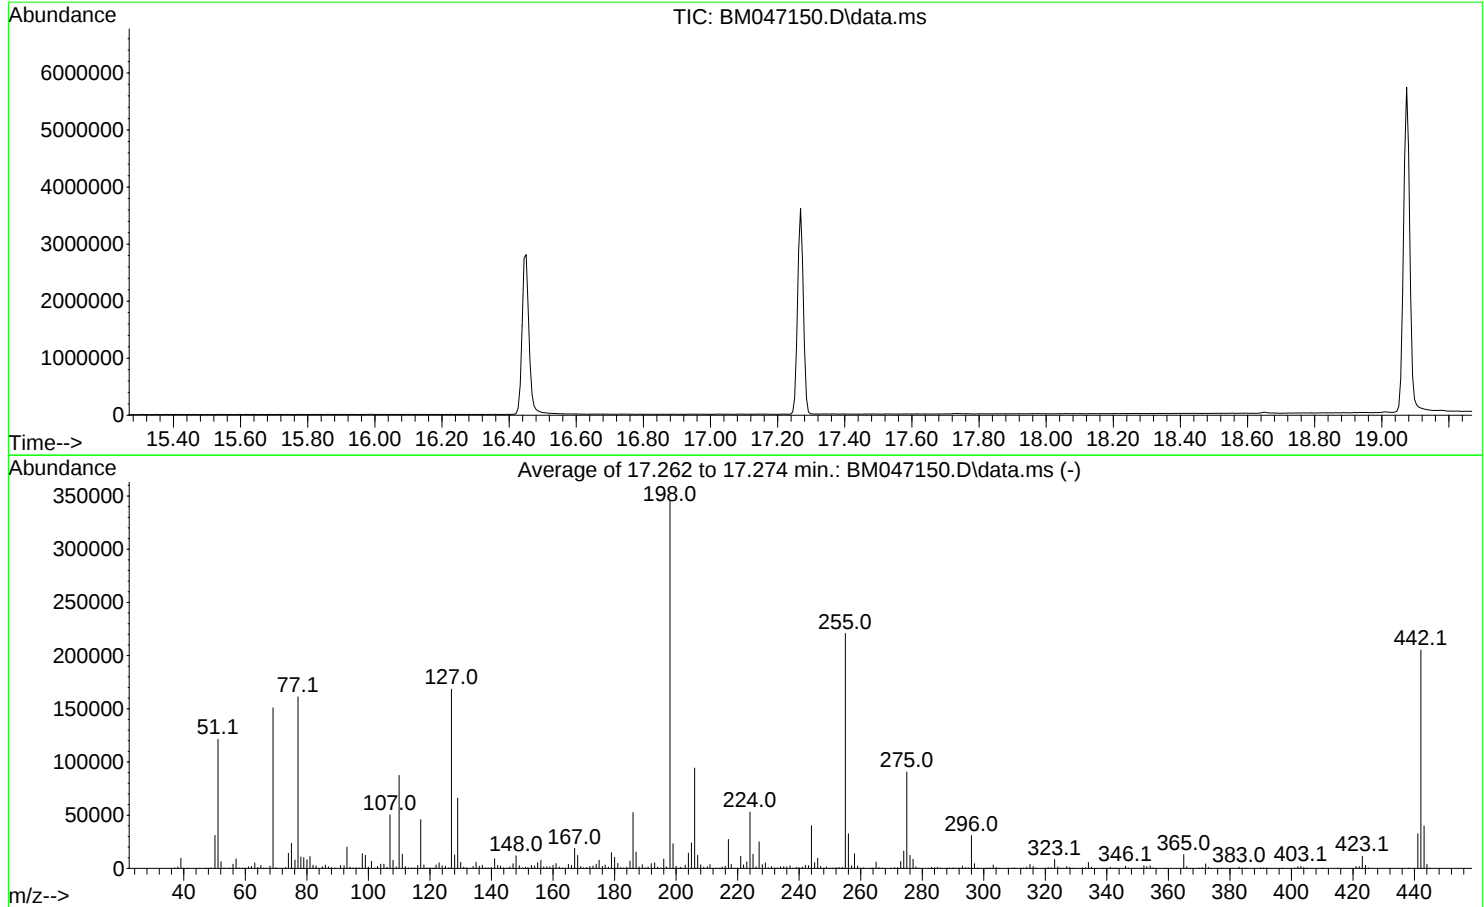




AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	121409	PASS
68	69	0.00	2	1.4	2125	PASS
69	198	0.00	100	43.6	150843	PASS
70	69	0.00	2	0.4	666	PASS
127	198	10	80	48.7	168405	PASS
197	198	0.00	2	0.4	1463	PASS
198	198	100	100	100.0	345792	PASS
199	198	5	9	6.7	23141	PASS
275	198	10	60	26.2	90501	PASS
365	198	1	100	3.8	12971	PASS
441	198	0.01	100	9.4	32568	PASS
442	442	50	100	100.0	205376	PASS
443	442	15	24	19.4	39891	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081224\
Data File : BM047150.D
Acq On : 12 Aug 2024 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 12 12:04:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

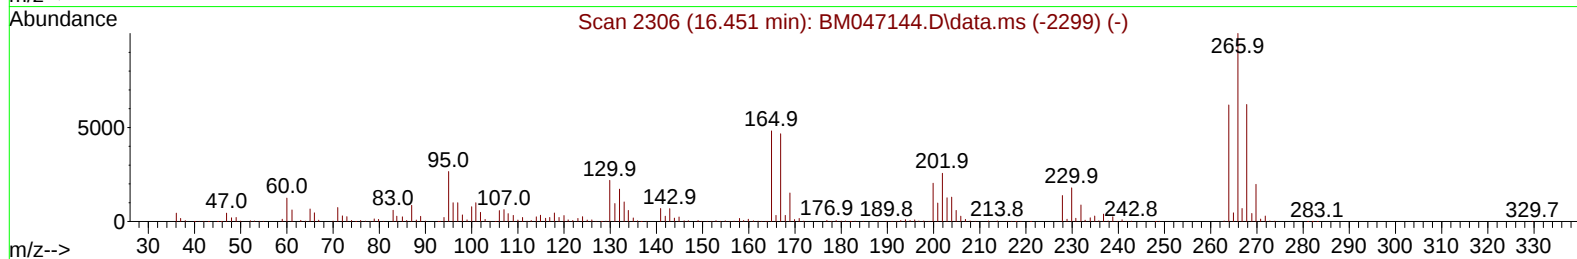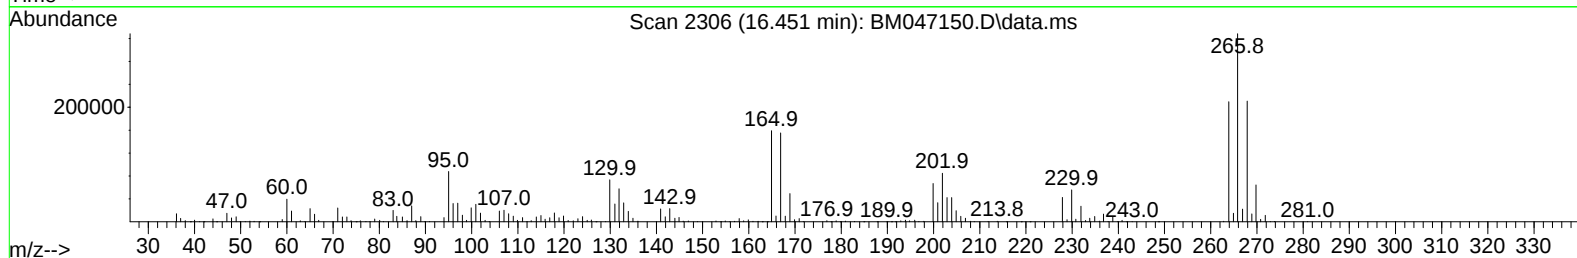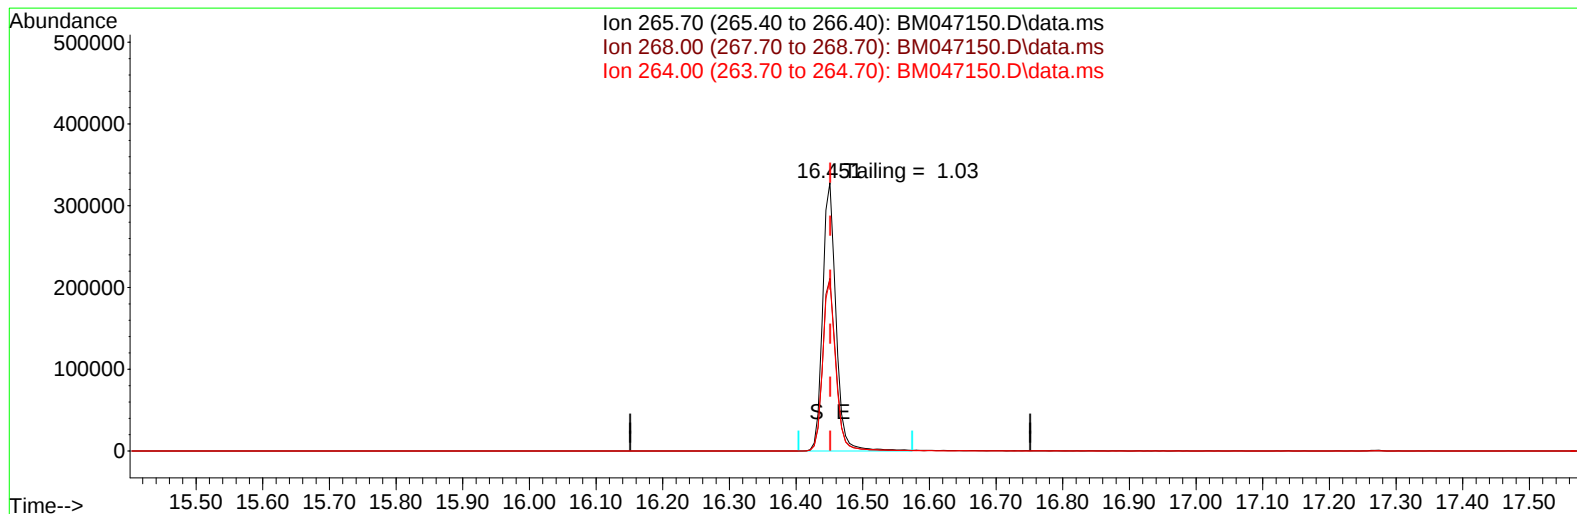

TIC: BM047150.D\data.ms

(70) Pentachlorophenol (C)

16.451min (-0.000) 0.00 ng




response 457600

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.23
264.00	62.00	63.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM081224\
Data File : BM047150.D
Acq On : 12 Aug 2024 10:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 12 12:04:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM081024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 11 23:47:58 2024
Response via : Initial Calibration

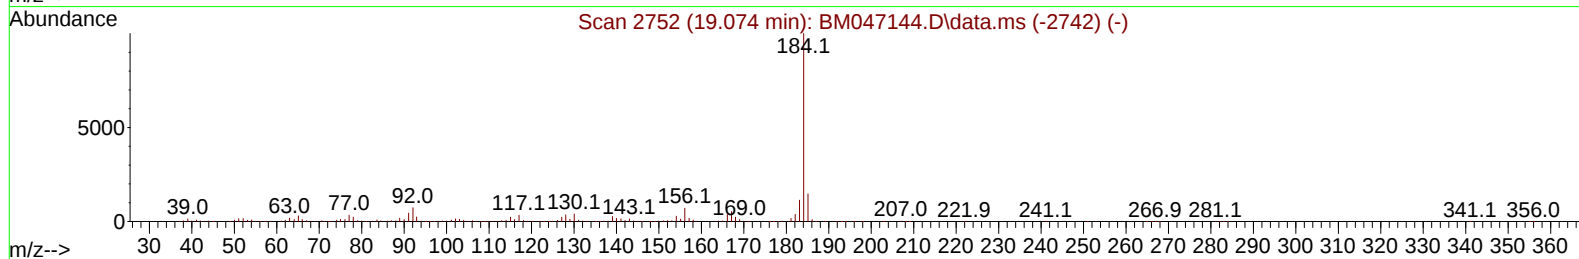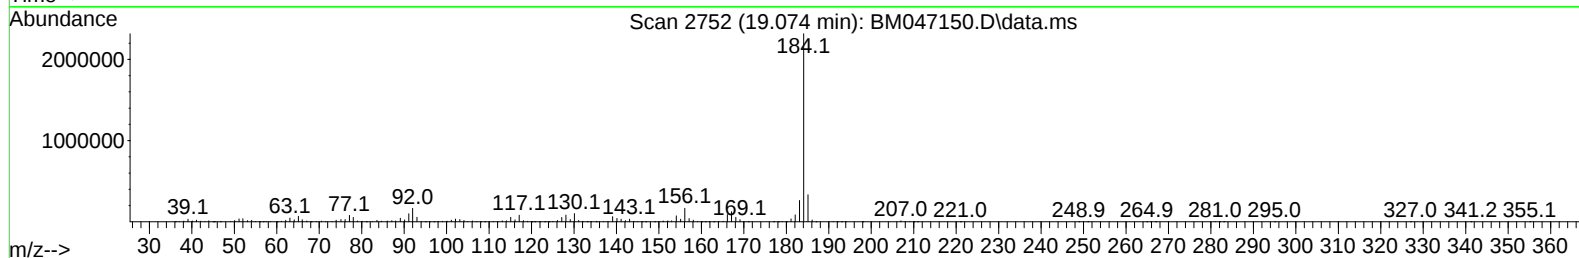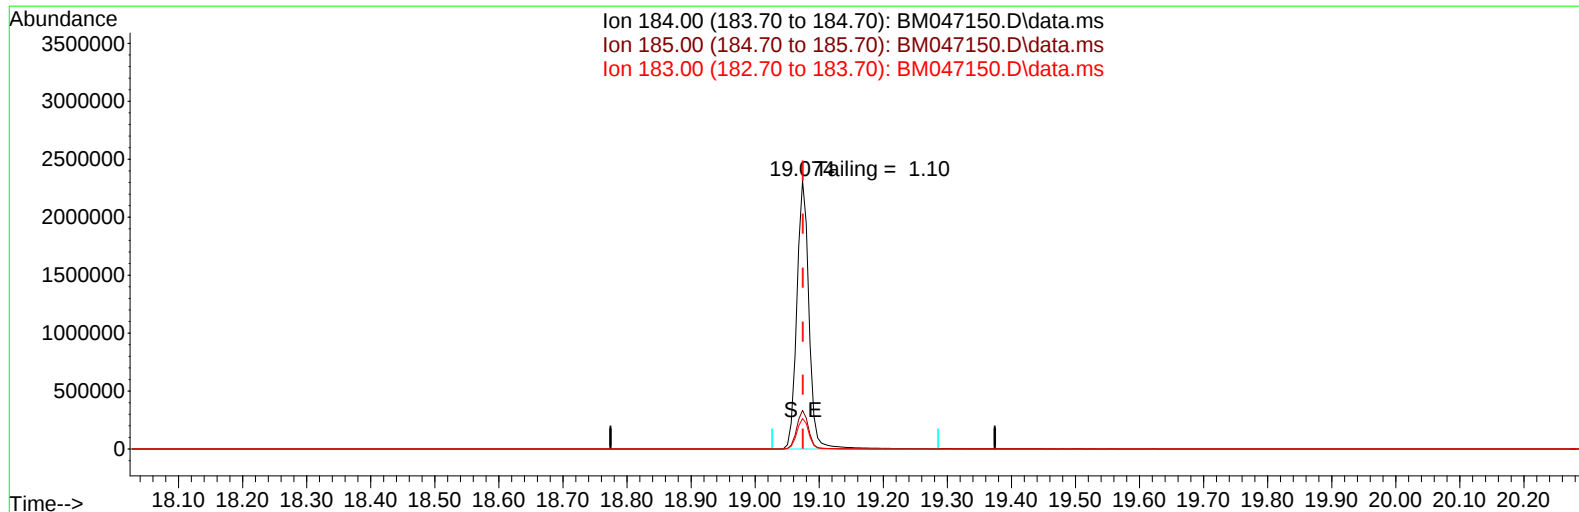

TIC: BM047150.D\data.ms

(77) Benzidine

19.074min (-0.000) 1383520.43 ng

response 3073571

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.42
183.00	11.30	11.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/12/2024	BNA_M	<u>BM047150.D</u>
Compound Name	Response	Retention Time
DDT	1324125	20.321
DDD	16577	19.927
DDE	1314	19.362
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17891	1342016	1.33

Instrument :
BNA_M
ClientSampleId :
DFTPP