

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
 Data File : BM007064.D
 Acq On : 13 Aug 2016 11:56
 Operator : UM/SJ
 Sample : H4389-13
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PR002-SS006-1218-01

Quant Time: Aug 15 10:20:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 00:47:53 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	252649	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	974141	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	563904	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.18	188	1332933	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1703900	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	1784798	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	25124	4.34	ng/uL	0.00
5) Phenol-d5	6.97	99	476079	23.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	282926	24.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	391265	24.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	379005	22.50	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	186541	26.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	204451	27.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	392000	24.76	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	431578	22.91	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	1255859	26.95	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1543112	27.57	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	169305	20.27	ng/ul	0.00
57) Fluorene-d10	15.43	176	1106027	27.16	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	161086	21.87	ng/ul	-0.01
70) Anthracene-d10	17.28	188	1769862	28.66	ng/ul	0.00
76) Pyrene-d10	19.57	212	2095640	29.14	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	2378174	29.13	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.90	163	939890	20.18	ng/ul	99
45) 2,6-Dinitrotoluene	13.90	165	10076	1.11	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007064.D
Acq On : 13 Aug 2016 11:56
Operator : UM/SJ
Sample : H4389-13
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PR002-SS006-1218-01

Quant Time: Aug 15 10:20:03 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 00:47:53 2016
Response via : Initial Calibration

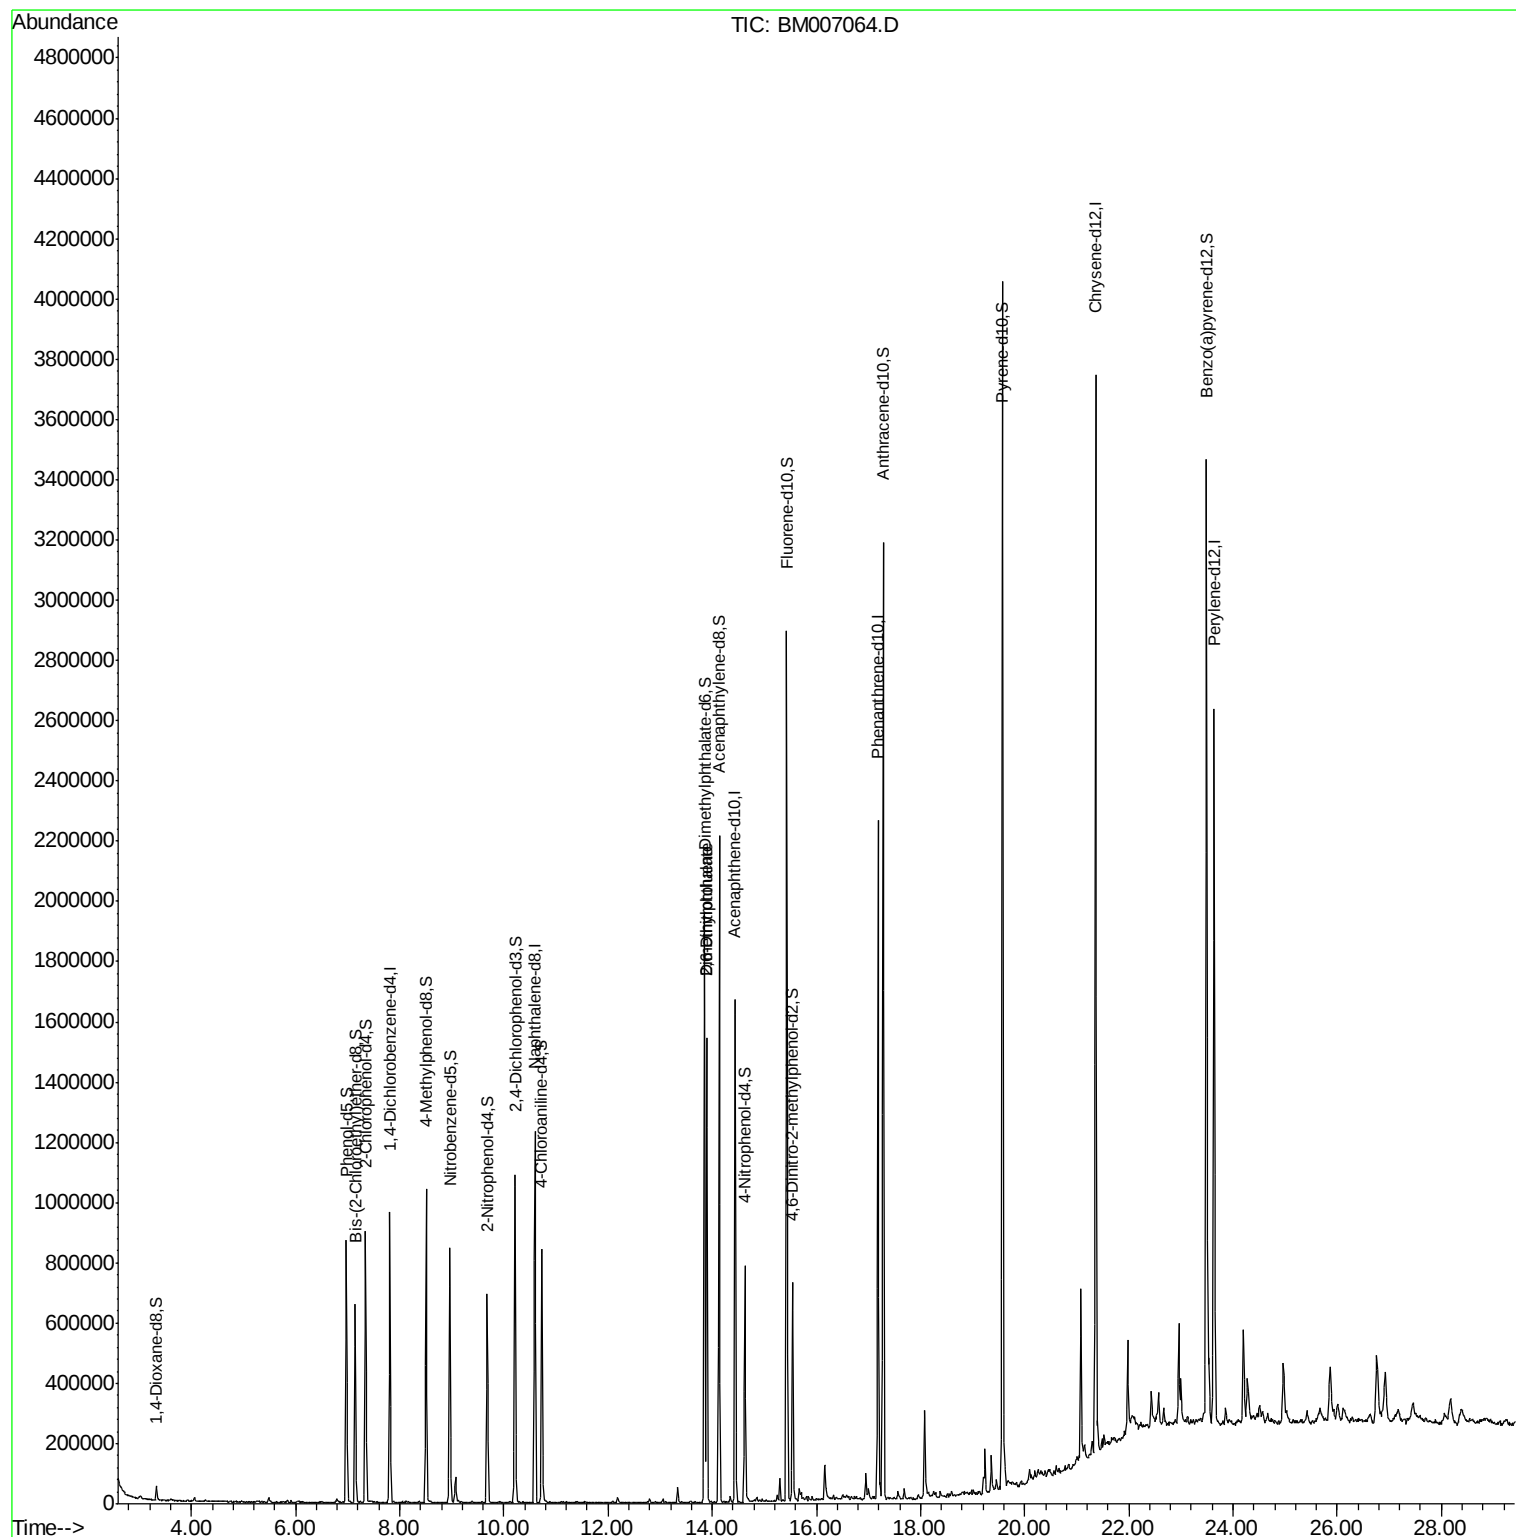

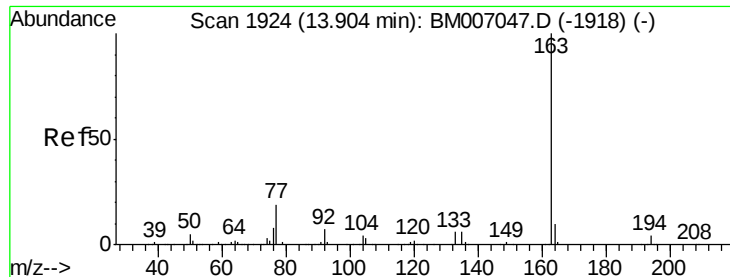

#44

Dimethylphthalate

Concen: 20.18 ng/ul

RT: 13.90 min Scan# 1923

Delta R.T. -0.01 min

Lab File: BM007064.D

Acq: 13 Aug 2016 11:56

Instrument :

BNA_M

ClientSampleId :

PR002-SS006-1218-01


Tgt Ion:163 Resp: 939890

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2




164 10.1 7.8 11.8

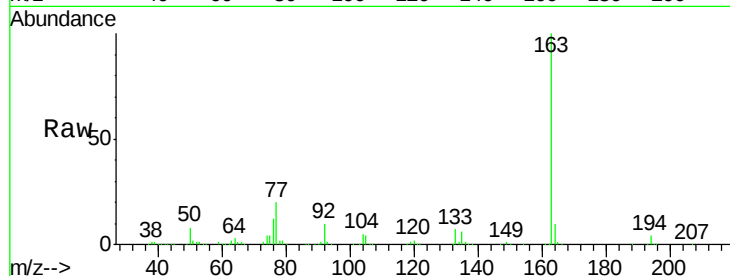

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

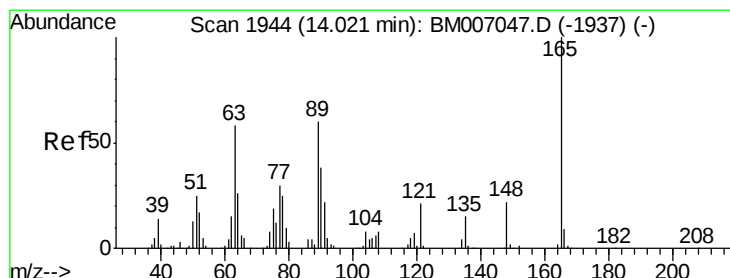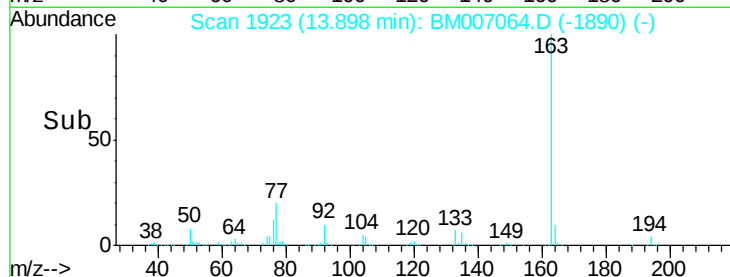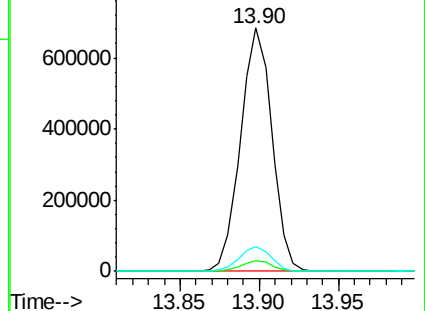

#45

2,6-Dinitrotoluene

Concen: 1.11 ng/ul

RT: 13.90 min Scan# 1923

Delta R.T. -0.12 min

Lab File: BM007064.D

Acq: 13 Aug 2016 11:56


Tgt Ion:165 Resp: 10076

Ion Ratio Lower Upper

165 100

89 14.6 46.6 69.8#

121 28.2 16.0 24.0#

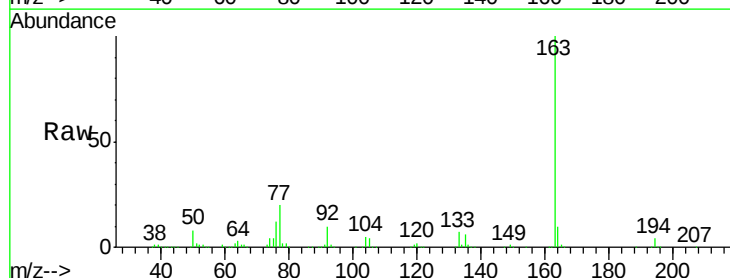

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM

Ion 121.00 (120.70 to 121.70): E

