

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
 Data File : BM007065.D
 Acq On : 13 Aug 2016 12:33
 Operator : UM/SJ
 Sample : H4389-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PR002-SS006-2430-01

Quant Time: Aug 15 10:20:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 00:47:53 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	235848	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	936486	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	560323	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1340356	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1697625	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	1775419	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	11522	2.13	ng/uL	0.00
5) Phenol-d5	6.97	99	226859	11.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	137348	12.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	186789	12.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	174677	11.11	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	89694	13.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	98343	13.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	191231	12.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	222330	12.28	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	668008	14.43	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	796961	14.33	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	94486	11.39	ng/ul	0.00
57) Fluorene-d10	15.43	176	591144	14.61	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	80425	10.86	ng/ul	-0.01
70) Anthracene-d10	17.28	188	955774	15.39	ng/ul	0.00
76) Pyrene-d10	19.57	212	1162932	16.23	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	1275135	15.70	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.90	163	592582	12.81	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007065.D
Acq On : 13 Aug 2016 12:33
Operator : UM/SJ
Sample : H4389-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PR002-SS006-2430-01

Quant Time: Aug 15 10:20:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 00:47:53 2016
Response via : Initial Calibration

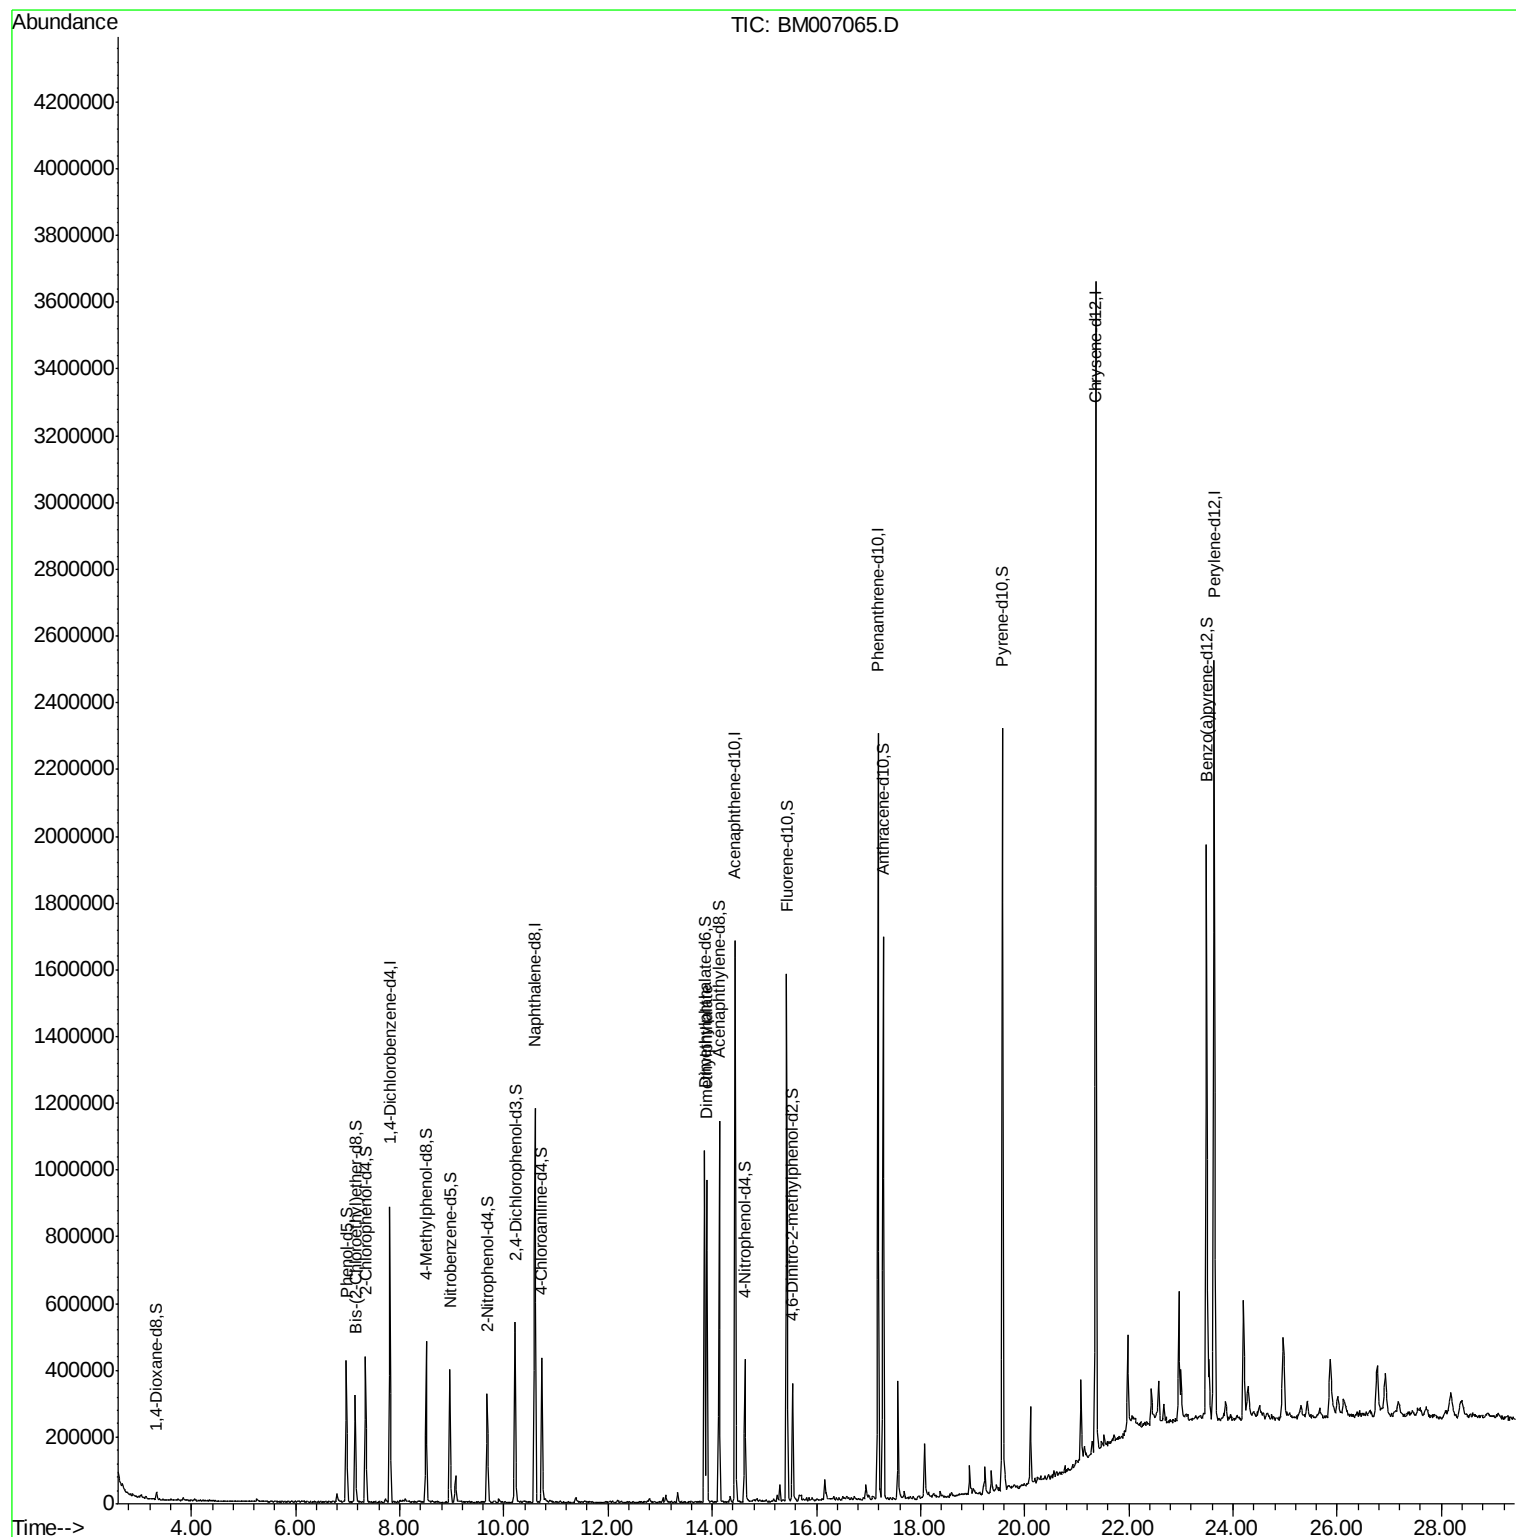

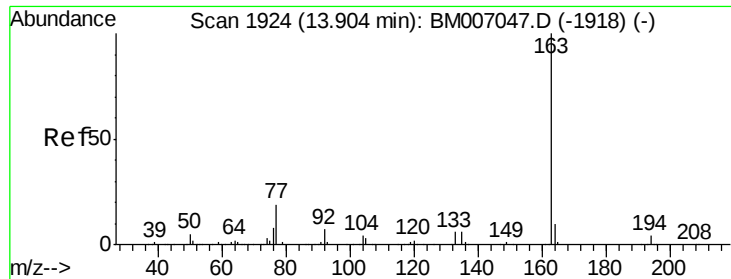

#44

Dimethylphthalate

Concen: 12.81 ng/ul

RT: 13.90 min Scan# 1923

Delta R.T. -0.01 min

Lab File: BM007065.D

Acq: 13 Aug 2016 12:33

Instrument :

BNA_M

ClientSampleId :

PR002-SS006-2430-01


Tgt Ion:163 Resp: 592582

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 10.0 7.8 11.8

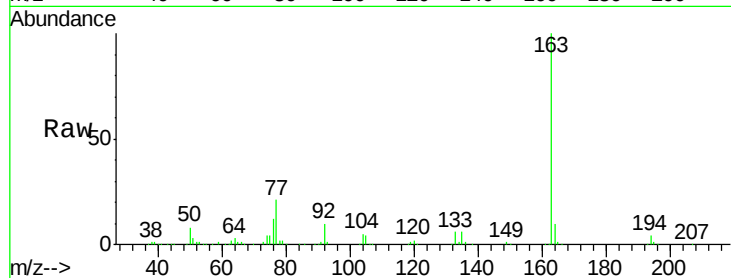

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

