

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
 Data File : BM007075.D
 Acq On : 13 Aug 2016 18:39
 Operator : UM/SJ
 Sample : H4314-04
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJT3

Quant Time: Aug 15 10:21:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 00:47:53 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	227644	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	938955	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	566480	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1344385	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1733808	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	1837098	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	20396	3.91	ng/uL	0.00
5) Phenol-d5	6.97	99	410304	22.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	240147	22.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	340589	23.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	328776	21.67	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	153743	22.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	172640	23.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	336324	22.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	412338	22.71	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	1091849	23.33	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1289074	22.93	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	135590	16.16	ng/ul	0.00
57) Fluorene-d10	15.43	176	953563	23.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	115409	15.53	ng/ul	-0.01
70) Anthracene-d10	17.28	188	1503338	24.14	ng/ul	0.00
76) Pyrene-d10	19.57	212	1888482	25.81	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	2150758	25.60	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.90	163	488106	10.43	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007075.D
Acq On : 13 Aug 2016 18:39
Operator : UM/SJ
Sample : H4314-04
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT3

Quant Time: Aug 15 10:21:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 00:47:53 2016
Response via : Initial Calibration

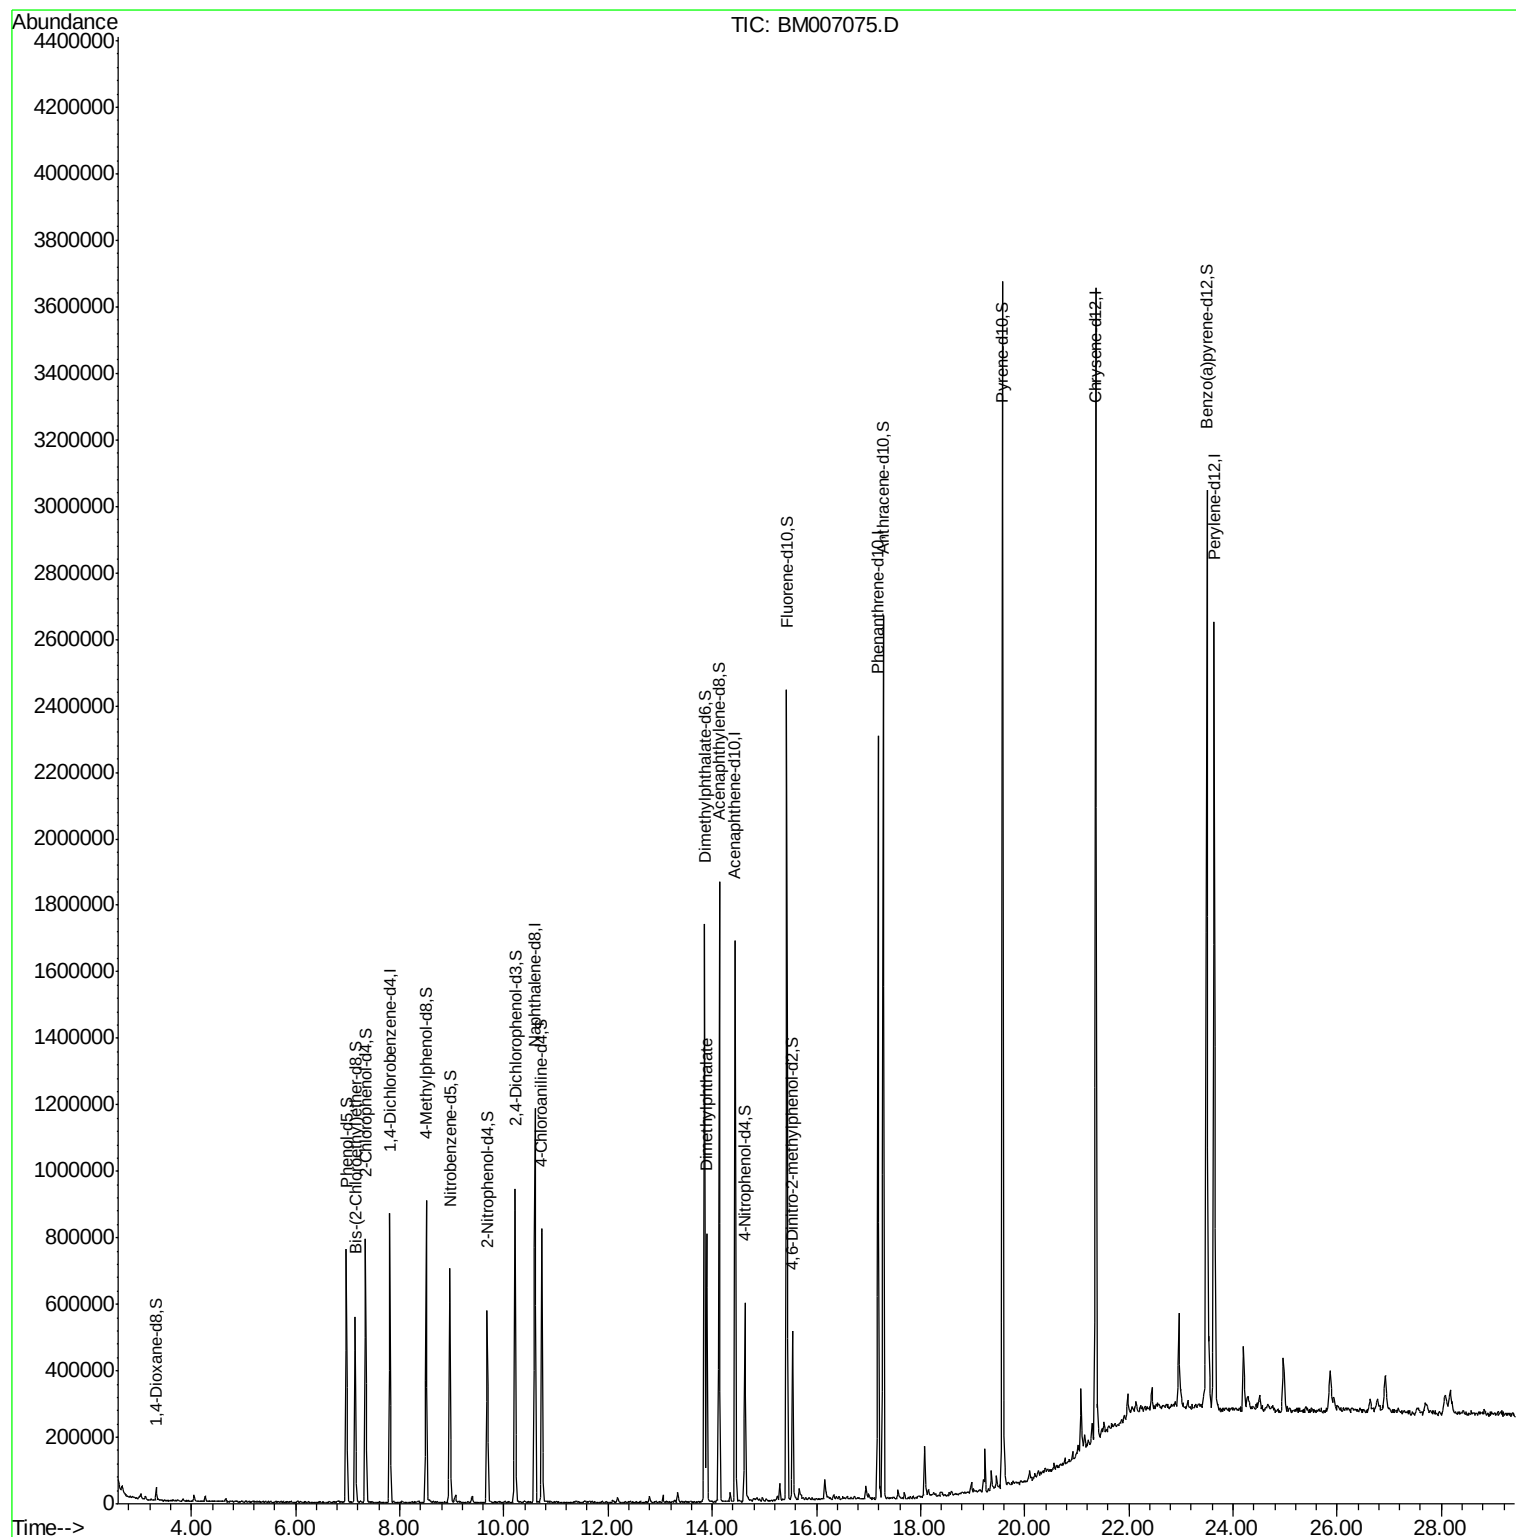


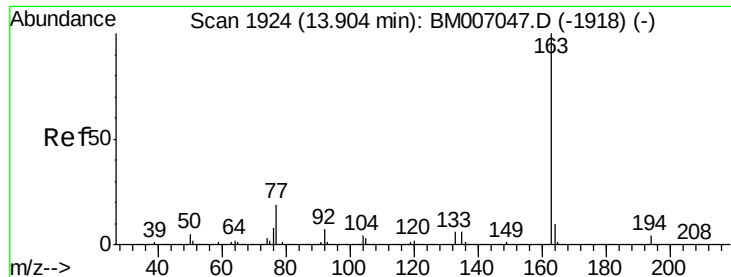

#44
 Dimethylphthalate
 Concen: 10.43 ng/ul
 RT: 13.90 min Scan# 1923
 Delta R.T. -0.01 min
 Lab File: BM007075.D
 Acq: 13 Aug 2016 18:39

Instrument :
 BNA_M
 ClientSampleId :
 BDJT3

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.4	5.2
164	9.8	7.8	11.8

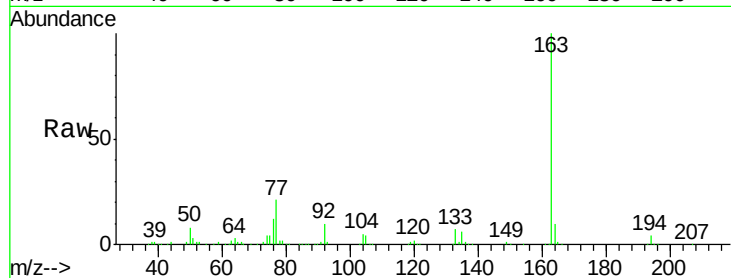

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

