

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
 Data File : BM007095.D
 Acq On : 14 Aug 2016 07:24
 Operator : UM/SJ
 Sample : H4387-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P003-SS001-1218-02

Quant Time: Aug 15 10:25:00 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 00:47:53 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	288647	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	1173764	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.44	164	690588	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.18	188	1645378	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1978212	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	2146736	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	13158	1.99	ng/uL	0.00
5) Phenol-d5	6.97	99	362878	15.52	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.15	67	234951	17.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	285262	15.32	ng/ul	-0.01
13) 4-Methylphenol-d8	8.50	113	298922	15.54	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	172405	20.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	203412	22.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	378802	19.85	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.73	131	360122	15.86	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	1355221	23.75	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1600995	23.36	ng/ul	-0.01
51) 4-Nitrophenol-d4	14.63	143	225073	22.01	ng/ul	0.00
57) Fluorene-d10	15.43	176	1244150	24.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	196890	21.65	ng/ul	-0.01
70) Anthracene-d10	17.28	188	2116331	27.76	ng/ul	0.00
76) Pyrene-d10	19.57	212	2633707	31.54	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	3035446	30.91	ng/ul	-0.01

Target Compounds


						Qvalue
44) Dimethylphthalate	13.90	163	1026508	18.00	ng/ul	100
47) Acenaphthylene	14.16	152	195649	2.77	ng/ul	98
69) Phenanthrene	17.22	178	656907	7.42	ng/ul	100
71) Anthracene	17.32	178	168441	1.85	ng/ul	97
74) Fluoranthene	19.24	202	1229526	11.46	ng/ul	100
77) Pyrene	19.60	202	1700679	15.55	ng/ul	98
80) Benzo(a)anthracene	21.34	228	863264	7.39	ng/ul	93
82) Chrysene	21.40	228	931095	8.72	ng/ul	96
85) Benzo(b)fluoranthene	22.96	252	1066888	8.25	ng/ul	98
86) Benzo(k)fluoranthene	22.96	252	1066888	8.79	ng/ul	99
88) Benzo(a)pyrene	23.54	252	832975	6.80	ng/ul	98
89) Indeno(1,2,3-cd)pyrene	25.93	276	556445	3.70	ng/ul	96
90) Dibenzo(a,h)anthracene	25.93	278	157469	1.25	ng/ul#	89
91) Benzo(g,h,i)perylene	26.63	276	574366	4.52	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007095.D
Acq On : 14 Aug 2016 07:24
Operator : UM/SJ
Sample : H4387-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P003-SS001-1218-02

Quant Time: Aug 15 10:25:00 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 00:47:53 2016
Response via : Initial Calibration

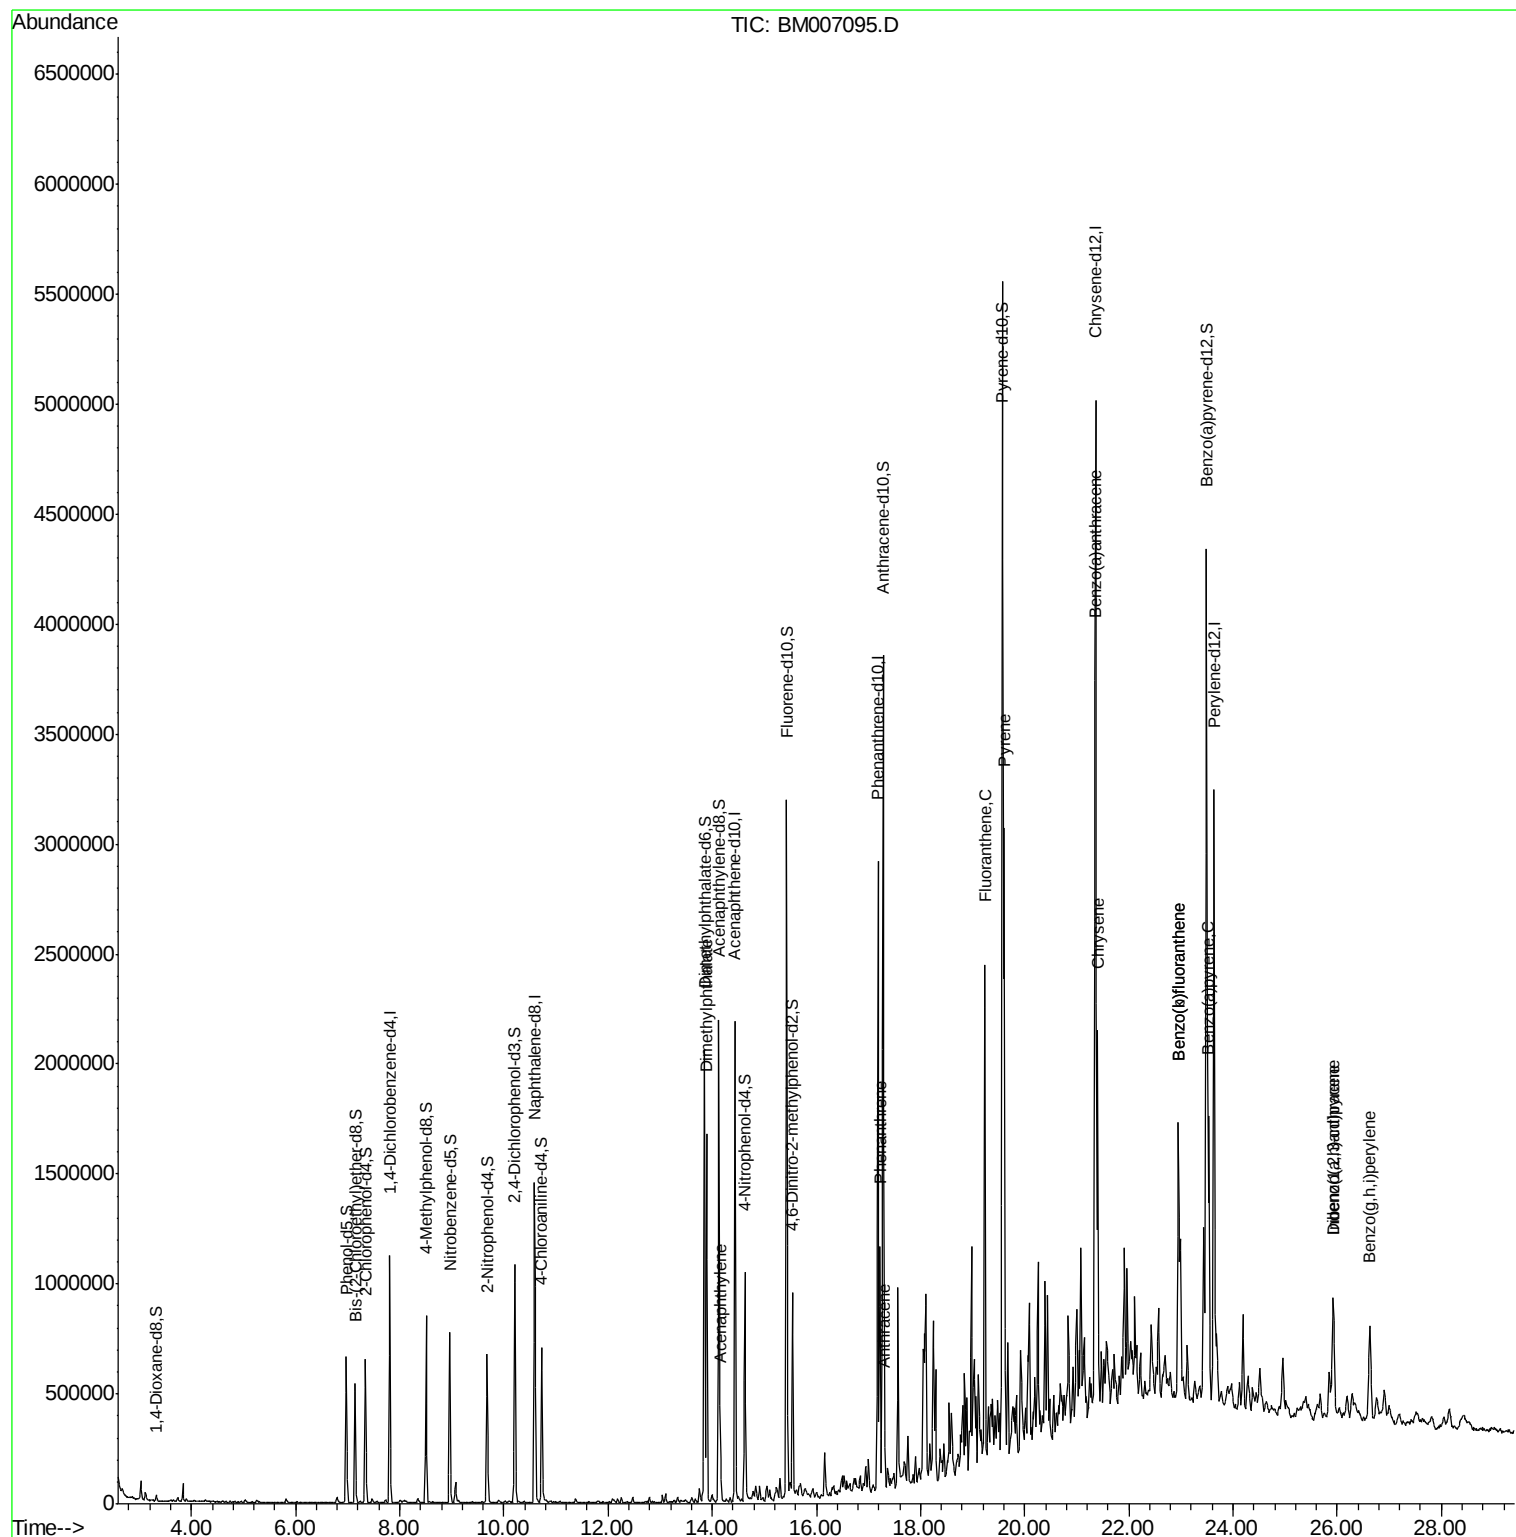



#44

Dimethylphthalate

Concen: 18.00 ng/ul

RT: 13.90 min Scan# 1923

Delta R.T. -0.01 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24

Instrument :

BNA_M

ClientSampleId :

P003-SS001-1218-02


Tgt Ion:163 Resp: 1026508

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2




164 9.8 7.8 11.8



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

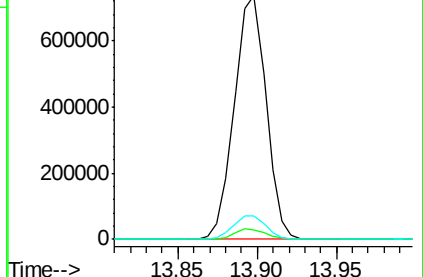

#47

Acenaphthylene

Concen: 2.77 ng/ul

RT: 14.16 min Scan# 1968

Delta R.T. -0.01 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24


Tgt Ion:152 Resp: 195649

Ion Ratio Lower Upper

152 100

151 19.8 16.0 24.0



153 12.5 11.0 16.6




Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

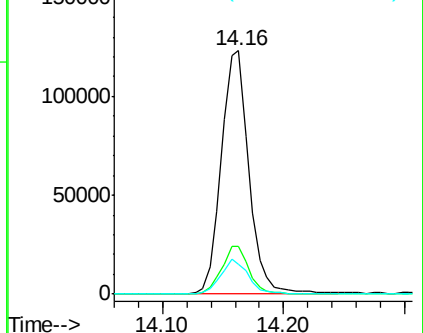

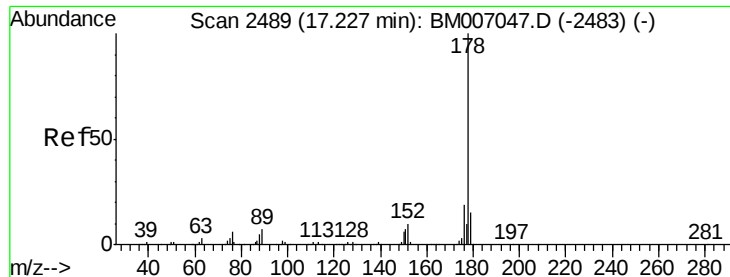

#69

Phenanthrene

Concen: 7.42 ng/ul

RT: 17.22 min Scan# 2488

Delta R.T. -0.01 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24

Instrument :

BNA_M

ClientSampleId :

P003-SS001-1218-02


Tgt Ion:178 Resp: 656907

Ion Ratio Lower Upper

178 100

179 15.2 12.2 18.2




176 18.6 15.1 22.7

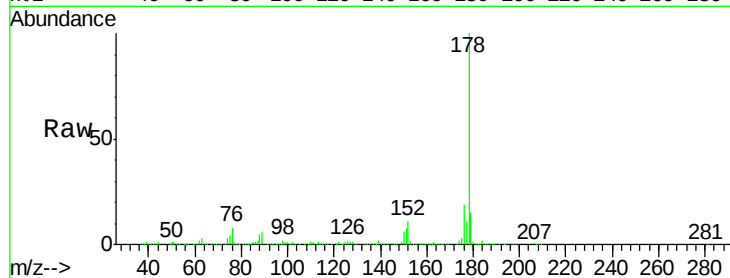

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

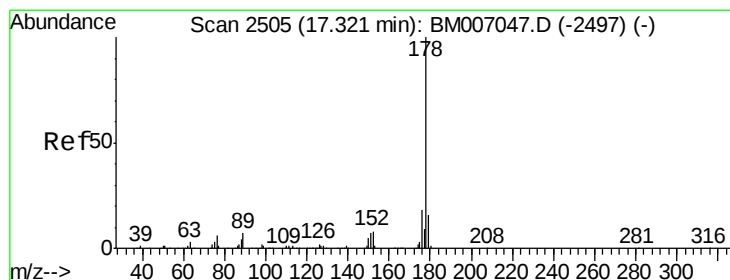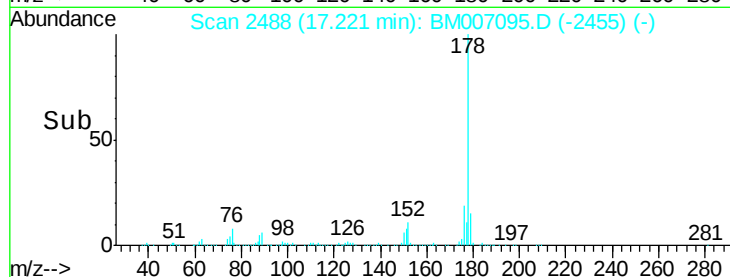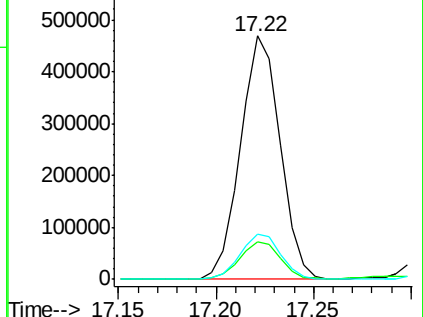

#71

Anthracene

Concen: 1.85 ng/ul

RT: 17.32 min Scan# 2504

Delta R.T. -0.01 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24


Tgt Ion:178 Resp: 168441

Ion Ratio Lower Upper

178 100

179 14.1 12.1 18.1



176 16.9 14.5 21.7

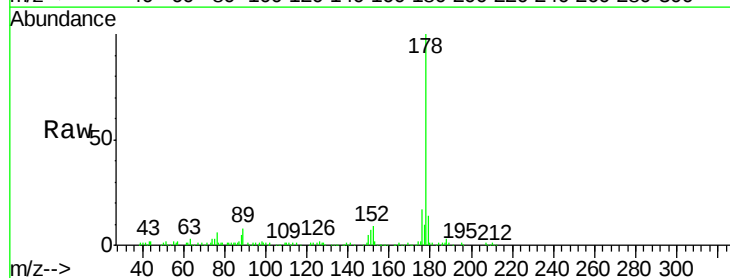


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

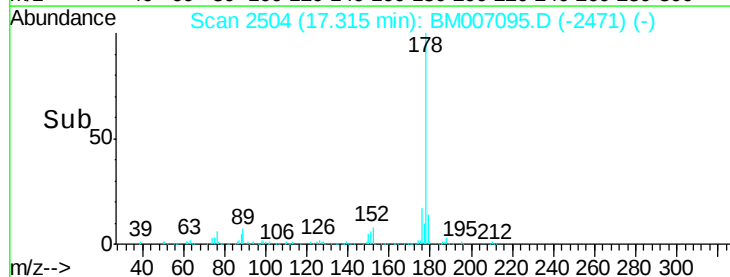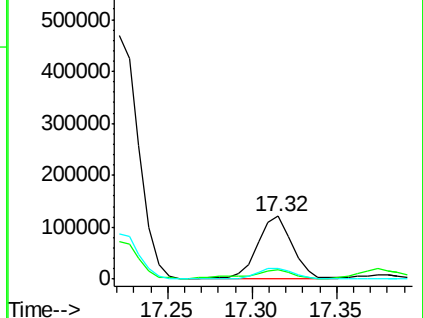

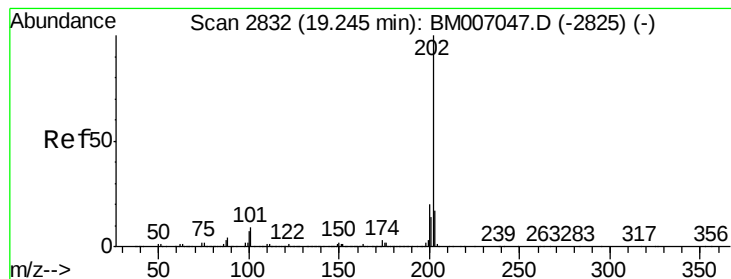

#74

Fluoranthene

Concen: 11.46 ng/ul

RT: 19.24 min Scan# 2831

Delta R.T. -0.01 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24

Instrument :

BNA_M

ClientSampleId :

P003-SS001-1218-02


Tgt Ion:202 Resp: 1229526

Ion Ratio Lower Upper

202 100

101 8.5 6.9 10.3




100 6.5 5.4 8.0



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

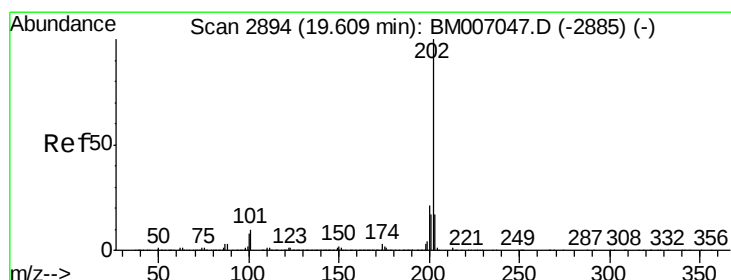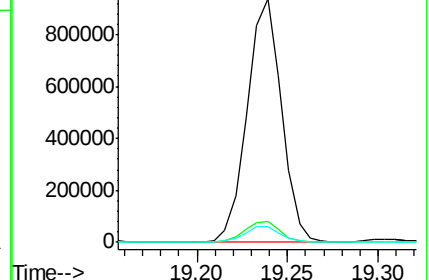

#77

Pyrene

Concen: 15.55 ng/ul

RT: 19.60 min Scan# 2893

Delta R.T. -0.01 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24


Tgt Ion:202 Resp: 1700679

Ion Ratio Lower Upper

202 100

101 9.5 8.4 12.6



100 7.8 6.9 10.3




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

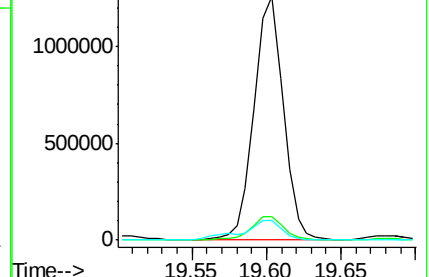

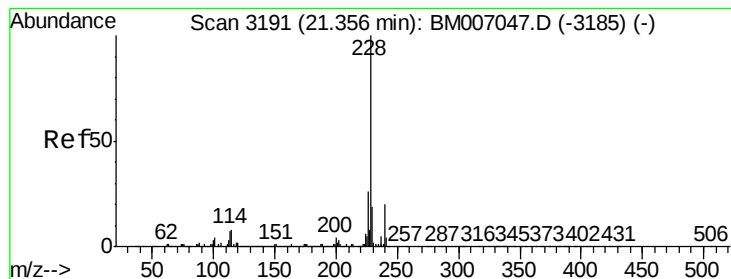

#80

Benzo(a)anthracene

Concen: 7.39 ng/ul

RT: 21.34 min Scan# 3189

Delta R.T. -0.01 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24

Instrument :

BNA_M

ClientSampleId :

P003-SS001-1218-02


Tgt Ion:228 Resp: 863264

Ion Ratio Lower Upper

228 100

229 23.1 15.6 23.4




226 30.7 21.8 32.8



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

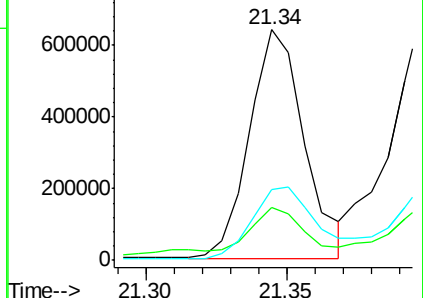

#82

Chrysene

Concen: 8.72 ng/ul

RT: 21.40 min Scan# 3198

Delta R.T. -0.01 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24


Tgt Ion:228 Resp: 931095

Ion Ratio Lower Upper

228 100

226 30.5 23.4 35.2



229 22.1 15.5 23.3




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

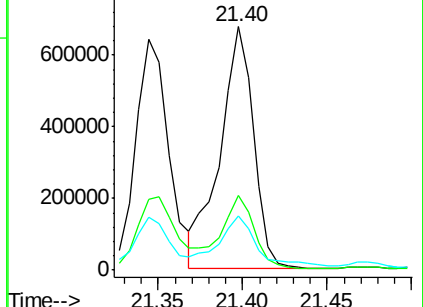



#85

Benzo(b)fluoranthene

Concen: 8.25 ng/ul

RT: 22.96 min Scan# 3463

Delta R.T. -0.01 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24

Instrument :

BNA_M

ClientSampleId :

P003-SS001-1218-02


Tgt Ion:252 Resp: 1066888

Ion Ratio Lower Upper

252 100

253 22.3 17.1 25.7




125 7.8 5.8 8.8



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

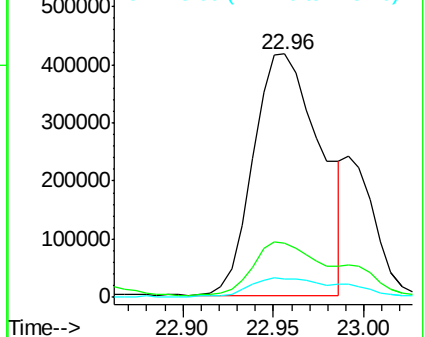

#86

Benzo(k)fluoranthene

Concen: 8.79 ng/ul

RT: 22.96 min Scan# 3463

Delta R.T. -0.05 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24


Tgt Ion:252 Resp: 1066888

Ion Ratio Lower Upper

252 100

253 22.3 17.6 26.4



125 7.8 5.7 8.5




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

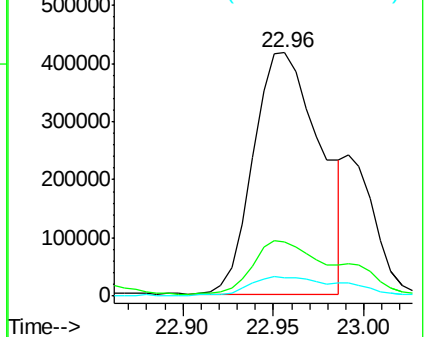

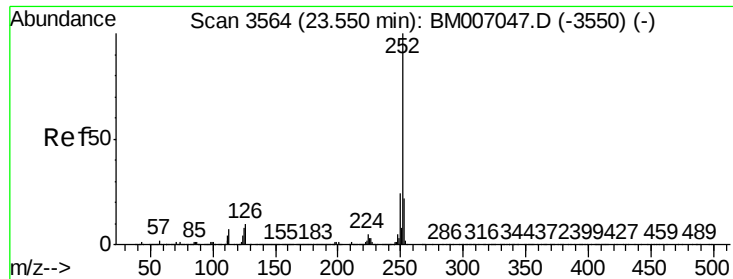

#88

Benzo(a)pyrene

Concen: 6.80 ng/ul

RT: 23.54 min Scan# 3562

Delta R.T. -0.01 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24





Instrument :

BNA_M

ClientSampleId :

P003-SS001-1218-02

Tgt Ion:	252	Resp:	832975
Ion Ratio		Lower	Upper
252	100		
253	23.5	17.7	26.5
125	8.1	6.6	9.8

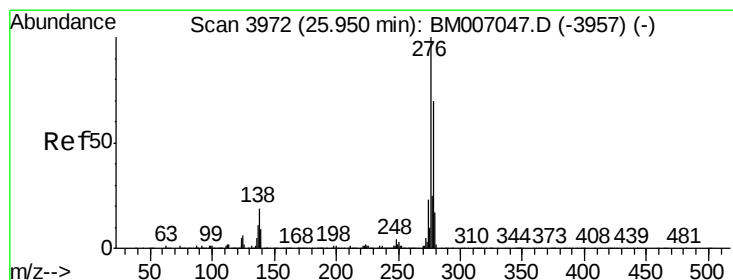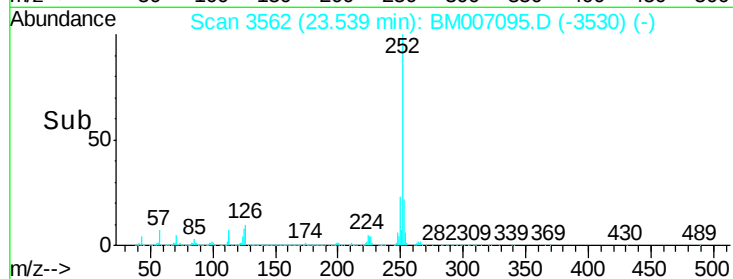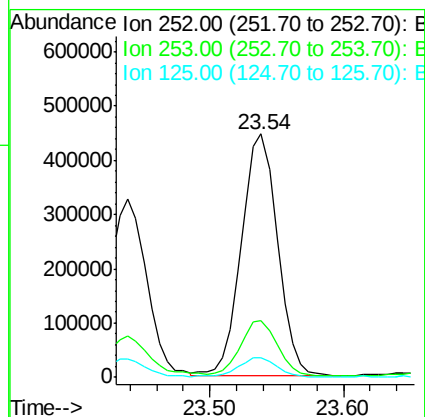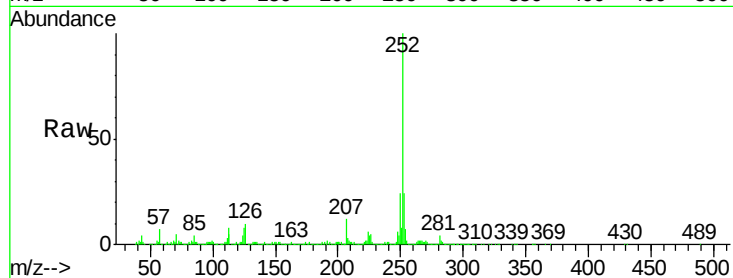

#89

Indeno(1,2,3-cd)pyrene

Concen: 3.70 ng/ul




RT: 25.93 min Scan# 3968


Delta R.T. -0.02 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24

Tgt Ion:	276	Resp:	556445
Ion Ratio		Lower	Upper
276	100		
138	15.4	13.9	20.9
277	23.6	20.1	30.1

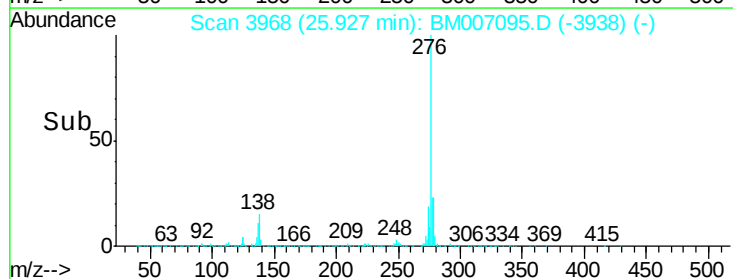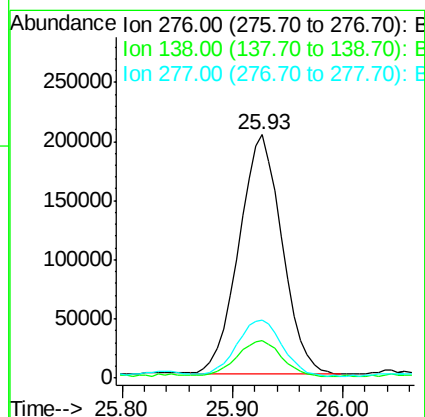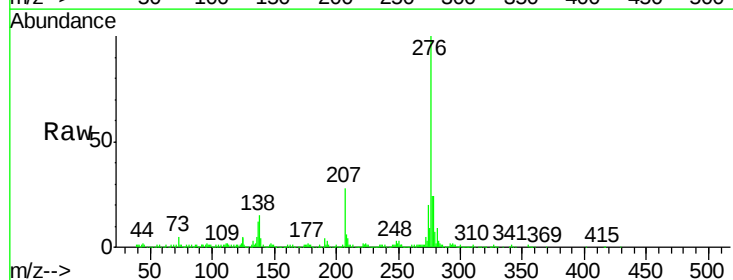

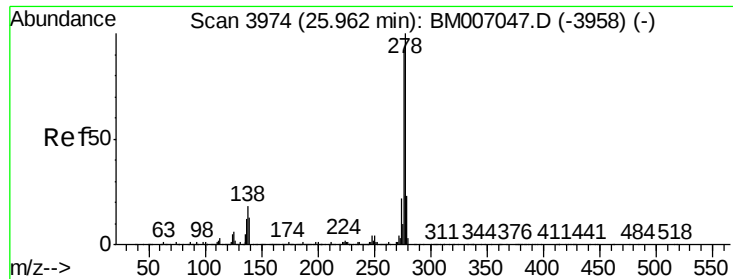

#90

Dibenzo(a,h)anthracene

Concen: 1.25 ng/ul

RT: 25.93 min Scan# 3969

Delta R.T. -0.03 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24





Instrument :

BNA_M

ClientSampleId :

P003-SS001-1218-02

Tgt Ion:	278	Resp:	157469
Ion	Ratio	Lower	Upper
278	100		
139	15.1	9.5	14.3#
279	30.3	19.1	28.7#

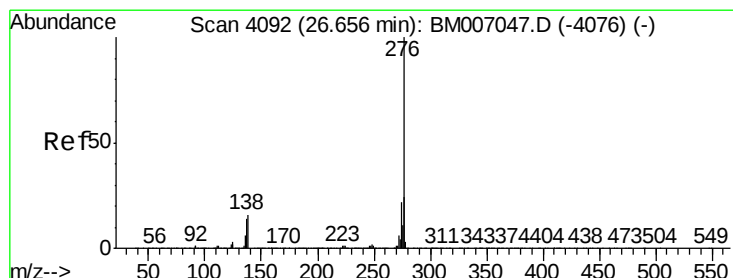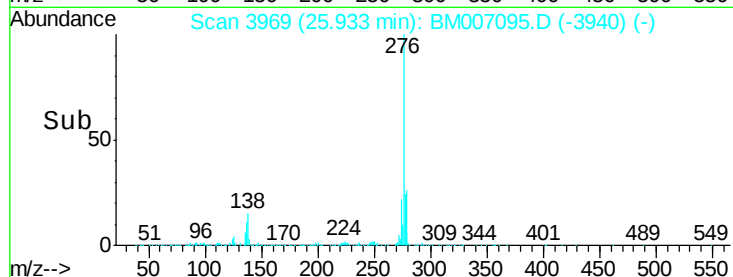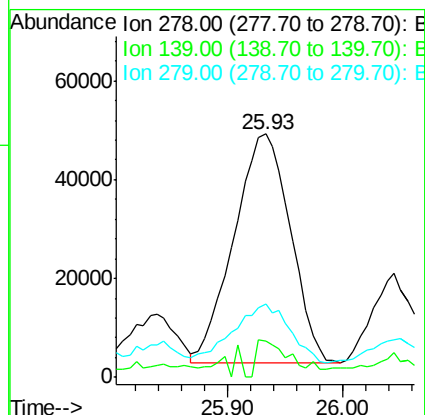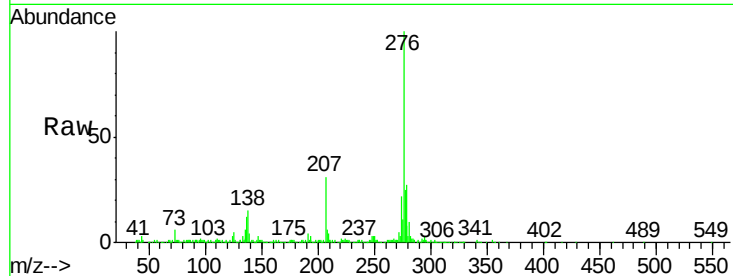

#91

Benzo(g,h,i)perylene

Concen: 4.52 ng/ul

RT: 26.63 min Scan# 4087

Delta R.T. -0.03 min

Lab File: BM007095.D

Acq: 14 Aug 2016 07:24

Tgt Ion:	276	Resp:	574366
Ion	Ratio	Lower	Upper
276	100		
138	17.5	13.5	20.3
277	23.9	19.3	28.9

