

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
 Data File : BM007106.D
 Acq On : 14 Aug 2016 14:04
 Operator : UM/SJ
 Sample : H4387-21
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PR002-SS001-1218-01

Quant Time: Aug 15 10:27:44 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 13 00:47:53 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	285538	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1118221	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	630792	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1426768	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	1736442	20.00	ng/ul	0.00
83) Perylene-d12	23.65	264	1958237	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	18587	2.84	ng/uL	0.00
5) Phenol-d5	6.97	99	378061	16.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	223359	16.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	308767	16.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	278597	14.64	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	148928	18.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	167081	19.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	311534	17.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	269389	12.46	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	938393	18.00	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1172426	18.73	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	148276	15.87	ng/ul	0.00
57) Fluorene-d10	15.43	176	832442	18.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	107265	13.60	ng/ul	0.00
70) Anthracene-d10	17.28	188	1315758	19.91	ng/ul	0.00
76) Pyrene-d10	19.58	212	1526909	20.83	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	1763712	19.69	ng/ul	0.00

Target Compounds


						Qvalue
6) Phenol	7.00	94	31433	1.29	ng/ul	92
28) Naphthalene	10.65	128	71556	1.29	ng/ul	96
34) 2-Methylnaphthalene	12.26	142	79078	1.85	ng/ul	97
44) Dimethylphthalate	13.90	163	953091	18.30	ng/ul	99
47) Acenaphthylene	14.16	152	902777	14.01	ng/ul	100
58) Fluorene	15.49	166	206424	4.12	ng/ul	99
64) N-Nitrosodiphenylamine	15.70	169	42443	1.05	ng/ul#	73
69) Phenanthrene	17.23	178	3182491	41.48	ng/ul	99
71) Anthracene	17.32	178	645229	8.19	ng/ul	99
74) Fluoranthene	19.24	202	3479814	37.39	ng/ul	99
77) Pyrene	19.61	202	6062904	63.15	ng/ul	98
80) Benzo(a)anthracene	21.40	228	3067573	29.90	ng/ul	93
82) Chrysene	21.40	228	3066625	32.71	ng/ul	95
85) Benzo(b)fluoranthene	22.97	252	3097287	26.25	ng/ul	96
86) Benzo(k)fluoranthene	22.97	252	3097287	27.96	ng/ul	97
88) Benzo(a)pyrene	23.55	252	2226414	19.91	ng/ul	97
89) Indeno(1,2,3-cd)pyrene	25.95	276	1352496	9.87	ng/ul	98
90) Dibenzo(a,h)anthracene	25.95	278	404636	3.52	ng/ul#	84
91) Benzo(g,h,i)perylene	26.66	276	1486288	12.83	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007106.D
Acq On : 14 Aug 2016 14:04
Operator : UM/SJ
Sample : H4387-21
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PR002-SS001-1218-01

Quant Time: Aug 15 10:27:44 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 13 00:47:53 2016
Response via : Initial Calibration

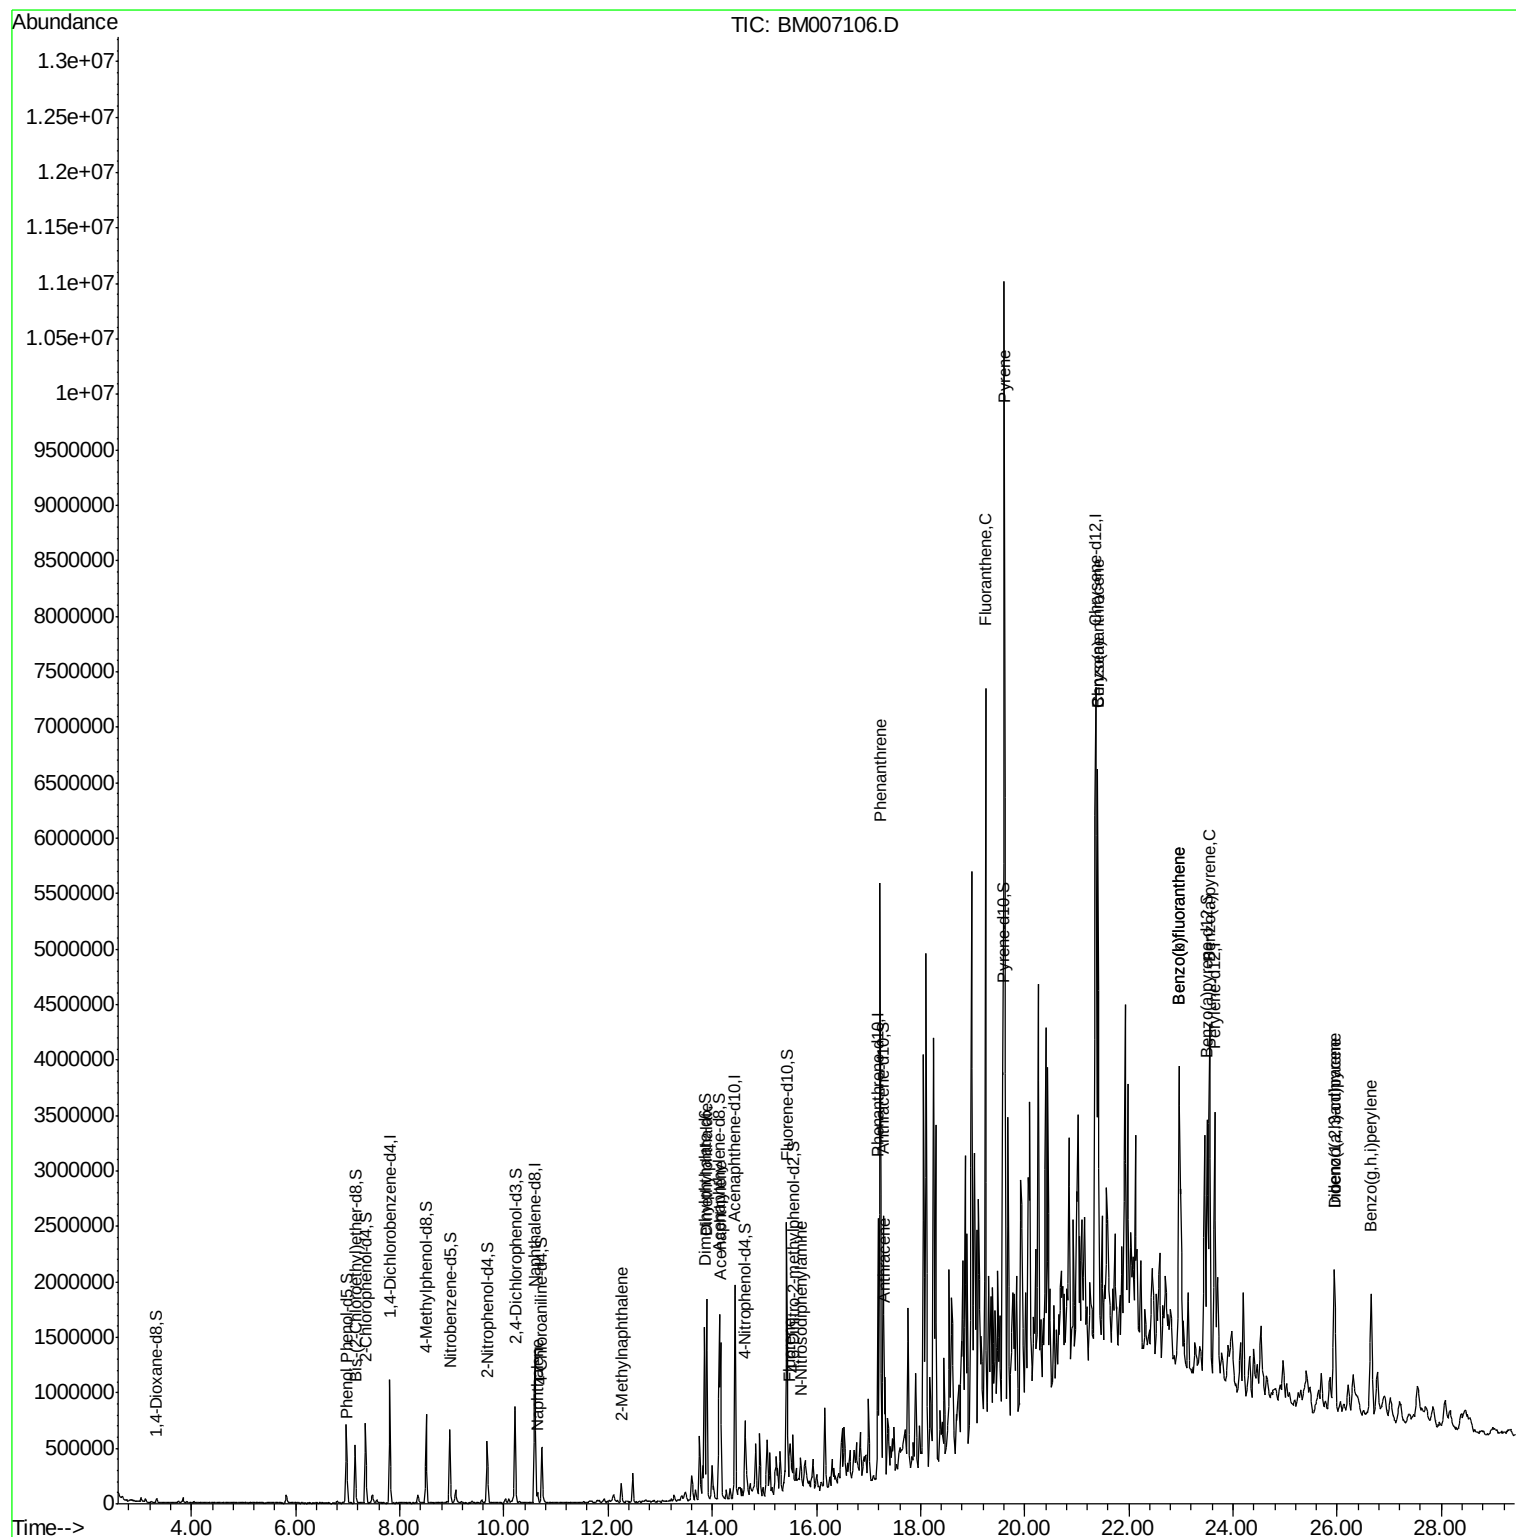

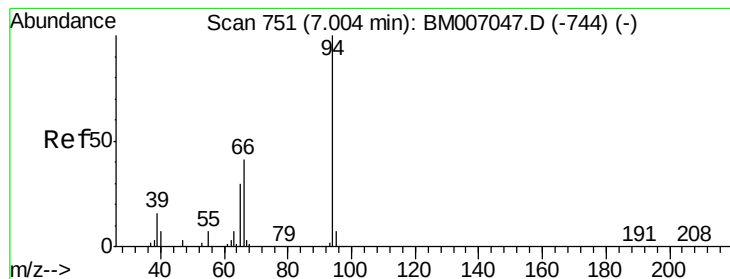

#6

Phenol

Concen: 1.29 ng/ul

RT: 7.00 min Scan# 750

Delta R.T. -0.01 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04

Instrument :

BNA_M

ClientSampleId :

PR002-SS001-1218-01


Tgt Ion: 94 Resp: 31433

Ion Ratio Lower Upper

94 100

65 31.8 23.9 35.9




66 48.8 33.5 50.3

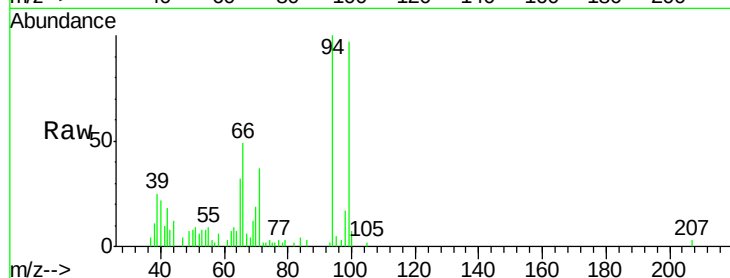

Abundance Ion 94.00 (93.70 to 94.70): BM007047.D (-744) (-)

Ion 65.00 (64.70 to 65.70): BM007047.D (-744) (-)

Ion 66.00 (65.70 to 66.70): BM007047.D (-744) (-)

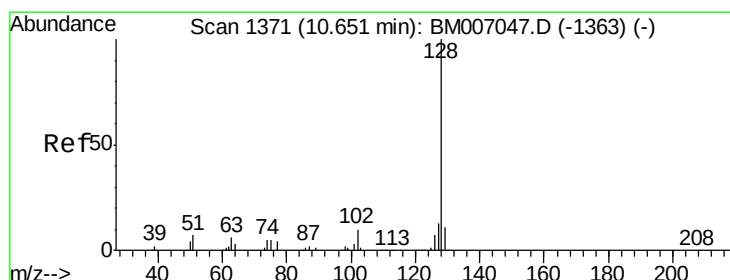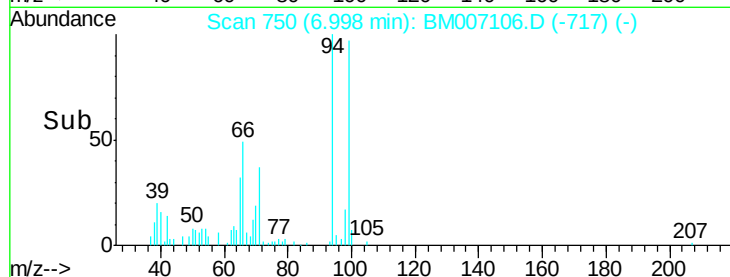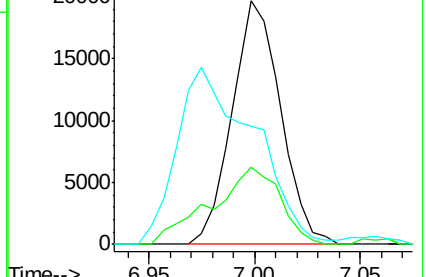

#28

Naphthalene

Concen: 1.29 ng/ul

RT: 10.65 min Scan# 1370

Delta R.T. -0.01 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04


Tgt Ion: 128 Resp: 71556

Ion Ratio Lower Upper

128 100

129 11.7 8.6 12.8



127 11.4 10.6 15.8

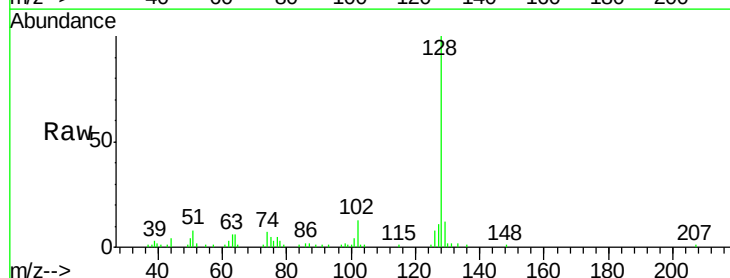


Abundance Ion 128.00 (127.70 to 128.70): BM007047.D (-1363) (-)

Ion 129.00 (128.70 to 129.70): BM007047.D (-1363) (-)

Ion 127.00 (126.70 to 127.70): BM007047.D (-1363) (-)

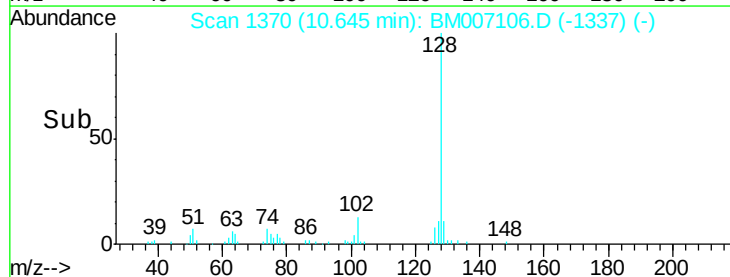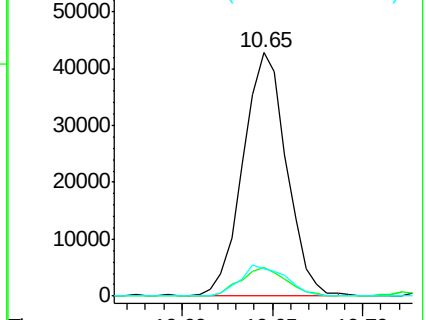

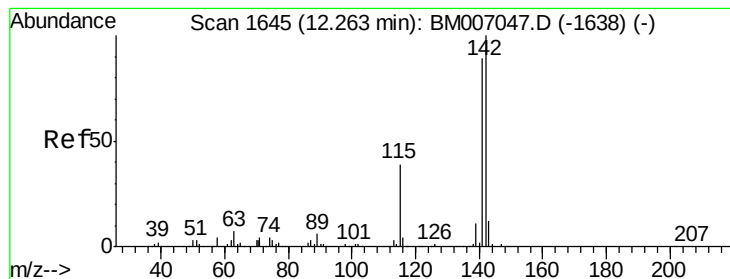

#34

2-Methylnaphthalene

Concen: 1.85 ng/ul

RT: 12.26 min Scan# 1644

Delta R.T. -0.01 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04

Instrument :

BNA_M

ClientSampleId :


PR002-SS001-1218-01

Tgt Ion:142 Resp: 79078

Ion Ratio Lower Upper




142 100

141 86.5 71.3 106.9

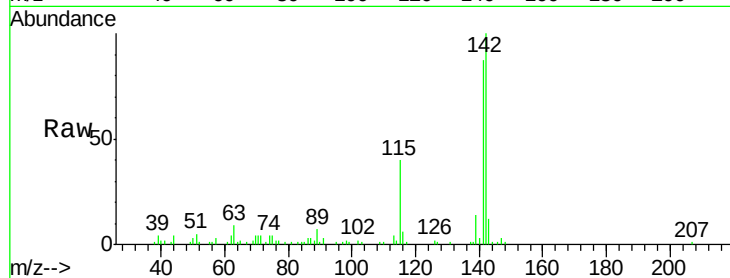

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

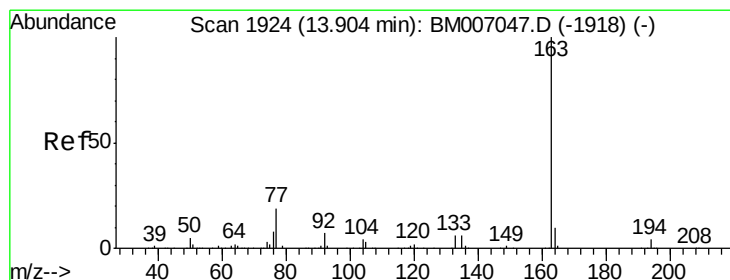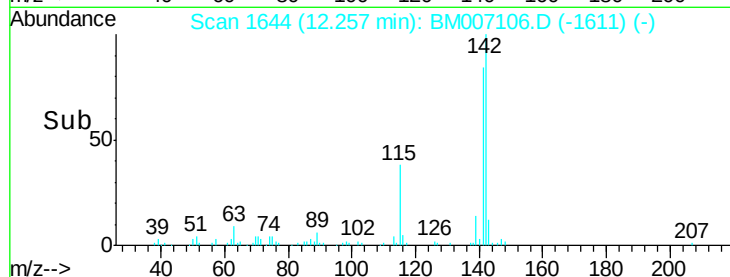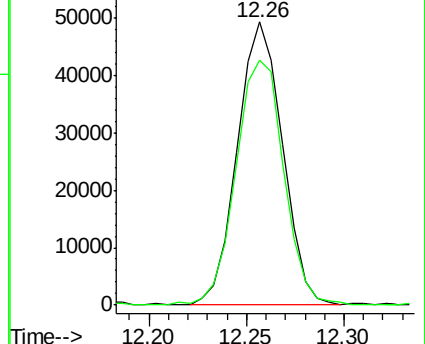

#44

Dimethylphthalate

Concen: 18.30 ng/ul

RT: 13.90 min Scan# 1923

Delta R.T. -0.01 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04


Tgt Ion:163 Resp: 953091

Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.2



164 9.7 7.8 11.8

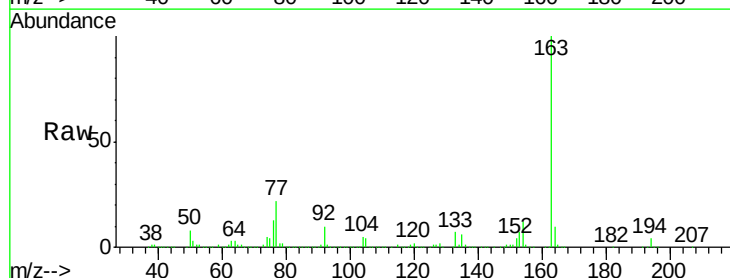


Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

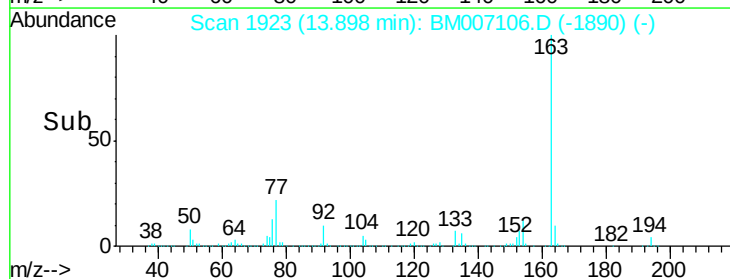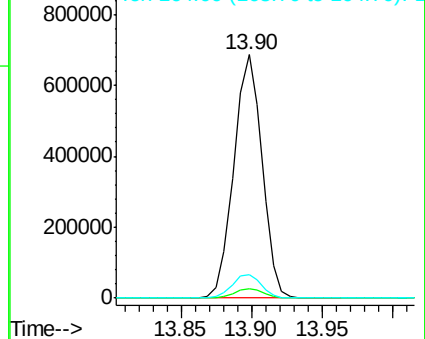

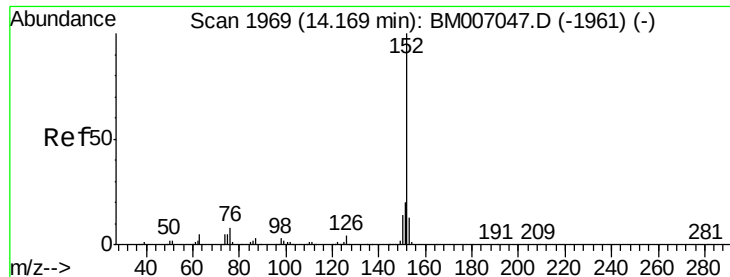

#47

Acenaphthylene

Concen: 14.01 ng/ul

RT: 14.16 min Scan# 1968

Delta R.T. -0.01 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04





Instrument :

BNA_M

ClientSampleId :

PR002-SS001-1218-01

Tgt Ion:	152	Resp:	902777
Ion	Ratio	Lower	Upper
152	100		
151	20.2	16.0	24.0
153	13.9	11.0	16.6

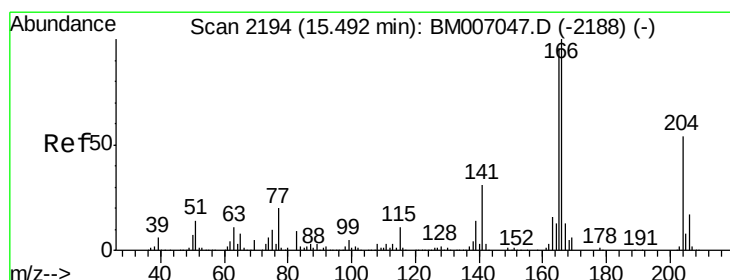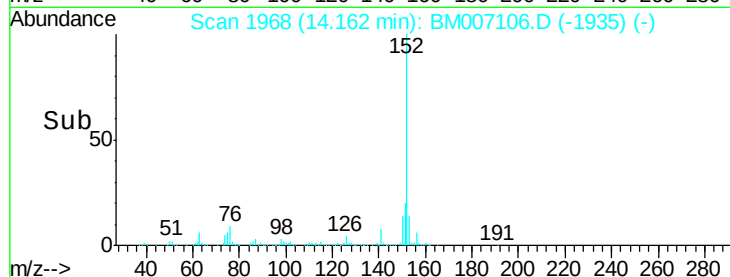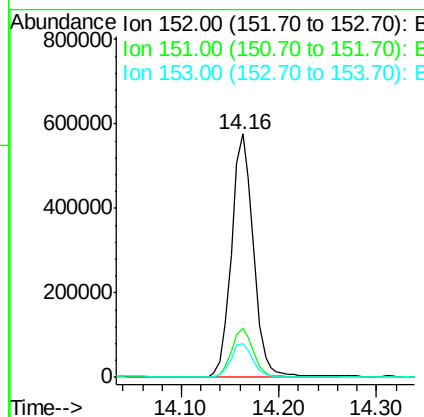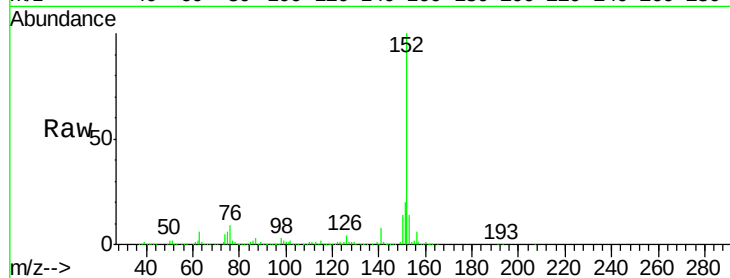

#58

Fluorene

Concen: 4.12 ng/ul




RT: 15.49 min Scan# 2194


Delta R.T. -0.00 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04

Tgt Ion:	166	Resp:	206424
Ion	Ratio	Lower	Upper
166	100		
165	99.3	79.9	119.9
167	15.6	10.5	15.7

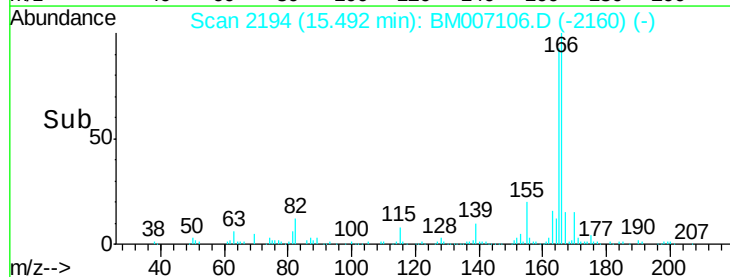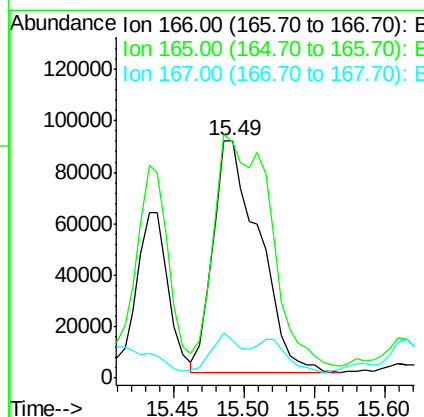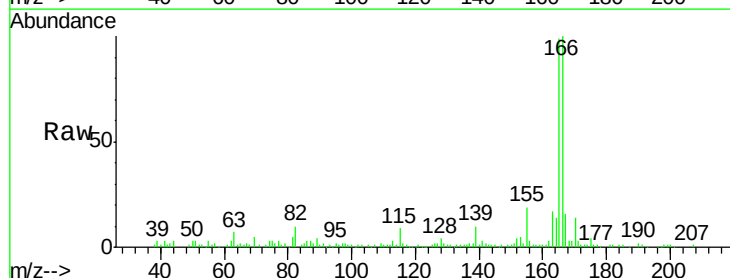

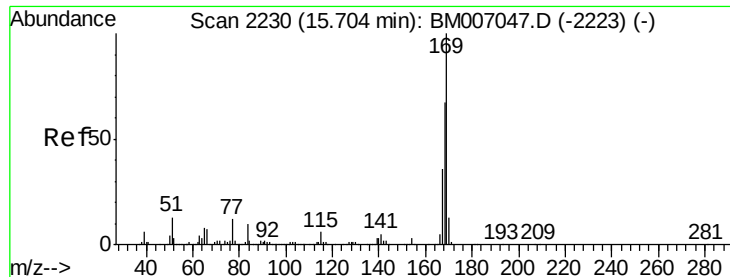

#64

N-Nitrosodiphenylamine

Concen: 1.05 ng/ul

RT: 15.70 min Scan# 2230

Delta R.T. -0.00 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04

Instrument :

BNA_M

ClientSampleId :

PR002-SS001-1218-01





Tgt Ion:169 Resp: 42443

Ion Ratio Lower Upper

169 100

168 35.9 52.6 79.0#

167 31.2 28.6 43.0

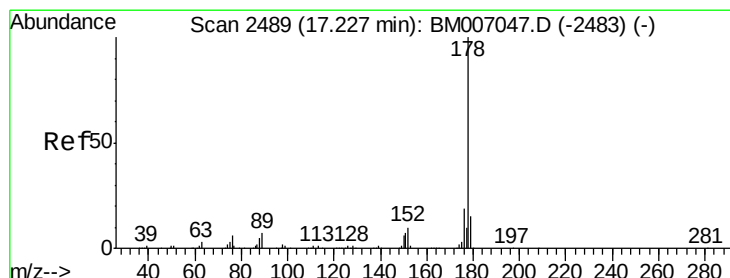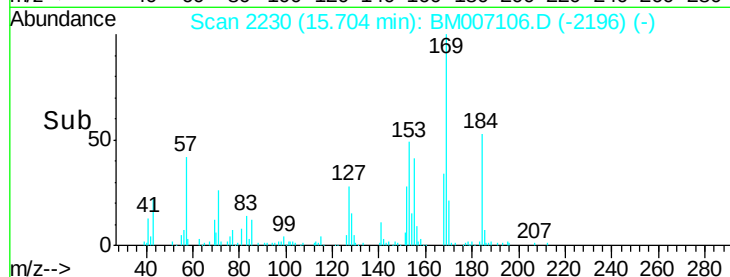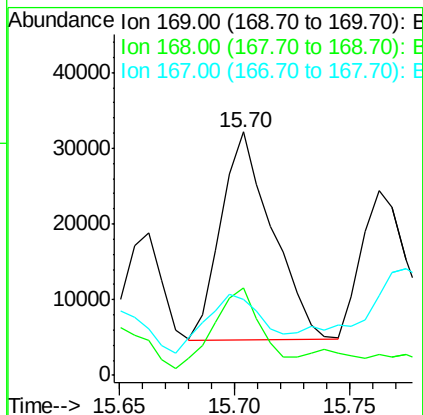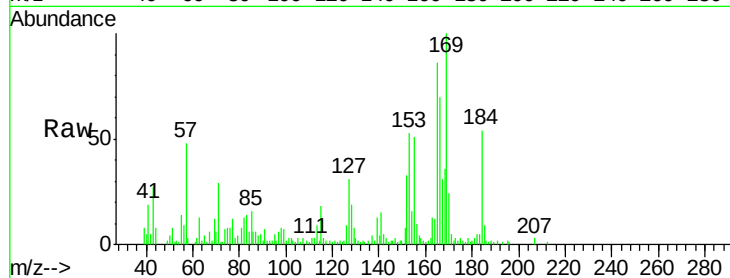

#69

Phenanthrene

Concen: 41.48 ng/ul

RT: 17.23 min Scan# 2489

Delta R.T. -0.00 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04




Tgt Ion:178 Resp: 3182491


Ion Ratio Lower Upper

178 100

179 15.5 12.2 18.2

176 19.4 15.1 22.7

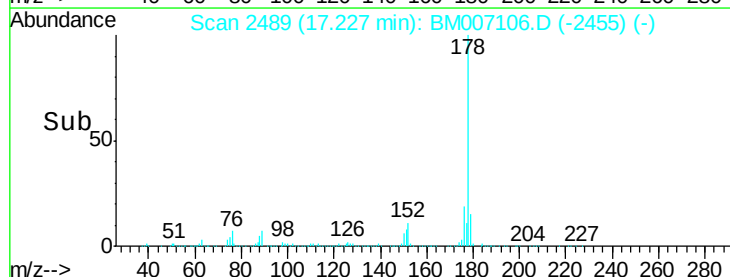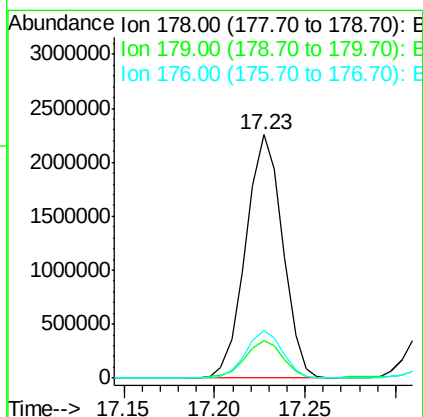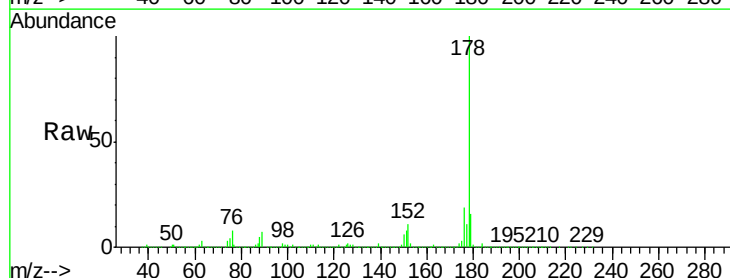

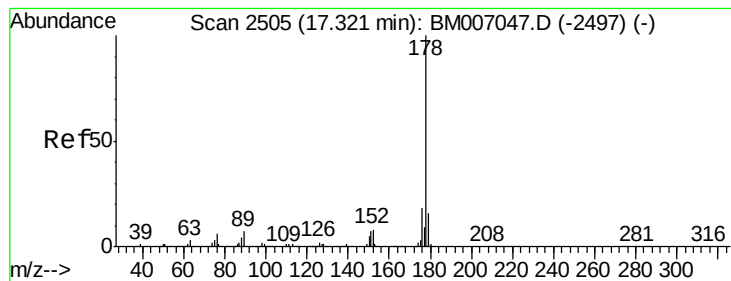

#71

Anthracene

Concen: 8.19 ng/ul

RT: 17.32 min Scan# 2504

Delta R.T. -0.01 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04

Instrument :

BNA_M

ClientSampleId :

PR002-SS001-1218-01


Tgt Ion:178 Resp: 645229

Ion Ratio Lower Upper

178 100

179 15.6 12.1 18.1




176 18.3 14.5 21.7



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

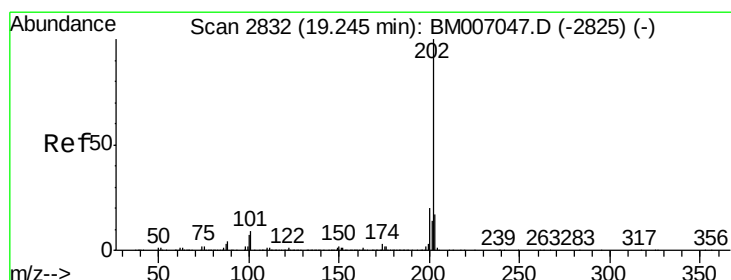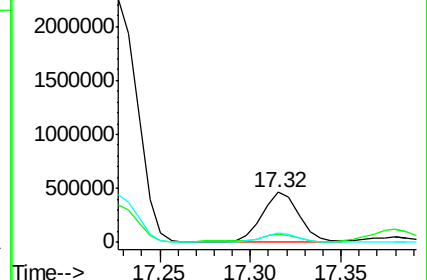

#74

Fluoranthene

Concen: 37.39 ng/ul

RT: 19.24 min Scan# 2832

Delta R.T. -0.00 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04


Tgt Ion:202 Resp: 3479814

Ion Ratio Lower Upper

202 100

101 8.7 6.9 10.3



100 6.2 5.4 8.0




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

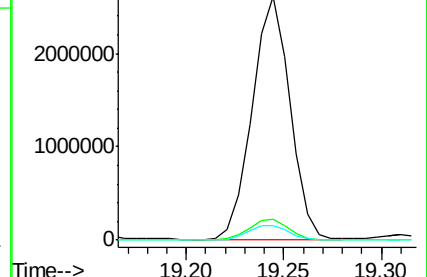



#77

Pyrene

Concen: 63.15 ng/ul

RT: 19.61 min Scan# 2894

Delta R.T. -0.00 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04

Instrument :

BNA_M

ClientSampleId :

PR002-SS001-1218-01


Tgt Ion:202 Resp: 6062904

Ion Ratio Lower Upper

202 100

101 9.9 8.4 12.6




100 8.1 6.9 10.3

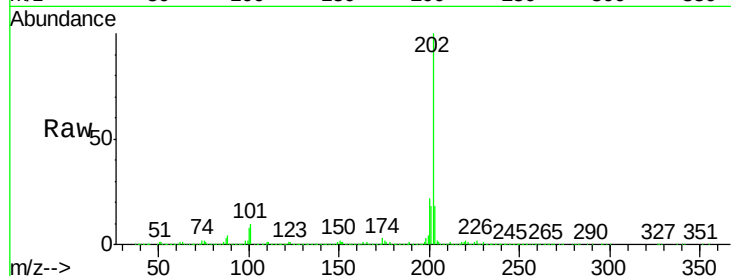

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

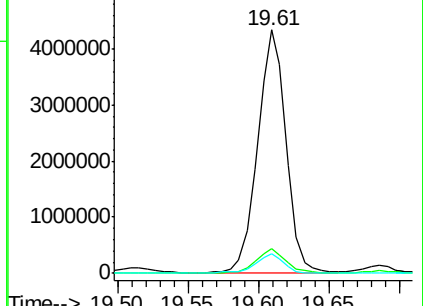

#80

Benzo(a)anthracene

Concen: 29.90 ng/ul

RT: 21.40 min Scan# 3199

Delta R.T. 0.05 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04


Tgt Ion:228 Resp: 3067573

Ion Ratio Lower Upper

228 100

229 22.8 15.6 23.4



226 31.2 21.8 32.8




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

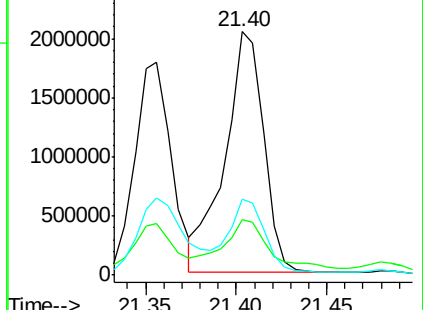



#82

Chrysene

Concen: 32.71 ng/ul

RT: 21.40 min Scan# 3199

Delta R.T. -0.01 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04

Instrument :

BNA_M

ClientSampleId :

PR002-SS001-1218-01


Tgt Ion:228 Resp: 3066625

Ion Ratio Lower Upper

228 100

226 31.2 23.4 35.2




229 22.8 15.5 23.3

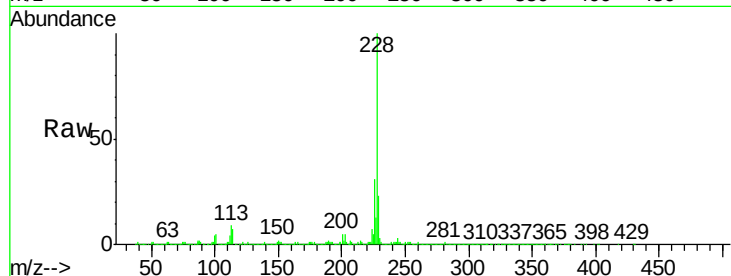

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

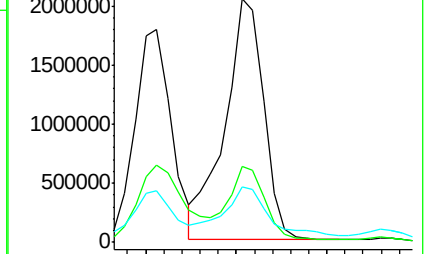

#85

Benzo(b)fluoranthene

Concen: 26.25 ng/ul

RT: 22.97 min Scan# 3465

Delta R.T. 0.01 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04


Tgt Ion:252 Resp: 3097287

Ion Ratio Lower Upper

252 100

253 23.6 17.1 25.7



125 8.2 5.8 8.8




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E




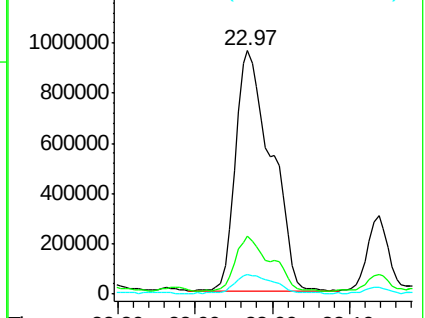


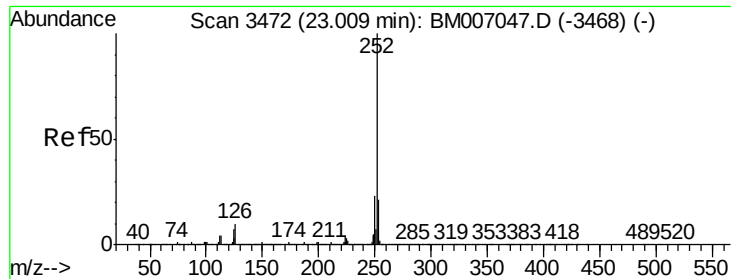

#86
Benzo(k)fluoranthene
Concen: 27.96 ng/ul
RT: 22.97 min Scan# 3465
Delta R.T. -0.04 min
Lab File: BM007106.D
Acq: 14 Aug 2016 14:04




Instrument :
BNA_M
ClientSampleId :
PR002-SS001-1218-01


Tgt Ion:252 Resp: 3097287
Ion Ratio Lower Upper
252 100
253 23.6 17.6 26.4
125 8.2 5.7 8.5

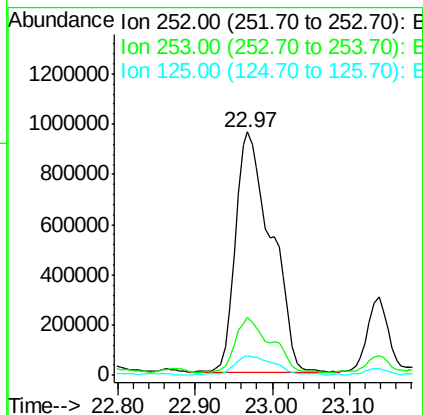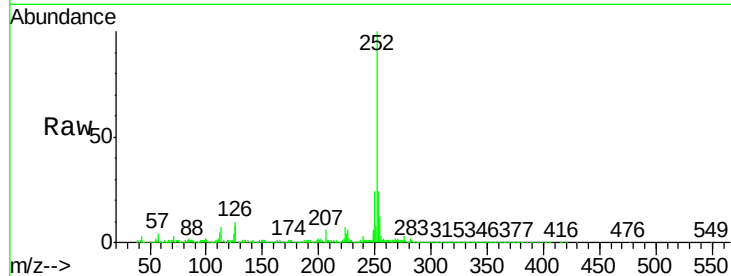

#88
Benzo(a)pyrene
Concen: 19.91 ng/ul
RT: 23.55 min Scan# 3564
Delta R.T. -0.00 min
Lab File: BM007106.D
Acq: 14 Aug 2016 14:04

Tgt Ion:252 Resp: 2226414
Ion Ratio Lower Upper
252 100
253 23.6 17.7 26.5
125 7.8 6.6 9.8

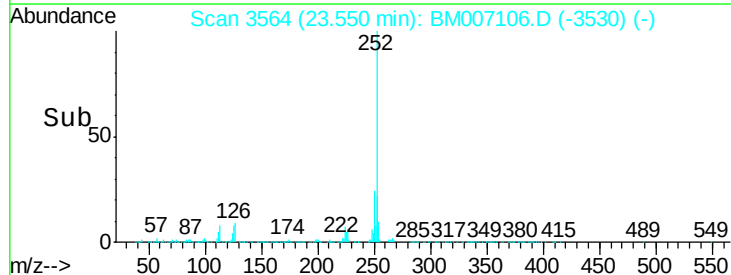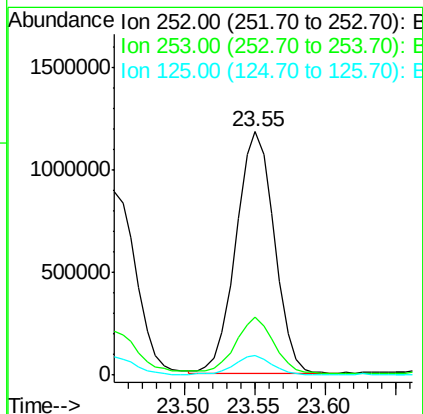



#89

Indeno(1,2,3-cd)pyrene

Concen: 9.87 ng/ul

RT: 25.95 min Scan# 3972

Delta R.T. -0.00 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04

Instrument :

BNA_M

ClientSampleId :

PR002-SS001-1218-01


Tgt Ion:276 Resp: 1352496

Ion Ratio Lower Upper

276 100

138 15.9 13.9 20.9




277 24.6 20.1 30.1



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

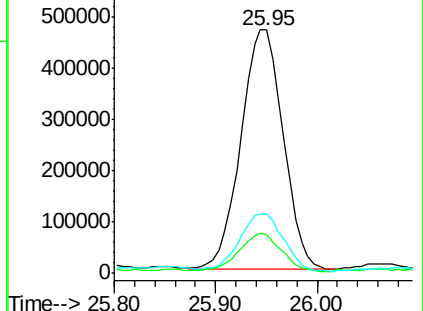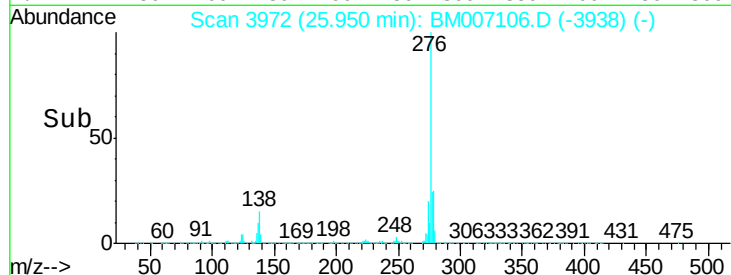

#90

Dibenzo(a,h)anthracene

Concen: 3.52 ng/ul

RT: 25.95 min Scan# 3972

Delta R.T. -0.01 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04


Tgt Ion:278 Resp: 404636

Ion Ratio Lower Upper

278 100

139 16.2 9.5 14.3#



279 32.8 19.1 28.7#




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

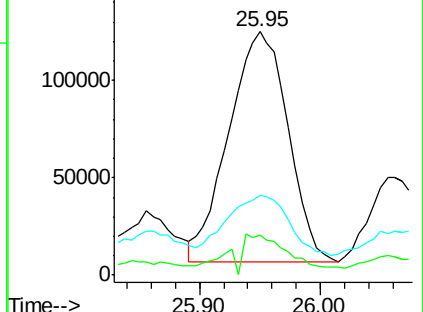

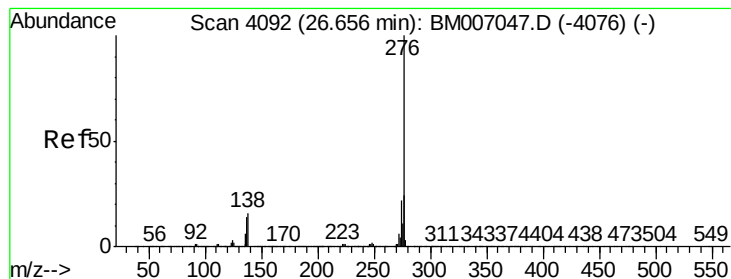

#91

Benzo(g,h,i)perylene

Concen: 12.83 ng/ul

RT: 26.66 min Scan# 4092

Delta R.T. -0.00 min

Lab File: BM007106.D

Acq: 14 Aug 2016 14:04

Instrument :

BNA_M

ClientSampleId :

PR002-SS001-1218-01

Tgt Ion: 276 Resp: 1486288

Ion Ratio Lower Upper

276 100

138 15.8 13.5 20.3

277 24.7 19.3 28.9

