

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
 Data File : BM007081.D
 Acq On : 13 Aug 2016 22:56
 Operator : UM/SJ
 Sample : H4314-09
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJT8

Quant Time: Aug 15 13:10:55 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 15 10:34:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	269372	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	1059765	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	616576	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	1469803	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	1897213	20.00	ng/ul	0.00
83) Perylene-d12	23.63	264	2026454	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.33	96	30990	5.03	ng/uL	0.00
5) Phenol-d5	6.97	99	577451	26.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	344030	27.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	483965	27.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	457613	25.48	ng/ul	-0.01
19) Nitrobenzene-d5	8.96	128	220337	28.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.68	143	244522	29.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	464004	26.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	578505	28.22	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	1472585	28.90	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	1764184	28.83	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	211879	23.20	ng/ul	0.00
57) Fluorene-d10	15.43	176	1276967	28.67	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	183848	22.64	ng/ul	-0.01
70) Anthracene-d10	17.28	188	2081213	30.57	ng/ul	0.00
76) Pyrene-d10	19.57	212	2572012	32.12	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	3035708	32.75	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.90	163	304628	5.98	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007081.D
Acq On : 13 Aug 2016 22:56
Operator : UM/SJ
Sample : H4314-09
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT8

Quant Time: Aug 15 13:10:55 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 15 10:34:14 2016
Response via : Initial Calibration

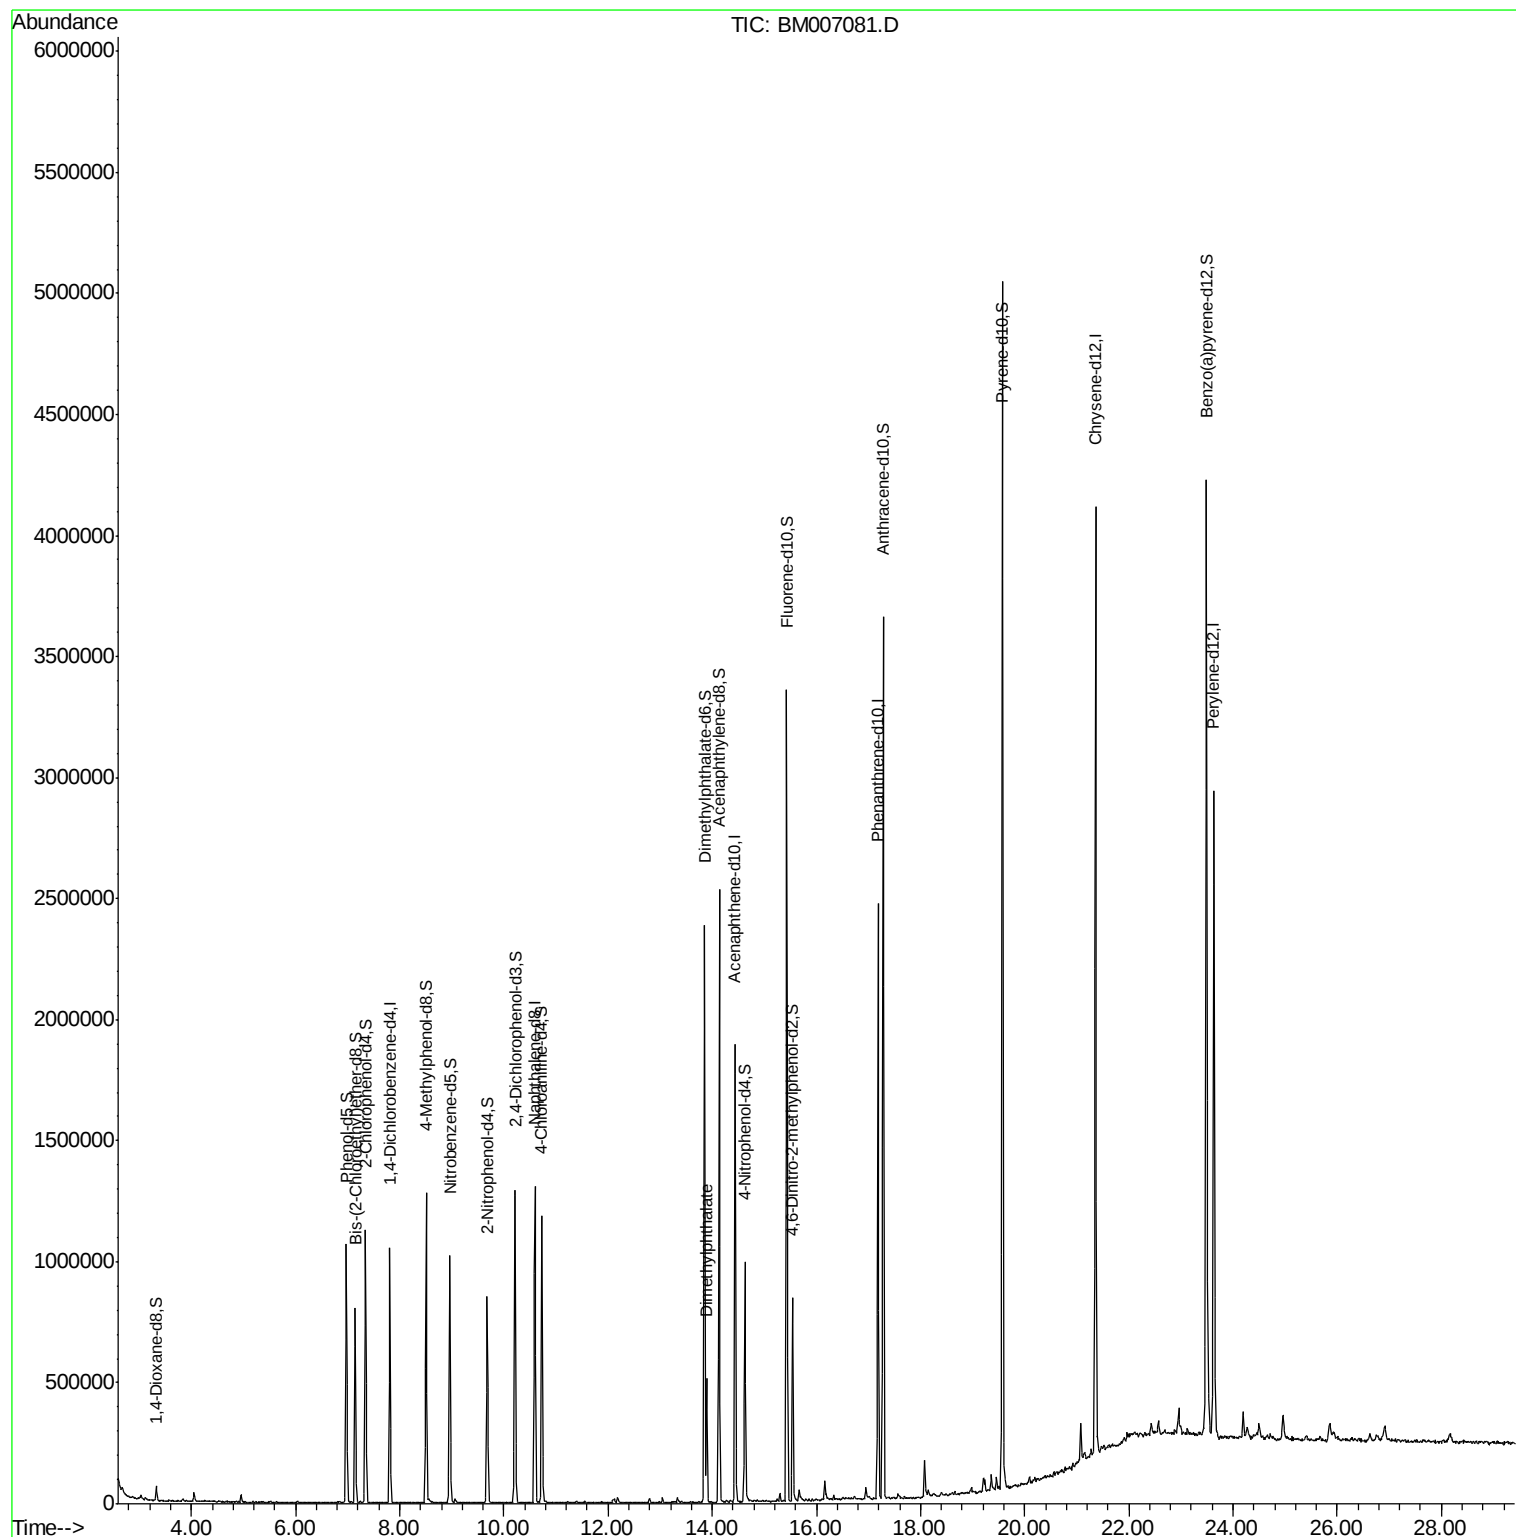

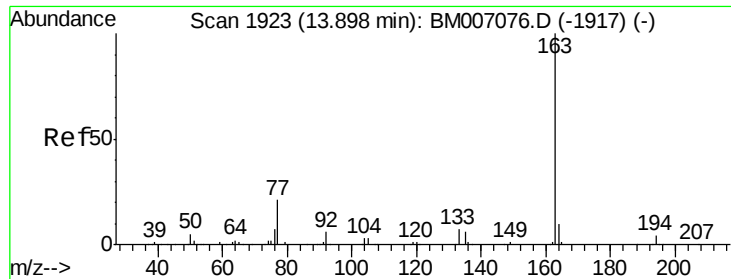

#44

Dimethylphthalate

Concen: 5.98 ng/ul

RT: 13.90 min Scan# 1923

Delta R.T. -0.01 min

Lab File: BM007081.D

Acq: 13 Aug 2016 22:56

Instrument :

BNA_M

ClientSampleId :

BDJT8

Tgt Ion:163 Resp: 304628

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 10.6 7.8 11.8

