

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
 Data File : BM007077.D
 Acq On : 13 Aug 2016 20:29
 Operator : UM/SJ
 Sample : H4314-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJT4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	121	126	133	rVB	57767	80994	1.13%	0.124%
2	6.975	739	746	754	rBV	1087079	1726194	24.19%	2.643%
3	7.145	768	775	785	rBV	793996	1239136	17.36%	1.898%
4	7.345	801	809	817	rBV	1134294	1787017	25.04%	2.737%
5	7.810	882	888	895	rBV	821454	1328778	18.62%	2.035%
6	8.510	1000	1007	1016	rBV	1302412	2156614	30.22%	3.303%
7	8.963	1077	1084	1095	rVB	984840	1630804	22.85%	2.497%
8	9.681	1196	1206	1217	rBV	848782	1385762	19.42%	2.122%
9	10.216	1289	1297	1305	rBV	1315246	2202537	30.86%	3.373%
10	10.598	1355	1362	1370	rVB	1059952	1787612	25.05%	2.738%
11	10.728	1377	1384	1395	rBV	1223387	2105736	29.51%	3.225%
12	13.851	1909	1915	1919	rBV	2330768	3142261	44.03%	4.812%
13	13.898	1919	1923	1932	rVB	790135	1060837	14.87%	1.625%
14	14.133	1956	1963	1972	rVB	2531480	3732374	52.30%	5.716%
15	14.439	2007	2015	2024	rBV2	1502105	2355272	33.00%	3.607%
16	14.627	2041	2047	2060	rBV	911171	1379682	19.33%	2.113%
17	15.433	2177	2184	2194	rBV	3268991	4681884	65.61%	7.170%
18	15.545	2197	2203	2217	rBV	717099	988504	13.85%	1.514%
19	17.186	2475	2482	2488	rBV	1968568	2894014	40.55%	4.432%
20	17.280	2491	2498	2507	rVV2	3545014	5127128	71.84%	7.852%
21	18.080	2629	2634	2642	rBV2	150426	226309	3.17%	0.347%
22	19.574	2882	2888	2894	rBV	4536442	6304047	88.34%	9.654%
23	21.080	3140	3144	3148	rBV	126328	175342	2.46%	0.269%
24	21.362	3186	3192	3198	rBV	3212856	4019272	56.32%	6.155%
25	22.950	3460	3462	3466	rVB	75495	90948	1.27%	0.139%
26	23.491	3546	3554	3568	rVB2	3628645	7136425	100.00%	10.929%
27	23.633	3571	3578	3589	rVB	2075802	4076420	57.12%	6.243%
28	24.197	3670	3674	3682	rVB2	118016	221001	3.10%	0.338%
29	24.962	3800	3804	3811	rVB2	129668	257660	3.61%	0.395%


Sum of corrected areas: 65300564

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007077.D
Acq On : 13 Aug 2016 20:29
Operator : UM/SJ
Sample : H4314-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

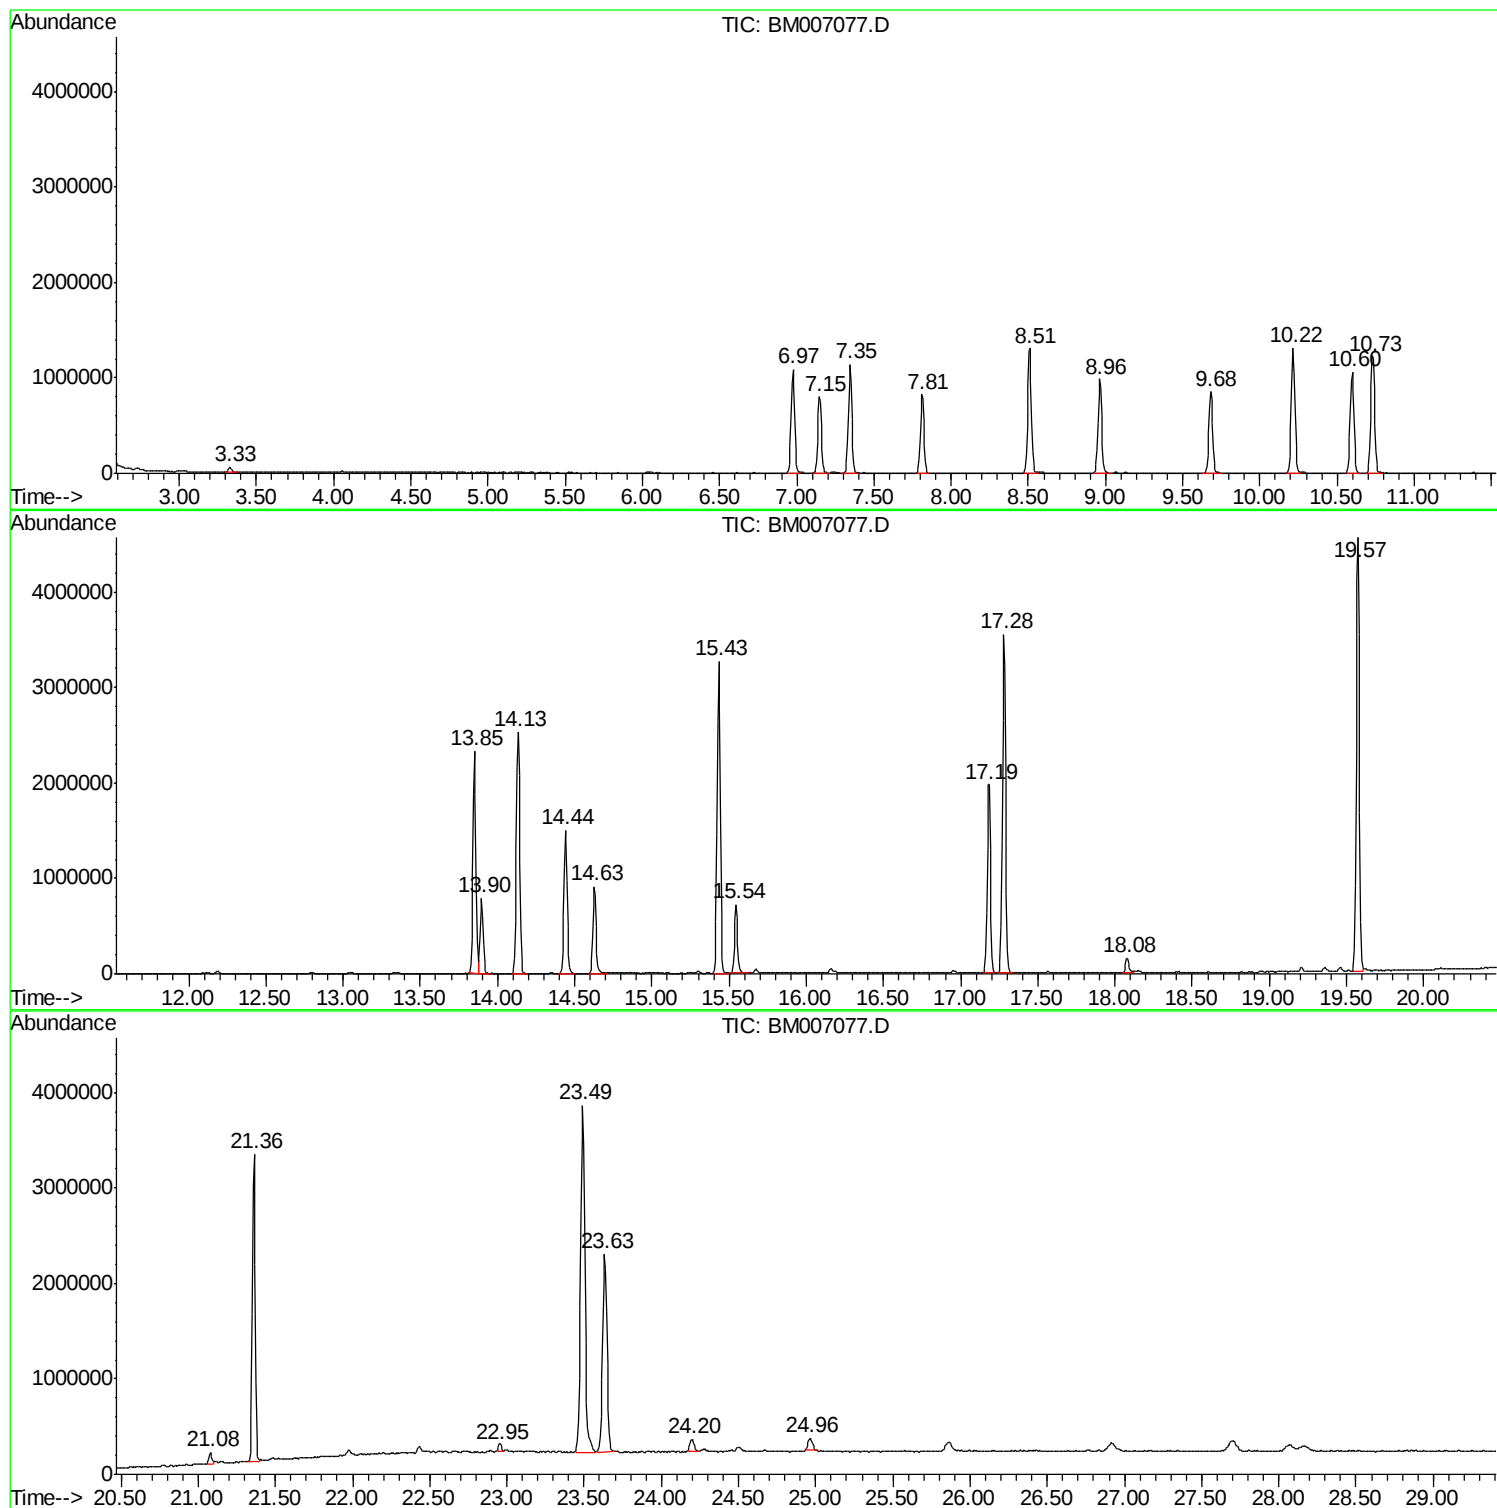

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007077.D
Acq On : 13 Aug 2016 20:29
Operator : UM/SJ
Sample : H4314-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007077.D
Acq On : 13 Aug 2016 20:29
Operator : UM/SJ
Sample : H4314-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc