

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
 Data File : BM007078.D
 Acq On : 13 Aug 2016 21:06
 Operator : UM/SJ
 Sample : H4314-06
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJT5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.669	11	14	25	rVB6	33707	69019	1.37%	0.132%
2	3.328	119	126	134	rVB	40869	61039	1.21%	0.117%
3	6.975	739	746	757	rBV	756909	1189136	23.61%	2.279%
4	7.146	769	775	785	rVB	580642	877449	17.42%	1.682%
5	7.346	802	809	818	rBV	797394	1269029	25.20%	2.433%
6	7.810	881	888	896	rVB	907419	1447488	28.74%	2.775%
7	8.504	998	1006	1016	rBV2	908119	1483792	29.47%	2.844%
8	8.963	1077	1084	1094	rVB	701583	1128770	22.42%	2.164%
9	9.681	1198	1206	1216	rBV	557028	926276	18.39%	1.776%
10	10.216	1289	1297	1308	rBV	906441	1528618	30.36%	2.930%
11	10.598	1354	1362	1370	rBV	1112715	1923589	38.20%	3.687%
12	10.728	1377	1384	1394	rBV	834846	1424737	28.29%	2.731%
13	13.851	1908	1915	1919	rBV	1599085	2210456	43.90%	4.237%
14	13.898	1919	1923	1930	rVB	463259	639744	12.70%	1.226%
15	14.133	1956	1963	1975	rVB	1729839	2581268	51.26%	4.948%
16	14.439	2008	2015	2023	rBV2	1605709	2503292	49.71%	4.798%
17	14.627	2040	2047	2056	rBV	523832	769325	15.28%	1.475%
18	15.433	2177	2184	2191	rBV	2288837	3281882	65.17%	6.291%
19	15.545	2197	2203	2215	rVB	402604	578562	11.49%	1.109%
20	17.180	2475	2481	2487	rBV	2107063	3110769	61.77%	5.963%
21	17.221	2487	2488	2492	rVV	55480	60406	1.20%	0.116%
22	17.280	2492	2498	2508	rVB	2514112	3615837	71.80%	6.931%
23	18.080	2627	2634	2643	rBV2	97502	169876	3.37%	0.326%
24	19.239	2827	2831	2837	rVB	139789	194317	3.86%	0.372%
25	19.356	2847	2851	2855	rBV5	43017	61475	1.22%	0.118%
26	19.574	2881	2888	2901	rBV	3261653	4720829	93.75%	9.049%
27	21.080	3140	3144	3150	rBV2	114654	152870	3.04%	0.293%
28	21.286	3175	3179	3182	rBV	72853	85160	1.69%	0.163%
29	21.362	3186	3192	3197	rBV	3287205	4371812	86.82%	8.380%
30	21.974	3293	3296	3304	rBV8	74556	100356	1.99%	0.192%
31	22.956	3459	3463	3467	rVB3	99483	144486	2.87%	0.277%
32	23.492	3546	3554	3566	rVB2	2520849	5035743	100.00%	9.653%
33	23.633	3571	3578	3594	rVB	2307155	4451639	88.40%	8.533%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007078.D
Acq On : 13 Aug 2016 21:06
Operator : UM/SJ
Sample : H4314-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Title : SVOA CALIBRATION


Sum of corrected areas: 52169046

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007078.D
Acq On : 13 Aug 2016 21:06
Operator : UM/SJ
Sample : H4314-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

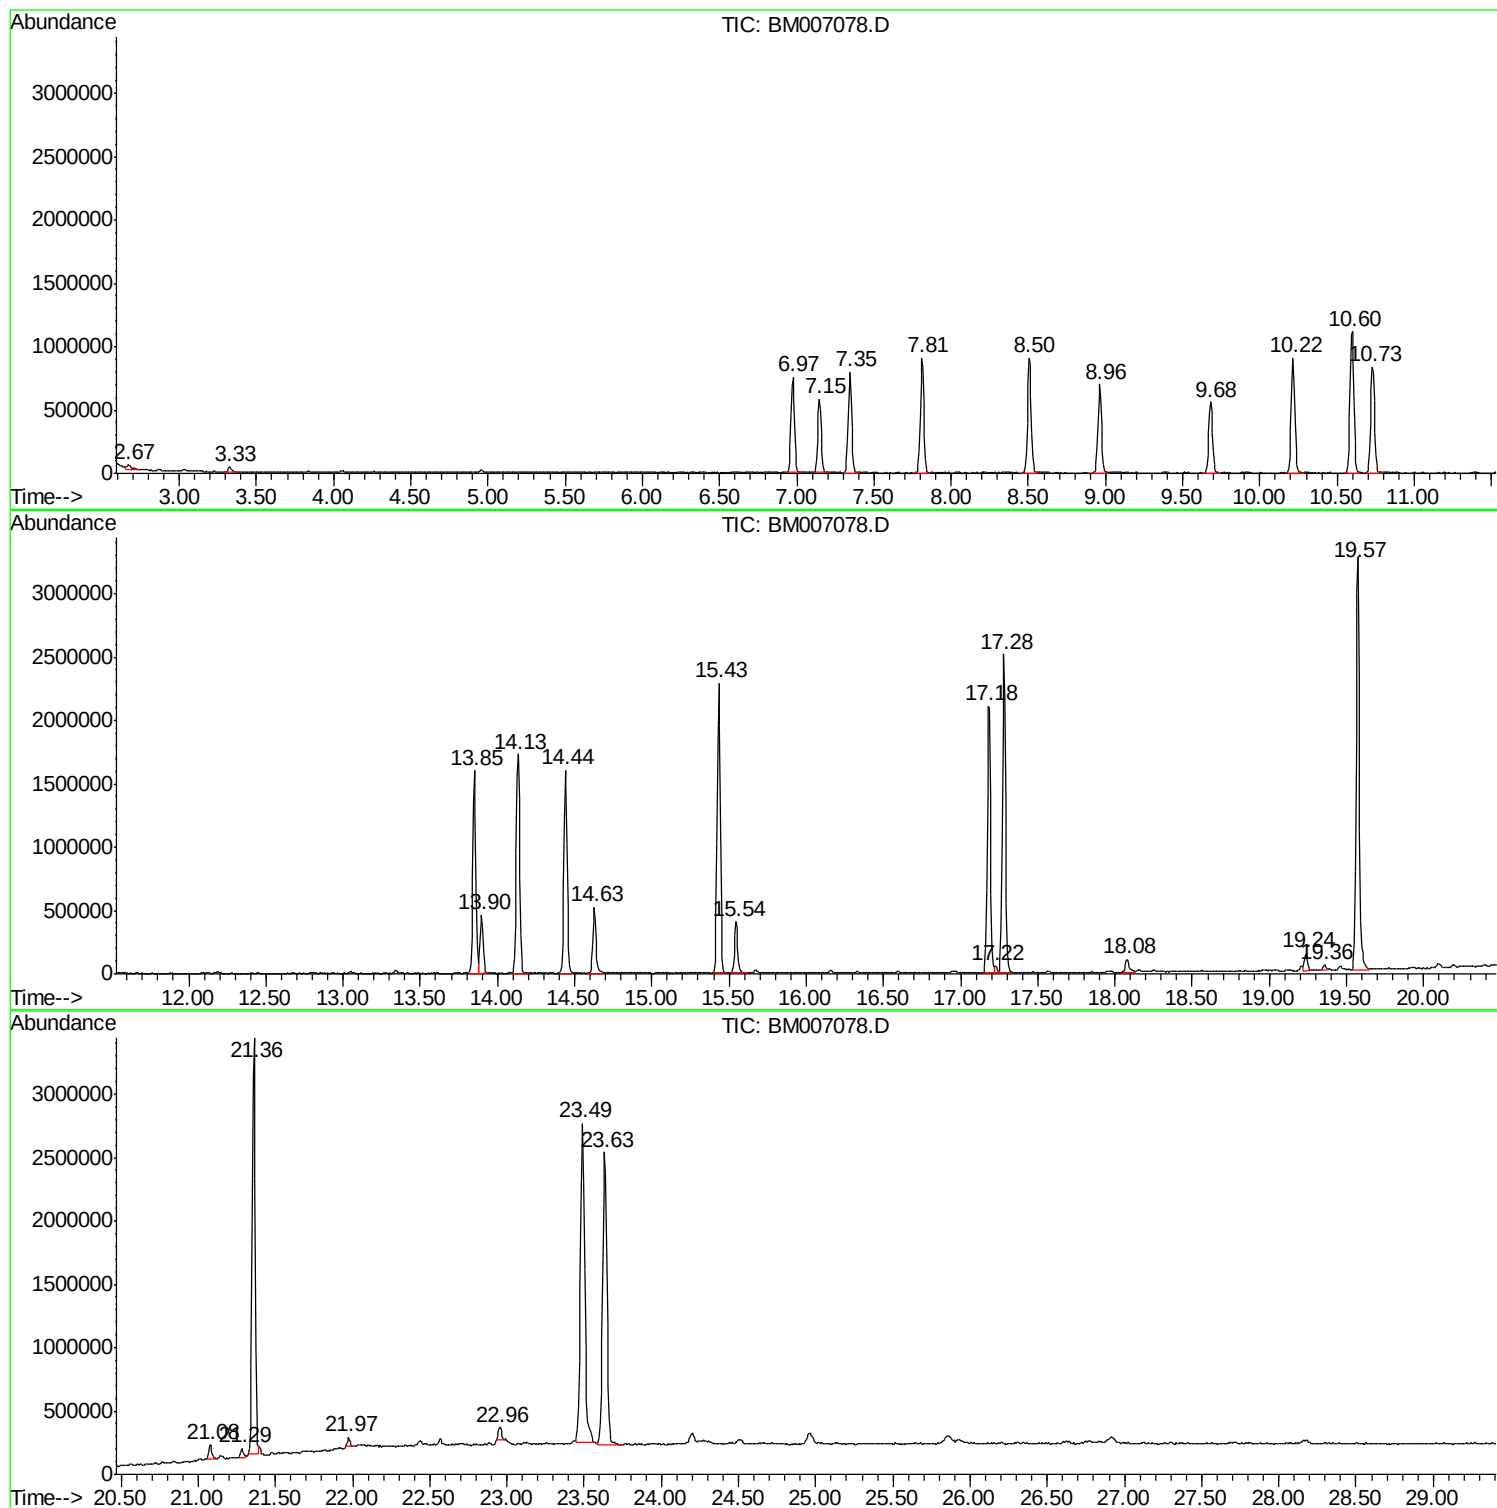

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007078.D
Acq On : 13 Aug 2016 21:06
Operator : UM/SJ
Sample : H4314-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007078.D
Acq On : 13 Aug 2016 21:06
Operator : UM/SJ
Sample : H4314-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc