

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
 Data File : BM007080.D
 Acq On : 13 Aug 2016 22:19
 Operator : UM/SJ
 Sample : H4314-08
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	121	126	133	rVB	52497	72647	1.13%	0.113%
2	6.975	739	746	755	rBV	963532	1538234	23.94%	2.398%
3	7.146	764	775	784	rBV	725934	1130193	17.59%	1.762%
4	7.346	801	809	818	rBV	1025256	1646412	25.62%	2.567%
5	7.810	881	888	898	rBV	1071070	1705788	26.55%	2.659%
6	8.504	998	1006	1014	rBV	1194373	1919395	29.87%	2.992%
7	8.963	1077	1084	1092	rBV	876884	1463091	22.77%	2.281%
8	9.681	1198	1206	1216	rBV	731729	1225013	19.06%	1.910%
9	10.216	1289	1297	1308	rBV	1163707	1980592	30.82%	3.088%
10	10.598	1352	1362	1375	rBV	1316400	2264279	35.24%	3.530%
11	10.728	1375	1384	1397	rBV	1050216	1834411	28.55%	2.860%
12	13.851	1908	1915	1919	rBV	1982810	2783015	43.31%	4.339%
13	13.898	1919	1923	1929	rVB	692721	954707	14.86%	1.488%
14	14.133	1956	1963	1973	rVB	2233233	3263434	50.79%	5.088%
15	14.439	2007	2015	2024	rVB2	1887250	2965521	46.15%	4.623%
16	14.627	2040	2047	2060	rBV	745998	1122041	17.46%	1.749%
17	15.433	2176	2184	2191	rBV	2838612	4186396	65.15%	6.527%
18	15.545	2198	2203	2217	rBV	617970	896304	13.95%	1.397%
19	16.327	2331	2336	2343	rVB3	46483	85119	1.32%	0.133%
20	16.592	2376	2381	2387	rBV5	36866	75051	1.17%	0.117%
21	17.180	2475	2481	2488	rBV2	2458627	3662601	57.00%	5.710%
22	17.280	2491	2498	2509	rVB2	3243099	4635826	72.14%	7.228%
23	18.074	2629	2633	2643	rBV	98083	156816	2.44%	0.244%
24	19.357	2848	2851	2859	rBV5	51572	81077	1.26%	0.126%
25	19.574	2881	2888	2894	rBV	4115208	5784507	90.02%	9.018%
26	21.286	3175	3179	3183	rBV	128804	151120	2.35%	0.236%
27	21.362	3186	3192	3197	rBV	3853595	5044249	78.50%	7.864%
28	23.492	3546	3554	3567	rVV2	3261479	6425757	100.00%	10.018%
29	23.639	3571	3579	3589	rVB	2531902	5086863	79.16%	7.931%


Sum of corrected areas: 64140459

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007080.D
Acq On : 13 Aug 2016 22:19
Operator : UM/SJ
Sample : H4314-08
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

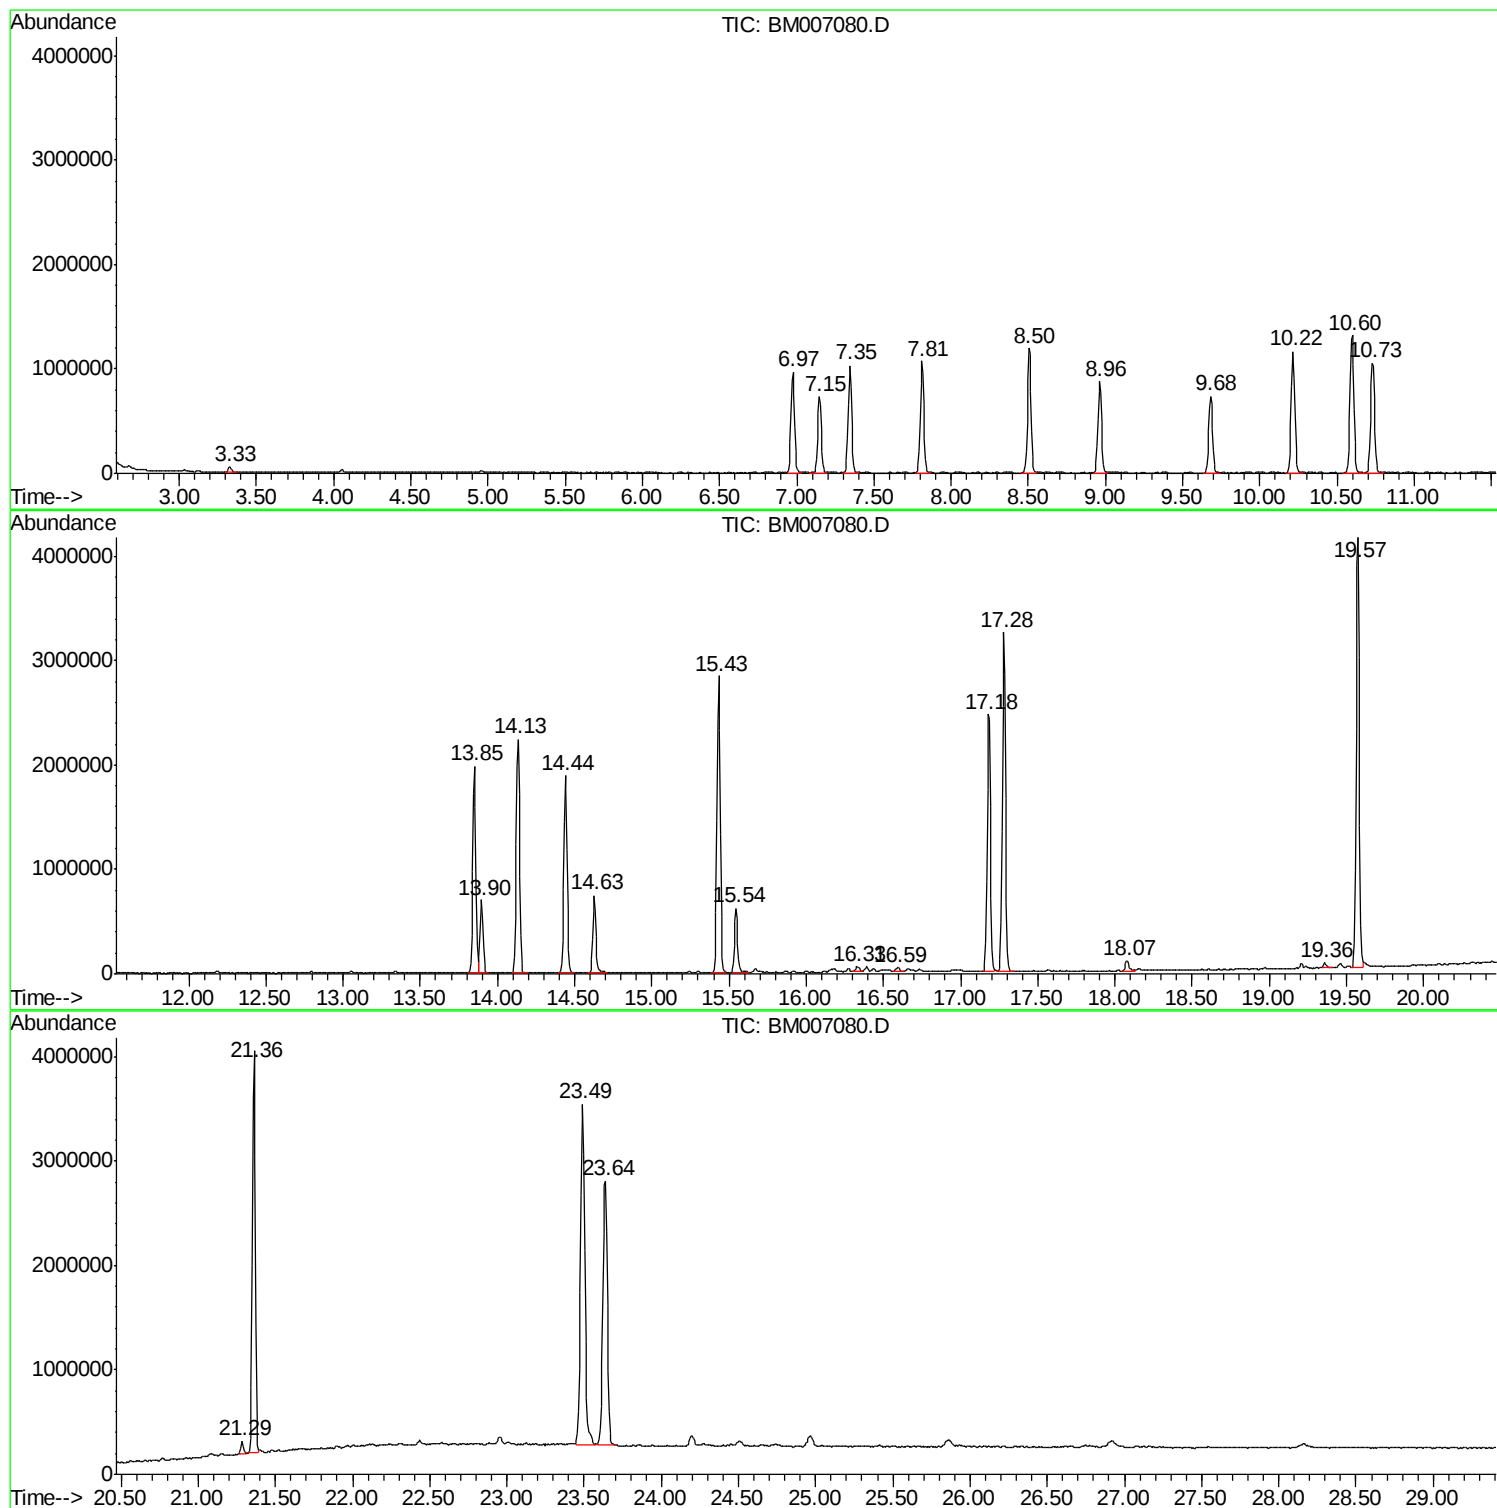

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007080.D
Acq On : 13 Aug 2016 22:19
Operator : UM/SJ
Sample : H4314-08
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007080.D
Acq On : 13 Aug 2016 22:19
Operator : UM/SJ
Sample : H4314-08
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJT7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc