

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
 Data File : BM007089.D
 Acq On : 14 Aug 2016 03:46
 Operator : UM/SJ
 Sample : H4314-19
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJW7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.969	738	745	758	rBV	726392	1184073	21.35%	2.158%
2	7.146	768	775	785	rVB	556009	867710	15.65%	1.581%
3	7.340	802	808	821	rVB	769827	1239729	22.36%	2.259%
4	7.810	881	888	897	rVB	930822	1490645	26.88%	2.717%
5	8.504	999	1006	1017	rBV2	877016	1431992	25.82%	2.610%
6	8.963	1076	1084	1094	rBV	681760	1156470	20.85%	2.108%
7	9.681	1199	1206	1216	rVB	552013	938028	16.92%	1.710%
8	10.210	1289	1296	1306	rBV	942329	1550799	27.97%	2.826%
9	10.592	1353	1361	1369	rBV	1173172	1976485	35.64%	3.602%
10	10.728	1377	1384	1393	rBV	844913	1463368	26.39%	2.667%
11	13.845	1908	1914	1919	rBV	1604000	2369966	42.74%	4.319%
12	13.898	1919	1923	1930	rVB	1141619	1595905	28.78%	2.908%
13	14.127	1956	1962	1972	rVB	1771793	2709554	48.86%	4.938%
14	14.439	2008	2015	2024	rVB2	1669034	2554749	46.07%	4.656%
15	14.627	2040	2047	2062	rBV	440533	693824	12.51%	1.264%
16	15.433	2177	2184	2196	rVB	2442533	3486747	62.88%	6.354%
17	15.545	2197	2203	2214	rBV	405131	577102	10.41%	1.052%
18	17.180	2474	2481	2487	rBV	2202929	3146908	56.75%	5.735%
19	17.280	2492	2498	2507	rVB2	2601692	3764469	67.88%	6.861%
20	17.568	2541	2547	2556	rBV5	48312	72879	1.31%	0.133%
21	18.074	2625	2633	2642	rBV4	81684	138244	2.49%	0.252%
22	19.233	2827	2830	2835	rVB	88793	124590	2.25%	0.227%
23	19.574	2881	2888	2902	rBV	3409541	4944630	89.17%	9.011%
24	20.109	2974	2979	2986	rVB2	113693	142172	2.56%	0.259%
25	21.362	3186	3192	3197	rBV	3372382	4516041	81.44%	8.230%
26	22.950	3458	3462	3467	rBV	185937	259508	4.68%	0.473%
27	23.486	3546	3553	3568	rVB2	2756777	5545370	100.00%	10.106%
28	23.633	3570	3578	3592	rVB	2312760	4616906	83.26%	8.414%
29	24.191	3670	3673	3681	rVB2	171549	312256	5.63%	0.569%


Sum of corrected areas: 54871119

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007089.D
Acq On : 14 Aug 2016 03:46
Operator : UM/SJ
Sample : H4314-19
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJW7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

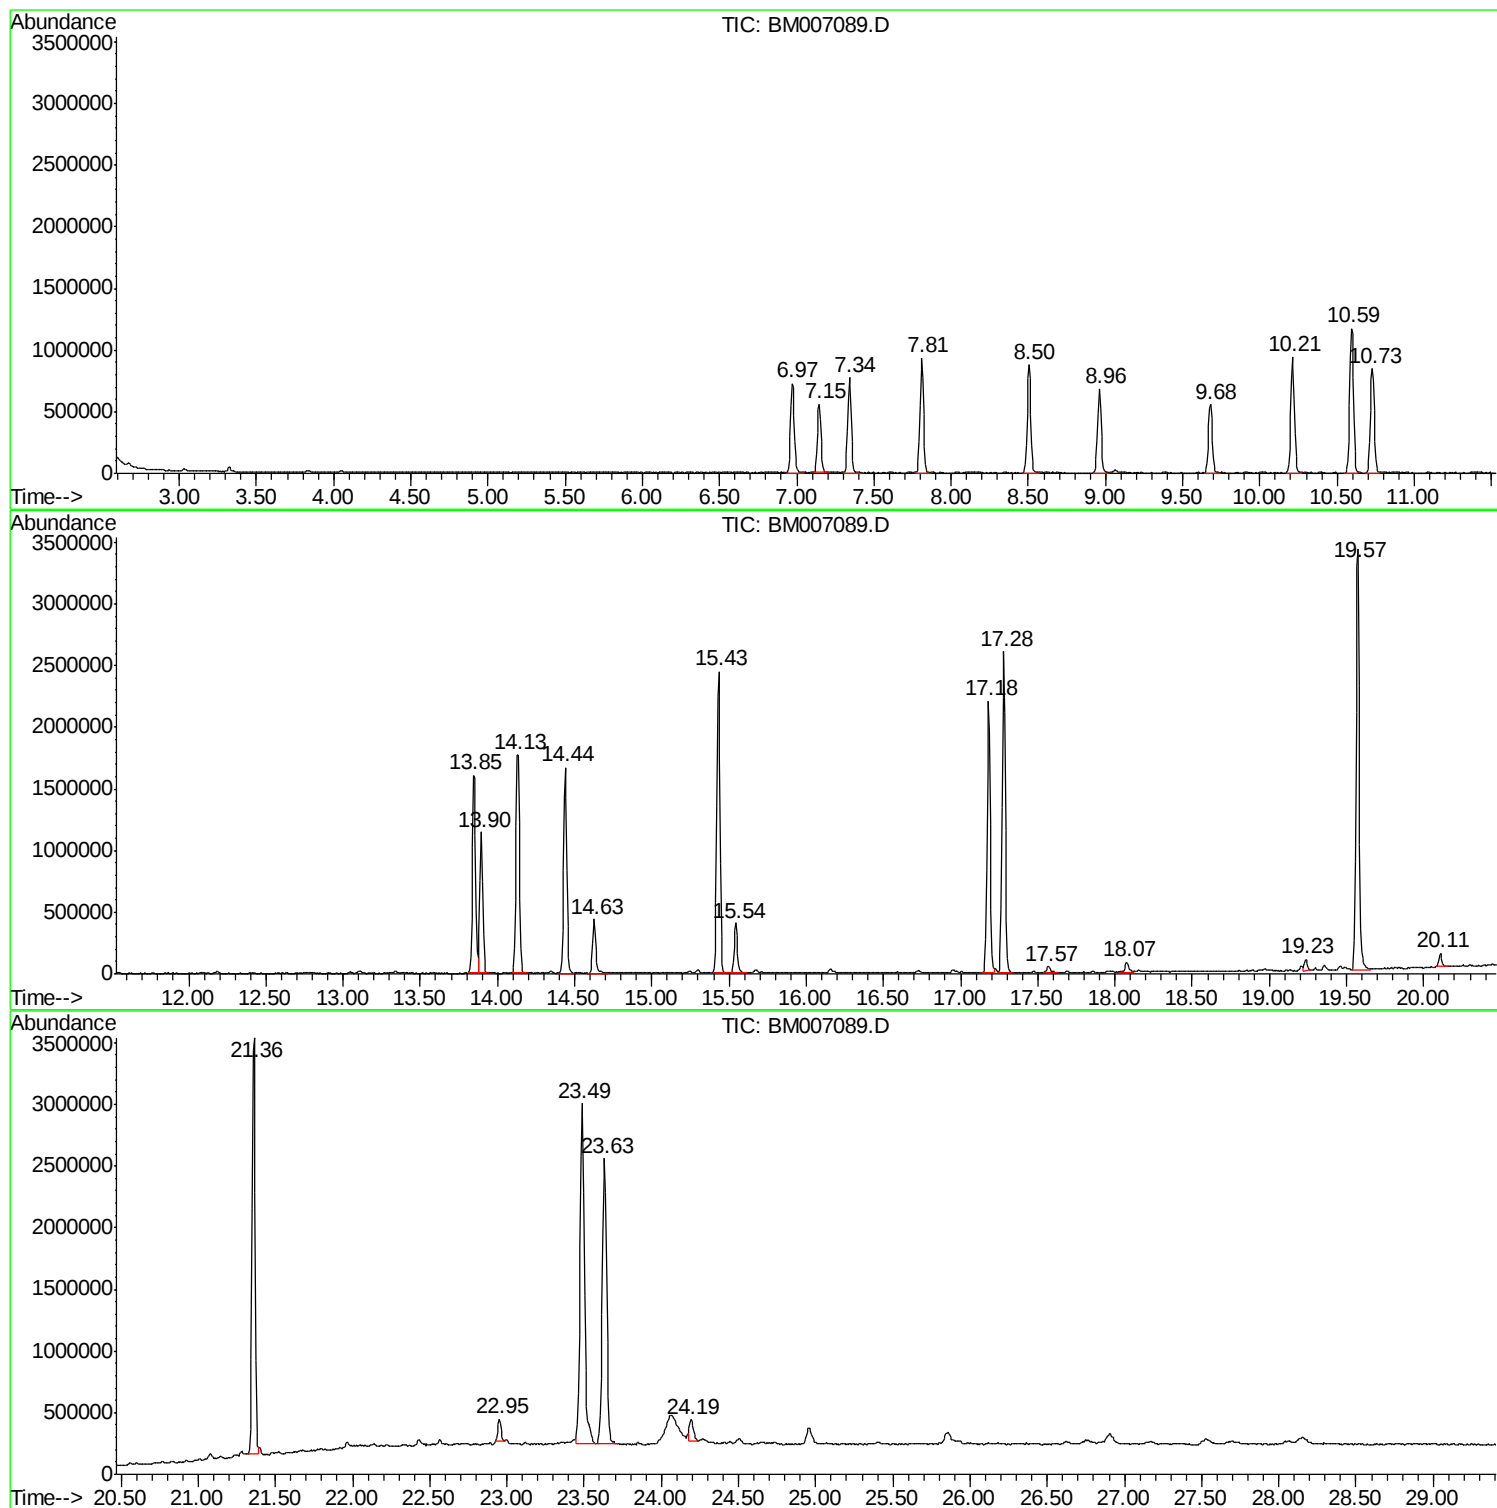

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007089.D
Acq On : 14 Aug 2016 03:46
Operator : UM/SJ
Sample : H4314-19
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJW7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081316\
Data File : BM007089.D
Acq On : 14 Aug 2016 03:46
Operator : UM/SJ
Sample : H4314-19
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJW7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc