

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081320\
 Data File : BM027096.D
 Acq On : 14 Aug 2020 19:43
 Operator : JU/CG
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD02023

Quant Time: Aug 17 01:23:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 13 11:47:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	93472	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	328201	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	222746	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	511631	20.00	ng/ul	0.00
78) Chrysene-d12	21.21	240	598580	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	614069	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	18204	8.85	ng/uL	0.00
5) Phenol-d5	6.82	99	137959	18.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	94660	19.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	114091	19.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	107202	18.92	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	51242	19.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	56663	21.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	126079	22.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	135528	20.58	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	351956	19.81	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	426652	20.16	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	58313	19.45	ng/ul	0.00
58) Fluorene-d10	15.27	176	320547	20.70	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	47963	17.16	ng/ul	0.00
71) Anthracene-d10	17.12	188	507621	20.14	ng/ul	0.00
79) Pyrene-d10	19.41	212	587649	19.68	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	692259	20.20	ng/ul	0.00

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) 1,4-Dioxane	3.23	88	20611	7.882	ng/uL	92
4) Benzaldehyde	6.79	77	106515	15.076	ng/ul	99
6) Phenol	6.85	94	151812	19.810	ng/ul	99
8) Bis(2-Chloroethyl)ether	7.07	93	118914	18.800	ng/ul	97
10) 2-Chlorophenol	7.21	128	119728	19.984	ng/ul	98
11) 2-Methylphenol	8.08	108	108832	19.551	ng/ul	99
12) 2,2'-oxybis(1-Chloropropan	8.17	45	84172	17.468	ng/ul#	93
14) Acetophenone	8.45	105	185994	19.531	ng/ul	98
15) N-Nitroso-di-n-propylamine	8.44	70	107337	19.428	ng/ul	96
16) 4-Methylphenol	8.40	108	115514	19.310	ng/ul	95
17) Hexachloroethane	8.71	117	54885	18.315	ng/ul	92
20) Nitrobenzene	8.82	77	167792	19.757	ng/ul	98
21) Isophorone	9.35	82	262014	19.443	ng/ul	99
23) 2-Nitrophenol	9.53	139	63489	21.231	ng/ul	96
24) 2,4-Dimethylphenol	9.60	107	142082	20.830	ng/ul	99
25) Bis(2-Chloroethoxy)methane	9.83	93	152143	19.928	ng/ul	98
27) 2,4-Dichlorophenol	10.06	162	127055	22.303	ng/ul	99
28) Naphthalene	10.46	128	362529	19.873	ng/ul	100
30) 4-Chloroaniline	10.57	127	142595	21.493	ng/ul	99
31) Hexachlorobutadiene	10.76	225	106012	22.073	ng/ul	99
32) Caprolactam	11.33	113	30227	19.088	ng/ul	92
33) 4-Chloro-3-methylphenol	11.70	107	124117	20.618	ng/ul	99
34) 2-Methylnaphthalene	12.08	142	272270	20.351	ng/ul	100

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081320\
 Data File : BM027096.D
 Acq On : 14 Aug 2020 19:43
 Operator : JU/CG
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD02023

Quant Time: Aug 17 01:23:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 13 11:47:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 1-Methylnaphthalene	12.30	142	254725	19.340	ng/ul#	97
37) 1,2,4,5-Tetrachlorobenzene	12.46	216	182750	22.171	ng/ul	96
38) Hexachlorocyclopentadiene	12.45	237	77723	14.301	ng/ul	99
39) 2,4,6-Trichlorophenol	12.70	196	108595	22.415	ng/ul	93
40) 2,4,5-Trichlorophenol	12.77	196	115662	22.432	ng/ul	91
41) 1,1'-Biphenyl	13.10	154	364367	20.017	ng/ul	99
42) 2-Chloronaphthalene	13.14	162	302330	20.485	ng/ul	97
43) 2-Nitroaniline	13.34	65	87943	20.571	ng/ul	97
45) Dimethylphthalate	13.73	163	369895	19.871	ng/ul	99
46) 2,6-Dinitrotoluene	13.84	165	72937	20.579	ng/ul	99
48) Acenaphthylene	13.99	152	430436	20.003	ng/ul	99
49) 3-Nitroaniline	14.17	138	67797	21.524	ng/ul	96
50) Acenaphthene	14.33	153	302837	19.857	ng/ul	99
51) 2,4-Dinitrophenol	14.38	184	31197	16.937	ng/ul	92
53) 4-Nitrophenol	14.49	109	67705	21.206	ng/ul	98
54) Dibenzofuran	14.67	168	450400	20.637	ng/ul	99
55) 2,4-Dinitrotoluene	14.63	165	108664	21.112	ng/ul	96
56) 2,3,4,6-Tetrachlorophenol	14.90	232	106995	23.024	ng/ul	93
57) Diethylphthalate	15.11	149	376478	20.163	ng/ul	99
59) Fluorene	15.32	166	374201	20.488	ng/ul	99
60) 4-Chlorophenyl-phenylether	15.33	204	206645	20.761	ng/ul	96
61) 4-Nitroaniline	15.33	138	74177	20.618	ng/ul	95
64) 4,6-Dinitro-2-methylphenol	15.40	198	51250	16.572	ng/ul	99
65) N-Nitrosodiphenylamine	15.53	169	319722	20.858	ng/ul	99
66) 4-Bromophenyl-phenylether	16.22	248	132739	20.743	ng/ul	96
67) Hexachlorobenzene	16.33	284	156036	20.791	ng/ul	96
68) Atrazine	16.49	200	120352	19.364	ng/ul	99
69) Pentachlorophenol	16.67	266	86426	20.781	ng/ul	97
70) Phenanthrene	17.06	178	609931	19.885	ng/ul	99
72) Anthracene	17.14	178	625453	20.040	ng/ul	99
73) 1,2,3,4-Tetrachlorobenzene	13.07	216	179167	22.390	ng/uL	100
74) Pentachlorobenzene	14.60	250	176525	21.149	ng/uL	99
75) Carbazole	17.42	167	528433	20.059	ng/ul	99
76) Di-n-butylphthalate	18.00	149	616210	19.089	ng/ul	100
77) Fluoranthene	19.08	202	748559	20.126	ng/ul	96
80) Pyrene	19.44	202	788992	19.419	ng/ul	96
81) Butylbenzylphthalate	20.36	149	276260	18.499	ng/ul	98
82) 3,3'-Dichlorobenzidine	21.13	252	259383	19.203	ng/ul	100
83) Benzo(a)anthracene	21.20	228	816490	20.262	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	21.15	149	385539	17.089	ng/ul	99
85) Chrysene	21.24	228	795314	20.107	ng/ul	99
87) Di-n-octyl phthalate	22.02	149	695267	16.923	ng/ul	100
88) Benzo(b)fluoranthene	22.75	252	861205	20.197	ng/ul	99
89) Benzo(k)fluoranthene	22.80	252	838182	19.834	ng/ul	99
91) Benzo(a)pyrene	23.31	252	752752	19.398	ng/ul	100
92) Indeno(1,2,3-cd)pyrene	25.61	276	964756	19.294	ng/ul	97
93) Dibenzo(a,h)anthracene	25.61	278	819975	19.360	ng/ul	99
94) Benzo(a,h,i)perylene	26.27	276	776484	18.801	ng/ul	99

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081320\
 Data File : BM027096.D
 Acq On : 14 Aug 2020 19:43
 Operator : JU/CG
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SSTD02023

Quant Time: Aug 17 01:23:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 13 11:47:07 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)




(#) = qualifier out of range (m) = manual integration (+) = signals summed						

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081320\
 Data File : BM027096.D
 Acq On : 14 Aug 2020 19:43
 Operator : JU/CG
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 SSTD02023

Quant Time: Aug 17 01:23:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 13 11:47:07 2020
 Response via : Initial Calibration




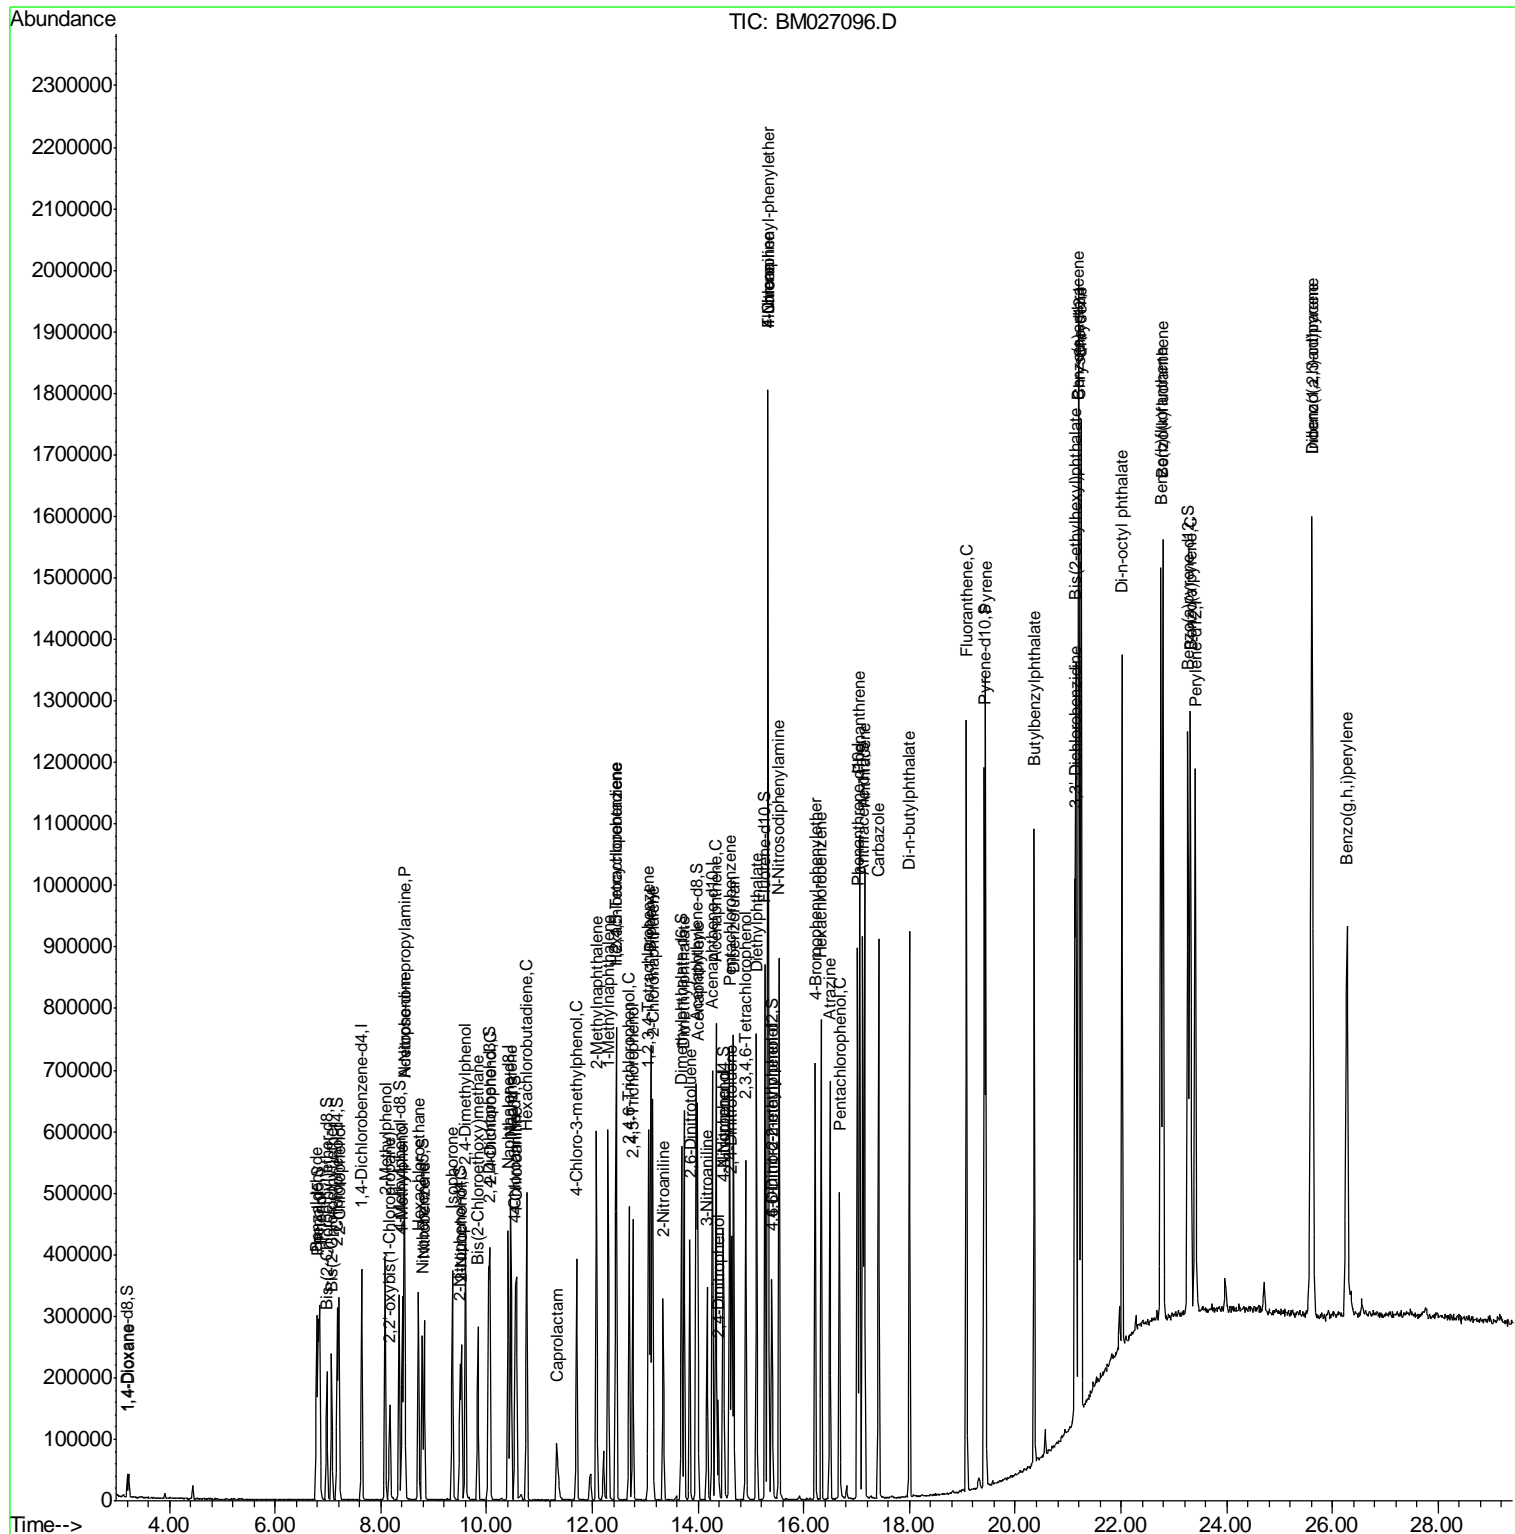




#2
 1,4-Dioxane
 Concen: 7.882 ng/uL
 RT: 3.23 min Scan# 42
 Delta R.T. 0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43


Instrument :
 BNA_M
ClientSampled :
 SST02023


Tgt Ion	Resp	Lower	Upper
88	100		
43	22.3	21.4	32.0
58	52.3	46.9	70.3

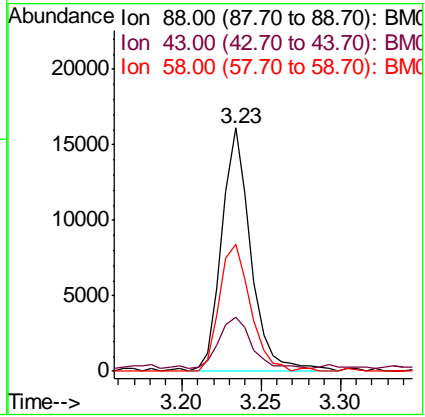

#4
 Benzaldehyde
 Concen: 15.076 ng/ul
 RT: 6.79 min Scan# 646
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
77	100		
105	84.5	65.9	98.9
106	79.1	63.3	94.9




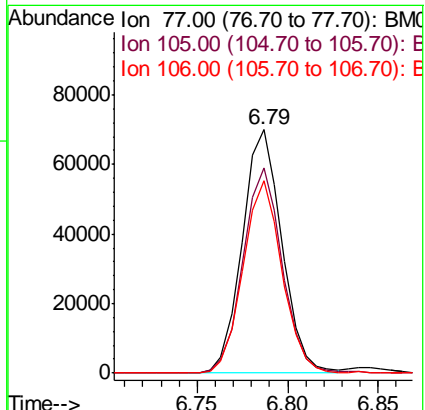


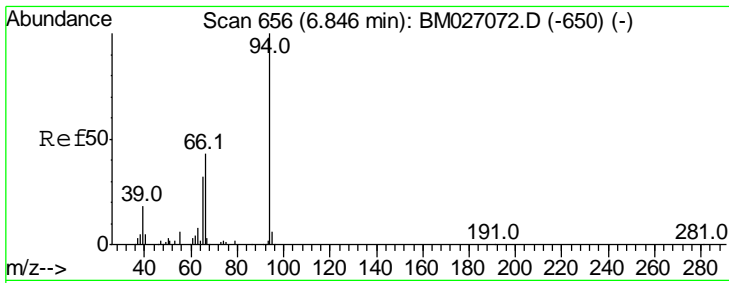

#6
 Phenol
 Concen: 19.810 ng/ul
 RT: 6.85 min Scan# 656
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
94	151812		
65	36.5	28.6	43.0
66	51.5	41.3	61.9

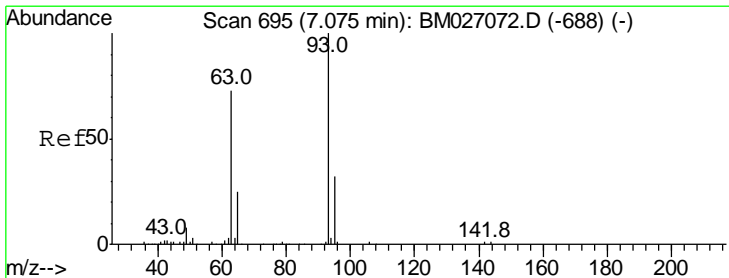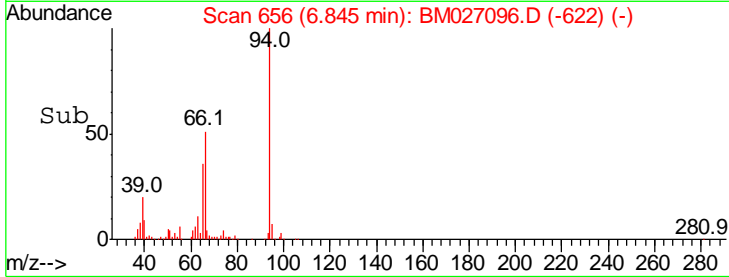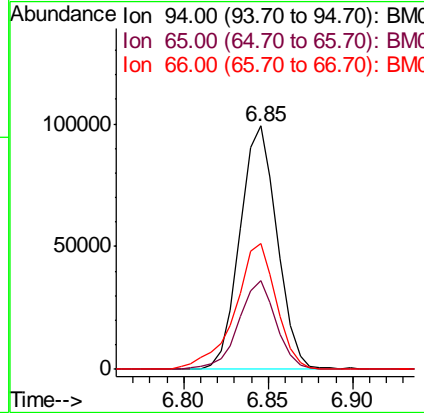

#8
 Bis(2-Chloroethyl)ether
 Concen: 18.800 ng/ul
 RT: 7.07 min Scan# 694
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
93	118914		
63	73.4	61.9	92.9
95	33.7	26.6	40.0


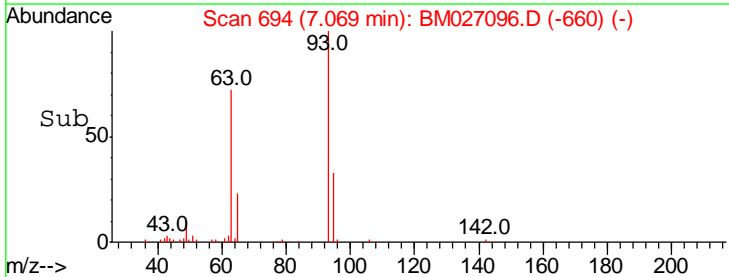
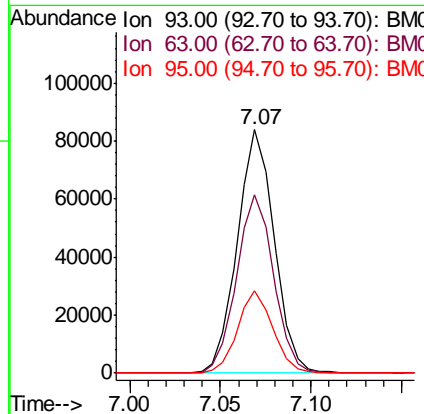
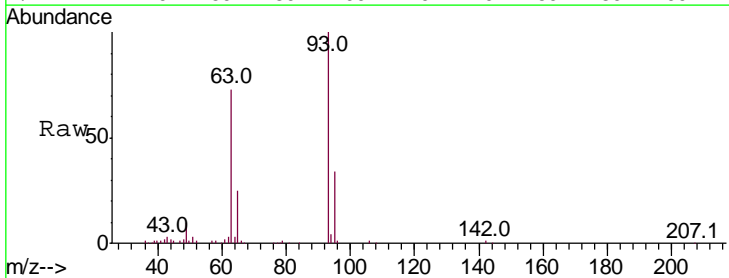




#10
 2-Chlorophenol
 Concen: 19.984 ng/ul
 RT: 7.21 min Scan# 718
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
ClientSampled :
 SST02023


Tgt Ion	Resp	Lower	Upper
128	119728		
64	51.6	39.4	59.2
130	32.4	25.4	38.2

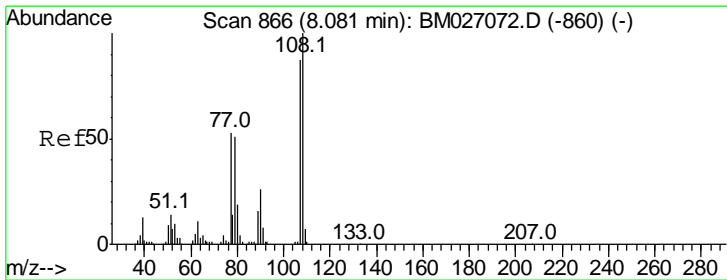

#11
 2-Methylphenol
 Concen: 19.551 ng/ul
 RT: 8.08 min Scan# 866
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
108	108832		
107	90.2	71.8	107.6








#12
 2,2'-oxybis(1-Chloropropane)
 Concen: 17.468 ng/ul
 RT: 8.17 min Scan# 882
 Delta R.T. 0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43





Instrument :
 BNA_M
 ClientSampled :
 SSTD02023




Tgt Ion	Resp	Lower	Upper
45	100		
77	30.7	22.2	33.2
79	24.6	16.3	24.5#



#14
 Acetophenone
 Concen: 19.531 ng/ul
 RT: 8.45 min Scan# 929
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
105	100		
77	93.3	75.7	113.5
51	22.0	19.1	28.7



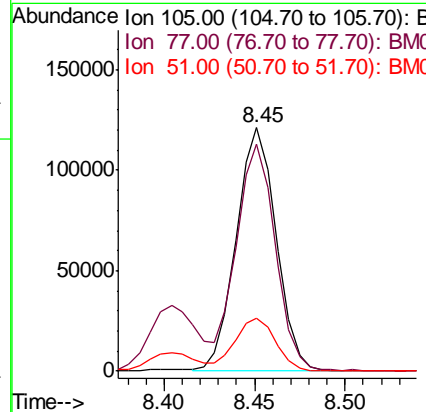



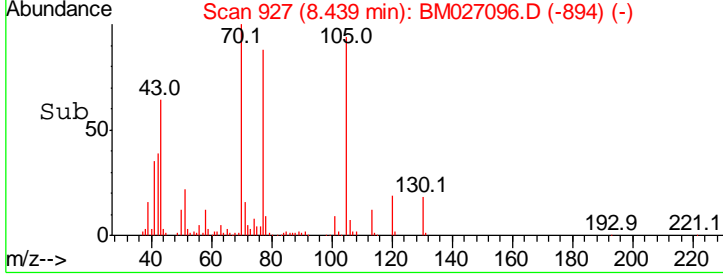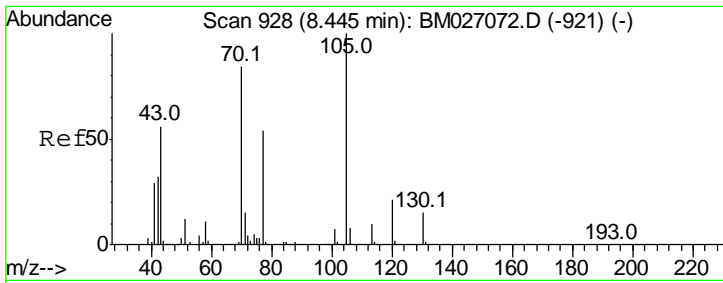

#15
 N-Nitroso-di-n-propylamine
 Concen: 19.428 ng/ul
 RT: 8.44 min Scan# 927
 Delta R.T. -0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43


Instrument :
 BNA_M
ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
70	100		
42	38.8	34.2	51.2
101	8.5	6.8	10.2
130	18.0	15.1	22.7

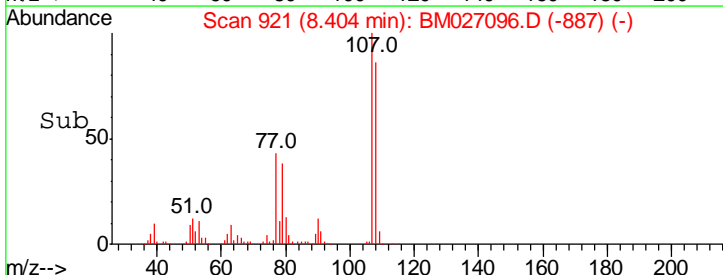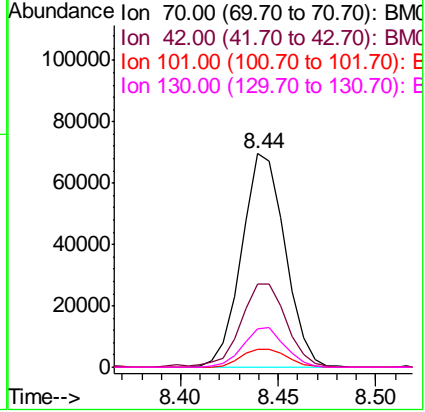

#16
 4-Methylphenol
 Concen: 19.310 ng/ul
 RT: 8.40 min Scan# 921
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
108	100		
107	116.8	89.2	133.8




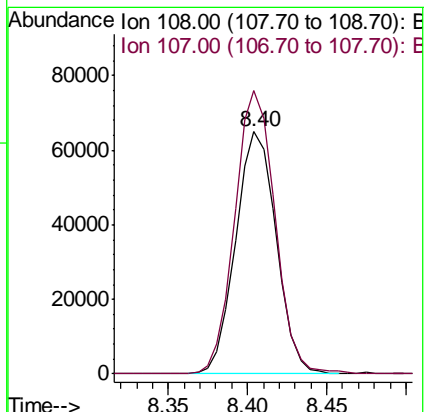


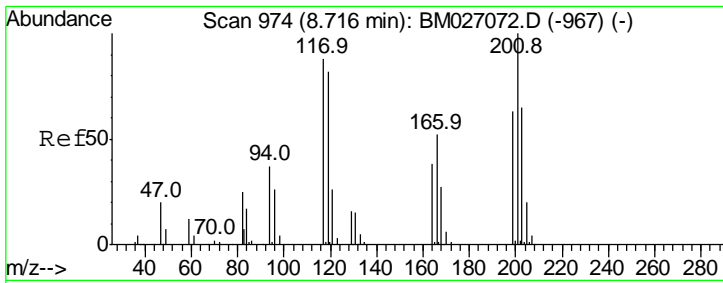

#17
 Hexachloroethane
 Concen: 18.315 ng/ul
 RT: 8.71 min Scan# 973
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
117	54885		
117	100		
201	116.7	87.8	131.8
199	74.7	53.6	80.4

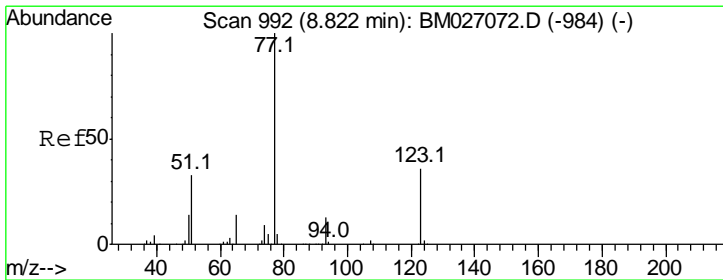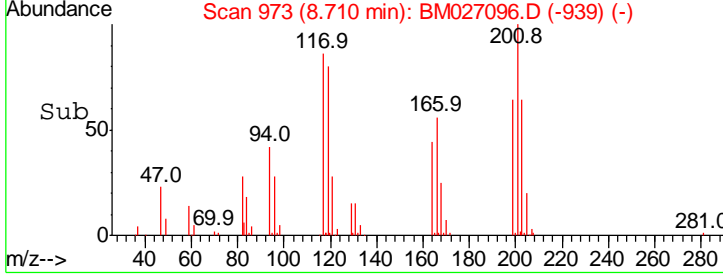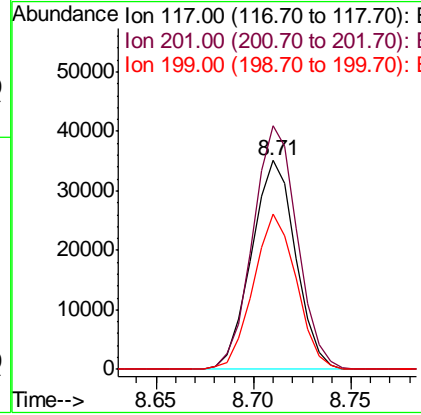

#20
 Nitrobenzene
 Concen: 19.757 ng/ul
 RT: 8.82 min Scan# 992
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
77	167792		
77	100		
123	35.6	29.7	44.5
65	14.0	11.7	17.5

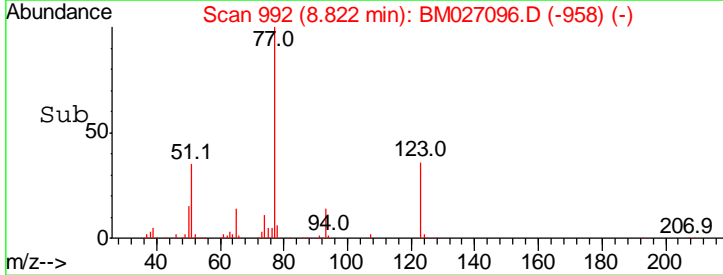
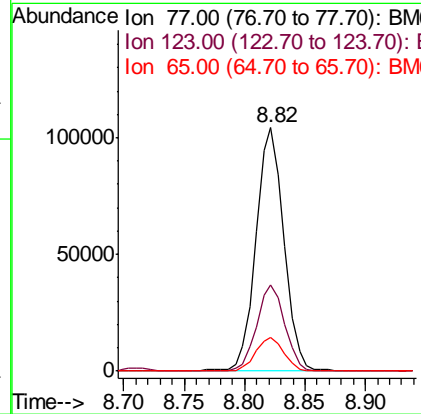





#21
 Isophorone
 Concen: 19.443 ng/ul
 RT: 9.35 min Scan# 1082
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43





Instrument :
 BNA_M
ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
82	100		
95	8.5	6.6	9.8
138	16.0	12.6	19.0

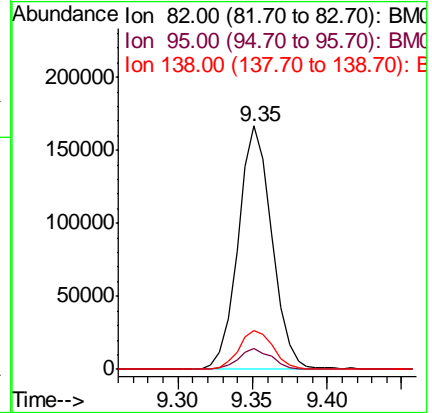

#23
 2-Nitrophenol
 Concen: 21.231 ng/ul
 RT: 9.53 min Scan# 1112
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
139	100		
65	64.5	54.5	81.7
109	40.9	31.4	47.0


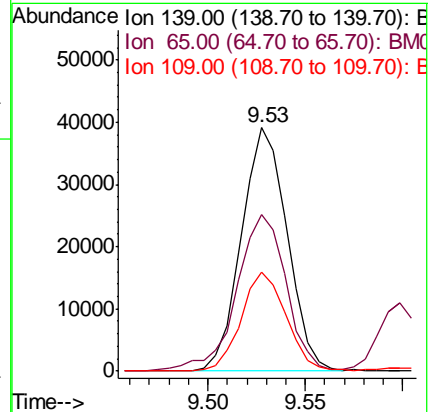



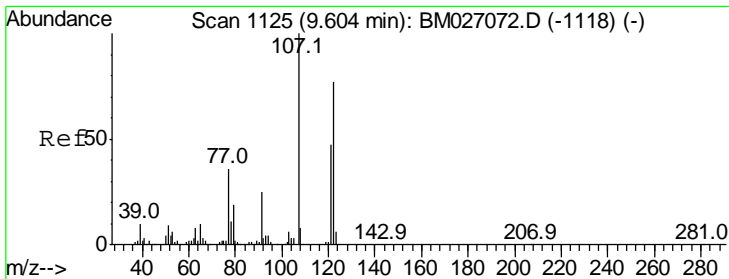

#24
 2,4-Dimethylphenol
 Concen: 20.830 ng/ul
 RT: 9.60 min Scan# 1124
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43





Instrument :
 BNA_M
ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
107	100		
121	44.1	35.4	53.2
122	77.4	60.8	91.2

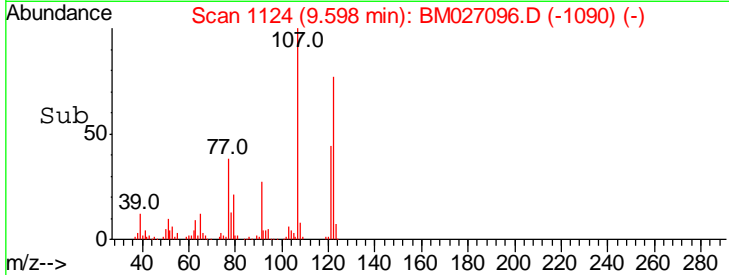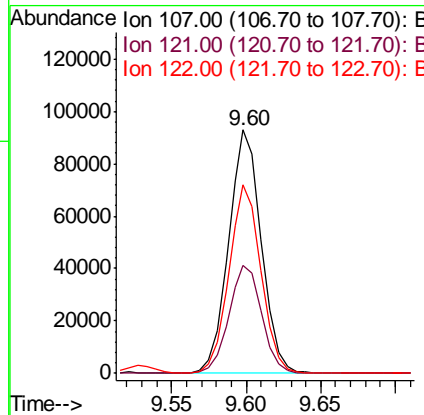

#25
 Bis(2-Chloroethoxy)methane
 Concen: 19.928 ng/ul
 RT: 9.83 min Scan# 1164
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
93	100		
95	31.8	26.3	39.5
123	11.0	8.3	12.5

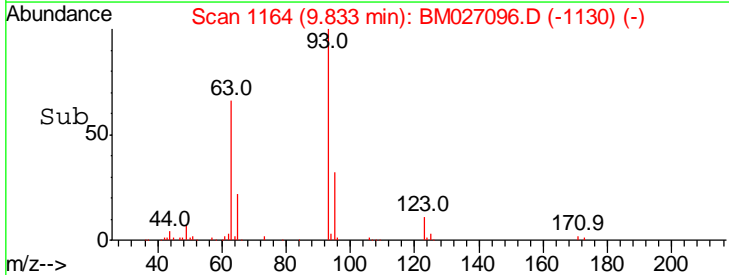

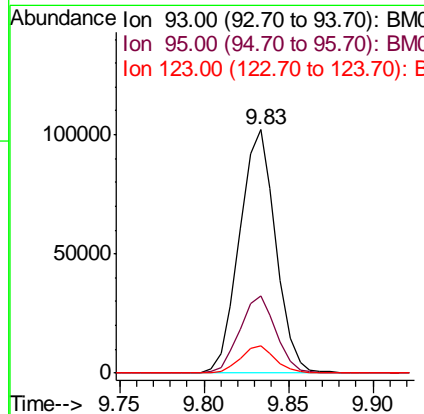
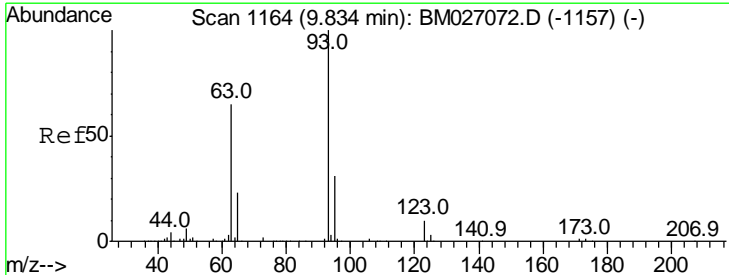




#27
 2,4-Dichlorophenol
 Concen: 22.303 ng/ul
 RT: 10.06 min Scan# 1203
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SST02023


Tgt Ion	Resp	Lower	Upper
162	100		
164	64.1	51.4	77.2
98	34.3	28.4	42.6

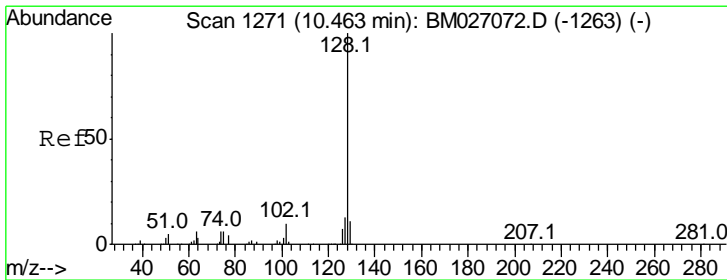

#28
 Naphthalene
 Concen: 19.873 ng/ul
 RT: 10.46 min Scan# 1270
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
128	100		
129	11.4	9.0	13.6
127	13.4	10.5	15.7




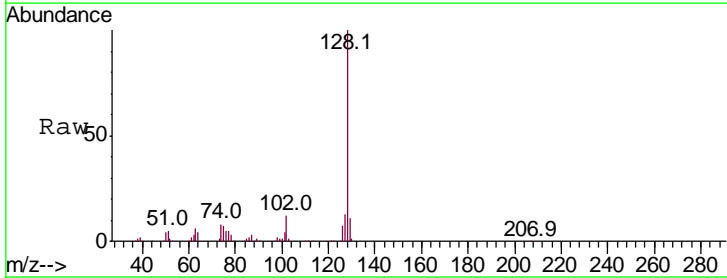




#30
 4-Chloroaniline
 Concen: 21.493 ng/ul
 RT: 10.57 min Scan# 1289
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampleID :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
127	100		
129	31.8	24.9	37.3



#31
 Hexachlorobutadiene
 Concen: 22.073 ng/ul
 RT: 10.76 min Scan# 1321
 Delta R.T. -0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
225	100		
223	62.6	49.8	74.8
227	64.1	52.5	78.7









#32
 Caprolactam
 Concen: 19.088 ng/ul
 RT: 11.33 min Scan# 1418
 Delta R.T. 0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
113	100		
55	118.2	101.3	151.9
56	103.9	90.9	136.3



#33
 4-Chloro-3-methylphenol
 Concen: 20.618 ng/ul
 RT: 11.70 min Scan# 1482
 Delta R.T. 0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
107	100		
144	24.5	20.7	31.1
142	77.6	62.6	94.0









#34
 2-Methylnaphthalene
 Concen: 20.351 ng/ul
 RT: 12.08 min Scan# 1546
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SST02023


Tgt Ion	Ratio	Lower	Upper
142	100		
141	90.8	72.4	108.6



#35
 1-Methylnaphthalene
 Concen: 19.340 ng/ul
 RT: 12.30 min Scan# 1583
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Ratio	Lower	Upper
142	100		
141	93.0	72.2	108.2
116	5.0	3.4	5.0#









#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 22.171 ng/ul
 RT: 12.46 min Scan# 1610
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampleID :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
216	182750		
216	100		
214	80.7	61.4	92.2
179	20.8	16.8	25.2
108	15.5	13.7	20.5

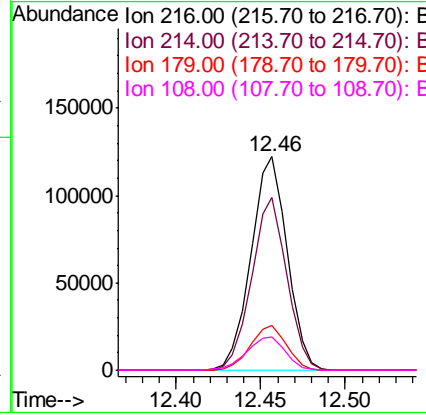

#38
 Hexachlorocyclopentadiene
 Concen: 14.301 ng/ul
 RT: 12.45 min Scan# 1608
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
237	77723		
237	100		
235	61.2	49.5	74.3
272	13.0	9.4	14.0









#39
 2,4,6-Trichlorophenol
 Concen: 22.415 ng/ul
 RT: 12.70 min Scan# 1651
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Instrument :
 BNA_M
 ClientSampled :
 SSTD02023

Tgt Ion:196 Resp: 108595




Ion	Ratio	Lower	Upper
196	100		
198	97.2	72.1	108.1
200	31.8	23.4	35.2

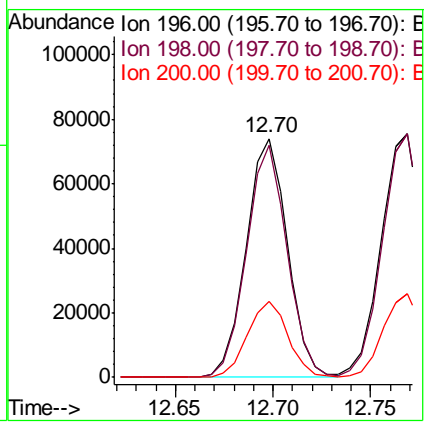


#40
 2,4,5-Trichlorophenol
 Concen: 22.432 ng/ul
 RT: 12.77 min Scan# 1663
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion:196 Resp: 115662

Ion	Ratio	Lower	Upper
196	100		
198	100.1	72.7	109.1
200	34.2	24.6	36.8


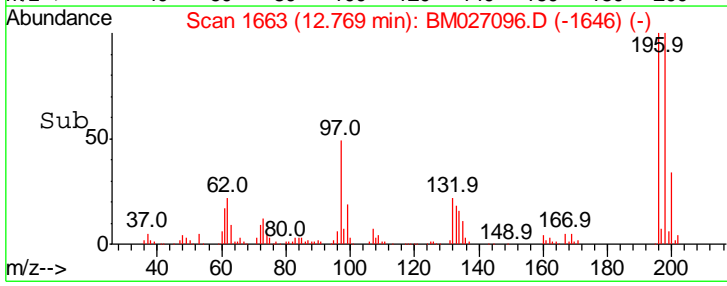
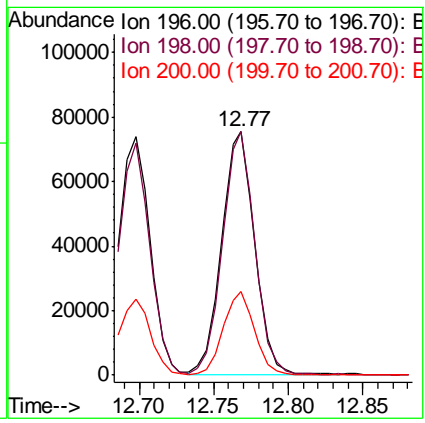





#41
 1,1'-Biphenyl
 Concen: 20.017 ng/ul
 RT: 13.10 min Scan# 1720
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SST02023


Tgt Ion	Resp	Lower	Upper
154	100		
153	39.9	31.6	47.4
76	10.9	9.3	13.9

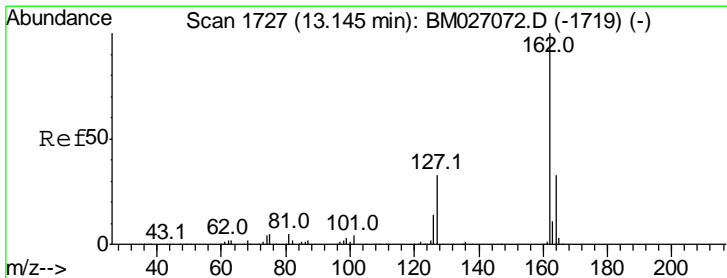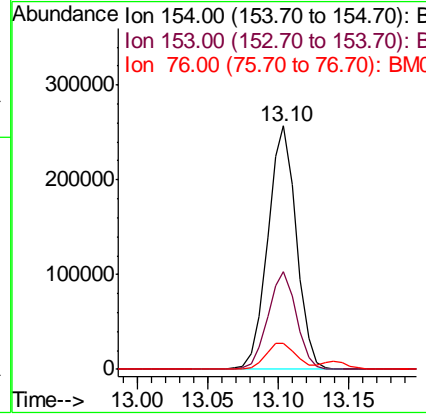

#42
 2-Chloronaphthalene
 Concen: 20.485 ng/ul
 RT: 13.14 min Scan# 1726
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
162	100		
164	31.8	26.5	39.7
127	35.8	30.0	45.0








#43
 2-Nitroaniline
 Concen: 20.571 ng/ul
 RT: 13.34 min Scan# 1760
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43





Instrument :
 BNA_M
 ClientSampleId :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
65	100		
92	64.1	50.5	75.7
138	88.4	74.6	111.8

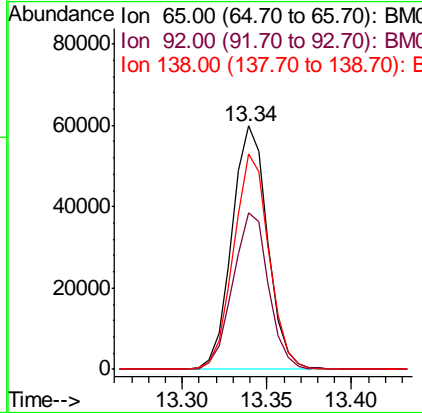

#45
 Dimethylphthalate
 Concen: 19.871 ng/ul
 RT: 13.73 min Scan# 1827
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
163	100		
194	4.2	3.2	4.8
164	9.9	8.2	12.2



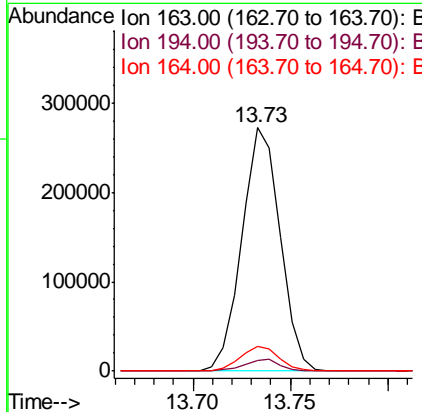





#46
 2,6-Dinitrotoluene
 Concen: 20.579 ng/ul
 RT: 13.84 min Scan# 1846
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
165	100		
89	69.6	56.1	84.1
121	20.9	17.9	26.9

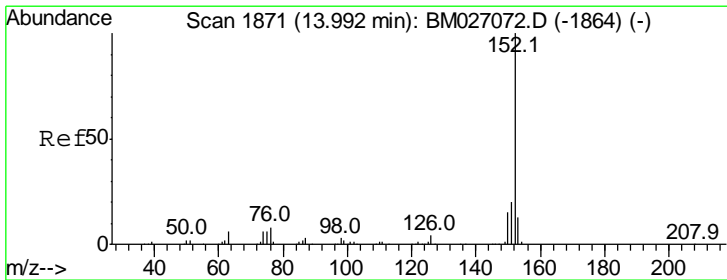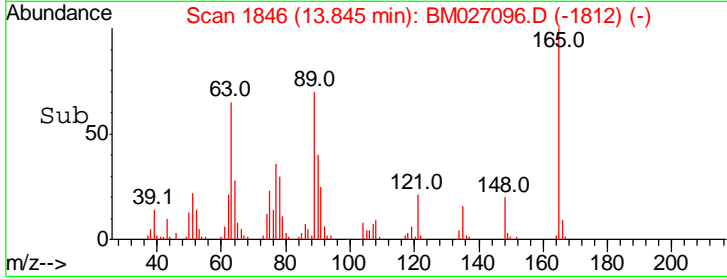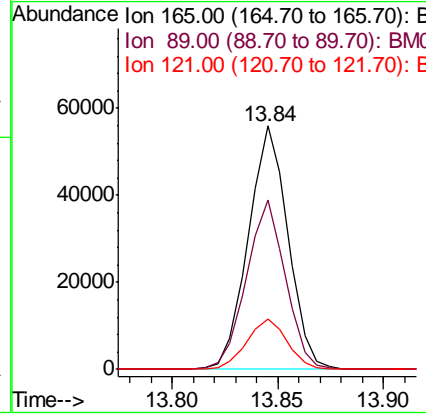

#48
 Acenaphthylene
 Concen: 20.003 ng/ul
 RT: 13.99 min Scan# 1871
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
152	100		
151	20.2	15.9	23.9
153	13.0	9.8	14.8



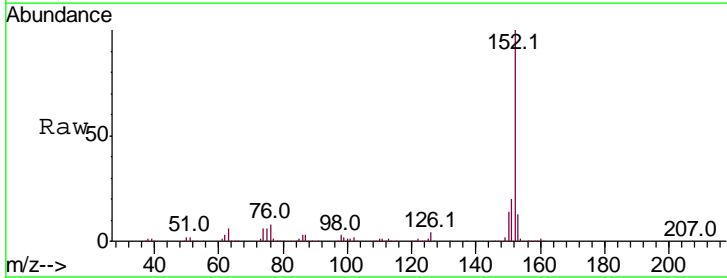




#49
 3-Nitroaniline
 Concen: 21.524 ng/ul
 RT: 14.17 min Scan# 1901
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43





Instrument :
 BNA_M
 ClientSampleID :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
138	100		
108	12.1	10.0	15.0
92	135.9	104.3	156.5



#50
 Acenaphthene
 Concen: 19.857 ng/ul
 RT: 14.33 min Scan# 1929
 Delta R.T. -0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
153	100		
152	44.8	35.9	53.9
154	87.4	69.4	104.0


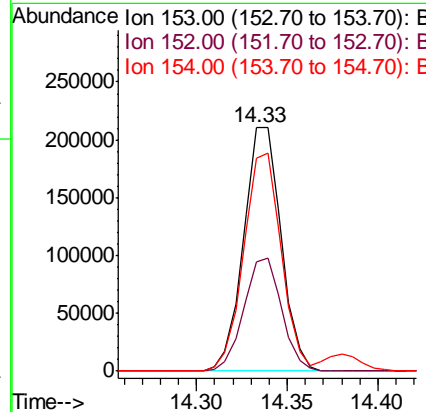



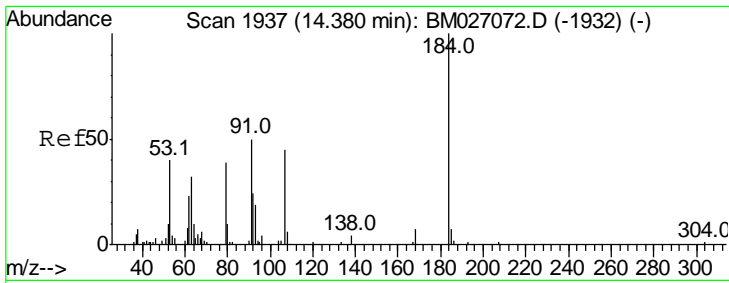

#51
 2,4-Dinitrophenol
 Concen: 16.937 ng/ul
 RT: 14.38 min Scan# 1937
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43





Instrument :
 BNA_M
 ClientSampled :
 SSTD02023


Tgt Ion	Ratio	Lower	Upper
184	100		
63	73.5	64.9	97.3
154	64.9	56.7	85.1

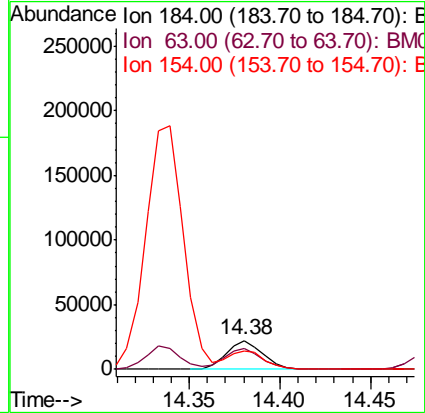

#53
 4-Nitrophenol
 Concen: 21.206 ng/ul
 RT: 14.49 min Scan# 1955
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Ratio	Lower	Upper
109	100		
139	100.1	77.4	116.2
65	124.0	100.6	150.8



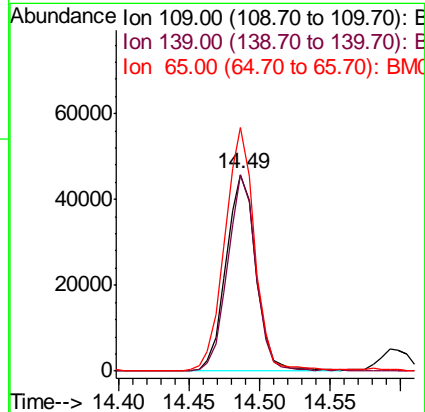
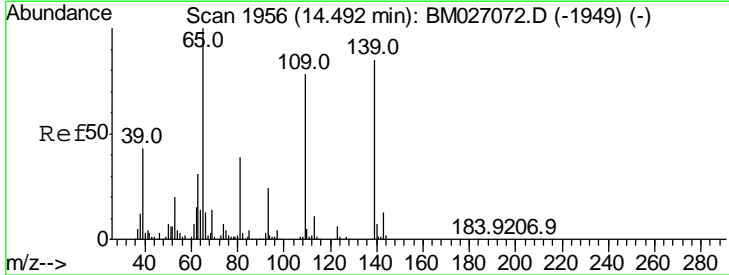


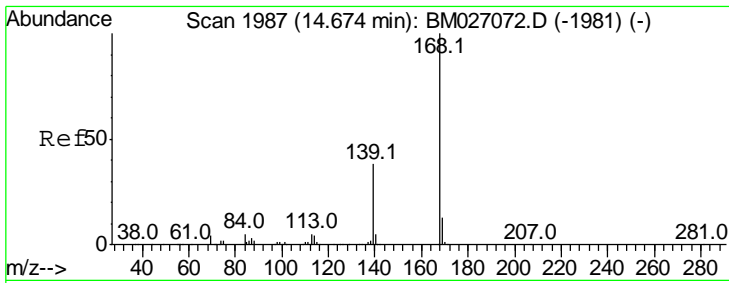

#54
 Dibenzofuran
 Concen: 20.637 ng/ul
 RT: 14.67 min Scan# 1987
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
168	100		
139	37.8	29.9	44.9

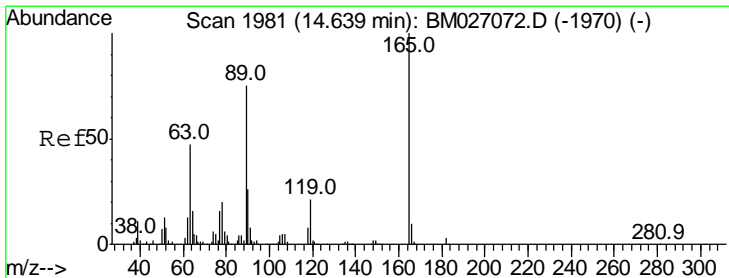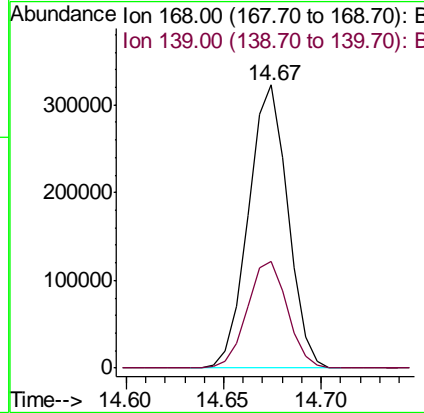

#55
 2,4-Dinitrotoluene
 Concen: 21.112 ng/ul
 RT: 14.63 min Scan# 1980
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
165	100		
63	51.2	43.4	65.0
182	3.6	3.0	4.4



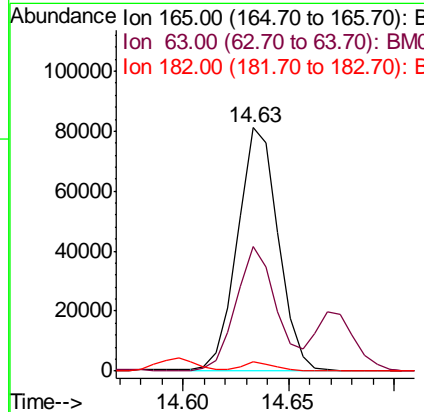
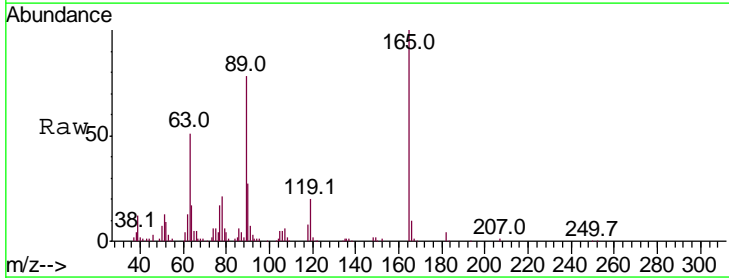


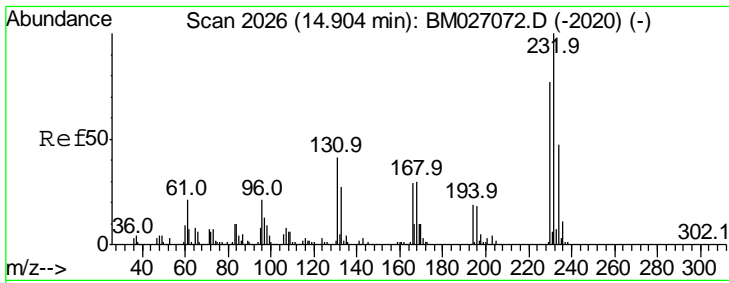

#56
 2,3,4,6-Tetrachlorophenol
 Concen: 23.024 ng/ul
 RT: 14.90 min Scan# 2026
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampleId :
 SST02023


Tgt Ion	Resp	Lower	Upper
232	106995		
131	39.0	34.6	52.0
130	2.3	2.2	3.4
166	27.9	25.5	38.3

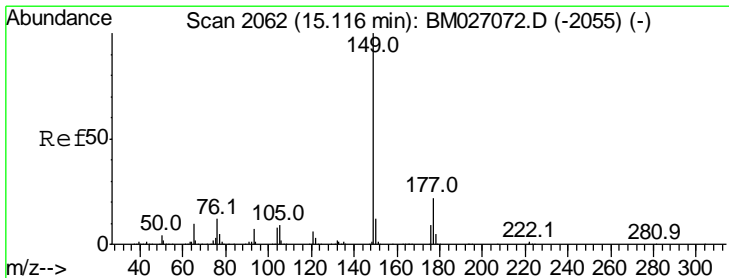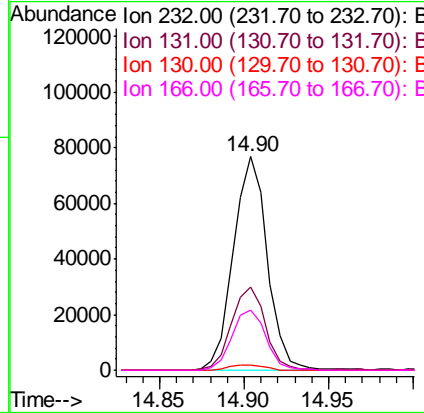

#57
 Diethylphthalate
 Concen: 20.163 ng/ul
 RT: 15.11 min Scan# 2061
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
149	376478		
177	22.6	17.4	26.2
150	12.9	10.1	15.1


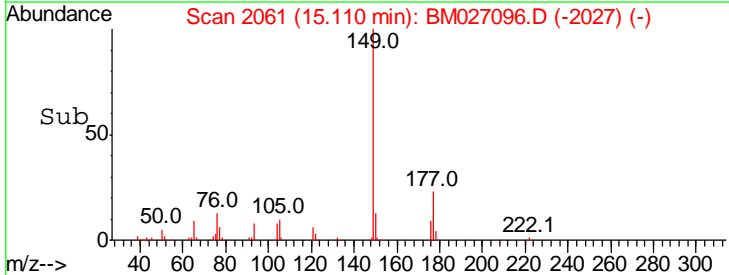
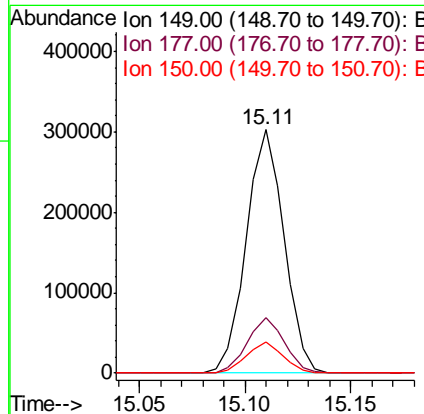



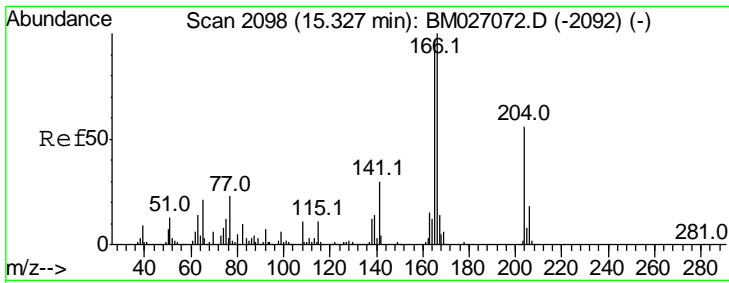

#59
 Fluorene
 Concen: 20.488 ng/ul
 RT: 15.32 min Scan# 2097
 Delta R.T. -0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
166	100		
165	97.3	76.9	115.3
167	13.5	10.5	15.7

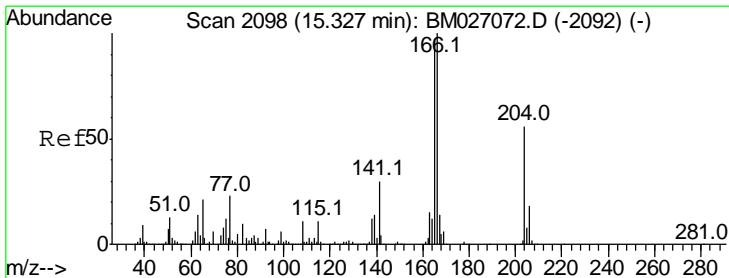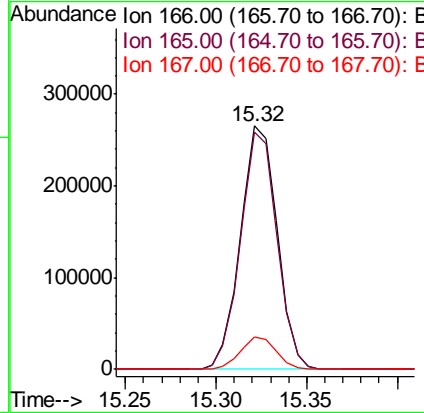

#60
 4-Chlorophenyl-phenylether
 Concen: 20.761 ng/ul
 RT: 15.33 min Scan# 2098
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
204	100		
206	33.5	25.8	38.8
141	54.3	46.7	70.1


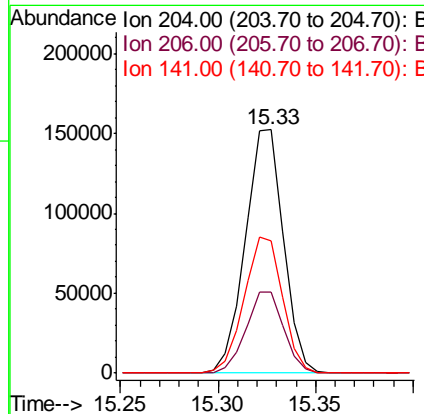
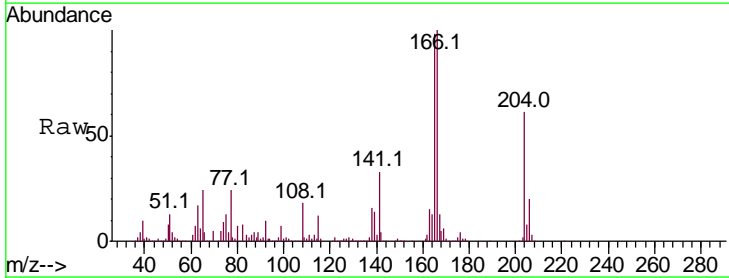


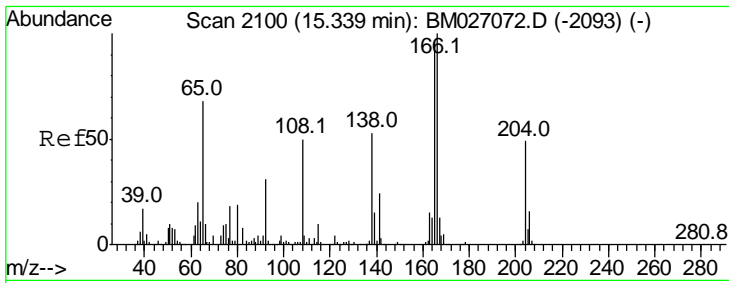

#61
 4-Nitroaniline
 Concen: 20.618 ng/ul
 RT: 15.33 min Scan# 2099
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43





Instrument :
 BNA_M
 ClientSampleId :
 SST02023


Tgt Ion	Resp	Lower	Upper
138	100		
92	63.1	46.9	70.3
108	116.5	89.0	133.6

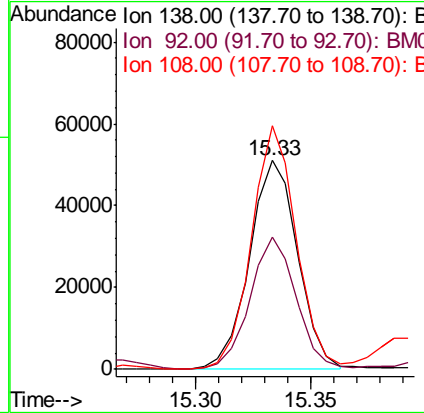

#64
 4,6-Dinitro-2-methylphenol
 Concen: 16.572 ng/ul
 RT: 15.40 min Scan# 2111
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
198	100		
182	4.0	3.8	5.6
77	31.4	25.3	37.9



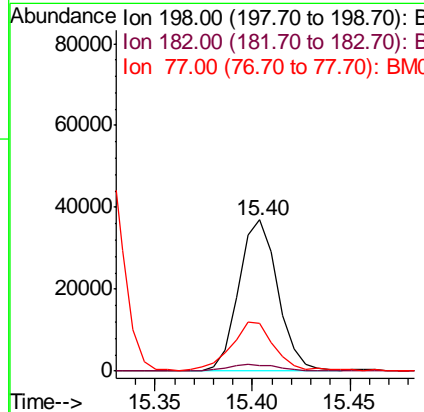
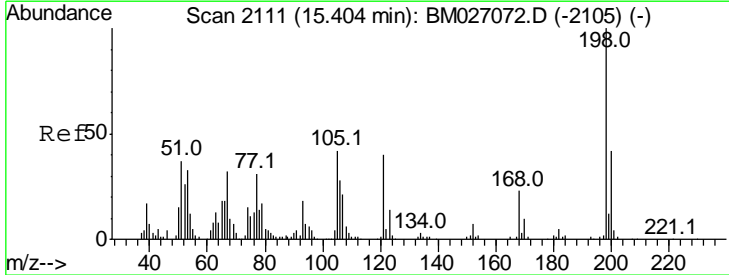


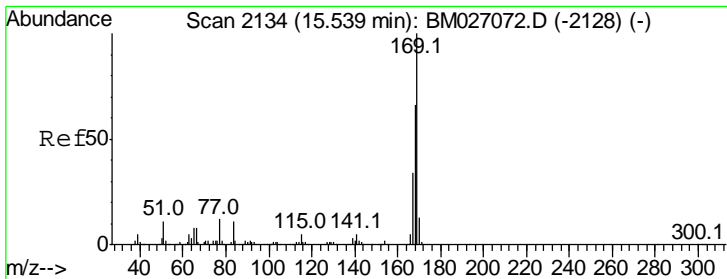

#65
 N-Nitrosodiphenylamine
 Concen: 20.858 ng/ul
 RT: 15.53 min Scan# 2133
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SST02023


Tgt Ion	Resp	Lower	Upper
169	100		
168	66.9	53.8	80.8
167	35.2	27.8	41.8

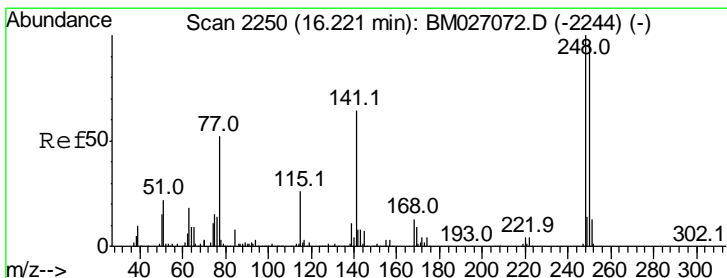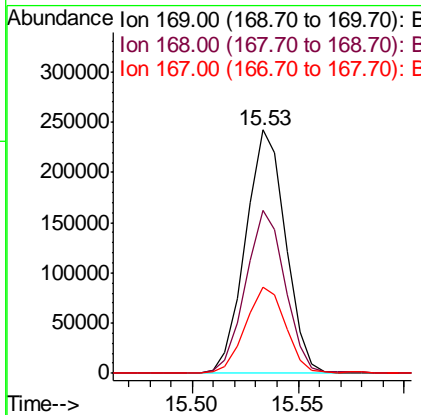

#66
 4-Bromophenyl-phenylether
 Concen: 20.743 ng/ul
 RT: 16.22 min Scan# 2249
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
248	100		
250	95.2	79.4	119.2
141	67.5	56.2	84.4



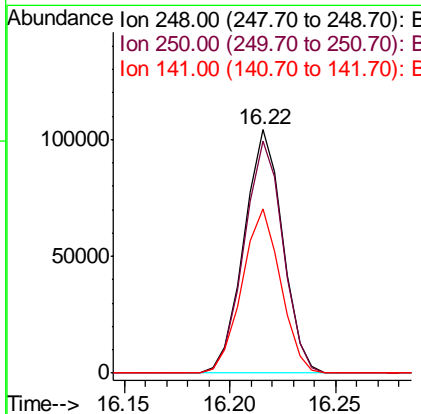
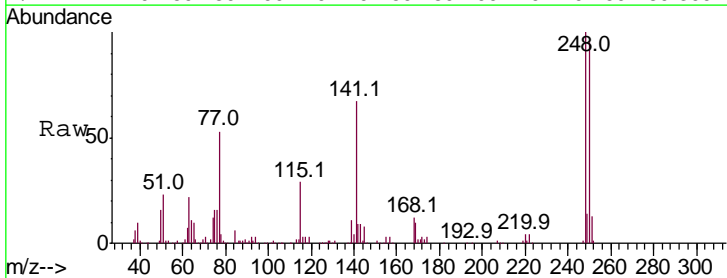


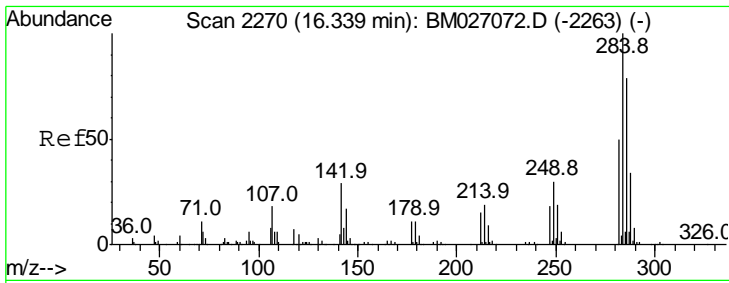

#67
 Hexachlorobenzene
 Concen: 20.791 ng/ul
 RT: 16.33 min Scan# 2269
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
284	100		
142	29.8	26.6	39.8
249	30.3	25.3	37.9

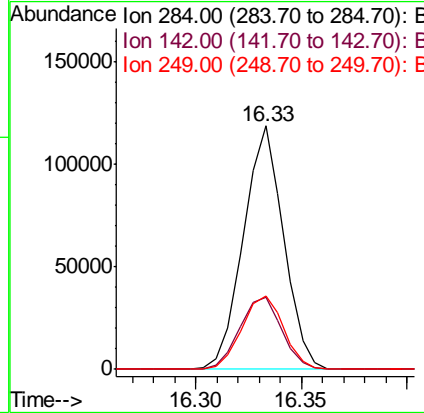

#68
 Atrazine
 Concen: 19.364 ng/ul
 RT: 16.49 min Scan# 2296
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
200	100		
173	25.3	20.3	30.5
215	49.9	38.8	58.2


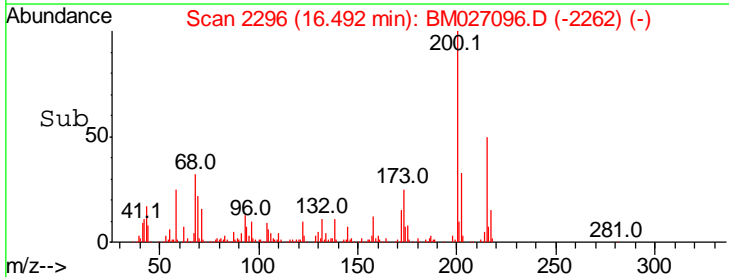
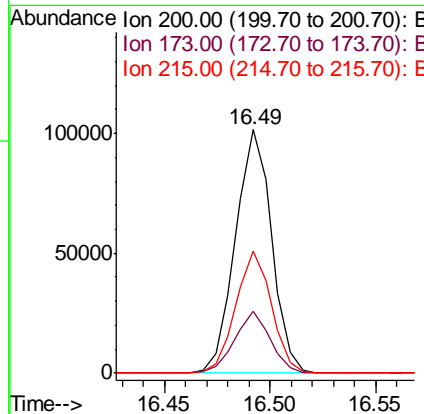



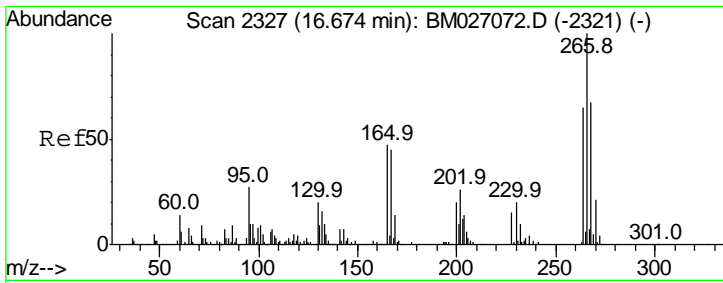

#69
 Pentachlorophenol
 Concen: 20.781 ng/ul
 RT: 16.67 min Scan# 2327
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampleID :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
266	100		
264	62.8	48.1	72.1
268	61.2	51.0	76.6

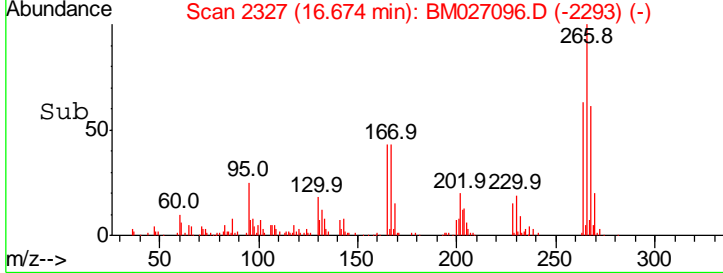

#70
 Phenanthrene
 Concen: 19.885 ng/ul
 RT: 17.06 min Scan# 2392
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
178	100		
179	15.5	11.9	17.9
176	18.2	14.6	22.0


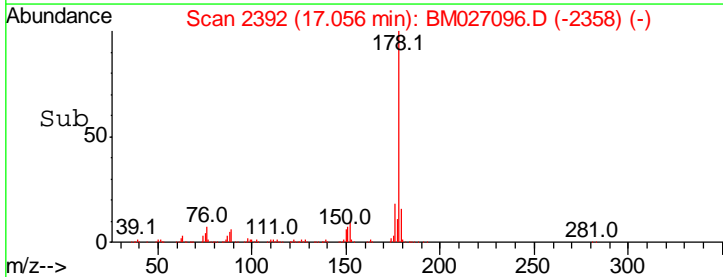




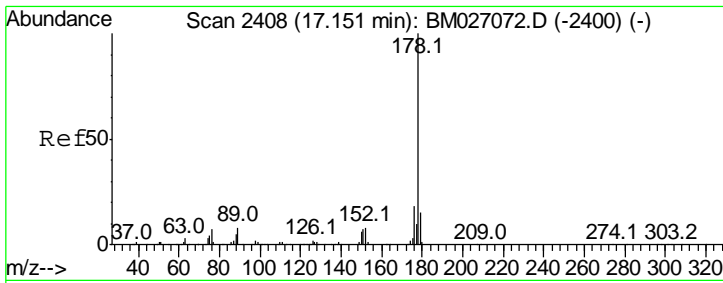

#72
 Anthracene
 Concen: 20.040 ng/ul
 RT: 17.14 min Scan# 2407
 Delta R.T. -0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SST02023


Tgt Ion	Resp	Lower	Upper
178	100		
179	15.3	12.0	18.0
176	18.1	14.3	21.5

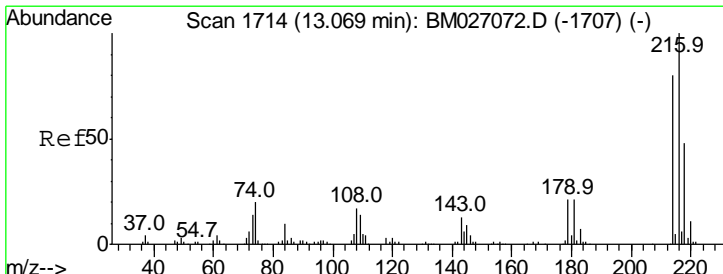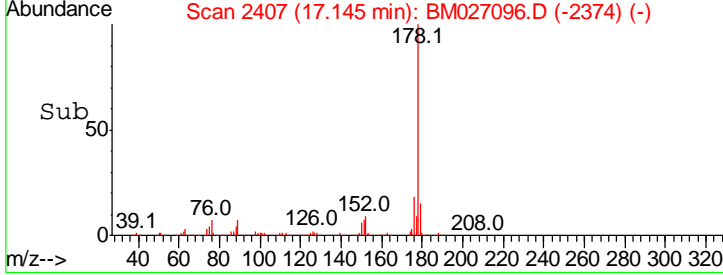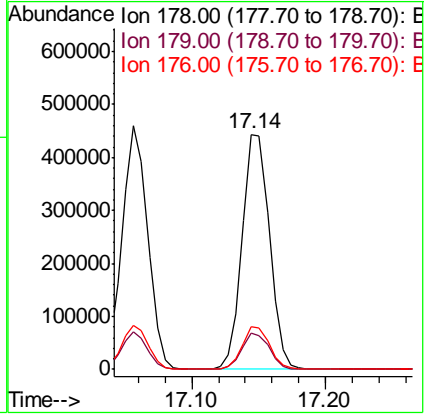

#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 22.390 ng/uL
 RT: 13.07 min Scan# 1714
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
216	100		
214	76.7	61.8	92.6
218	48.7	39.0	58.4


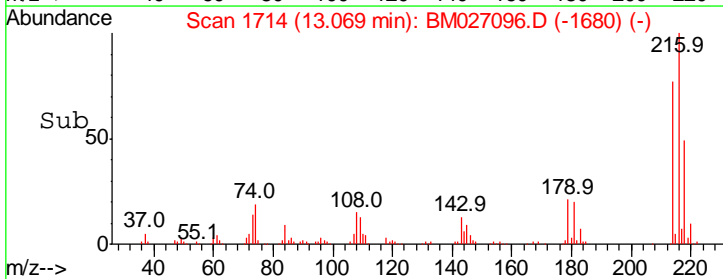
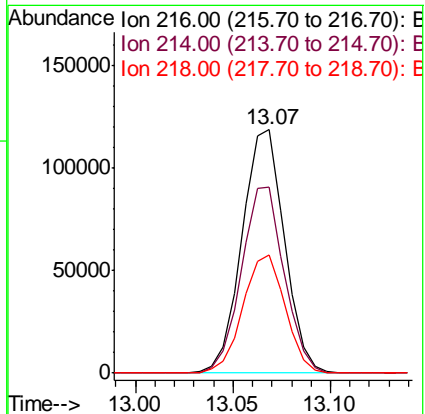





#74
 Pentachlorobenzene
 Concen: 21.149 ng/uL
 RT: 14.60 min Scan# 1974
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
250	100		
248	62.3	49.5	74.3
252	64.1	52.1	78.1



#75
 Carbazole
 Concen: 20.059 ng/uL
 RT: 17.42 min Scan# 2453
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
167	100		
166	21.8	17.0	25.6
139	12.2	9.8	14.6









#76
 Di-n-butylphthalate
 Concen: 19.089 ng/ul
 RT: 18.00 min Scan# 2552
 Delta R.T. -0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SST02023


Tgt Ion	Resp	Lower	Upper
149	100		
150	9.2	7.4	11.0
104	6.3	5.0	7.6

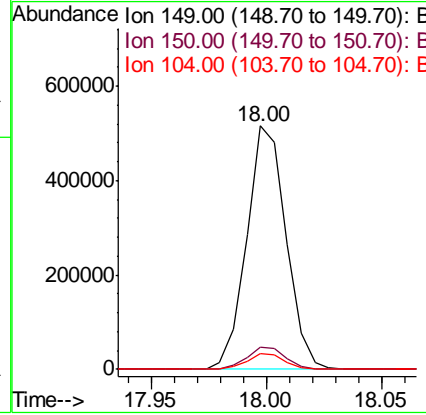

#77
 Fluoranthene
 Concen: 20.126 ng/ul
 RT: 19.08 min Scan# 2736
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
202	100		
101	7.0	6.7	10.1
100	5.6	5.4	8.2







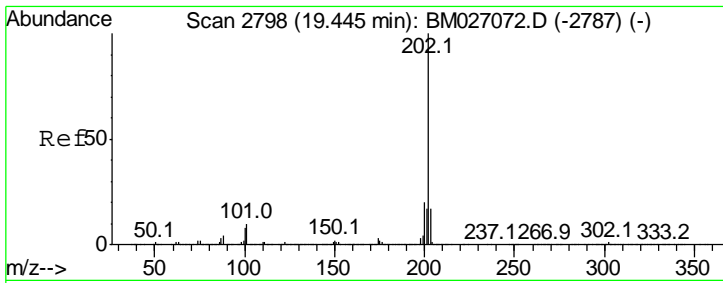

#80
 Pyrene
 Concen: 19.419 ng/ul
 RT: 19.44 min Scan# 2798
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampleId :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
202	100		
101	8.2	7.6	11.4
100	6.6	6.3	9.5

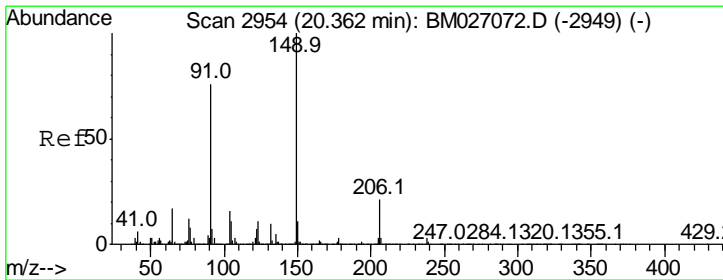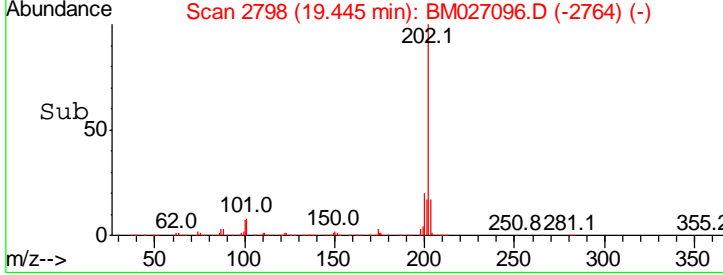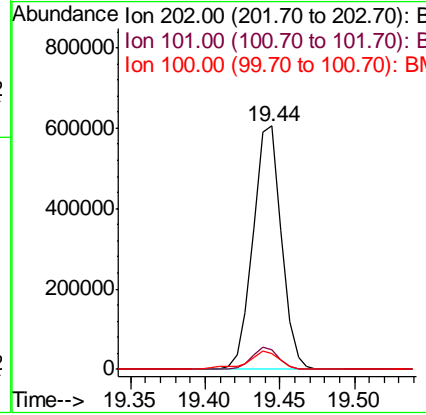

#81
 Butylbenzylphthalate
 Concen: 18.499 ng/ul
 RT: 20.36 min Scan# 2954
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
149	100		
91	72.9	57.4	86.2
206	23.0	17.4	26.2


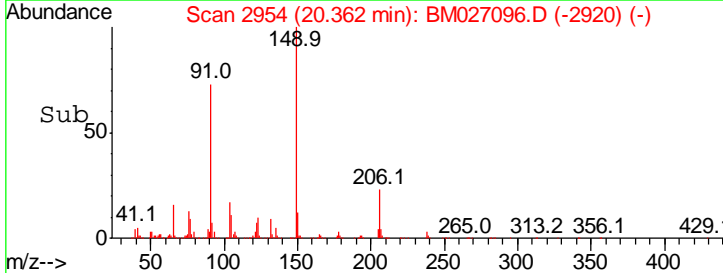




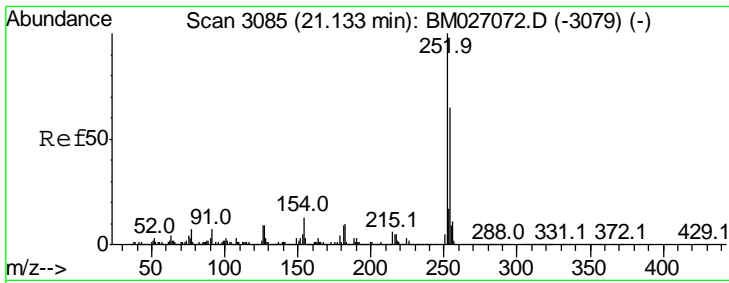

#82
 3,3'-Dichlorobenzidine
 Concen: 19.203 ng/ul
 RT: 21.13 min Scan# 3085
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
252	100		
254	65.4	52.3	78.5
126	7.9	7.3	10.9

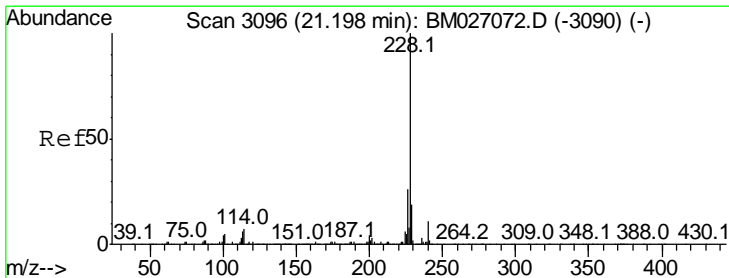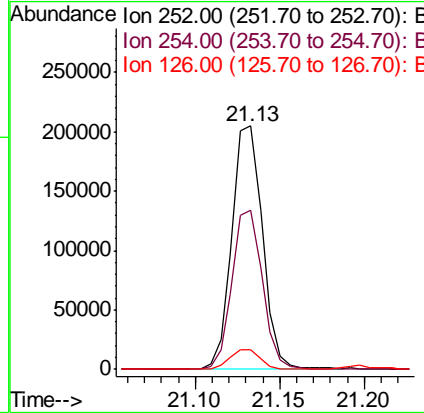

#83
 Benzo(a)anthracene
 Concen: 20.262 ng/ul
 RT: 21.20 min Scan# 3096
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
228	100		
229	19.9	15.8	23.6
226	26.8	21.2	31.8


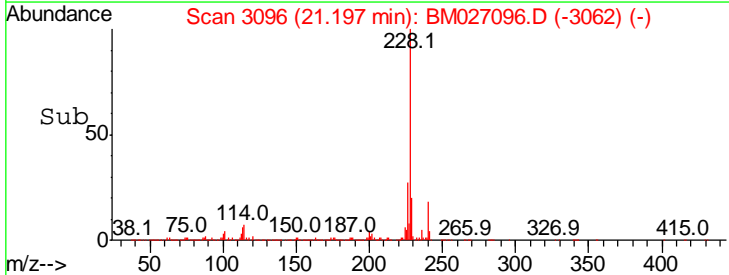
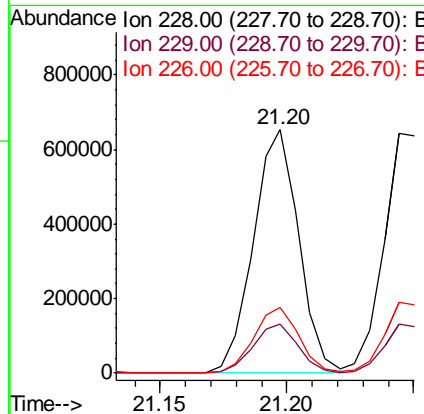



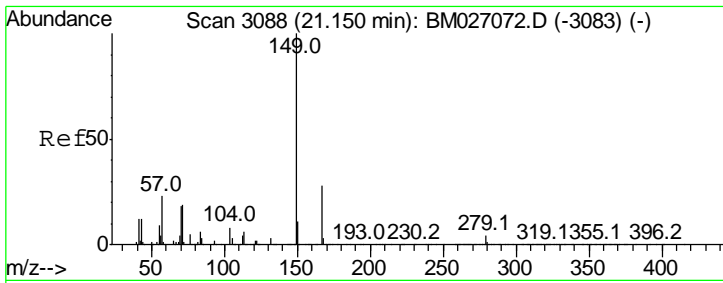

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 17.089 ng/ul
 RT: 21.15 min Scan# 3088
 Delta R.T. -0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
149	100		
167	27.7	21.6	32.4
279	5.0	3.9	5.9

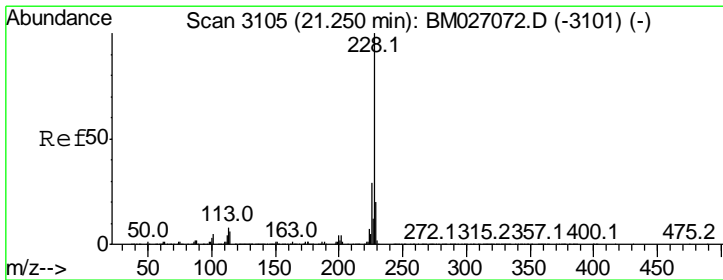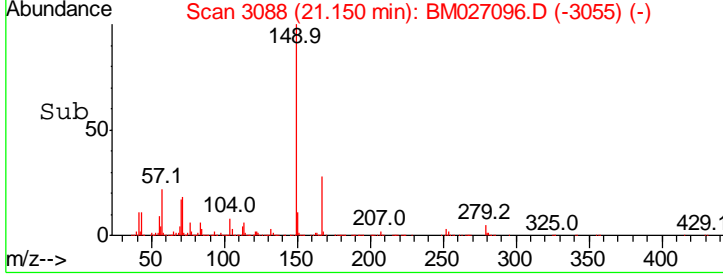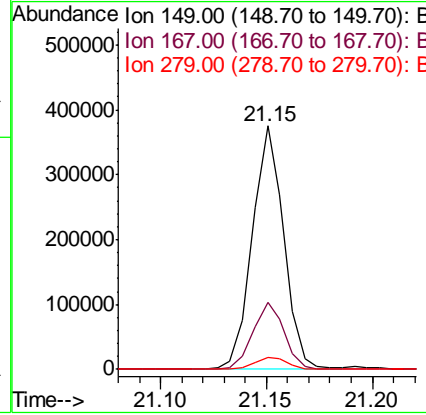

#85
 Chrysene
 Concen: 20.107 ng/ul
 RT: 21.24 min Scan# 3104
 Delta R.T. -0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43





Tgt Ion	Resp	Lower	Upper
228	100		
226	29.3	23.8	35.6
229	20.3	15.8	23.8

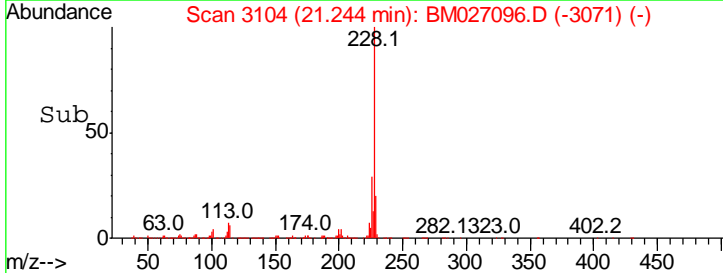






#87
 Di-n-octyl phthalate
 Concen: 16.923 ng/ul
 RT: 22.02 min Scan# 3236
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43
 Tgt Ion:149 Resp: 695267


Instrument :
 BNA_M
 ClientSampled :
 SSTD02023

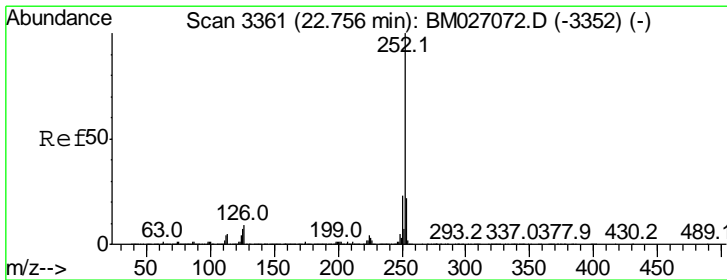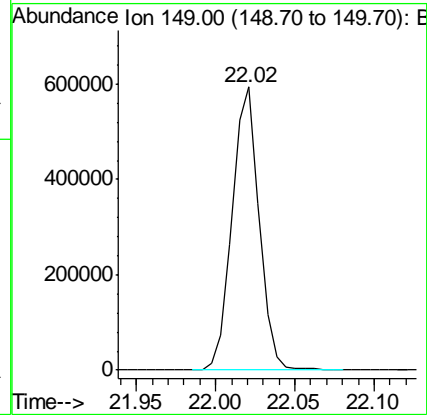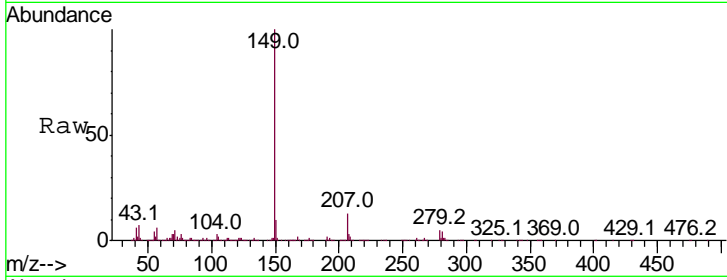

#88
 Benzo(b)fluoranthene
 Concen: 20.197 ng/ul
 RT: 22.75 min Scan# 3360
 Delta R.T. -0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.9	17.6	26.4
125	6.3	6.0	9.0



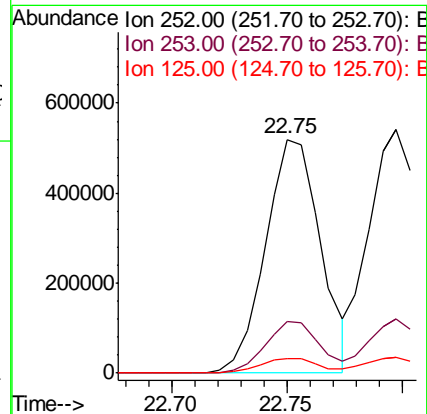
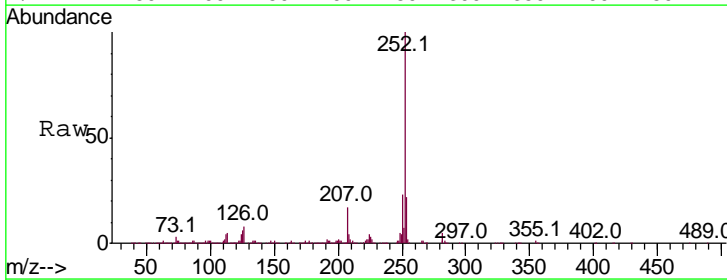


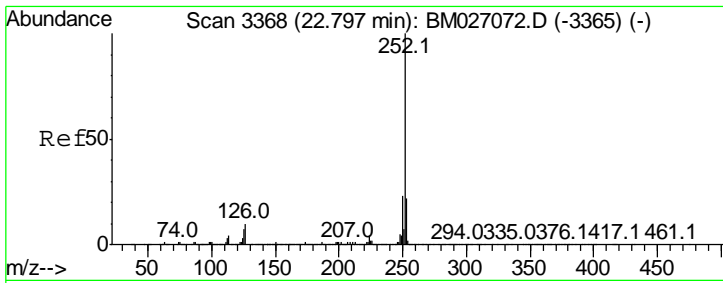

#89
 Benzo(k)fluoranthene
 Concen: 19.834 ng/ul
 RT: 22.80 min Scan# 3368
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SSTD02023


Tgt Ion	Resp	Lower	Upper
252	100		
253	22.0	17.2	25.8
125	6.6	5.5	8.3

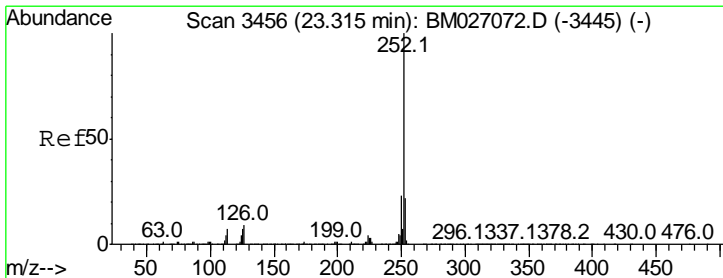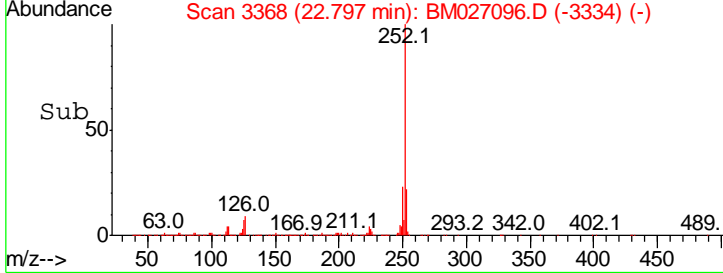

#91
 Benzo(a)pyrene
 Concen: 19.398 ng/ul
 RT: 23.31 min Scan# 3456
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
252	100		
253	21.1	17.0	25.4
125	6.9	5.8	8.8


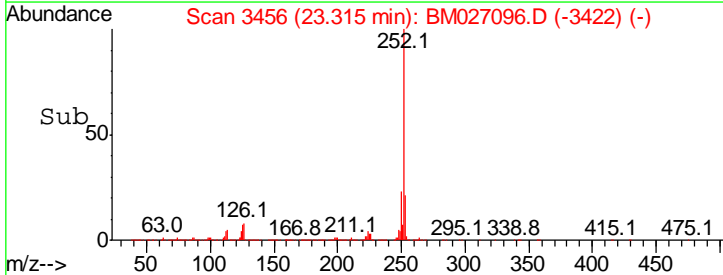






#92
 Indeno(1,2,3-cd)pyrene
 Concen: 19.294 ng/ul
 RT: 25.61 min Scan# 3846
 Delta R.T. 0.01 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43




Instrument :
 BNA_M
 ClientSampled :
 SST02023


Tgt Ion	Resp	Lower	Upper
276	100		
138	15.1	13.9	20.9
277	25.4	19.8	29.8

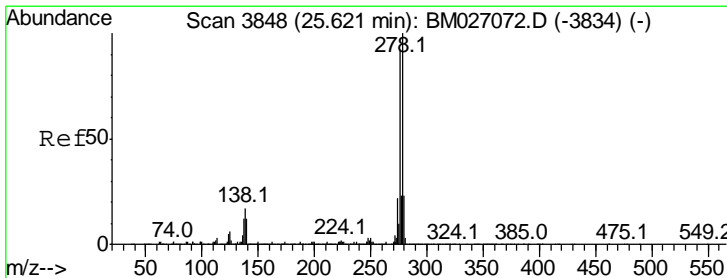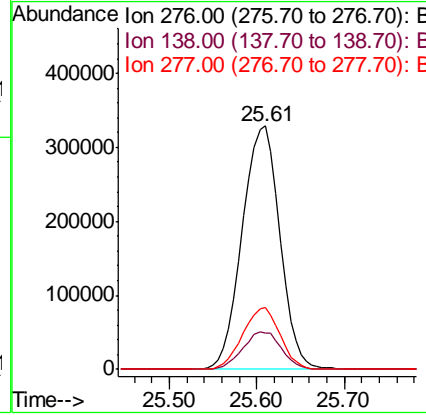

#93
 Dibenzo(a,h)anthracene
 Concen: 19.360 ng/ul
 RT: 25.61 min Scan# 3847
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Tgt Ion	Resp	Lower	Upper
278	100		
139	10.9	9.4	14.0
279	23.9	18.7	28.1

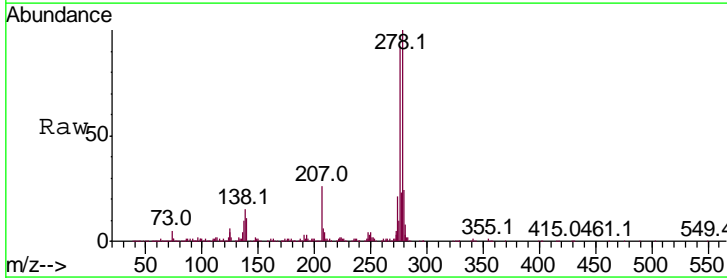

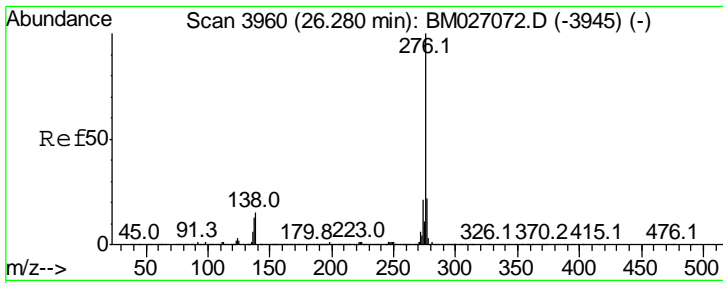

#94
 Benzo(a,h,i)perylene
 Concen: 18.801 ng/ul
 RT: 26.27 min Scan# 3959
 Delta R.T. -0.00 min
 Lab File: BM027096.D
 Acq: 14 Aug 2020 19:43

Instrument :
 BNA_M
 ClientSampled :
 SSTD02023

Tot Ion	Ion	Ratio	Lower	Upper
776484	276	100		
	138	14.8	12.3	18.5
	277	23.6	19.0	28.6

