

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081320\
 Data File : BM027067.D
 Acq On : 13 Aug 2020 18:51
 Operator : JU/CG
 Sample : L3630-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFMK9

Quant Time: Aug 14 05:22:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 13 11:47:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	126000	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	468921	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	296130	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	615583	20.00	ng/ul	0.00
78) Chrysene-d12	21.21	240	630932	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	643825	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	9230	3.33	ng/uL	0.00
5) Phenol-d5	6.82	99	177780	18.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	127044	18.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	141944	18.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	137861	18.05	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	69071	18.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	71029	18.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	147829	18.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	162668	17.29	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	466703	19.76	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	539102	19.16	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	57352	14.39	ng/ul	0.00
58) Fluorene-d10	15.27	176	385383	18.72	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	47109	14.01	ng/ul	0.00
71) Anthracene-d10	17.12	188	564859	18.63	ng/ul	0.00
79) Pyrene-d10	19.42	212	622130	19.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	662584	18.44	ng/ul	0.00

Target Compounds


					Ovalue
45) Dimethylphthalate	13.73	163	124133	5.016	ng/ul 99
70) Phenanthrene	17.06	178	68613	1.859	ng/ul 99
77) Fluoranthene	19.08	202	151722	3.390	ng/ul 99
80) Pyrene	19.44	202	152889	3.570	ng/ul 99
83) Benzo(a)anthracene	21.20	228	71446	1.682	ng/ul 92
85) Chrysene	21.24	228	83966	2.014	ng/ul 98
88) Benzo(b)fluoranthene	22.76	252	115257	2.578	ng/ul# 96
91) Benzo(a)pyrene	23.31	252	73009	1.794	ng/ul# 95
92) Indeno(1,2,3-cd)pyrene	25.60	276	53594	1.022	ng/ul 98
94) Benzo(g,h,i)perylene	26.27	276	49210	1.136	ng/ul 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081320\
Data File : BM027067.D
Acq On : 13 Aug 2020 18:51
Operator : JU/CG
Sample : L3630-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFMK9

Quant Time: Aug 14 05:22:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 13 11:47:07 2020
Response via : Initial Calibration

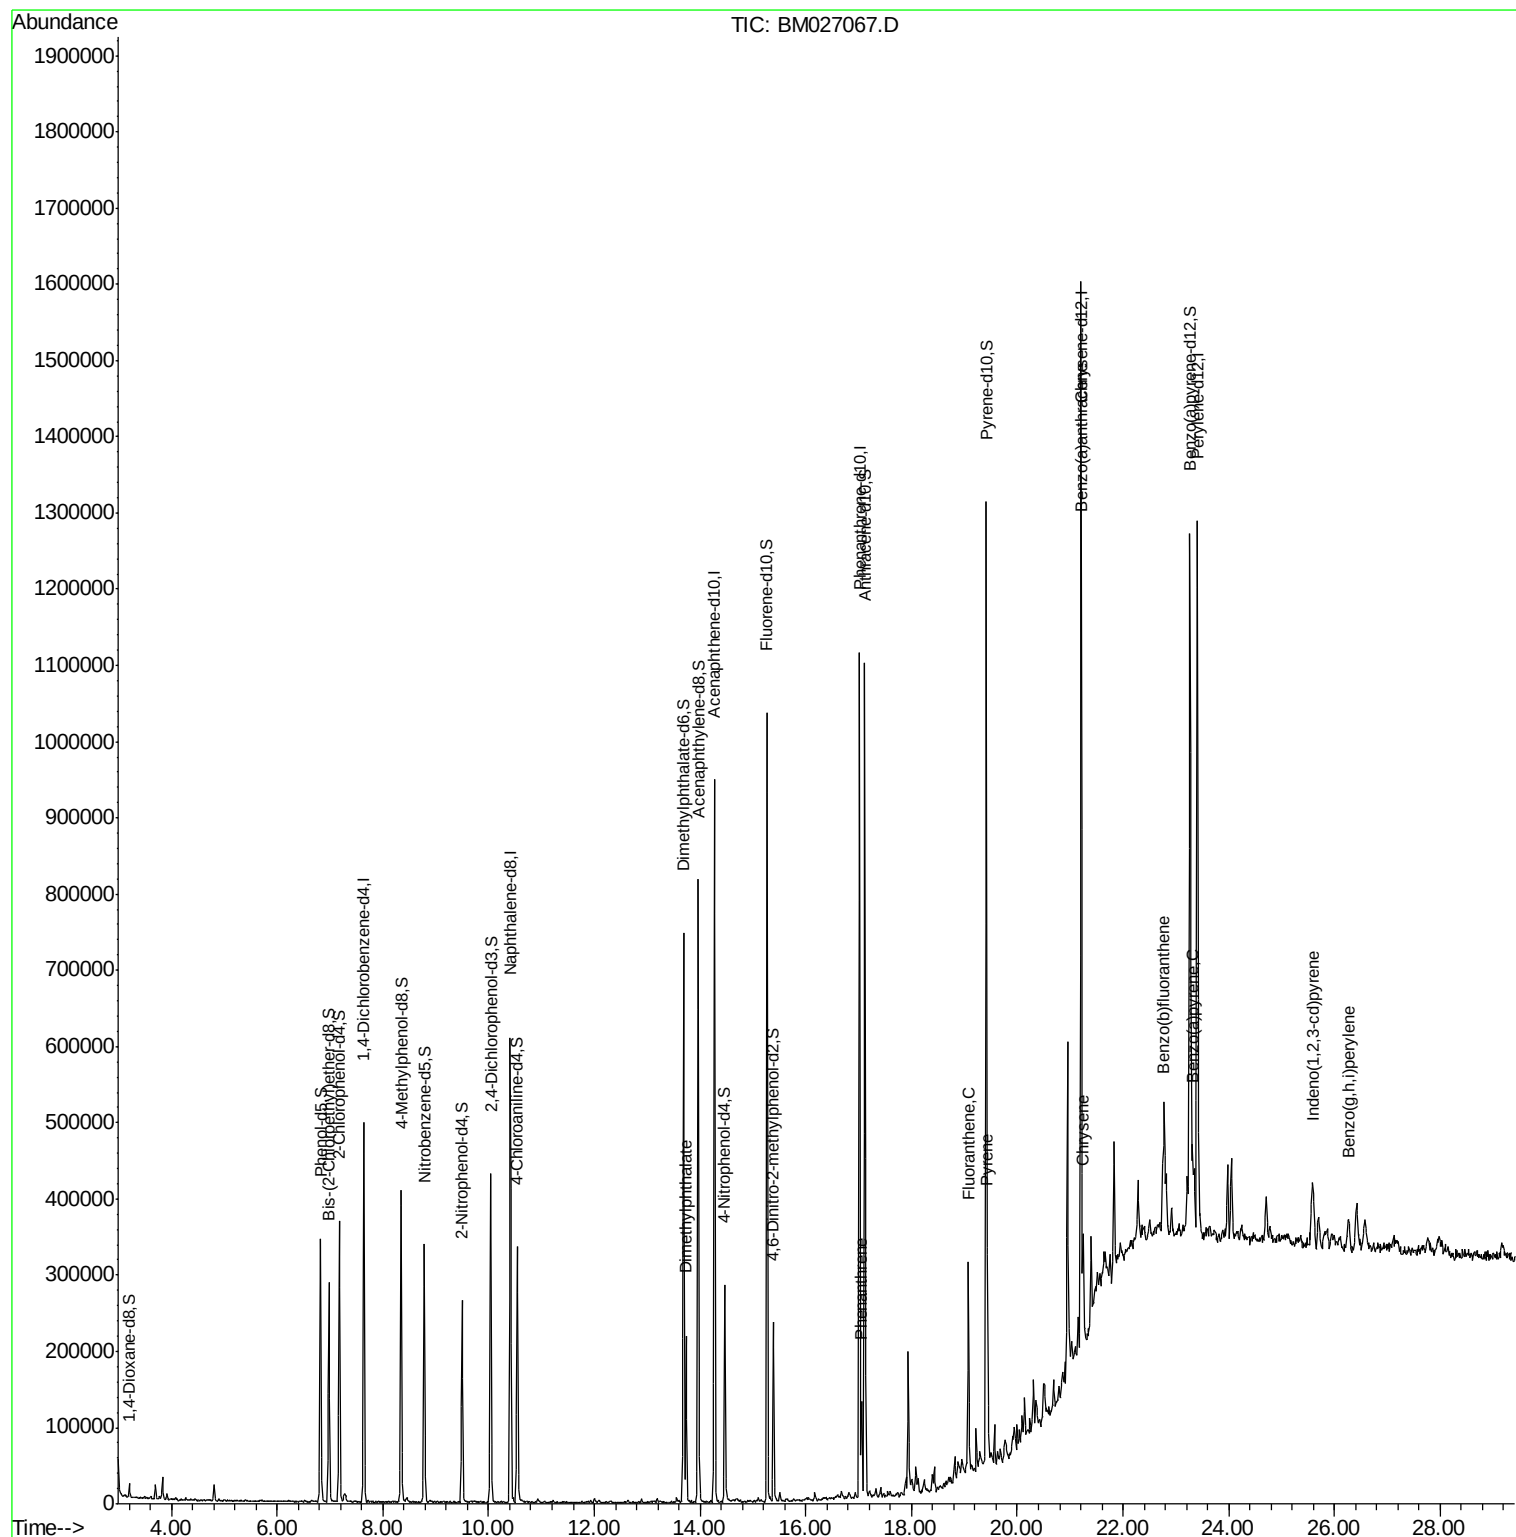

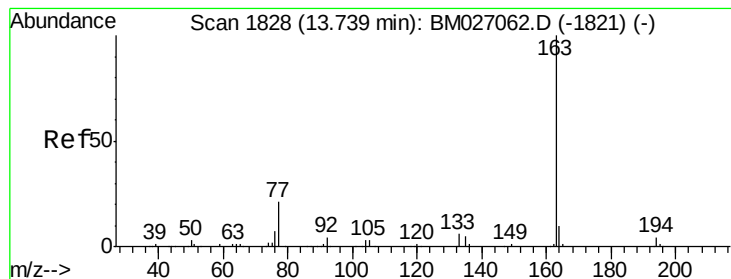

#45

Dimethylphthalate

Concen: 5.016 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. -0.00 min

Lab File: BM027067.D

Acq: 13 Aug 2020 18:51

Instrument :

BNA_M

ClientSampleId :

BFMK9


Tot Ion:163 Resp: 124133

Ion Ratio Lower Upper




163 100

194 3.8 3.2 4.8

164 10.0 8.2 12.2

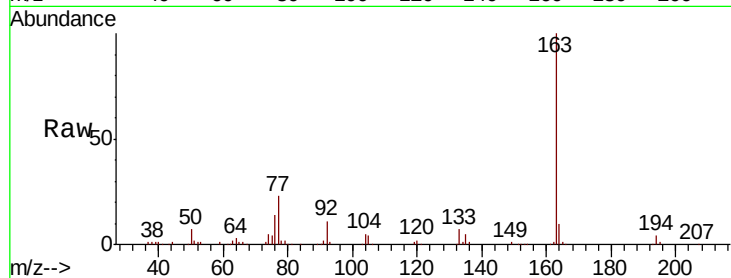

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

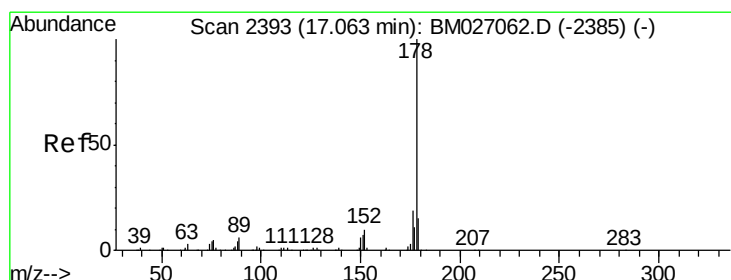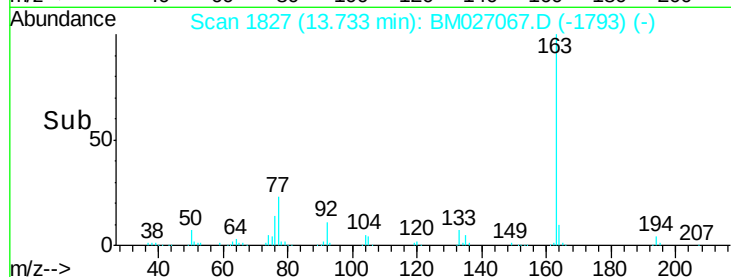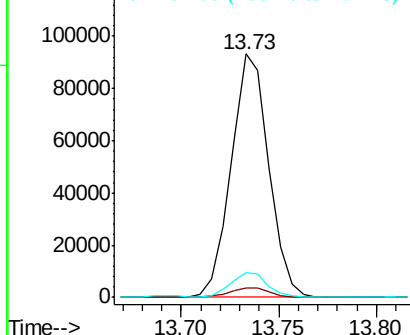

#70

Phenanthrene

Concen: 1.859 ng/ul

RT: 17.06 min Scan# 2392

Delta R.T. -0.00 min

Lab File: BM027067.D

Acq: 13 Aug 2020 18:51


Tgt Ion:178 Resp: 68613

Ion Ratio Lower Upper



178 100


179 15.5 11.9 17.9

176 18.7 14.6 22.0

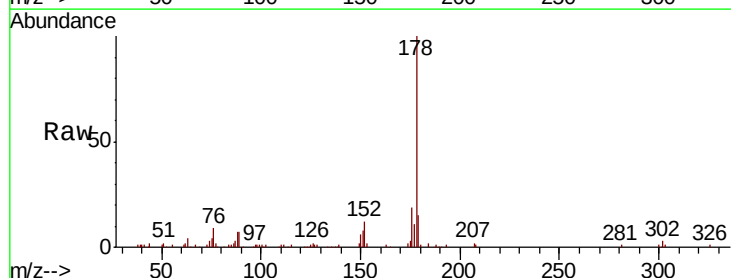

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E



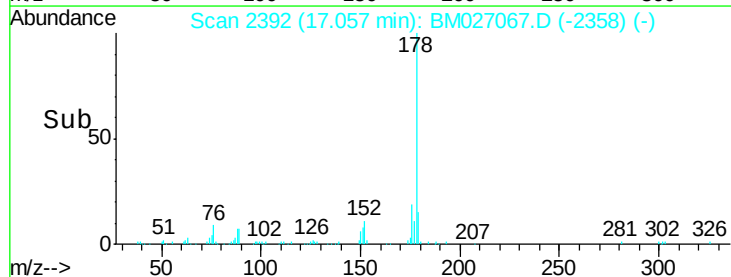
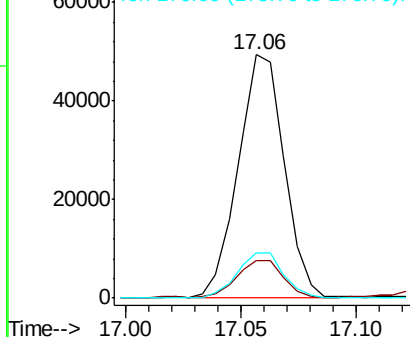


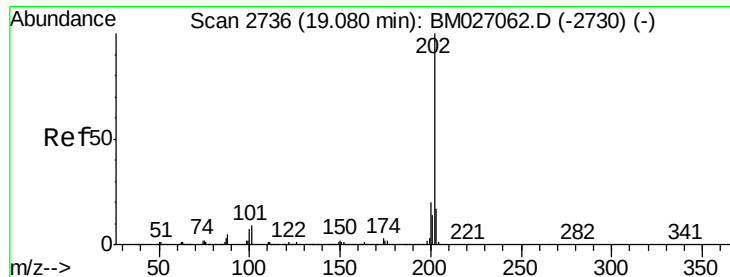

#77
 Fluoranthene
 Concen: 3.390 ng/ul
 RT: 19.08 min Scan# 2736
 Delta R.T. -0.00 min
 Lab File: BM027067.D
 Acq: 13 Aug 2020 18:51




Instrument :
 BNA_M
 ClientSampleId :
 BFMK9


Tot Ion	Ratio	Resp	Lower	Upper
202	100	151722		
101	8.3		6.7	10.1
100	6.3		5.4	8.2

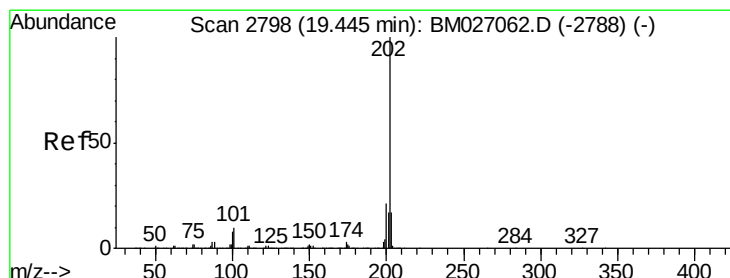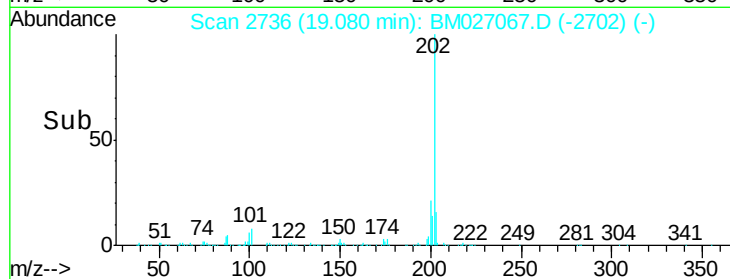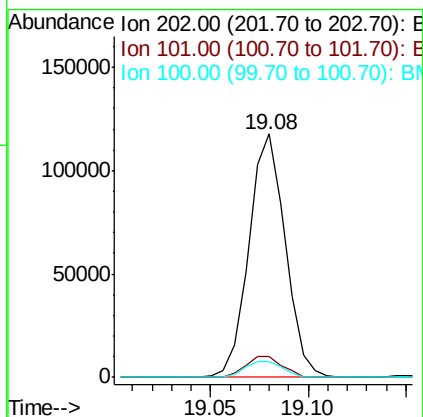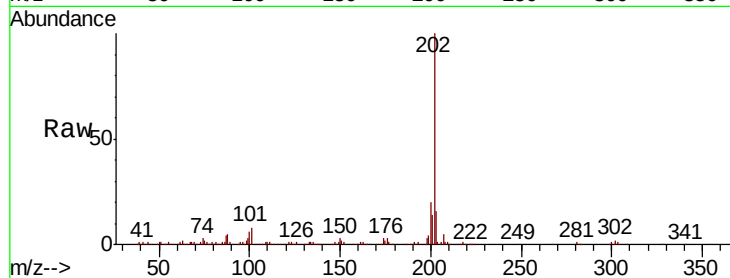

#80
 Pyrene
 Concen: 3.570 ng/ul
 RT: 19.44 min Scan# 2797
 Delta R.T. -0.01 min
 Lab File: BM027067.D
 Acq: 13 Aug 2020 18:51

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	152889		
101	9.6		7.6	11.4
100	8.4		6.3	9.5

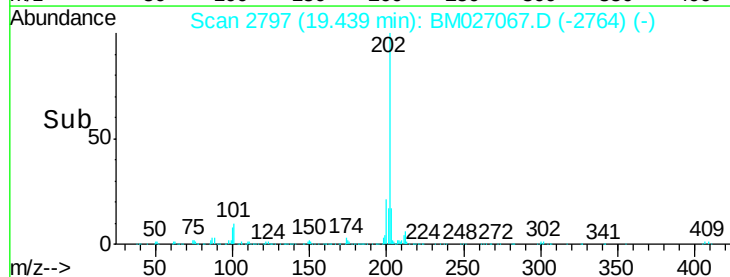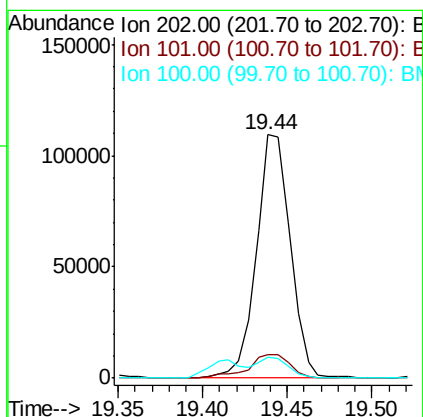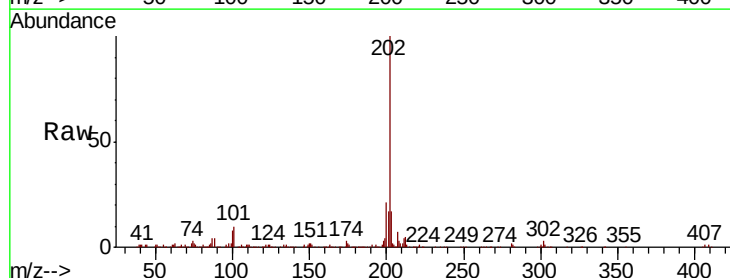

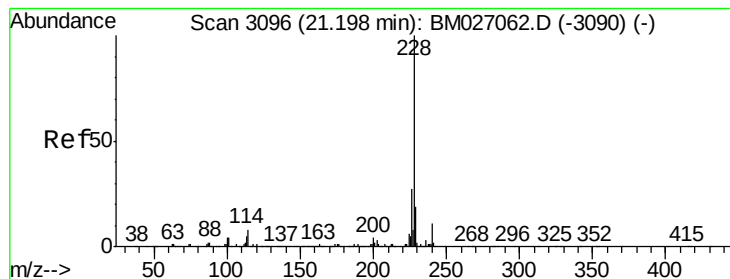

#83

Benzo(a)anthracene

Concen: 1.682 ng/ul

RT: 21.20 min Scan# 3096

Delta R.T. -0.00 min

Lab File: BM027067.D

Acq: 13 Aug 2020 18:51

Instrument :

BNA_M

ClientSampleId :

BFMK9


Tot Ion:228 Resp: 71446

Ion Ratio Lower Upper

228 100

229 21.6 15.8 23.6




226 31.8 21.2 31.8

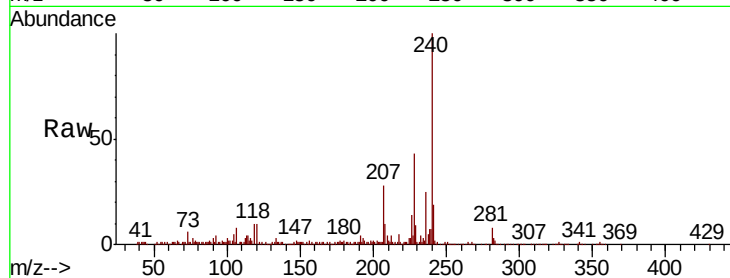

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

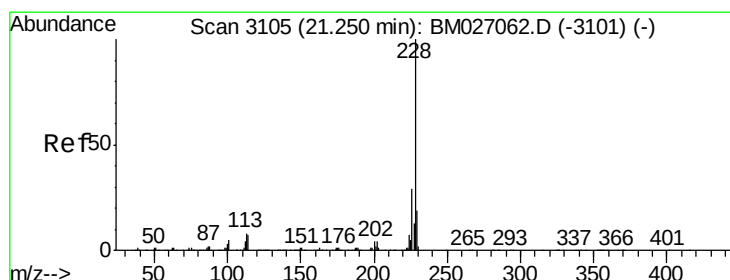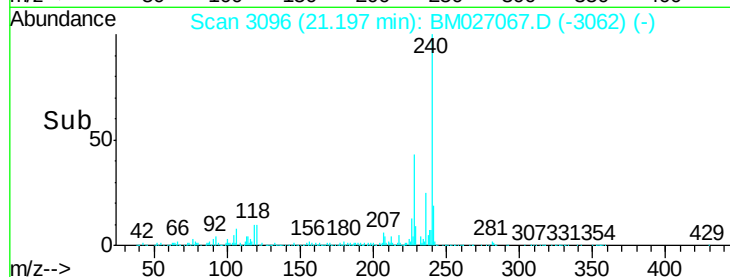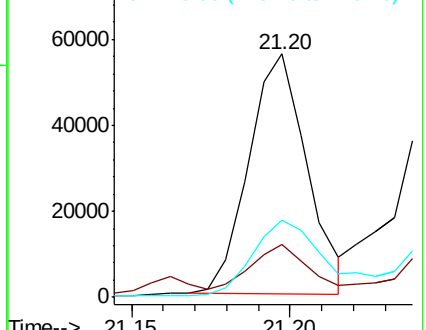

#85

Chrysene

Concen: 2.014 ng/ul

RT: 21.24 min Scan# 3104

Delta R.T. -0.01 min

Lab File: BM027067.D

Acq: 13 Aug 2020 18:51


Tgt Ion:228 Resp: 83966

Ion Ratio Lower Upper

228 100

226 29.2 23.8 35.6



229 21.1 15.8 23.8

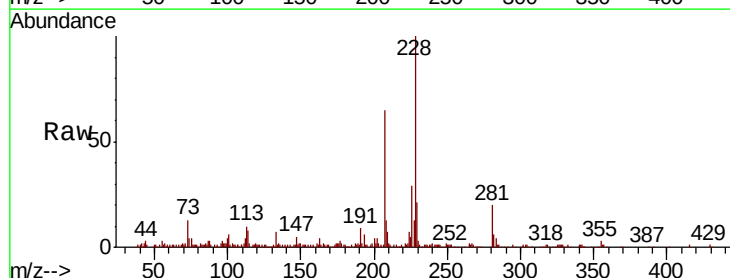


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

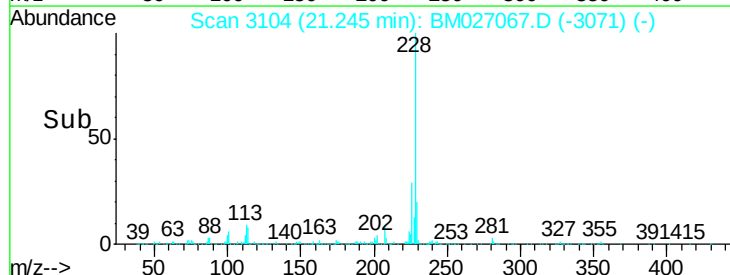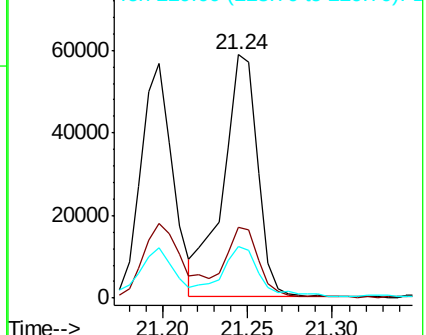

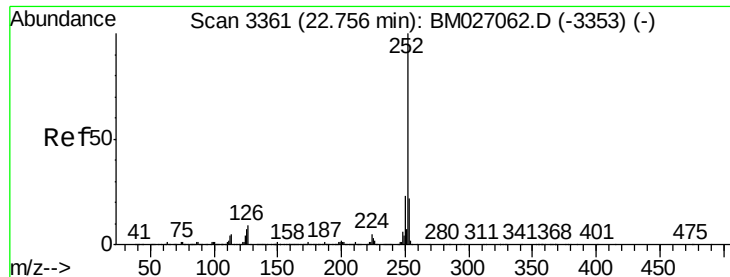

#88

Benzo(b)fluoranthene

Concen: 2.578 ng/ul

RT: 22.76 min Scan# 3361

Delta R.T. -0.00 min

Lab File: BM027067.D

Acq: 13 Aug 2020 18:51

Instrument :

BNA_M

ClientSampleId :

BFMK9


Tot Ion:252 Resp: 115257

Ion Ratio Lower Upper

252 100

253 23.9 17.6 26.4




125 9.1 6.0 9.0#

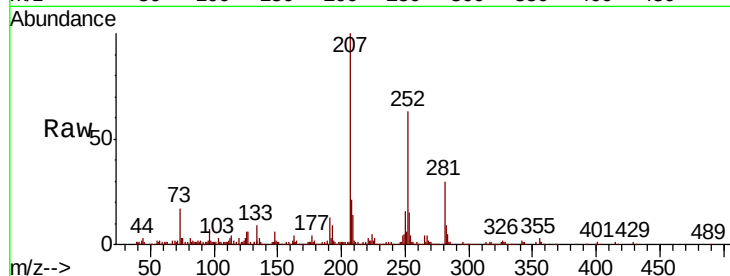

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

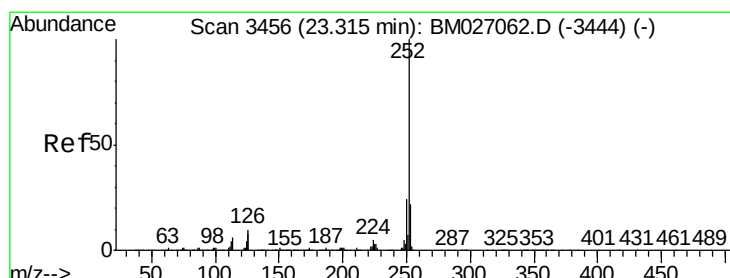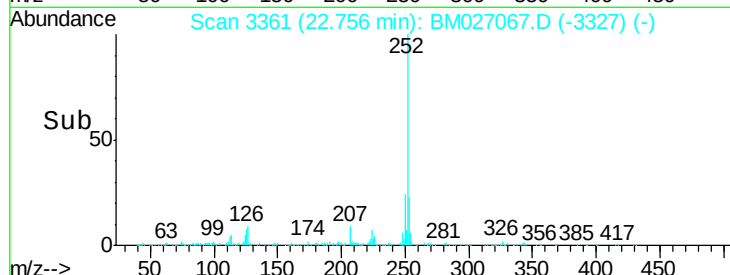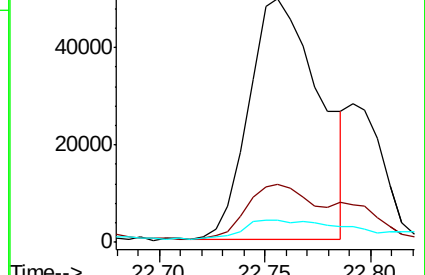

#91

Benzo(a)pyrene

Concen: 1.794 ng/ul

RT: 23.31 min Scan# 3455

Delta R.T. -0.01 min

Lab File: BM027067.D

Acq: 13 Aug 2020 18:51


Tgt Ion:252 Resp: 73009

Ion Ratio Lower Upper

252 100

253 23.8 17.0 25.4



125 8.8 5.8 8.8#

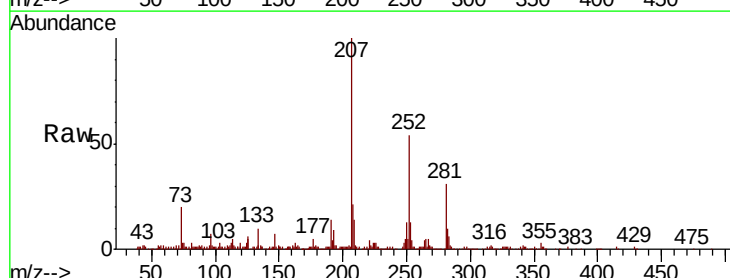


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

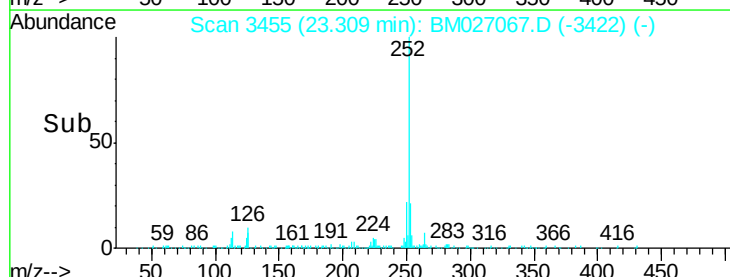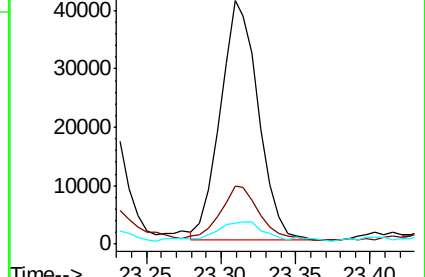




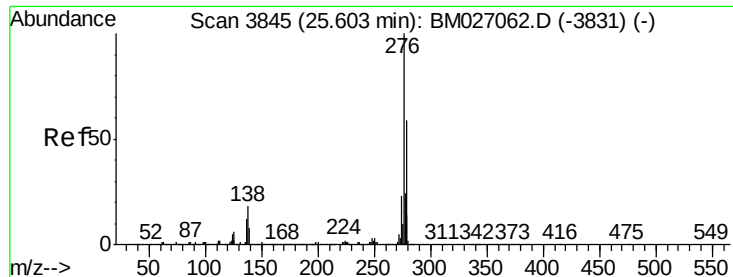


#92

Indeno(1,2,3-cd)pyrene
Concen: 1.022 ng/ul
RT: 25.60 min Scan# 3844
Delta R.T. -0.01 min
Lab File: BM027067.D
Acq: 13 Aug 2020 18:51

Instrument :
BNA_M
ClientSampled :
BFMK9

Tot Ion	Ratio	Lower	Upper
276	100		
138	17.9	13.9	20.9
277	23.3	19.8	29.8

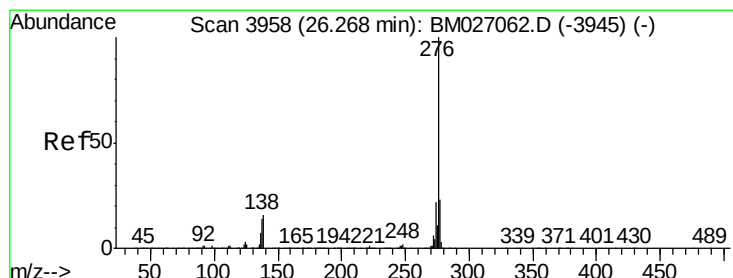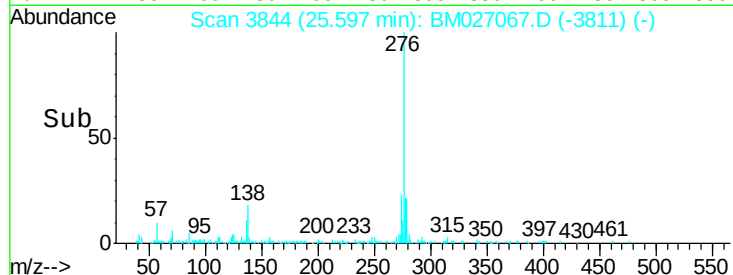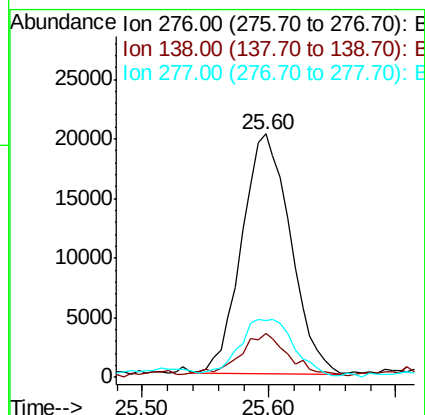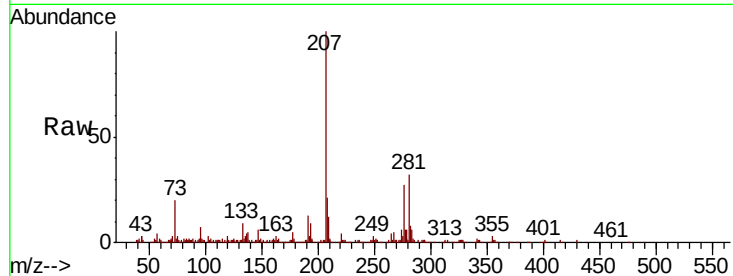

#94

Benzo(g,h,i)perylene
Concen: 1.136 ng/ul
RT: 26.27 min Scan# 3958
Delta R.T. -0.01 min
Lab File: BM027067.D
Acq: 13 Aug 2020 18:51

Tgt Ion	Ratio	Lower	Upper
276	100		
138	16.7	12.3	18.5
277	21.4	19.0	28.6

