

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081320\
 Data File : BM027091.D
 Acq On : 14 Aug 2020 16:40
 Operator : JU/CG
 Sample : L3647-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB7H6

Quant Time: Aug 14 17:13:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 13 11:47:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	99642	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	341895	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	215578	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.02	188	470102	20.00	ng/ul	0.00
78) Chrysene-d12	21.21	240	537520	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	577918	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	11486	5.24	ng/uL	0.00
5) Phenol-d5	6.82	99	58602	7.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	132085	24.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	137357	22.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	92187	15.26	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	73568	27.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	78090	27.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	163680	27.73	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	12318	1.80	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	517353	30.10	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	601486	29.36	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	19992	6.89	ng/ul	0.00
58) Fluorene-d10	15.27	176	437153	29.17	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	62702	24.42	ng/ul	0.00
71) Anthracene-d10	17.12	188	737305	31.84	ng/ul	0.00
79) Pyrene-d10	19.42	212	883709	32.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	1066792	33.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.73	163	121908	6.767	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM081320\
Data File : BM027091.D
Acq On : 14 Aug 2020 16:40
Operator : JU/CG
Sample : L3647-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB7H6

Quant Time: Aug 14 17:13:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM080720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 13 11:47:07 2020
Response via : Initial Calibration

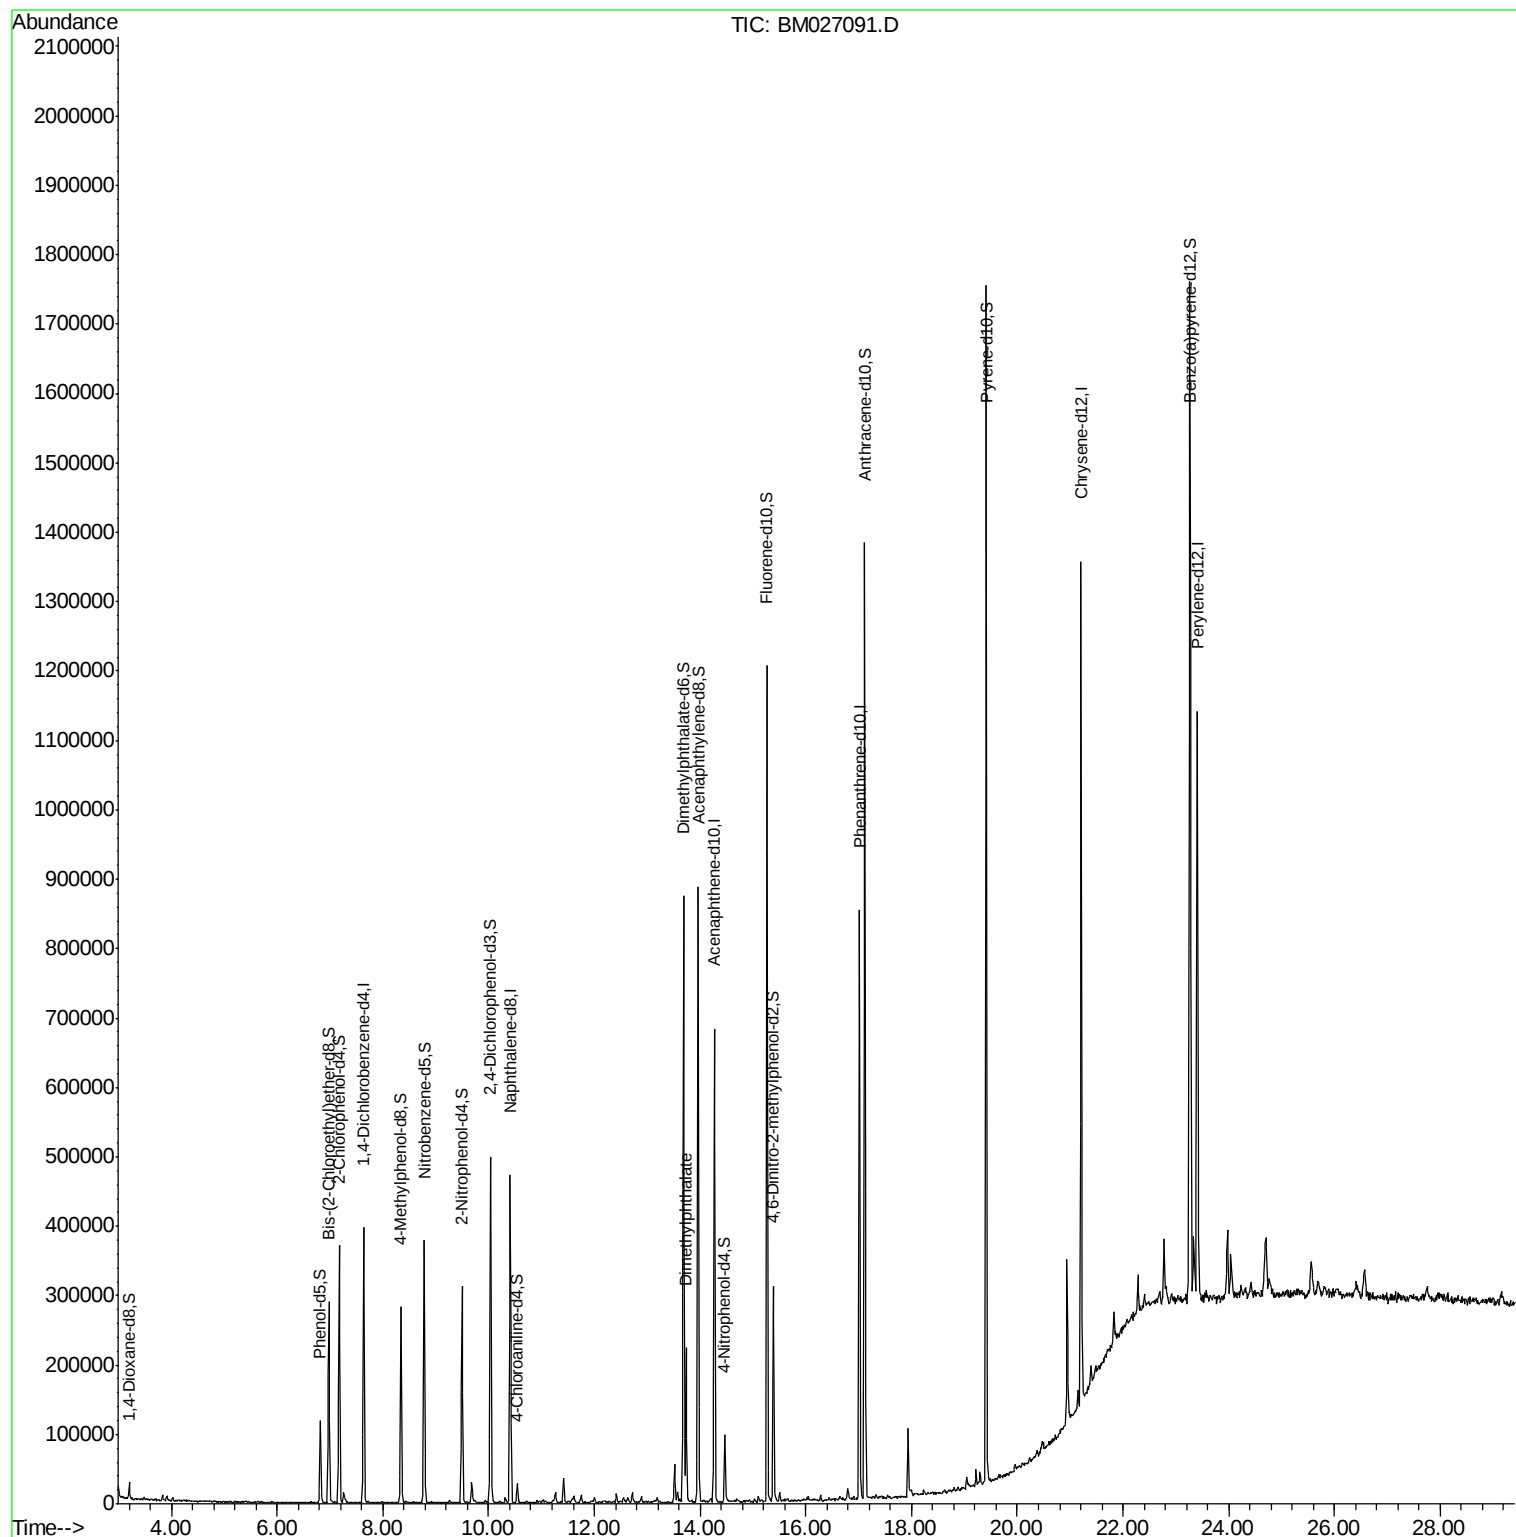

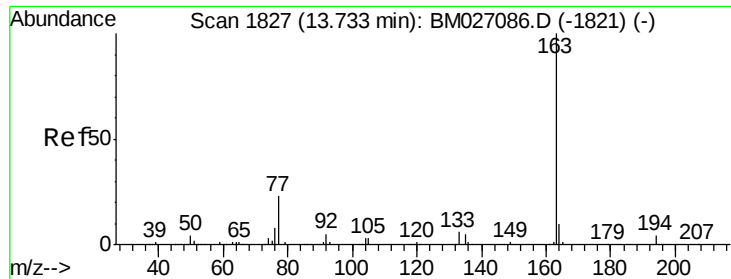

#45

Dimethylphthalate

Concen: 6.767 ng/ul

RT: 13.73 min Scan# 1827

Delta R.T. -0.00 min

Lab File: BM027091.D

Acq: 14 Aug 2020 16:40

Instrument :

BNA_M

ClientSampleId :

CB7H6


Tot Ion:163 Resp: 121908

Ion Ratio Lower Upper

163 100

194 4.6 3.2 4.8

164 10.0 8.2 12.2

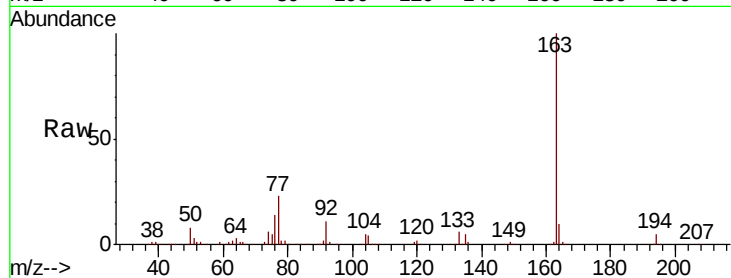

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

