

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
 Data File : BM002400.D
 Acq On : 15 Aug 2015 00:05
 Operator : UM/IZ
 Sample : SSTDICC020
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 17 01:56:26 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 17 01:53:35 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	80348	20.00	ng/ul	0.00
2) Naphthalene-d8	11.74	136	397611	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.45	164	232264	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.15	188	511309	20.00	ng/ul	0.00
17) Chrysene-d12	22.23	240	550638	20.00	ng/ul	0.00
22) Perylene-d12	24.89	264	564677	20.00	ng/ul	0.00

System Monitoring Compounds

7) Acenaphthylene-d8	15.15	160	471693	19.86	ng/ul	0.00
10) Fluorene-d10	16.42	176	330023	19.79	ng/ul	0.00
14) Anthracene-d10	18.25	188	488258	19.80	ng/ul	0.00
18) Pyrene-d10	20.46	212	510103	20.90	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.71	264	584334	19.70	ng/ul	0.00

Target Compounds


						Ovalue
3) Naphthalene	11.79	128	400089	19.72	ng/ul	100
4) 2-Methylnaphthalene	13.33	142	300407	19.76	ng/ul	98
5) 1-Methylnaphthalene	13.55	142	297143	19.76	ng/ul	100
8) Acenaphthylene	15.18	152	491542	19.78	ng/ul	100
9) Acenaphthene	15.51	153	324115	19.80	ng/ul	99
11) Fluorene	16.47	166	374878	19.98	ng/ul	99
13) Phenanthrene	18.19	178	583267	19.75	ng/ul	99
15) Anthracene	18.28	178	591663	19.77	ng/ul	100
16) Fluoranthene	20.14	202	647690	19.38	ng/ul	100
19) Pyrene	20.49	202	676490	20.97	ng/ul	99
20) Benzo(a)anthracene	22.21	228	648511	19.69	ng/ul	100
21) Chrysene	22.27	228	610076	19.81	ng/ul	99
23) Benzo(b)fluoranthene	24.06	252	662793	19.42	ng/ul	99
24) Benzo(k)fluoranthene	24.12	252	644131	19.91	ng/ul	99
26) Benzo(a)pyrene	24.77	252	643936	19.75	ng/ul	99
27) Indeno(1,2,3-cd)pyrene	27.69	276	757205	20.19	ng/ul	99
28) Dibenzo(a,h)anthracene	27.70	278	637221	20.33	ng/ul	99
29) Benzo(a,h,i)perylene	28.57	276	631441	20.23	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
Data File : BM002400.D
Acq On : 15 Aug 2015 00:05
Operator : UM/IZ
Sample : SSTDICC020
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 17 01:56:26 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 17 01:53:35 2015
Response via : Initial Calibration

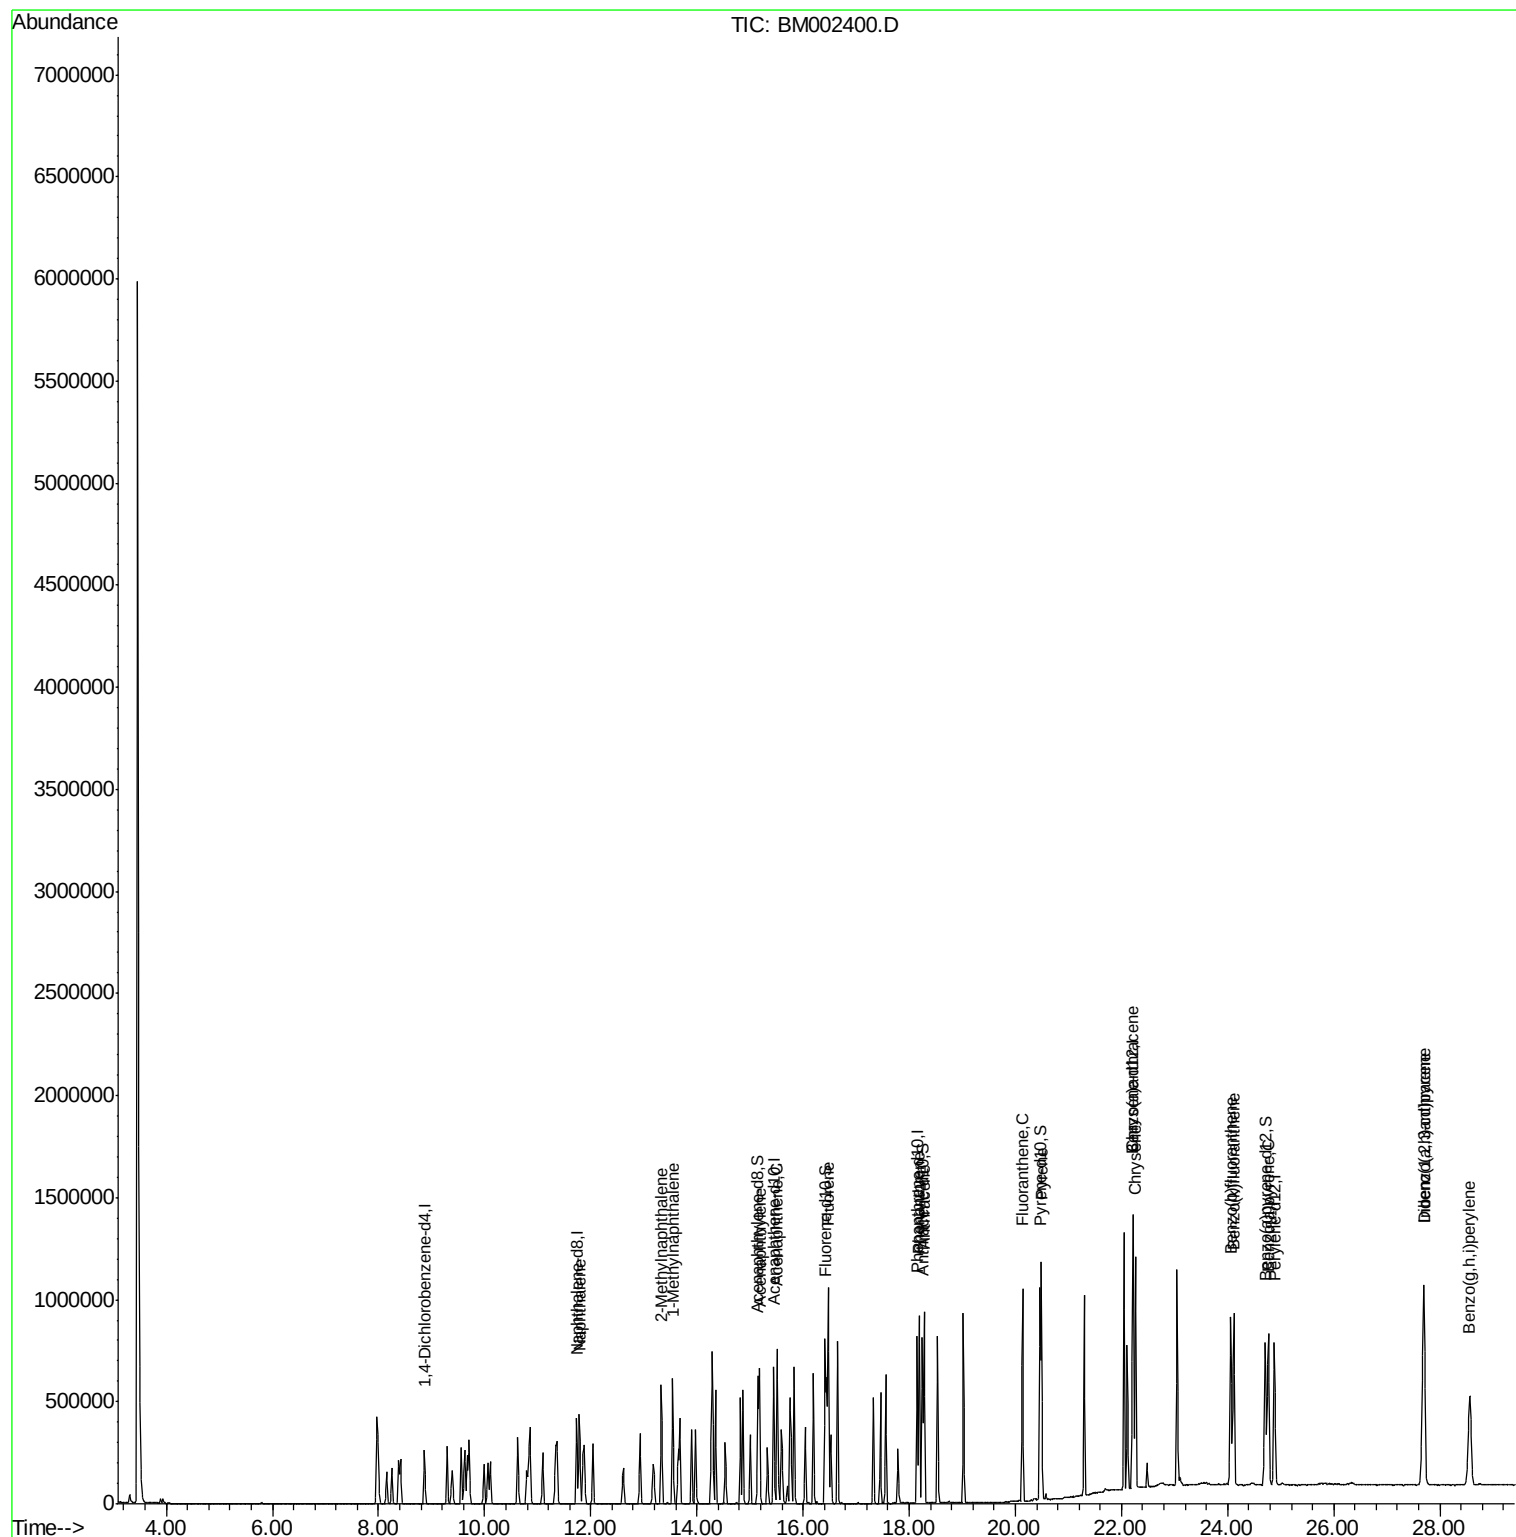

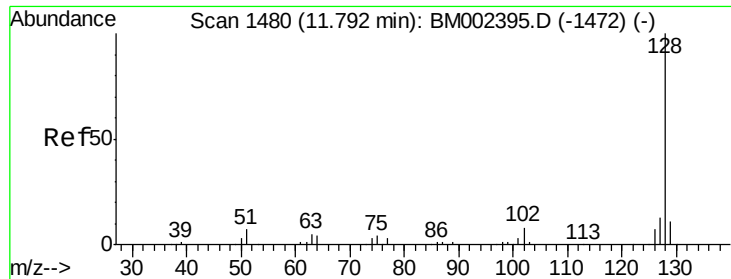

#3

Naphthalene

Concen: 19.72 ng/ul

RT: 11.79 min Scan# 1479

Delta R.T. -0.01 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05

Instrument :

BNA_M

ClientSampleId :


Tot Ion:128 Resp: 400089

Ion Ratio Lower Upper

128 100

129 10.7 8.6 12.8




127 13.2 10.4 15.6

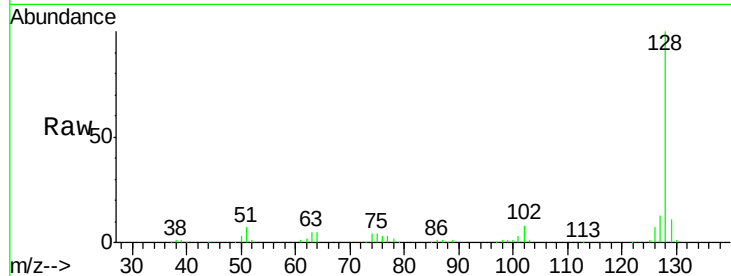

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

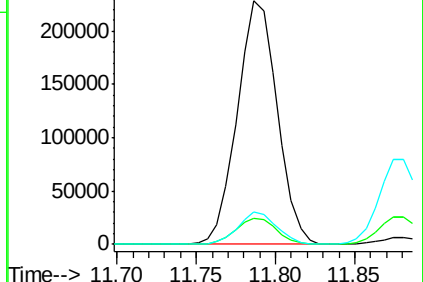

#4

2-Methylnaphthalene

Concen: 19.76 ng/ul

RT: 13.33 min Scan# 1741

Delta R.T. -0.01 min

Lab File: BM002400.D


Acq: 15 Aug 2015 00:05

Tgt Ion:142 Resp: 300407

Ion Ratio Lower Upper



142 100


141 88.7 72.2 108.2



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

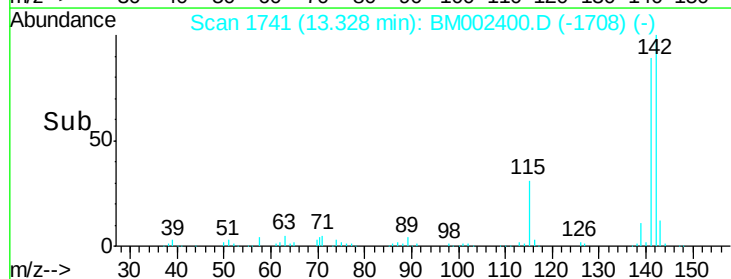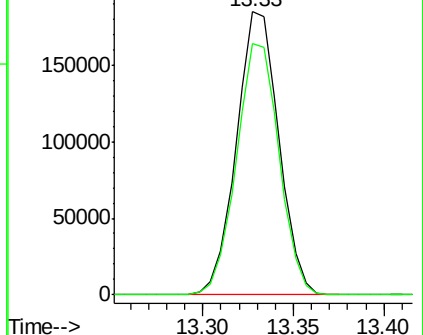



#5

1-Methylnaphthalene

Concen: 19.76 ng/ul

RT: 13.55 min Scan# 1778

Delta R.T. 0.00 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05

Instrument :

BNA_M

ClientSampled :


Tot Ion:142 Resp: 297143

Ion Ratio Lower Upper

142 100

141 92.0 73.9 110.9

116 3.6 3.0 4.4




Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E


Ion 116.00 (115.70 to 116.70): E

Time-->



Abundance

Time-->



#8

Acenaphthylene

Concen: 19.78 ng/ul

RT: 15.18 min Scan# 2056

Delta R.T. 0.00 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05


Tgt Ion:152 Resp: 491542

Ion Ratio Lower Upper

152 100

151 19.5 15.7 23.5

153 13.2 10.2 15.4




Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E


Ion 153.00 (152.70 to 153.70): E

Time-->



Abundance

Time-->



#9

Acenaphthene

Concen: 19.80 ng/ul

RT: 15.51 min Scan# 2112

Delta R.T. 0.00 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05

Instrument :

BNA_M

ClientSampled :


Tot Ion:153 Resp: 324115

Ion Ratio Lower Upper

153 100

152 46.5 36.9 55.3




154 88.1 71.3 106.9



Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

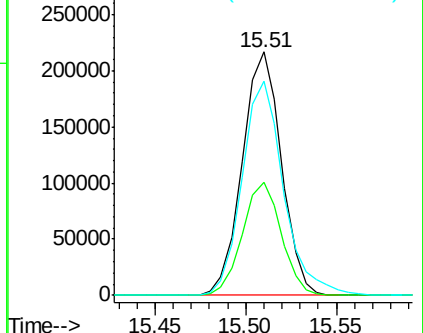

#11

Fluorene

Concen: 19.98 ng/ul

RT: 16.47 min Scan# 2275

Delta R.T. -0.01 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05


Tgt Ion:166 Resp: 374878

Ion Ratio Lower Upper

166 100

165 96.2 77.6 116.4



167 13.1 10.7 16.1




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

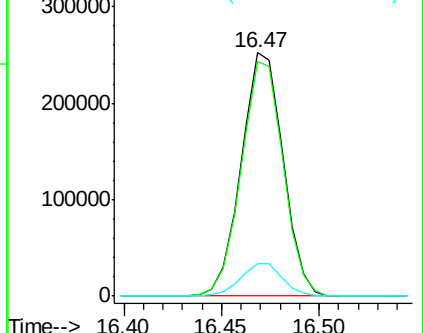

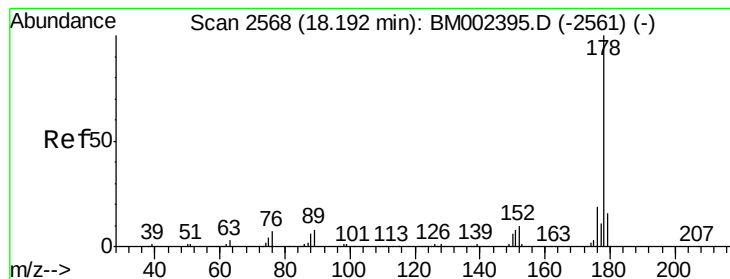

#13

Phenanthrene

Concen: 19.75 ng/ul

RT: 18.19 min Scan# 2568

Delta R.T. 0.00 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05


Instrument :

BNA_M

ClientSampleId :

Tot Ion:178 Resp: 583267


Ion	Ratio	Lower	Upper
178	100		
179	15.0	12.4	18.6
176	19.0	15.1	22.7

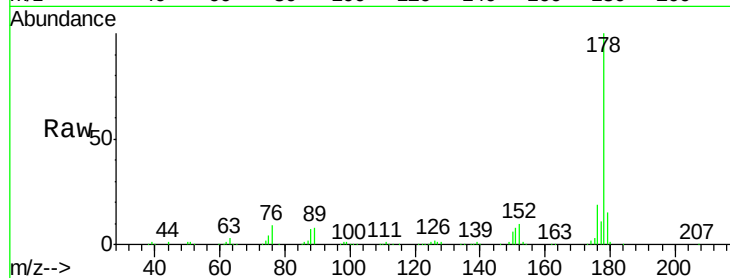


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

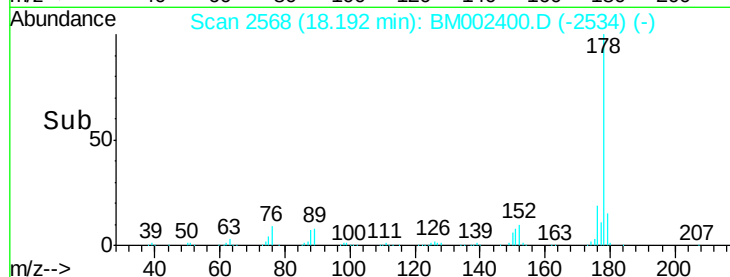

Time-->

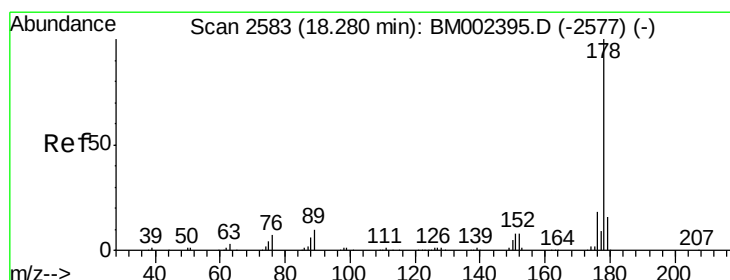

#15

Anthracene

Concen: 19.77 ng/ul

RT: 18.28 min Scan# 2583


Delta R.T. 0.00 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05

Tgt Ion:178 Resp: 591663


Ion	Ratio	Lower	Upper
178	100		
179	15.4	12.6	18.8
176	18.1	14.5	21.7

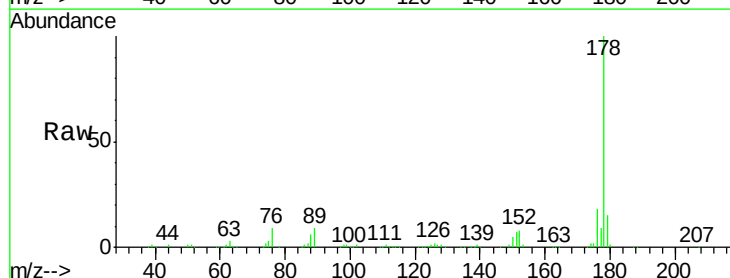


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

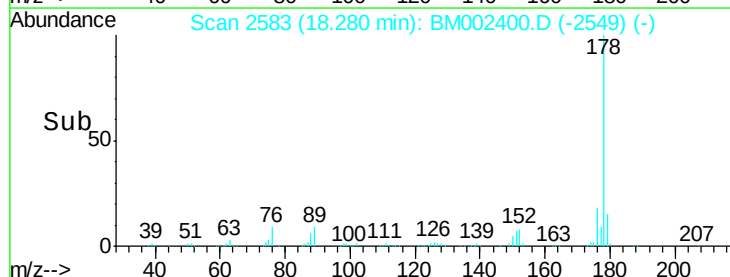





Time-->



#16
 Fluoranthene
 Concen: 19.38 ng/ul
 RT: 20.14 min Scan# 2899
 Delta R.T. 0.00 min
 Lab File: BM002400.D
 Acq: 15 Aug 2015 00:05




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
202	100		
101	12.0	9.7	14.5
100	9.3	7.4	11.2

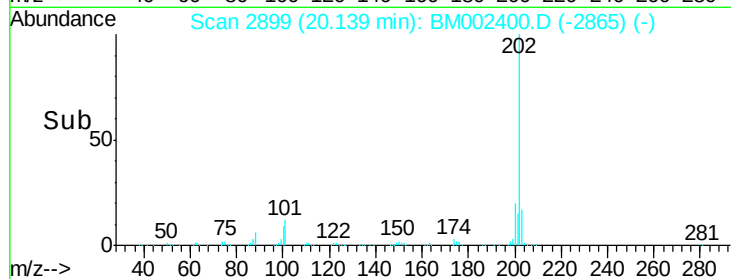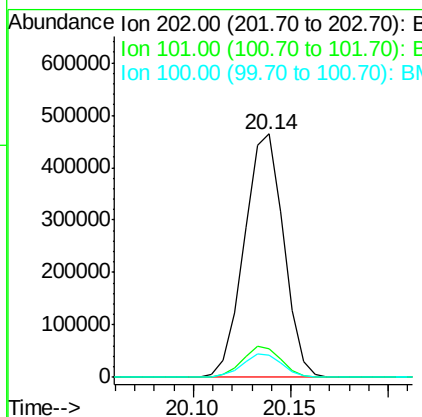

#19
 Pyrene
 Concen: 20.97 ng/ul
 RT: 20.49 min Scan# 2959
 Delta R.T. 0.00 min
 Lab File: BM002400.D
 Acq: 15 Aug 2015 00:05

Tgt Ion	Ratio	Lower	Upper
202	100		
101	15.2	12.0	18.0
100	12.4	9.7	14.5

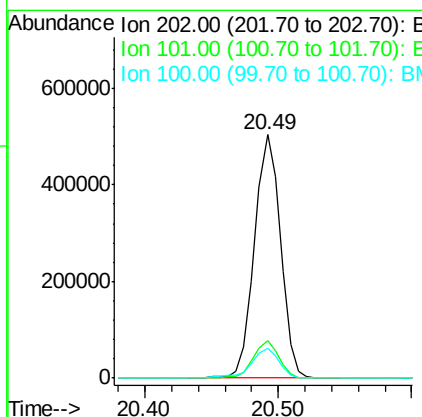

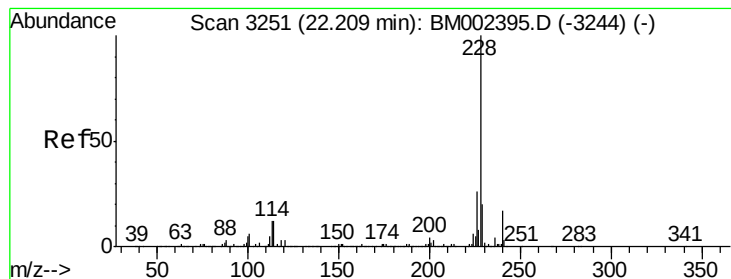

#20

Benzo(a)anthracene

Concen: 19.69 ng/ul

RT: 22.21 min Scan# 3251

Delta R.T. 0.00 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05

Instrument :

BNA_M

ClientSampled :


Tot Ion:228 Resp: 648511

Ion Ratio Lower Upper




228 100

229 19.6 15.8 23.6

226 26.4 21.1 31.7



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

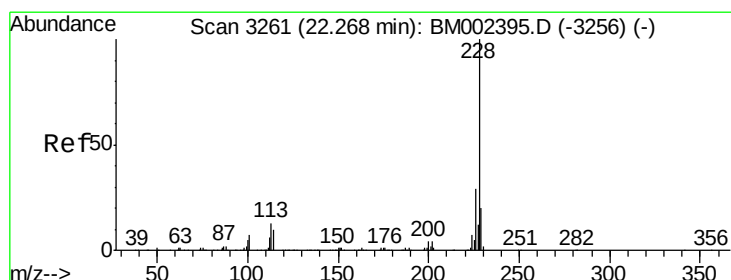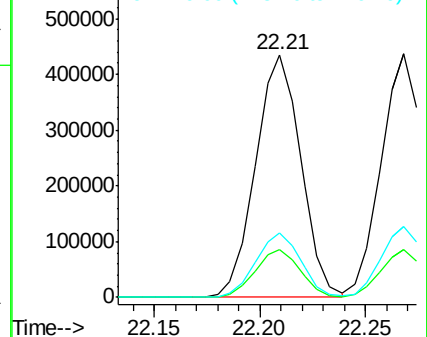

#21

Chrysene

Concen: 19.81 ng/ul

RT: 22.27 min Scan# 3261

Delta R.T. 0.00 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05


Tgt Ion:228 Resp: 610076

Ion Ratio Lower Upper



228 100


226 29.0 23.4 35.2

229 19.4 15.7 23.5



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

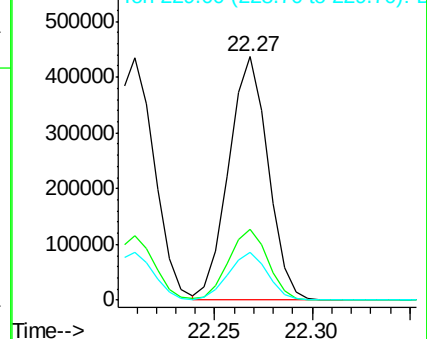



#23

Benzo(b)fluoranthene

Concen: 19.42 ng/ul

RT: 24.06 min Scan# 3566

Delta R.T. 0.00 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 662793

Ion Ratio Lower Upper

252 100

253 22.1 17.4 26.0




125 12.7 10.0 15.0



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

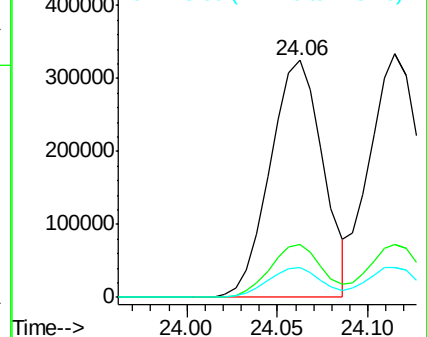

#24

Benzo(k)fluoranthene

Concen: 19.91 ng/ul

RT: 24.12 min Scan# 3575

Delta R.T. 0.00 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05


Tgt Ion:252 Resp: 644131

Ion Ratio Lower Upper

252 100

253 21.8 17.8 26.6



125 12.5 9.8 14.8




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

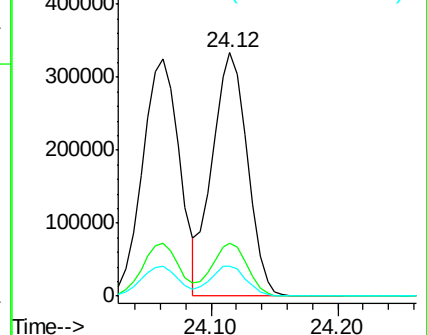

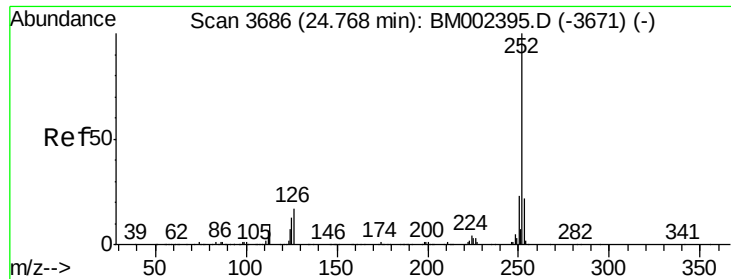

#26

Benzo(a)pyrene

Concen: 19.75 ng/ul

RT: 24.77 min Scan# 3686

Delta R.T. 0.00 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 643936

Ion Ratio Lower Upper

252 100

253 21.5 17.6 26.4




125 13.6 10.7 16.1

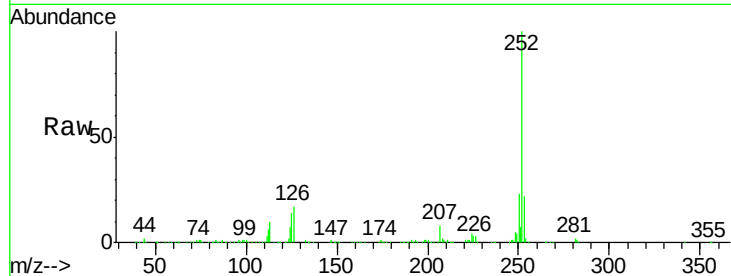

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

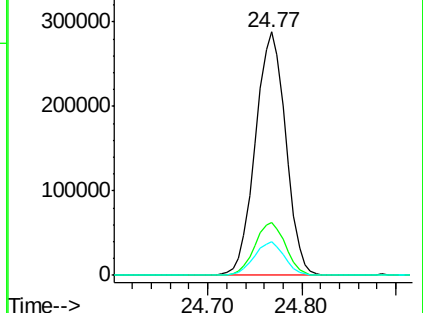

#27

Indeno(1,2,3-cd)pyrene

Concen: 20.19 ng/ul

RT: 27.69 min Scan# 4183

Delta R.T. -0.01 min

Lab File: BM002400.D

Acq: 15 Aug 2015 00:05


Tgt Ion:276 Resp: 757205

Ion Ratio Lower Upper

276 100

138 31.2 25.3 37.9



277 25.0 20.2 30.2




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

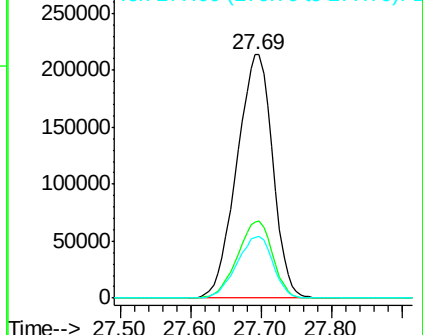




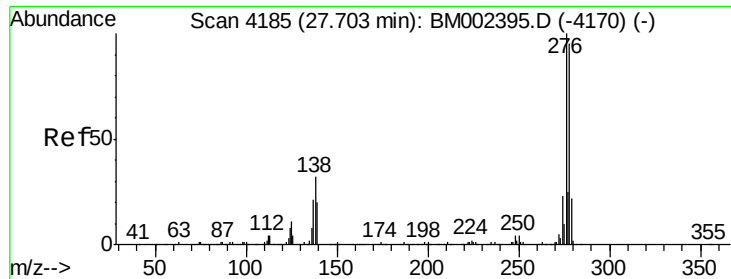


#28
Dibenzo(a,h)anthracene
Concen: 20.33 ng/ul
RT: 27.70 min Scan# 4184
Delta R.T. -0.01 min
Lab File: BM002400.D
Acq: 15 Aug 2015 00:05

Instrument :
BNA_M
ClientSampleId :

Tot Ion:278 Resp: 637221

Ion	Ratio	Lower	Upper
278	100		
139	19.9	16.5	24.7
279	23.2	18.8	28.2

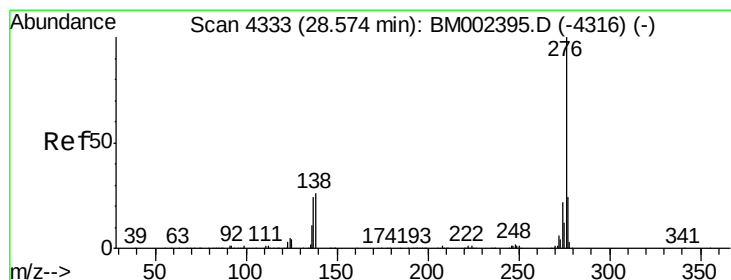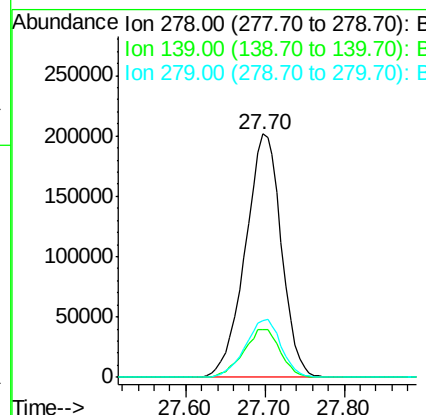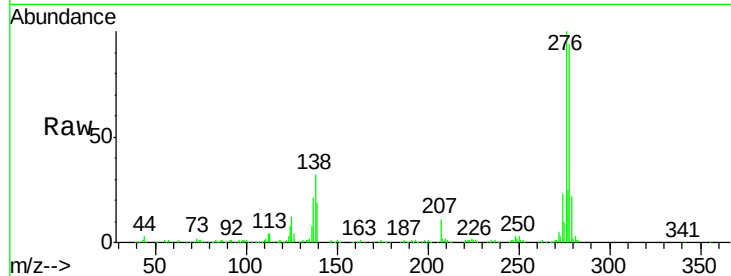

#29
Benzo(g,h,i)perylene
Concen: 20.23 ng/ul
RT: 28.57 min Scan# 4332
Delta R.T. -0.01 min
Lab File: BM002400.D
Acq: 15 Aug 2015 00:05

Tgt Ion:276 Resp: 631441

Ion	Ratio	Lower	Upper
276	100		
138	26.3	21.0	31.6
277	23.7	19.2	28.8

