

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
 Data File : BM002414.D
 Acq On : 15 Aug 2015 08:32
 Operator : UM/IZ
 Sample : G3194-21
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 17 02:55:54 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 17 02:54:04 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	164847	20.00	ng/ul	0.00
2) Naphthalene-d8	11.74	136	767654	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.45	164	398925	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.15	188	811176	20.00	ng/ul	0.00
17) Chrysene-d12	22.22	240	674681	20.00	ng/ul	0.00
22) Perylene-d12	24.88	264	526940	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	15.15	160	679971	16.67	ng/ul	0.00
10) Fluorene-d10	16.42	176	450018	15.71	ng/ul	0.00
14) Anthracene-d10	18.24	188	648817	16.58	ng/ul	0.00
18) Pyrene-d10	20.46	212	621906	20.80	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.71	264	423872	15.31	ng/ul	0.00
Target Compounds				Ovalue		
13) Phenanthrene	18.19	178	223319	4.77	ng/ul	99
16) Fluoranthene	20.13	202	388659	7.33	ng/ul	99
19) Pyrene	20.49	202	312881	7.92	ng/ul	99
20) Benzo(a)anthracene	22.20	228	169567	4.20	ng/ul	99
21) Chrysene	22.20	228	169344	4.49	ng/ul	95
23) Benzo(b)fluoranthene	24.06	252	225775	7.09	ng/ul	96
26) Benzo(a)pyrene	24.76	252	127867	4.20	ng/ul	96
27) Indeno(1,2,3-cd)pyrene	27.68	276	92505	2.64	ng/ul	96
29) Benzo(g,h,i)perylene	28.56	276	83576	2.87	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
Data File : BM002414.D
Acq On : 15 Aug 2015 08:32
Operator : UM/IZ
Sample : G3194-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 17 02:55:54 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 17 02:54:04 2015
Response via : Initial Calibration

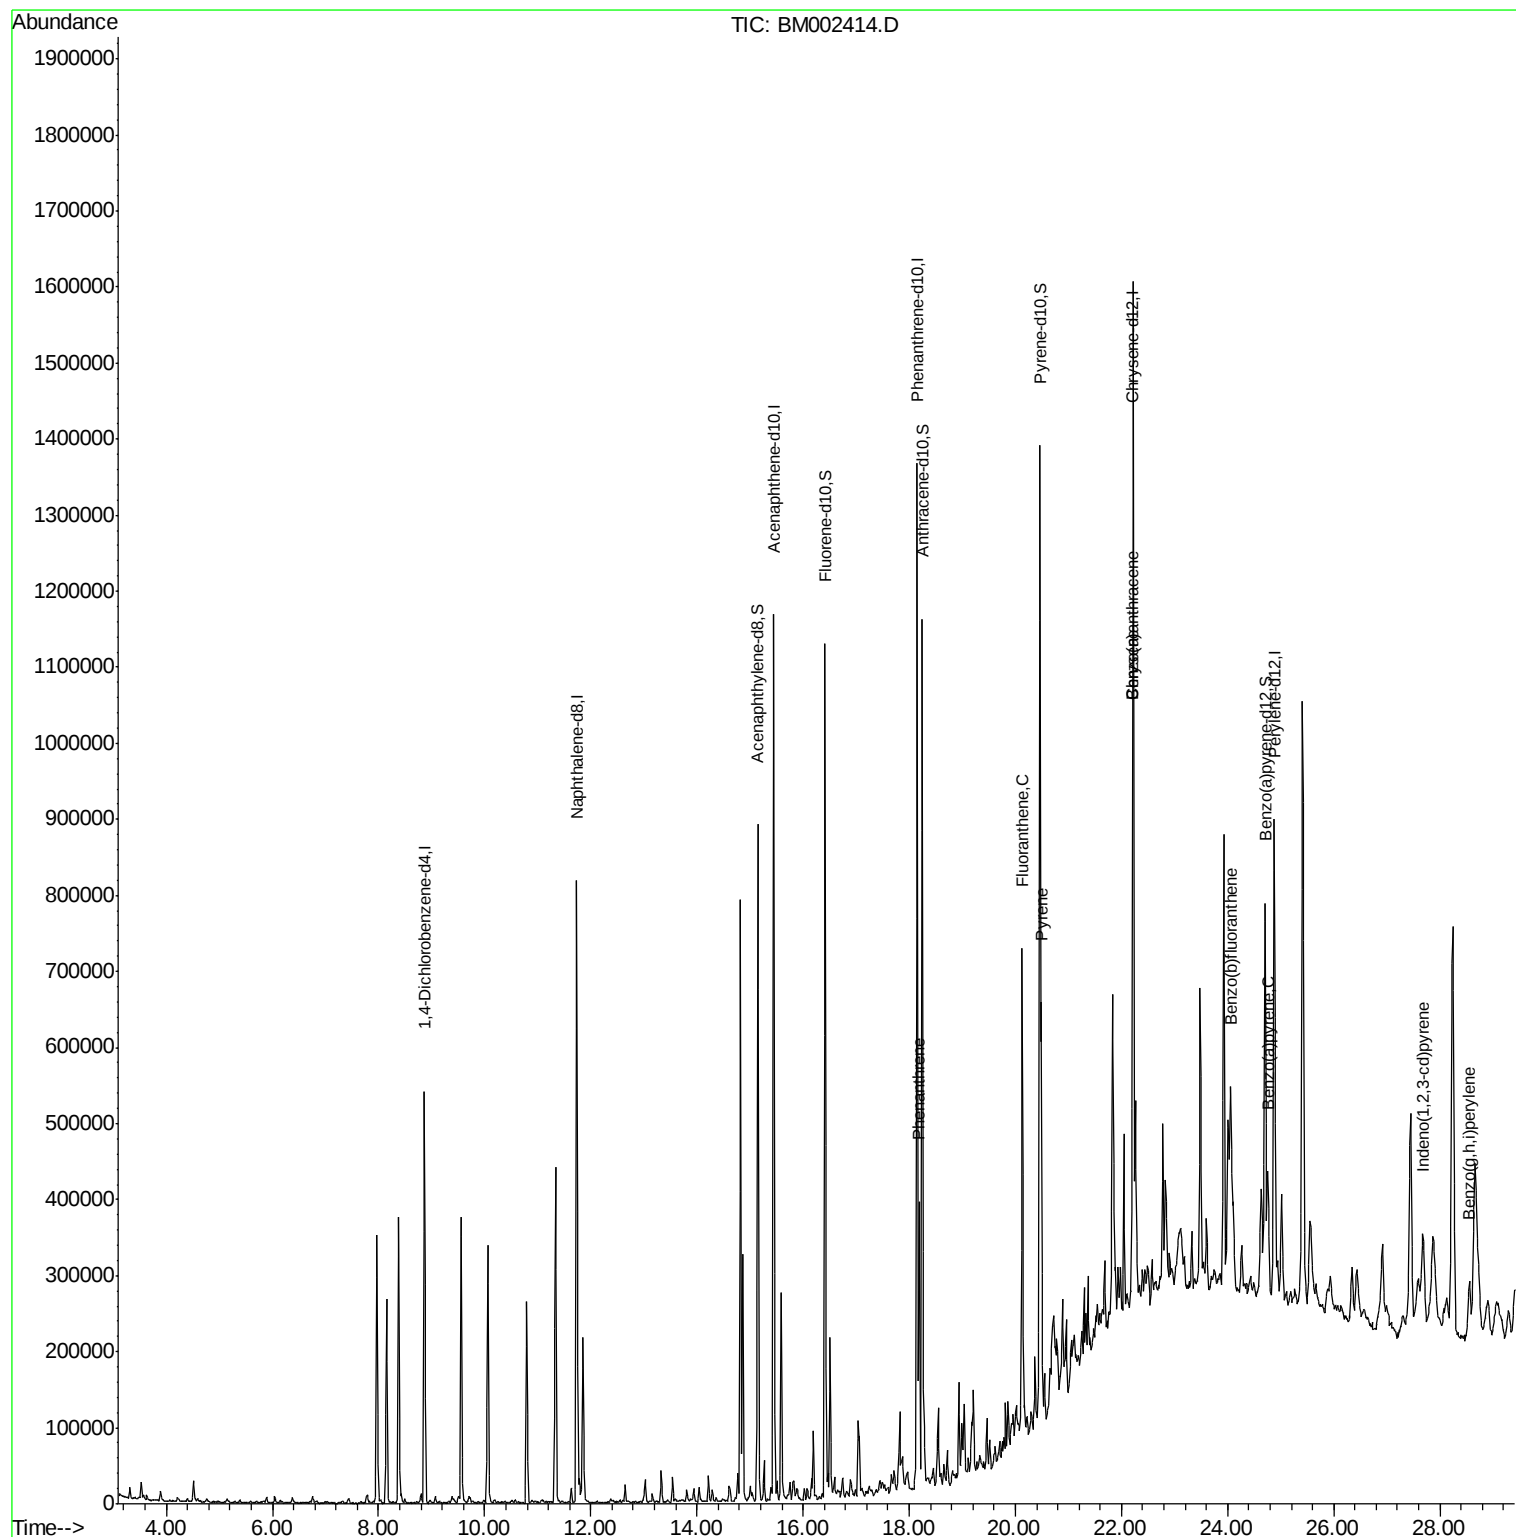

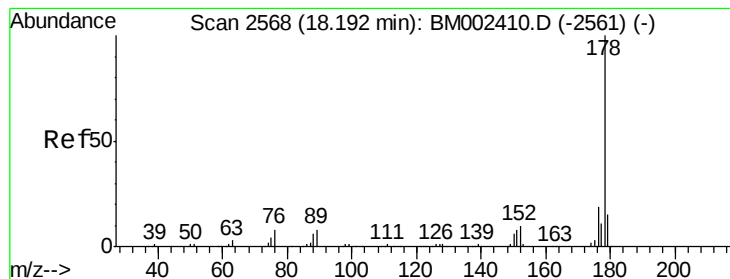

#13

Phenanthrene

Concen: 4.77 ng/ul

RT: 18.19 min Scan# 2568

Delta R.T. 0.00 min

Lab File: BM002414.D

Acq: 15 Aug 2015 08:32

Instrument :

BNA_M

ClientSampleId :


Tot Ion:178 Resp: 223319

Ion Ratio Lower Upper

178 100

179 15.6 12.4 18.6




176 18.5 15.1 22.7

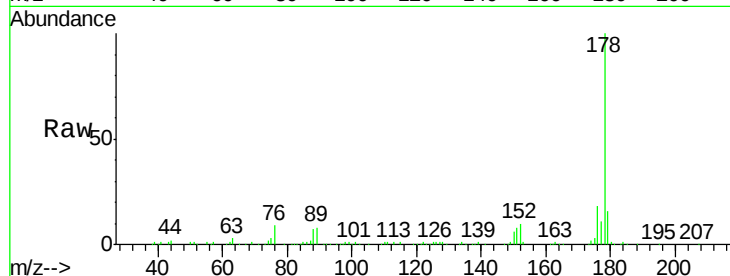

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

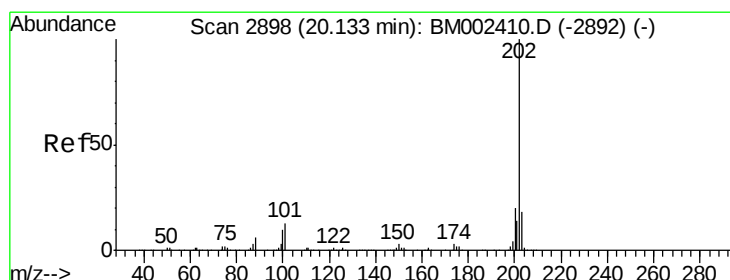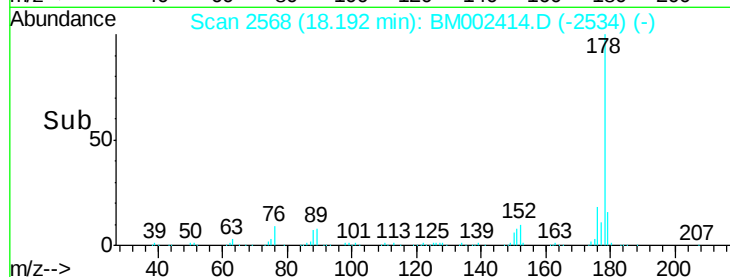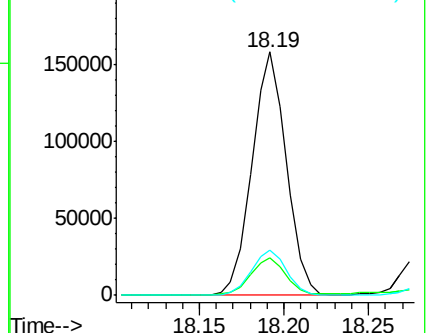

#16

Fluoranthene

Concen: 7.33 ng/ul

RT: 20.13 min Scan# 2898

Delta R.T. 0.00 min

Lab File: BM002414.D

Acq: 15 Aug 2015 08:32


Tgt Ion:202 Resp: 388659

Ion Ratio Lower Upper

202 100

101 12.6 9.7 14.5



100 9.5 7.4 11.2

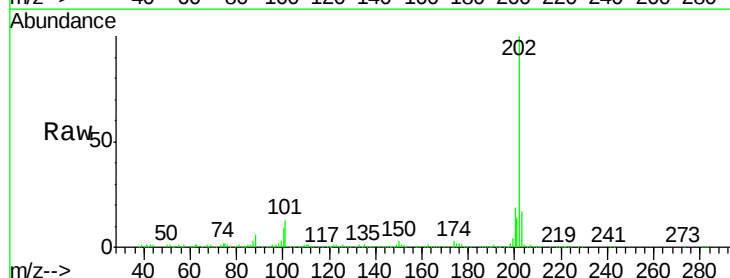


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

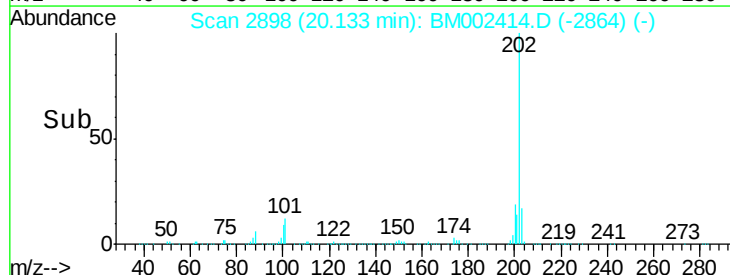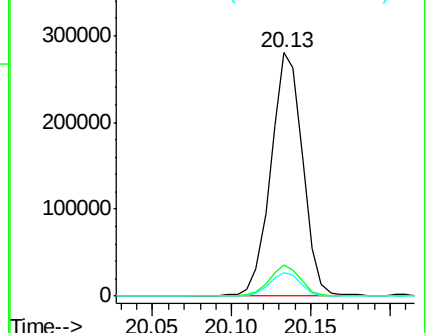

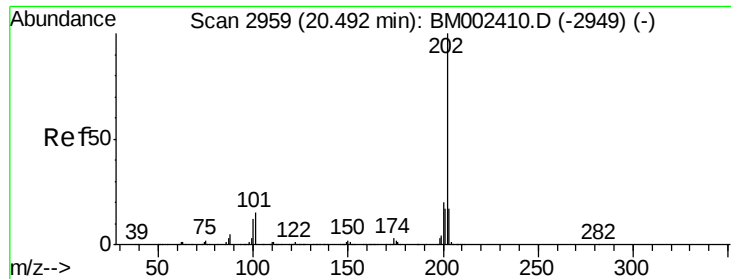

#19

Pvrene

Concen: 7.92 ng/ul

RT: 20.49 min Scan# 2959

Delta R.T. 0.00 min

Lab File: BM002414.D

Acq: 15 Aug 2015 08:32

Instrument :

BNA_M

ClientSampleId :


Tot Ion:202 Resp: 312881

Ion Ratio Lower Upper

202 100

101 14.5 12.0 18.0




100 11.7 9.7 14.5

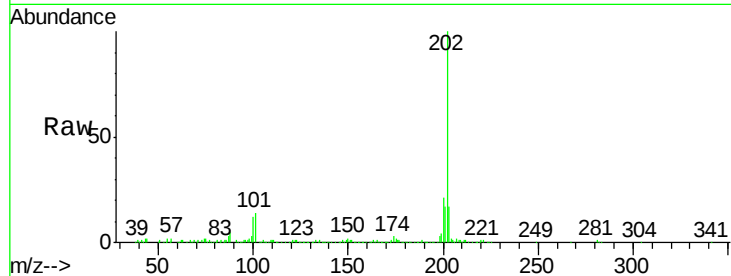

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

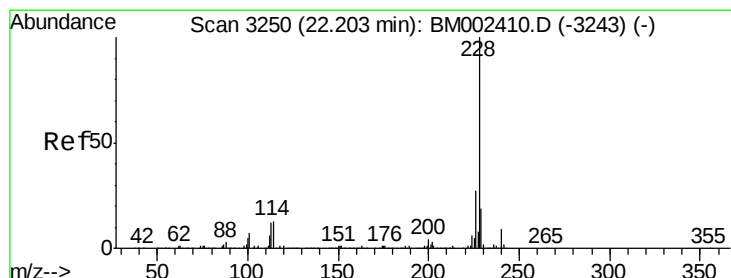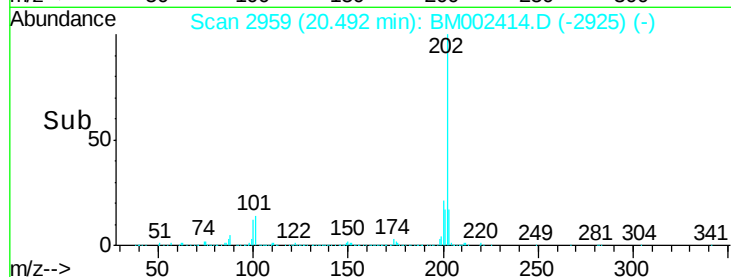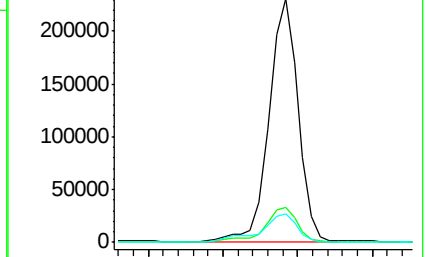

#20

Benzo(a)anthracene

Concen: 4.20 ng/ul

RT: 22.20 min Scan# 3250

Delta R.T. 0.00 min

Lab File: BM002414.D

Acq: 15 Aug 2015 08:32


Tgt Ion:228 Resp: 169567

Ion Ratio Lower Upper

228 100

229 21.2 15.8 23.6



226 26.5 21.1 31.7

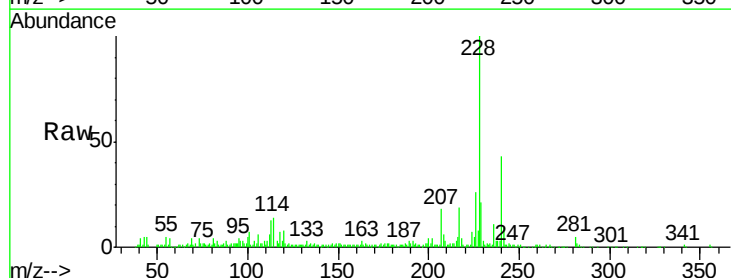


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

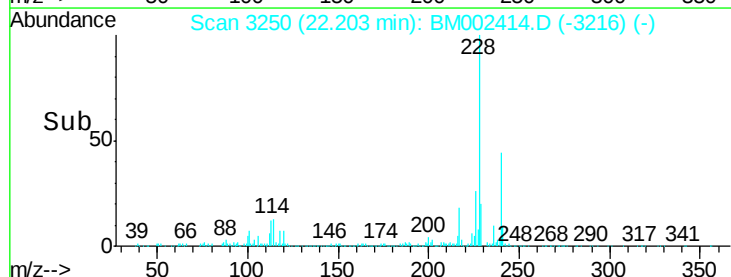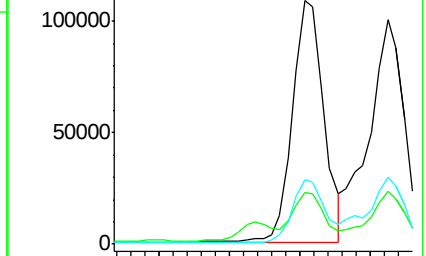

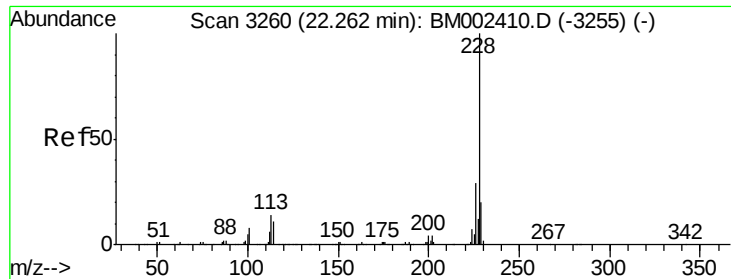

#21

Chrysene

Concen: 4.49 ng/u1

RT: 22.20 min Scan# 3250

Delta R.T. -0.06 min

Lab File: BM002414.D

Acq: 15 Aug 2015 08:32

Instrument :

BNA_M

ClientSampled :


Tot Ion:228 Resp: 169344

Ion Ratio Lower Upper

228 100

226 26.5 23.4 35.2




229 21.2 15.7 23.5

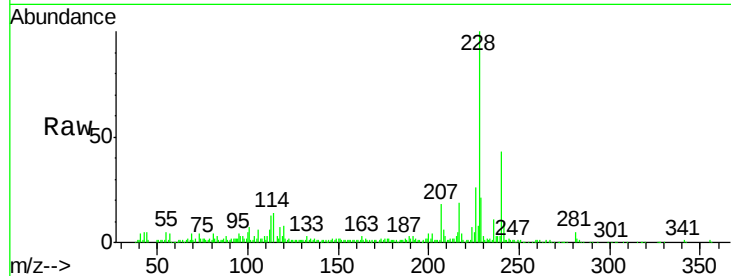

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

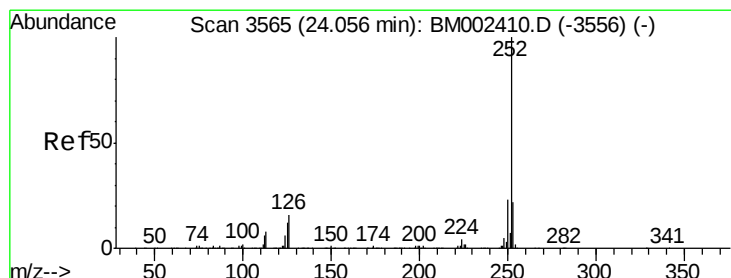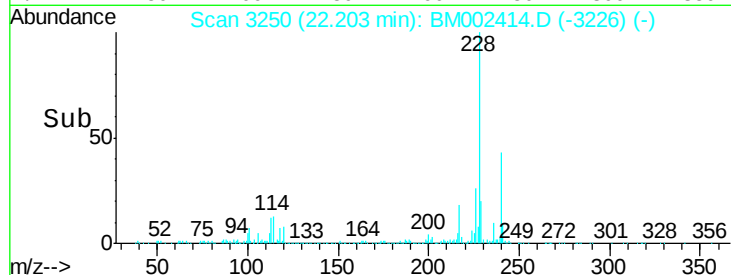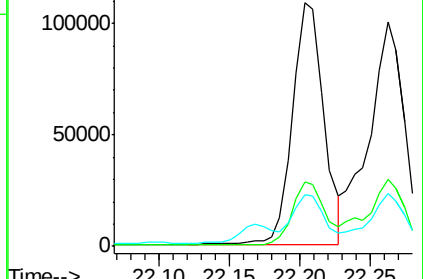

#23

Benzo(b)fluoranthene

Concen: 7.09 ng/u1

RT: 24.06 min Scan# 3565

Delta R.T. 0.00 min

Lab File: BM002414.D

Acq: 15 Aug 2015 08:32


Tgt Ion:252 Resp: 225775

Ion Ratio Lower Upper

252 100

253 23.0 17.4 26.0



125 14.8 10.0 15.0

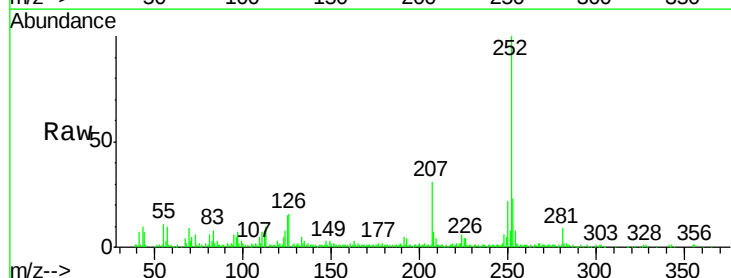


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

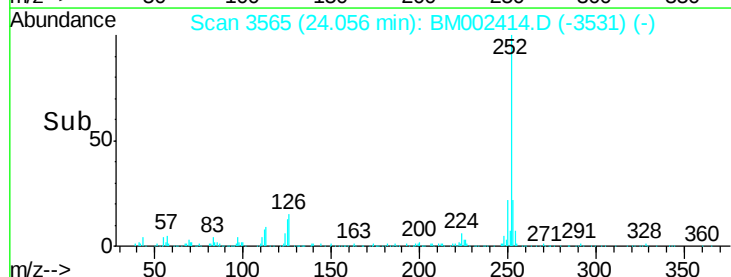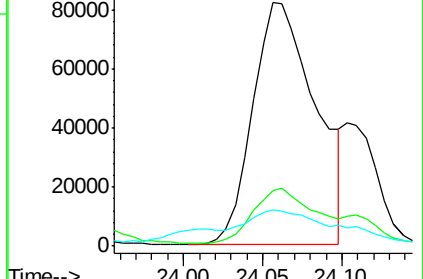

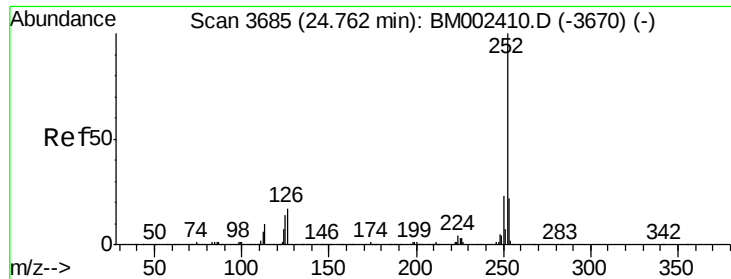

#26

Benzo(a)pyrene

Concen: 4.20 ng/ul

RT: 24.76 min Scan# 3685

Delta R.T. 0.00 min

Lab File: BM002414.D

Acq: 15 Aug 2015 08:32

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 127867

Ion Ratio Lower Upper

252 100

253 23.4 17.6 26.4




125 15.6 10.7 16.1

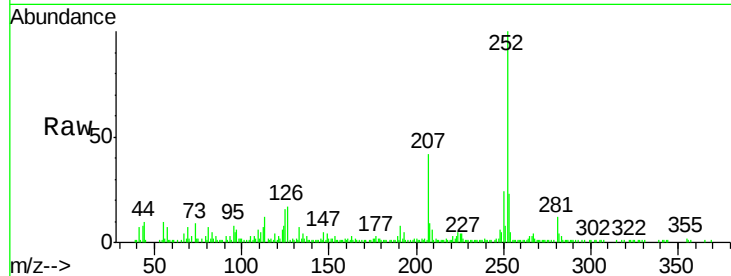

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

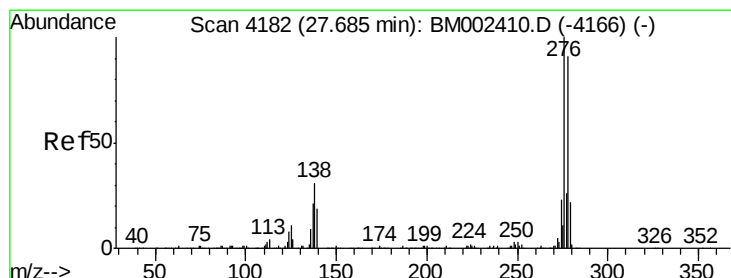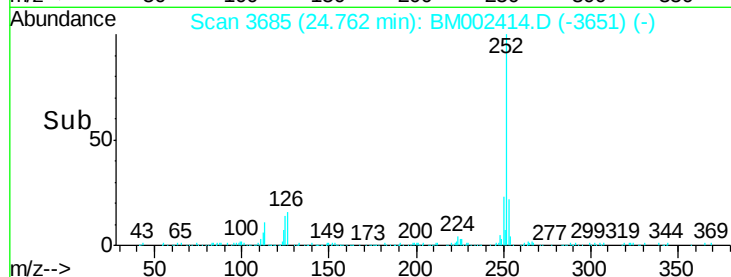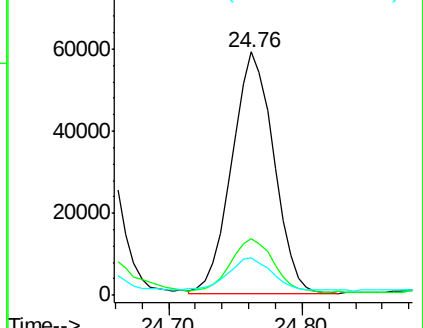

#27

Indeno(1,2,3-cd)pyrene

Concen: 2.64 ng/ul

RT: 27.68 min Scan# 4181

Delta R.T. -0.01 min

Lab File: BM002414.D

Acq: 15 Aug 2015 08:32


Tgt Ion:276 Resp: 92505

Ion Ratio Lower Upper

276 100

138 29.2 25.3 37.9



277 26.7 20.2 30.2

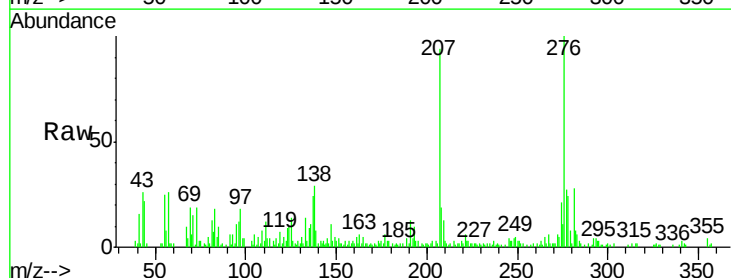


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

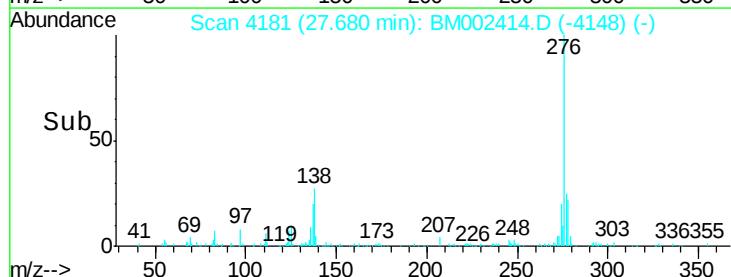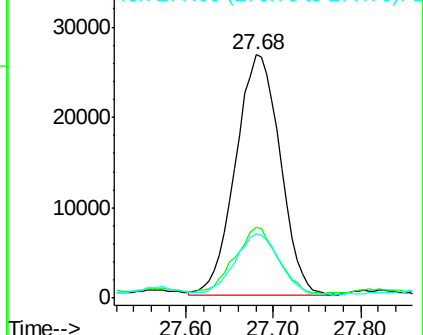

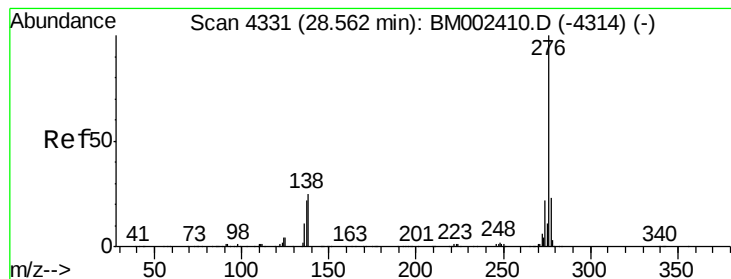

#29
 Benzo(a,h,i)perylene
 Concen: 2.87 ng/ul
 RT: 28.56 min Scan# 4331
 Delta R.T. 0.00 min
 Lab File: BM002414.D
 Acq: 15 Aug 2015 08:32

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
276	100		
138	28.1	21.0	31.6
277	25.4	19.2	28.8

