

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
 Data File : BM002424.D
 Acq On : 15 Aug 2015 14:45
 Operator : UM/IZ
 Sample : G3219-11DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9DA4DL

Quant Time: Aug 17 02:57:32 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 17 02:54:04 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	173968	20.00	ng/ul	0.00
2) Naphthalene-d8	11.74	136	813626	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.45	164	443809	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.16	188	913679	20.00	ng/ul	0.00
17) Chrysene-d12	22.23	240	699261	20.00	ng/ul	0.00
22) Perylene-d12	24.90	264	570432	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
7) Acenaphthylene-d8	15.15	160	123045	2.71	ng/ul	0.00
10) Fluorene-d10	16.42	176	86752	2.72	ng/ul	0.00
14) Anthracene-d10	18.25	188	120759	2.74	ng/ul	0.00
18) Pyrene-d10	20.47	212	111383	3.59	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.72	264	72283	2.41	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Phenanthrene	18.20	178	76497	1.45	ng/ul	99
16) Fluoranthene	20.14	202	350827	5.87	ng/ul	99
19) Pyrene	20.50	202	350577	8.56	ng/ul	99
20) Benzo(a)anthracene	22.22	228	422705	10.11	ng/ul	99
21) Chrysene	22.27	228	501319	12.82	ng/ul	98
23) Benzo(b)fluoranthene	24.07	252	939680	27.25	ng/ul	98
24) Benzo(k)fluoranthene	24.28	252	75419	2.31	ng/ul#	90
26) Benzo(a)pyrene	24.78	252	564542	17.14	ng/ul	99
27) Indeno(1,2,3-cd)pyrene	27.71	276	486596	12.85	ng/ul	94
28) Dibenzo(a,h)anthracene	27.71	278	160842	5.08	ng/ul#	92
29) Benzo(g,h,i)perylene	28.60	276	442480	14.03	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
Data File : BM002424.D
Acq On : 15 Aug 2015 14:45
Operator : UM/IZ
Sample : G3219-11DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9DA4DL

Quant Time: Aug 17 02:57:32 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 17 02:54:04 2015
Response via : Initial Calibration

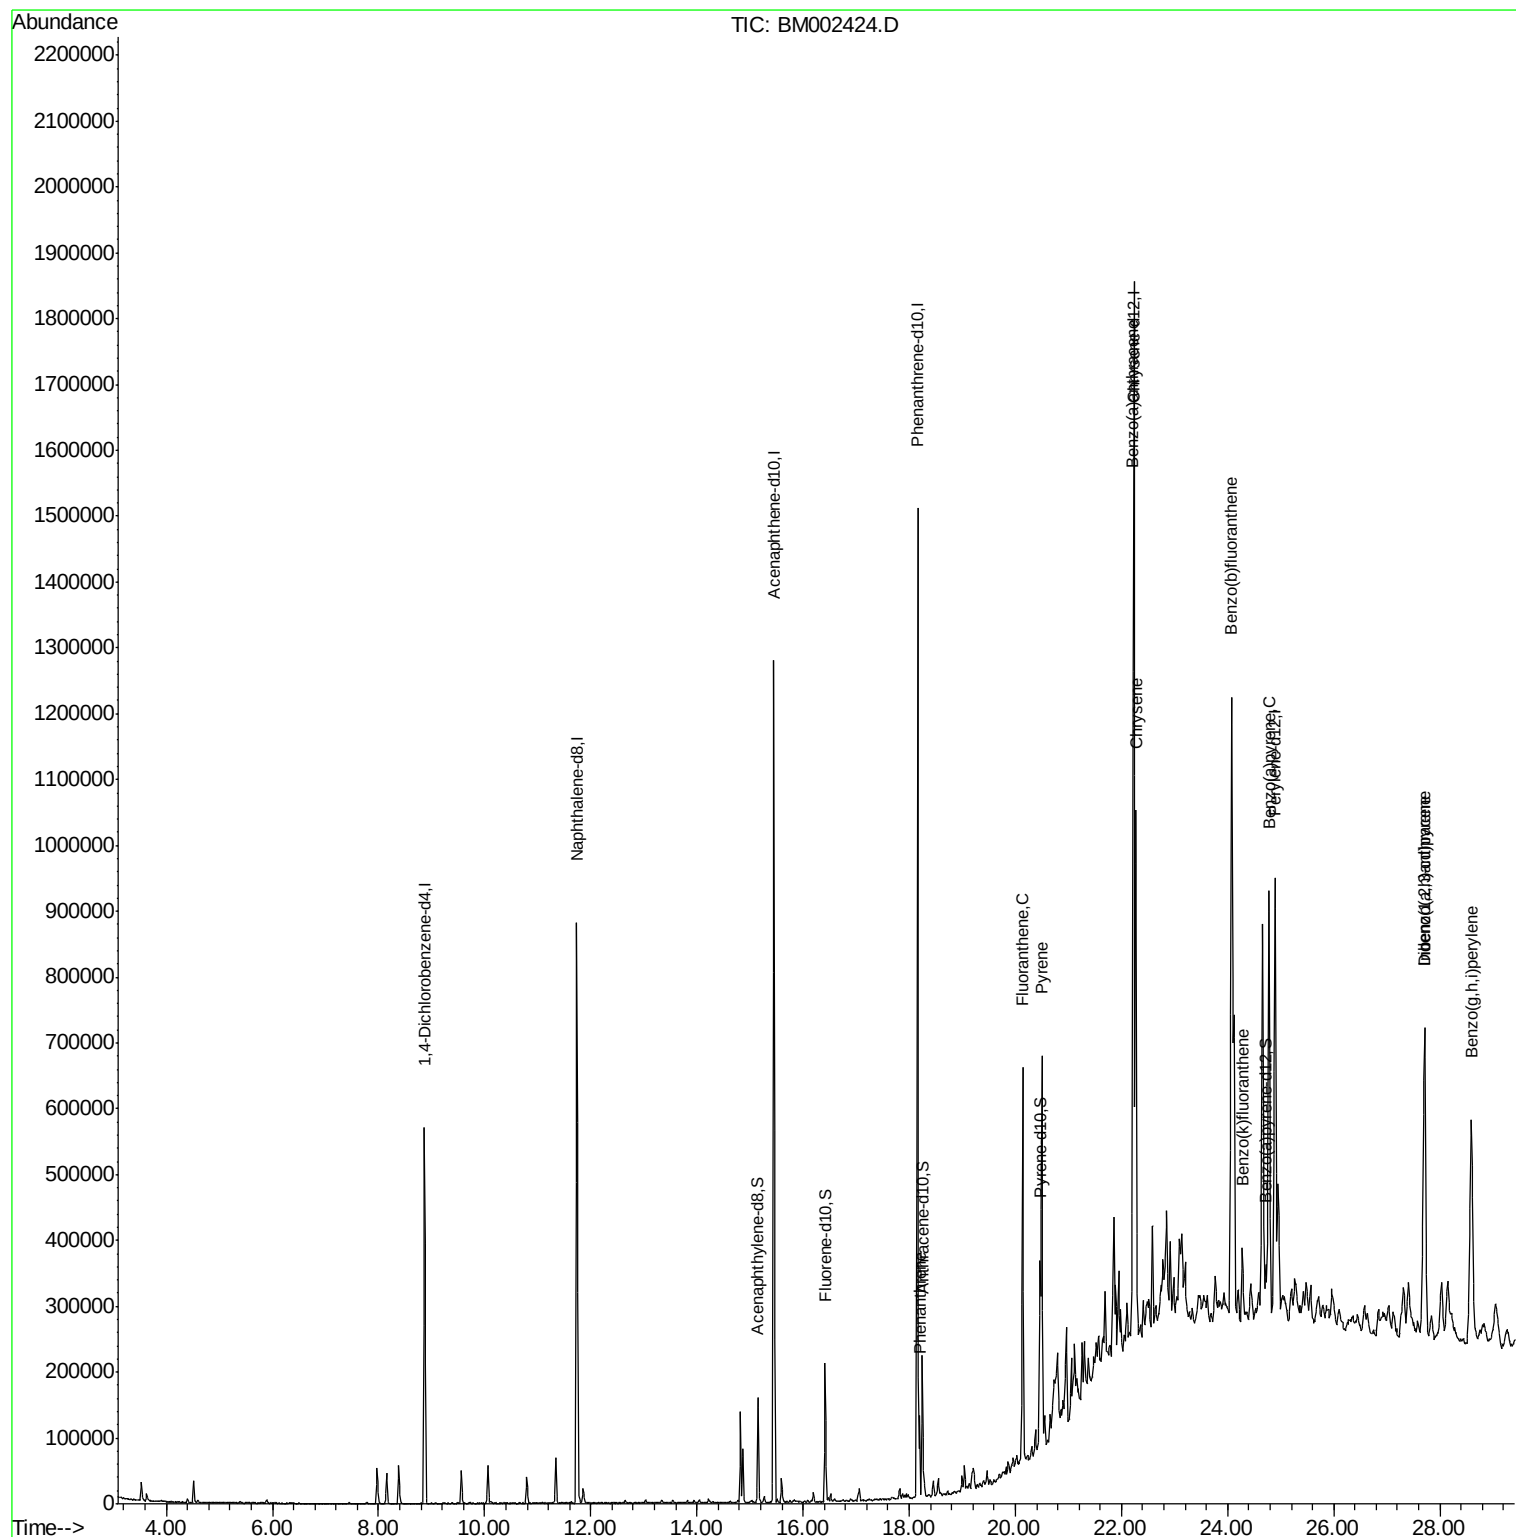

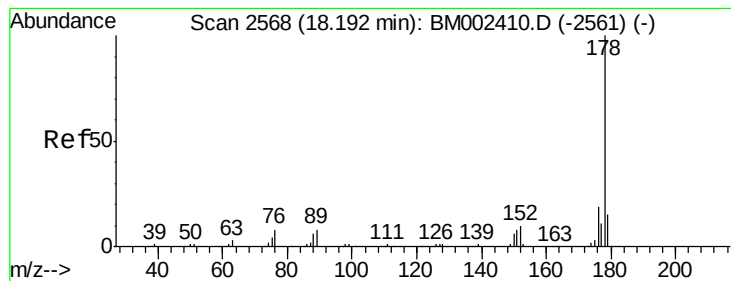

#13

Phenanthrene

Concen: 1.45 ng/ul

RT: 18.20 min Scan# 2569

Delta R.T. 0.01 min

Lab File: BM002424.D

Acq: 15 Aug 2015 14:45

Instrument :

BNA_M

ClientSampleID :

D9DA4DL


Tot Ion:178 Resp: 76497

Ion	Ratio	Lower	Upper
178	100		
179	15.5	12.4	18.6
176	18.3	15.1	22.7

178 100

179 15.5 12.4 18.6




176 18.3 15.1 22.7

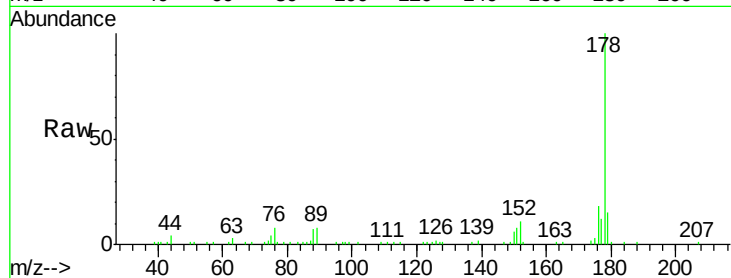

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

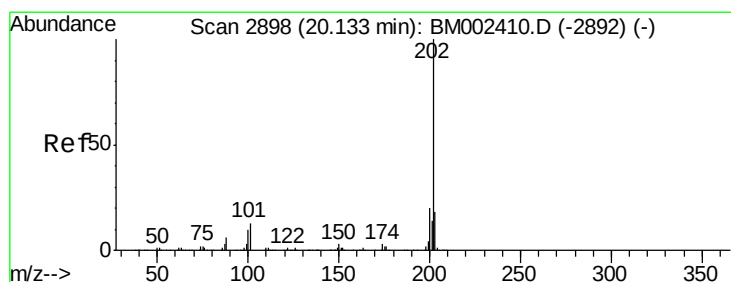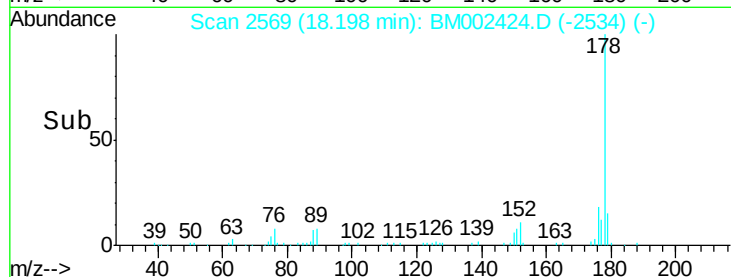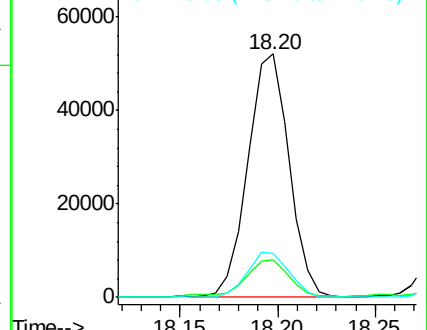

#16

Fluoranthene

Concen: 5.87 ng/ul

RT: 20.14 min Scan# 2899

Delta R.T. 0.01 min

Lab File: BM002424.D

Acq: 15 Aug 2015 14:45


Tgt Ion:202 Resp: 350827

Ion	Ratio	Lower	Upper
202	100		
101	12.4	9.7	14.5
100	9.5	7.4	11.2

202 100

101 12.4 9.7 14.5



100 9.5 7.4 11.2

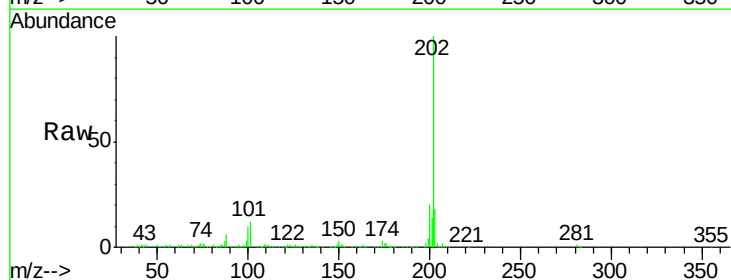


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



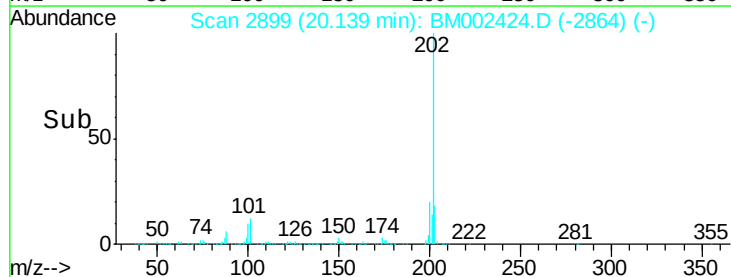
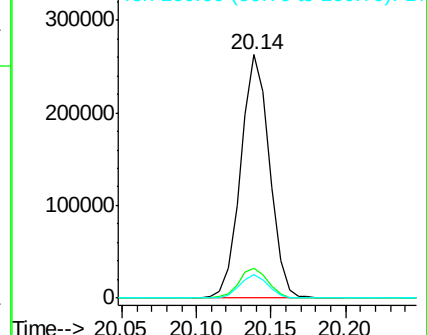


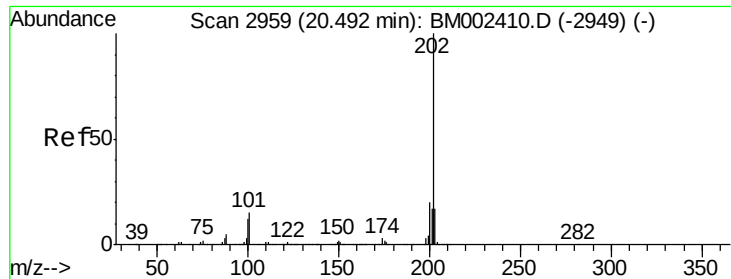

#19
Pvrene
Concen: 8.56 ng/ul
RT: 20.50 min Scan# 2960
Delta R.T. 0.01 min
Lab File: BM002424.D
Acq: 15 Aug 2015 14:45




Instrument :
BNA_M
ClientSampleId :
D9DA4DL


Tot Ion	Ratio	Lower	Upper
202	100		
101	14.1	12.0	18.0
100	11.9	9.7	14.5

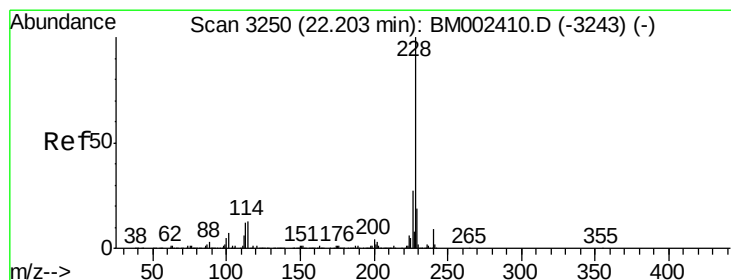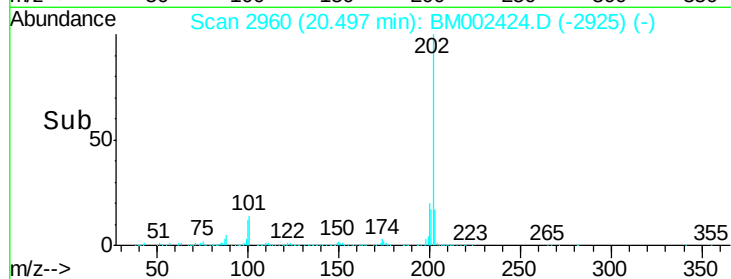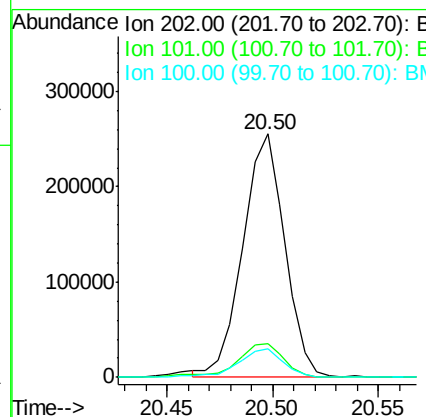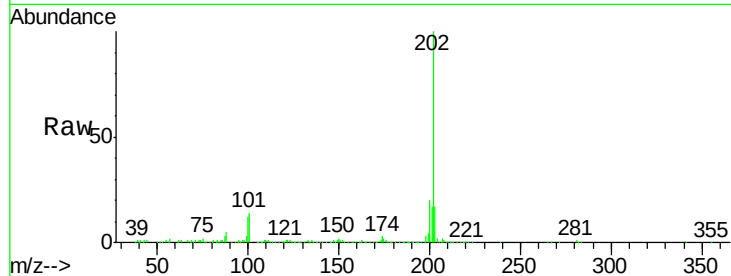

#20
Benzo(a)anthracene
Concen: 10.11 ng/ul
RT: 22.22 min Scan# 3252
Delta R.T. 0.01 min
Lab File: BM002424.D
Acq: 15 Aug 2015 14:45

Tgt Ion	Ratio	Lower	Upper
228	100		
229	20.1	15.8	23.6
226	26.7	21.1	31.7

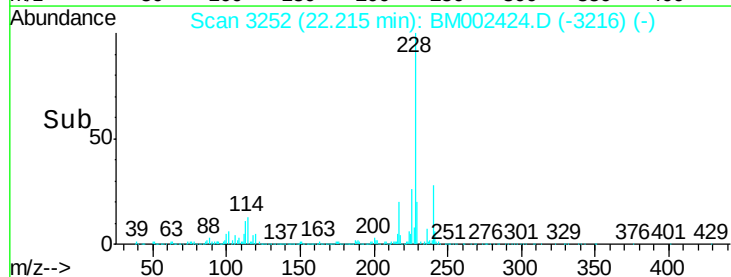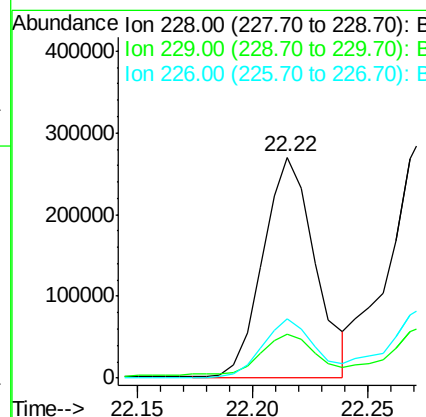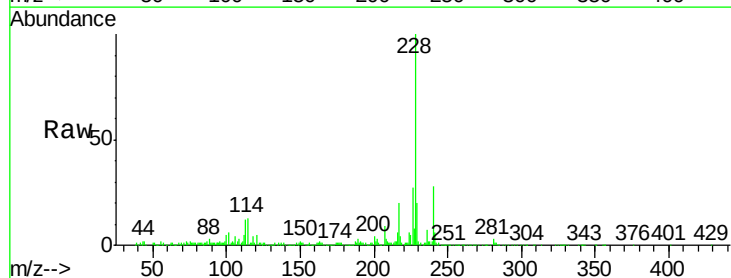

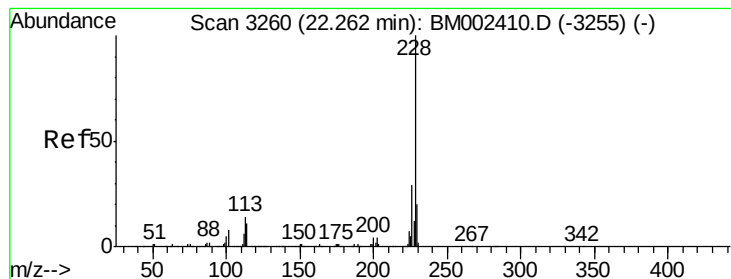

#21

Chrysene

Concen: 12.82 ng/ul

RT: 22.27 min Scan# 3262

Delta R.T. 0.01 min

Lab File: BM002424.D

Acq: 15 Aug 2015 14:45





Instrument :

BNA_M

ClientSampleId :

D9DA4DL

Tot Ion:228	Resp:	501319
Ion	Ratio	Lower Upper
228	100	
226	29.3	23.4 35.2
229	21.3	15.7 23.5

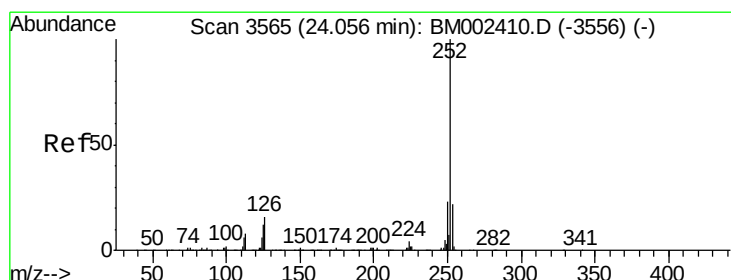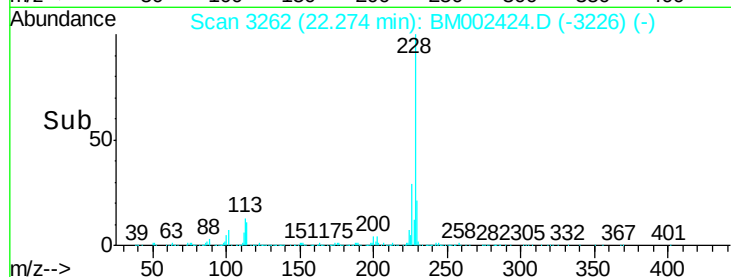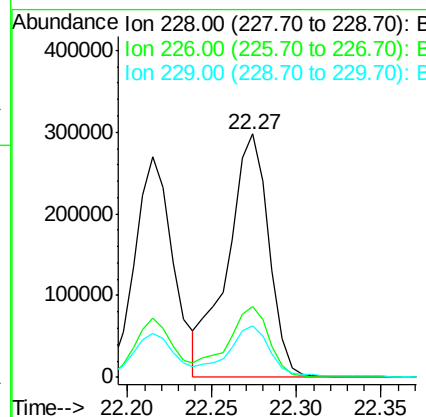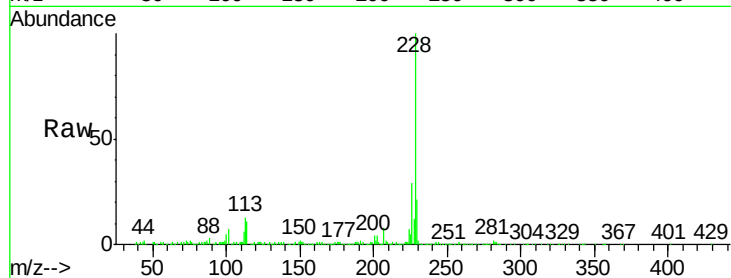

#23

Benzo(b)fluoranthene

Concen: 27.25 ng/ul




RT: 24.07 min Scan# 3568


Delta R.T. 0.02 min

Lab File: BM002424.D

Acq: 15 Aug 2015 14:45

Tgt Ion:252	Resp:	939680
Ion	Ratio	Lower Upper
252	100	
253	22.8	17.4 26.0
125	12.7	10.0 15.0


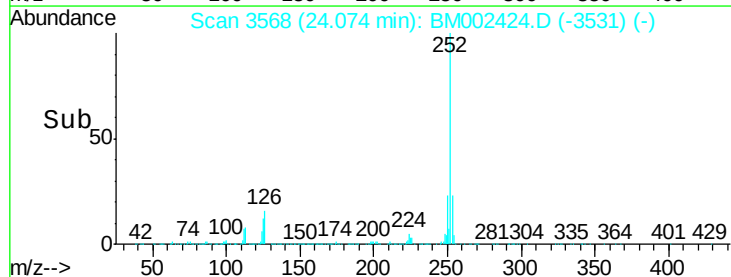
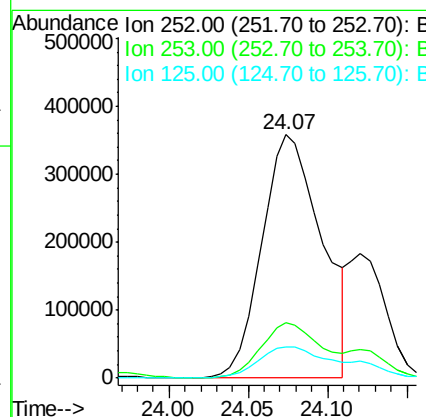
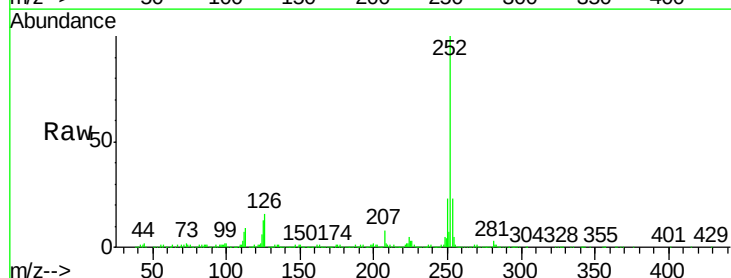


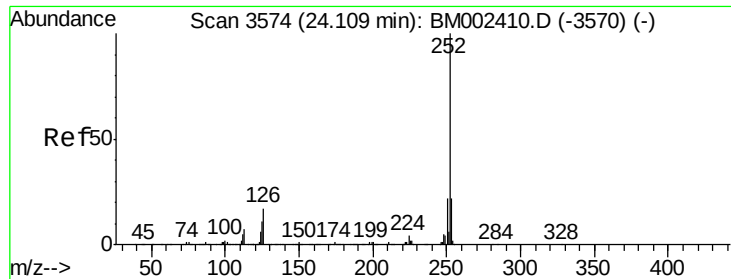

#24
Benzo(k)fluoranthene
Concen: 2.31 ng/ul
RT: 24.28 min Scan# 3603
Delta R.T. 0.17 min
Lab File: BM002424.D
Acq: 15 Aug 2015 14:45




Instrument :
BNA_M
ClientSampleId :
D9DA4DL


Tot Ion:252 Resp: 75419
Ion Ratio Lower Upper
252 100
253 26.3 17.8 26.6
125 17.3 9.8 14.8#

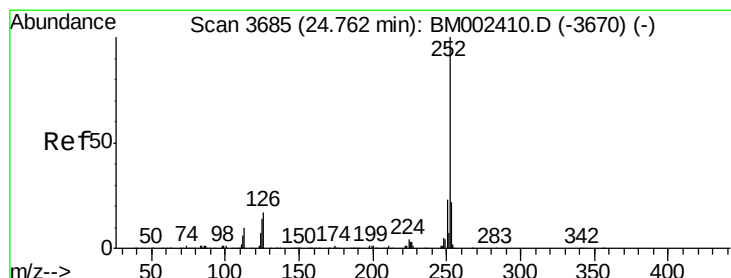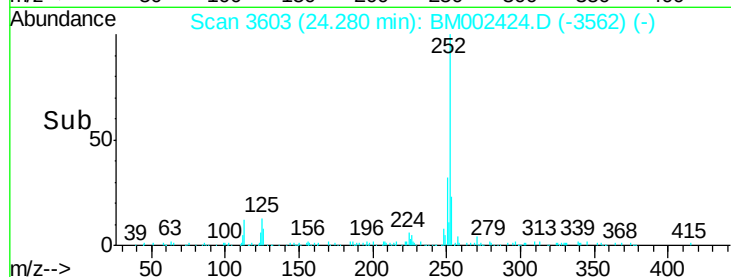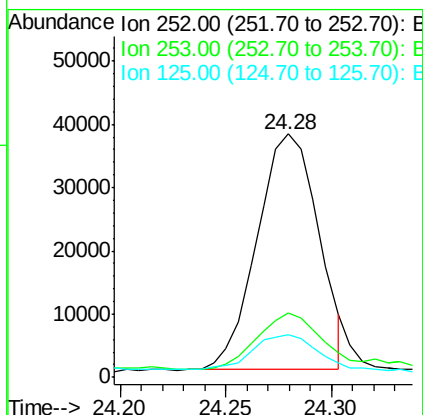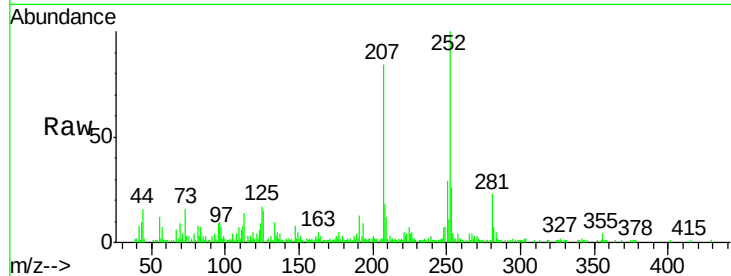

#26
Benzo(a)pyrene
Concen: 17.14 ng/ul
RT: 24.78 min Scan# 3688
Delta R.T. 0.02 min
Lab File: BM002424.D
Acq: 15 Aug 2015 14:45

Tgt Ion:252 Resp: 564542
Ion Ratio Lower Upper
252 100
253 21.6 17.6 26.4
125 13.8 10.7 16.1


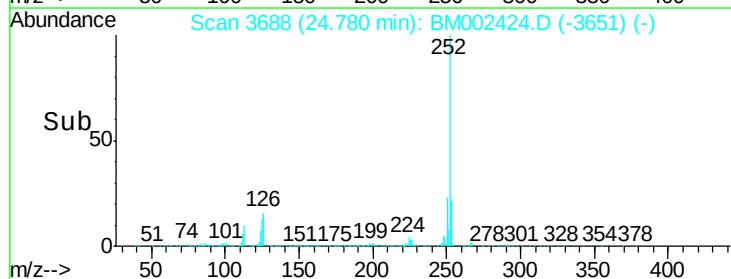
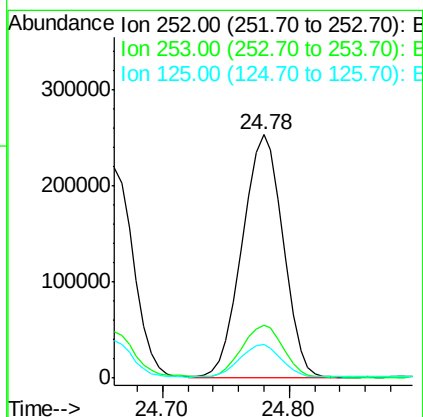
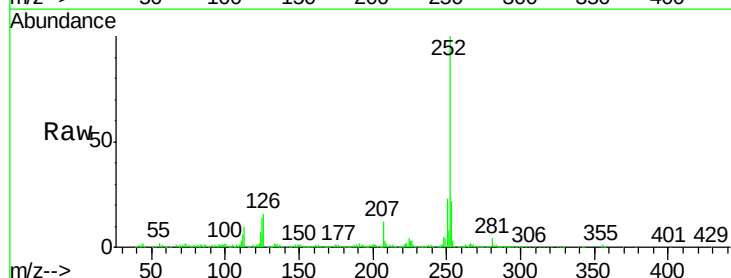


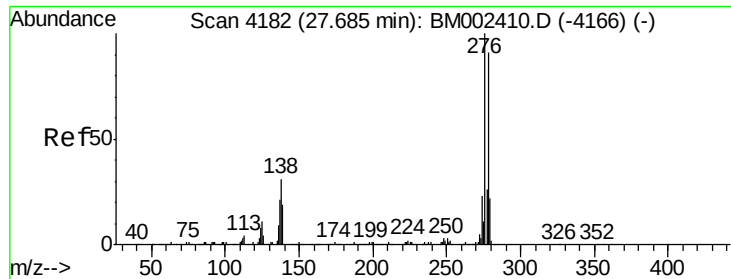

#27
 Indeno(1,2,3-cd)pyrene
 Concen: 12.85 ng/ul
 RT: 27.71 min Scan# 4186
 Delta R.T. 0.02 min
 Lab File: BM002424.D
 Acq: 15 Aug 2015 14:45




Instrument :
 BNA_M
 ClientSampleId :
 D9DA4DL


Tot Ion:276 Resp: 486596
 Ion Ratio Lower Upper
 276 100
 138 26.8 25.3 37.9
 277 23.9 20.2 30.2

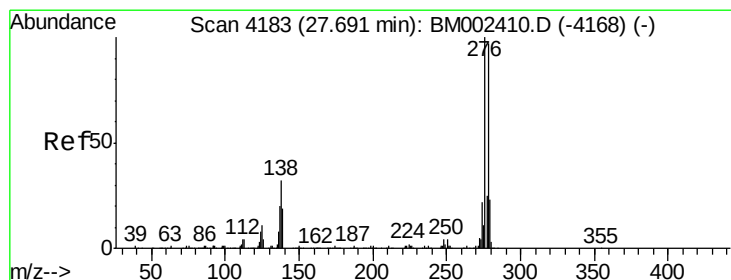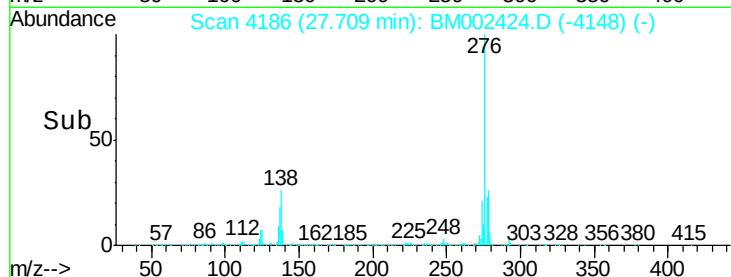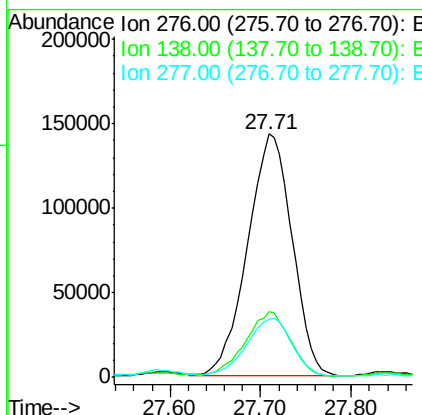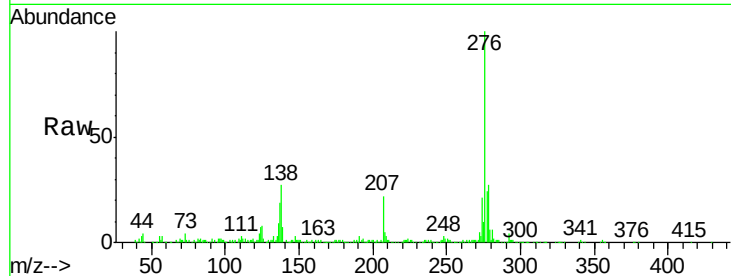

#28
 Dibenzo(a,h)anthracene
 Concen: 5.08 ng/ul
 RT: 27.71 min Scan# 4186
 Delta R.T. 0.02 min
 Lab File: BM002424.D
 Acq: 15 Aug 2015 14:45

Tgt Ion:278 Resp: 160842
 Ion Ratio Lower Upper
 278 100
 139 27.4 16.5 24.7#
 279 24.2 18.8 28.2

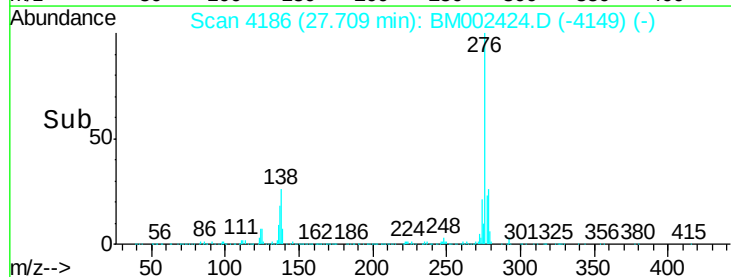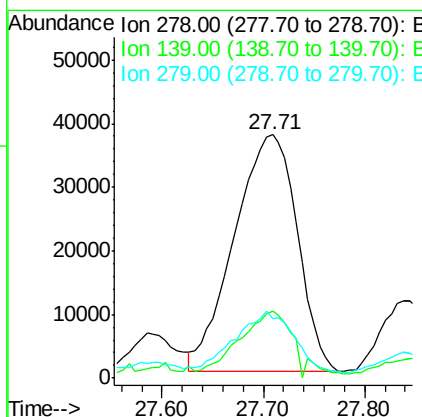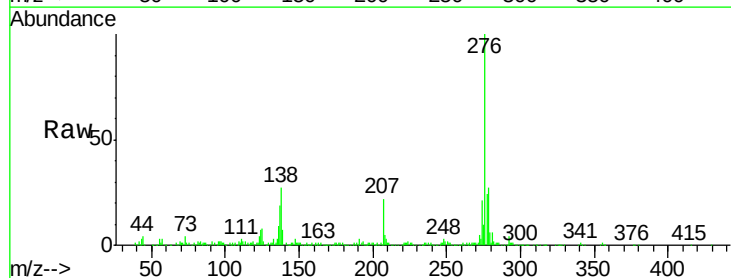

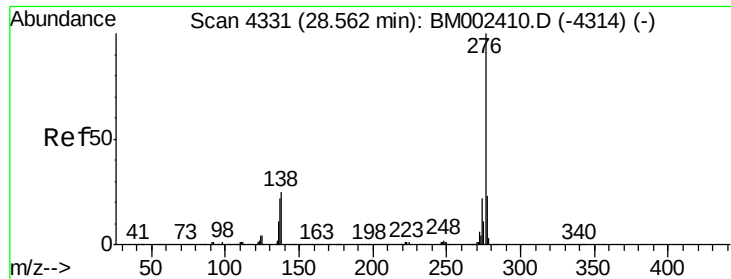

#29

Benzo(a,h,i)perylene

Concen: 14.03 ng/ul

RT: 28.60 min Scan# 4337

Delta R.T. 0.04 min

Lab File: BM002424.D

Acq: 15 Aug 2015 14:45

Instrument :

BNA_M

ClientSampleId :

D9DA4DL


Tot Ion: 276 Resp: 442480

Ion Ratio Lower Upper

276 100

138 26.9 21.0 31.6

277 24.1 19.2 28.8

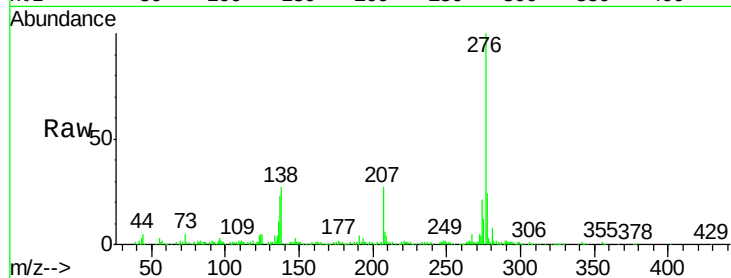

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

