

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081415\
 Data File : BM002406.D
 Acq On : 15 Aug 2015 03:42
 Operator : UM/IZ
 Sample : G3219-06 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9D99DL

Manual Integrations
 APPROVED

MMDadoda
 8/17/2015 2:44:21 PM

Quant Time: Aug 17 02:40:47 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 17 02:04:41 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	129740	20.00	ng/ul	0.00
2) Naphthalene-d8	11.73	136	644043	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.44	164	369649	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.15	188	793011	20.00	ng/ul	0.00
17) Chrysene-d12	22.22	240	829779	20.00	ng/ul	0.00
22) Perylene-d12	24.89	264	783776	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	15.15	160	154947	4.10	ng/ul	0.00
10) Fluorene-d10	16.42	176	109003	4.11	ng/ul	0.00
14) Anthracene-d10	18.24	188	159599	4.17	ng/ul	0.00
18) Pyrene-d10	20.46	212	163216	4.44	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.70	264	151953	3.69	ng/ul	0.00
Target Compounds						
13) Phenanthrene	18.19	178	256734	5.61	ng/ul	Qvalue 100
15) Anthracene	18.28	178	56349	1.21	ng/ul	100
16) Fluoranthene	20.13	202	402885	7.77	ng/ul	98
19) Pyrene	20.49	202	352086	7.24	ng/ul	98
20) Benzo(a)anthracene	22.20	228	281596	5.67	ng/ul	98
21) Chrysene	22.26	228	329856	7.11	ng/ul	98
23) Benzo(b)fluoranthene	24.06	252	671922	14.18	ng/ul	99
24) Benzo(k)fluoranthene	24.11	252	175627m	3.91	ng/ul	
26) Benzo(a)pyrene	24.76	252	366031	8.09	ng/ul	99
27) Indeno(1,2,3-cd)pyrene	27.68	276	291580	5.60	ng/ul	95
28) Dibenzo(a,h)anthracene	27.69	278	96968m	2.23	ng/ul	
29) Benzo(g,h,i)perylene	28.56	276	248952	5.75	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081415\
Data File : BM002406.D
Acq On : 15 Aug 2015 03:42
Operator : UM/IZ
Sample : G3219-06 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
D9D99DL

Manual Integrations
APPROVED

MMDadoda
8/17/2015 2:44:21 PM

Quant Time: Aug 17 02:40:47 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 17 02:04:41 2015
Response via : Initial Calibration

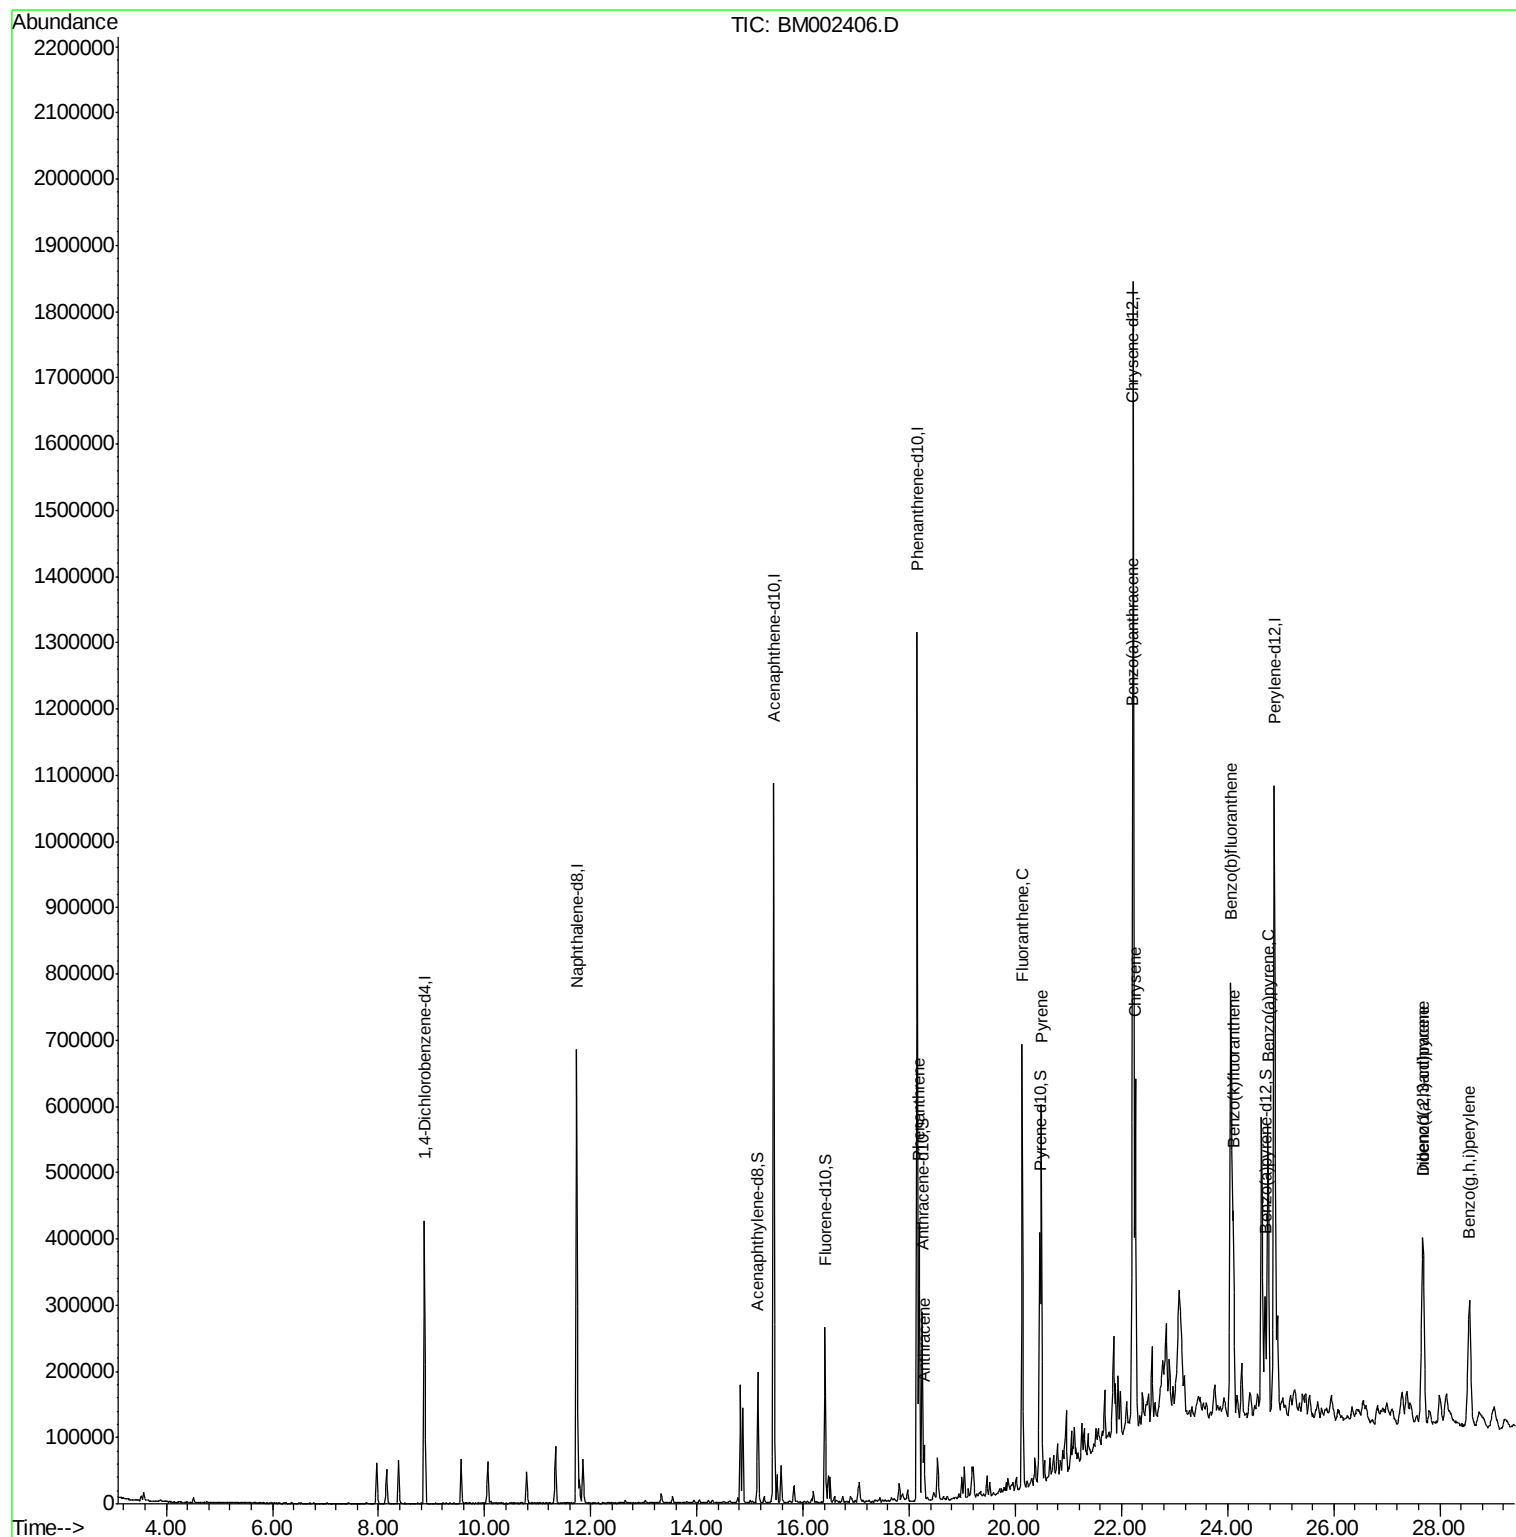

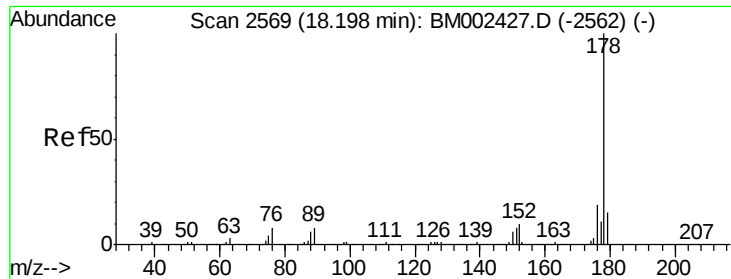





#13
Phenanthrene
Concen: 5.61 ng/ul
RT: 18.19 min Scan# 2568
Delta R.T. -0.00 min
Lab File: BM002406.D
Acq: 15 Aug 2015 03:42

Instrument :
BNA_M
ClientSampleId :
D9D99DL

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	256734		
179	15.5		12.4	18.6
176	18.6		15.1	22.7




Manual Integrations
APPROVED


MMDadoda
8/17/2015 2:44:21 PM

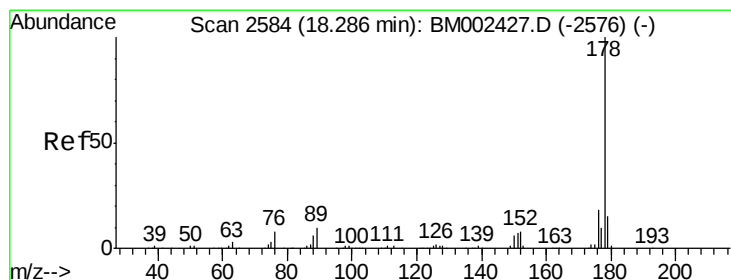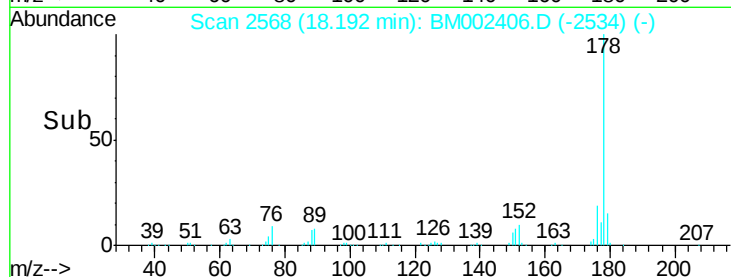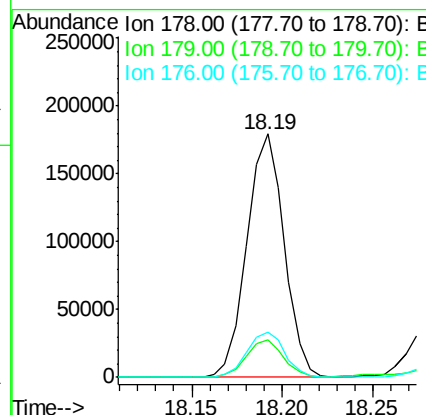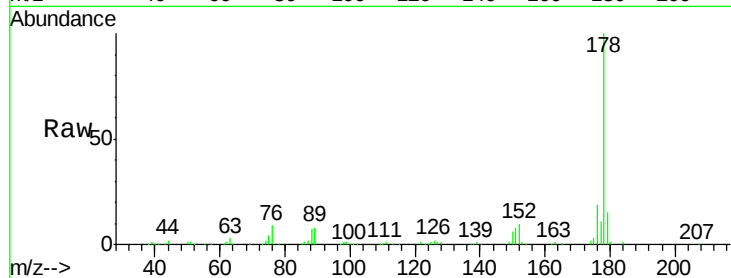

#15
Anthracene
Concen: 1.21 ng/ul
RT: 18.28 min Scan# 2583
Delta R.T. -0.00 min
Lab File: BM002406.D
Acq: 15 Aug 2015 03:42

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	56349		
179	15.7		12.6	18.8
176	17.8		14.5	21.7

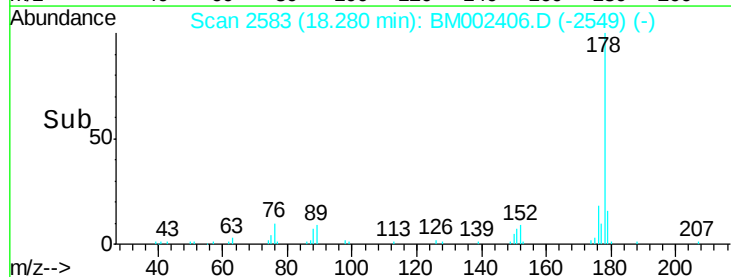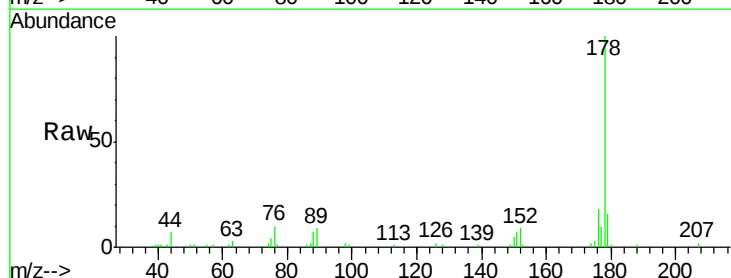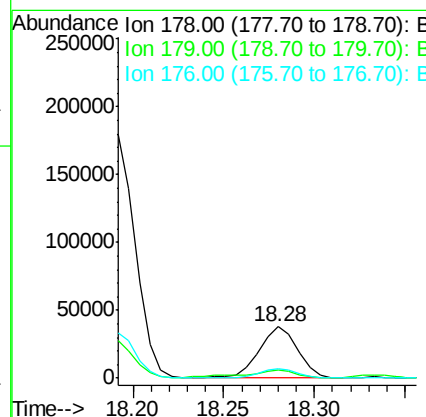

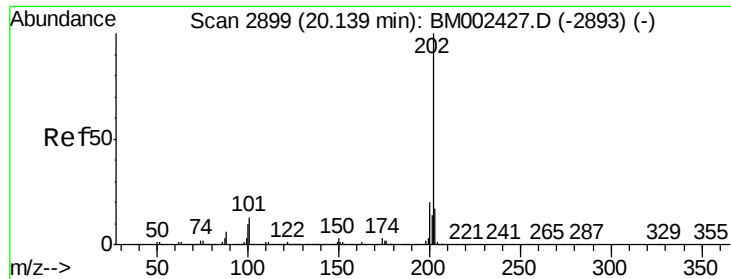





#16
Fluoranthene
 Concen: 7.77 ng/ul
 RT: 20.13 min Scan# 2898
 Delta R.T. -0.01 min
 Lab File: BM002406.D
 Acq: 15 Aug 2015 03:42

Instrument :
 BNA_M
 ClientSampleId :
 D9D99DL

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	13.2	9.7	14.5
100	9.7	7.4	11.2




Manual Integrations
 APPROVED


MMDadoda
 8/17/2015 2:44:21 PM

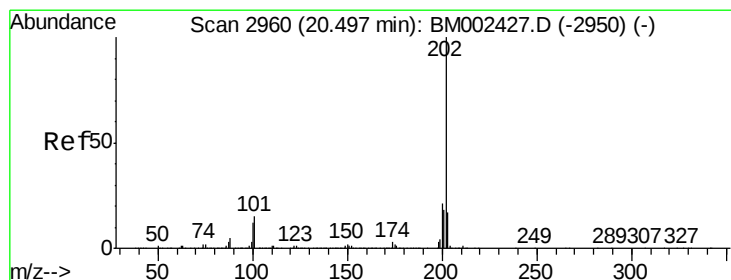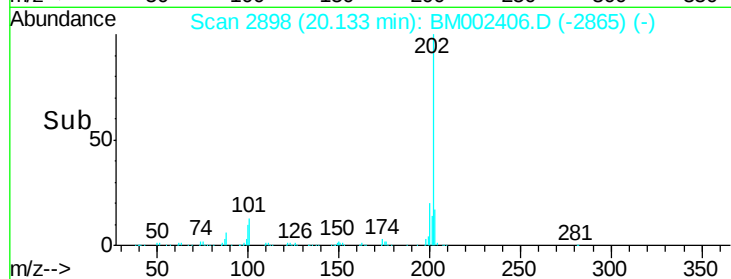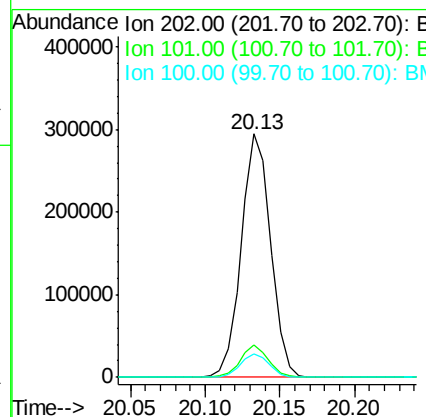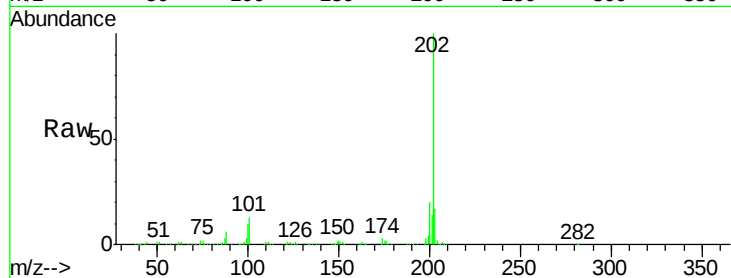

#19
Pyrene
 Concen: 7.24 ng/ul
 RT: 20.49 min Scan# 2959
 Delta R.T. -0.00 min
 Lab File: BM002406.D
 Acq: 15 Aug 2015 03:42

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	14.1	12.0	18.0
100	11.4	9.7	14.5

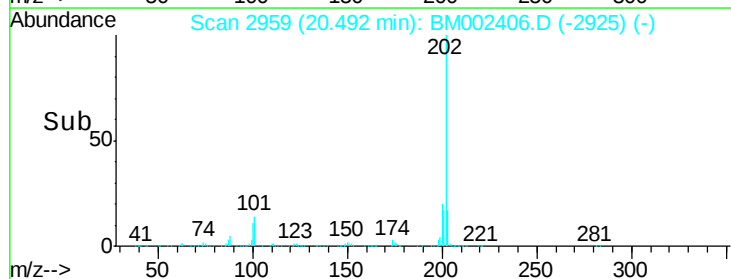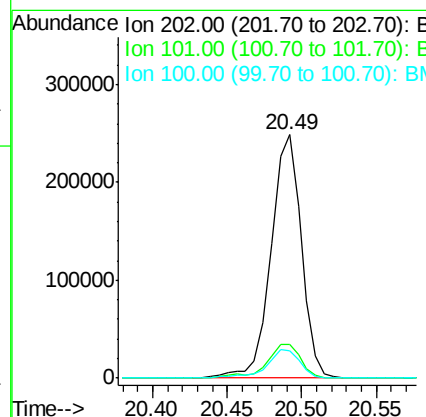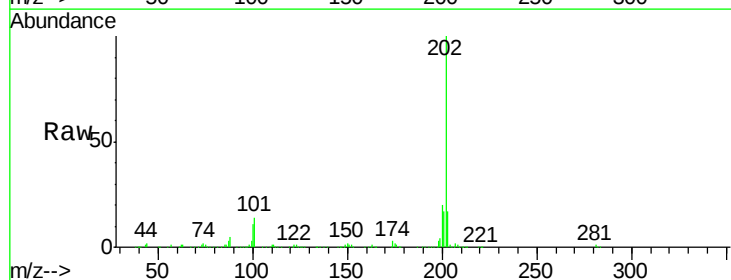

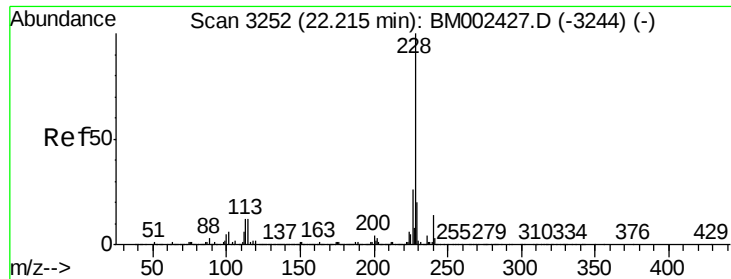





#20
Benzo(a)anthracene
Concen: 5.67 ng/ul
RT: 22.20 min Scan# 3250
Delta R.T. -0.01 min
Lab File: BM002406.D
Acq: 15 Aug 2015 03:42

Instrument :
BNA_M
ClientSampleId :
D9D99DL

Tgt Ion	Ratio	Resp Lower	Resp Upper
228	100		
229	20.9	15.8	23.6
226	27.3	21.1	31.7




Manual Integrations
APPROVED


MMDadoda
8/17/2015 2:44:21 PM

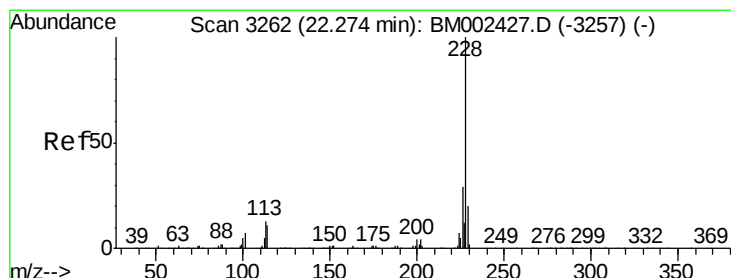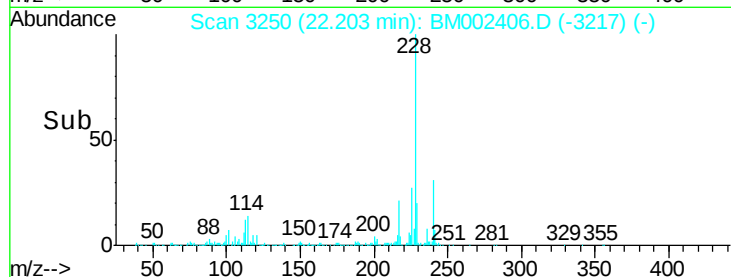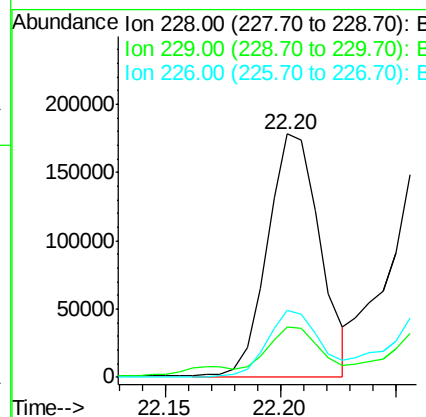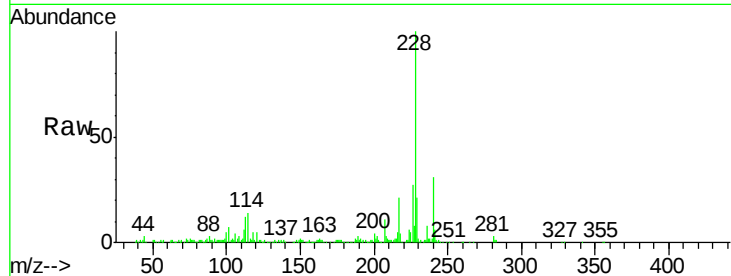

#21
Chrysene
Concen: 7.11 ng/ul
RT: 22.26 min Scan# 3260
Delta R.T. -0.01 min
Lab File: BM002406.D
Acq: 15 Aug 2015 03:42

Tgt Ion	Ratio	Resp Lower	Resp Upper
228	100		
226	29.1	23.4	35.2
229	21.6	15.7	23.5

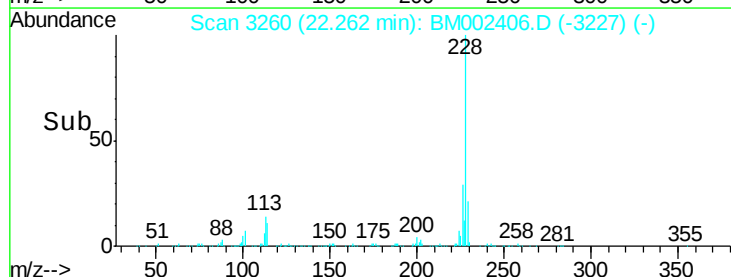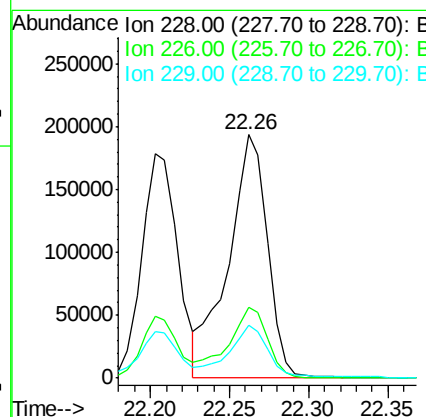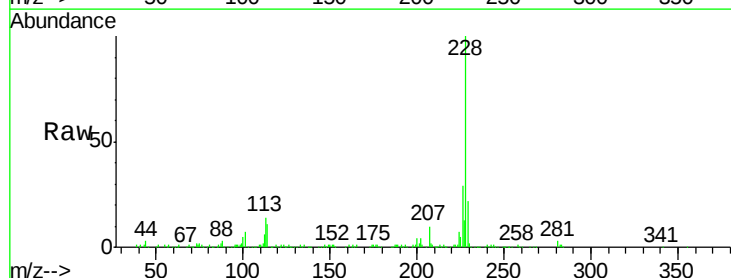

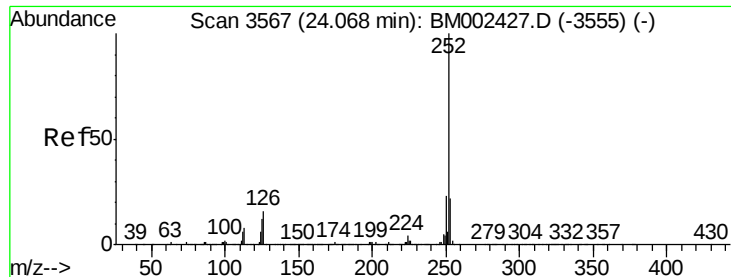

#23

Benzo(b)fluoranthene

Concen: 14.18 ng/ul

RT: 24.06 min Scan# 3566

Delta R.T. -0.00 min

Lab File: BM002406.D

Acq: 15 Aug 2015 03:42

Instrument :

BNA_M





ClientSampleId :

D9D99DL

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.2	17.4	26.0
125	12.5	10.0	15.0

Manual Integrations
APPROVED

MMDadoda
8/17/2015 2:44:21 PM

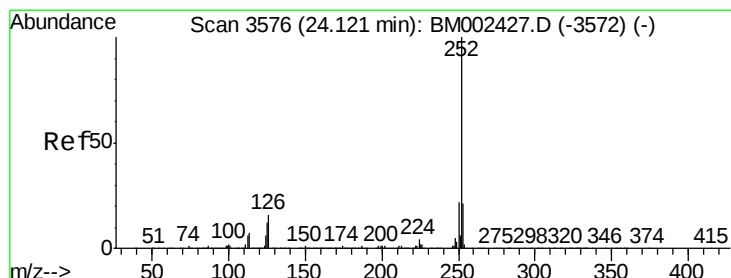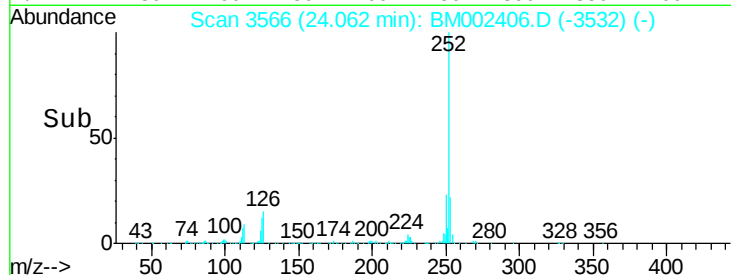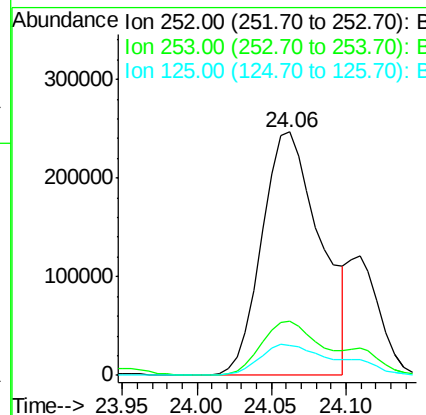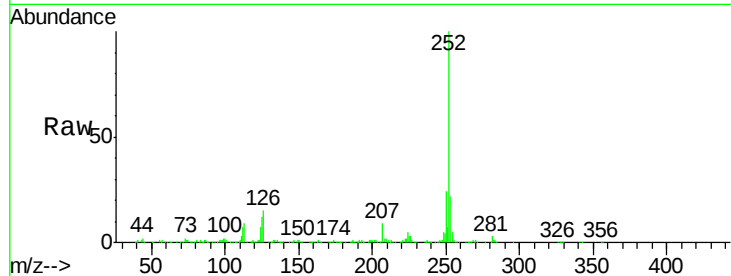

#24

Benzo(k)fluoranthene

Concen: 3.91 ng/ul m




RT: 24.11 min Scan# 3574


Delta R.T. -0.01 min

Lab File: BM002406.D

Acq: 15 Aug 2015 03:42

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.5	17.8	26.6
125	13.2	9.8	14.8

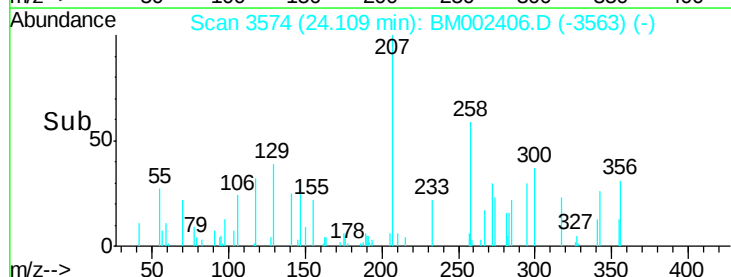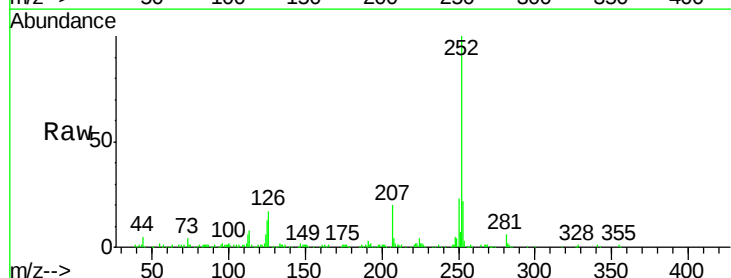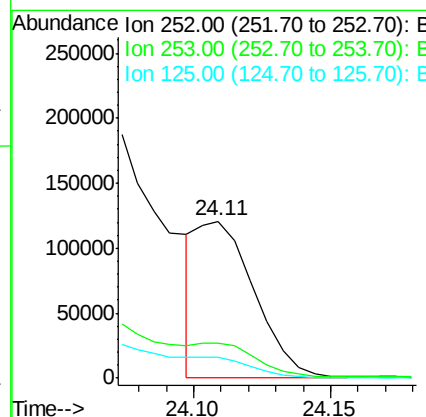

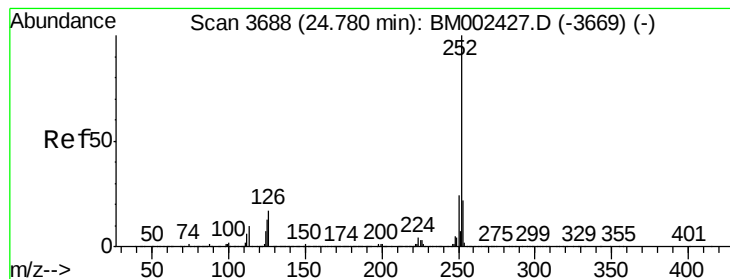

#26

Benzo(a)pyrene

Concen: 8.09 ng/ul

RT: 24.76 min Scan# 3685

Delta R.T. -0.01 min

Lab File: BM002406.D

Acq: 15 Aug 2015 03:42

Instrument :

BNA_M


ClientSampleId :

D9D99DL




Tgt	Ion	Ratio	Resp	Lower	Upper
252	100		366031		
253	22.1	17.6	26.4		
125	14.0	10.7	16.1		

Manual Integrations
APPROVED

MMDadoda
8/17/2015 2:44:21 PM

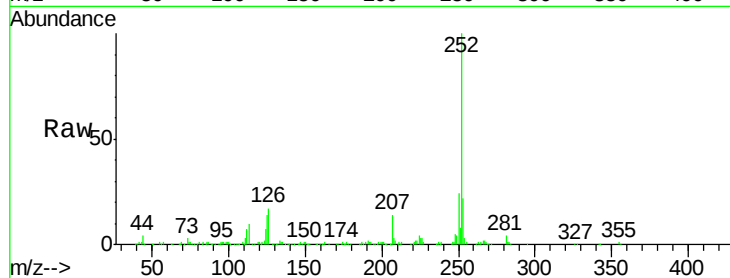

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

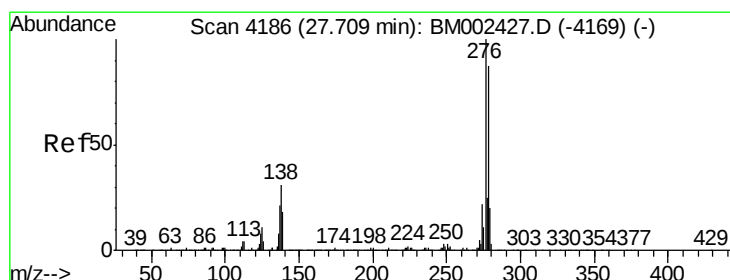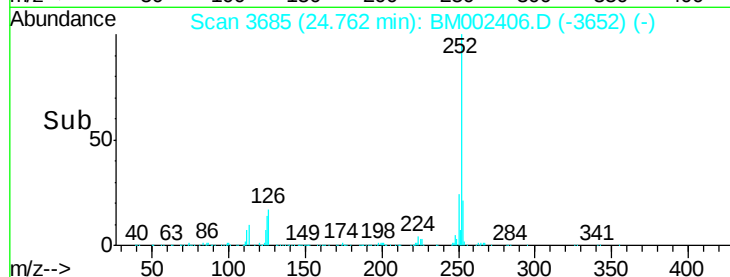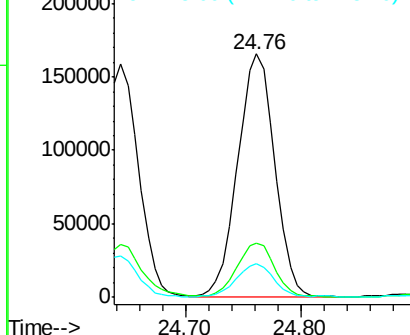

#27

Indeno(1,2,3-cd)pyrene

Concen: 5.60 ng/ul


RT: 27.68 min Scan# 4181

Delta R.T. -0.01 min



Lab File: BM002406.D


Acq: 15 Aug 2015 03:42

Tgt	Ion	Ratio	Resp	Lower	Upper
276	100		291580		
138	26.6	25.3	37.9		
277	24.6	20.2	30.2		

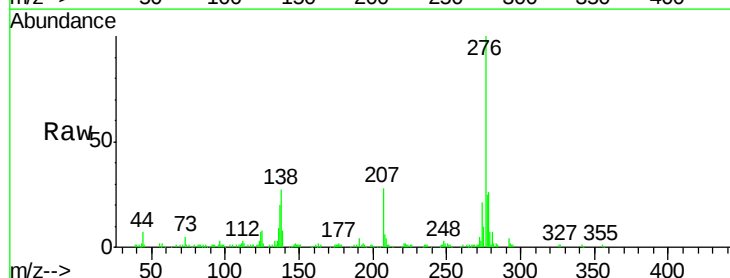

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

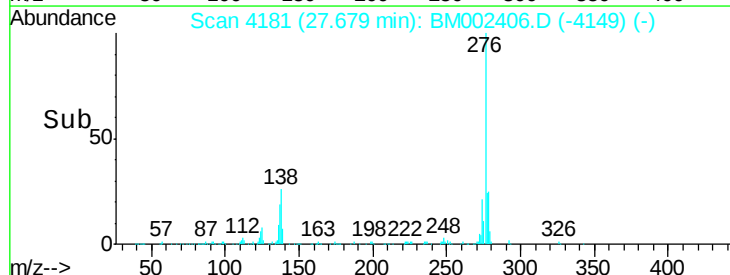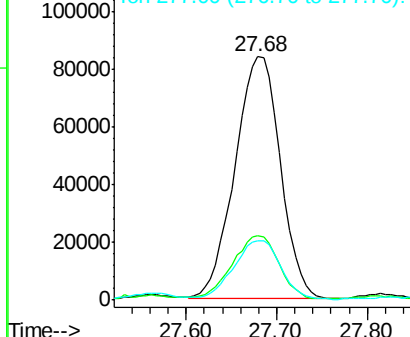

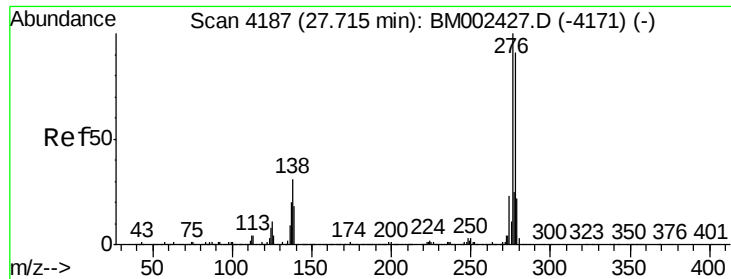





#28
Dibenzo(a,h)anthracene
Concen: 2.23 ng/ul m
RT: 27.69 min Scan# 4182
Delta R.T. -0.01 min
Lab File: BM002406.D
Acq: 15 Aug 2015 03:42

Instrument :
BNA_M
ClientSampleId :
D9D99DL

Tgt Ion	Ratio	Lower	Upper
278	100		
139	0.0	16.5	24.7#
279	25.8	18.8	28.2

Manual Integrations
APPROVED

MMDadoda
8/17/2015 2:44:21 PM

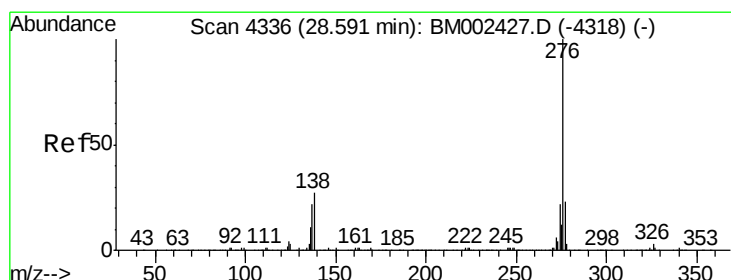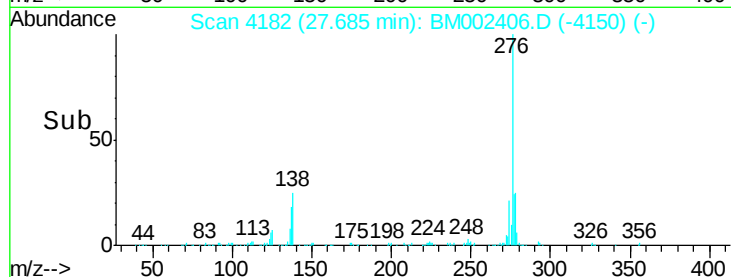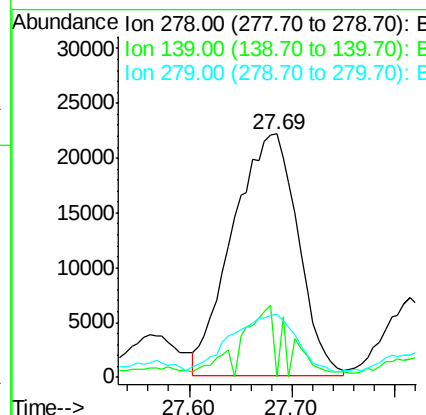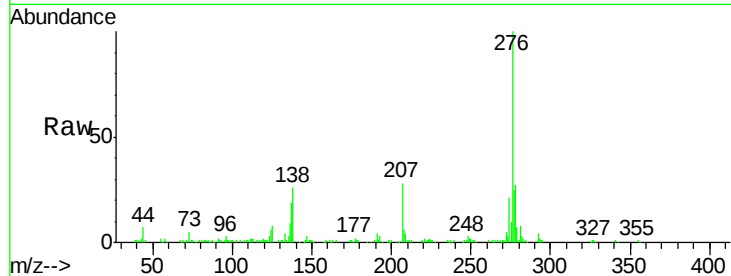

#29
Benzo(g,h,i)perylene
Concen: 5.75 ng/ul
RT: 28.56 min Scan# 4330
Delta R.T. -0.01 min
Lab File: BM002406.D
Acq: 15 Aug 2015 03:42

Tgt Ion	Ratio	Lower	Upper
276	100		
138	27.0	21.0	31.6
277	24.6	19.2	28.8

