

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081415\
 Data File : BM002413.D
 Acq On : 15 Aug 2015 07:56
 Operator : UM/IZ
 Sample : G3219-22
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9DB3

Manual Integrations
 APPROVED

MMDadoda
 8/17/2015 2:44:46 PM

Quant Time: Aug 17 03:06:36 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 17 02:54:04 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	170932	20.00	ng/ul	0.00
2) Naphthalene-d8	11.74	136	816074	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.44	164	434629	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.15	188	910248	20.00	ng/ul	0.00
17) Chrysene-d12	22.23	240	839576	20.00	ng/ul	0.00
22) Perylene-d12	24.89	264	647747	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	15.15	160	757496	17.05	ng/ul	0.00
10) Fluorene-d10	16.42	176	508409	16.29	ng/ul	0.00
14) Anthracene-d10	18.24	188	719884	16.40	ng/ul	0.00
18) Pyrene-d10	20.46	212	740338	19.89	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.71	264	552132	16.23	ng/ul	0.00
Target Compounds						
8) Acenaphthylene	15.18	152	80848	1.74	ng/ul	Qvalue 98
13) Phenanthrene	18.19	178	72285	1.38	ng/ul	99
15) Anthracene	18.28	178	72910	1.37	ng/ul	99
16) Fluoranthene	20.13	202	440162	7.40	ng/ul	98
19) Pyrene	20.49	202	427062	8.68	ng/ul	100
20) Benzo(a)anthracene	22.21	228	321715	6.41	ng/ul	98
21) Chrysene	22.27	228	300945	6.41	ng/ul	96
23) Benzo(b)fluoranthene	24.06	252	444596	11.35	ng/ul	96
24) Benzo(k)fluoranthene	24.11	252	144754m	3.90	ng/ul	
26) Benzo(a)pyrene	24.77	252	210412	5.63	ng/ul	98
27) Indeno(1,2,3-cd)pyrene	27.69	276	153446	3.57	ng/ul	94
28) Dibenzo(a,h)anthracene	27.68	278	41751	1.16	ng/ul#	87
29) Benzo(g,h,i)perylene	28.56	276	124223	3.47	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081415\
Data File : BM002413.D
Acq On : 15 Aug 2015 07:56
Operator : UM/IZ
Sample : G3219-22
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
D9DB3

Manual Integrations
APPROVED

MMDadoda
8/17/2015 2:44:46 PM

Quant Time: Aug 17 03:06:36 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 17 02:54:04 2015
Response via : Initial Calibration

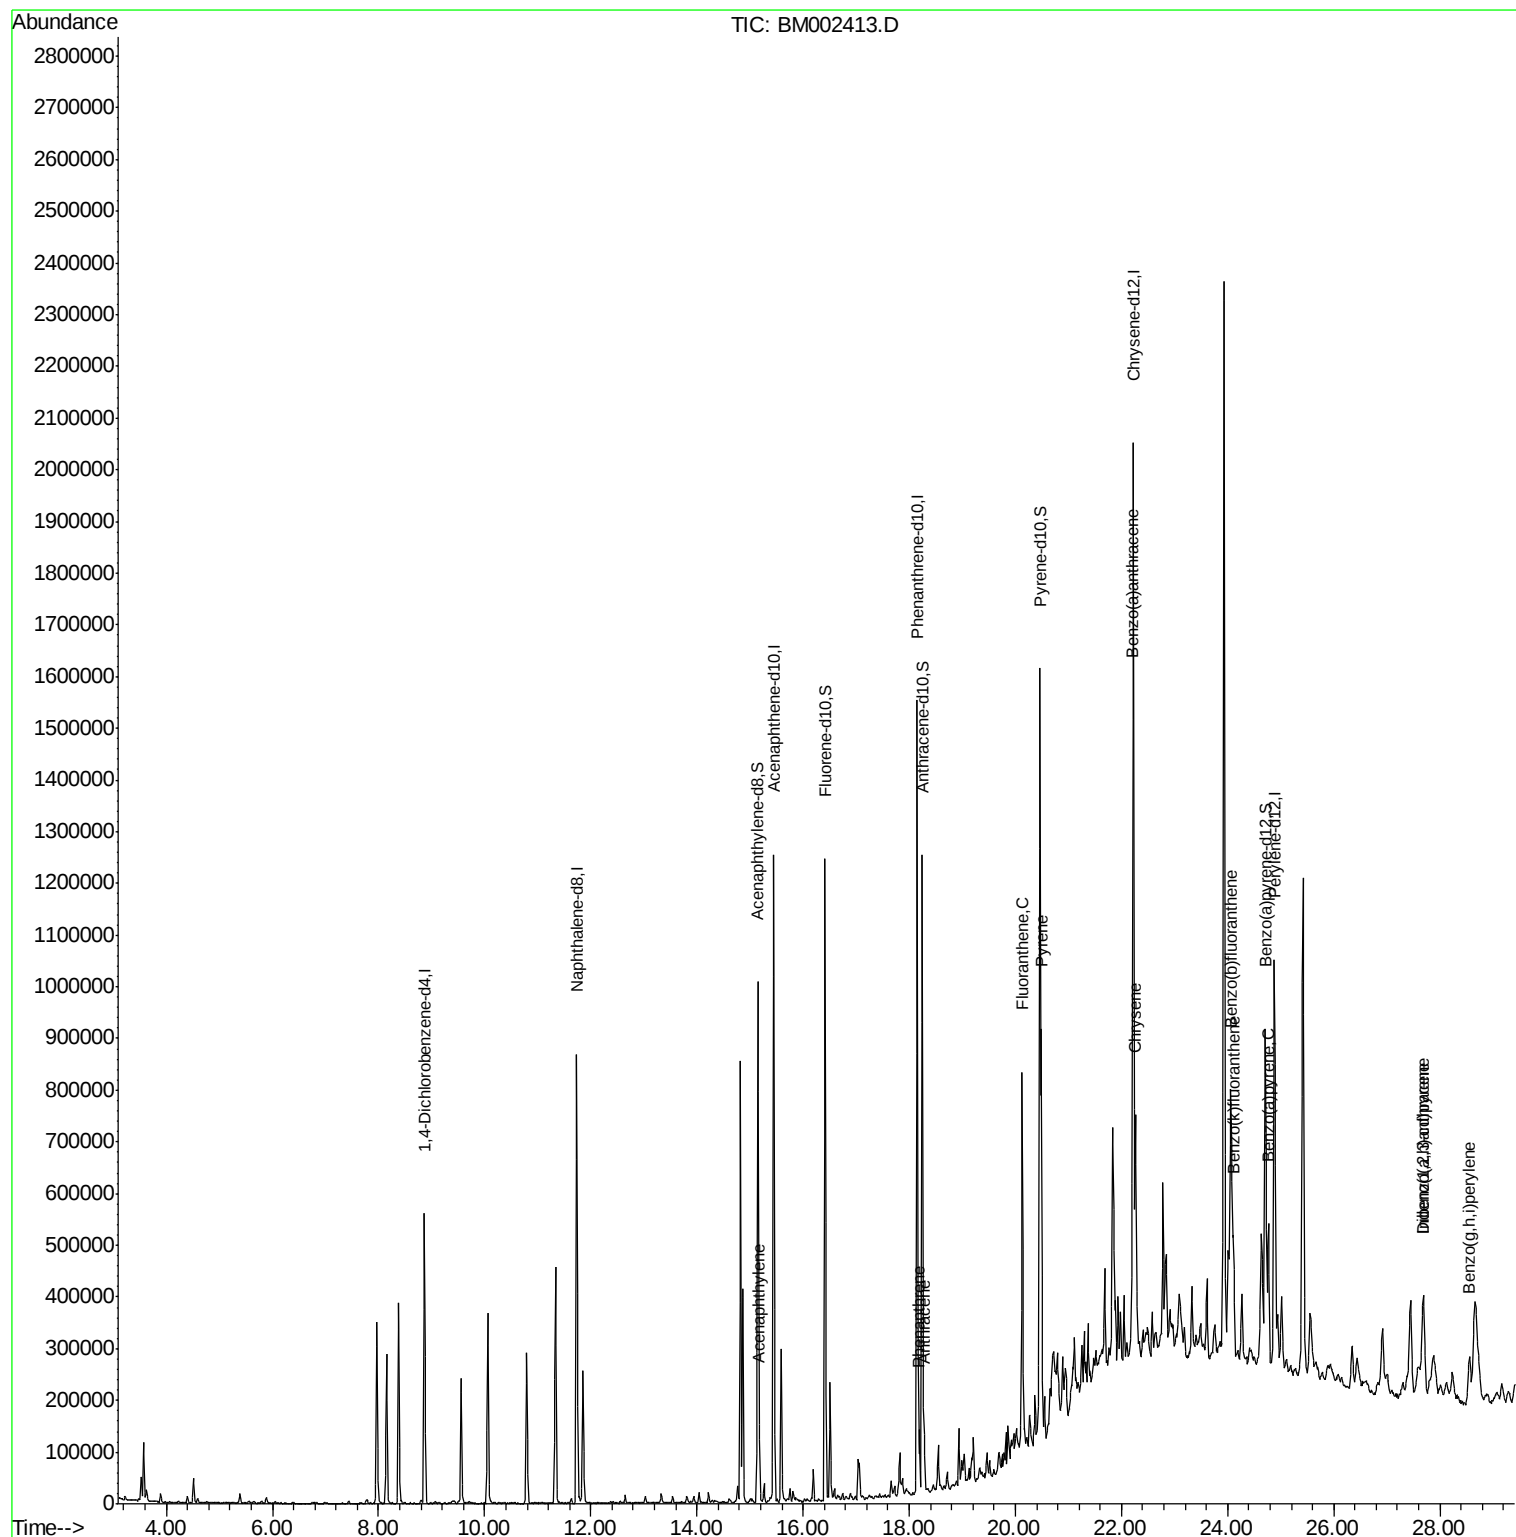

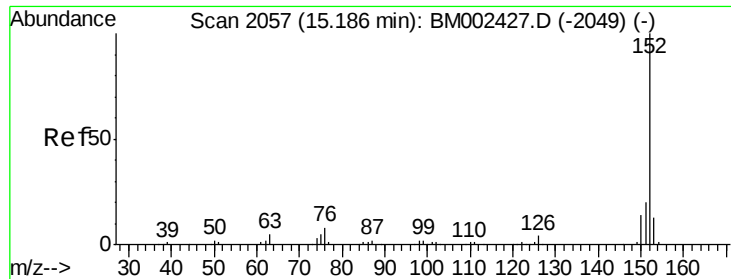

#8

Acenaphthylene

Concen: 1.74 ng/ul

RT: 15.18 min Scan# 2056

Delta R.T. -0.00 min

Lab File: BM002413.D


Acq: 15 Aug 2015 07:56

Instrument :

BNA_M

ClientSampleId :




D9DB3



Tgt Ion:	152	Resp:	80848
Ion Ratio	Lower	Upper	
152	100		
151	20.5	15.7	23.5
153	13.1	10.2	15.4

Manual Integrations
APPROVED

MMDadoda
8/17/2015 2:44:46 PM

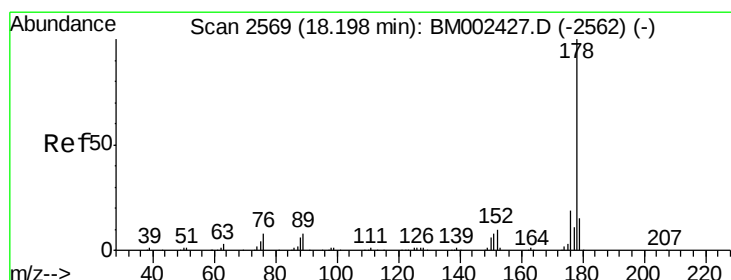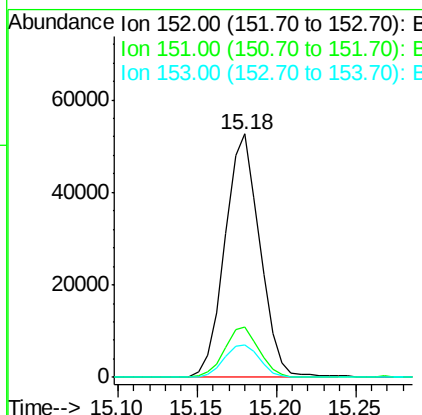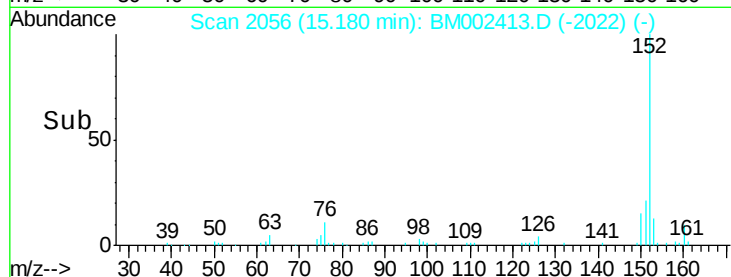

#13

Phenanthrene

Concen: 1.38 ng/ul




RT: 18.19 min Scan# 2568


Delta R.T. -0.00 min

Lab File: BM002413.D

Acq: 15 Aug 2015 07:56

Tgt Ion:	178	Resp:	72285
Ion Ratio	Lower	Upper	
178	100		
179	15.4	12.4	18.6
176	18.4	15.1	22.7

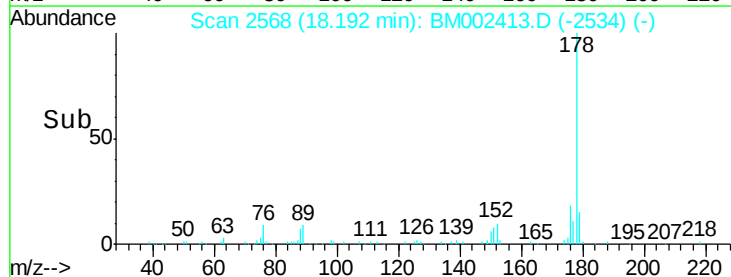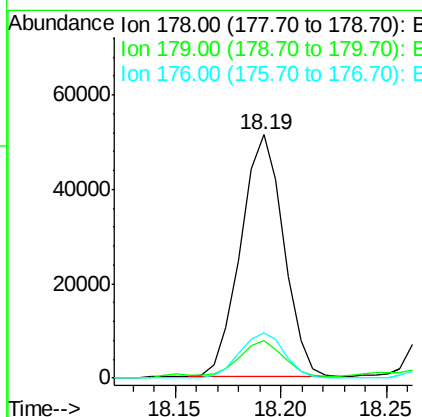

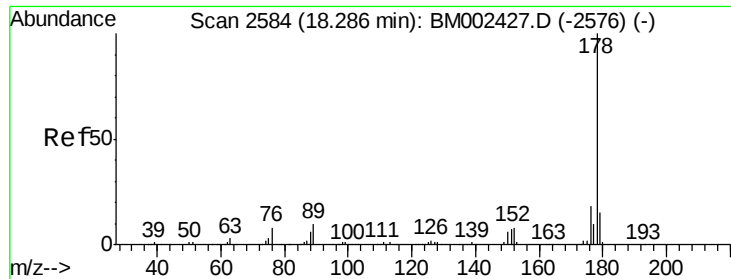

#15

Anthracene

Concen: 1.37 ng/ul

RT: 18.28 min Scan# 2583

Delta R.T. -0.00 min

Lab File: BM002413.D

Acq: 15 Aug 2015 07:56

Instrument :

BNA_M





ClientSampleId :

D9DB3

Tgt Ion:	178	Resp:	72910
Ion Ratio	Lower	Upper	
178	100		
179	15.2	12.6	18.8
176	18.3	14.5	21.7

Manual Integrations
APPROVED

MMDadoda
8/17/2015 2:44:46 PM

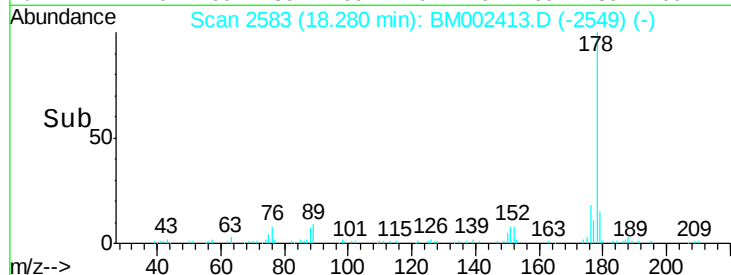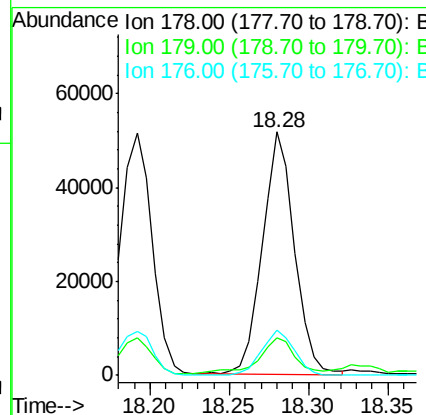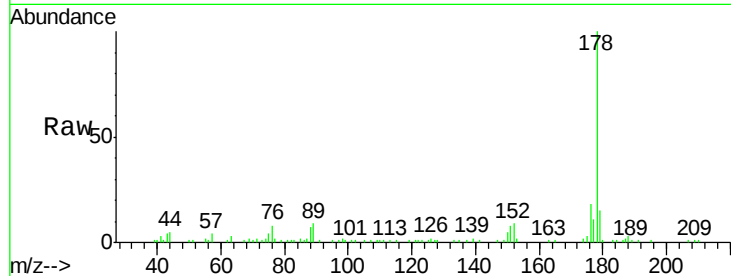

#16

Fluoranthene

Concen: 7.40 ng/ul




RT: 20.13 min Scan# 2898


Delta R.T. -0.00 min

Lab File: BM002413.D

Acq: 15 Aug 2015 07:56

Tgt Ion:	202	Resp:	440162
Ion Ratio	Lower	Upper	
202	100		
101	13.0	9.7	14.5
100	9.6	7.4	11.2

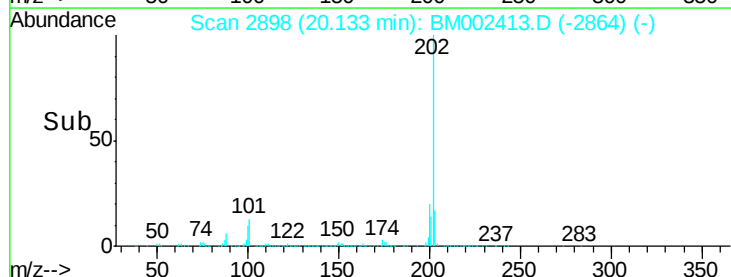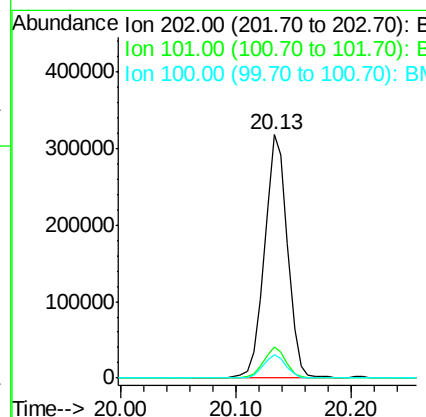

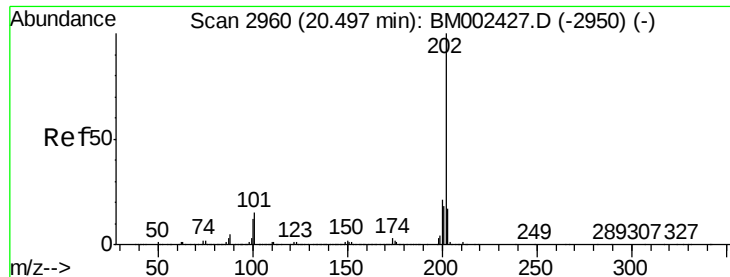





#19
 Pyrene
 Concen: 8.68 ng/ul
 RT: 20.49 min Scan# 2959
 Delta R.T. -0.00 min
 Lab File: BM002413.D
 Acq: 15 Aug 2015 07:56

Instrument :
 BNA_M
 ClientSampleId :
 D9DB3

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	427062		
101	14.8	12.0	18.0	
100	12.1	9.7	14.5	




Manual Integrations
 APPROVED


MMDadoda
 8/17/2015 2:44:46 PM

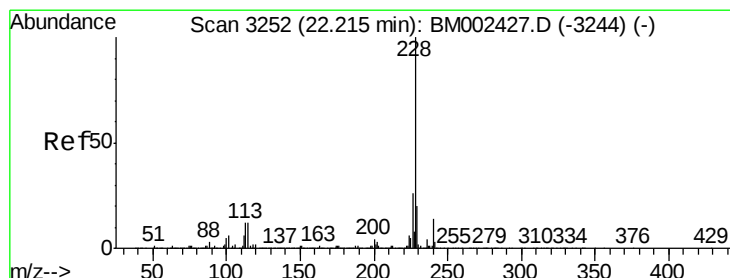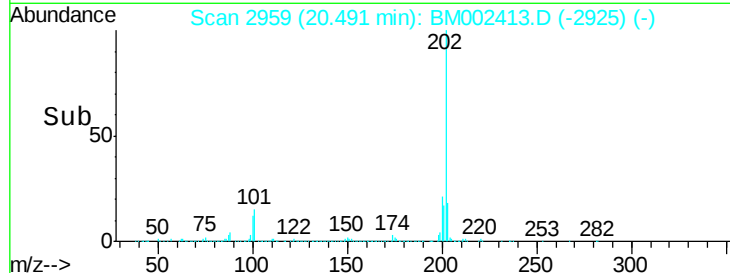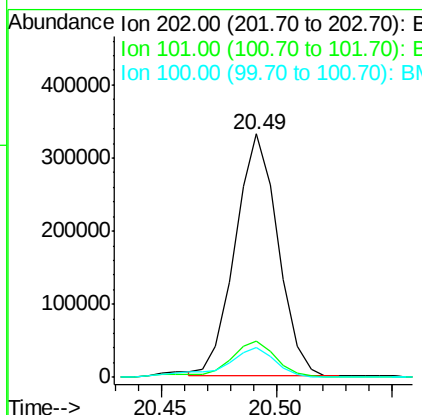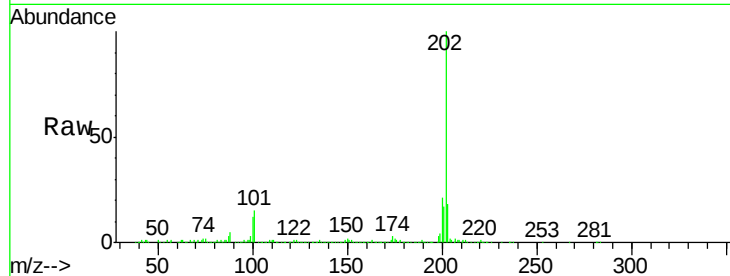

#20
 Benzo(a)anthracene
 Concen: 6.41 ng/ul
 RT: 22.21 min Scan# 3251
 Delta R.T. 0.01 min
 Lab File: BM002413.D
 Acq: 15 Aug 2015 07:56

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	321715		
229	21.4	15.8	23.6	
226	27.2	21.1	31.7	

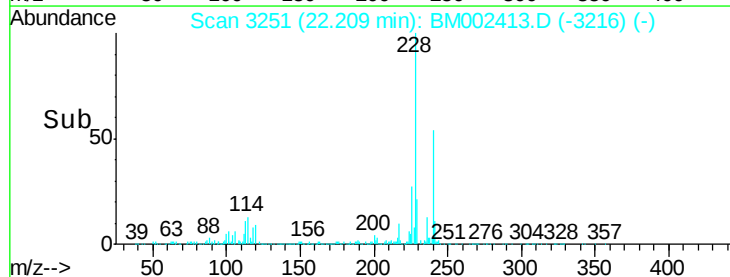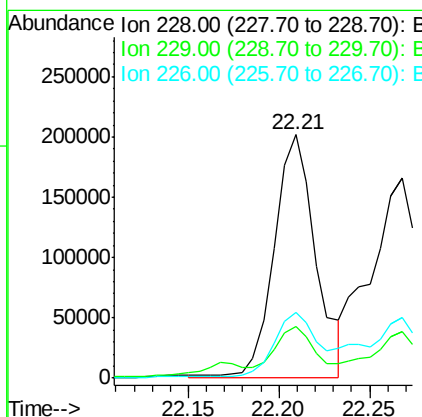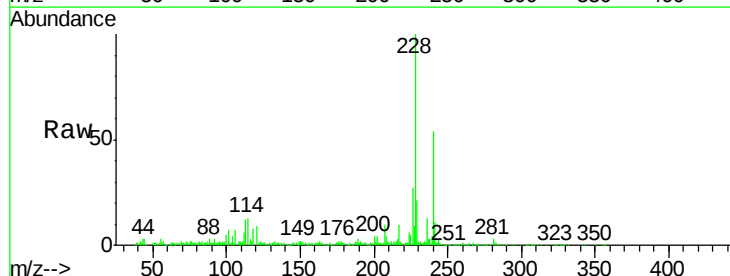

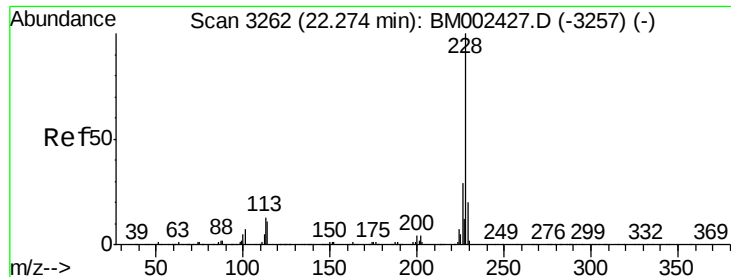





#21
Chrysene
Concen: 6.41 ng/ul
RT: 22.27 min Scan# 3261
Delta R.T. 0.01 min
Lab File: BM002413.D
Acq: 15 Aug 2015 07:56

Instrument :
BNA_M
ClientSampleId :
D9DB3

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.2	23.4	35.2
229	23.2	15.7	23.5




Manual Integrations
APPROVED


MMDadoda
8/17/2015 2:44:46 PM

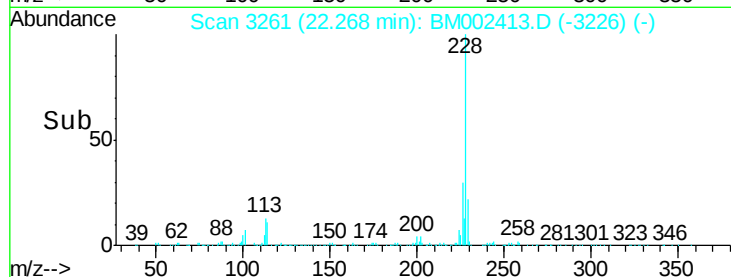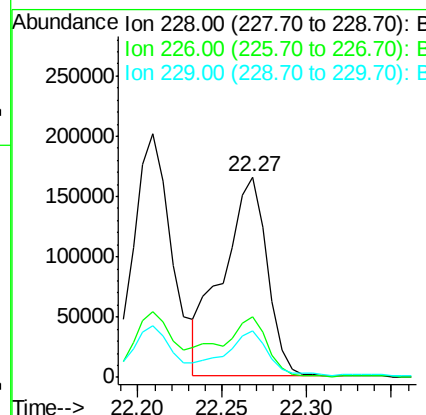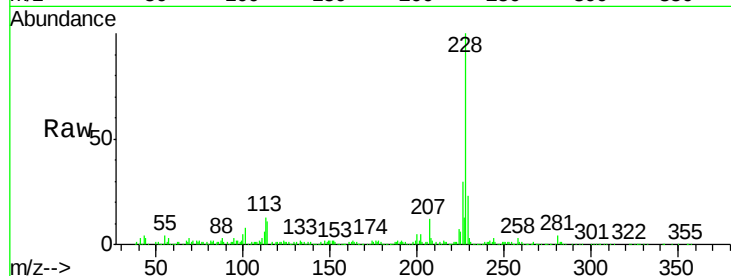

#23
Benzo(b)fluoranthene
Concen: 11.35 ng/ul
RT: 24.06 min Scan# 3566
Delta R.T. 0.01 min
Lab File: BM002413.D
Acq: 15 Aug 2015 07:56

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	17.4	26.0
125	14.4	10.0	15.0

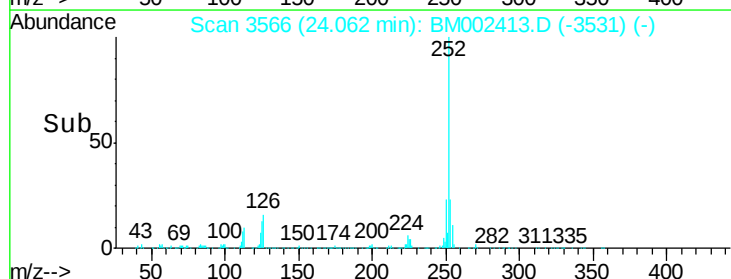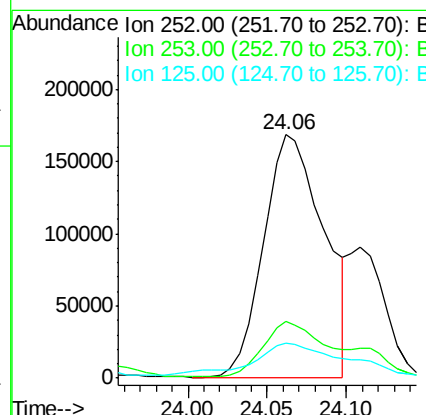

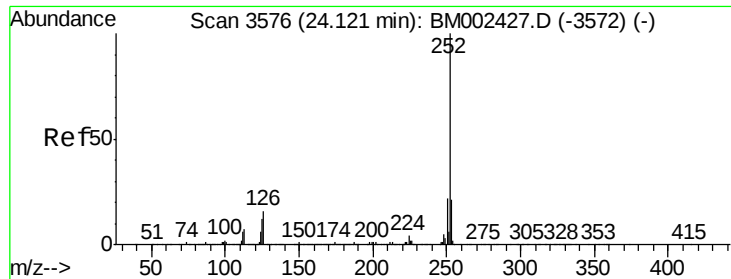

#24

Benzo(k)fluoranthene

Concen: 3.90 ng/ul m

RT: 24.11 min Scan# 3574

Delta R.T. -0.00 min

Lab File: BM002413.D

Acq: 15 Aug 2015 07:56

Instrument :

BNA_M





ClientSampleId :

D9DB3

Tgt Ion:	252	Resp:	144754
Ion Ratio	Lower	Upper	
252	100		
253	23.1	17.8	26.6
125	14.1	9.8	14.8

Manual Integrations
APPROVED

MMDadoda
8/17/2015 2:44:46 PM

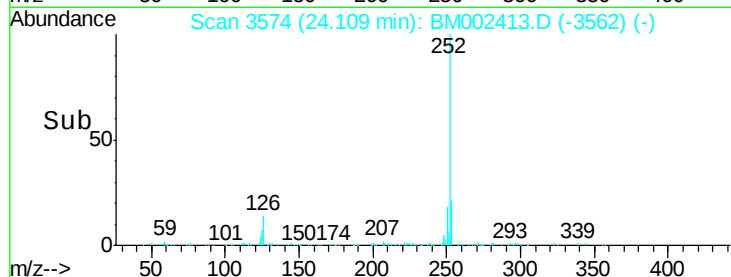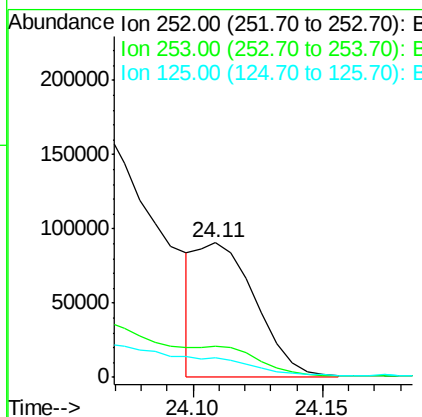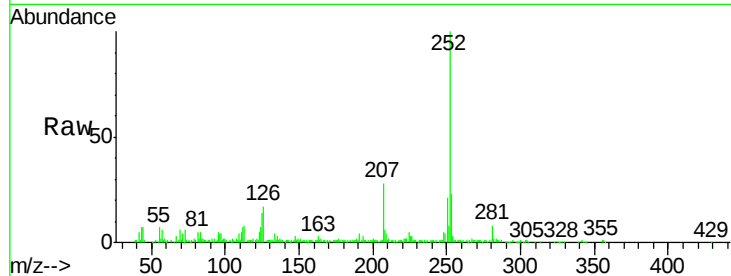

#26

Benzo(a)pyrene

Concen: 5.63 ng/ul




RT: 24.77 min Scan# 3686


Delta R.T. 0.01 min

Lab File: BM002413.D

Acq: 15 Aug 2015 07:56

Tgt Ion:	252	Resp:	210412
Ion Ratio	Lower	Upper	
252	100		
253	22.9	17.6	26.4
125	14.3	10.7	16.1

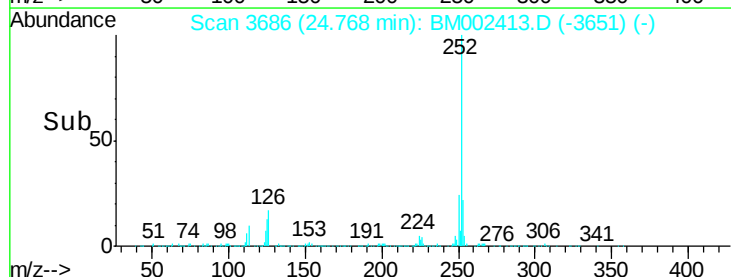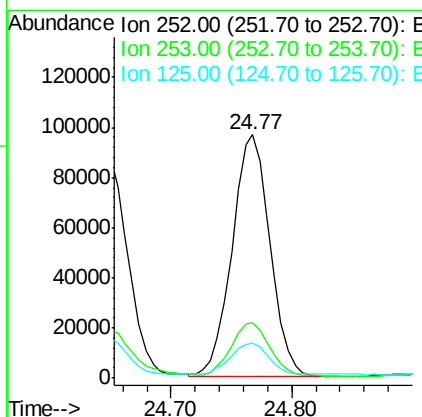

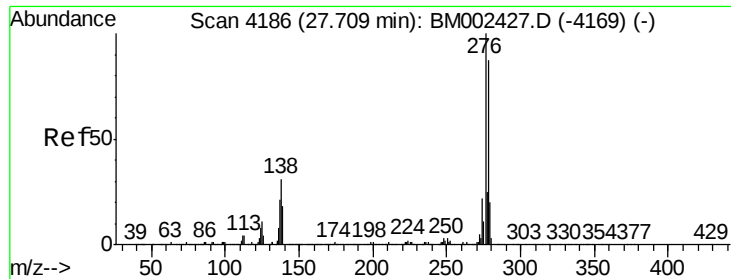





#27
 Indeno(1,2,3-cd)pyrene
 Concen: 3.57 ng/ul
 RT: 27.69 min Scan# 4182
 Delta R.T. -0.00 min
 Lab File: BM002413.D
 Acq: 15 Aug 2015 07:56

Instrument :
 BNA_M
 ClientSampleId :
 D9DB3

Tgt Ion	Ratio	Lower	Upper
276	100		
138	25.7	25.3	37.9
277	24.9	20.2	30.2




Manual Integrations
 APPROVED


MMDadoda
 8/17/2015 2:44:46 PM

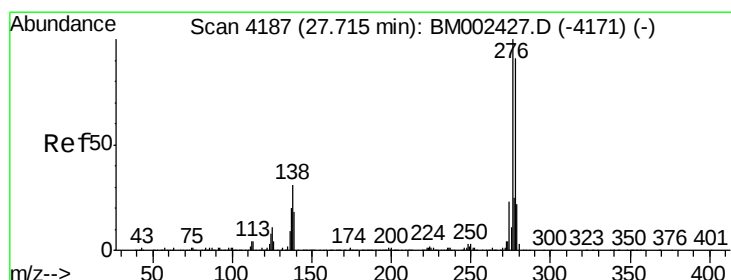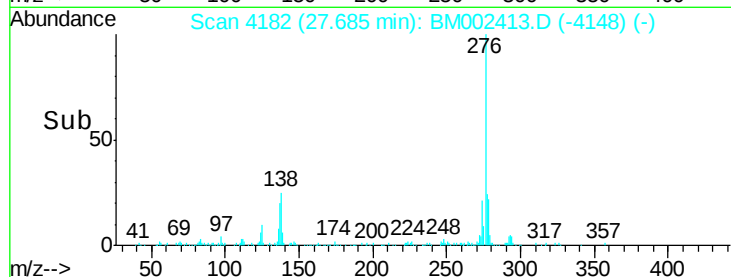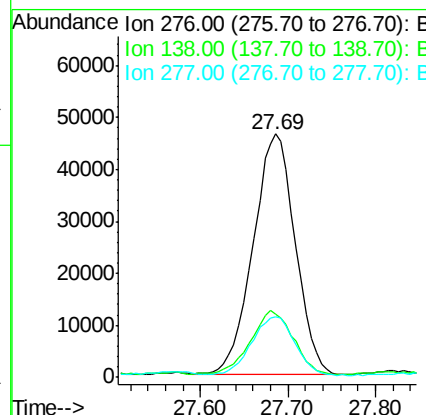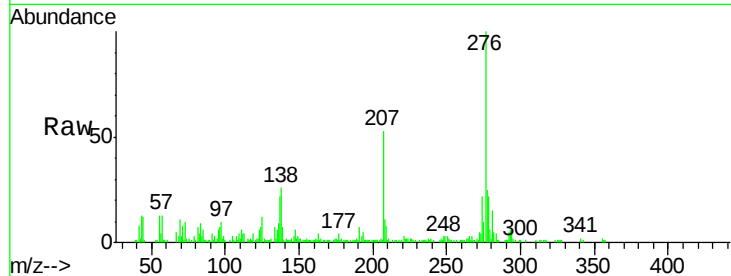

#28
 Dibenzo(a,h)anthracene
 Concen: 1.16 ng/ul
 RT: 27.68 min Scan# 4181
 Delta R.T. -0.01 min
 Lab File: BM002413.D
 Acq: 15 Aug 2015 07:56

Tgt Ion	Ratio	Lower	Upper
278	100		
139	29.5	16.5	24.7#
279	27.6	18.8	28.2

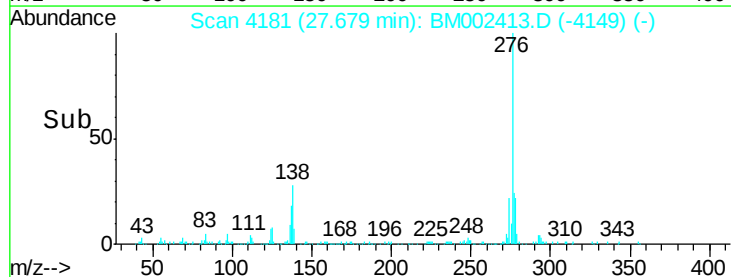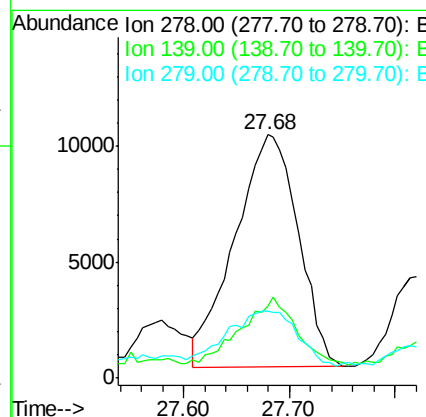

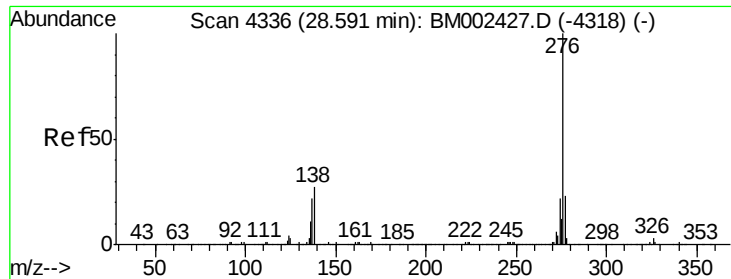

#29

Benzo(g,h,i)perylene

Concen: 3.47 ng/ul

RT: 28.56 min Scan# 4330

Delta R.T. -0.01 min

Lab File: BM002413.D


Acq: 15 Aug 2015 07:56

Instrument :

BNA_M

ClientSampleId :

D9DB3



Tgt Ion	Ratio	Resp	Lower	Upper
276	100	124223		
138	29.5		21.0	31.6
277	25.2		19.2	28.8

Manual Integrations
APPROVED

MMDadoda
8/17/2015 2:44:46 PM

