

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081415\
 Data File : BM002422.D
 Acq On : 15 Aug 2015 13:32
 Operator : UM/IZ
 Sample : G3219-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9DA2

Quant Time: Aug 17 02:57:18 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 17 02:54:04 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	199402	20.00	ng/ul	0.00
2) Naphthalene-d8	11.74	136	922574	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.45	164	488311	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.16	188	984172	20.00	ng/ul	0.00
17) Chrysene-d12	22.23	240	712624	20.00	ng/ul	0.00
22) Perylene-d12	24.89	264	588101	20.00	ng/ul	0.01
System Monitoring Compounds						
7) Acenaphthylene-d8	15.16	160	1488782	29.82	ng/ul	0.00
10) Fluorene-d10	16.42	176	986872	28.14	ng/ul	0.00
14) Anthracene-d10	18.26	188	1375819	28.98	ng/ul	0.01
18) Pyrene-d10	20.47	212	1268828	40.17	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.72	264	903500	29.25	ng/ul	0.01
Target Compounds						
23) Benzo(b)fluoranthene	24.07	252	54053	1.52	ng/ul#	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM081415\
Data File : BM002422.D
Acq On : 15 Aug 2015 13:32
Operator : UM/IZ
Sample : G3219-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9DA2

Quant Time: Aug 17 02:57:18 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM081415MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 17 02:54:04 2015
Response via : Initial Calibration

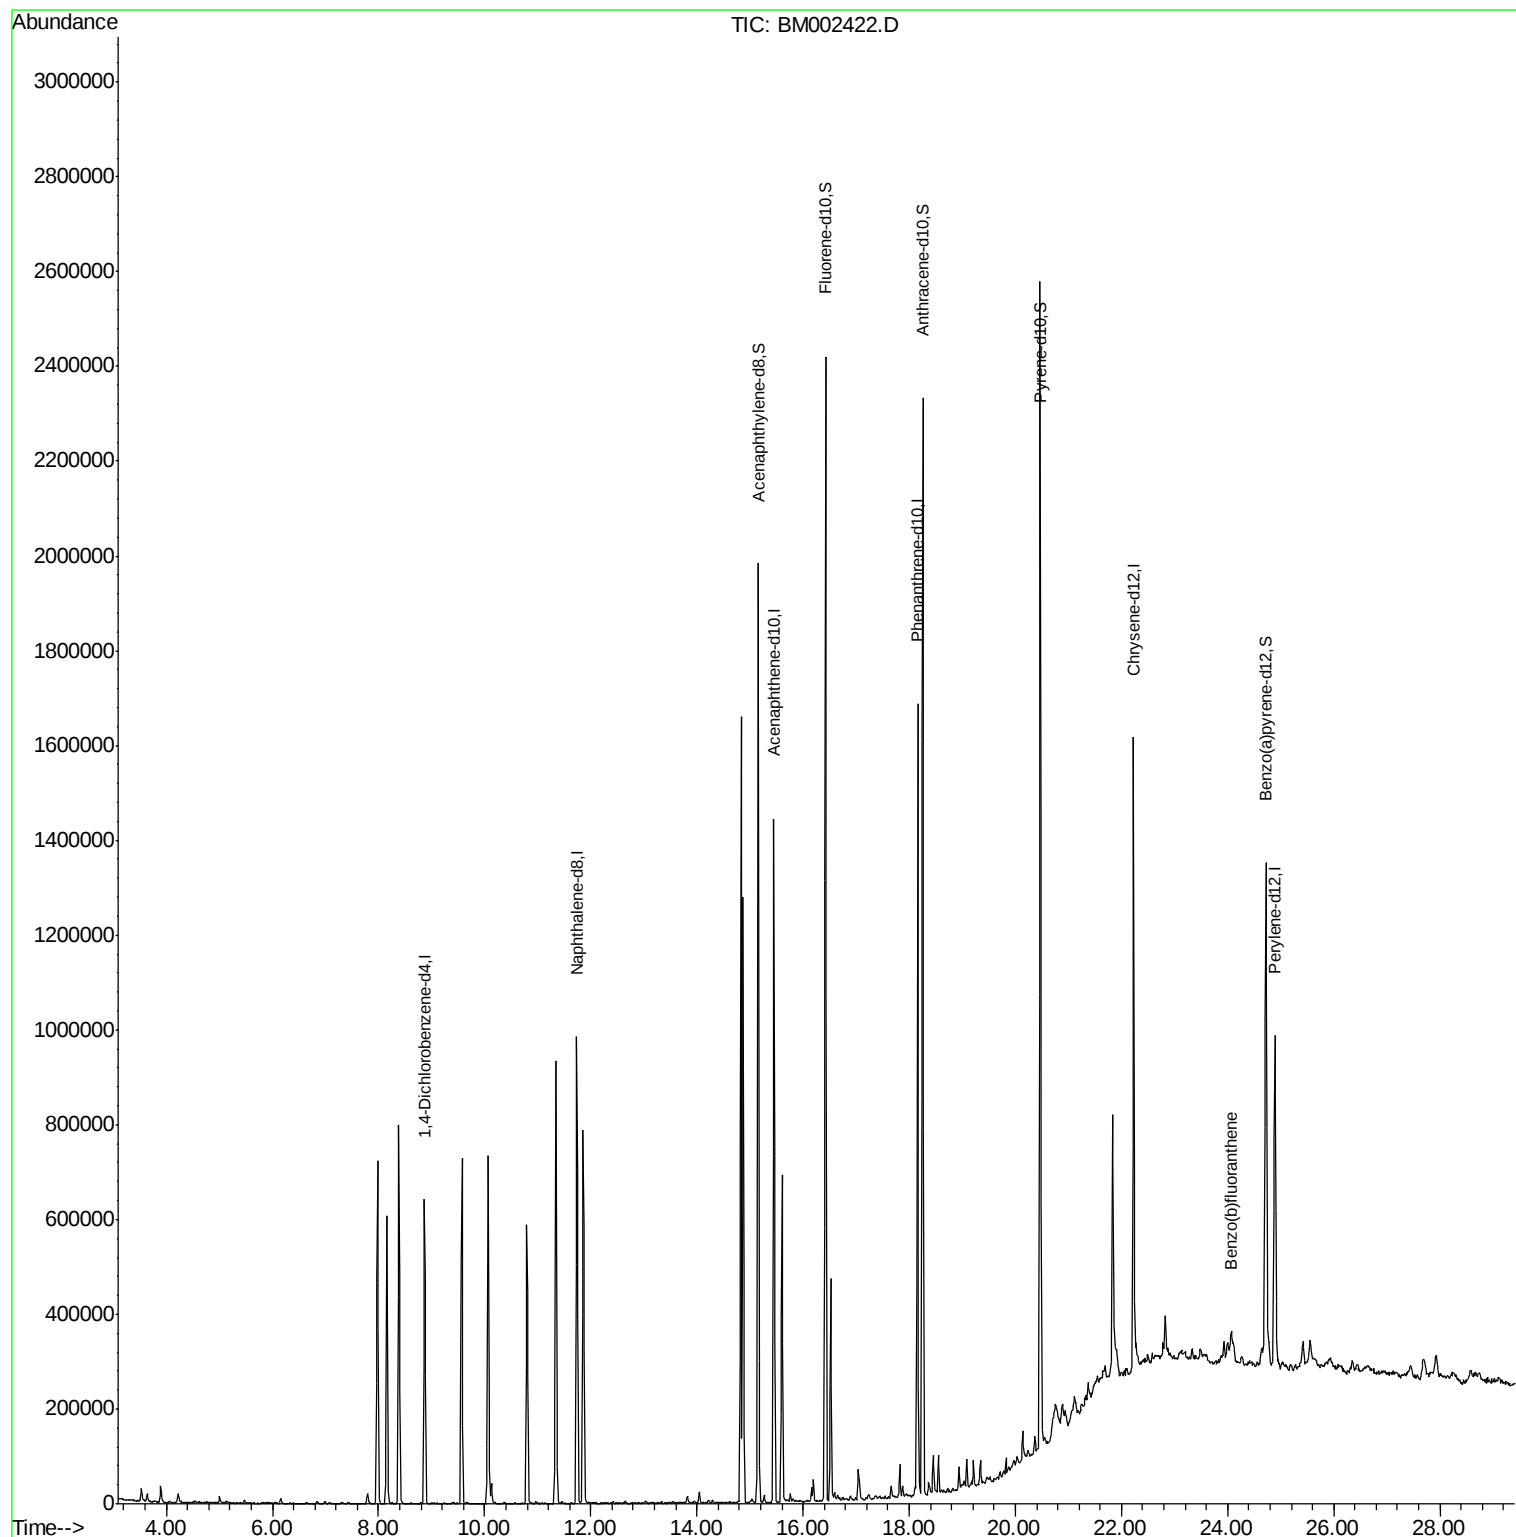

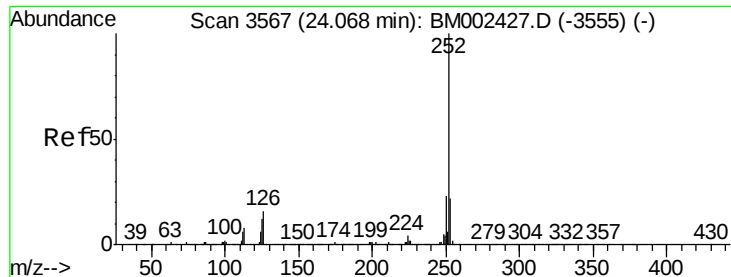

#23

Benzo(b)fluoranthene

Concen: 1.52 ng/ul

RT: 24.07 min Scan# 3567

Delta R.T. 0.01 min

Lab File: BM002422.D

Acq: 15 Aug 2015 13:32

Instrument :

BNA_M

ClientSampleId :

D9DA2


Tgt Ion: 252 Resp: 54053

Ion Ratio Lower Upper

252 100

253 27.0 17.4 26.0#

125 18.7 10.0 15.0#

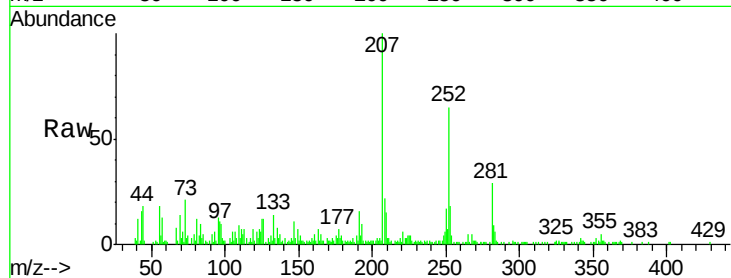

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

