

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
 Data File : BM002403.D
 Acq On : 15 Aug 2015 01:54
 Operator : UM/IZ
 Sample : G3219-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9DA3

Quant Time: Aug 17 02:05:55 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 17 02:04:41 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	114459	20.00	ng/ul	0.00
2) Naphthalene-d8	11.74	136	584149	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.45	164	342919	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.15	188	744962	20.00	ng/ul	0.00
17) Chrysene-d12	22.23	240	782418	20.00	ng/ul	0.00
22) Perylene-d12	24.89	264	761128	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	15.15	160	1047092	29.87	ng/ul	0.00
10) Fluorene-d10	16.42	176	713655	28.98	ng/ul	0.00
14) Anthracene-d10	18.24	188	1029012	28.64	ng/ul	0.00
18) Pyrene-d10	20.46	212	1108516	31.96	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.71	264	1162538	29.08	ng/ul	0.00
Target Compounds						
23) Benzo(b)fluoranthene	24.06	252	62239	1.35	ng/ul	Ovalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
Data File : BM002403.D
Acq On : 15 Aug 2015 01:54
Operator : UM/IZ
Sample : G3219-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9DA3

Quant Time: Aug 17 02:05:55 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 17 02:04:41 2015
Response via : Initial Calibration

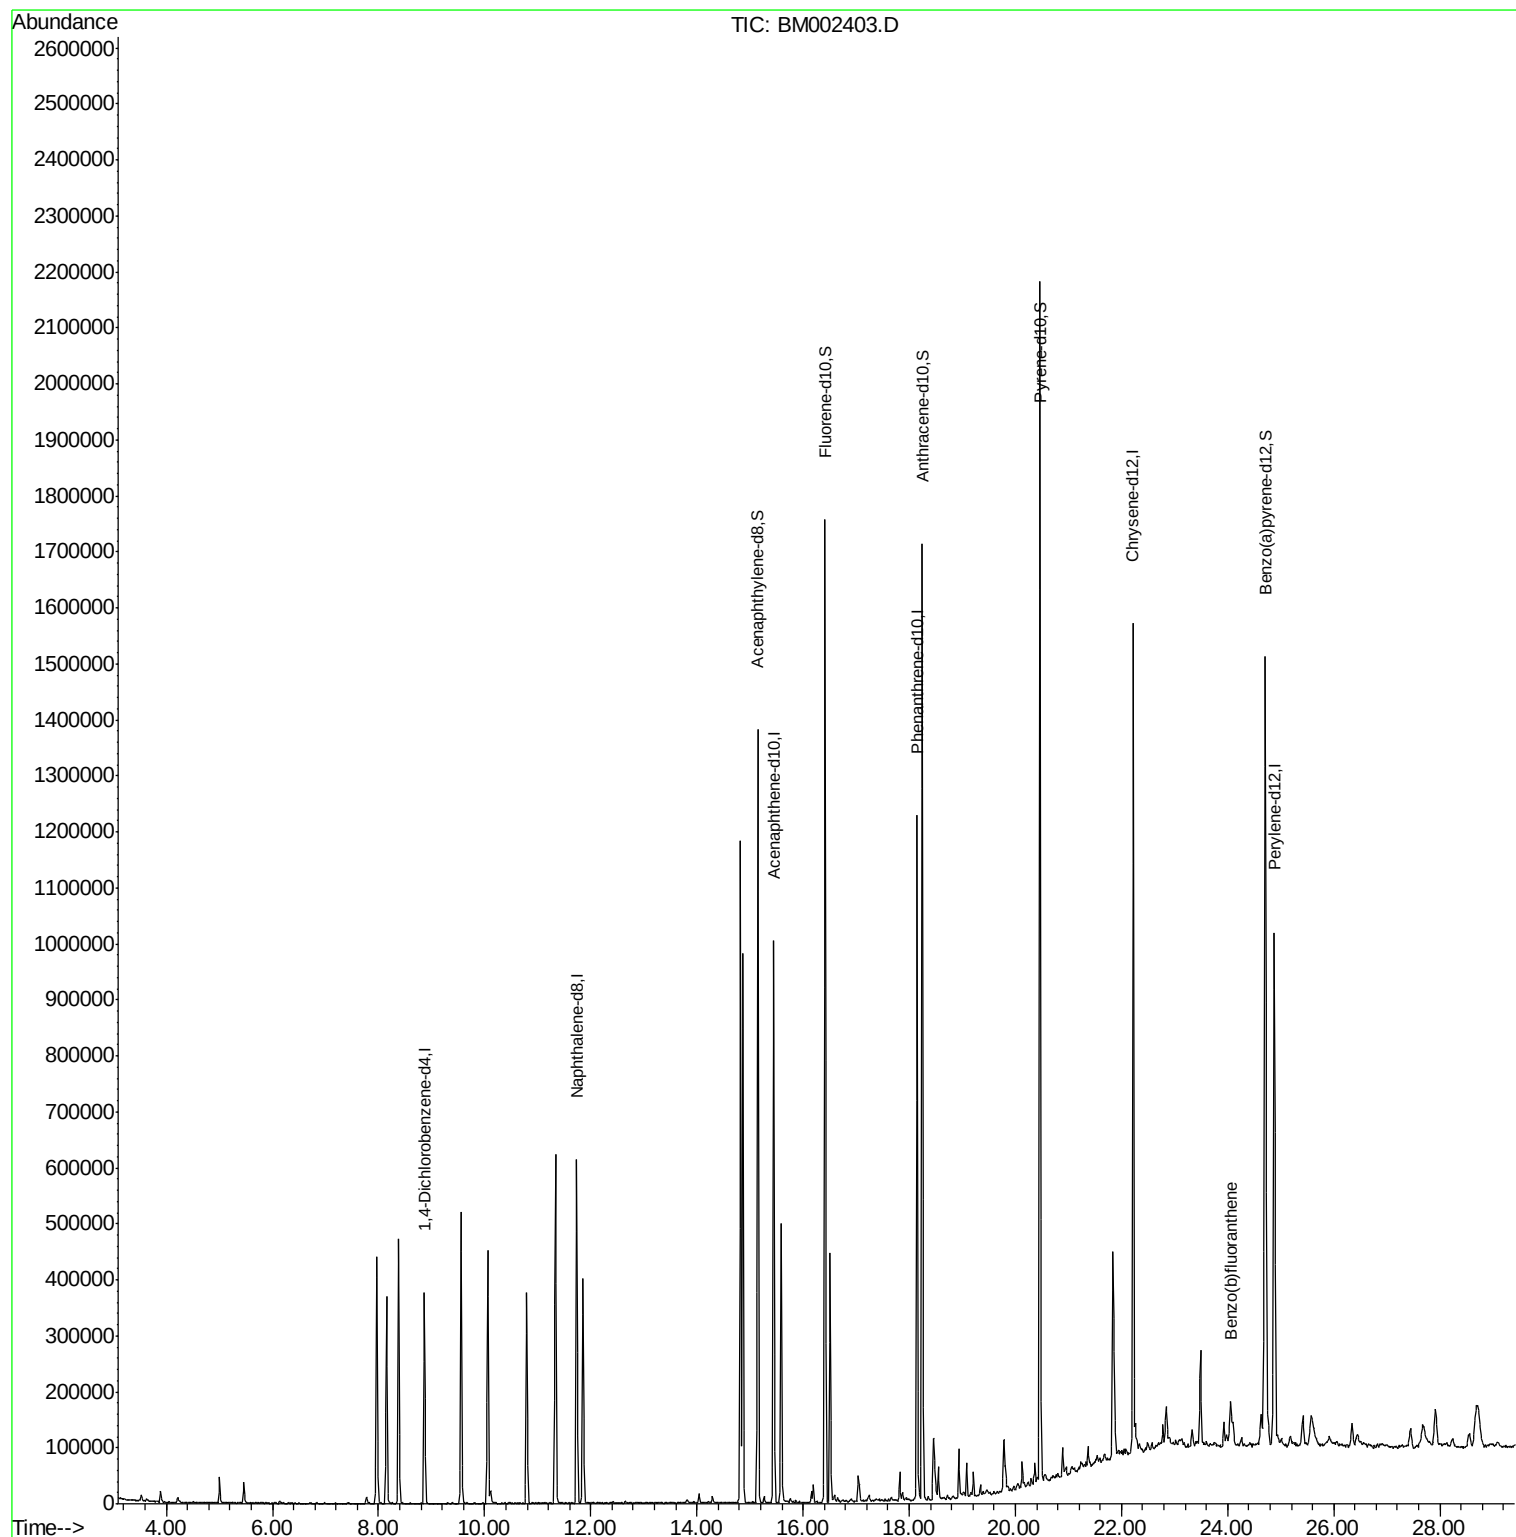

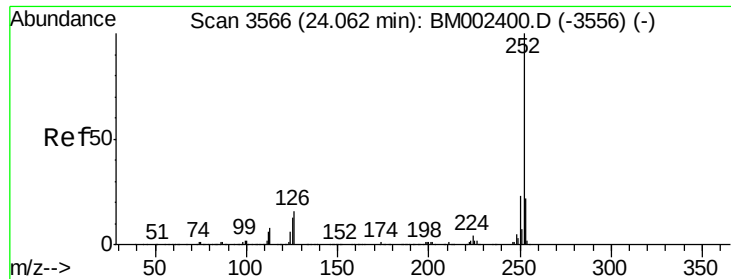

#23

Benzo(b)fluoranthene

Concen: 1.35 ng/ul

RT: 24.06 min Scan# 3565

Delta R.T. -0.01 min

Lab File: BM002403.D

Acq: 15 Aug 2015 01:54

Instrument :

BNA_M

ClientSampleId :

D9DA3


Tot Ion: 252 Resp: 62239

Ion Ratio Lower Upper

252 100

253 23.3 17.4 26.0

125 14.9 10.0 15.0

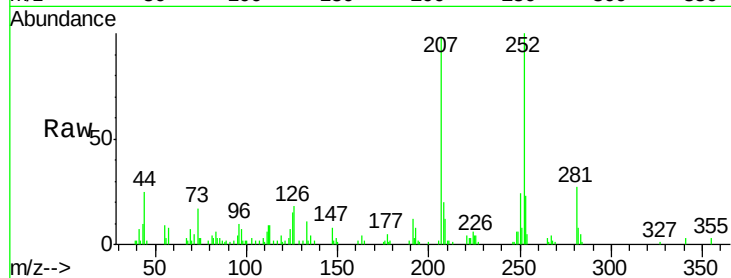

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

