


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
Data File : BM002430.D
Acq On : 15 Aug 2015 18:24
Operator : UM/IZ
Sample : G3194-14
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Aug 17 05:30:16 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
Quant Title : SVOA CALIBRATION
OLast Update : Mon Aug 17 05:12:59 2015
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
D9DB5

Manual Integrations
APPROVED

MMDadoda
8/17/2015 2:46:16 PM

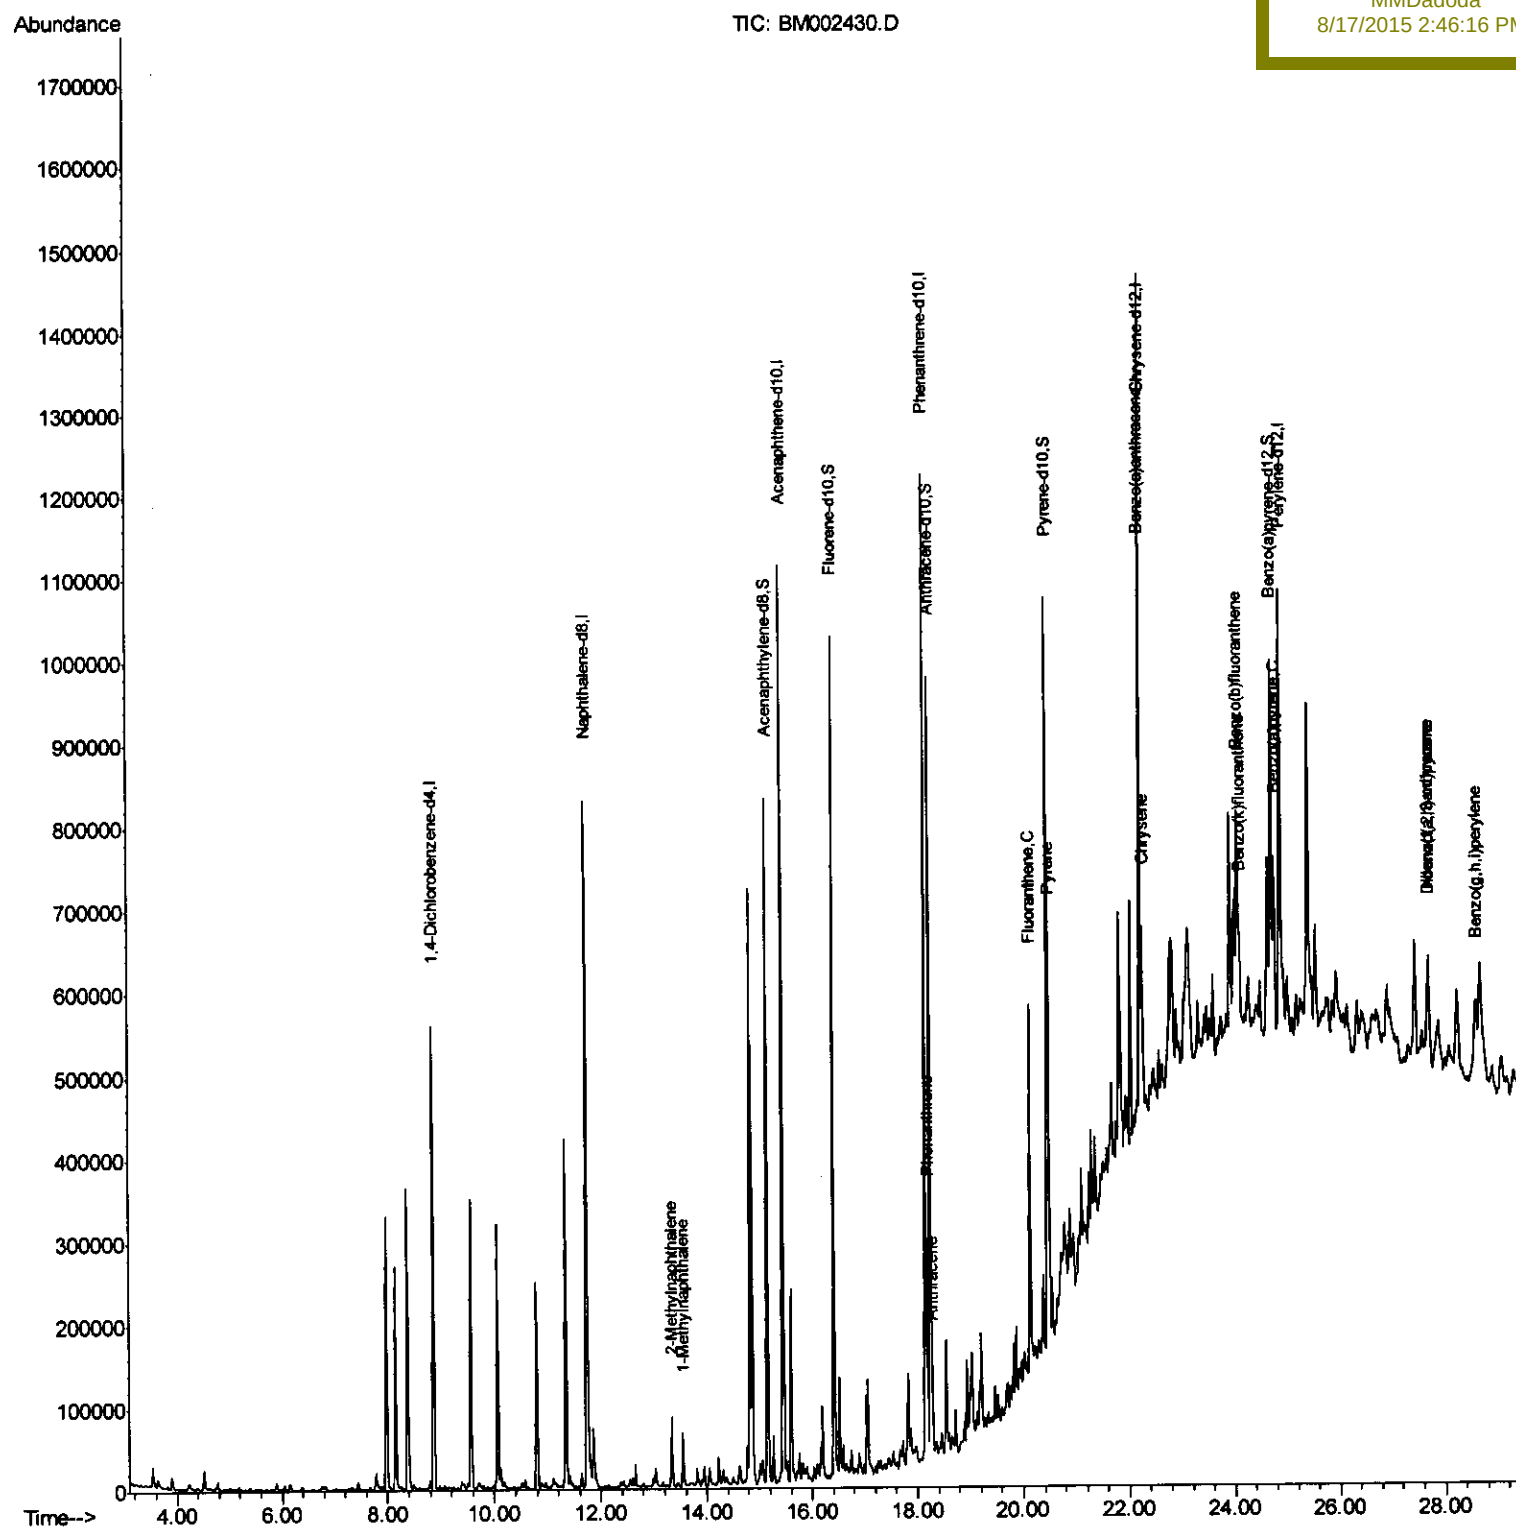




Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
 Data File : BM002430.D
 Acq On : 15 Aug 2015 18:24
 Operator : UM/IZ
 Sample : G3194-14
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Quant Time: Aug 17 05:17:37 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 17 05:12:59 2015
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 D9DB5

Manual Integrations
 APPROVED

MMDadoda
 8/17/2015 2:46:16 PM

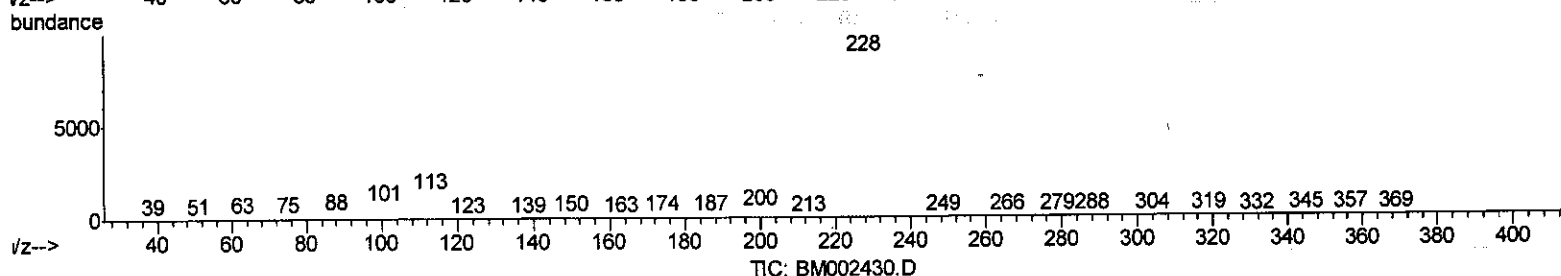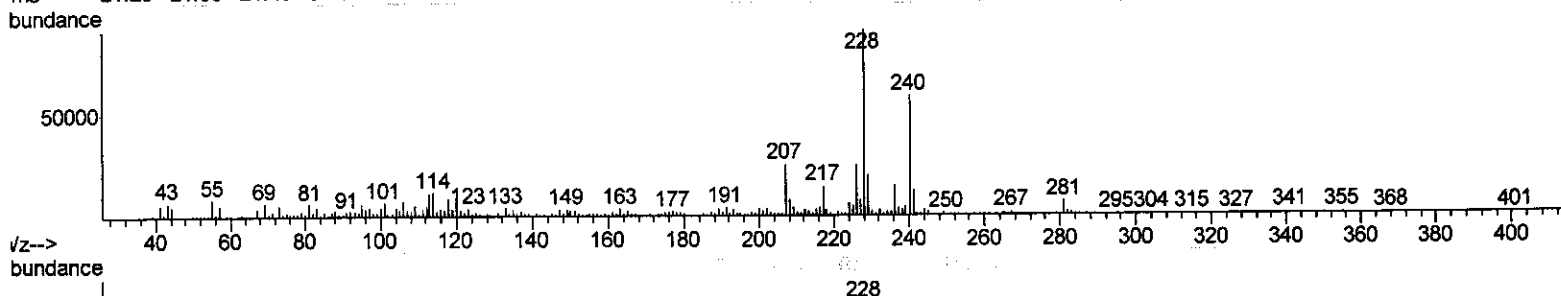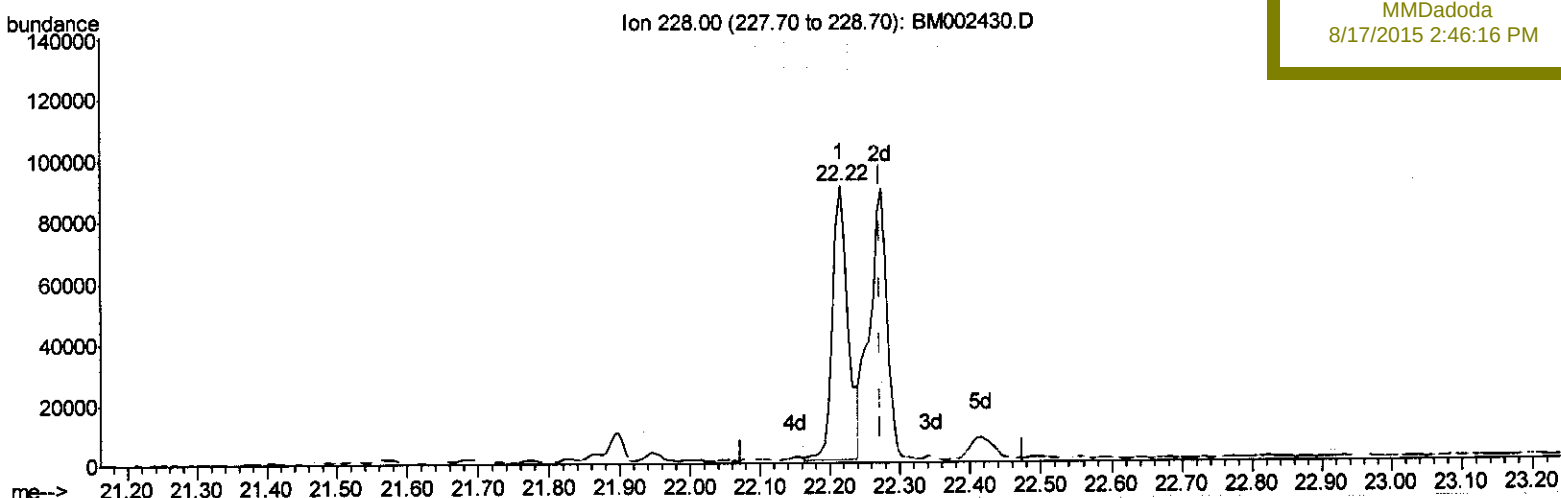

(21) Chrysene

22.215min (-0.059) 5.24ng/ul

response 141275

Ion	Exp%	Act%
228.00	100	100
226.00	29.30	27.77
229.00	19.60	22.47
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
 Data File : BM002430.D
 Acq On : 15 Aug 2015 18:24
 Operator : UM/IZ
 Sample : G3194-14
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9DB5

Manual Integrations
 APPROVED

MMDadoda
 8/17/2015 2:46:16 PM

Quant Time: Aug 17 05:17:37 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 17 05:12:59 2015
 Response via : Initial Calibration

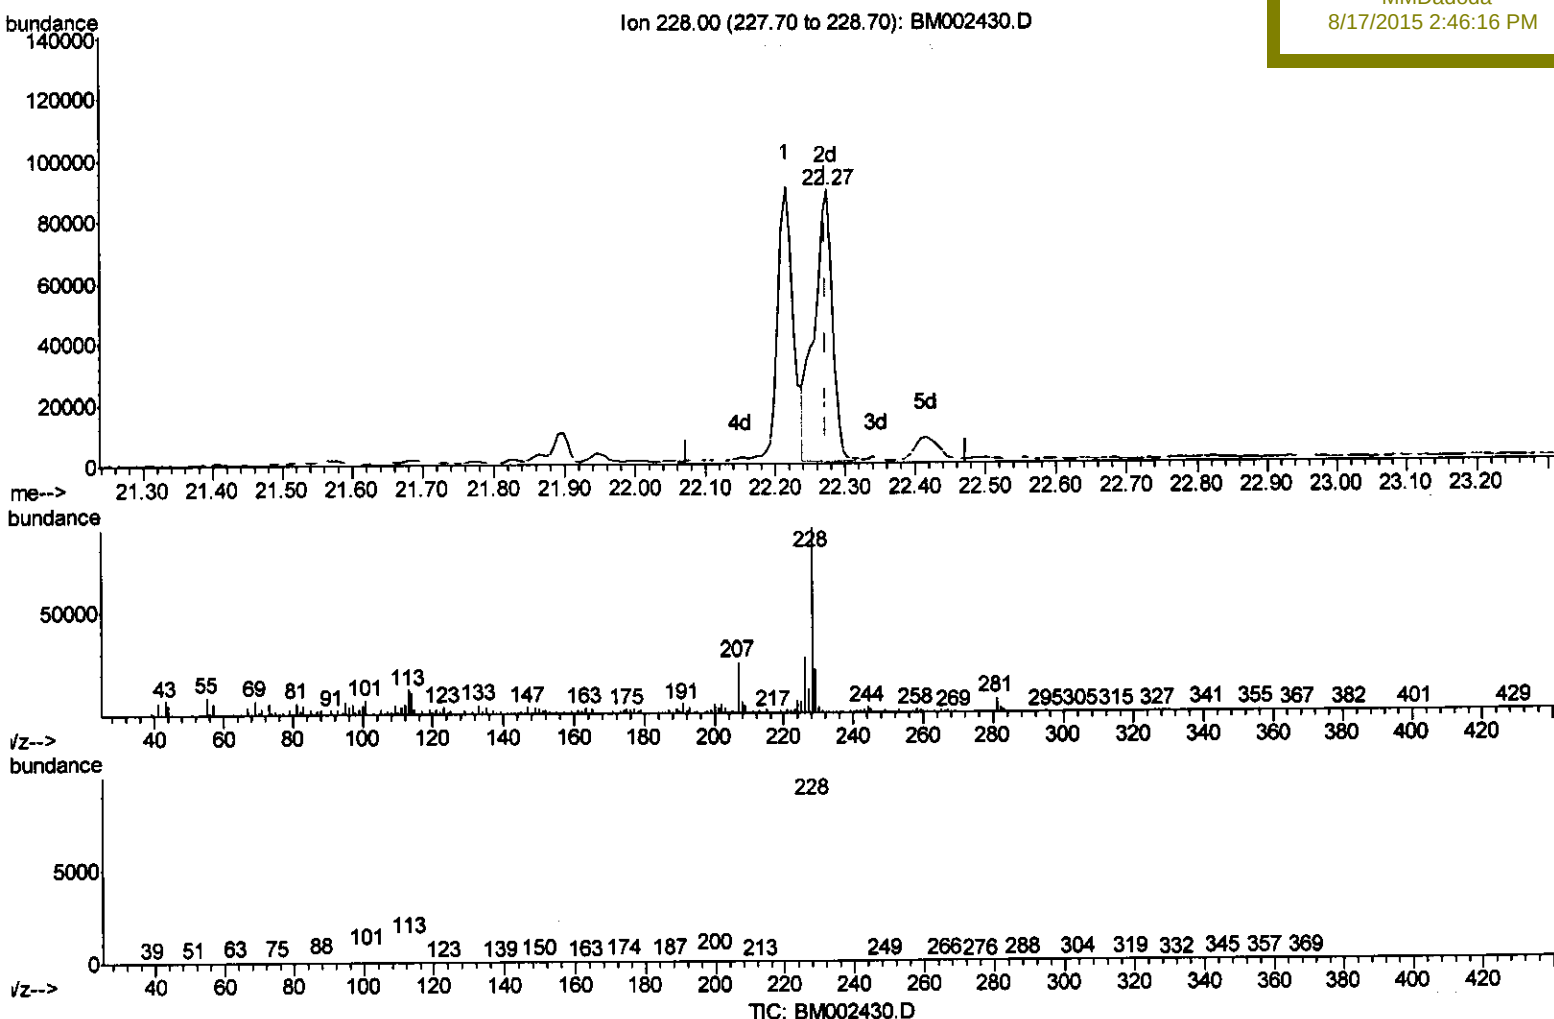

(21) Chrysene

22.274min (+0.000) 5.88ng/ul m

response 158561

U.M.
 08/18/15

Ion	Exp%	Act%
228.00	100	100
226.00	29.30	30.19
229.00	19.60	24.33#
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
 Data File : BM002430.D
 Acq On : 15 Aug 2015 18:24
 Operator : UM/IZ
 Sample : G3194-14
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Quant Time: Aug 17 05:28:41 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 Last Update : Mon Aug 17 05:12:59 2015
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 D9DB5

Manual Integrations
 APPROVED

MMDadoda
 8/17/2015 2:46:16 PM

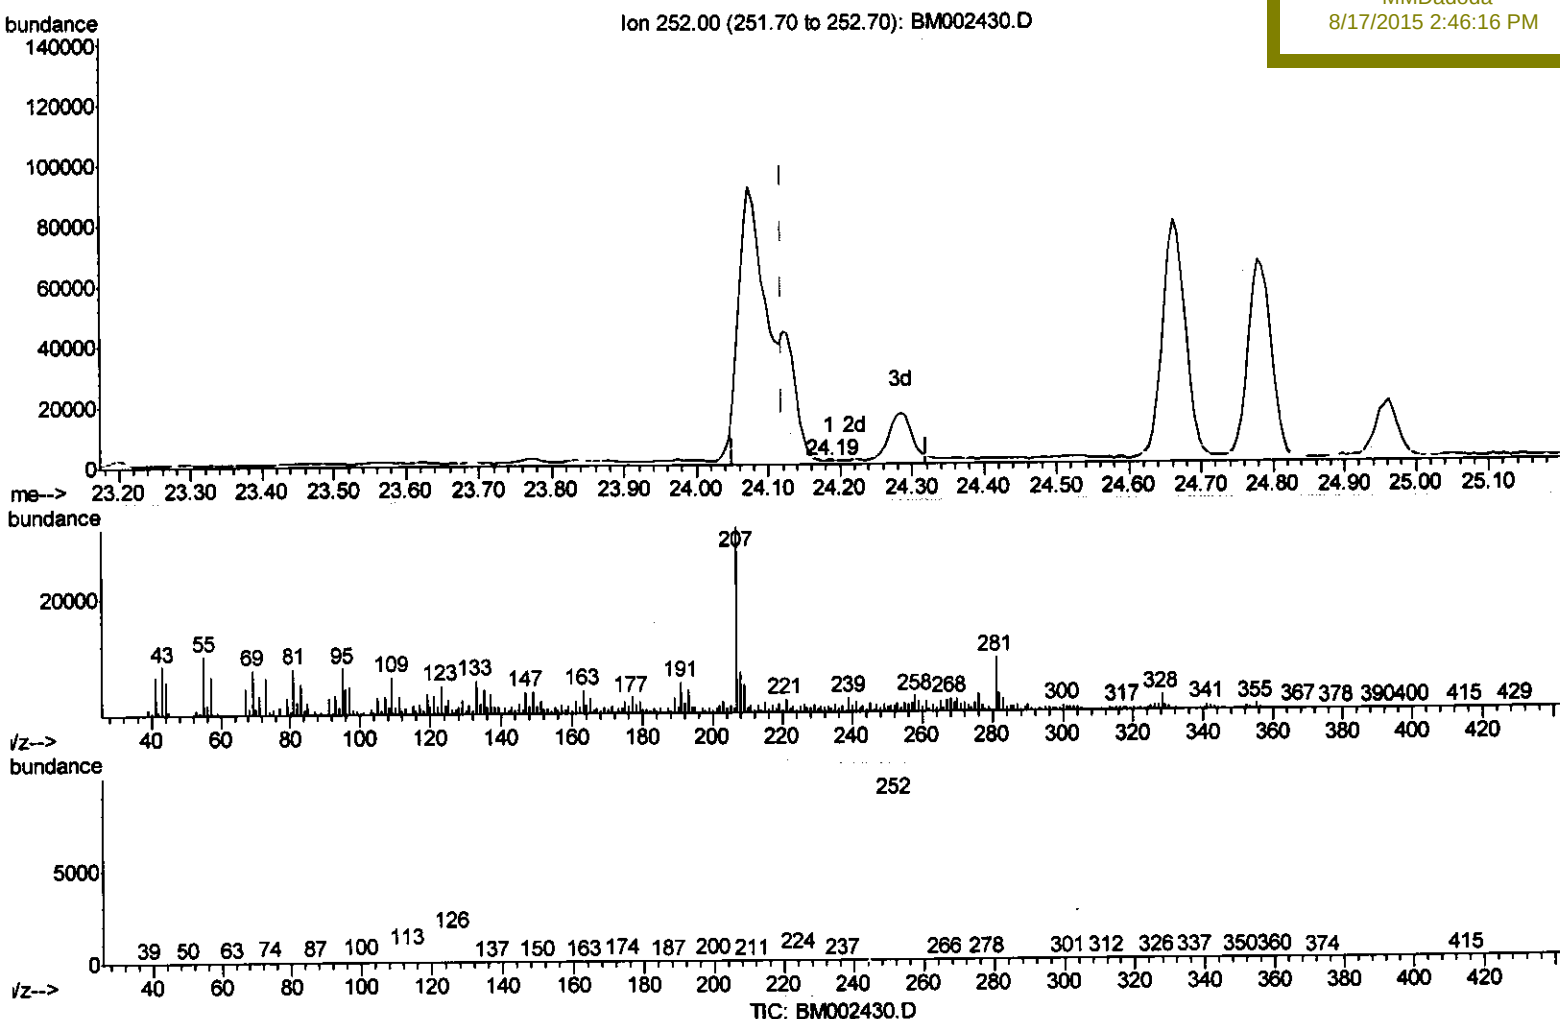

(24) Benzo(k)fluoranthene

24.185min (+0.065) 0.01ng/ul

response 178

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	129.55#
125.00	12.30	182.05#
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
 Data File : BM002430.D
 Acq On : 15 Aug 2015 18:24
 Operator : UM/IZ
 Sample : G3194-14
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Quant Time: Aug 17 05:28:41 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 17 05:12:59 2015
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 D9DB5

Manual Integrations
 APPROVED

MMDadoda
 8/17/2015 2:46:16 PM

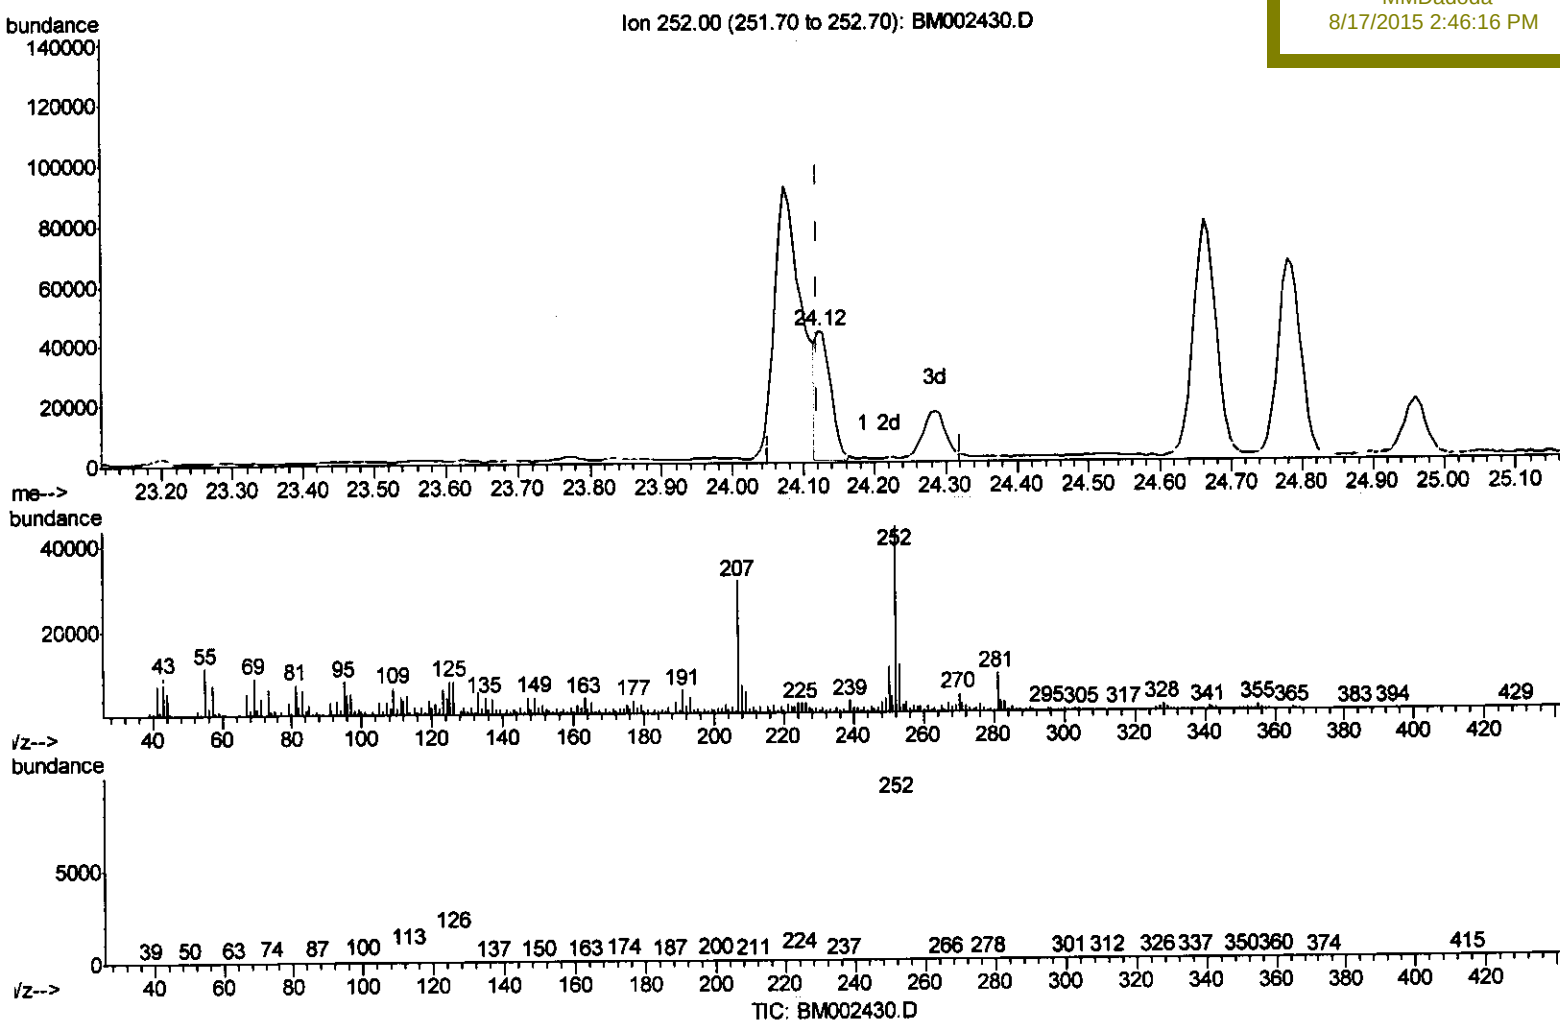

(24) Benzo(k)fluoranthene

24.121min (+0.000) 2.25ng/ul m

response 59148

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	26.37
125.00	12.30	18.48#
0.00	0.00	0.00

U.M.
 08/18/15

Data Path : Z:\HPCHEM1\BNA M\DATA\BM081415\
 Data File : BM002430.D
 Acq On : 15 Aug 2015 18:24
 Operator : UM/IZ
 Sample : G3194-14
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Quant Time: Aug 17 05:30:16 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM081415MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 17 05:12:59 2015
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 D9DB5

Manual Integrations
 APPROVED

MMDadoda
 8/17/2015 2:46:16 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	174012	20.00	ng/ul	0.00
2) Naphthalene-d8	11.74	136	764590	20.00	ng/ul	0.00
6) Acenaphthene-d10	15.45	164	380234	20.00	ng/ul	0.00
12) Phenanthrene-d10	18.16	188	700141	20.00	ng/ul	0.00
17) Chrysene-d12	22.23	240	481846	20.00	ng/ul	0.00
22) Perylene-d12	24.90	264	457927	20.00	ng/ul	0.00

System Monitoring Compounds						
7) Acenaphthylene-d8	15.16	160	623391	16.04	ng/ul	0.00
10) Fluorene-d10	16.42	176	413649	15.15	ng/ul	0.00
14) Anthracene-d10	18.25	188	543457	16.09	ng/ul	0.00
18) Pvrene-d10	20.47	212	441743	20.68	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.73	264	356800	14.83	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
4) 2-Methylnaphthalene	13.33	142	43901	1.50	ng/ul	96
5) 1-Methylnaphthalene	13.55	142	33048	1.14	ng/ul	100
13) Phenanthrene	18.20	178	158997	3.93	ng/ul	99
15) Anthracene	18.29	178	50594	1.23	ng/ul	99
16) Fluoranthene	20.14	202	264107	5.77	ng/ul	98
19) Pvrene	20.50	202	252029	8.93	ng/ul	99
20) Benzo(a)anthracene	22.22	228	142426	4.94	ng/ul	96
21) Chrysene	22.27	228	158561m	5.88	ng/ul	94
23) Benzo(b)fluoranthene	24.07	252	242175	8.75	ng/ul#	94
24) Benzo(k)fluoranthene	24.12	252	59148m	2.25	ng/ul	94
26) Benzo(a)pvrene	24.78	252	147259	5.57	ng/ul#	94
27) Indeno(1,2,3-cd)pvrene	27.72	276	108034	3.55	ng/ul	94
28) Dibenzo(a,h)anthracene	27.71	278	33310	1.31	ng/ul#	63
29) Benzo(a,h,i)perylene	28.60	276	142551	5.63	ng/ul	94

U. M.
 08/18/15

(#) = qualifier out of range (m) = manual integration (+) = signals summed